

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL056994.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 03:51
 Operator : AJ\MA
 Sample : L1723-02
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 04:38:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	116.7E6	29999741	13.694	14.061
28)	SA Decachlor...	8.214	8.985	123.7E6	28644164	12.794	13.481
Target Compounds							
4)	MA Heptachlor	0.000	5.140	0	10950659	N.D.	3.518 #
7)	B delta-BHC	0.000	5.045f	0	1917753	N.D.	0.788 #
8)	B Heptachlo...	0.000	5.814	0	15851456	N.D.	5.720 #
13)	MA Dieldrin	5.751	0.000	16058816	0	1.313	N.D. #
14)	MA Endrin	6.017	0.000	14877606	0	1.367	N.D. #
15)	B Endosulfa...	0.000	6.872	0	1897686	N.D.	0.676 #
16)	A 4,4'-DDD	0.000	6.771	0	2709814	N.D.	1.112 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL056994.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 03:51
Operator : AJ\MA
Sample : L1723-02
Misc :
ALS Vial : 28 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 04:38:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

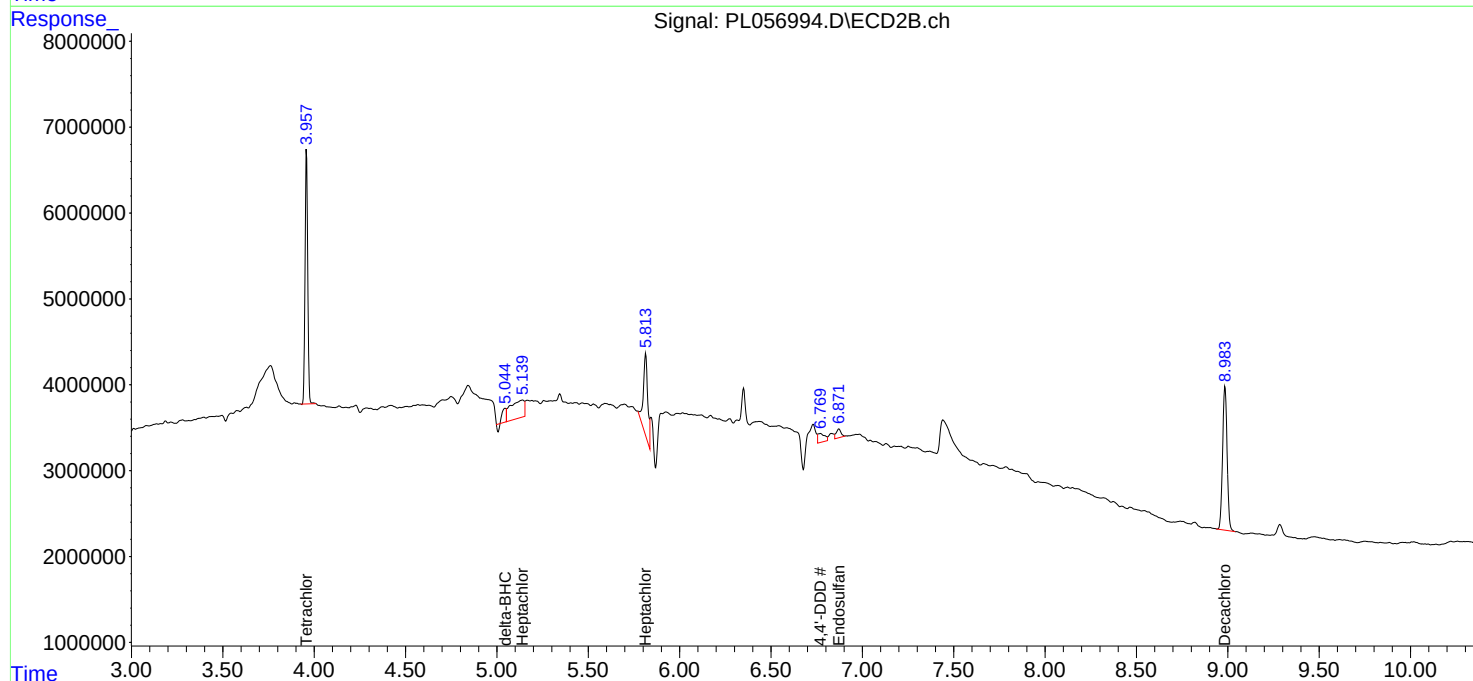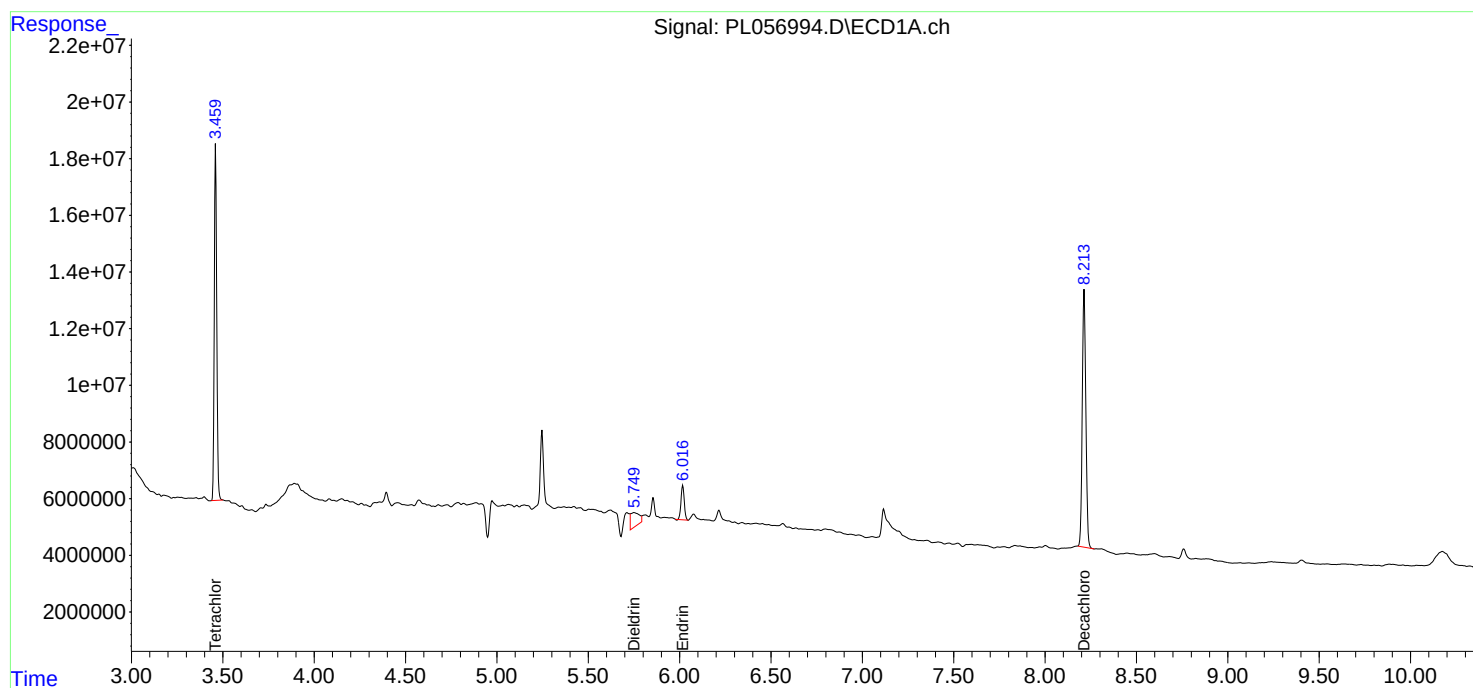

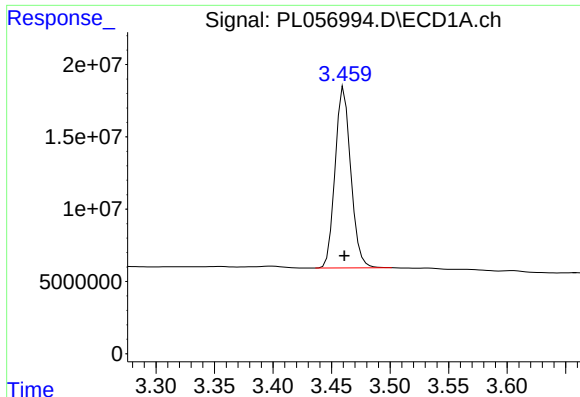


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 116701204
Conc: 13.69 ng/ml

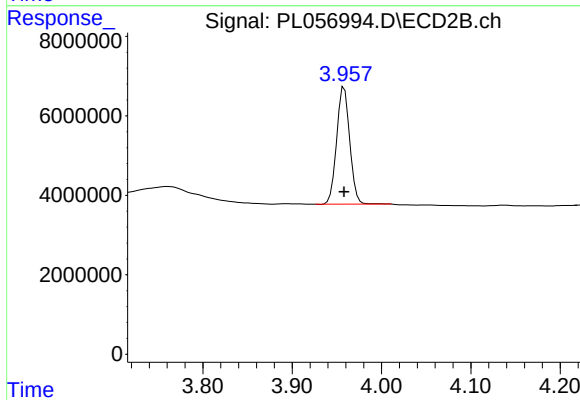


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 29999741
Conc: 14.06 ng/ml

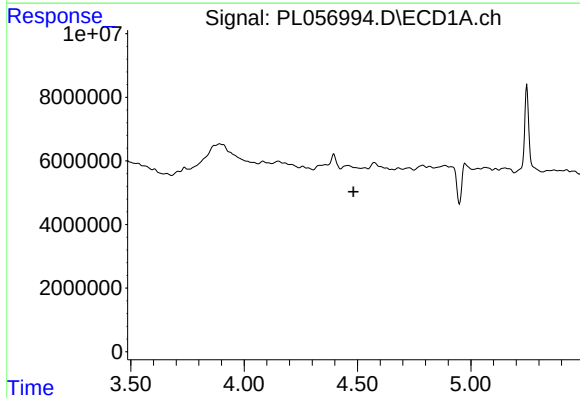


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

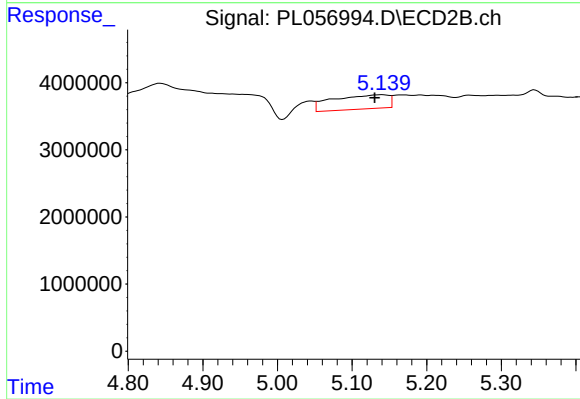


#4 Heptachlor

R.T.: 5.140 min
Delta R.T.: 0.010 min
Response: 10950659
Conc: 3.52 ng/ml

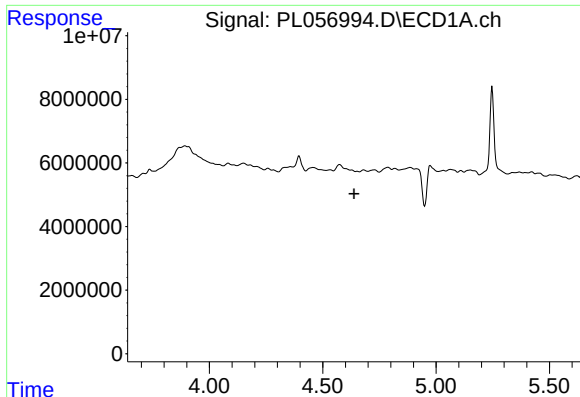


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

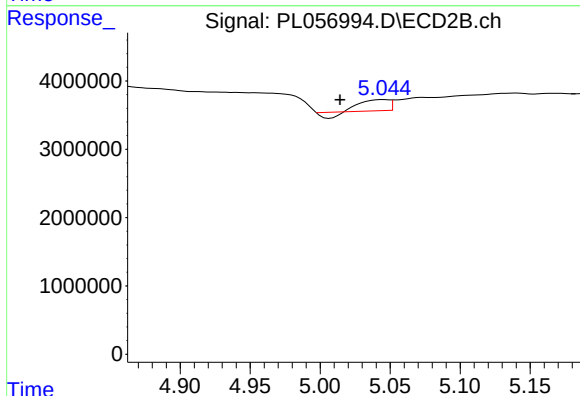


#7 delta-BHC

R.T.: 5.045 min
Delta R.T.: 0.031 min
Response: 1917753
Conc: 0.79 ng/ml

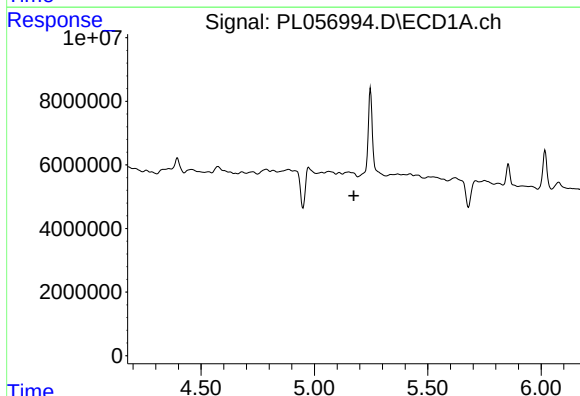


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

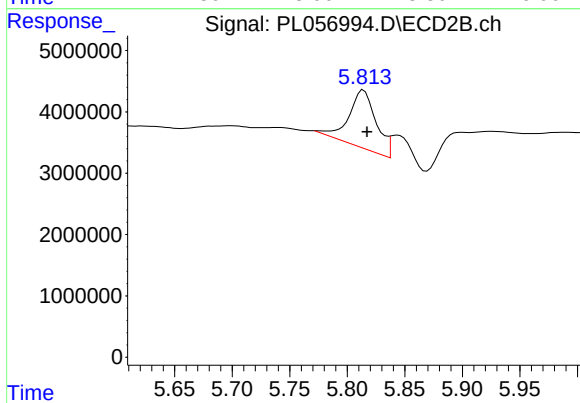


#8 Heptachlor epoxide

R.T.: 5.814 min
Delta R.T.: -0.003 min
Response: 15851456
Conc: 5.72 ng/ml

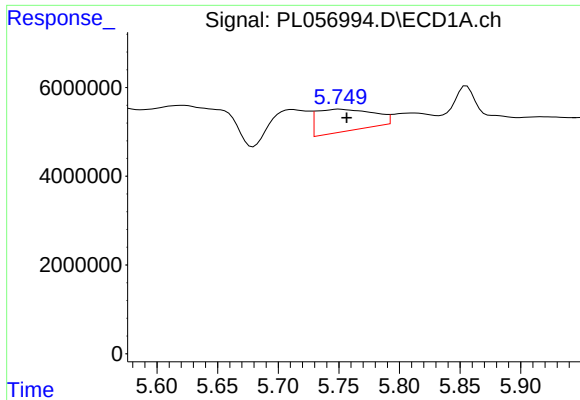


#13 Dieldrin

R.T.: 5.751 min
Delta R.T.: -0.006 min
Response: 16058816
Conc: 1.31 ng/ml

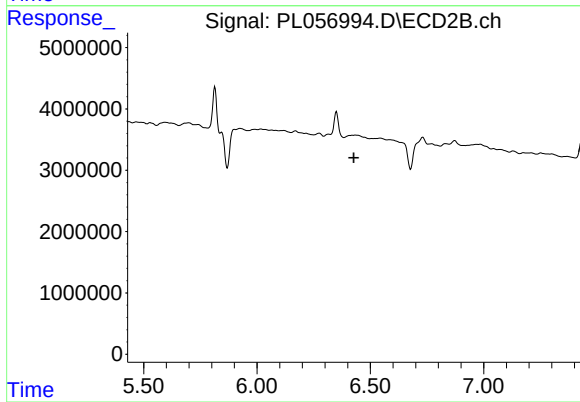


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.428 min
Response: 0
Conc: N.D.

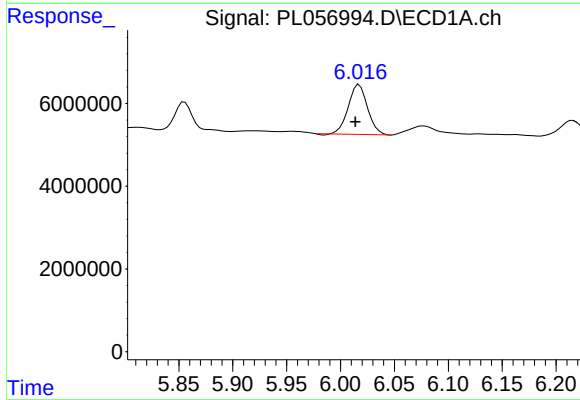


#14 Endrin

R.T.: 6.017 min
Delta R.T.: 0.004 min
Response: 14877606
Conc: 1.37 ng/ml

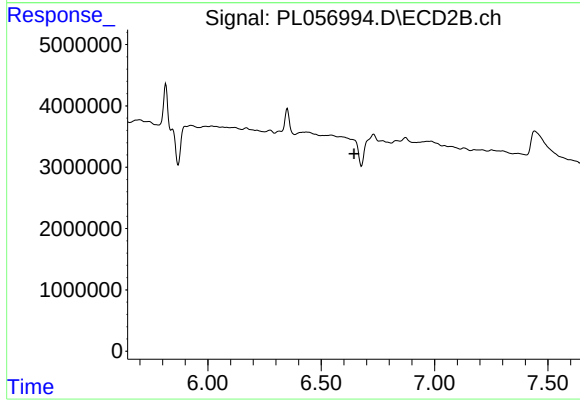


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.645 min
Response: 0
Conc: N.D.

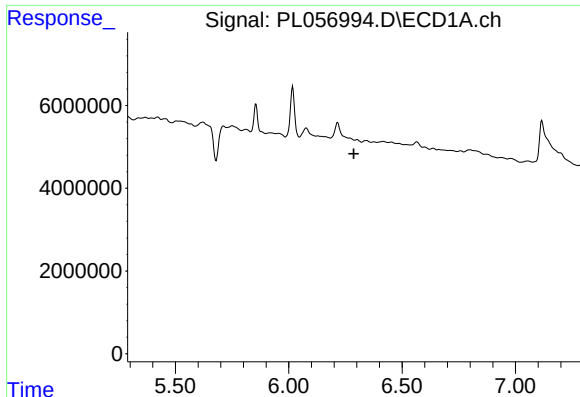


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

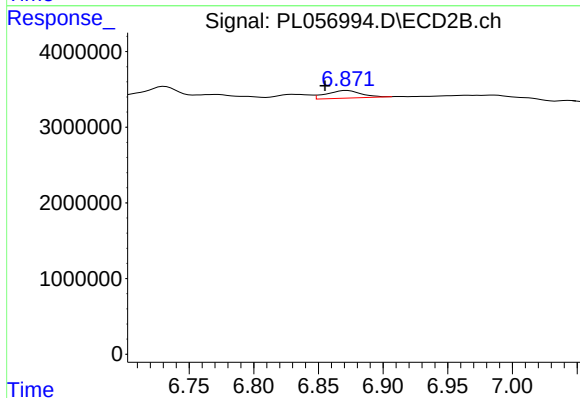


#15 Endosulfan II

R.T.: 6.872 min
Delta R.T.: 0.017 min
Response: 1897686
Conc: 0.68 ng/ml

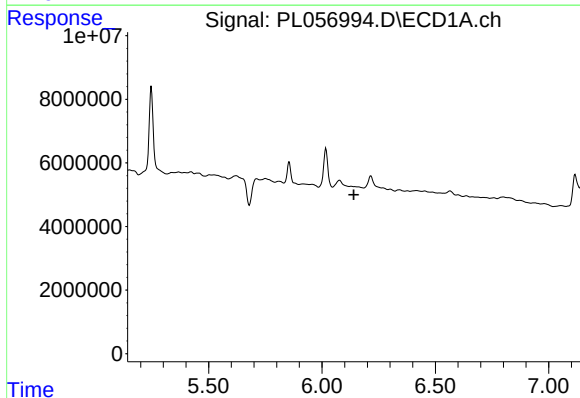


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.141 min
Response: 0
Conc: N.D.

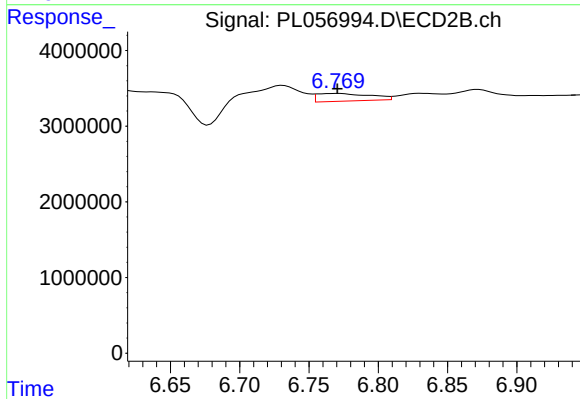


#16 4,4'-DDD

R.T.: 6.771 min
Delta R.T.: 0.000 min
Response: 2709814
Conc: 1.11 ng/ml

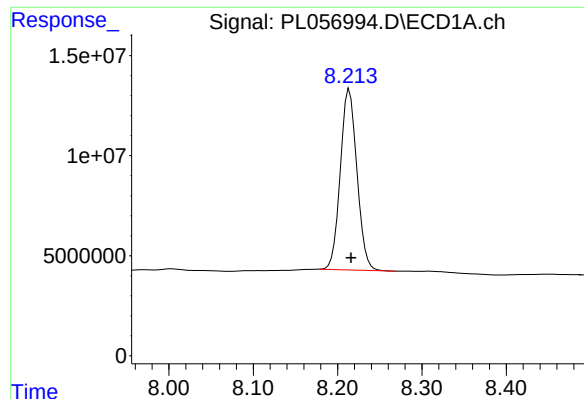

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.002 min
Response: 123658138
Conc: 12.79 ng/ml

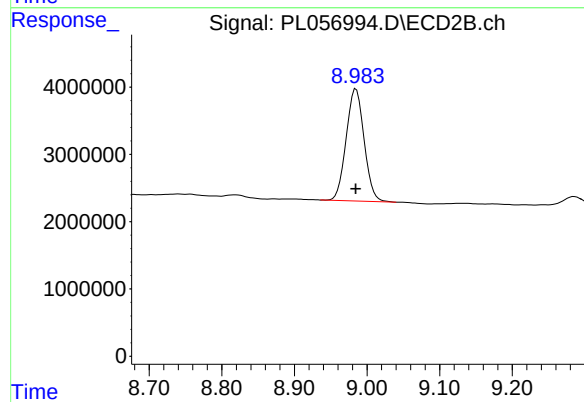

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 28644164
Conc: 13.48 ng/ml