

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL057002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 05:44
 Operator : AJ\MA
 Sample : L1743-10
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 06:31:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	108.3E6	27330656	12.704	12.810
28)	SA Decachlor...	8.214	8.984	142.1E6	30588465	14.706	14.396
Target Compounds							
4)	MA Heptachlor	4.482	5.131	8013665	26386553	0.590	8.478 #
5)	MB Aldrin	0.000	5.408f	0	3100956	N.D.	1.037 #
8)	B Heptachlo...	0.000	5.814	0	36315711	N.D.	13.105 #
10)	B gamma-Chl...	5.423f	6.050	17806508	1965736	1.434	0.657 #
11)	B alpha-Chl...	5.458	6.124	10779171	6178812	0.877	2.050 #
12)	B 4,4'-DDE	5.623	6.279	60320797	1405328	5.148	0.495 #
14)	MA Endrin	6.016	0.000	11022191	0	1.013	N.D. #
15)	B Endosulfa...	6.295	6.872	8369337	12294498	0.775	4.381 #
16)	A 4,4'-DDD	0.000	6.732f	0	38932127	N.D.	15.982 #
23)	Chlordane-1	4.330	4.942	12454200	10734428	40.974	133.835 #
24)	Chlordane-2	4.832	5.408	67003845	3100956	189.994	32.486 #
25)	Chlordane-3	5.423f	6.050	17806508	1965736	16.508	5.187 #
26)	Chlordane-4	5.458	6.124	10779171	6178812	11.729	13.475
27)	Chlordane-5	6.295	6.925	8369337	5111516	23.042	61.267 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL057002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 05:44
Operator : AJ\MA
Sample : L1743-10
Misc :
ALS Vial : 34 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 06:31:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

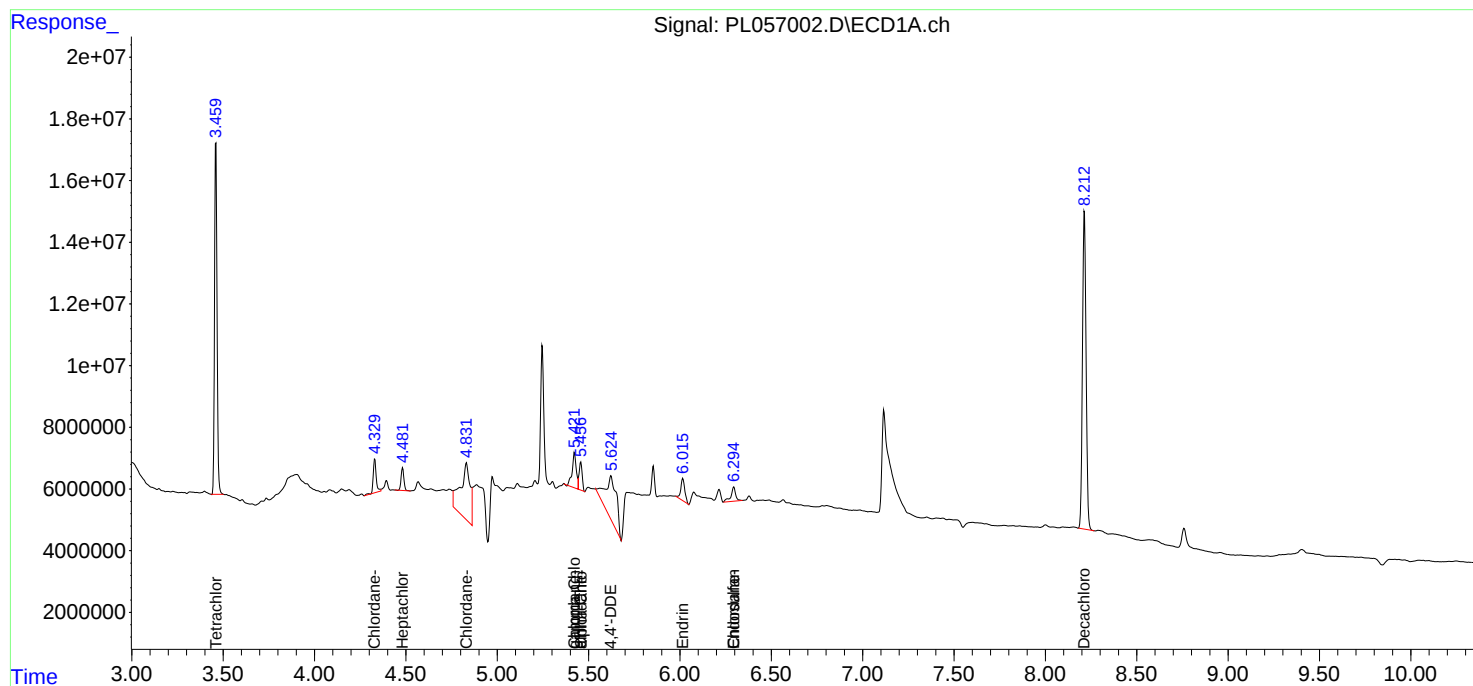

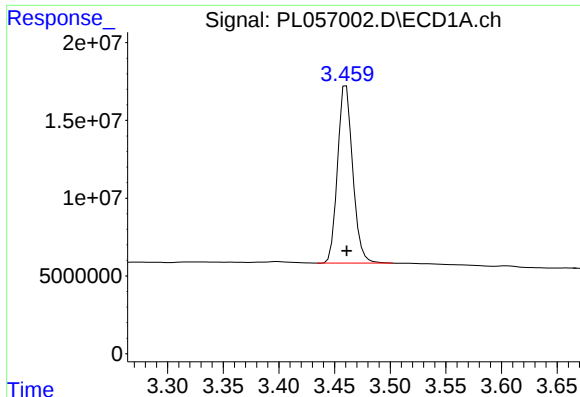


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 108270890
Conc: 12.70 ng/ml

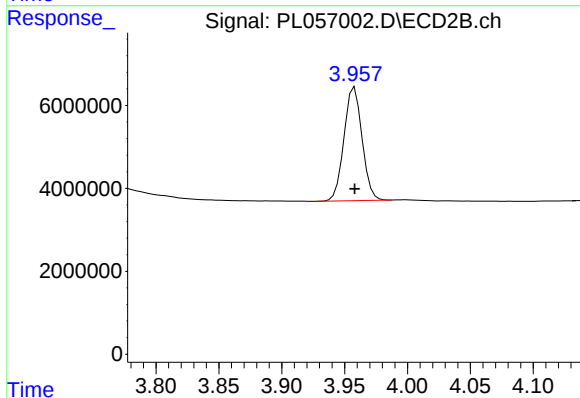


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 27330656
Conc: 12.81 ng/ml

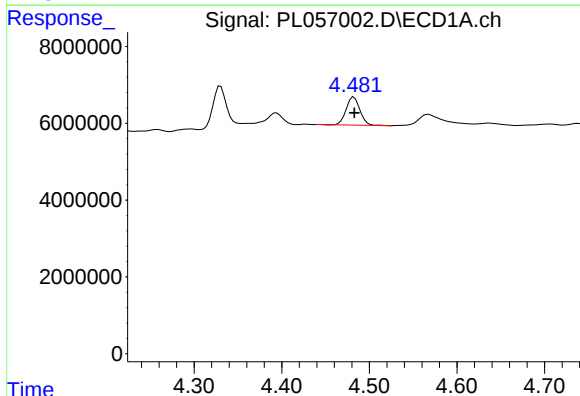


#4 Heptachlor

R.T.: 4.482 min
Delta R.T.: 0.000 min
Response: 8013665
Conc: 0.59 ng/ml

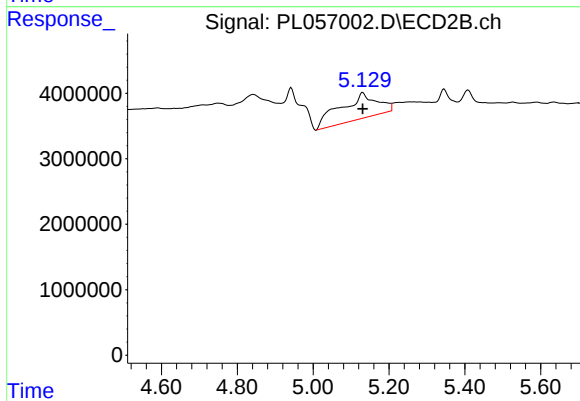


#4 Heptachlor

R.T.: 5.131 min
Delta R.T.: 0.000 min
Response: 26386553
Conc: 8.48 ng/ml

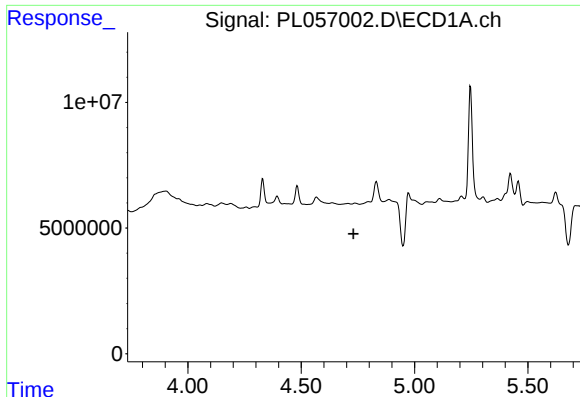


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

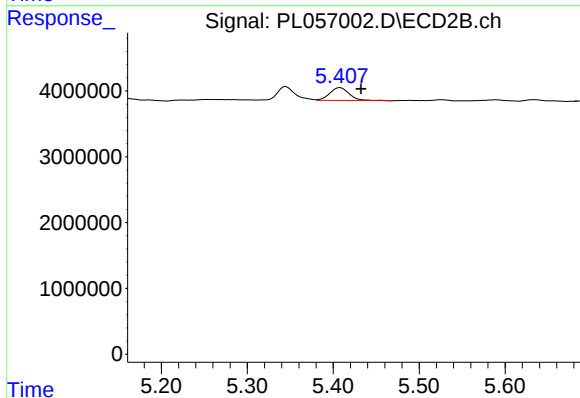


#5 Aldrin

R.T.: 5.408 min
Delta R.T.: -0.024 min
Response: 3100956
Conc: 1.04 ng/ml

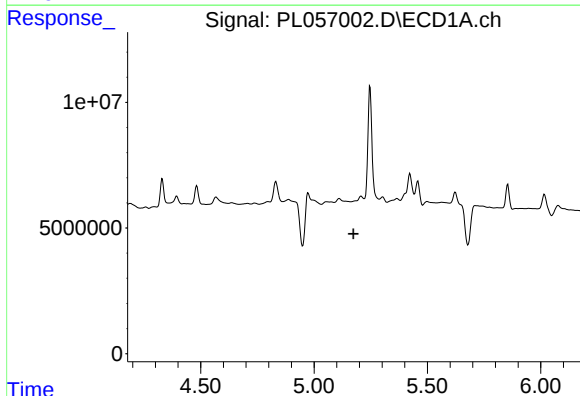


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

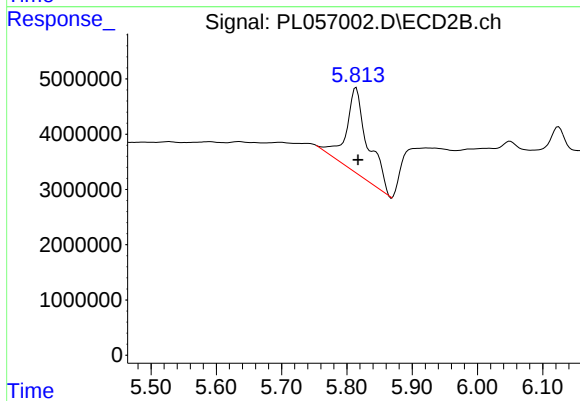


#8 Heptachlor epoxide

R.T.: 5.814 min
Delta R.T.: -0.003 min
Response: 36315711
Conc: 13.11 ng/ml

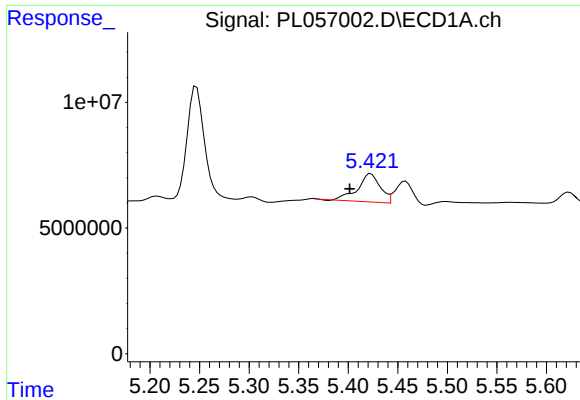


#10 gamma-Chlordane

R.T.: 5.423 min
Delta R.T.: 0.021 min
Response: 17806508
Conc: 1.43 ng/ml

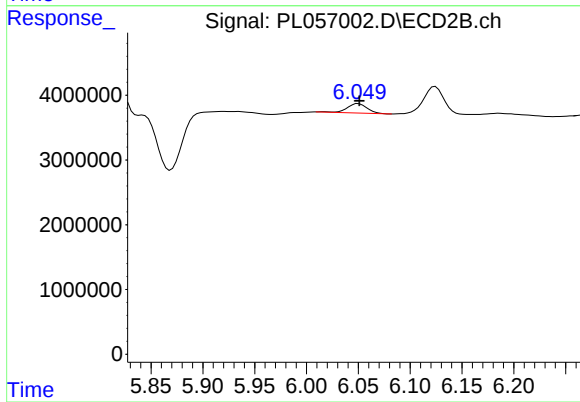


#10 gamma-Chlordane

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 1965736
Conc: 0.66 ng/ml

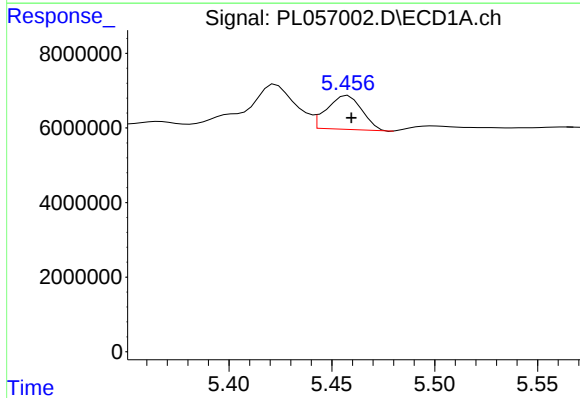


#11 alpha-Chlordane

R.T.: 5.458 min
Delta R.T.: -0.002 min
Response: 10779171
Conc: 0.88 ng/ml

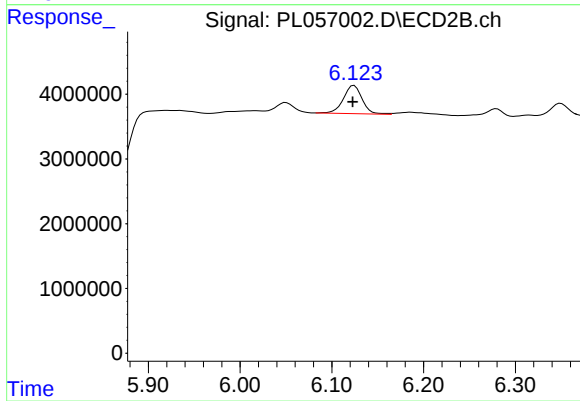


#11 alpha-Chlordane

R.T.: 6.124 min
Delta R.T.: 0.002 min
Response: 6178812
Conc: 2.05 ng/ml

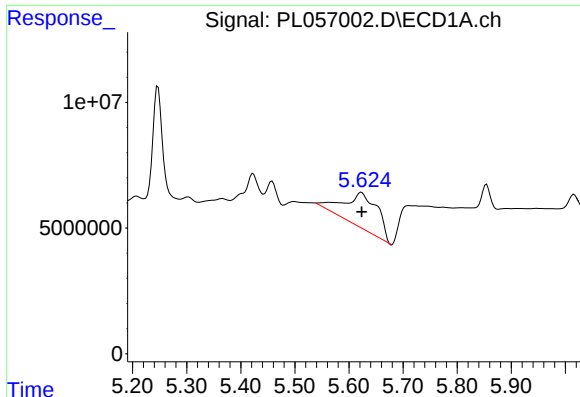


#12 4,4'-DDE

R.T.: 5.623 min
Delta R.T.: -0.001 min
Response: 60320797
Conc: 5.15 ng/ml

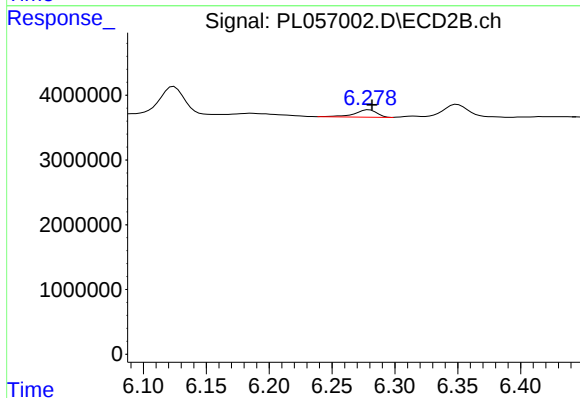


#12 4,4'-DDE

R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 1405328
Conc: 0.50 ng/ml

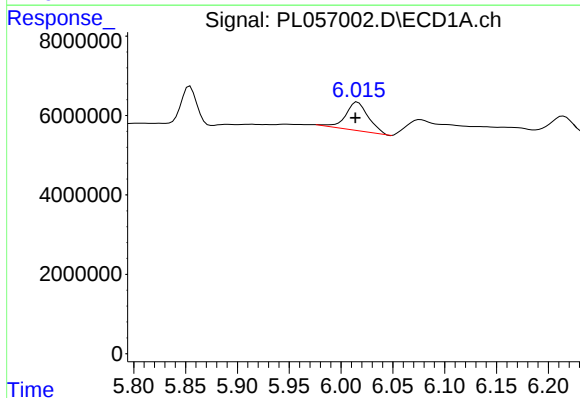


#14 Endrin

R.T.: 6.016 min
Delta R.T.: 0.002 min
Response: 11022191
Conc: 1.01 ng/ml

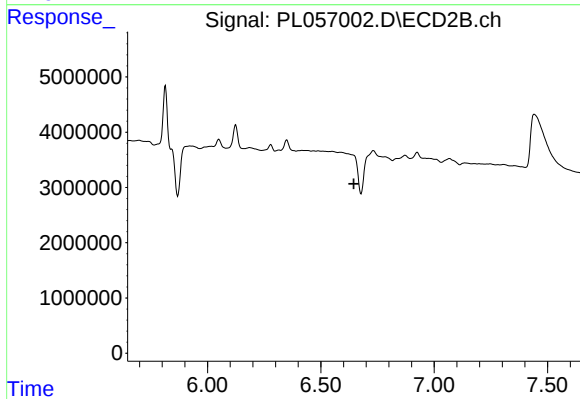


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.645 min
Response: 0
Conc: N.D.

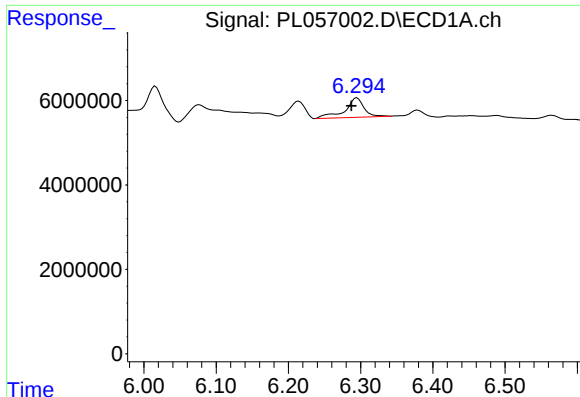


#15 Endosulfan II

R.T.: 6.295 min
Delta R.T.: 0.008 min
Response: 8369337
Conc: 0.77 ng/ml

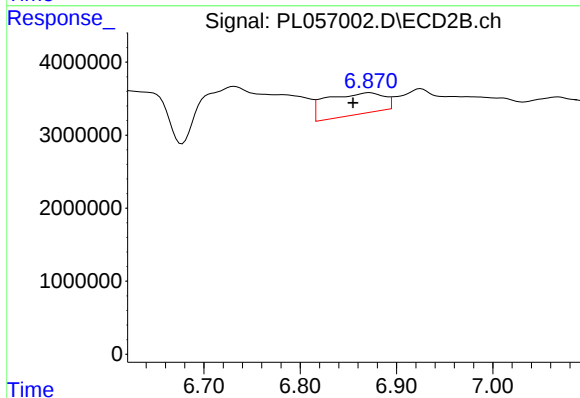


#15 Endosulfan II

R.T.: 6.872 min
Delta R.T.: 0.017 min
Response: 12294498
Conc: 4.38 ng/ml

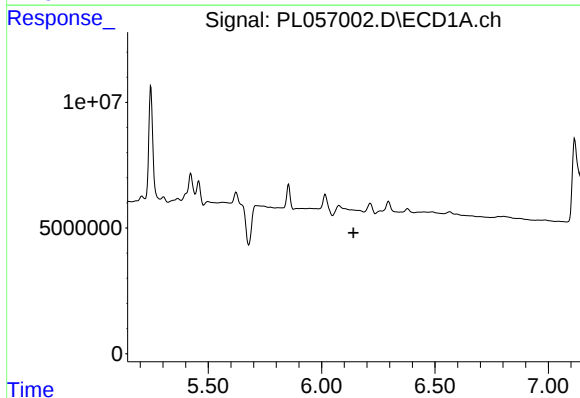


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.141 min
Response: 0
Conc: N.D.

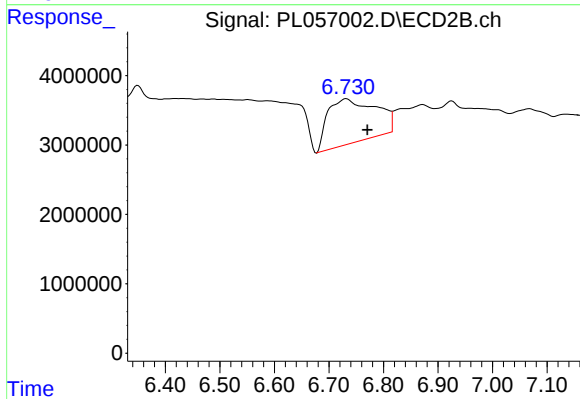


#16 4,4'-DDD

R.T.: 6.732 min
Delta R.T.: -0.039 min
Response: 38932127
Conc: 15.98 ng/ml

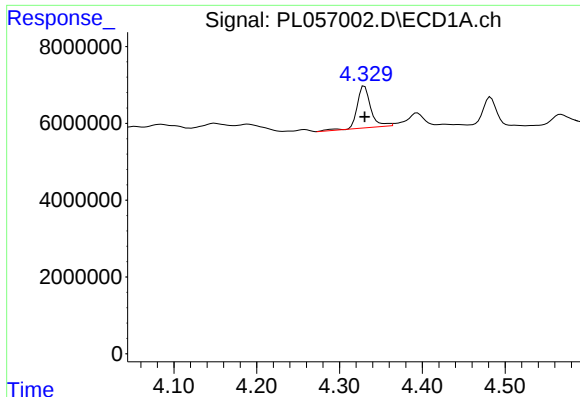


#23 Chlordane-1

R.T.: 4.330 min
Delta R.T.: 0.000 min
Response: 12454200
Conc: 40.97 ng/ml

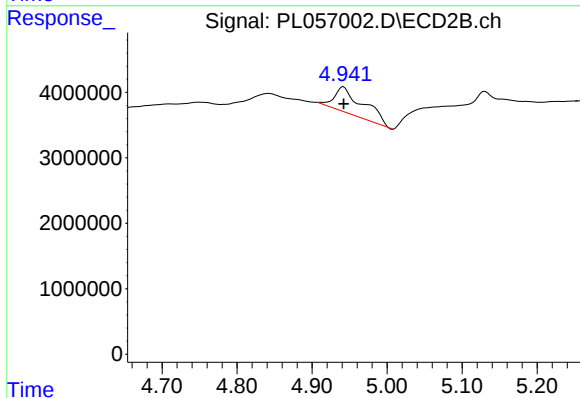


#23 Chlordane-1

R.T.: 4.942 min
Delta R.T.: 0.000 min
Response: 10734428
Conc: 133.83 ng/ml

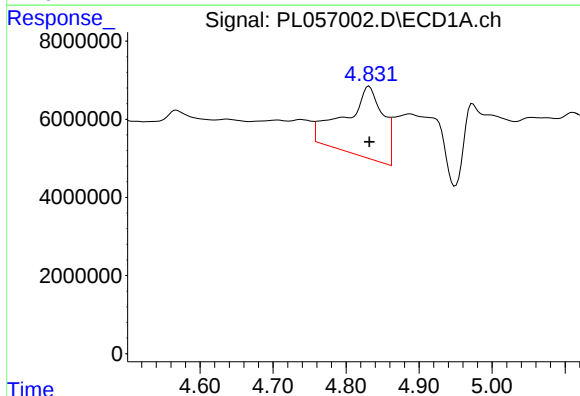


#24 Chlordane-2

R.T.: 4.832 min
Delta R.T.: 0.000 min
Response: 67003845
Conc: 189.99 ng/ml

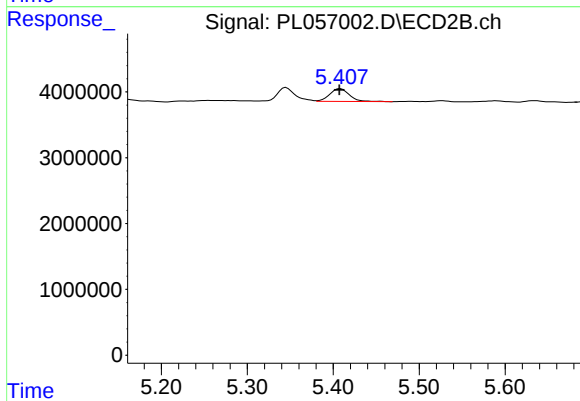


#24 Chlordane-2

R.T.: 5.408 min
Delta R.T.: 0.000 min
Response: 3100956
Conc: 32.49 ng/ml

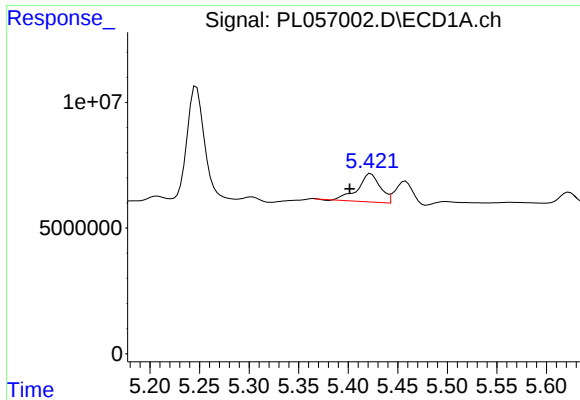


#25 Chlordane-3

R.T.: 5.423 min
Delta R.T.: 0.021 min
Response: 17806508
Conc: 16.51 ng/ml

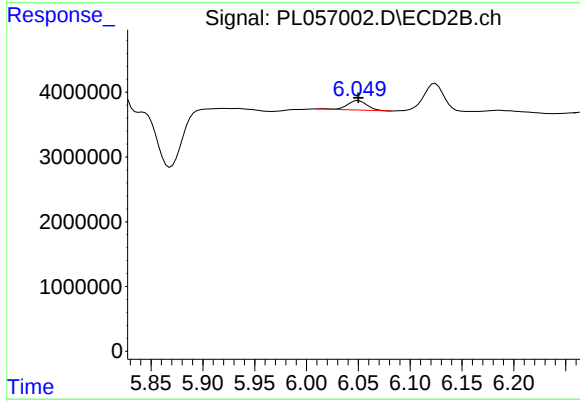


#25 Chlordane-3

R.T.: 6.050 min
Delta R.T.: 0.000 min
Response: 1965736
Conc: 5.19 ng/ml

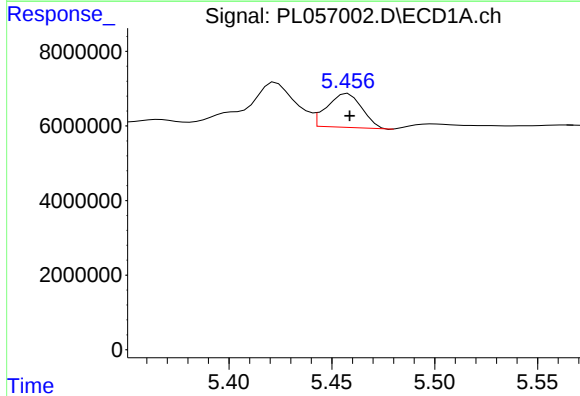


#26 Chlordane-4

R.T.: 5.458 min
Delta R.T.: 0.000 min
Response: 10779171
Conc: 11.73 ng/ml

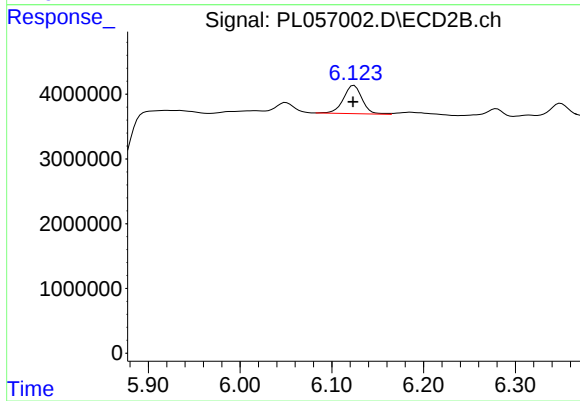


#26 Chlordane-4

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 6178812
Conc: 13.48 ng/ml

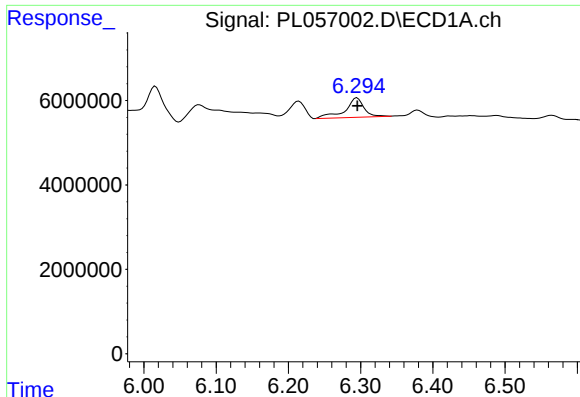


#27 Chlordane-5

R.T.: 6.295 min
Delta R.T.: 0.000 min
Response: 8369337
Conc: 23.04 ng/ml

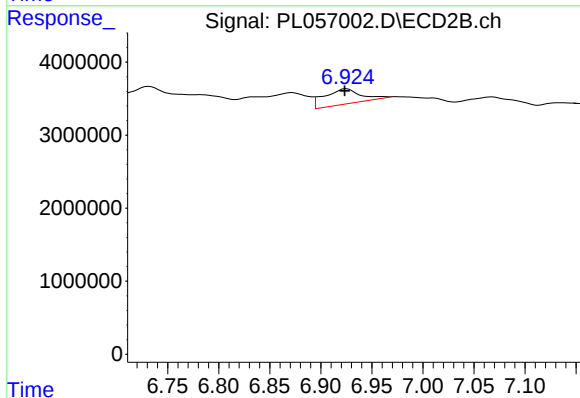


#27 Chlordane-5

R.T.: 6.925 min
Delta R.T.: 0.002 min
Response: 5111516
Conc: 61.27 ng/ml

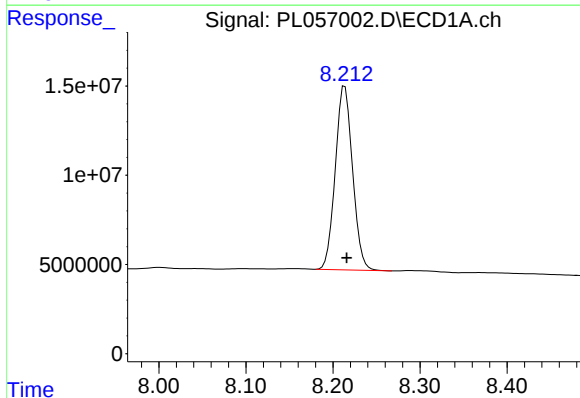

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.002 min
Response: 142134972
Conc: 14.71 ng/ml

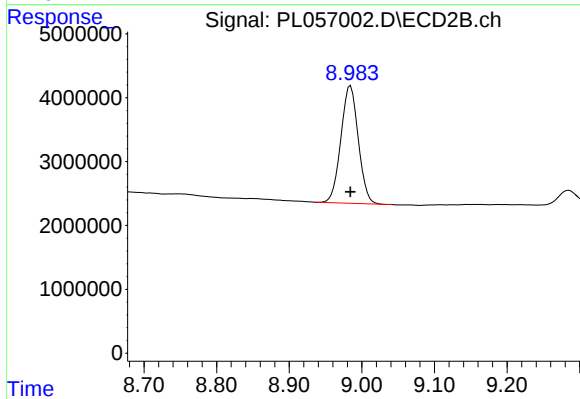

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 30588465
Conc: 14.40 ng/ml