

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL057009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 07:23
 Operator : AJ\MA
 Sample : L1762-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 07:56:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	111.0E6	28107596	13.022	13.174
28)	SA Decachlor...	8.213	8.984	105.3E6	24628968	10.899	11.591
Target Compounds							
4)	MA Heptachlor	4.482	5.132	-328560	21232075	N.D.	6.822
5)	MB Aldrin	0.000	5.408f	0	2927713	N.D.	0.979 #
10)	B gamma-Chl...	5.422	0.000	4409983	0	0.355	N.D. #
11)	B alpha-Chl...	0.000	6.124	0	2508675	N.D.	0.832 #
12)	B 4,4'-DDE	5.622	6.278	7887543	2144374	0.673	0.756
15)	B Endosulfa...	0.000	6.871	0	2232728	N.D.	0.796 #
17)	MA 4,4'-DDT	6.377	0.000	4952690	0	0.506	N.D. #
24)	Chlordane-2	0.000	5.408	0	2927713	N.D.	30.671 #
25)	Chlordane-3	5.422f	0.000	4409983	0	4.088	N.D. #
26)	Chlordane-4	0.000	6.124	0	2508675	N.D.	5.471 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL057009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 07:23
Operator : AJ\MA
Sample : L1762-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 07:56:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

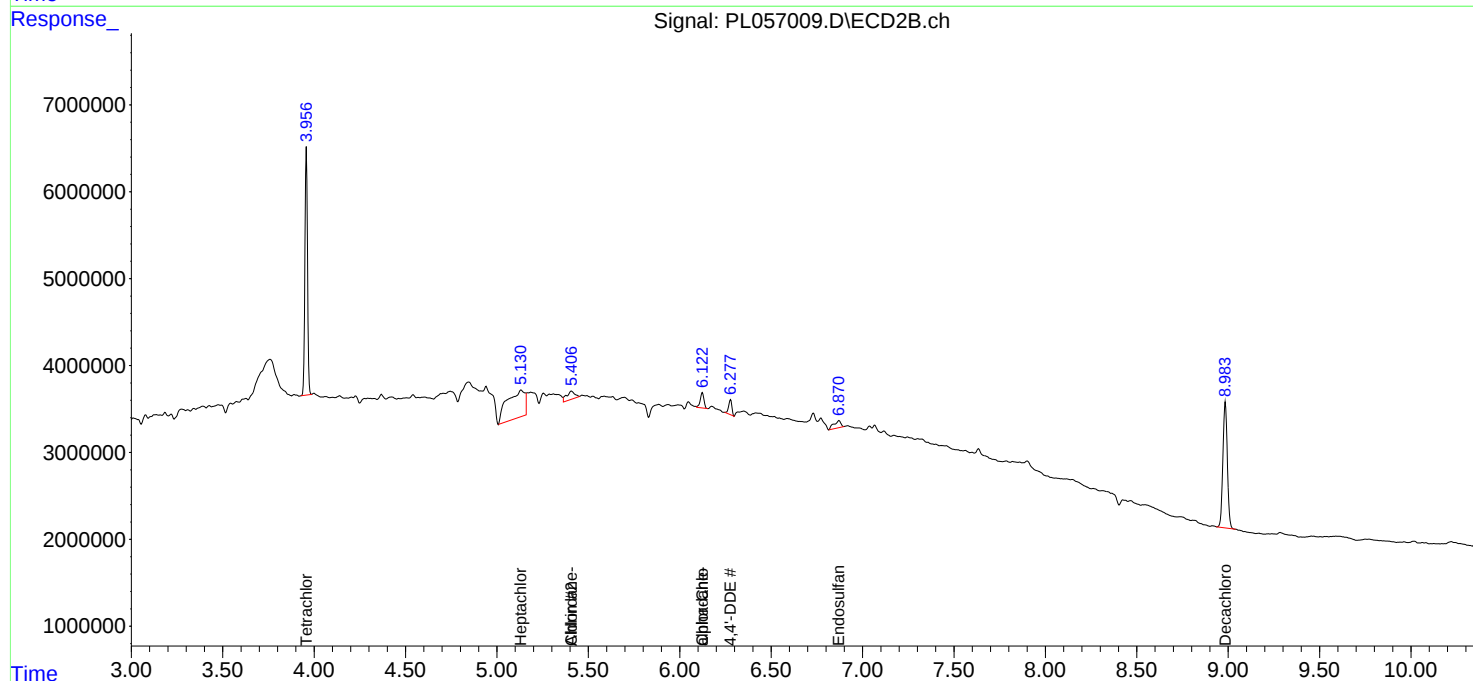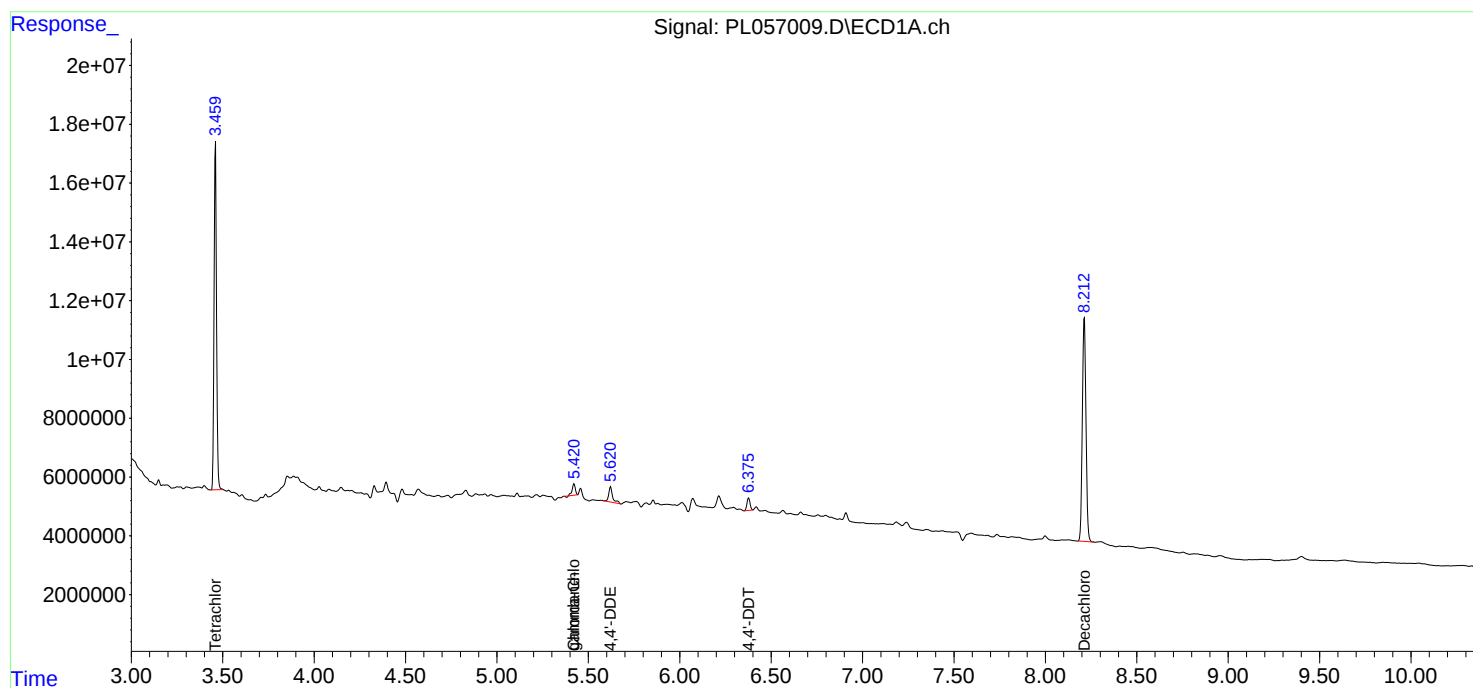

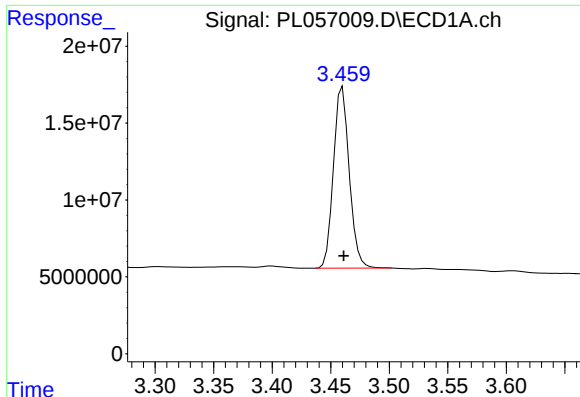


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 110981371
Conc: 13.02 ng/ml

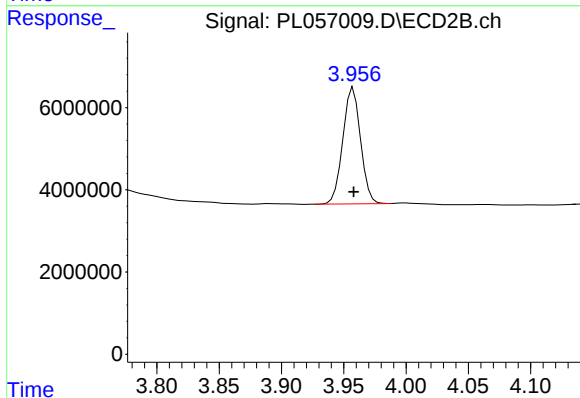


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 28107596
Conc: 13.17 ng/ml

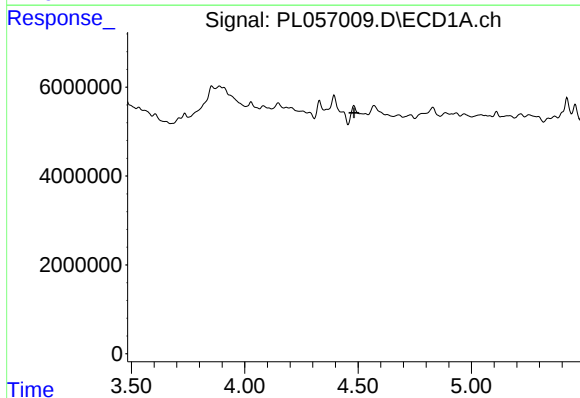


#4 Heptachlor

R.T.: 4.482 min
Delta R.T.: -0.001 min
Response: -328560
Conc: N.D.

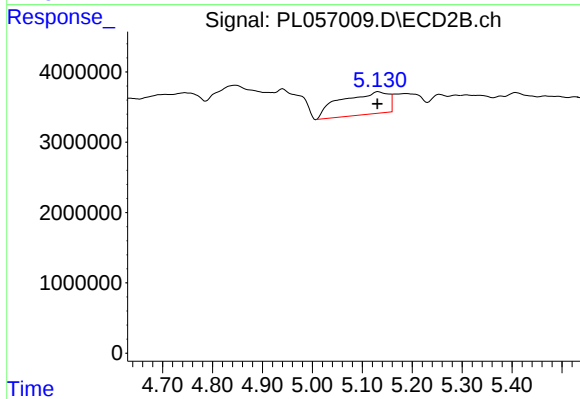


#4 Heptachlor

R.T.: 5.132 min
Delta R.T.: 0.001 min
Response: 21232075
Conc: 6.82 ng/ml

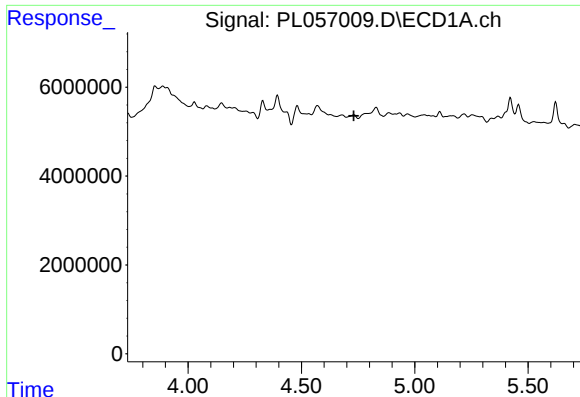


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

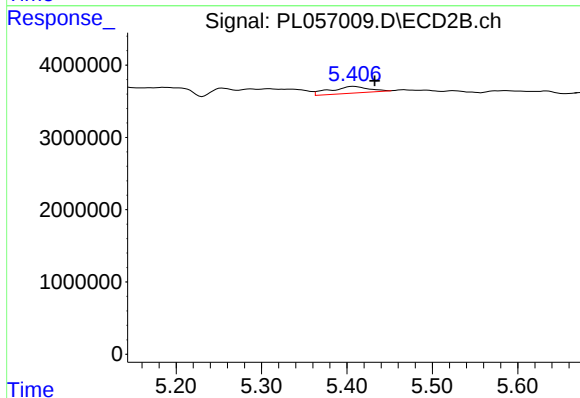


#5 Aldrin

R.T.: 5.408 min
Delta R.T.: -0.025 min
Response: 2927713
Conc: 0.98 ng/ml

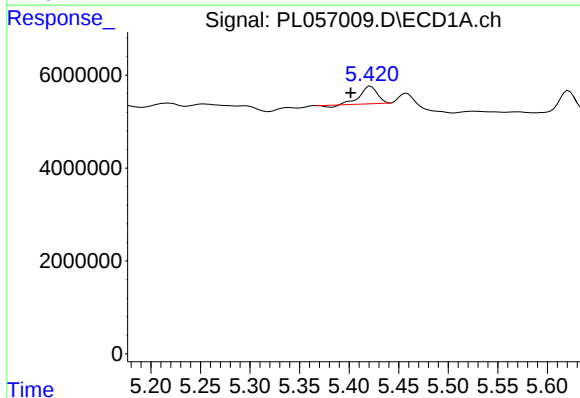


#10 gamma-Chlordane

R.T.: 5.422 min
Delta R.T.: 0.020 min
Response: 4409983
Conc: 0.36 ng/ml

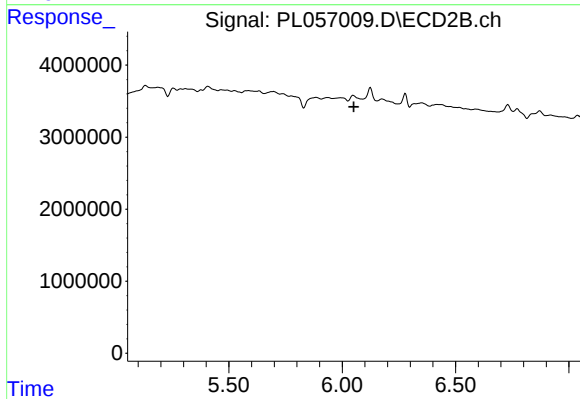


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

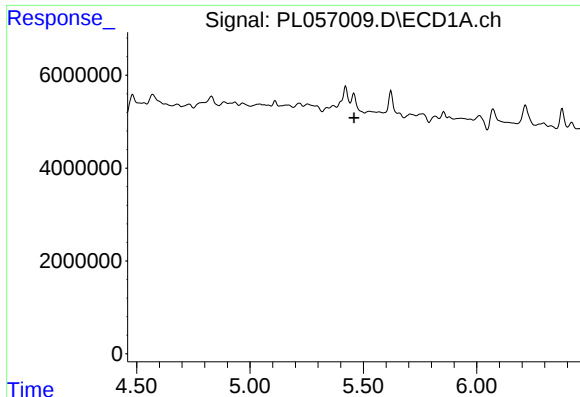


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

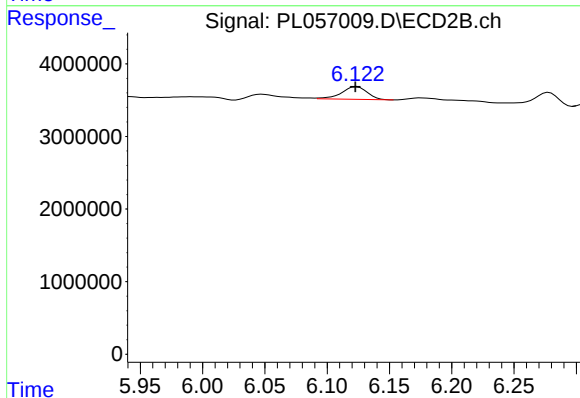


#11 alpha-Chlordane

R.T.: 6.124 min
Delta R.T.: 0.001 min
Response: 2508675
Conc: 0.83 ng/ml

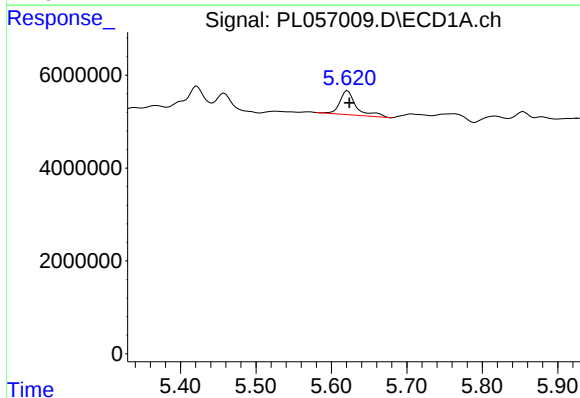


#12 4,4'-DDE

R.T.: 5.622 min
Delta R.T.: -0.002 min
Response: 7887543
Conc: 0.67 ng/ml

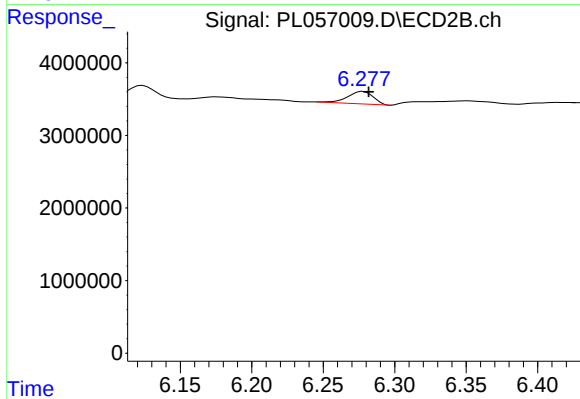


#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: -0.004 min
Response: 2144374
Conc: 0.76 ng/ml

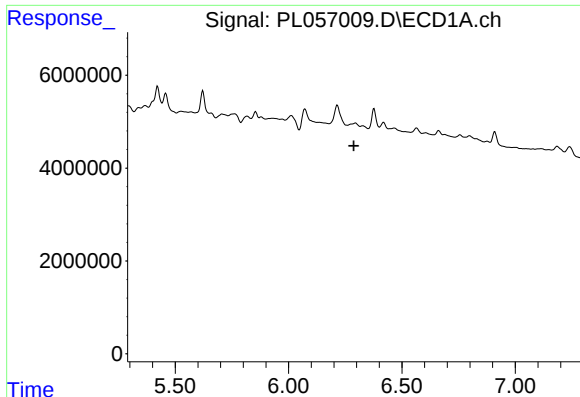


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

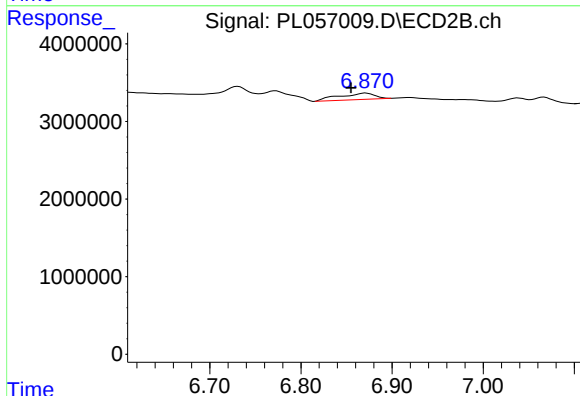


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.016 min
Response: 2232728
Conc: 0.80 ng/ml

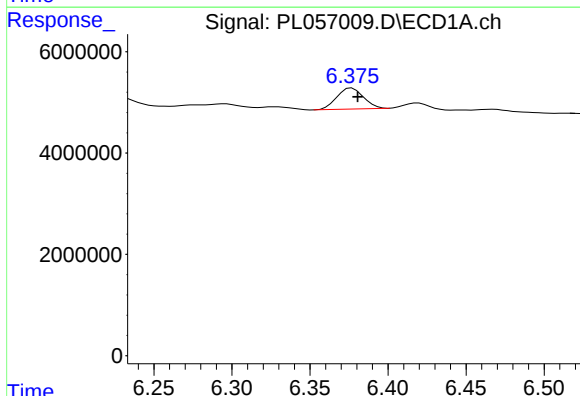


#17 4,4'-DDT

R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 4952690
Conc: 0.51 ng/ml

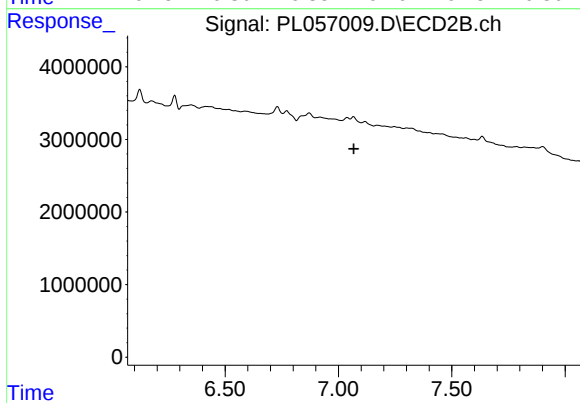


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.068 min
Response: 0
Conc: N.D.

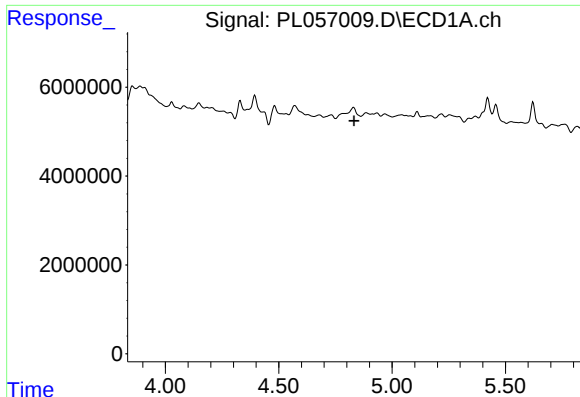


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

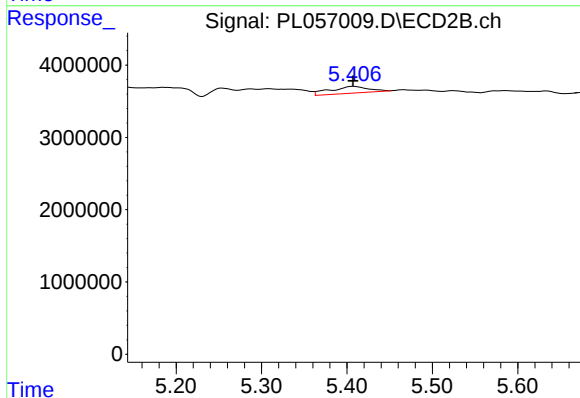


#24 Chlordane-2

R.T.: 5.408 min
Delta R.T.: 0.000 min
Response: 2927713
Conc: 30.67 ng/ml

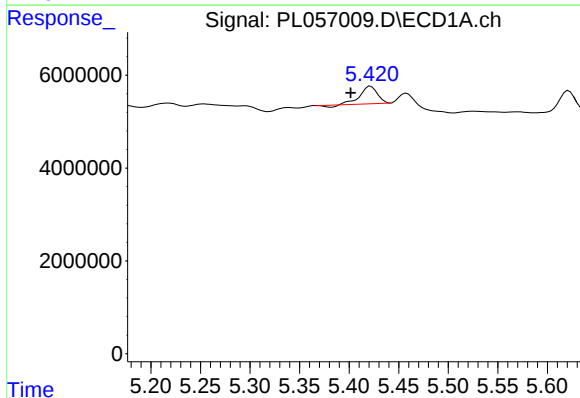


#25 Chlordane-3

R.T.: 5.422 min
Delta R.T.: 0.020 min
Response: 4409983
Conc: 4.09 ng/ml

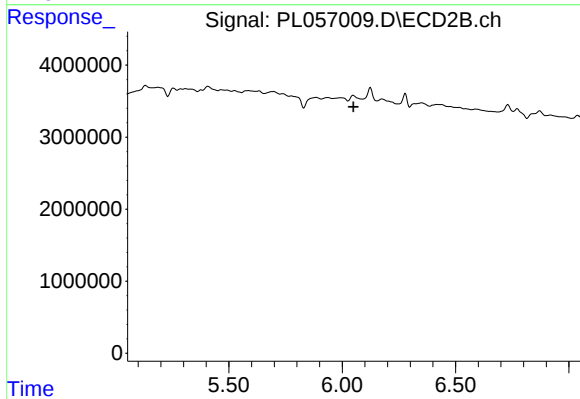


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

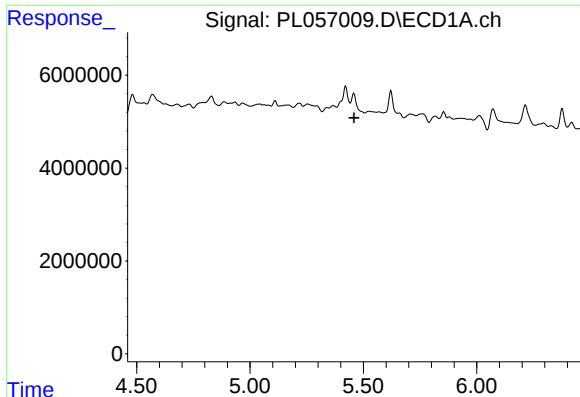


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

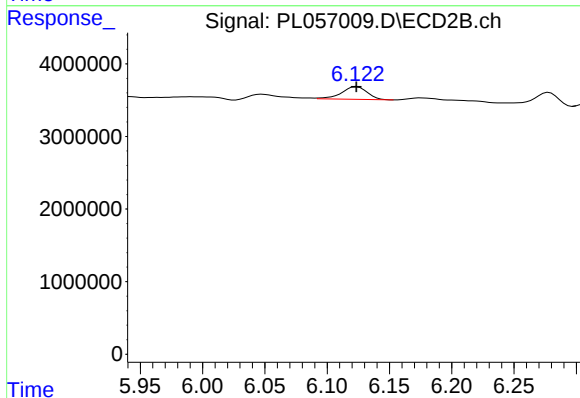


#26 Chlordane-4

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 2508675
Conc: 5.47 ng/ml

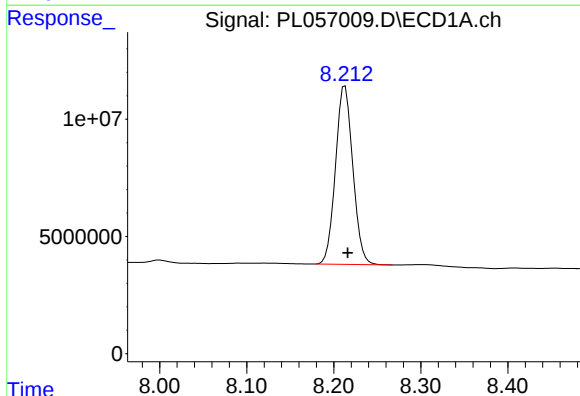

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 105343014
Conc: 10.90 ng/ml

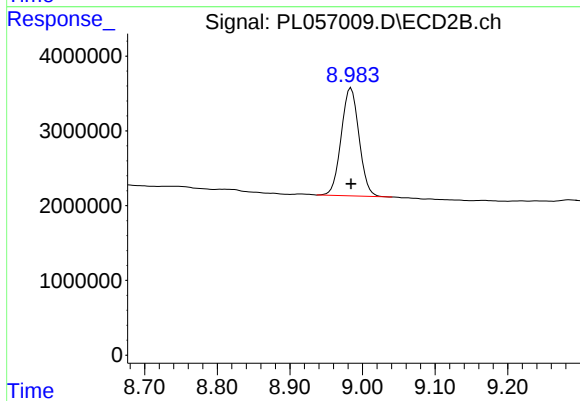

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 24628968
Conc: 11.59 ng/ml