

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL057010.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 07:37
 Operator : AJ\MA
 Sample : L1757-06
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 15:18:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	196.7E6	49909831	23.079	23.393
28)	SA Decachlor...	8.213	8.984	187.5E6	42714501	19.405	20.103
Target Compounds							
4)	MA Heptachlor	0.000	5.140	0	18903237	N.D.	6.074 #
7)	B delta-BHC	0.000	4.982f	0	9449897	N.D.	3.881 #
8)	B Heptachlo...	0.000	5.800	0	13341575	N.D.	4.815 #
15)	B Endosulfa...	0.000	6.871	0	3557065	N.D.	1.268 #
19)	B Endosulfa...	6.660	7.170f	9001449	2000441	0.901	0.798
23)	Chlordane-1	4.357f	0.000	2620472	0	8.621	N.D. #
24)	Chlordane-2	4.855f	0.000	34781027	0	98.624	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL057010.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 07:37
Operator : AJ\MA
Sample : L1757-06
Misc :
ALS Vial : 42 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 15:18:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

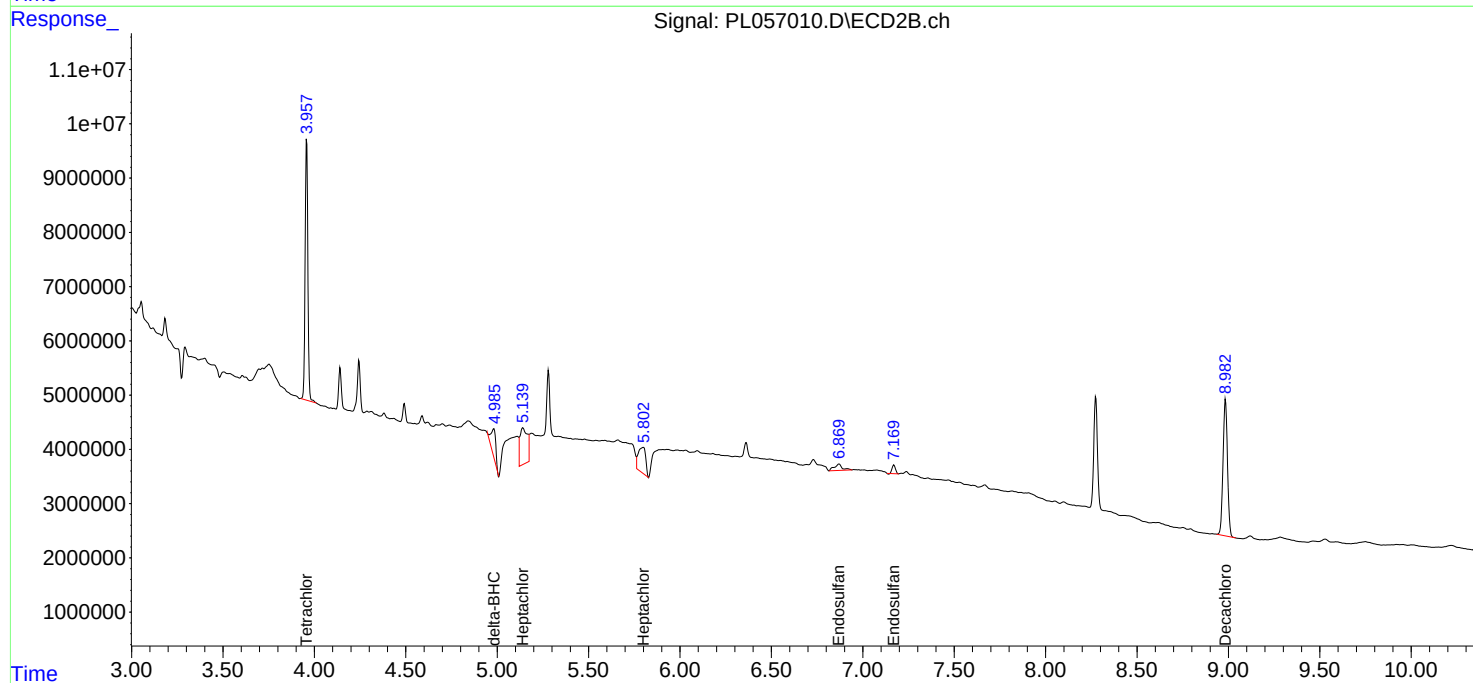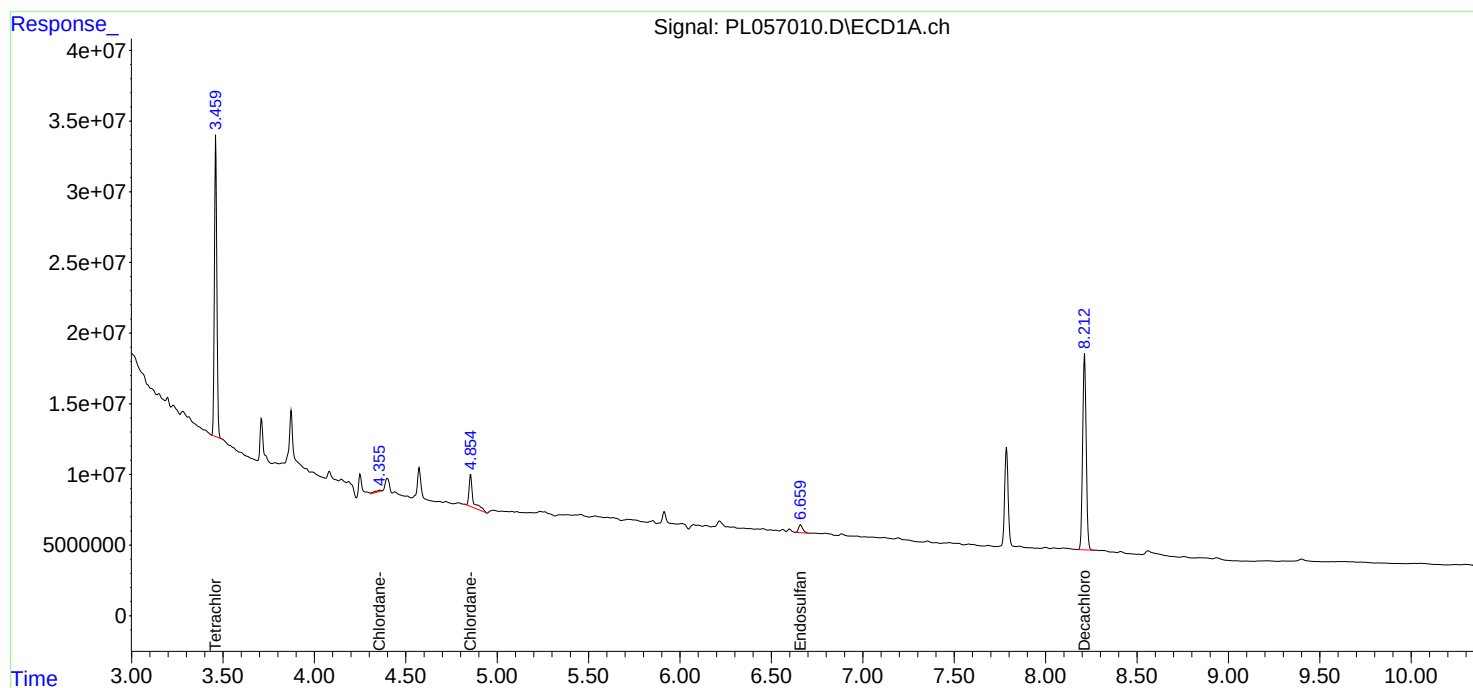

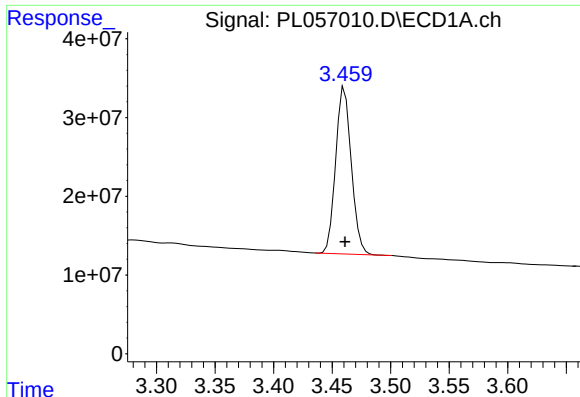


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 196682774
Conc: 23.08 ng/ml

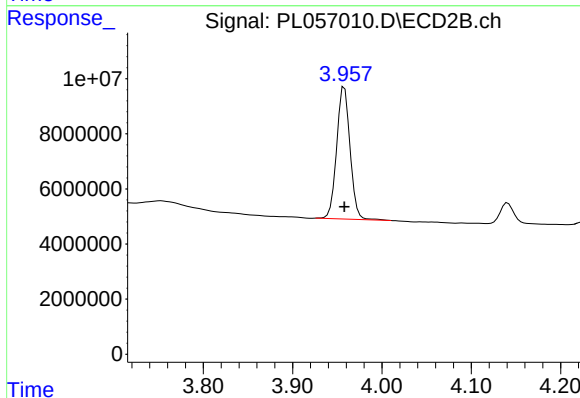


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 49909831
Conc: 23.39 ng/ml

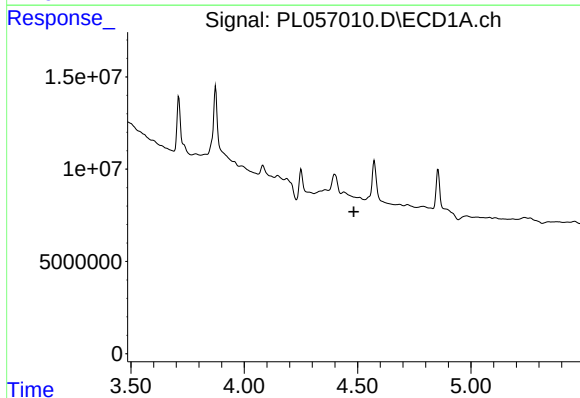


#4 Heptachlor

R.T.: 0.000 min
Exp R.T.: 4.483 min
Response: 0
Conc: N.D.

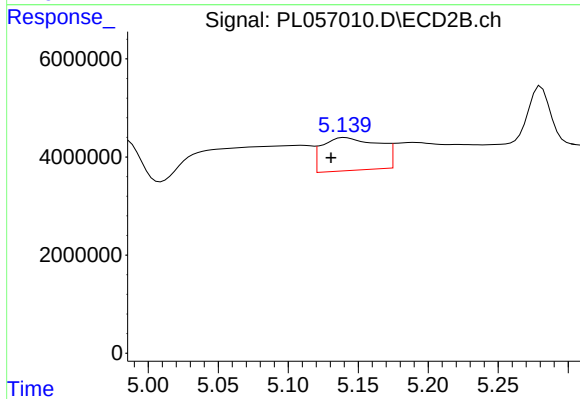


#4 Heptachlor

R.T.: 5.140 min
Delta R.T.: 0.010 min
Response: 18903237
Conc: 6.07 ng/ml

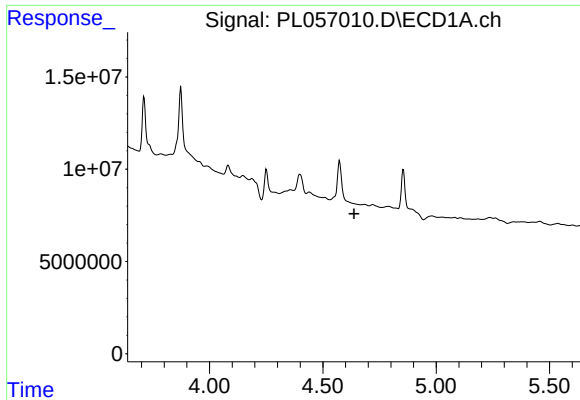


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.638 min
Response: 0
Conc: N.D.

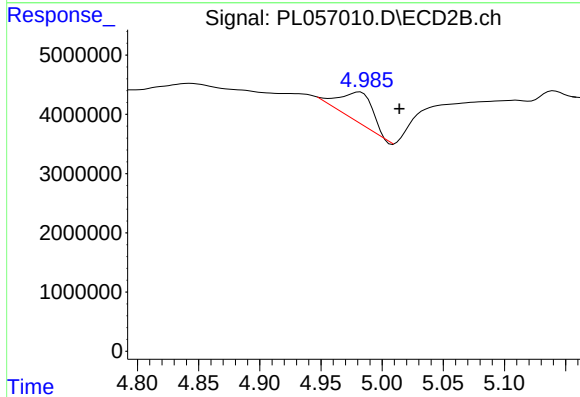


#7 delta-BHC

R.T.: 4.982 min
Delta R.T.: -0.032 min
Response: 9449897
Conc: 3.88 ng/ml

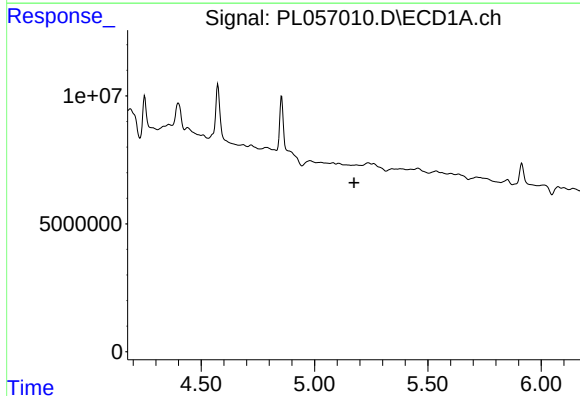


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

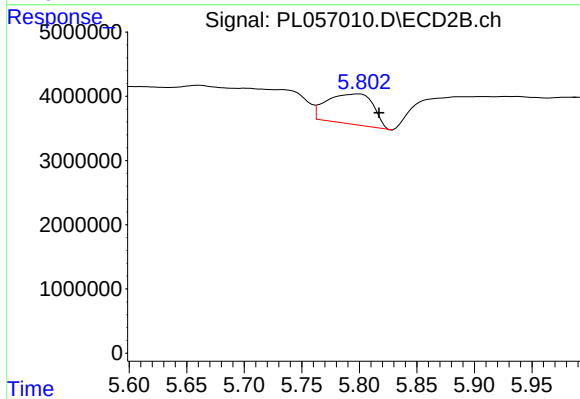


#8 Heptachlor epoxide

R.T.: 5.800 min
Delta R.T.: -0.017 min
Response: 13341575
Conc: 4.81 ng/ml

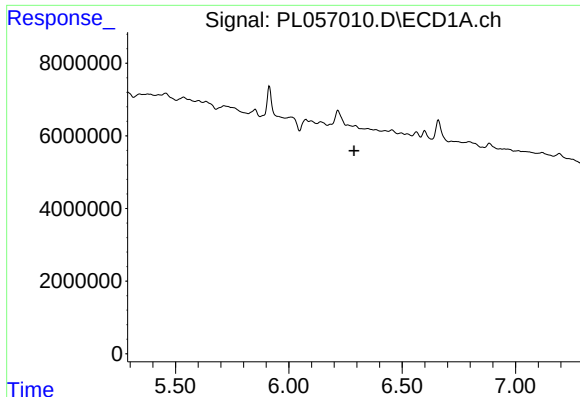


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

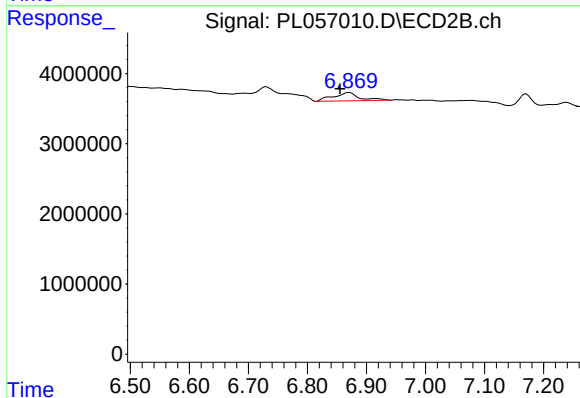


#15 Endosulfan II

R.T.: 6.871 min
Delta R.T.: 0.016 min
Response: 3557065
Conc: 1.27 ng/ml

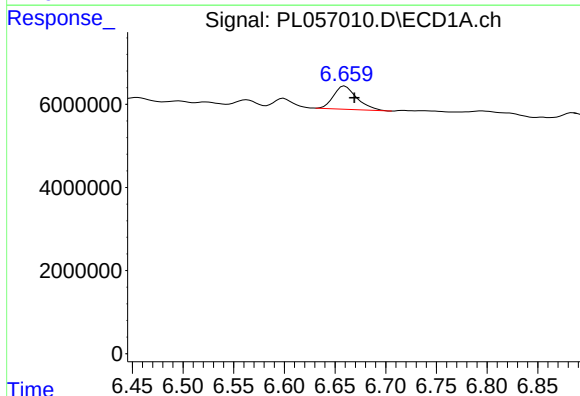


#19 Endosulfan Sulfate

R.T.: 6.660 min
Delta R.T.: -0.010 min
Response: 9001449
Conc: 0.90 ng/ml

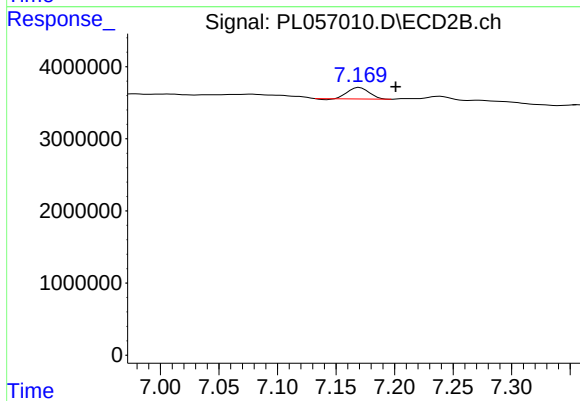


#19 Endosulfan Sulfate

R.T.: 7.170 min
Delta R.T.: -0.031 min
Response: 2000441
Conc: 0.80 ng/ml

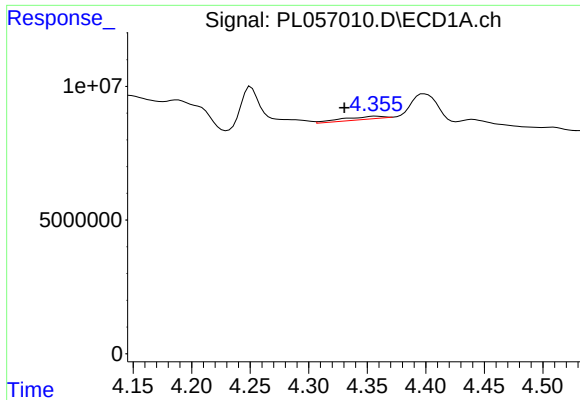


#23 Chlordane-1

R.T.: 4.357 min
Delta R.T.: 0.027 min
Response: 2620472
Conc: 8.62 ng/ml

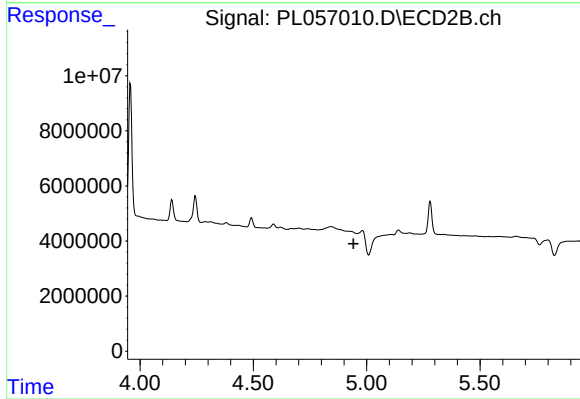


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

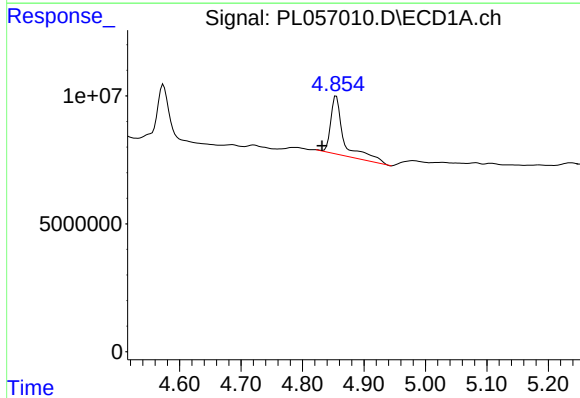


#24 Chlordane-2

R.T.: 4.855 min
Delta R.T.: 0.023 min
Response: 34781027
Conc: 98.62 ng/ml

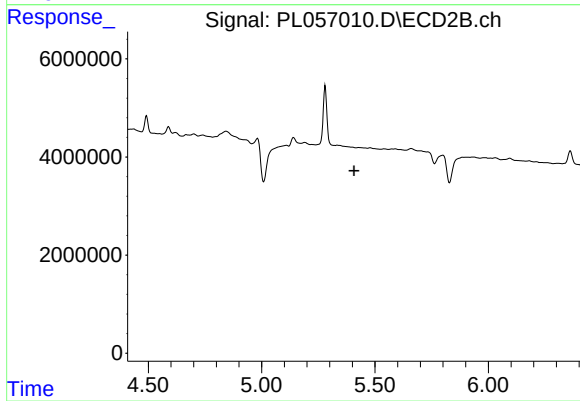


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 5.407 min
Response: 0
Conc: N.D.

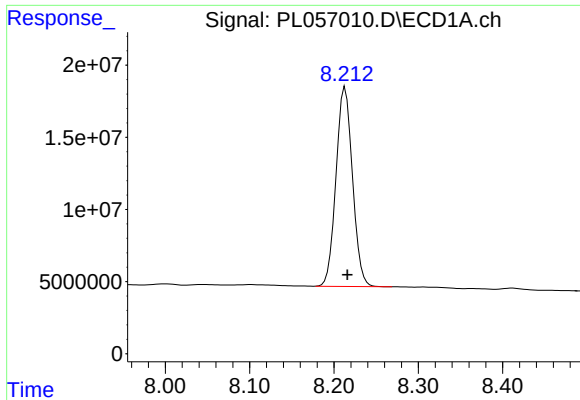

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 187549896
Conc: 19.40 ng/ml

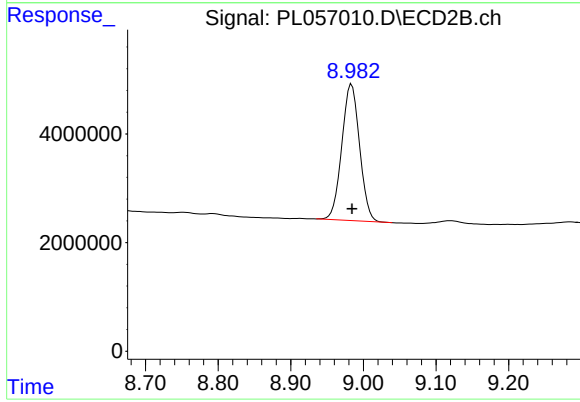

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 42714501
Conc: 20.10 ng/ml