

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL057011.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 07:51
 Operator : AJ\MA
 Sample : L1372-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 15:18:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	184.1E6	46284268	21.597	21.694
28)	SA Decachlor...	8.213	8.984	171.7E6	38593137	17.764	18.164
Target Compounds							
4)	MA Heptachlor	0.000	5.140	0	30724283	N.D.	9.872 #
8)	B Heptachlo...	0.000	5.801	0	12451061	N.D.	4.493 #
15)	B Endosulfa...	0.000	6.872	0	2156912	N.D.	0.769 #
19)	B Endosulfa...	6.659	7.171f	15787149	3667871	1.581	1.463
23)	Chlordane-1	4.342	0.000	4761675	0	15.666	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL057011.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 07:51
Operator : AJ\MA
Sample : L1372-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 15:18:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

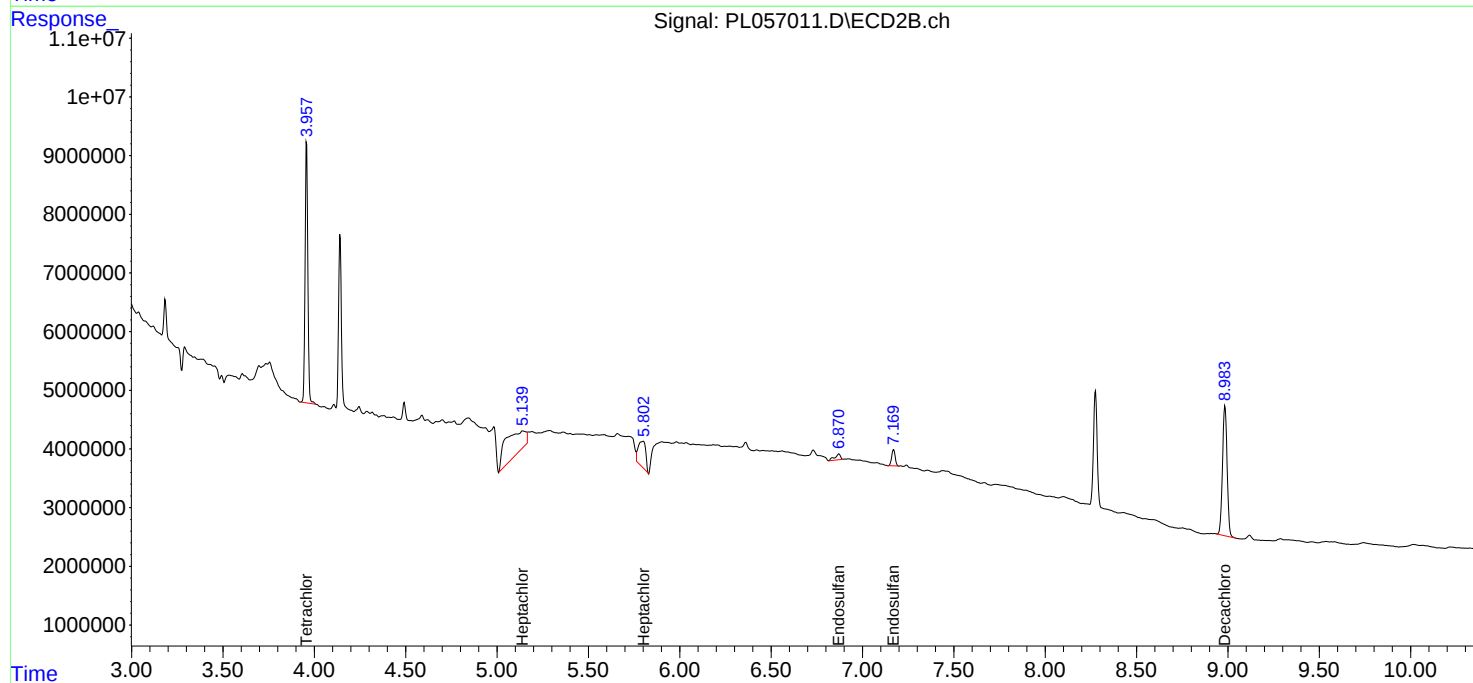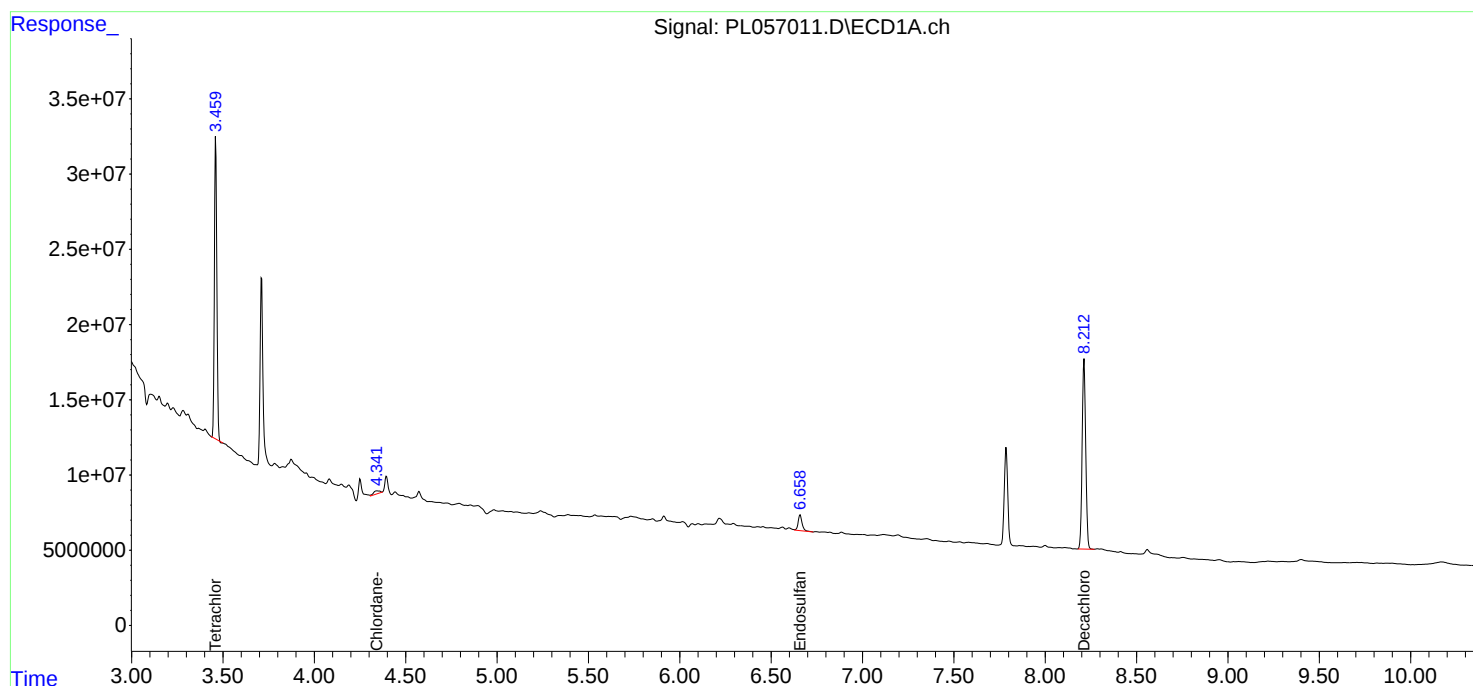

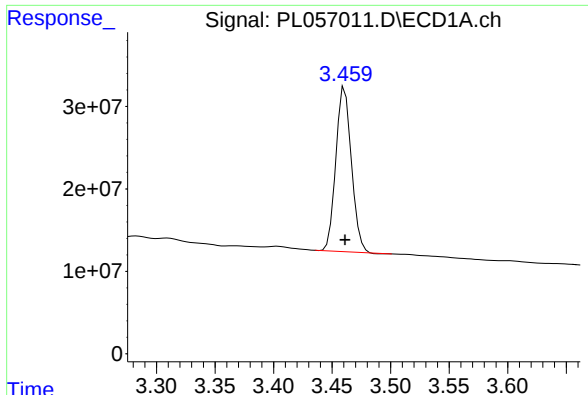


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 184054430
Conc: 21.60 ng/ml

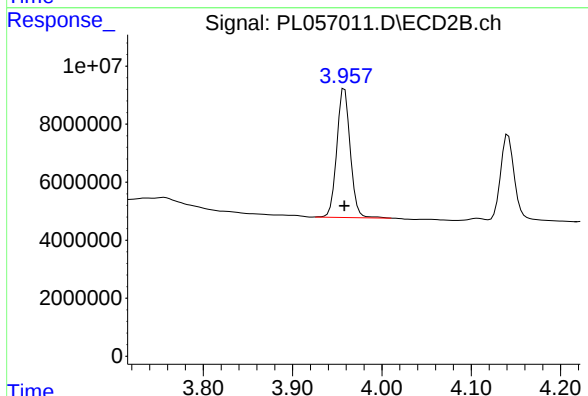


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 46284268
Conc: 21.69 ng/ml

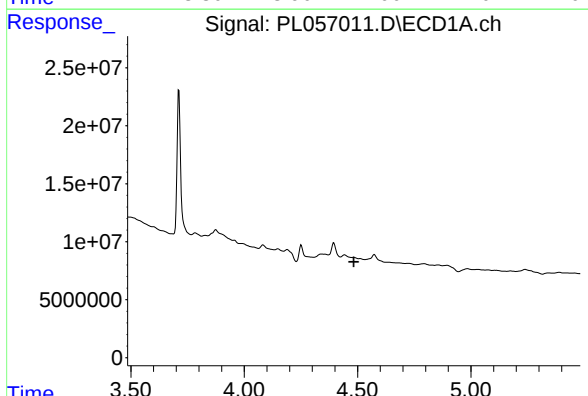


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

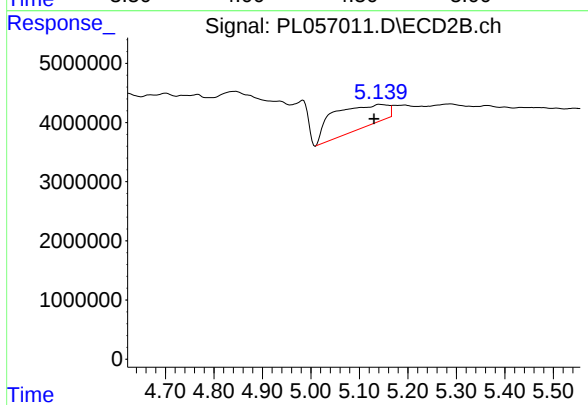


#4 Heptachlor

R.T.: 5.140 min
Delta R.T.: 0.010 min
Response: 30724283
Conc: 9.87 ng/ml

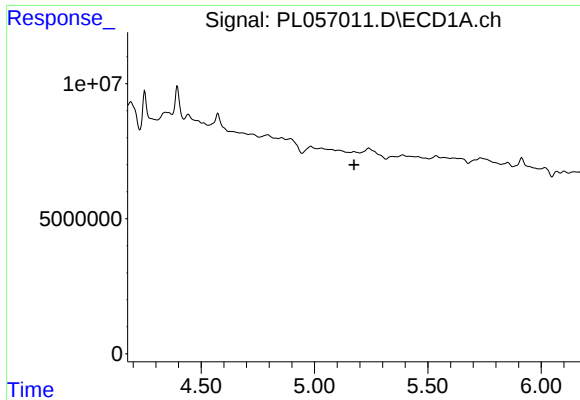


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

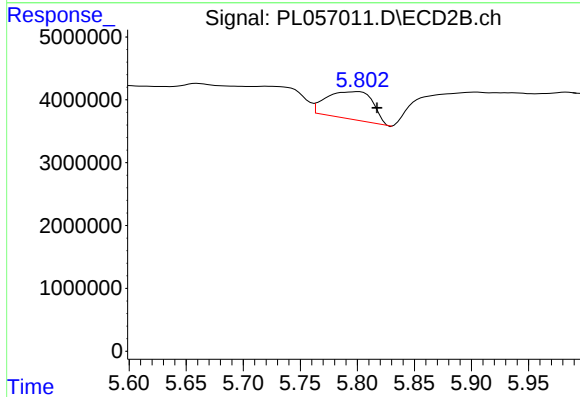


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: -0.016 min
Response: 12451061
Conc: 4.49 ng/ml

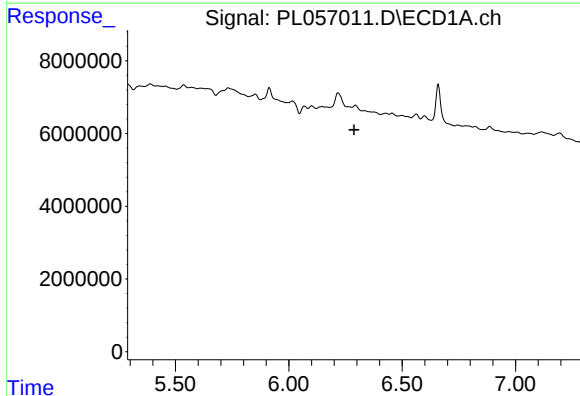


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

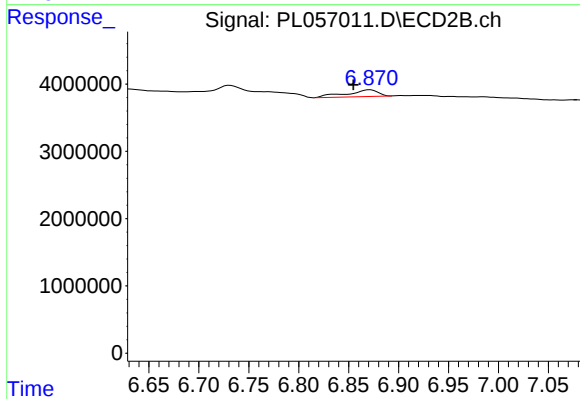


#15 Endosulfan II

R.T.: 6.872 min
Delta R.T.: 0.017 min
Response: 2156912
Conc: 0.77 ng/ml

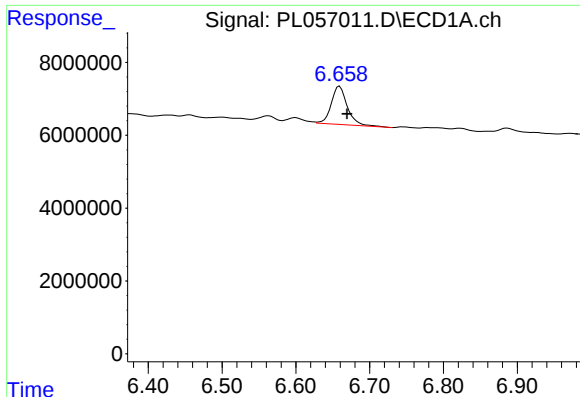


#19 Endosulfan Sulfate

R.T.: 6.659 min
Delta R.T.: -0.010 min
Response: 15787149
Conc: 1.58 ng/ml

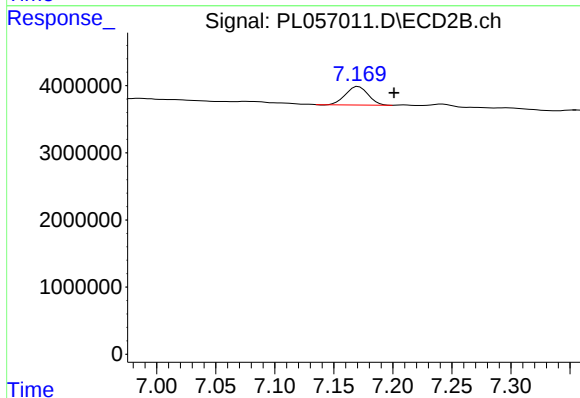


#19 Endosulfan Sulfate

R.T.: 7.171 min
Delta R.T.: -0.030 min
Response: 3667871
Conc: 1.46 ng/ml

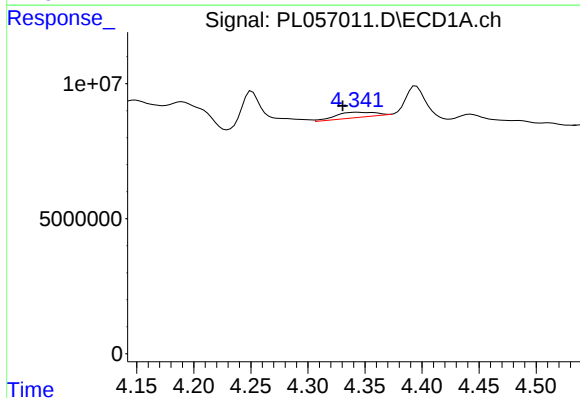


#23 Chlordane-1

R.T.: 4.342 min
Delta R.T.: 0.012 min
Response: 4761675
Conc: 15.67 ng/ml

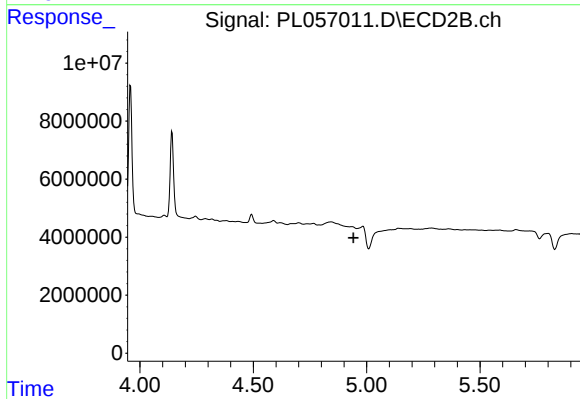


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

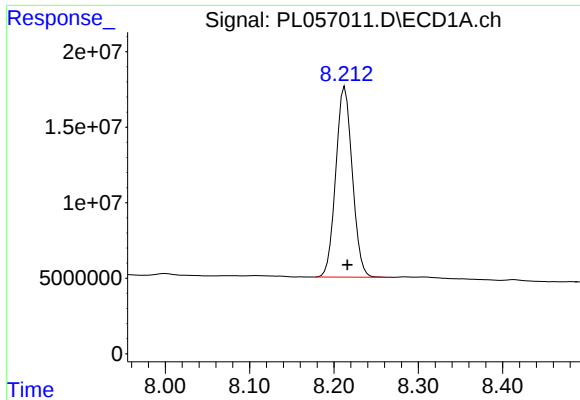

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 171688757
Conc: 17.76 ng/ml

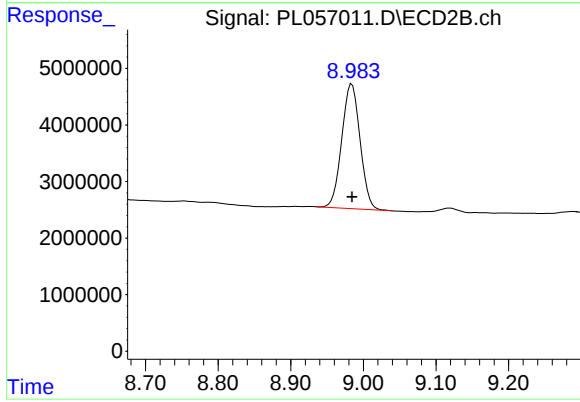

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 38593137
Conc: 18.16 ng/ml