

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL057015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 08:48
 Operator : AJ\MA
 Sample : L1745-02
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 15:19:16 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml



System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	188.0E6	49190393	22.056	23.056
28)	SA Decachlor...	8.212	8.983	200.2E6	43180842	20.719	20.323
Target Compounds							
4)	MA Heptachlor	0.000	5.145	0	21390854	N.D.	6.873 #
5)	MB Aldrin	0.000	5.456f	0	5429245	N.D.	1.816 #
8)	B Heptachlo...	0.000	5.801	0	19364229	N.D.	6.988 #
15)	B Endosulfa...	0.000	6.869	0	2936299	N.D.	1.046 #
19)	B Endosulfa...	6.659	7.170f	5833825	1783758	0.584	0.711
23)	Chlordane-1	4.334	0.000	8005748	0	26.339	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL057015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 08:48
Operator : AJ\MA
Sample : L1745-02
Misc :
ALS Vial : 47 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 15:19:16 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

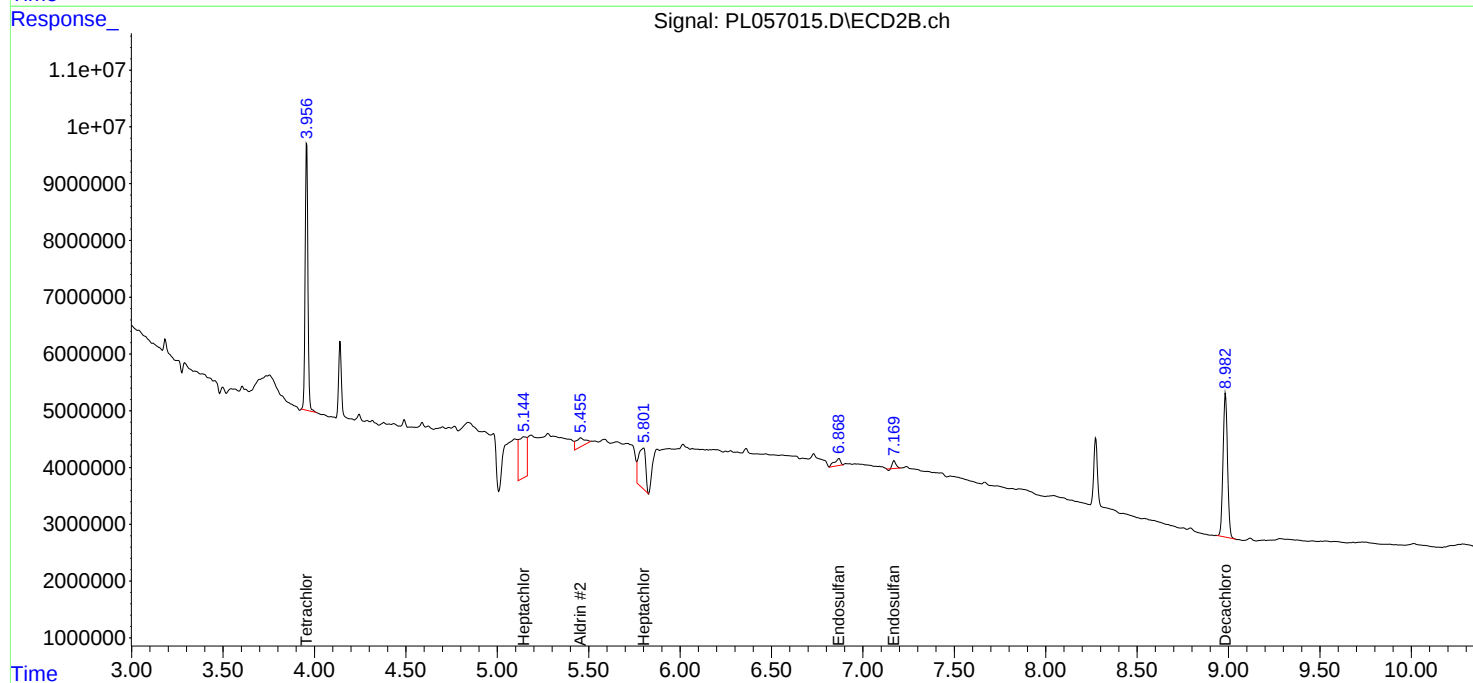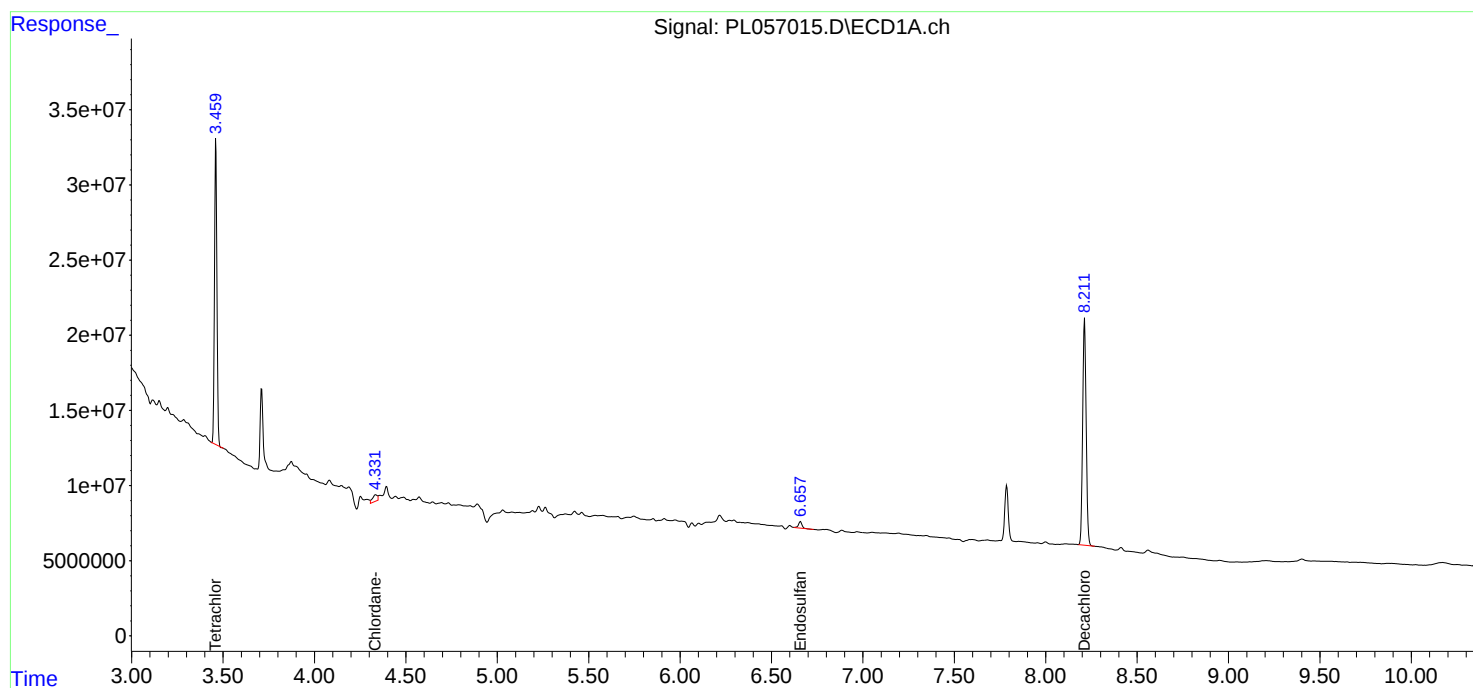

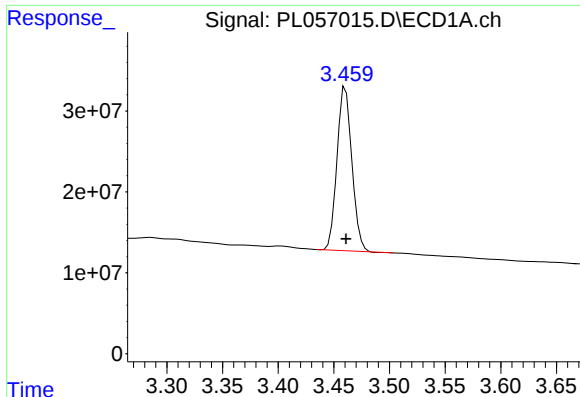


#1 Tetrachloro-m-xylene

R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 187964861
Conc: 22.06 ng/ml

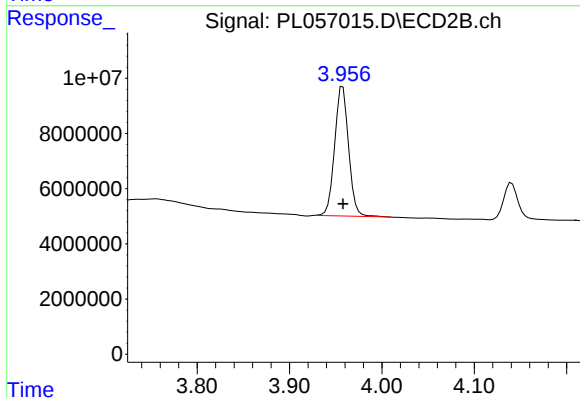


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 49190393
Conc: 23.06 ng/ml

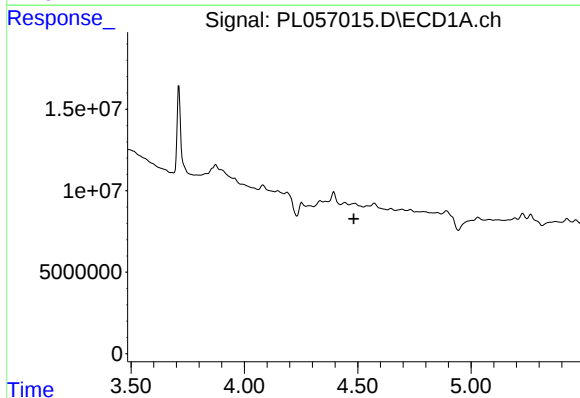


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

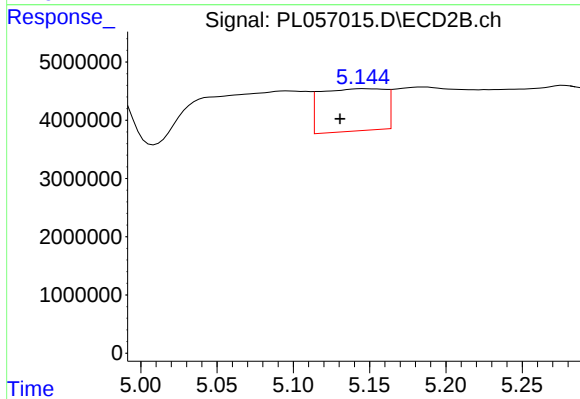


#4 Heptachlor

R.T.: 5.145 min
Delta R.T.: 0.015 min
Response: 21390854
Conc: 6.87 ng/ml

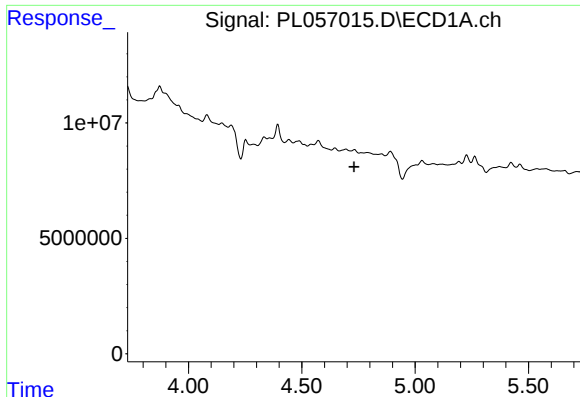


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

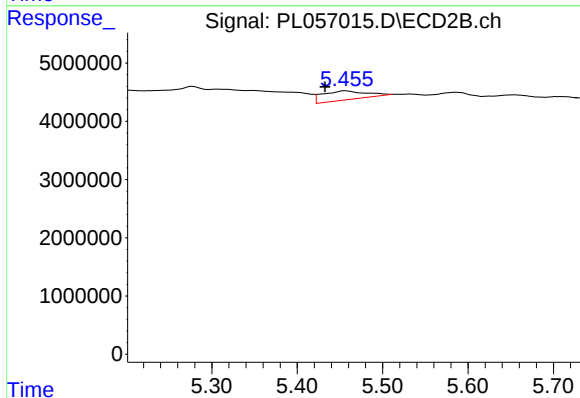


#5 Aldrin

R.T.: 5.456 min
Delta R.T.: 0.024 min
Response: 5429245
Conc: 1.82 ng/ml

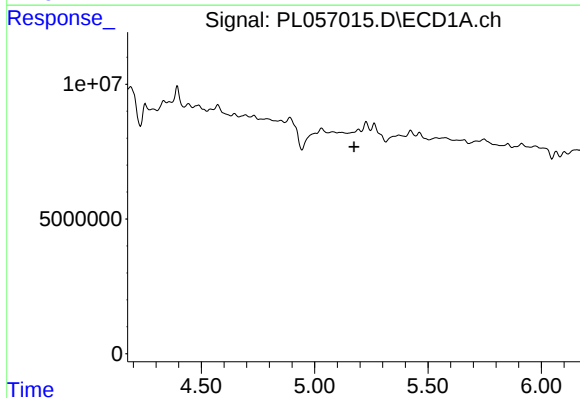


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

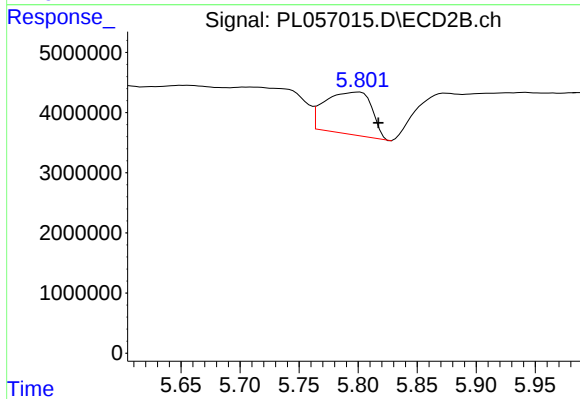


#8 Heptachlor epoxide

R.T.: 5.801 min
Delta R.T.: -0.016 min
Response: 19364229
Conc: 6.99 ng/ml

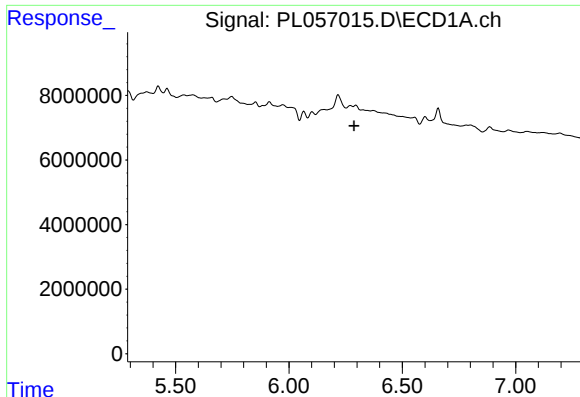


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

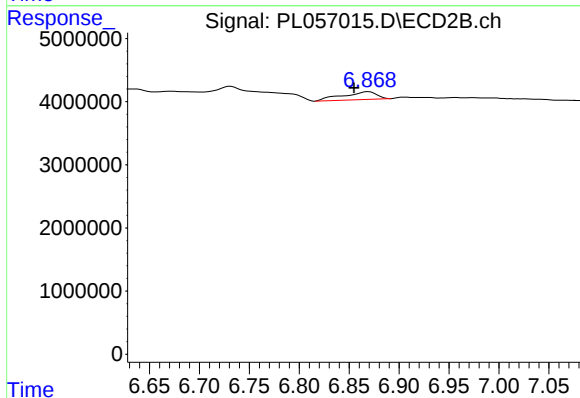


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.014 min
Response: 2936299
Conc: 1.05 ng/ml

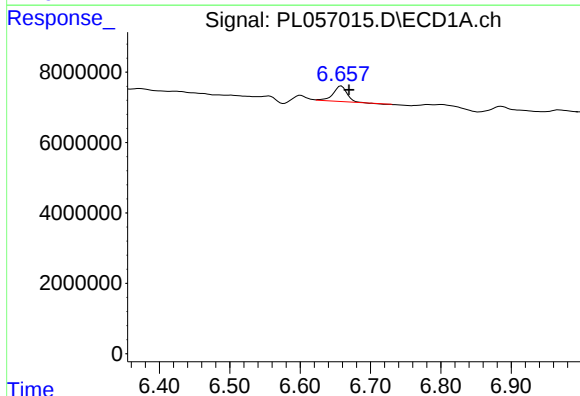


#19 Endosulfan Sulfate

R.T.: 6.659 min
Delta R.T.: -0.011 min
Response: 5833825
Conc: 0.58 ng/ml

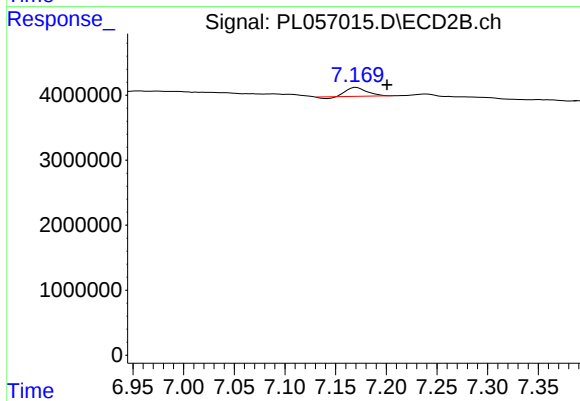


#19 Endosulfan Sulfate

R.T.: 7.170 min
Delta R.T.: -0.030 min
Response: 1783758
Conc: 0.71 ng/ml

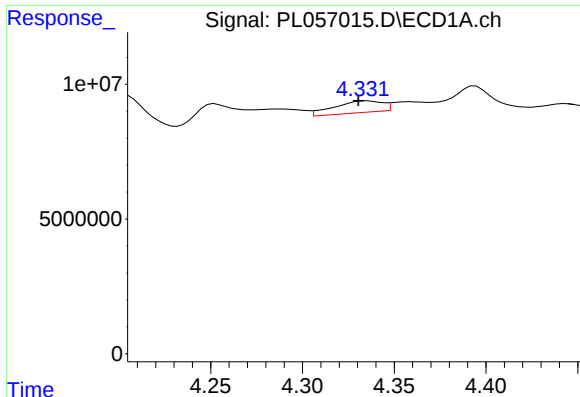


#23 Chlordane-1

R.T.: 4.334 min
Delta R.T.: 0.004 min
Response: 8005748
Conc: 26.34 ng/ml

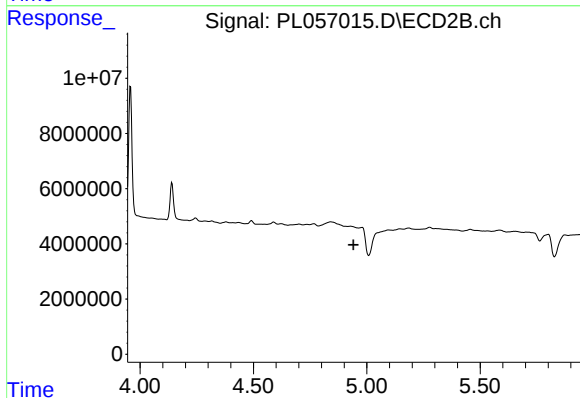


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

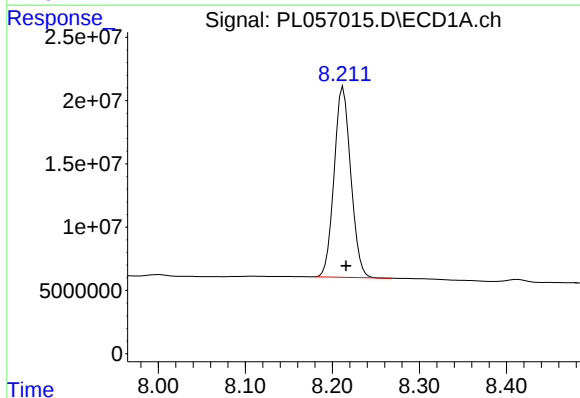

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.003 min
Response: 200249184
Conc: 20.72 ng/ml

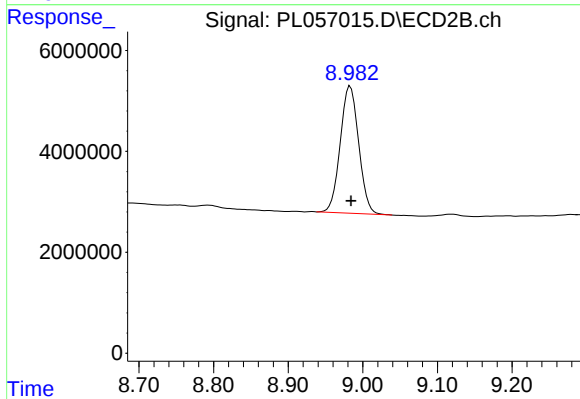

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: -0.001 min
Response: 43180842
Conc: 20.32 ng/ml