

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL056989.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 02:40
 Operator : AJ\MA
 Sample : L1737-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-BPM-03-013-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 04:37:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.958	202.0E6	50553678	23.699	23.695
28)	SA Decachlor...	8.215	8.985	209.0E6	43528496	21.620	20.486

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL056989.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 02:40
Operator : AJ\MA
Sample : L1737-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-013-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 04:37:58 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

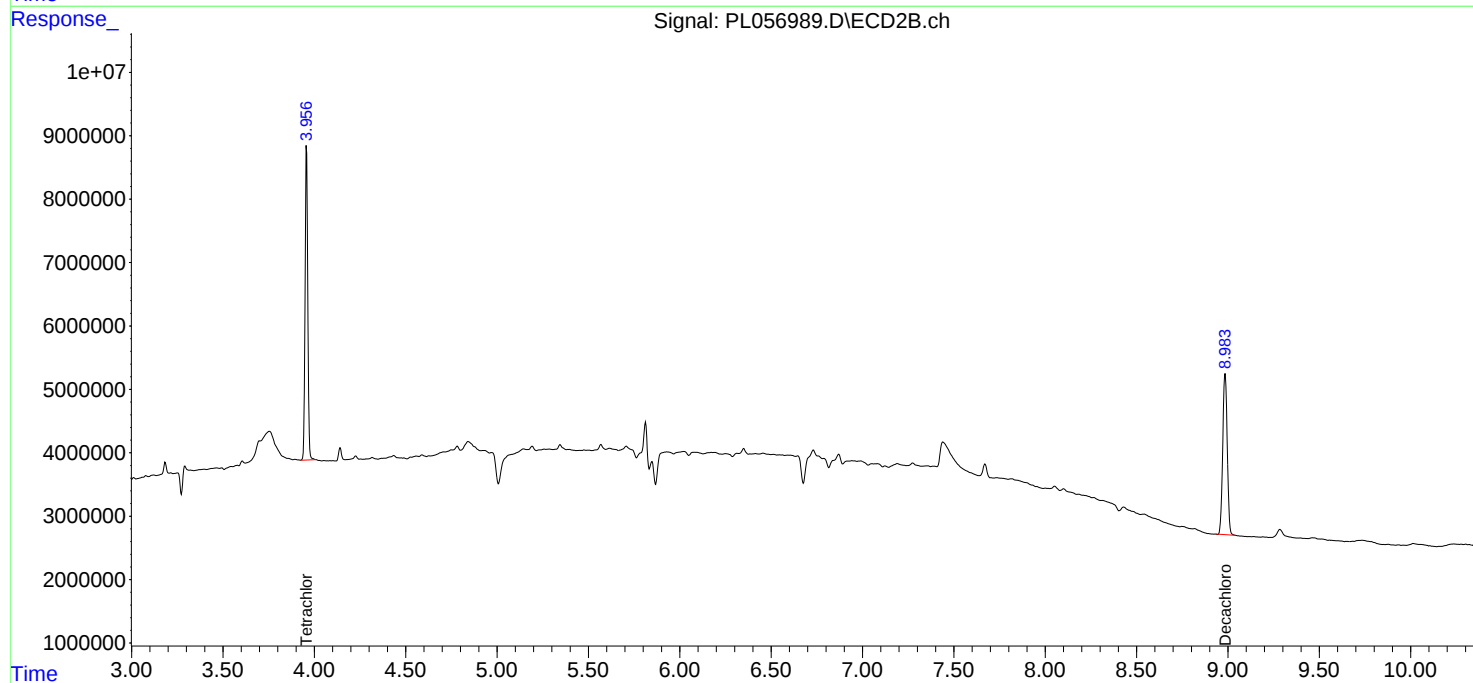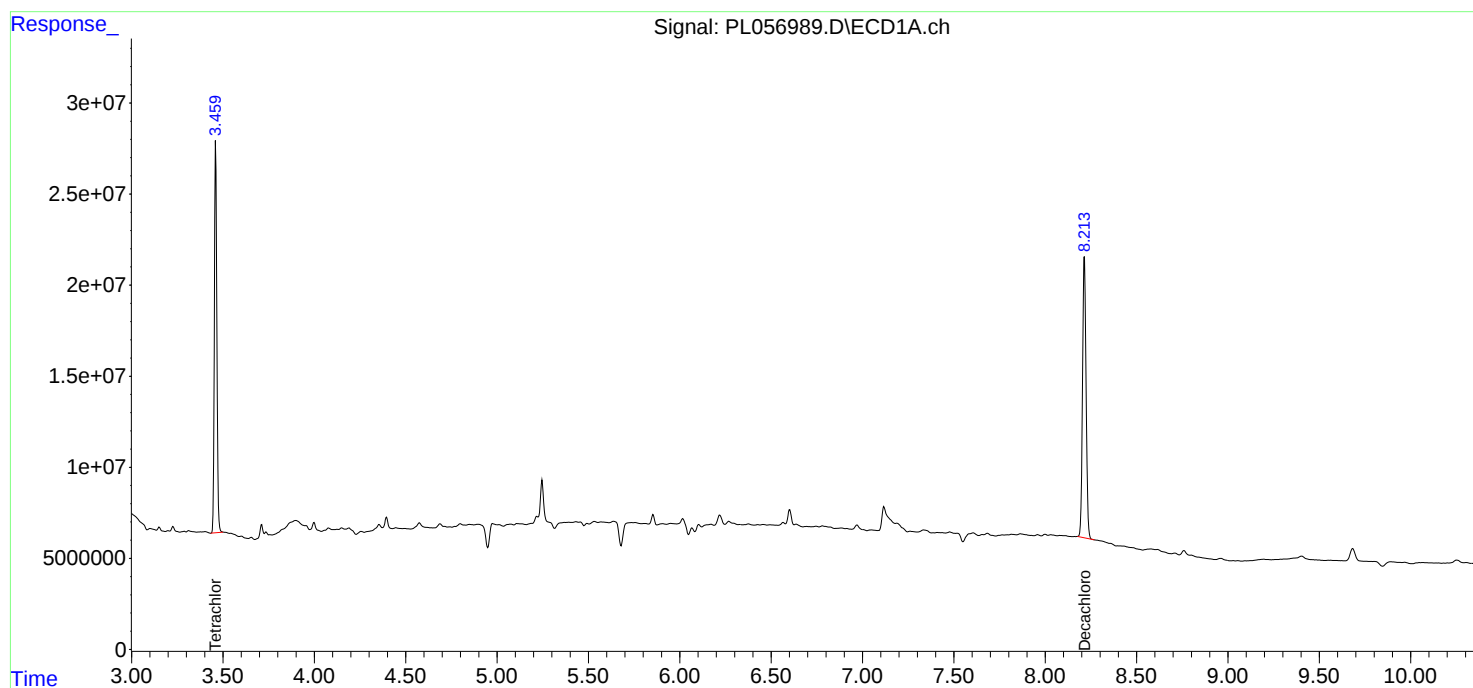


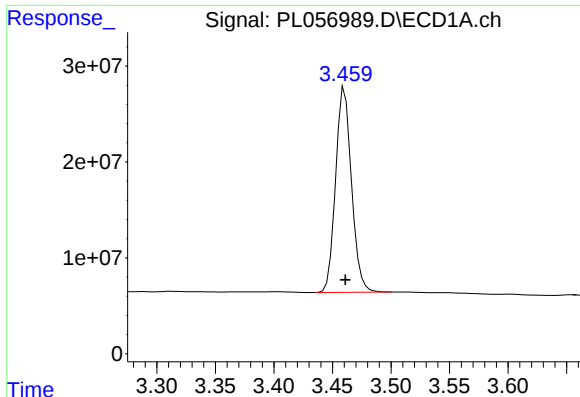

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 201966492
Conc: 23.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-03-013-ABCD

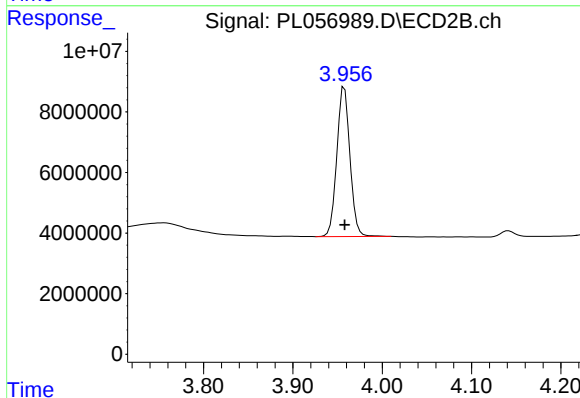


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 50553678
Conc: 23.70 ng/ml

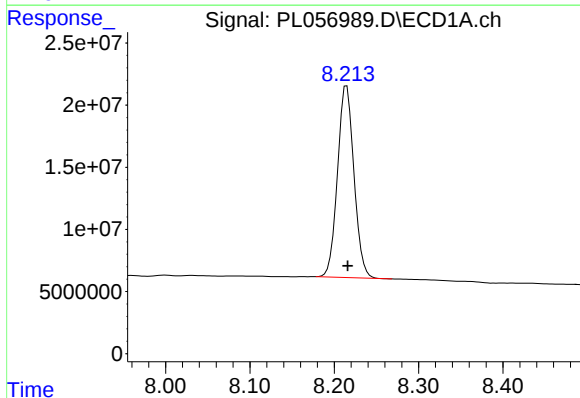

#28 Decachlorobiphenyl

R.T.: 8.215 min
Delta R.T.: -0.001 min
Response: 208955209
Conc: 21.62 ng/ml

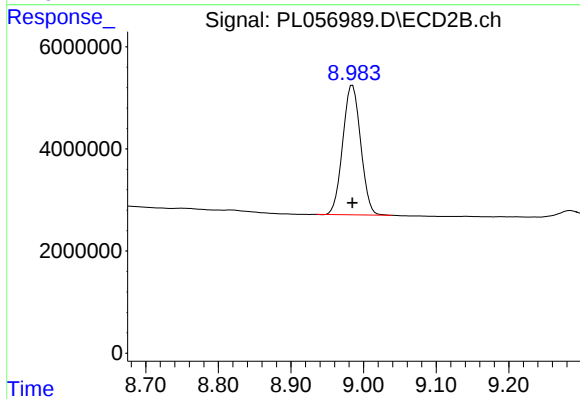

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.000 min
Response: 43528496
Conc: 20.49 ng/ml