

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
 Data File : PL057009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 07:23
 Operator : AJ\MA
 Sample : L1762-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-030220

Manual Integrations
 APPROVED

mohammad
 3/5/2020 11:40:38 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 07:56:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	111.0E6	28107596	13.022	13.174
28)	SA Decachlor...	8.213	8.984	105.3E6	24628968	10.899	11.591
Target Compounds							
12)	B 4,4'-DDE	5.620	6.278	5765988	2144374	0.492m	0.756 #
17)	MA 4,4'-DDT	6.377	7.065	4952690	1024941	0.506	0.417m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030320\
Data File : PL057009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 07:23
Operator : AJ\MA
Sample : L1762-01
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-04-030220


Manual Integrations
APPROVED

mohammad
3/5/2020 11:40:38 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 07:56:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

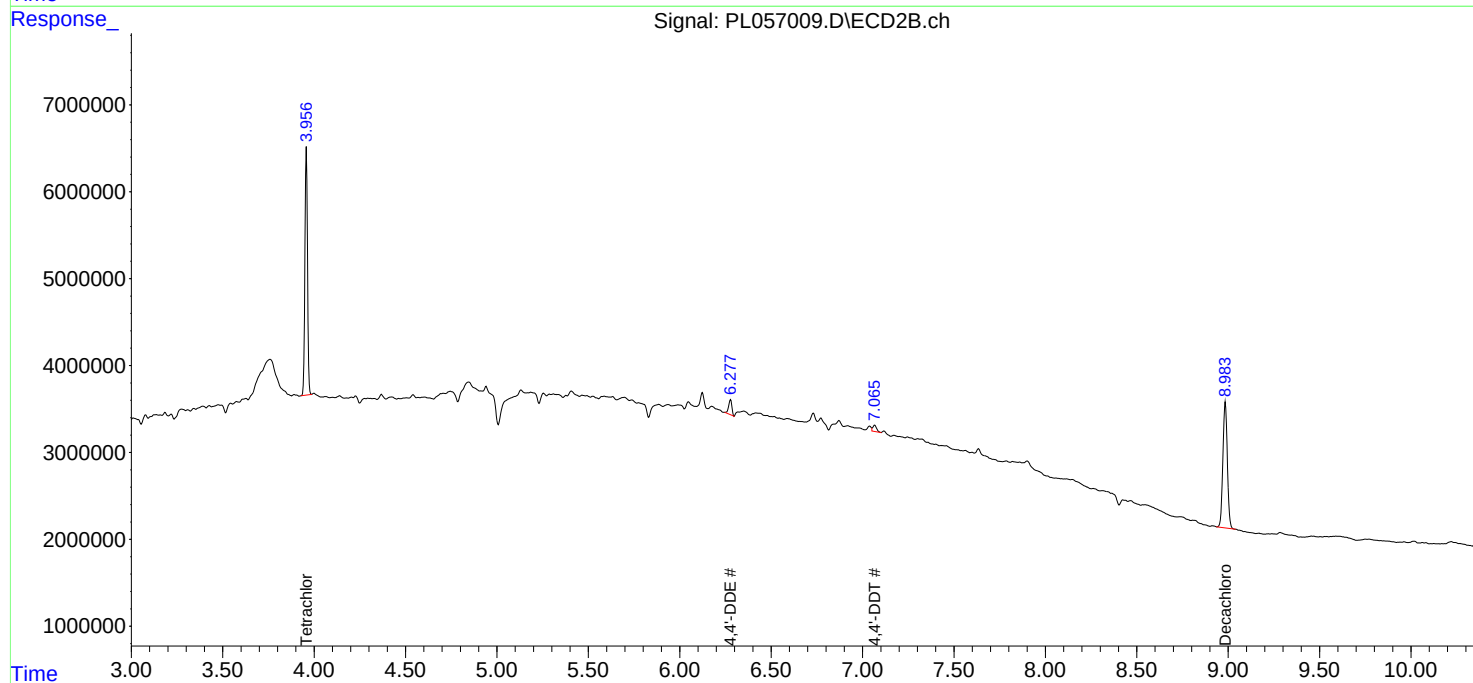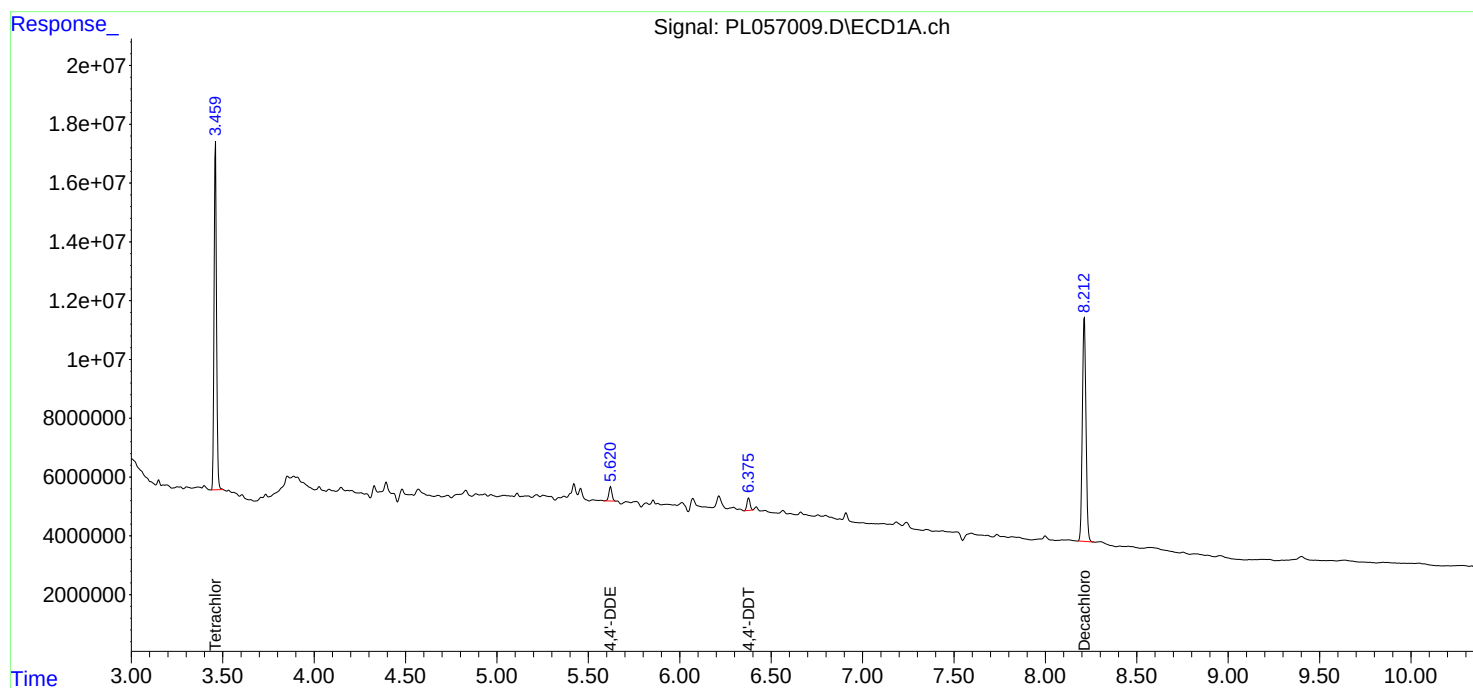

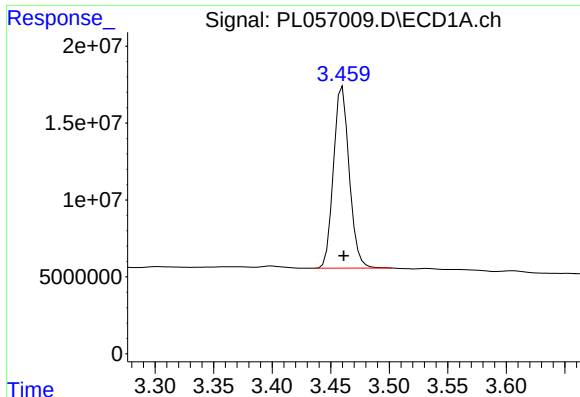


#1 Tetrachloro-m-xylene

R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 110981371
Conc: 13.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-030220


Manual Integrations
APPROVED

mohammad
3/5/2020 11:40:38 AM

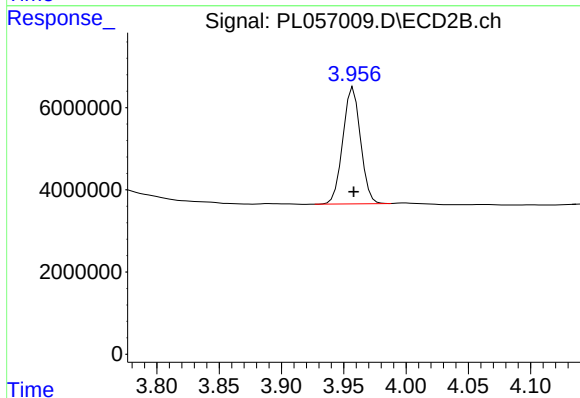


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 28107596
Conc: 13.17 ng/ml

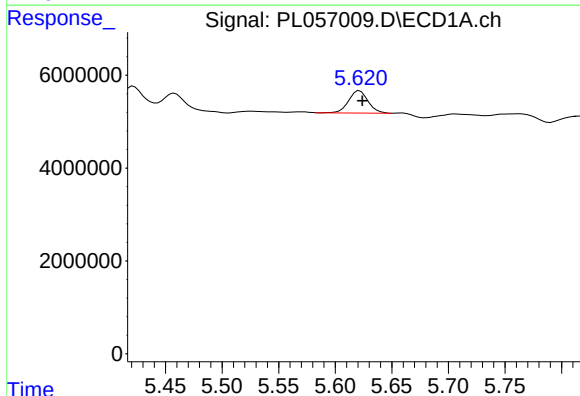


#12 4,4'-DDE

R.T.: 5.620 min
Delta R.T.: -0.004 min
Response: 5765988
Conc: 0.49 ng/ml m

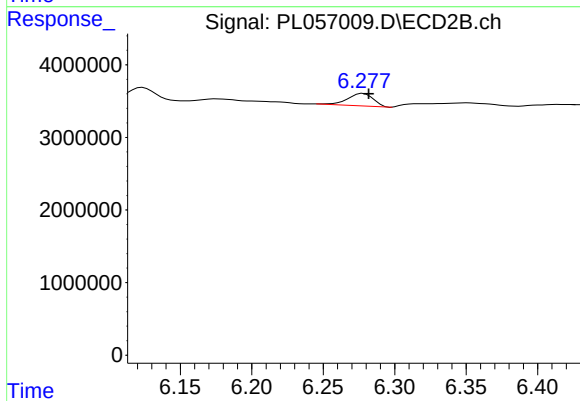

#12 4,4'-DDE

R.T.: 6.278 min
Delta R.T.: -0.004 min
Response: 2144374
Conc: 0.76 ng/ml

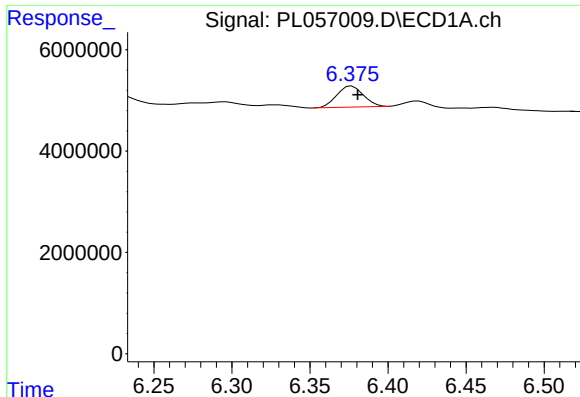


#17 4,4'-DDT

R.T.: 6.377 min
Delta R.T.: -0.004 min
Response: 4952690
Conc: 0.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-030220


Manual Integrations
APPROVED

mohammad
3/5/2020 11:40:38 AM

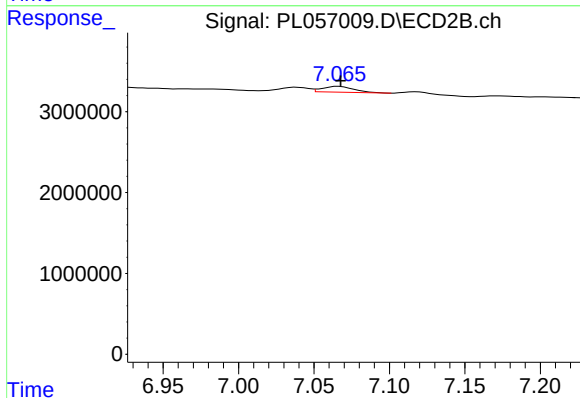


#17 4,4'-DDT

R.T.: 7.065 min
Delta R.T.: -0.002 min
Response: 1024941
Conc: 0.42 ng/ml m

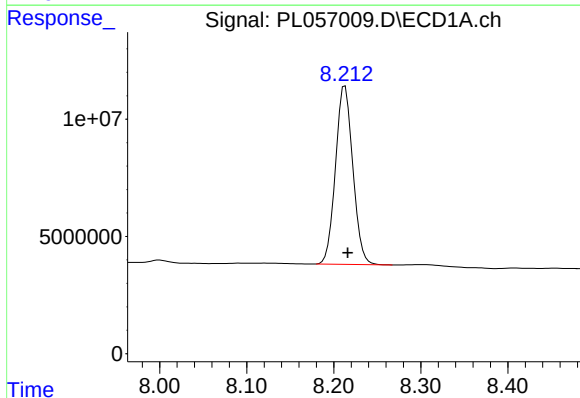

#28 Decachlorobiphenyl

R.T.: 8.213 min
Delta R.T.: -0.003 min
Response: 105343014
Conc: 10.90 ng/ml

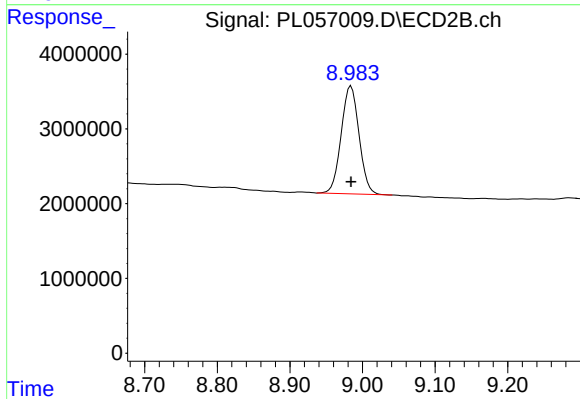

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 24628968
Conc: 11.59 ng/ml