

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030322\
 Data File : PL073124.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 15:48
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 03:59:48 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.646	5.490	6717175	31491627	20.961	21.700
28)	SA Decachlor...	10.425	11.330	10389850	34645721	22.197	21.962
Target Compounds							
3)	MA gamma-BHC...	5.781	0.000	30248	0	0.068	N.D. #
6)	B beta-BHC	0.000	6.677	0	692515	N.D.	0.768 #
7)	B delta-BHC	6.413	6.940	5885	1352705	0.013	0.715 #
10)	B gamma-Chl...	7.355f	0.000	37501	0	0.079	N.D. #
13)	MA Dieldrin	7.788	0.000	47438	0	0.106	N.D. #
14)	MA Endrin	8.098f	0.000	57854	0	0.146	N.D. #
15)	B Endosulfa...	0.000	9.052	0	320497	N.D.	0.232 #
16)	A 4,4'-DDD	8.260f	0.000	7364	0	0.021	N.D. #
17)	MA 4,4'-DDT	0.000	9.310	0	59781	N.D.	0.044 #
22)	Mirex	9.511	0.000	3987	0	0.007	N.D. #
23)	Chlordane-1	0.000	6.848	0	1012454	N.D.	15.013 #
25)	Chlordane-3	7.355f	0.000	37501	0	0.758	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL073124\
Data File : PL073124.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 15:48
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 03:59:48 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

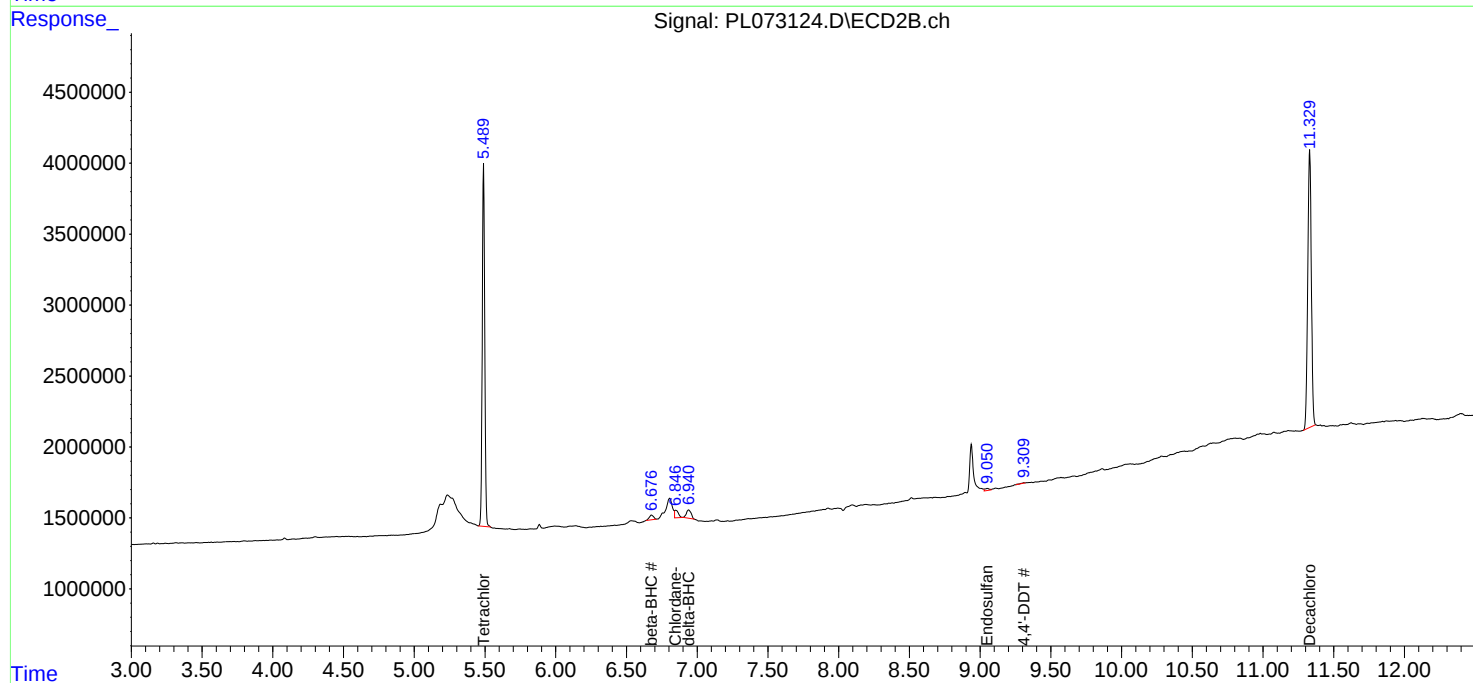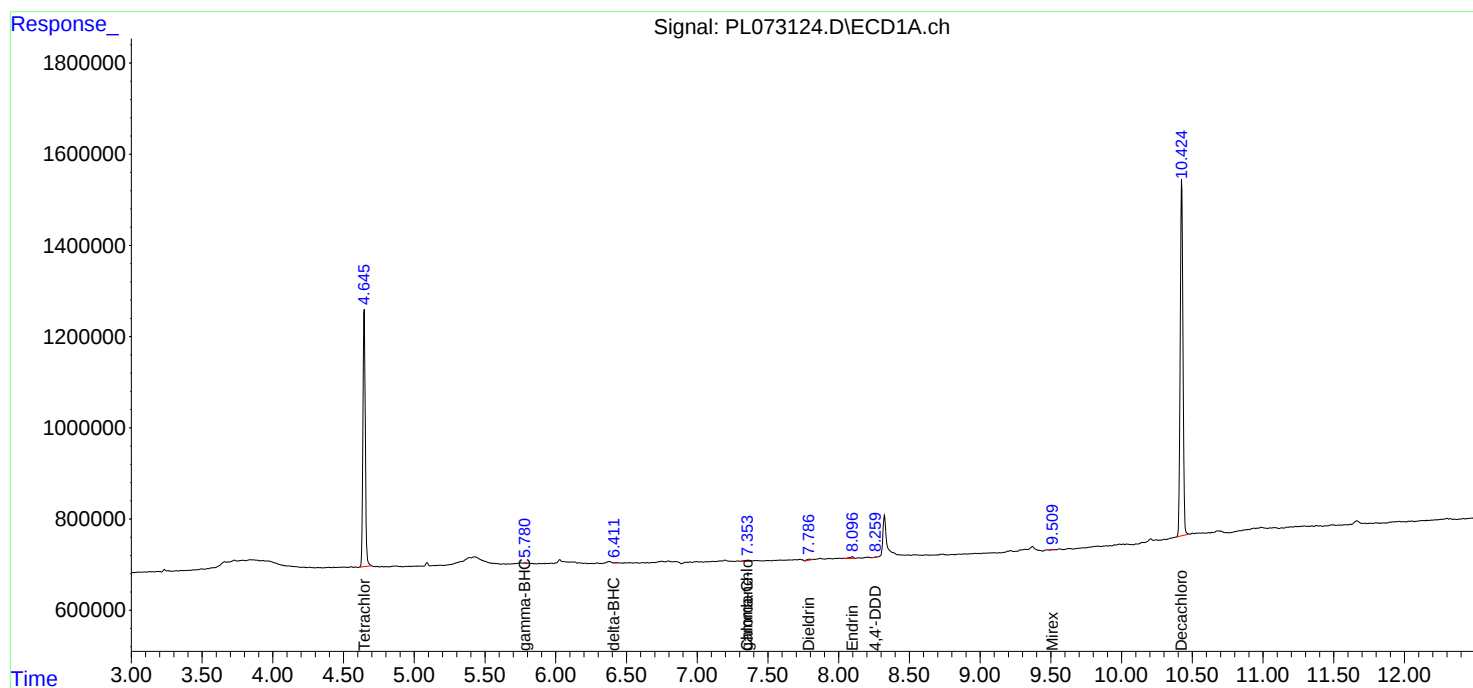


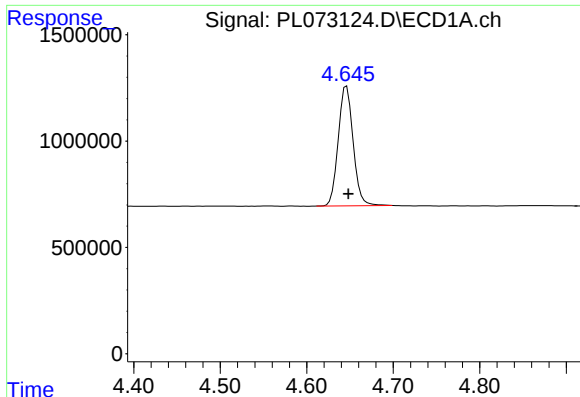

#1 Tetrachloro-m-xylene


R.T.: 4.646 min
Delta R.T.: -0.002 min
Response: 6717175
Conc: 20.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

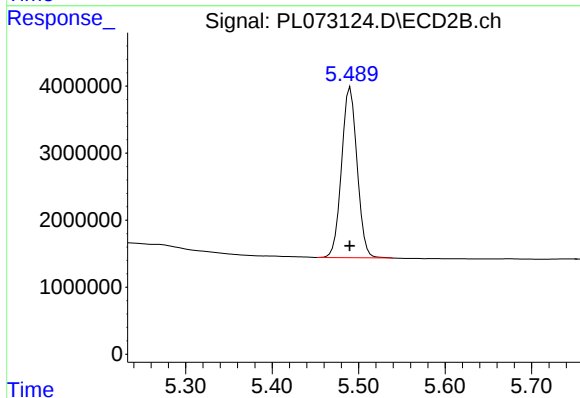


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: 0.000 min
Response: 31491627
Conc: 21.70 ng/ml

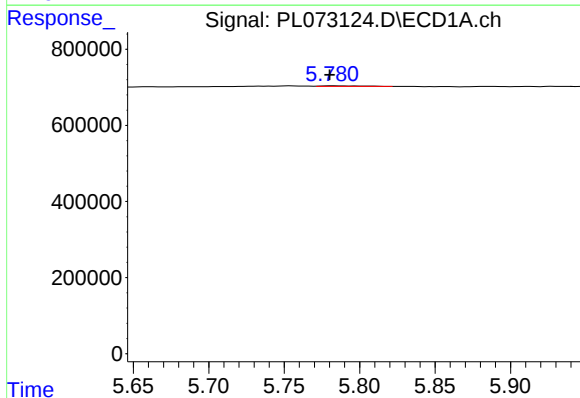


#3 gamma-BHC (Lindane)

R.T.: 5.781 min
Delta R.T.: 0.001 min
Response: 30248
Conc: 0.07 ng/ml

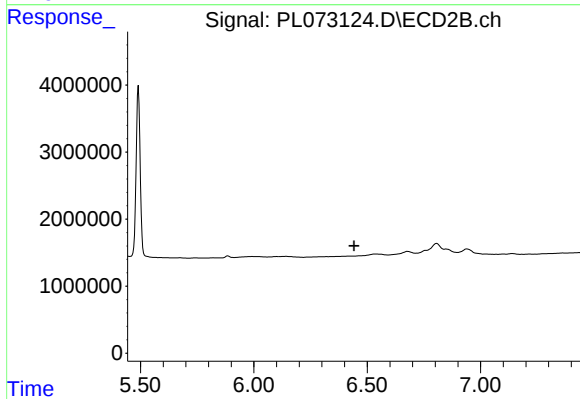

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 6.442 min
Response: 0
Conc: N.D.

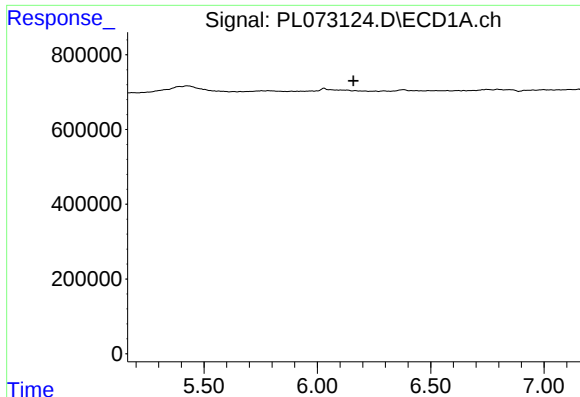

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

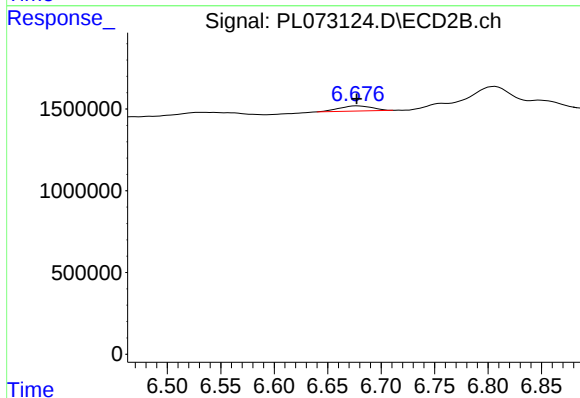


#6 beta-BHC

R.T.: 6.677 min
Delta R.T.: 0.000 min
Response: 692515
Conc: 0.77 ng/ml

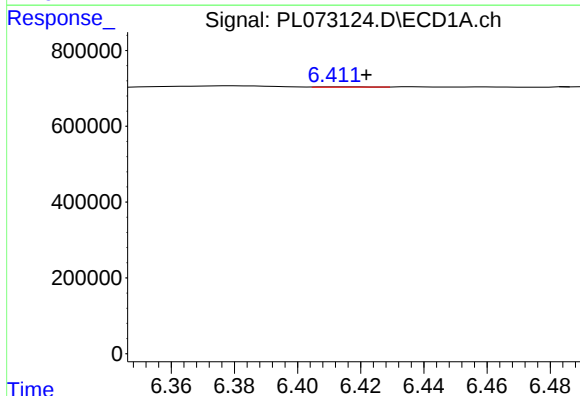


#7 delta-BHC

R.T.: 6.413 min
Delta R.T.: -0.009 min
Response: 5885
Conc: 0.01 ng/ml

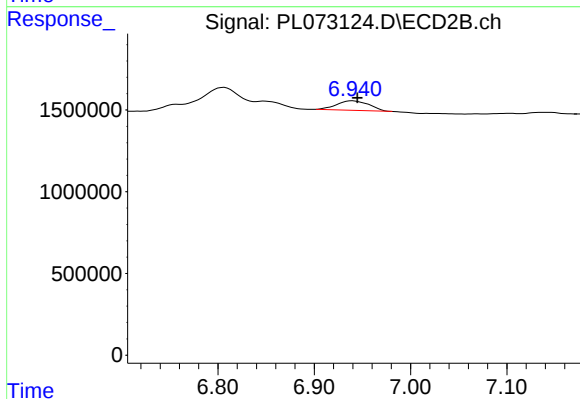

#7 delta-BHC


R.T.: 6.940 min
Delta R.T.: -0.005 min
Response: 1352705
Conc: 0.71 ng/ml

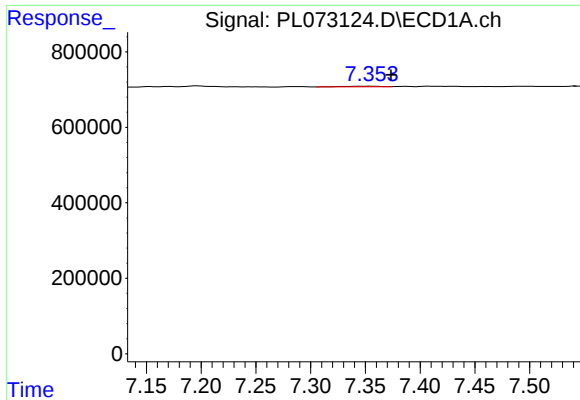

#10 gamma-Chlordane


R.T.: 7.355 min
Delta R.T.: -0.018 min
Response: 37501
Conc: 0.08 ng/ml

Instrument :
ECD_L
ClientSampleId :

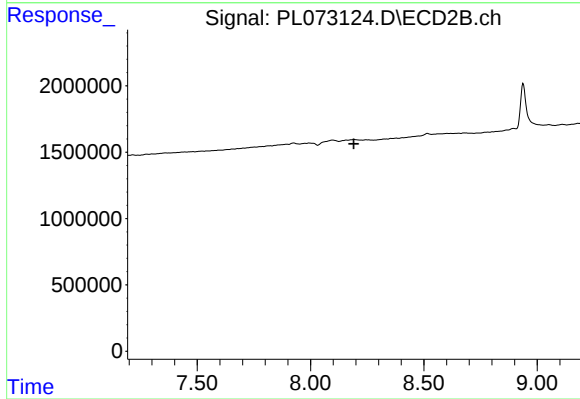


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

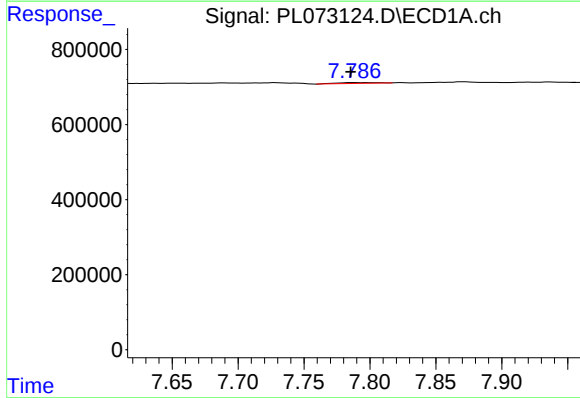


#13 Dieldrin

R.T.: 7.788 min
Delta R.T.: 0.002 min
Response: 47438
Conc: 0.11 ng/ml

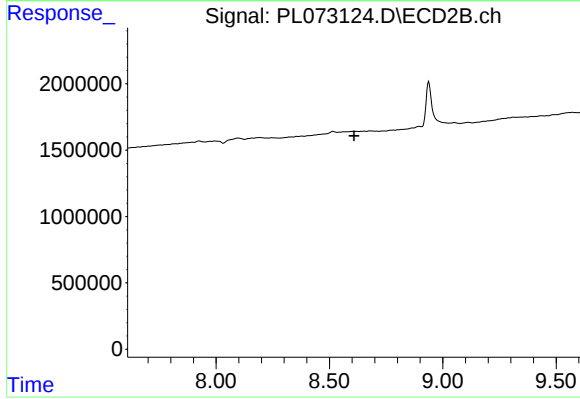

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 8.609 min
Response: 0
Conc: N.D.

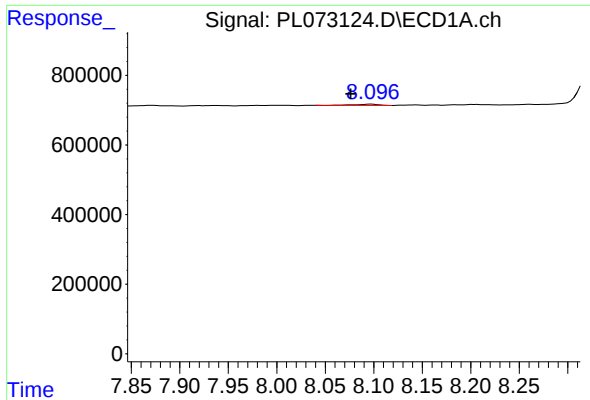

#14 Endrin


R.T.: 8.098 min
Delta R.T.: 0.021 min
Response: 57854
Conc: 0.15 ng/ml

Instrument :
ECD_L
ClientSampleId :

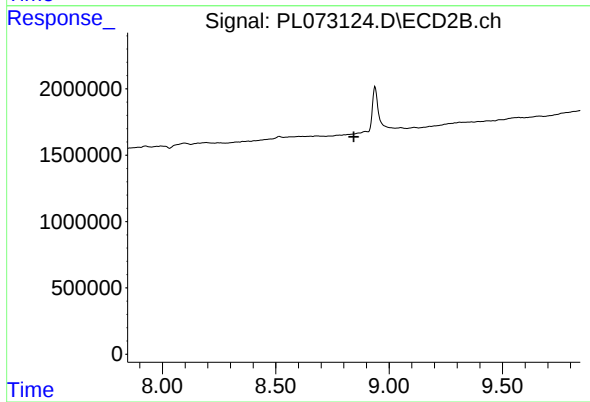


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

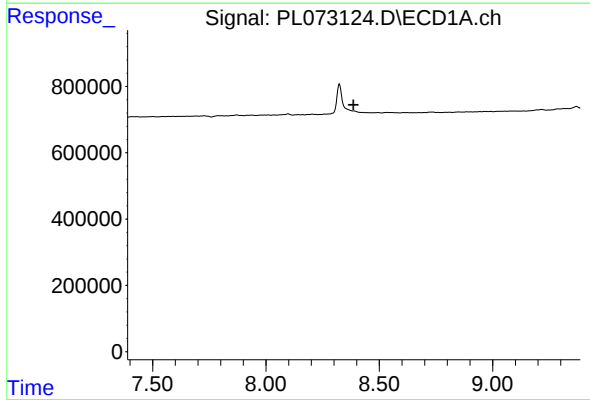


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.386 min
Response: 0
Conc: N.D.

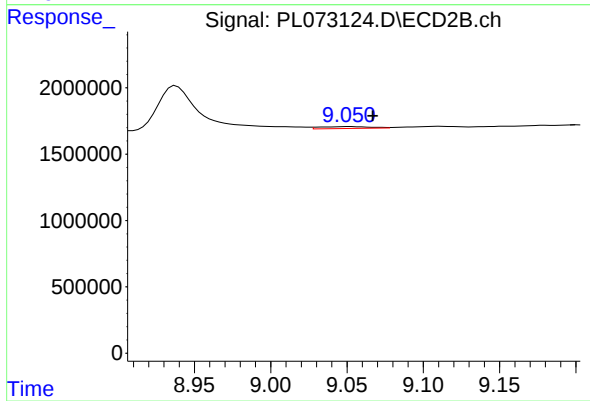

#15 Endosulfan II


R.T.: 9.052 min
Delta R.T.: -0.015 min
Response: 320497
Conc: 0.23 ng/ml

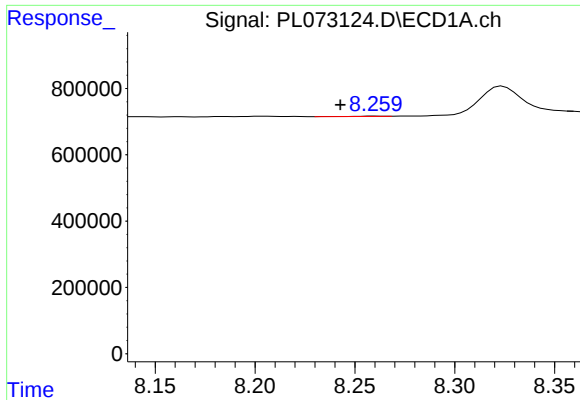

#16 4,4'-DDD


R.T.: 8.260 min
Delta R.T.: 0.018 min
Response: 7364
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

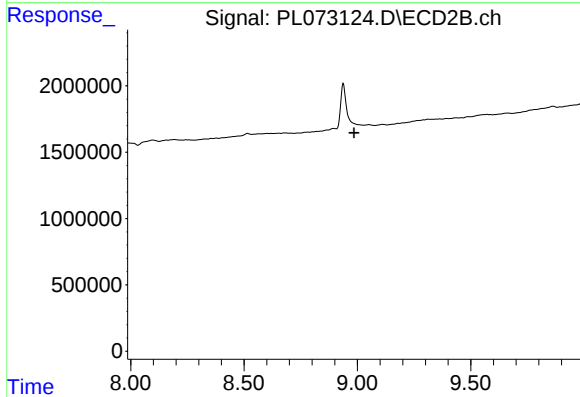


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 8.985 min
Response: 0
Conc: N.D.

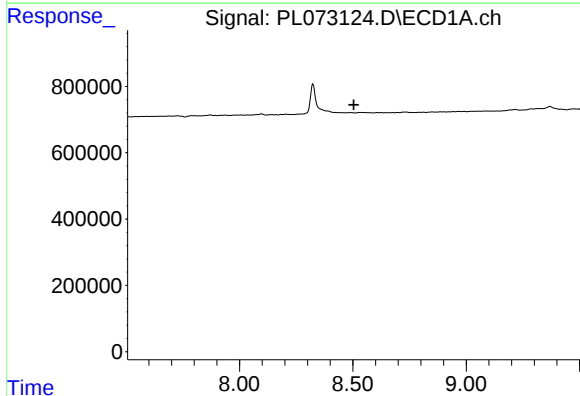


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 8.505 min
Response: 0
Conc: N.D.

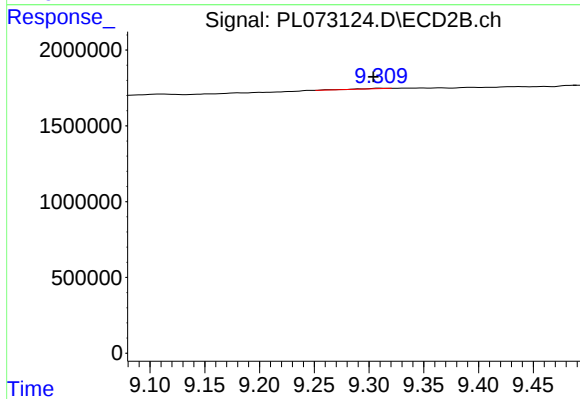

#17 4,4'-DDT


R.T.: 9.310 min
Delta R.T.: 0.006 min
Response: 59781
Conc: 0.04 ng/ml

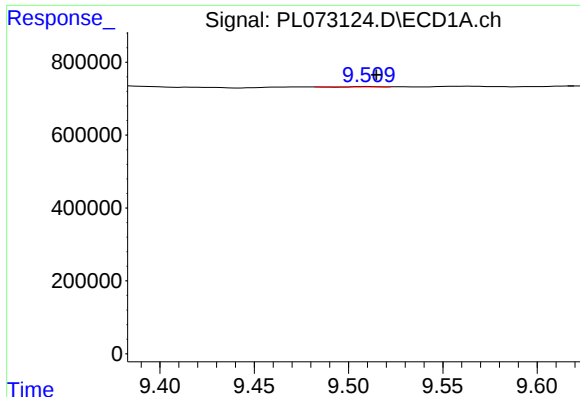

#22 Mirex


R.T.: 9.511 min
Delta R.T.: -0.004 min
Response: 3987
Conc: 0.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

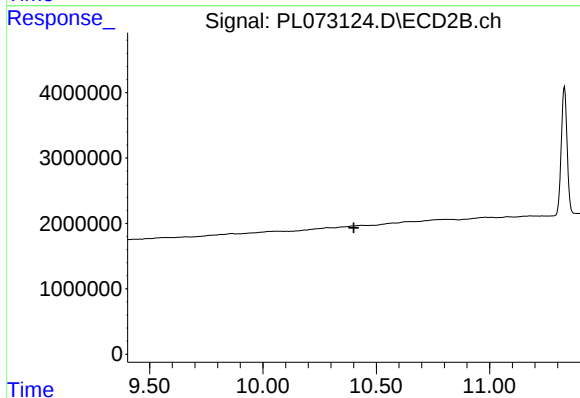


#22 Mirex

R.T.: 0.000 min
Exp R.T. : 10.400 min
Response: 0
Conc: N.D.

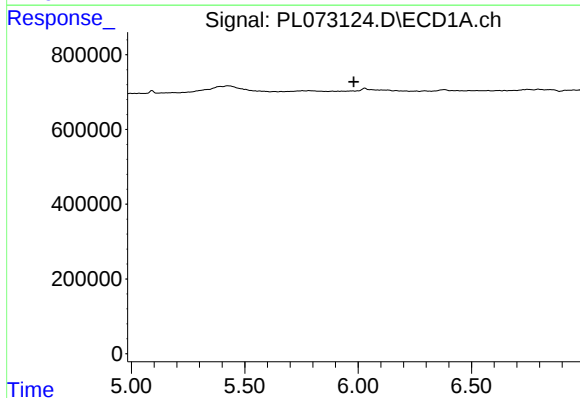


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.981 min
Response: 0
Conc: N.D.

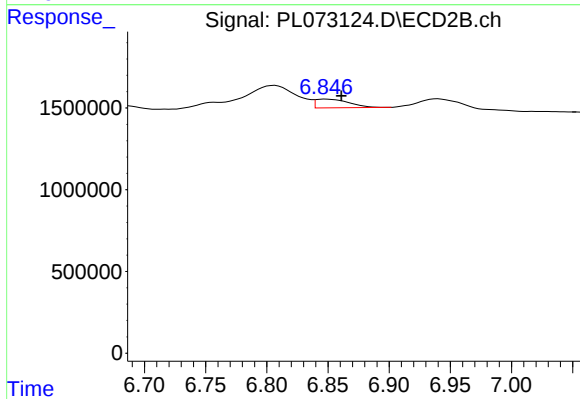

#23 Chlordane-1


R.T.: 6.848 min
Delta R.T.: -0.013 min
Response: 1012454
Conc: 15.01 ng/ml

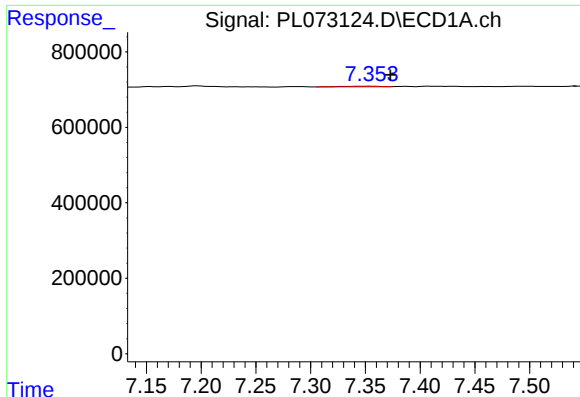

#25 Chlordane-3


R.T.: 7.355 min
Delta R.T.: -0.018 min
Response: 37501
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

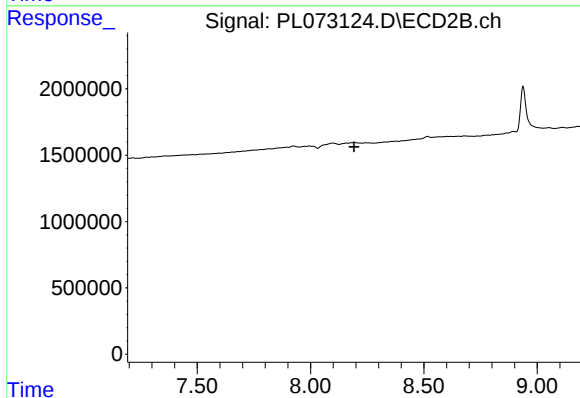


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

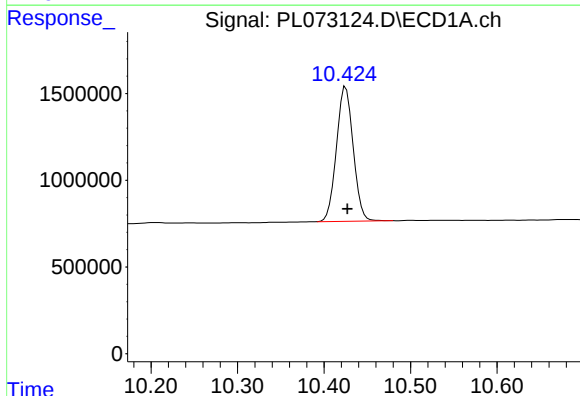

#28 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: -0.002 min
Response: 10389850
Conc: 22.20 ng/ml

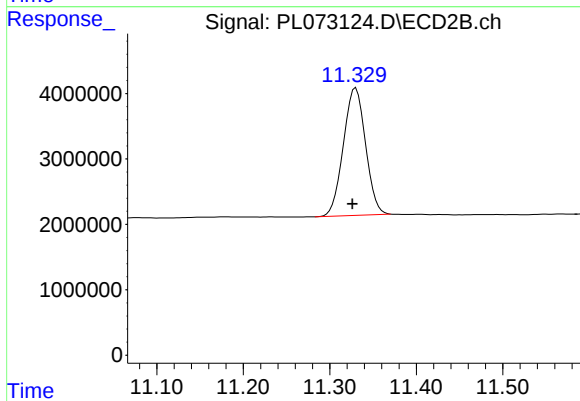

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: 0.004 min
Response: 34645721
Conc: 21.96 ng/ml