

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030323\
 Data File : PL081245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 14:17
 Operator : AR\AJ
 Sample : 01770-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-223

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/06/2023
 Supervised By : Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 20:54:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 03 01:48:45 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.334	2.665	41935152	38838029	19.409	19.190
28) SA Decachlor...	8.759	7.790	29284546	32548553	19.209	16.992
Target Compounds						
17) MA 4,4'-DDT	6.793	5.915	1818975	2544819	1.146m	1.586 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030323\
Data File : PL081245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 14:17
Operator : AR\AJ
Sample : 01770-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-223


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/06/2023
Supervised By : Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 20:54:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030223.M
Quant Title : GC Extractables
QLast Update : Fri Mar 03 01:48:45 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

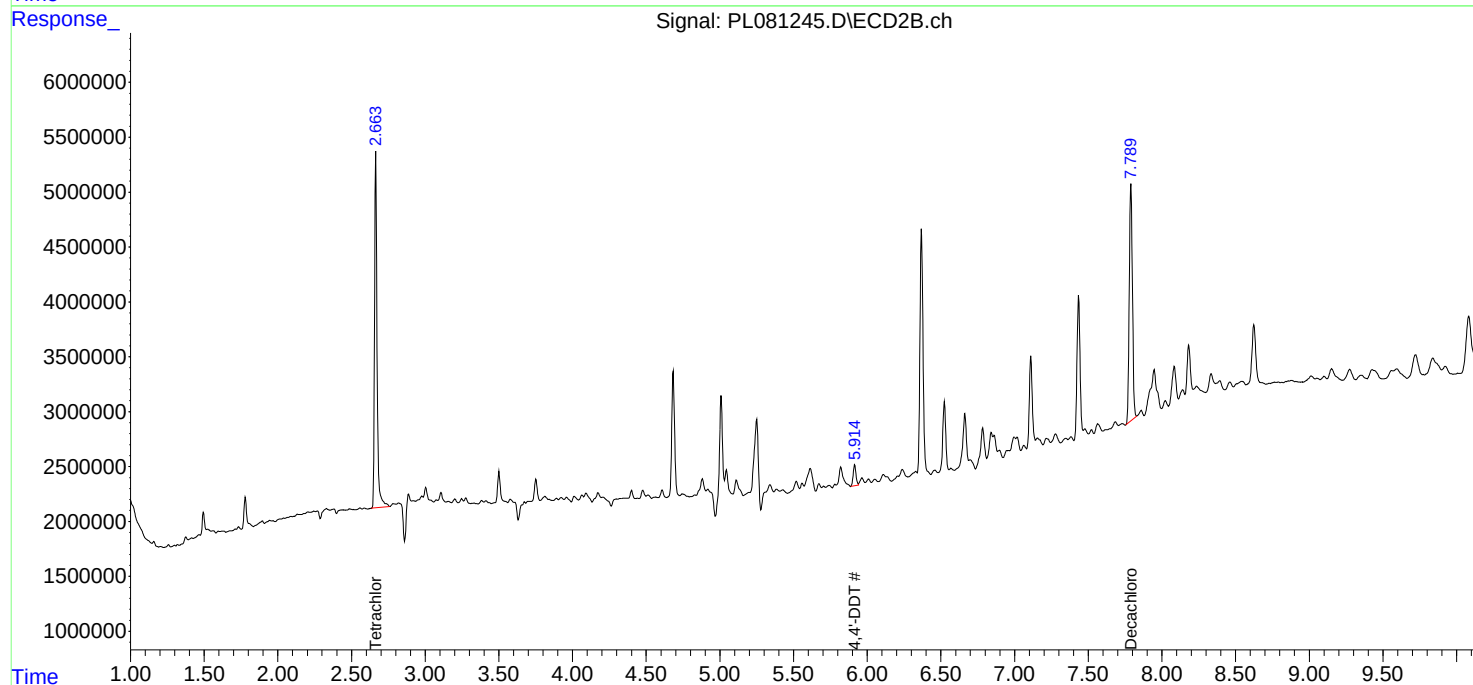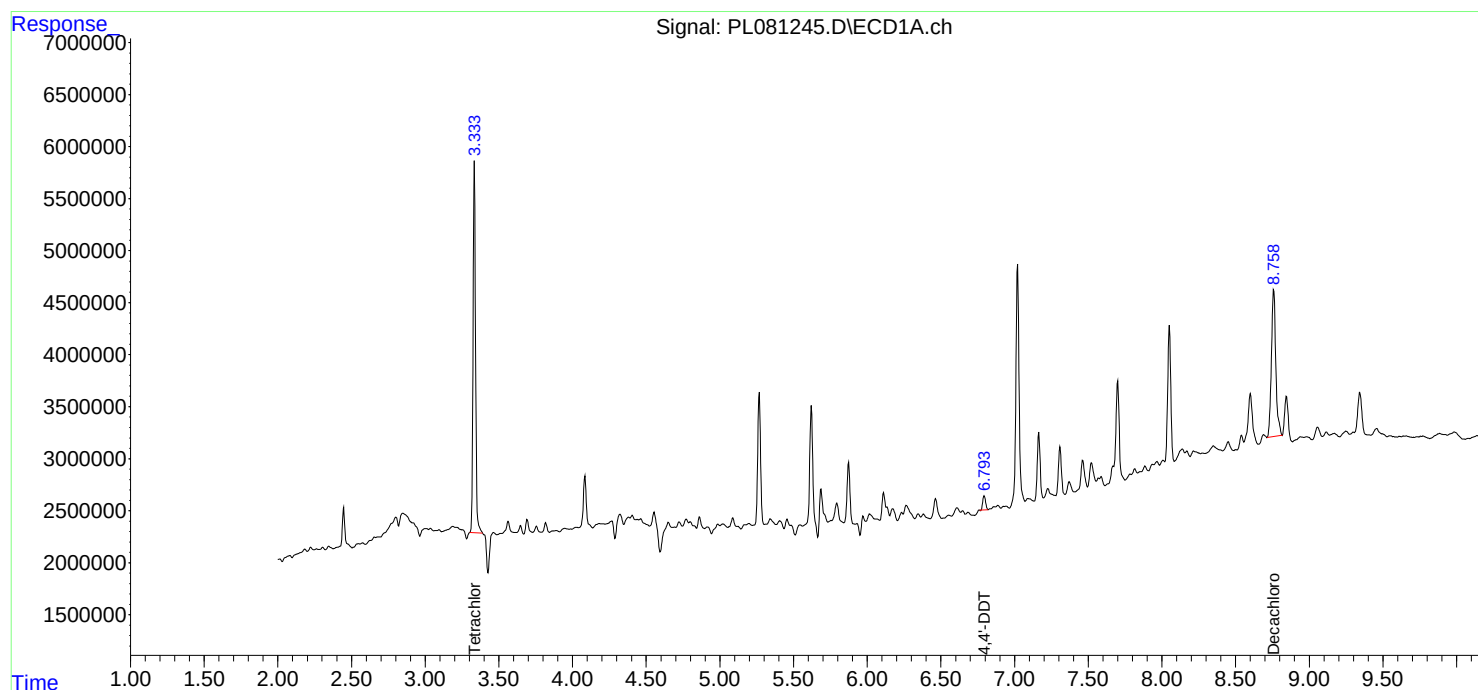

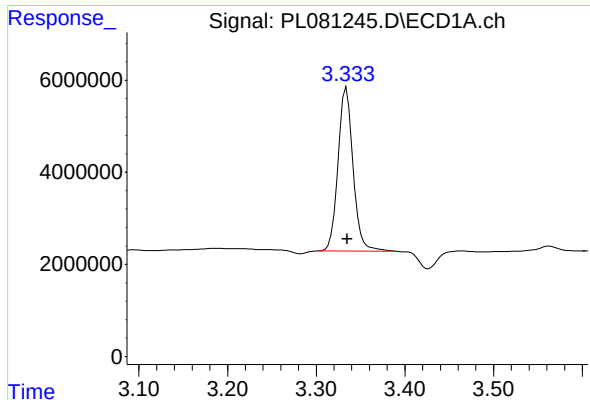


#1 Tetrachloro-m-xylene

R.T.: 3.334 min
Delta R.T.: 0.000 min
Response: 41935152
Conc: 19.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-223


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

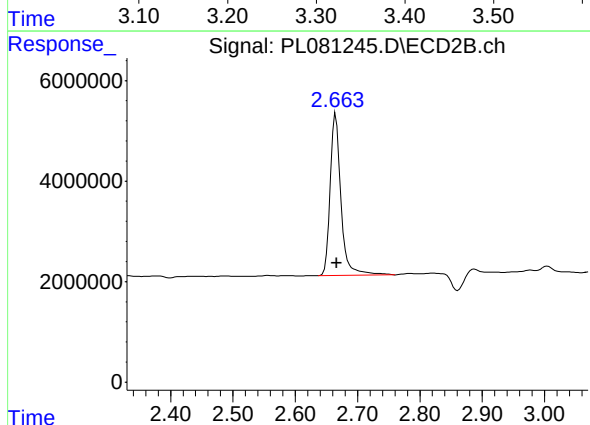


#1 Tetrachloro-m-xylene

R.T.: 2.665 min
Delta R.T.: -0.002 min
Response: 38838029
Conc: 19.19 ng/ml

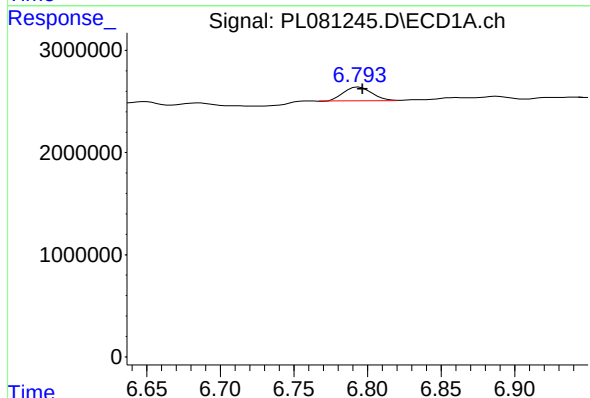


#17 4,4'-DDT

R.T.: 6.793 min
Delta R.T.: -0.004 min
Response: 1818975
Conc: 1.15 ng/ml m

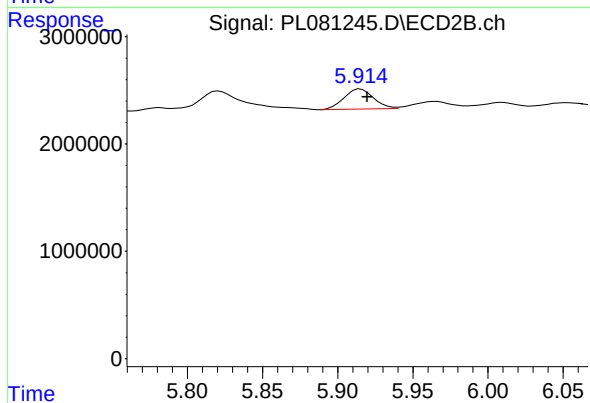

#17 4,4'-DDT

R.T.: 5.915 min
Delta R.T.: -0.004 min
Response: 2544819
Conc: 1.59 ng/ml

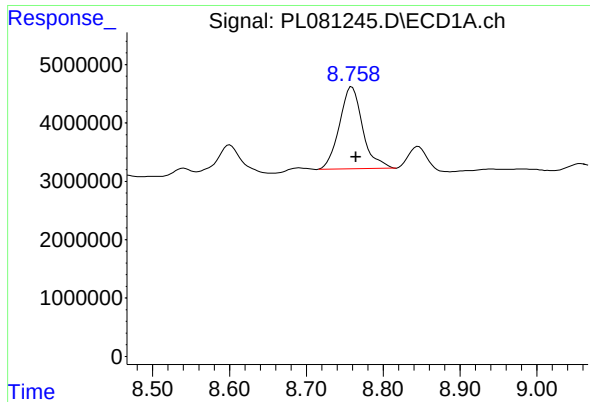


#28 Decachlorobiphenyl

R.T.: 8.759 min
Delta R.T.: -0.005 min
Response: 29284546
Conc: 19.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-223

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

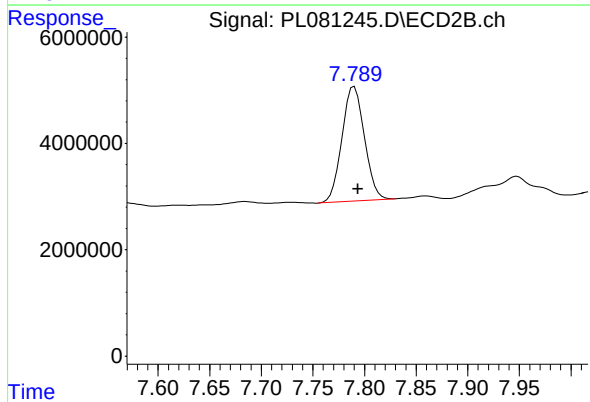

#28 Decachlorobiphenyl

R.T.: 7.790 min
Delta R.T.: -0.004 min
Response: 32548553
Conc: 16.99 ng/ml