

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030325\
 Data File : PL094464.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2025 09:41
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 13:08:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	0.000	2.775	0	287950	N.D.	0.090 #
Target Compounds							
7)	B delta-BHC	0.000	4.131	0	164675	N.D.	0.035 #
8)	B Heptachlo...	0.000	4.706f	0	42764	N.D.	0.010 #
9)	A Endosulfan I	0.000	5.088	0	745906	N.D.	0.187 #
13)	MA Dieldrin	0.000	5.376f	0	101670	N.D.	0.023 #
14)	MA Endrin	0.000	5.657f	0	469505	N.D.	0.138 #
15)	B Endosulfa...	0.000	5.920	0	209537	N.D.	0.056 #
16)	A 4,4'-DDD	0.000	5.807f	0	283730	N.D.	0.089 #
17)	MA 4,4'-DDT	0.000	6.057f	0	324156	N.D.	0.091 #
18)	B Endrin al...	0.000	6.097	0	271735	N.D.	0.086 #
19)	B Endosulfa...	0.000	6.334	0	96662	N.D.	0.026 #
20)	A Methoxychlor	0.000	6.615	0	505691	N.D.	0.259 #
21)	B Endrin ke...	0.000	6.828	0	55093	N.D.	0.013 #
22)	Mirex	0.000	6.997f	0	412617	N.D.	0.118 #
23)	Chlordane-1	0.000	3.786f	0	131953	N.D.	0.972 #
27)	Chlordane-5	0.000	5.920	0	209537	N.D.	1.280 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030325\
Data File : PL094464.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2025 09:41
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 13:08:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

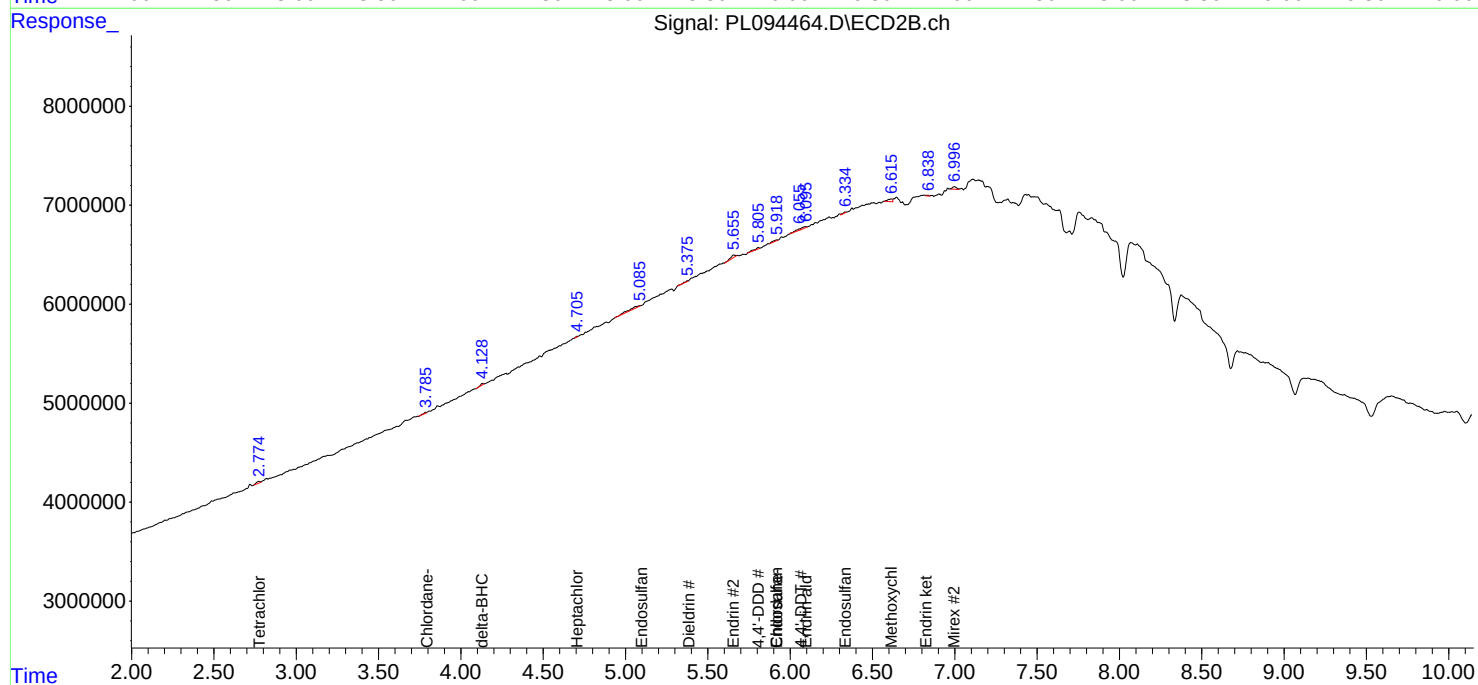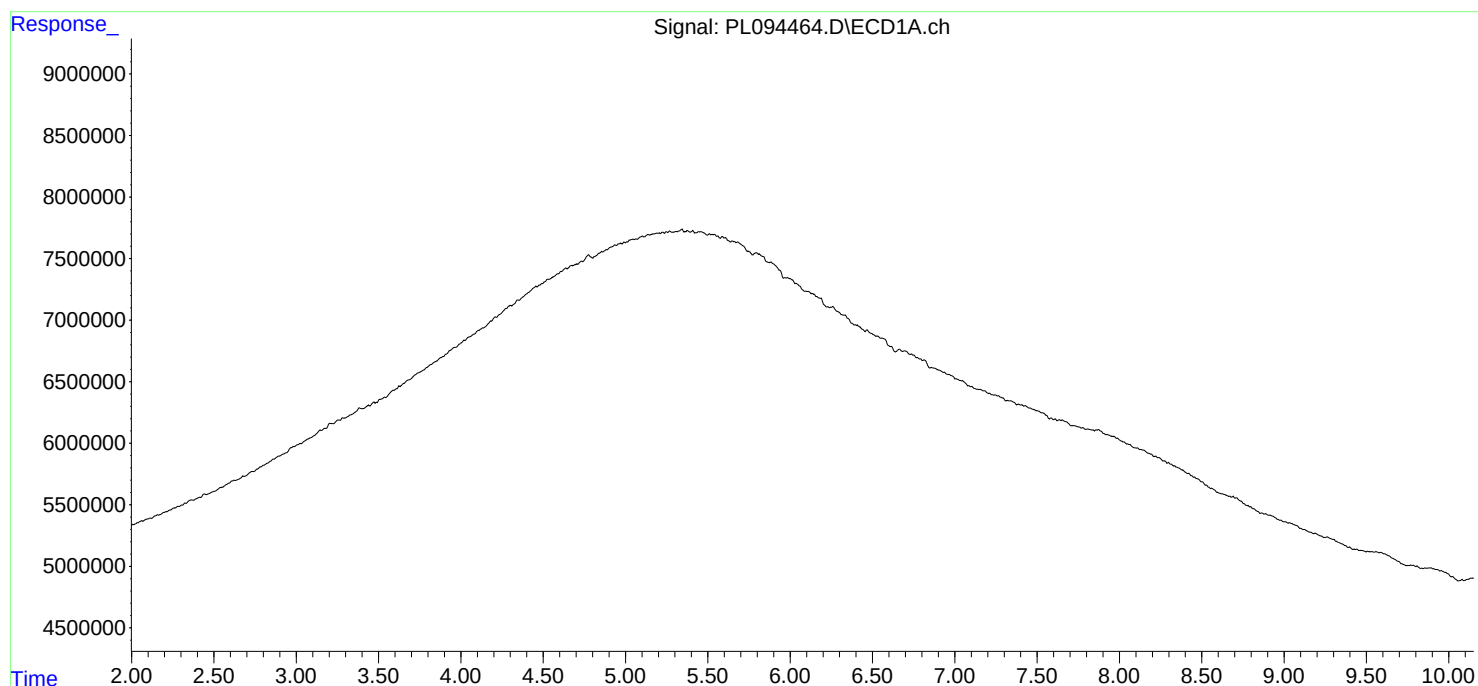


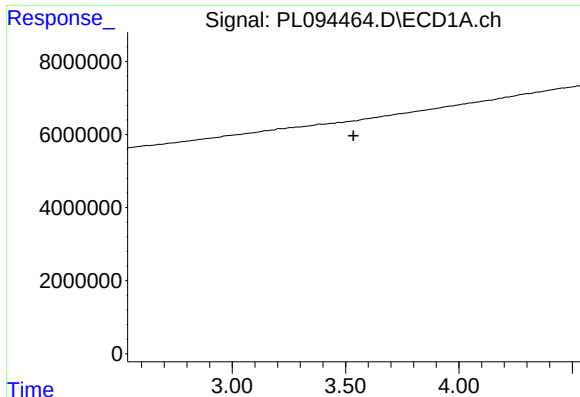

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.535 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

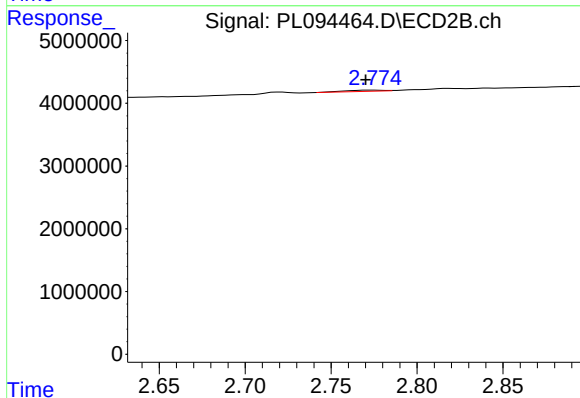


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.005 min
Response: 287950
Conc: 0.09 ng/ml

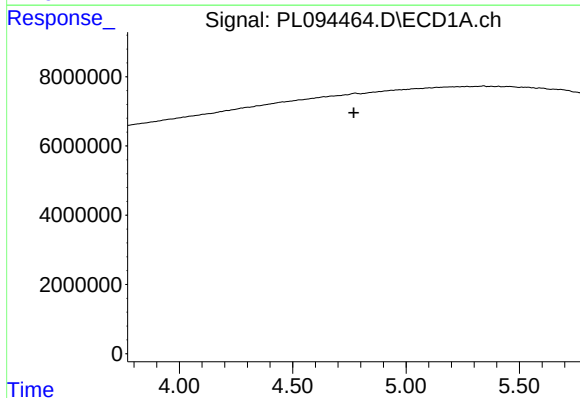


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.769 min
Response: 0
Conc: N.D.

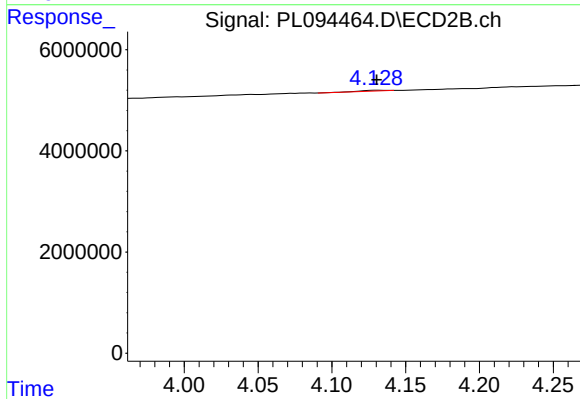

#7 delta-BHC


R.T.: 4.131 min
Delta R.T.: 0.000 min
Response: 164675
Conc: 0.03 ng/ml

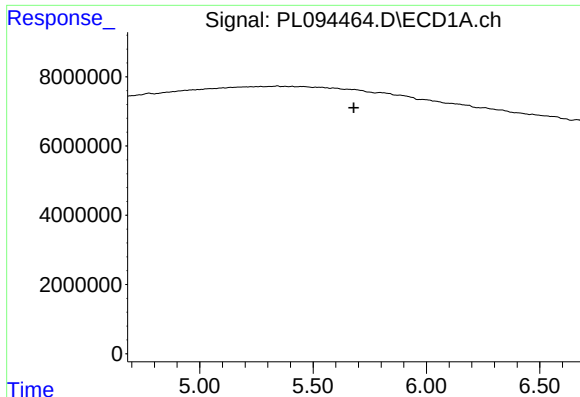

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.679 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

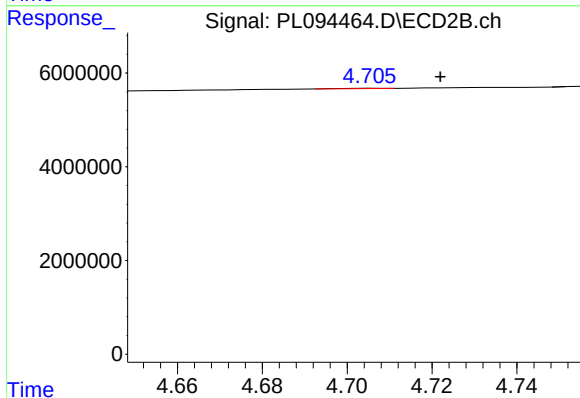


#8 Heptachlor epoxide

R.T.: 4.706 min
Delta R.T.: -0.016 min
Response: 42764
Conc: 0.01 ng/ml

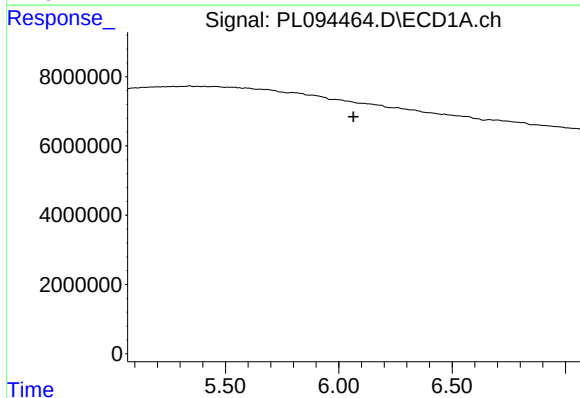


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 6.065 min
Response: 0
Conc: N.D.

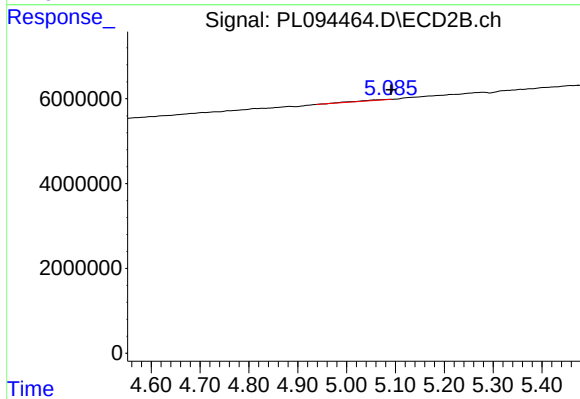

#9 Endosulfan I


R.T.: 5.088 min
Delta R.T.: -0.003 min
Response: 745906
Conc: 0.19 ng/ml

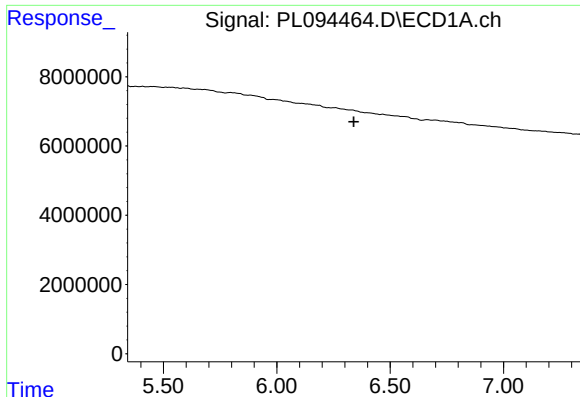

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.340 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

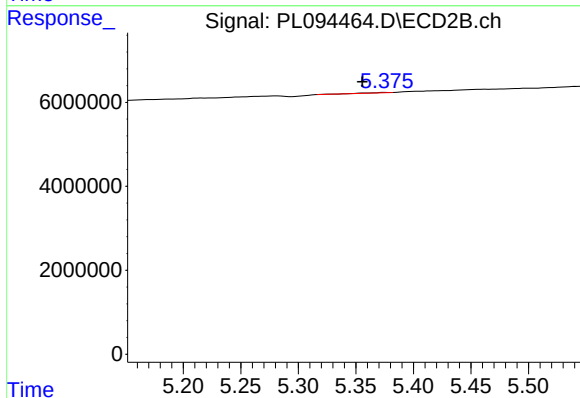


#13 Dieldrin

R.T.: 5.376 min
Delta R.T.: 0.020 min
Response: 101670
Conc: 0.02 ng/ml

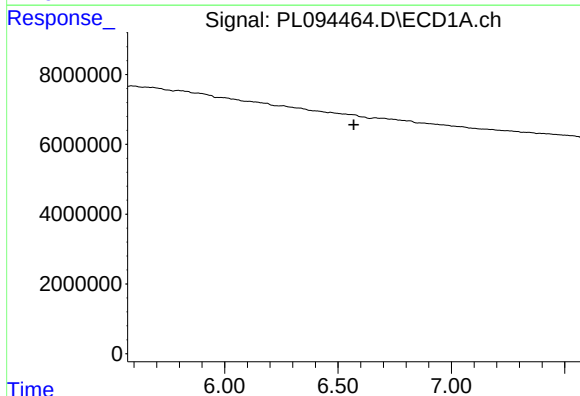


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.570 min
Response: 0
Conc: N.D.

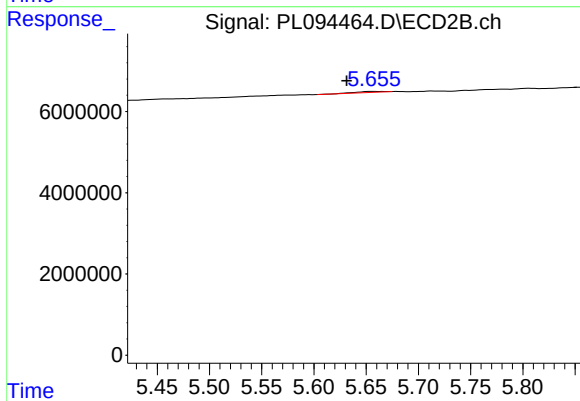

#14 Endrin


R.T.: 5.657 min
Delta R.T.: 0.025 min
Response: 469505
Conc: 0.14 ng/ml

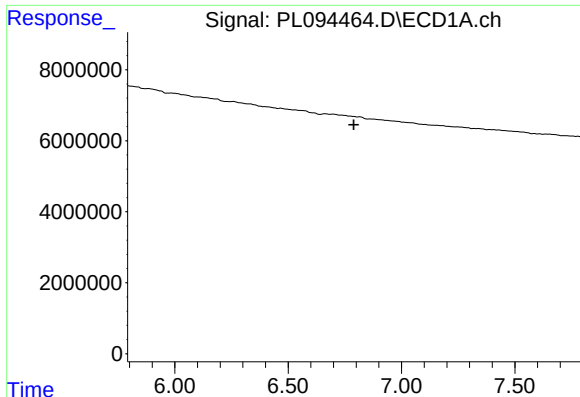

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.790 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

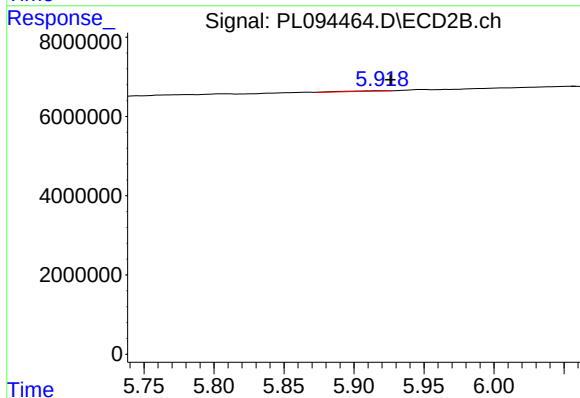


#15 Endosulfan II

R.T.: 5.920 min
Delta R.T.: -0.006 min
Response: 209537
Conc: 0.06 ng/ml

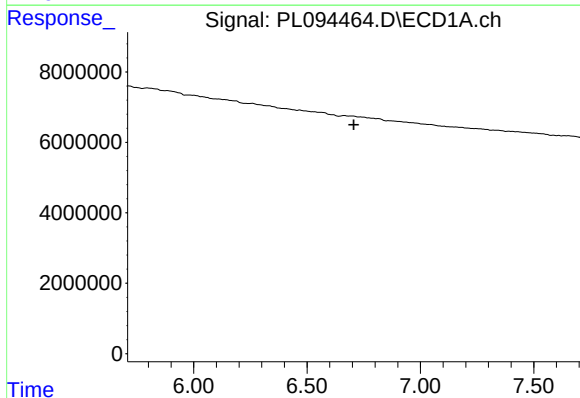


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.706 min
Response: 0
Conc: N.D.

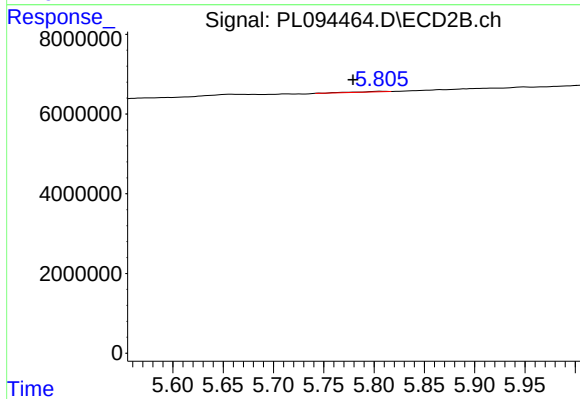

#16 4,4'-DDD


R.T.: 5.807 min
Delta R.T.: 0.028 min
Response: 283730
Conc: 0.09 ng/ml

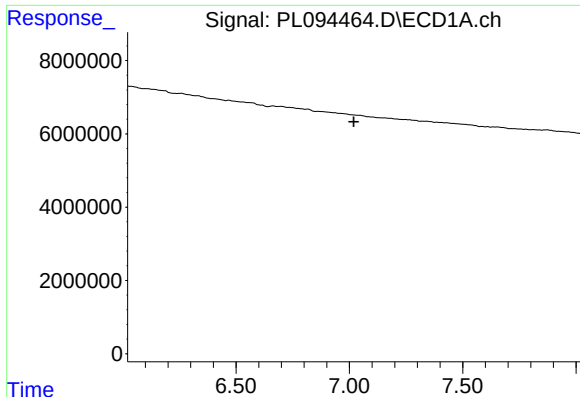

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.019 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

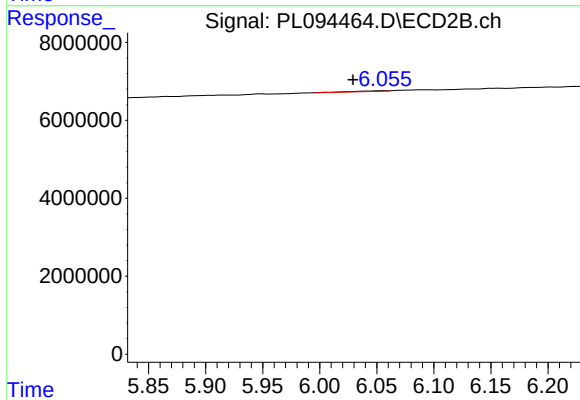


#17 4,4'-DDT

R.T.: 6.057 min
Delta R.T.: 0.027 min
Response: 324156
Conc: 0.09 ng/ml

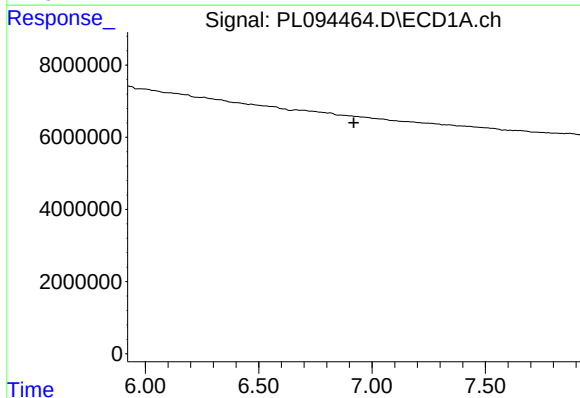


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 6.920 min
Response: 0
Conc: N.D.

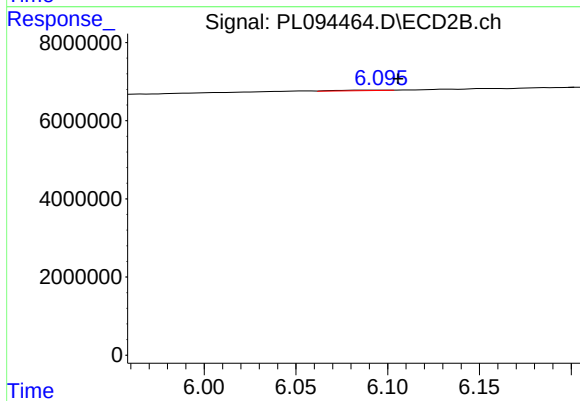

#18 Endrin aldehyde


R.T.: 6.097 min
Delta R.T.: -0.009 min
Response: 271735
Conc: 0.09 ng/ml

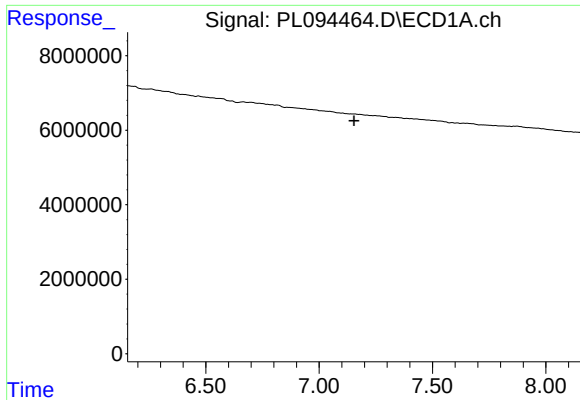

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.154 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

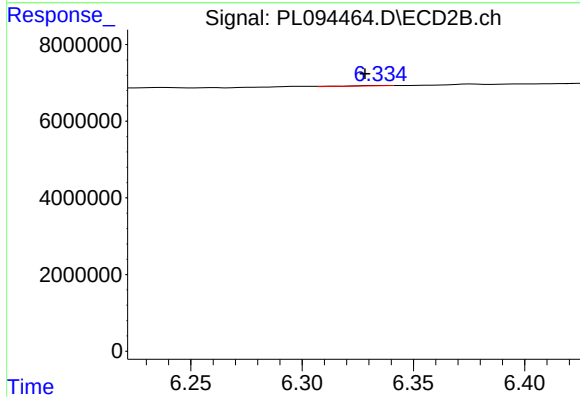


#19 Endosulfan Sulfate

R.T.: 6.334 min
Delta R.T.: 0.006 min
Response: 96662
Conc: 0.03 ng/ml

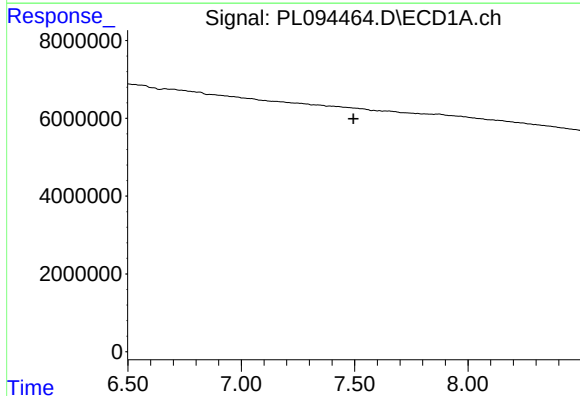


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.496 min
Response: 0
Conc: N.D.

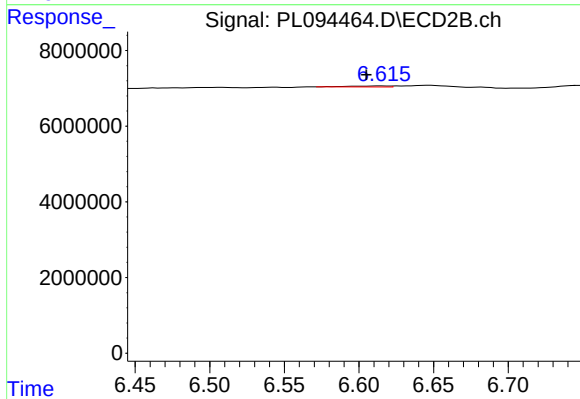

#20 Methoxychlor


R.T.: 6.615 min
Delta R.T.: 0.010 min
Response: 505691
Conc: 0.26 ng/ml

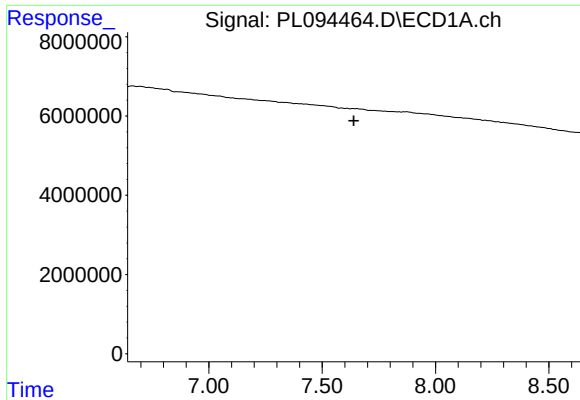

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.639 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

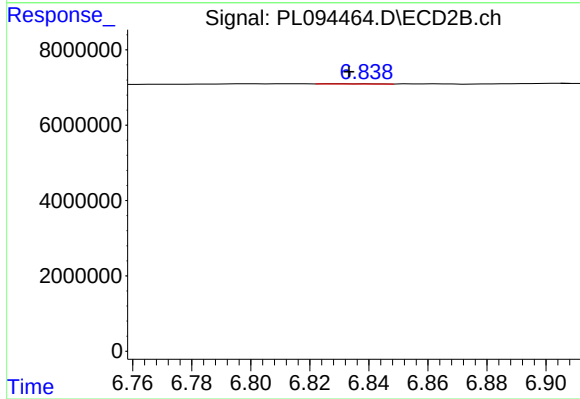


#21 Endrin ketone

R.T.: 6.828 min
Delta R.T.: -0.005 min
Response: 55093
Conc: 0.01 ng/ml

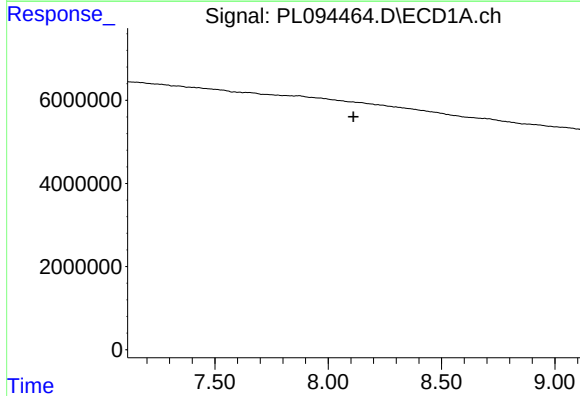


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 8.112 min
Response: 0
Conc: N.D.

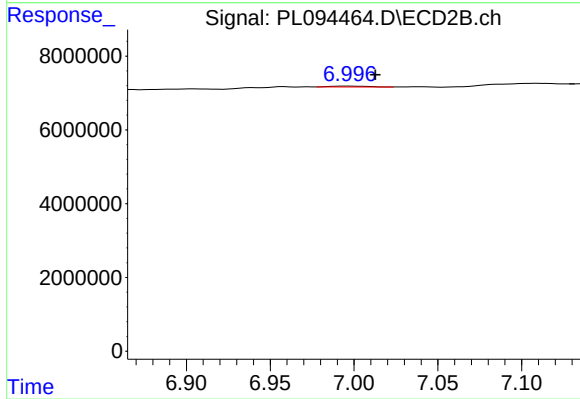

#22 Mirex


R.T.: 6.997 min
Delta R.T.: -0.015 min
Response: 412617
Conc: 0.12 ng/ml

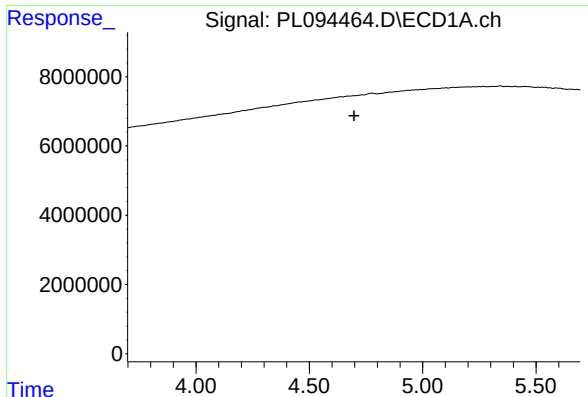

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.698 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

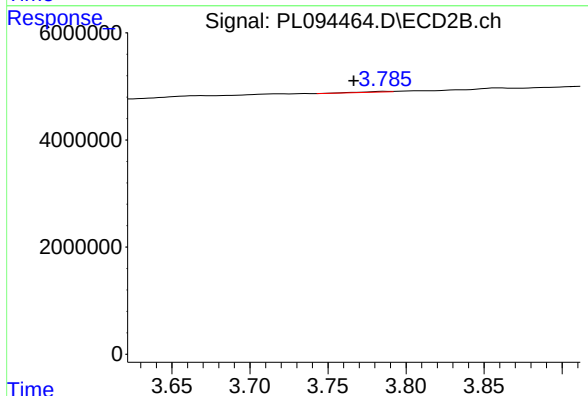


#23 Chlordane-1

R.T.: 3.786 min
Delta R.T.: 0.020 min
Response: 131953
Conc: 0.97 ng/ml

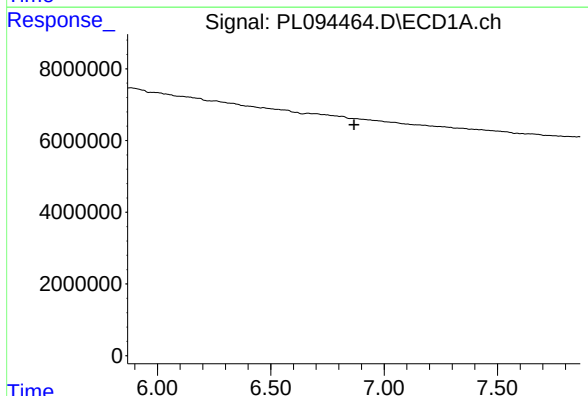


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.868 min
Response: 0
Conc: N.D.

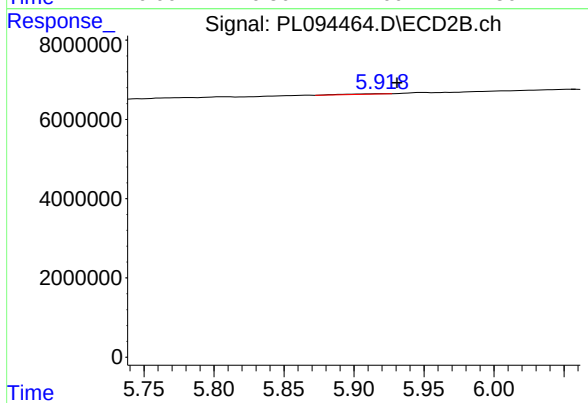

#27 Chlordane-5


R.T.: 5.920 min
Delta R.T.: -0.011 min
Response: 209537
Conc: 1.28 ng/ml

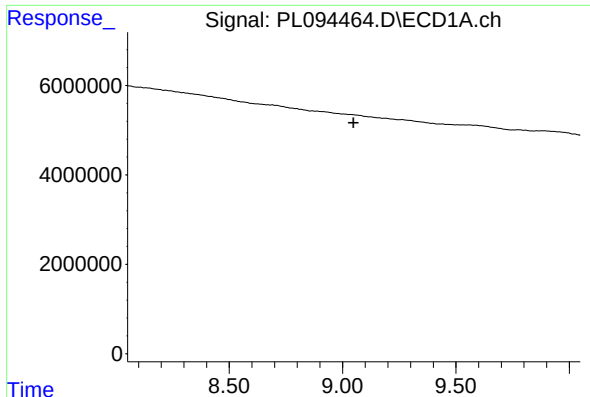

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

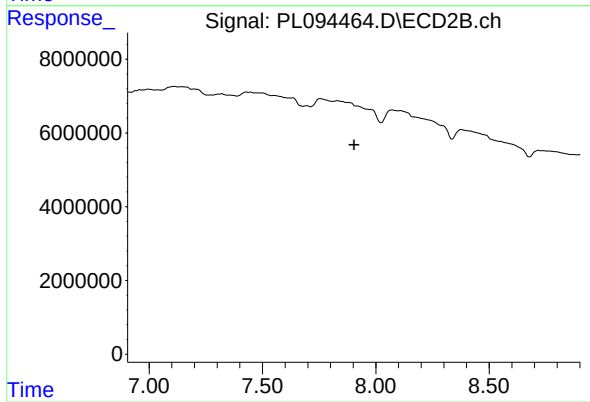

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.904 min
Response: 0
Conc: N.D.