

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
 Data File : PL045385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 12:38
 Operator : AJ\SJ
 Sample : K1688-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-030119-F

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 23:50:46 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.364	3.982	59583802	19444663	8.661	9.080
28) SA Decachlor...	8.049	9.043	75303957	23609770	9.000	10.333
Target Compounds						
4) MA Heptachlor	0.000	5.164	0	2318432	N.D.	0.779 #
10) B gamma-Chl...	5.282f	6.091	21692862	3122135	2.217	1.164 #
11) B alpha-Chl...	5.318	6.164	9822214	8763734	1.013	3.249 #
23) Chlordane-1	4.211	4.975	6755343	2626831	20.049	23.295
24) Chlordane-2	4.705	0.000	6769834	0	17.501	N.D. #
25) Chlordane-3	5.282f	6.091	21692862	3122135	18.912	8.013 #
26) Chlordane-4	5.318	6.164	9822214	8763734	9.266	18.733 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
Data File : PL045385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 12:38
Operator : AJ\SJ
Sample : K1688-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-F

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 23:50:46 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

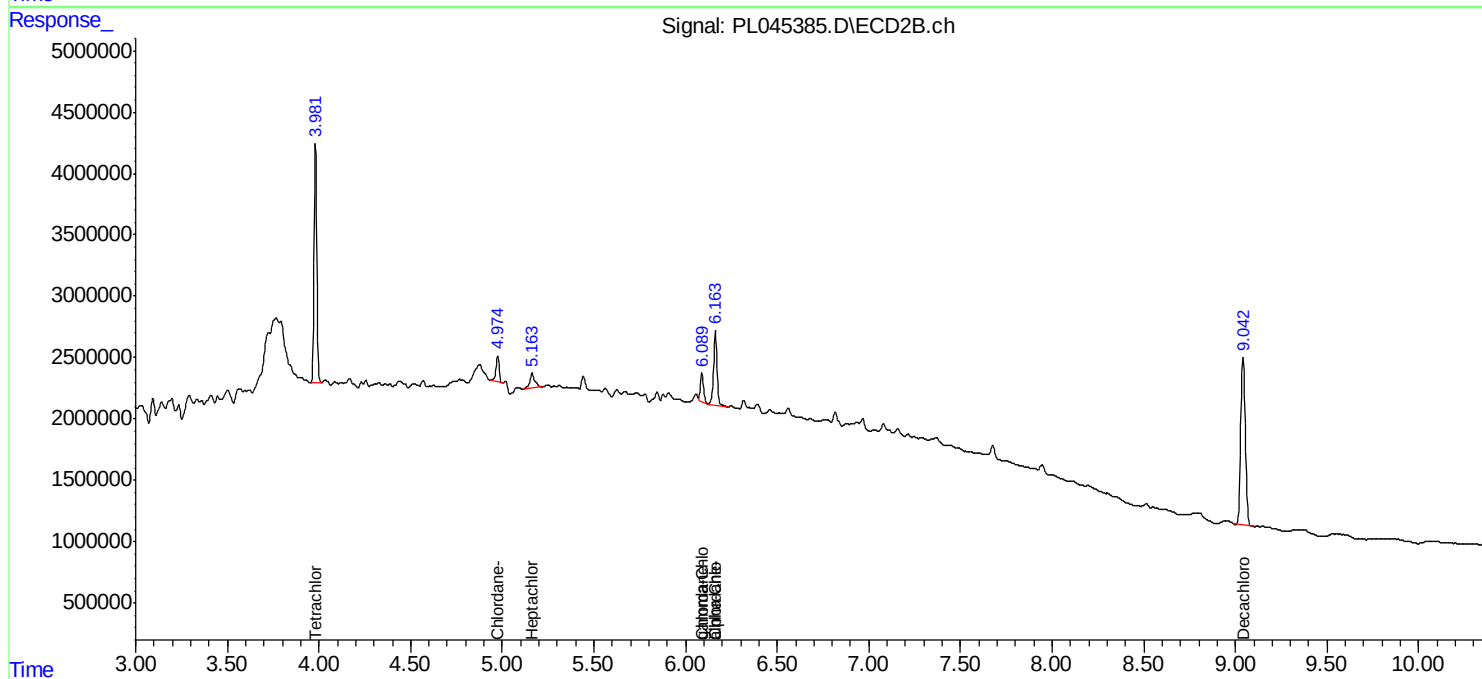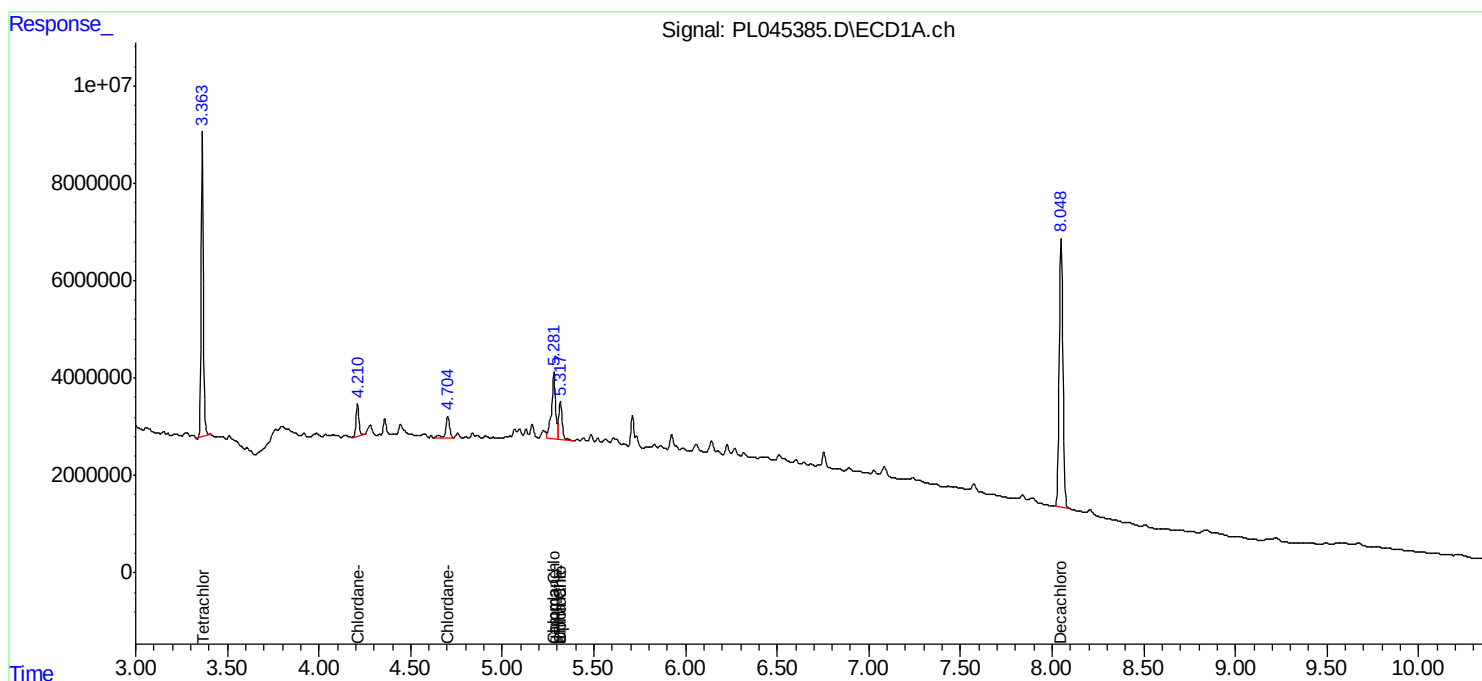


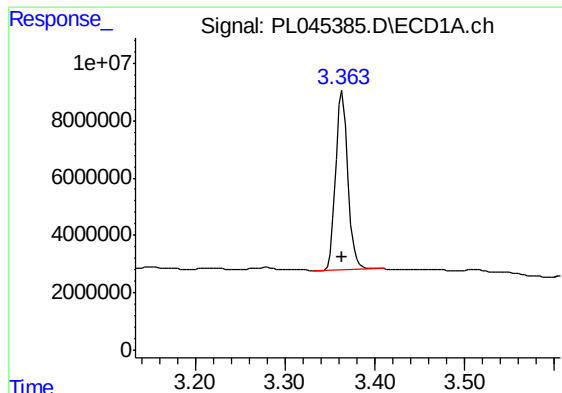

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.001 min
Response: 59583802
Conc: 8.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-F

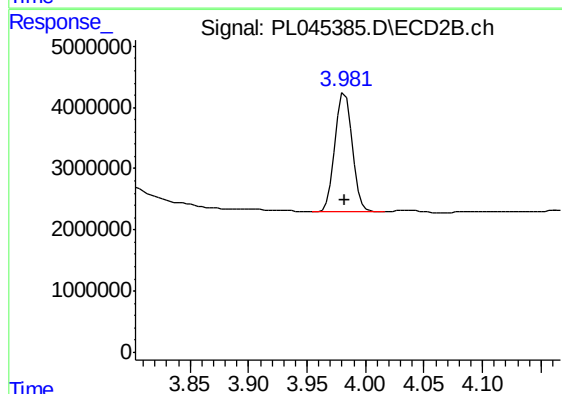


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 19444663
Conc: 9.08 ng/ml

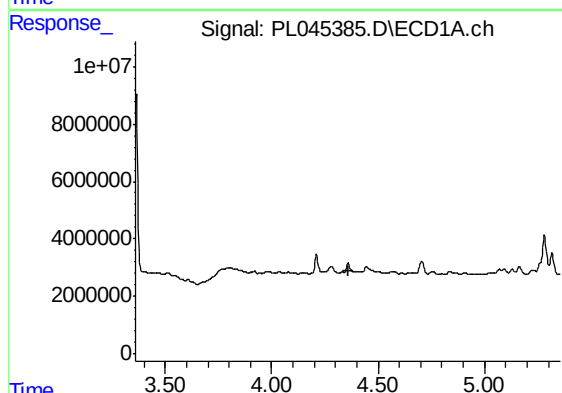


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.358 min
Response: 0
Conc: N.D.

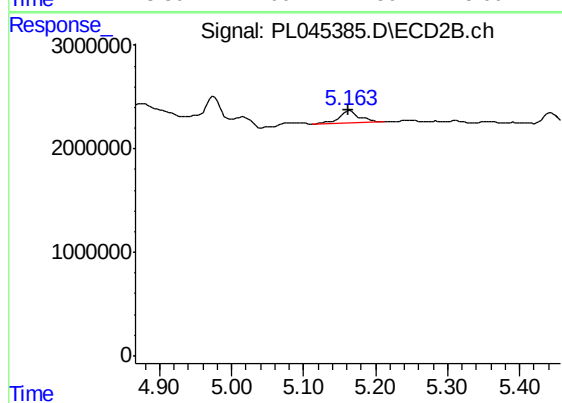

#4 Heptachlor


R.T.: 5.164 min
Delta R.T.: 0.000 min
Response: 2318432
Conc: 0.78 ng/ml

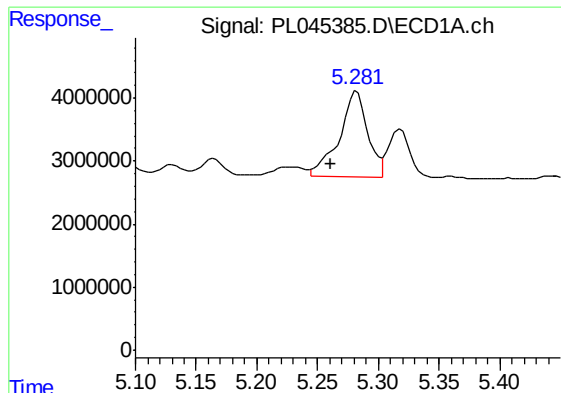

#10 gamma-Chlordane


R.T.: 5.282 min
Delta R.T.: 0.022 min
Response: 21692862
Conc: 2.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-F

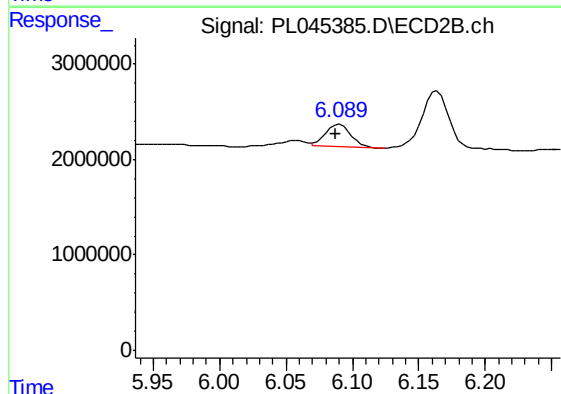


#10 gamma-Chlordane

R.T.: 6.091 min
Delta R.T.: 0.003 min
Response: 3122135
Conc: 1.16 ng/ml

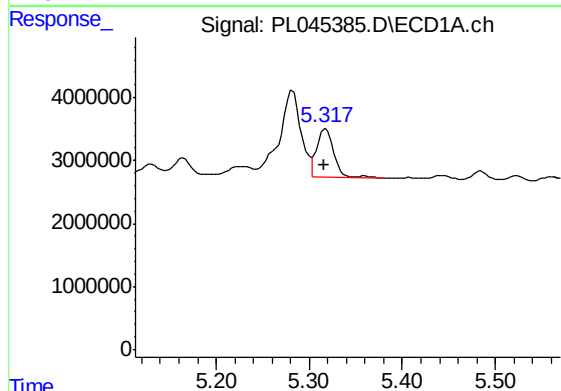


#11 alpha-Chlordane

R.T.: 5.318 min
Delta R.T.: 0.002 min
Response: 9822214
Conc: 1.01 ng/ml

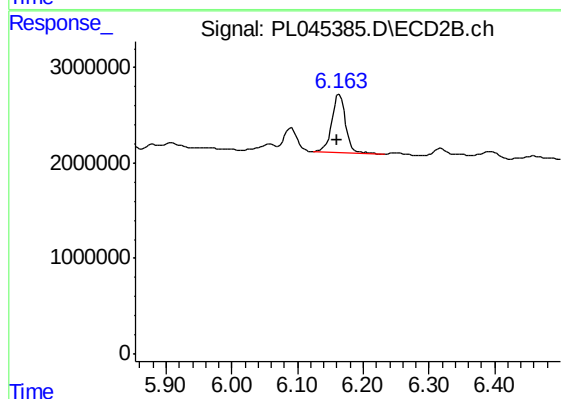

#11 alpha-Chlordane


R.T.: 6.164 min
Delta R.T.: 0.004 min
Response: 8763734
Conc: 3.25 ng/ml

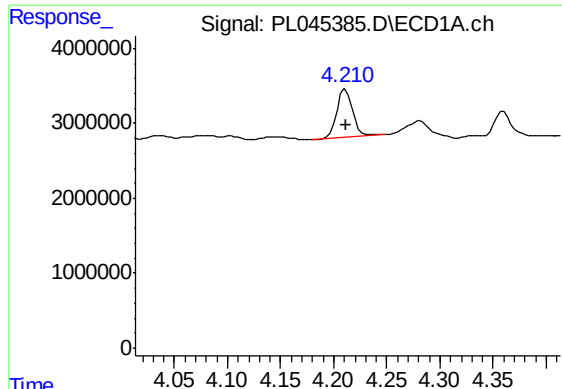

#23 Chlordane-1


R.T.: 4.211 min
Delta R.T.: 0.000 min
Response: 6755343
Conc: 20.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-F

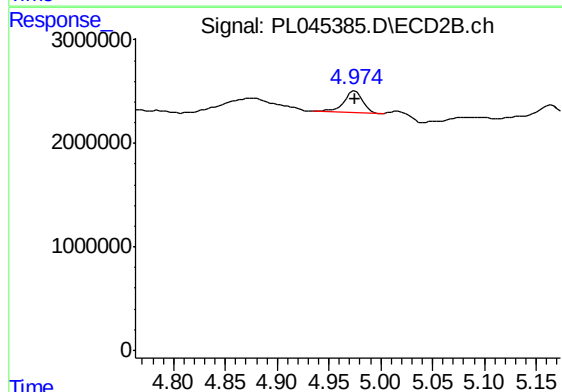


#23 Chlordane-1

R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 2626831
Conc: 23.30 ng/ml

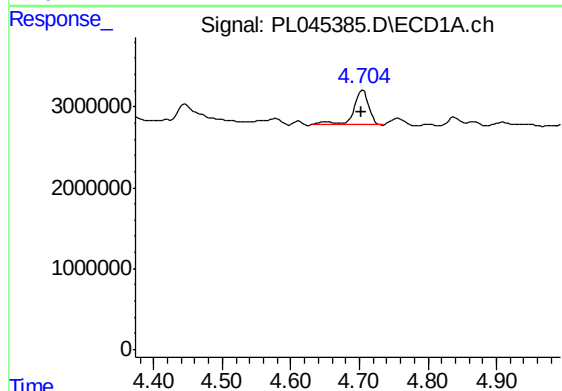


#24 Chlordane-2

R.T.: 4.705 min
Delta R.T.: 0.001 min
Response: 6769834
Conc: 17.50 ng/ml

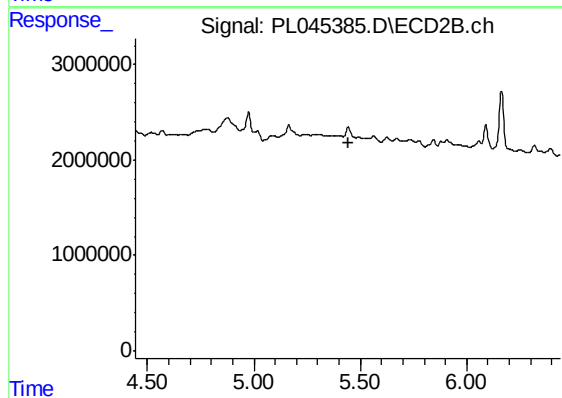

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.443 min
Response: 0
Conc: N.D.

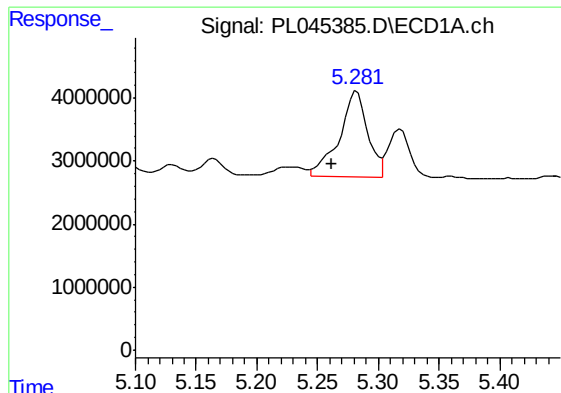

#25 Chlordane-3


R.T.: 5.282 min
Delta R.T.: 0.021 min
Response: 21692862
Conc: 18.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-F

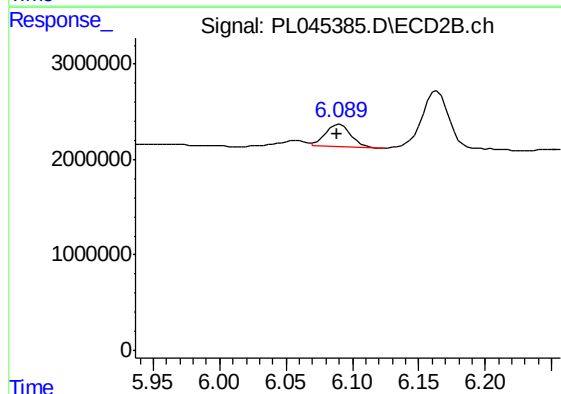


#25 Chlordane-3

R.T.: 6.091 min
Delta R.T.: 0.002 min
Response: 3122135
Conc: 8.01 ng/ml

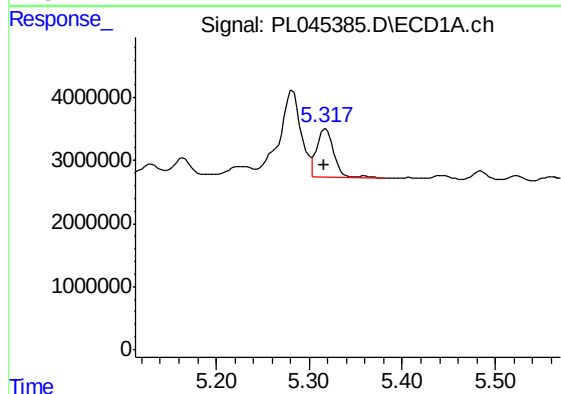


#26 Chlordane-4

R.T.: 5.318 min
Delta R.T.: 0.001 min
Response: 9822214
Conc: 9.27 ng/ml

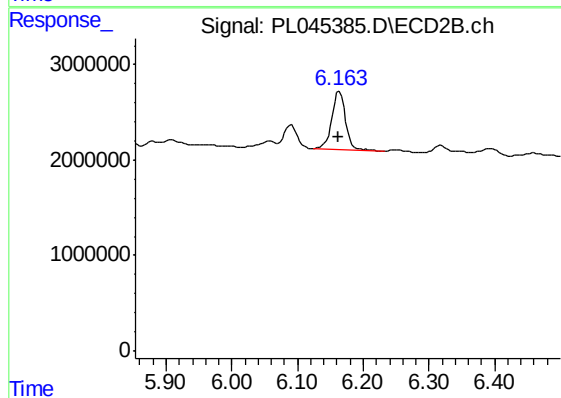

#26 Chlordane-4


R.T.: 6.164 min
Delta R.T.: 0.002 min
Response: 8763734
Conc: 18.73 ng/ml

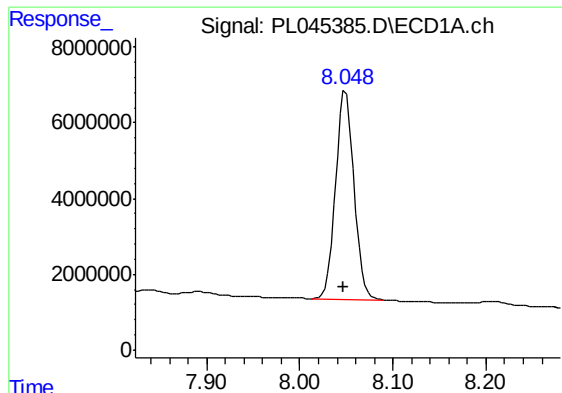

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 75303957
Conc: 9.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-F

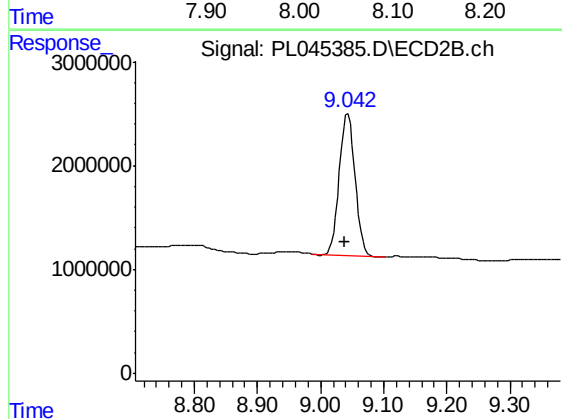

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.004 min
Response: 23609770
Conc: 10.33 ng/ml