

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
 Data File : PL045388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 13:21
 Operator : AJ\SJ
 Sample : K1688-19
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-03-030119-J

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 23:51:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.983	63236249	20441387	9.192	9.545
28)	SA Decachlor...	8.049	9.043	70052692	21223127	8.372	9.288
Target Compounds							
10)	B gamma-Chl...	5.281f	0.000	6853201	0	0.700	N.D. #
11)	B alpha-Chl...	0.000	6.165	0	3518828	N.D.	1.304 #
16)	A 4,4'-DDD	0.000	6.816	0	1572130	N.D.	0.818 #
25)	Chlordane-3	5.281f	0.000	6853201	0	5.975	N.D. #
26)	Chlordane-4	0.000	6.165	0	3518828	N.D.	7.522 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
Data File : PL045388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 13:21
Operator : AJ\SJ
Sample : K1688-19
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-J

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 23:51:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

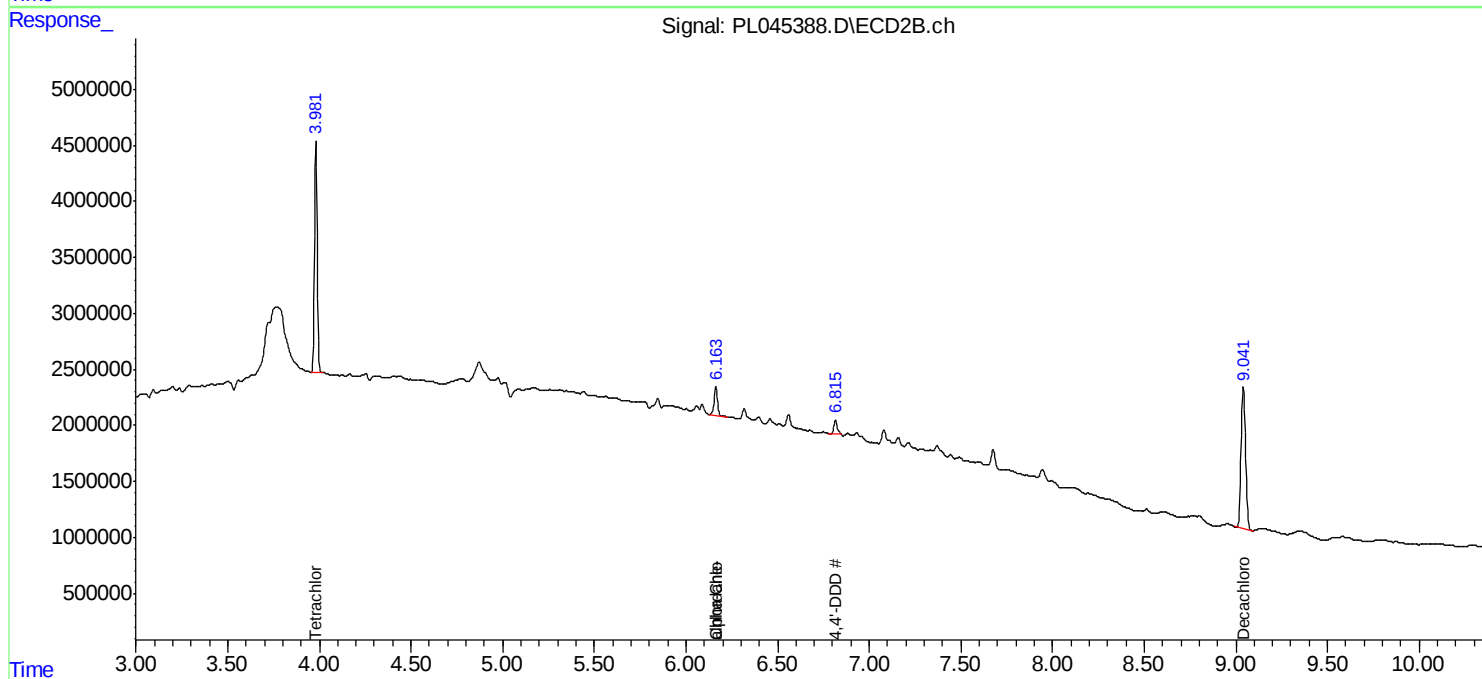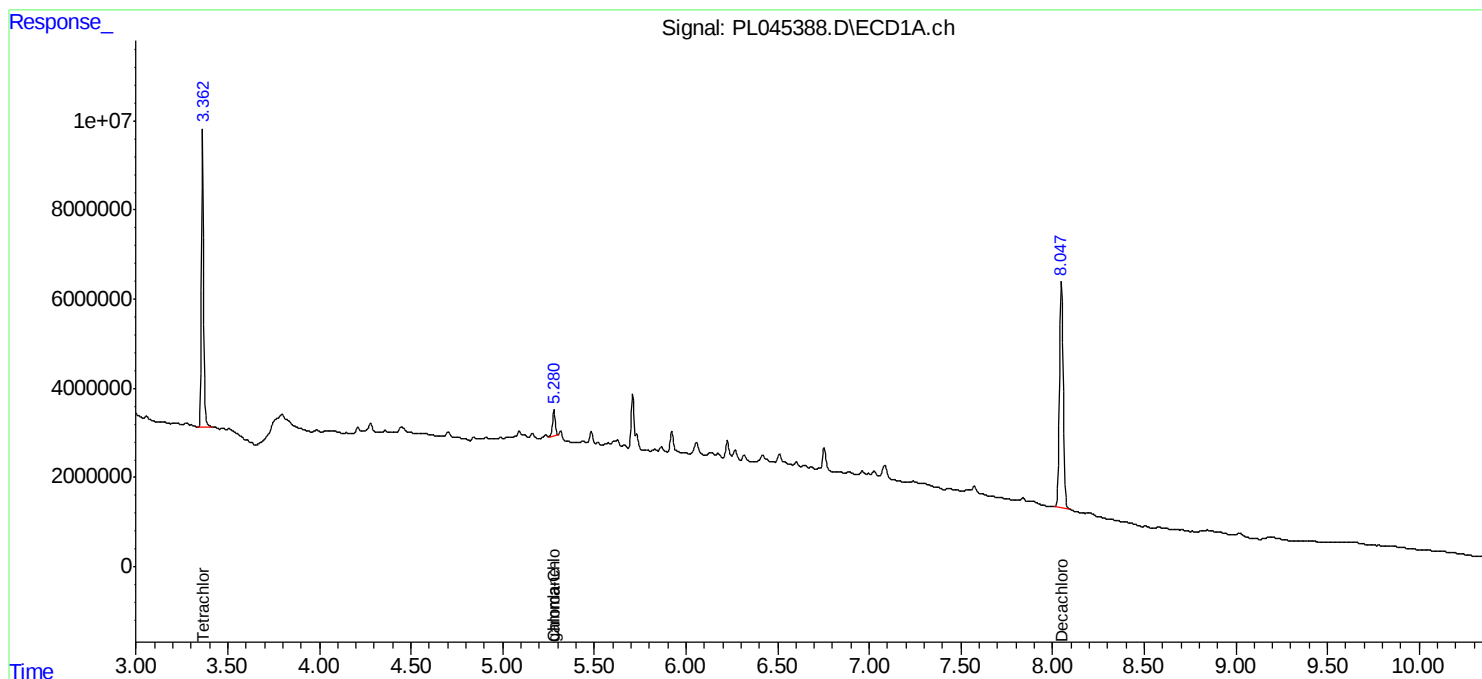


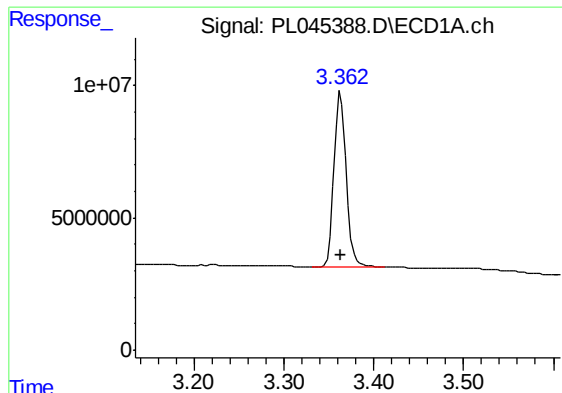

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 63236249
Conc: 9.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-J

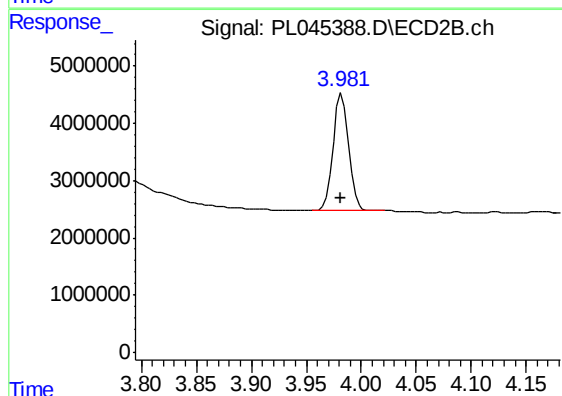


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 20441387
Conc: 9.55 ng/ml

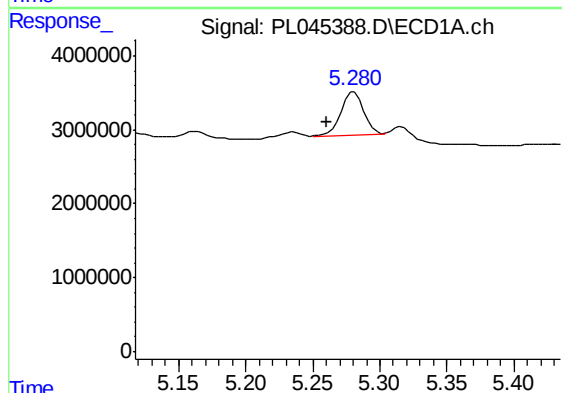


#10 gamma-Chlordane

R.T.: 5.281 min
Delta R.T.: 0.020 min
Response: 6853201
Conc: 0.70 ng/ml

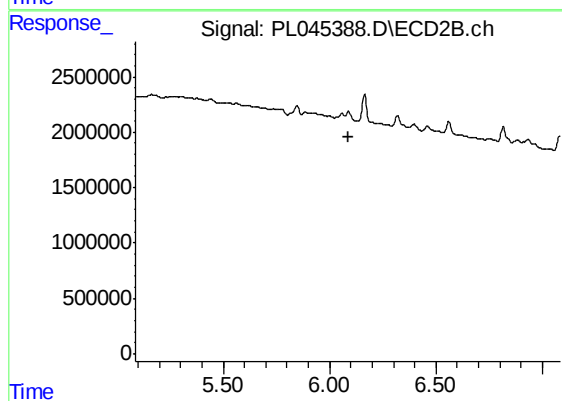

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

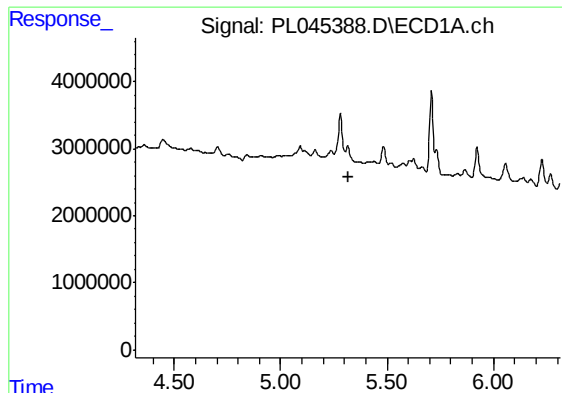

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-J

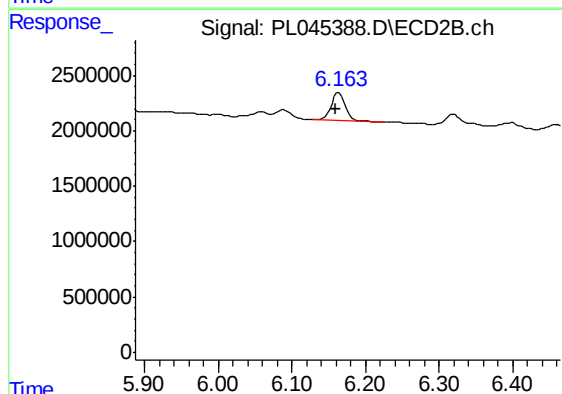


#11 alpha-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.004 min
Response: 3518828
Conc: 1.30 ng/ml

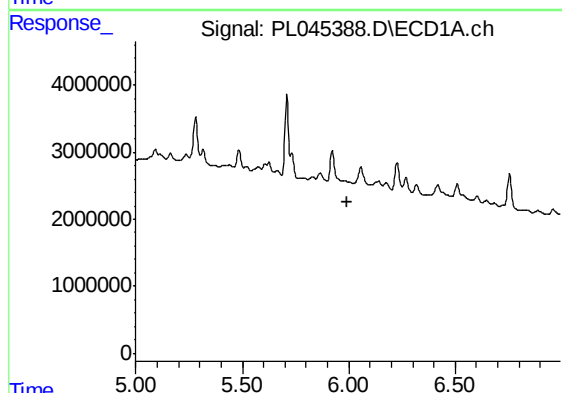


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

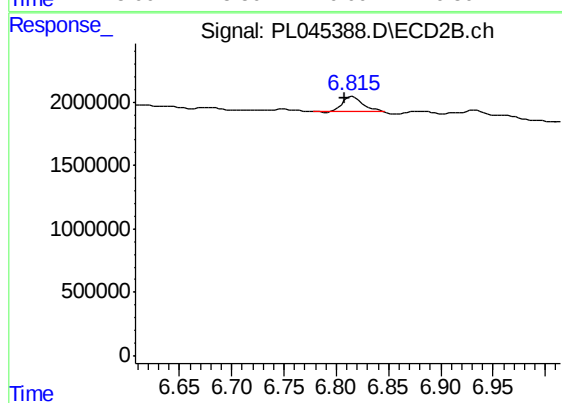

#16 4,4'-DDD


R.T.: 6.816 min
Delta R.T.: 0.008 min
Response: 1572130
Conc: 0.82 ng/ml

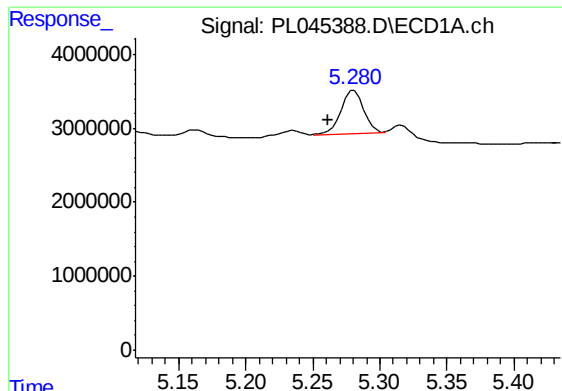

#25 Chlordane-3


R.T.: 5.281 min
Delta R.T.: 0.019 min
Response: 6853201
Conc: 5.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-J

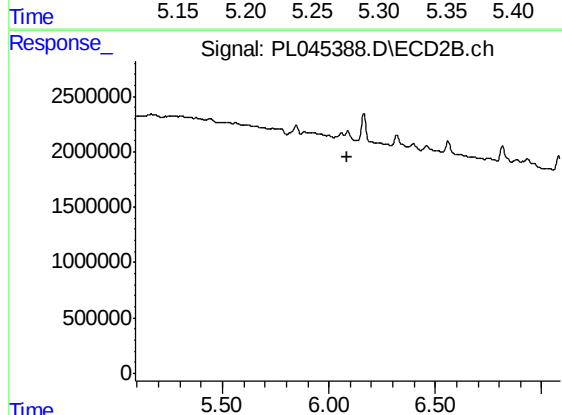


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

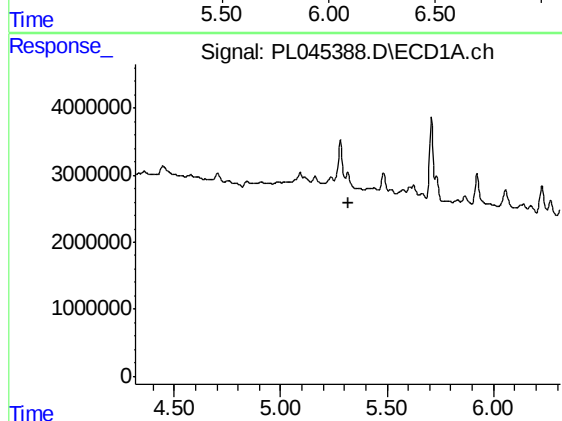


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

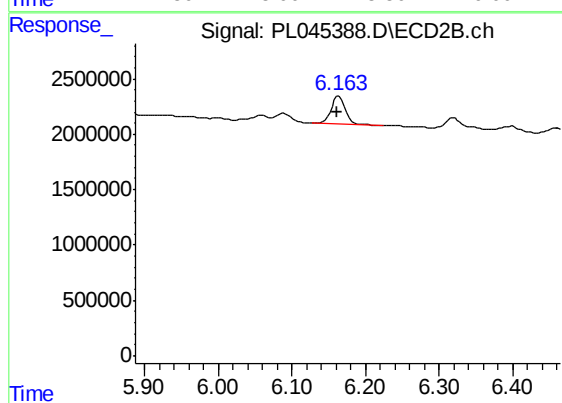

#26 Chlordane-4


R.T.: 6.165 min
Delta R.T.: 0.002 min
Response: 3518828
Conc: 7.52 ng/ml

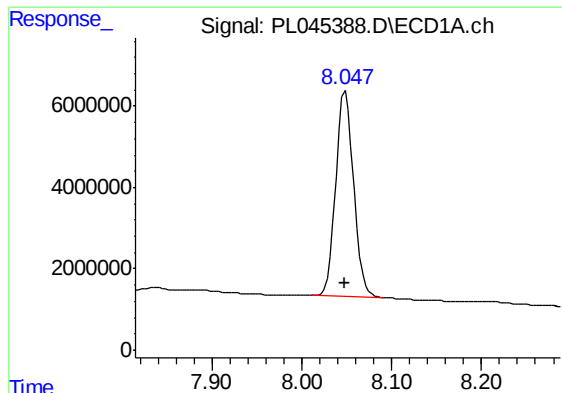

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.001 min
Response: 70052692
Conc: 8.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-03-030119-J

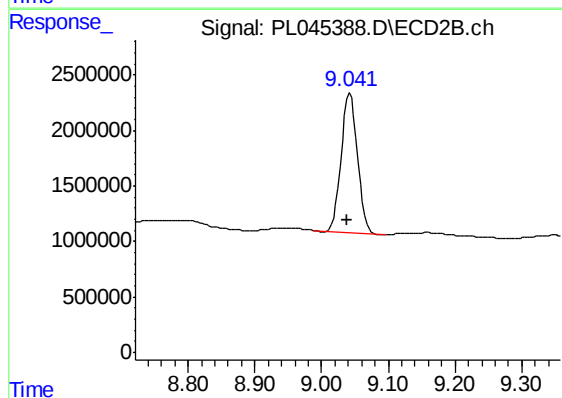

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.004 min
Response: 21223127
Conc: 9.29 ng/ml