

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
 Data File : PL045389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 13:35
 Operator : AJ\SJ
 Sample : K1707-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 23:51:50 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.983	51203915	16886586	7.443	7.885
28)	SA Decachlor...	8.049	9.043	75984409	22456729	9.081	9.828
Target Compounds							
12)	B 4,4'-DDE	0.000	6.320	0	1922426	N.D.	0.823 #
16)	A 4,4'-DDD	0.000	6.816	0	4474281	N.D.	2.327 #
17)	MA 4,4'-DDT	6.227	7.081f	15842648	972797	2.112	0.493 #
18)	B Endrin al...	6.319f	0.000	7323642	0	1.002	N.D. #
19)	B Endosulfa...	6.510	7.214f	15887798	291861	1.955	0.130 #
20)	A Methoxychlor	6.756f	0.000	27515310	0	6.265	N.D. #
21)	B Endrin ke...	7.028f	0.000	11475479	0	1.246	N.D. #
22)	Mirex	0.000	8.193f	0	2680905	N.D.	1.346 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
Data File : PL045389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 13:35
Operator : AJ\SJ
Sample : K1707-01
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
S10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 23:51:50 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

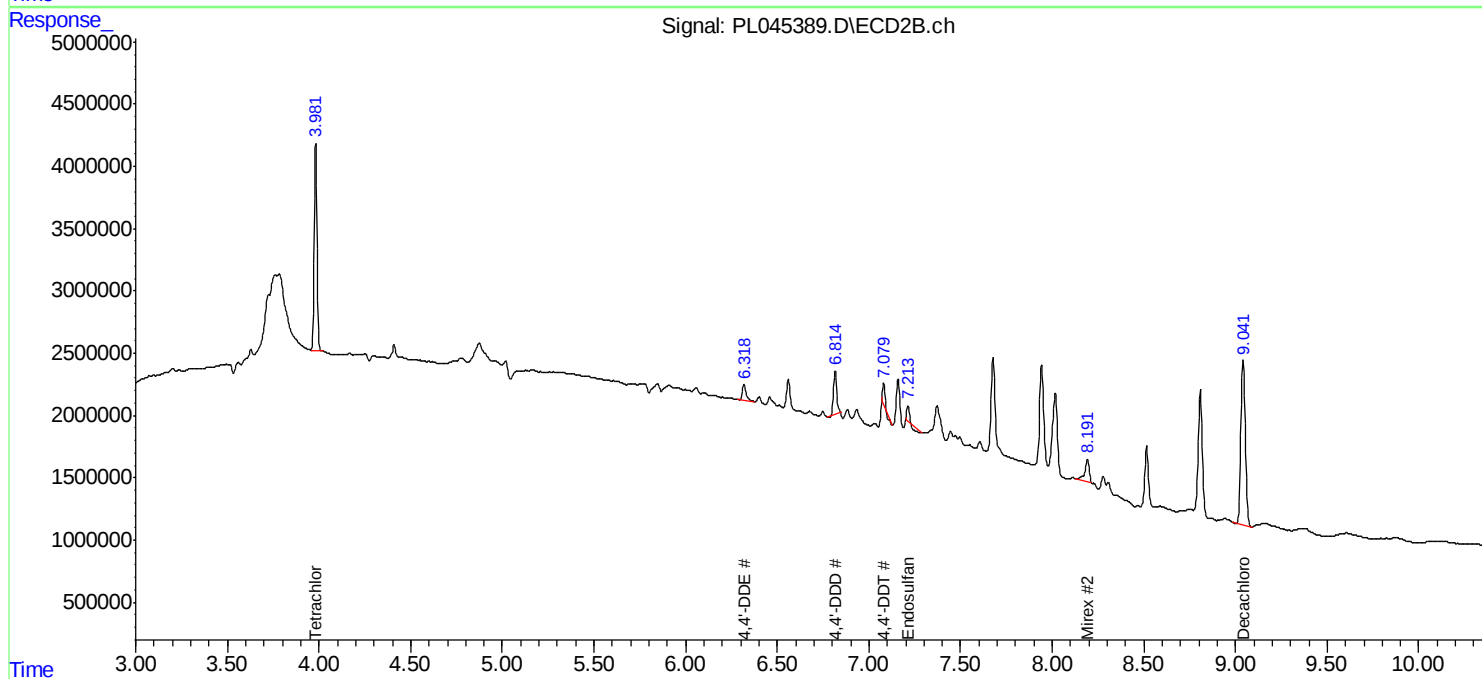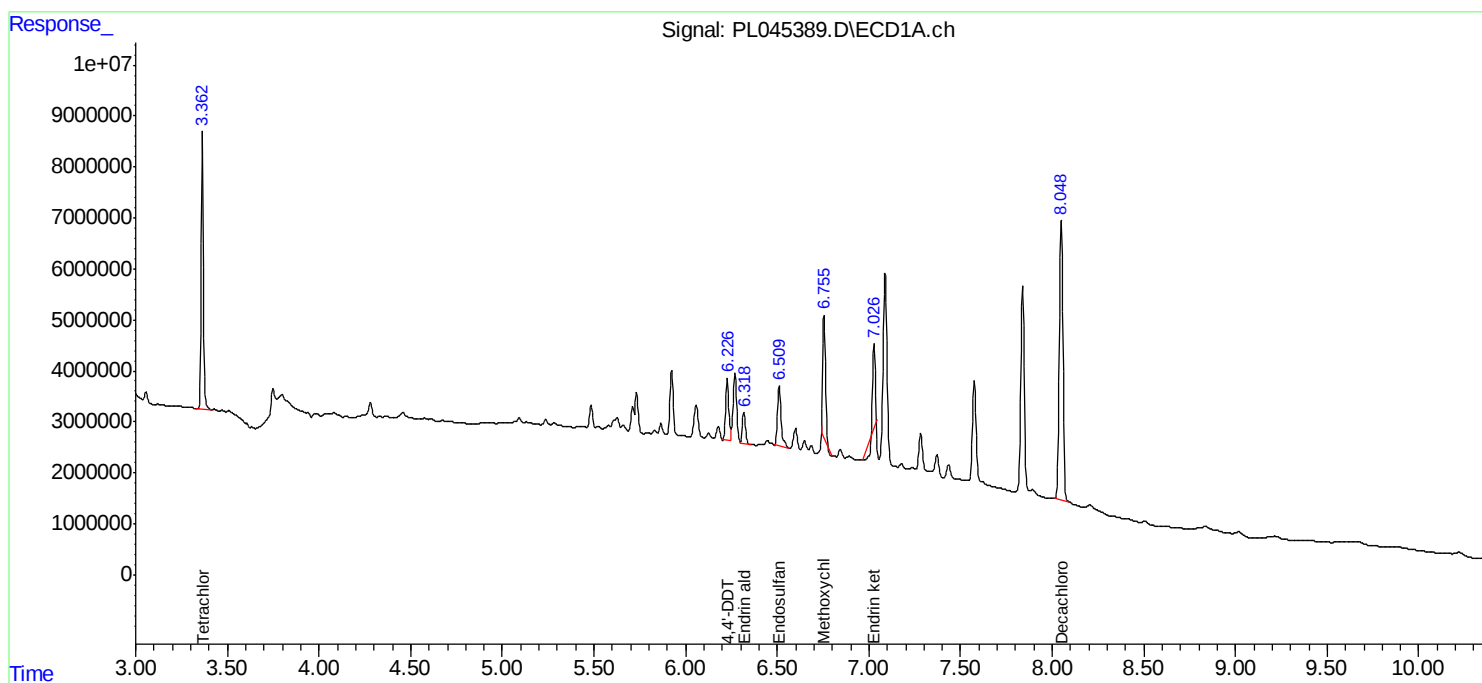


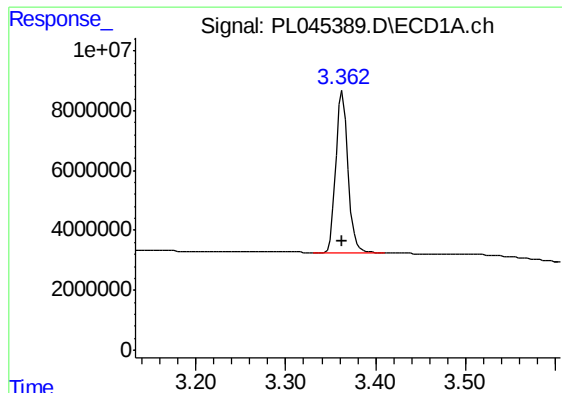

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 51203915
Conc: 7.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
S10

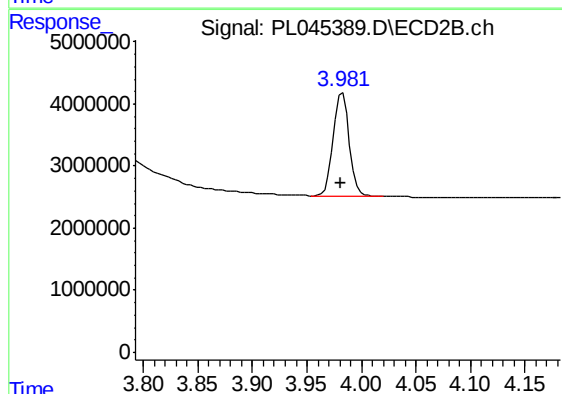


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 16886586
Conc: 7.89 ng/ml

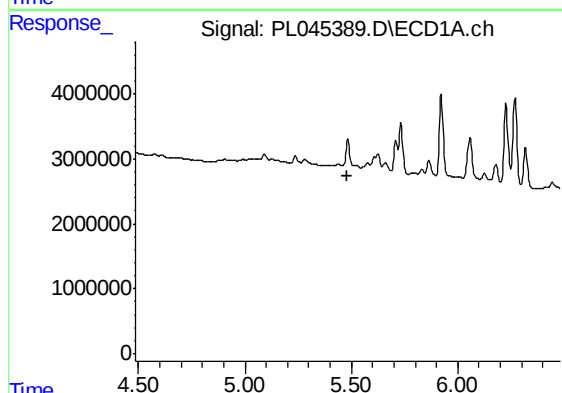


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.484 min
Response: 0
Conc: N.D.

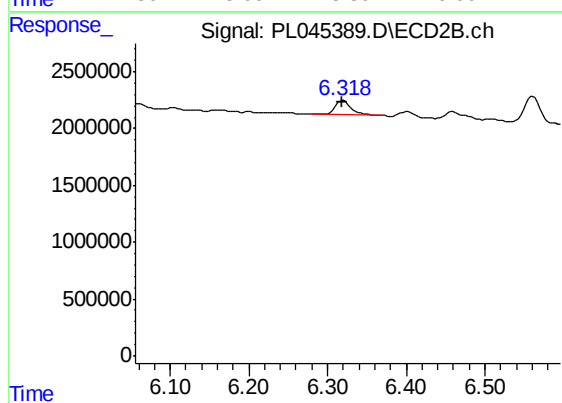

#12 4,4'-DDE


R.T.: 6.320 min
Delta R.T.: 0.002 min
Response: 1922426
Conc: 0.82 ng/ml

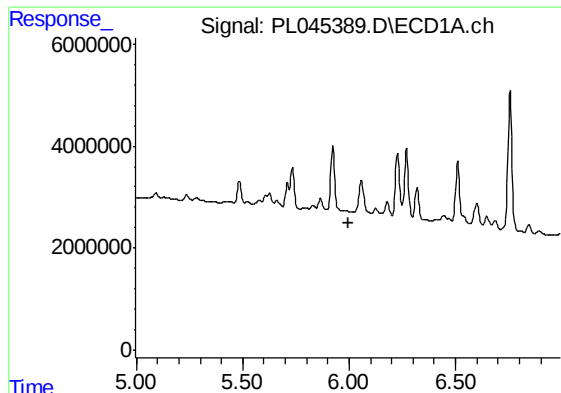

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S10

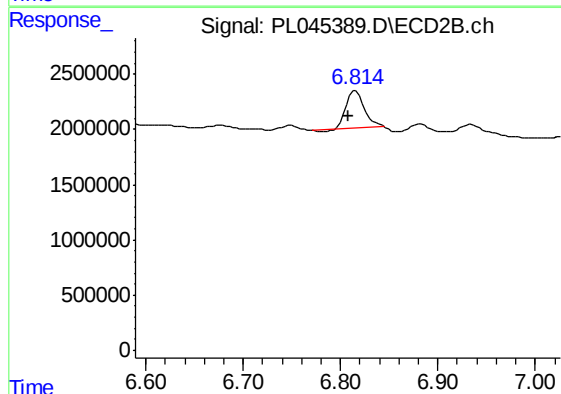


#16 4,4'-DDD

R.T.: 6.816 min
Delta R.T.: 0.008 min
Response: 4474281
Conc: 2.33 ng/ml

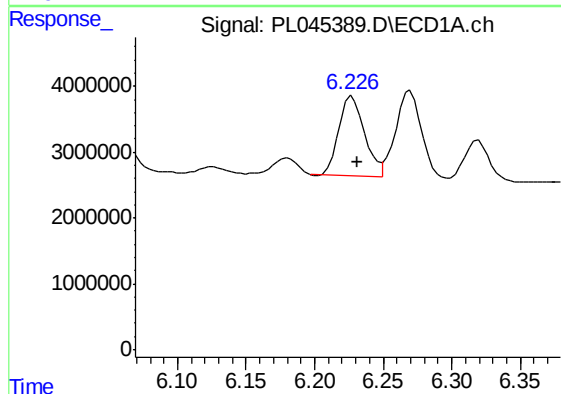


#17 4,4'-DDT

R.T.: 6.227 min
Delta R.T.: -0.003 min
Response: 15842648
Conc: 2.11 ng/ml

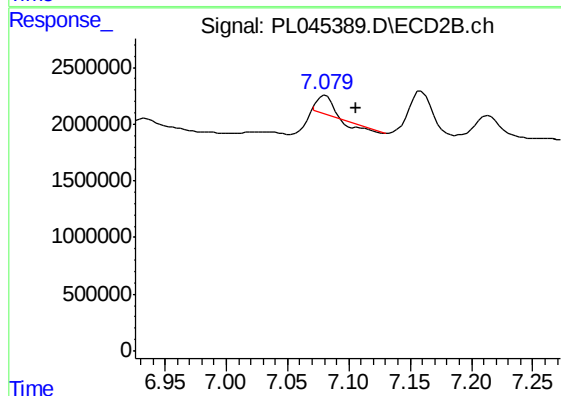

#17 4,4'-DDT


R.T.: 7.081 min
Delta R.T.: -0.025 min
Response: 972797
Conc: 0.49 ng/ml

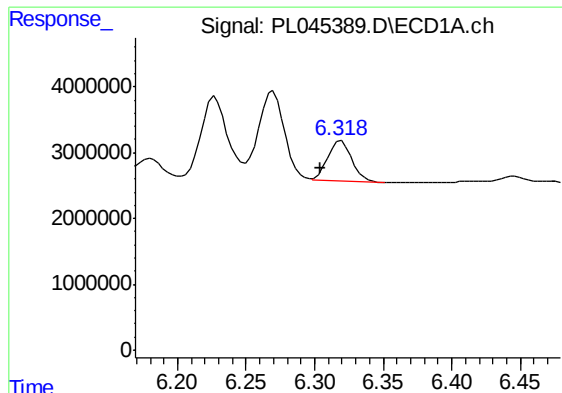

#18 Endrin aldehyde


R.T.: 6.319 min
Delta R.T.: 0.015 min
Response: 7323642
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
S10

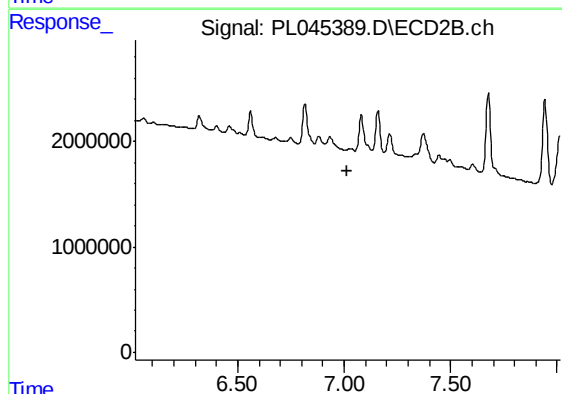


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

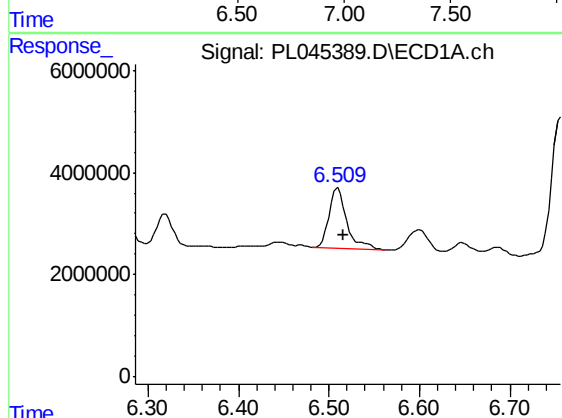


#19 Endosulfan Sulfate

R.T.: 6.510 min
Delta R.T.: -0.005 min
Response: 15887798
Conc: 1.95 ng/ml

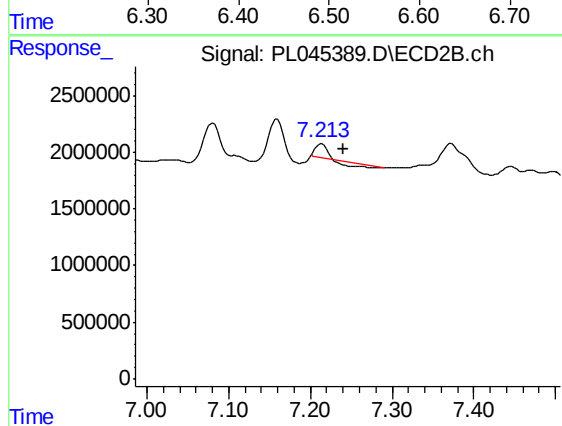

#19 Endosulfan Sulfate


R.T.: 7.214 min
Delta R.T.: -0.027 min
Response: 291861
Conc: 0.13 ng/ml

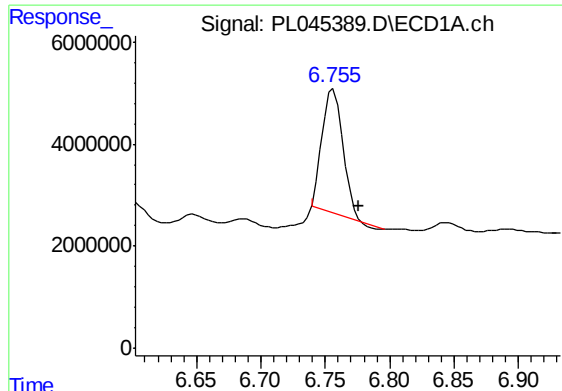

#20 Methoxychlor


R.T.: 6.756 min
Delta R.T.: -0.020 min
Response: 27515310
Conc: 6.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
S10

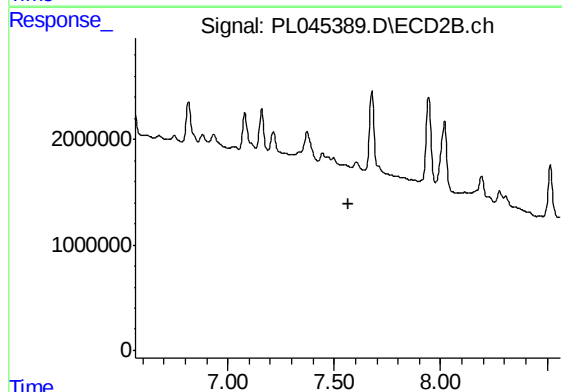


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

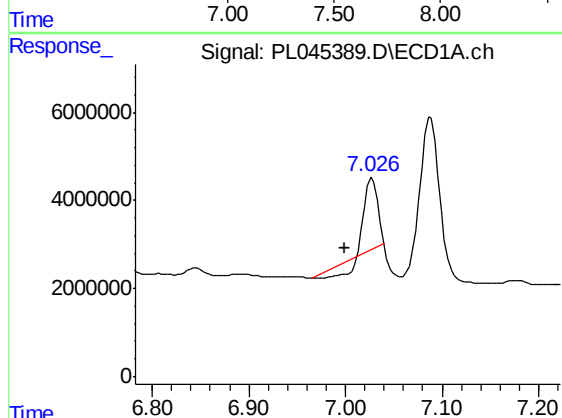


#21 Endrin ketone

R.T.: 7.028 min
Delta R.T.: 0.028 min
Response: 11475479
Conc: 1.25 ng/ml

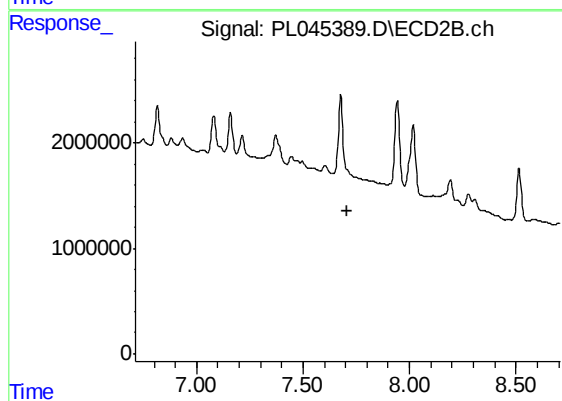

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

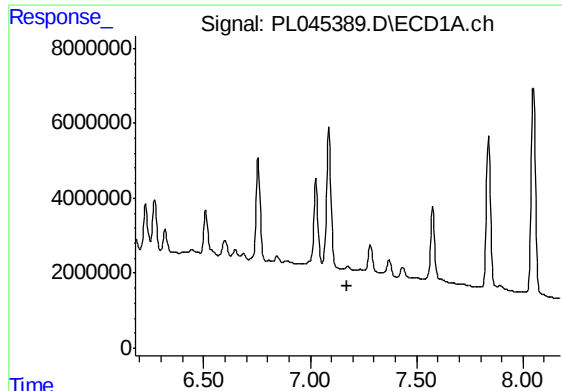

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S10

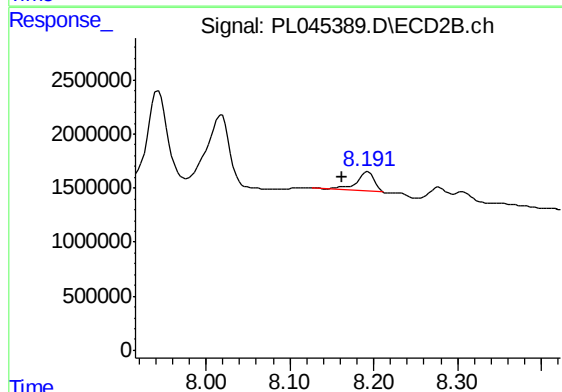


#22 Mirex

R.T.: 8.193 min
Delta R.T.: 0.030 min
Response: 2680905
Conc: 1.35 ng/ml

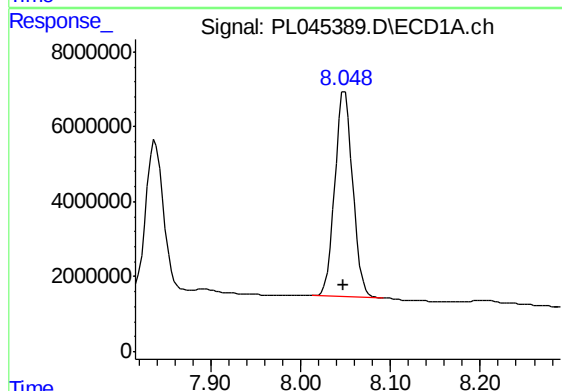

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 75984409
Conc: 9.08 ng/ml

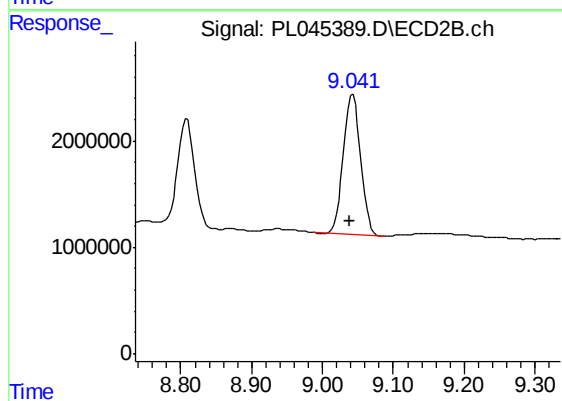

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.004 min
Response: 22456729
Conc: 9.83 ng/ml