

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
 Data File : PL045390.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 13:49
 Operator : AJ\SJ
 Sample : K1707-03
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S11

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 23:52:04 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.983	43829236	14606993	6.371	6.821
28)	SA Decachlor...	8.049	9.043	76345887	22610135	9.124	9.895
Target Compounds							
12)	B 4,4'-DDE	5.485	6.320	11279257	4656547	1.285	1.993 #
13)	MA Dieldrin	5.626f	6.460	7192310	2629582	0.752	1.023 #
15)	B Endosulfa...	0.000	6.881	0	2427178	N.D.	1.032 #
16)	A 4,4'-DDD	0.000	6.815	0	7752913	N.D.	4.031 #
17)	MA 4,4'-DDT	6.227	7.080f	26578672	1173051	3.544	0.594 #
18)	B Endrin al...	6.319f	0.000	17700320	0	2.422	N.D. #
19)	B Endosulfa...	6.510	7.214f	40617476	1001534	4.997	0.445 #
20)	A Methoxychlor	6.756f	0.000	56650067	0	12.899	N.D. #
21)	B Endrin ke...	7.028f	0.000	27214784	0	2.954	N.D. #
22)	Mirex	0.000	8.193f	0	6762518	N.D.	3.395 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
Data File : PL045390.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 13:49
Operator : AJ\SJ
Sample : K1707-03
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
S11

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 23:52:04 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

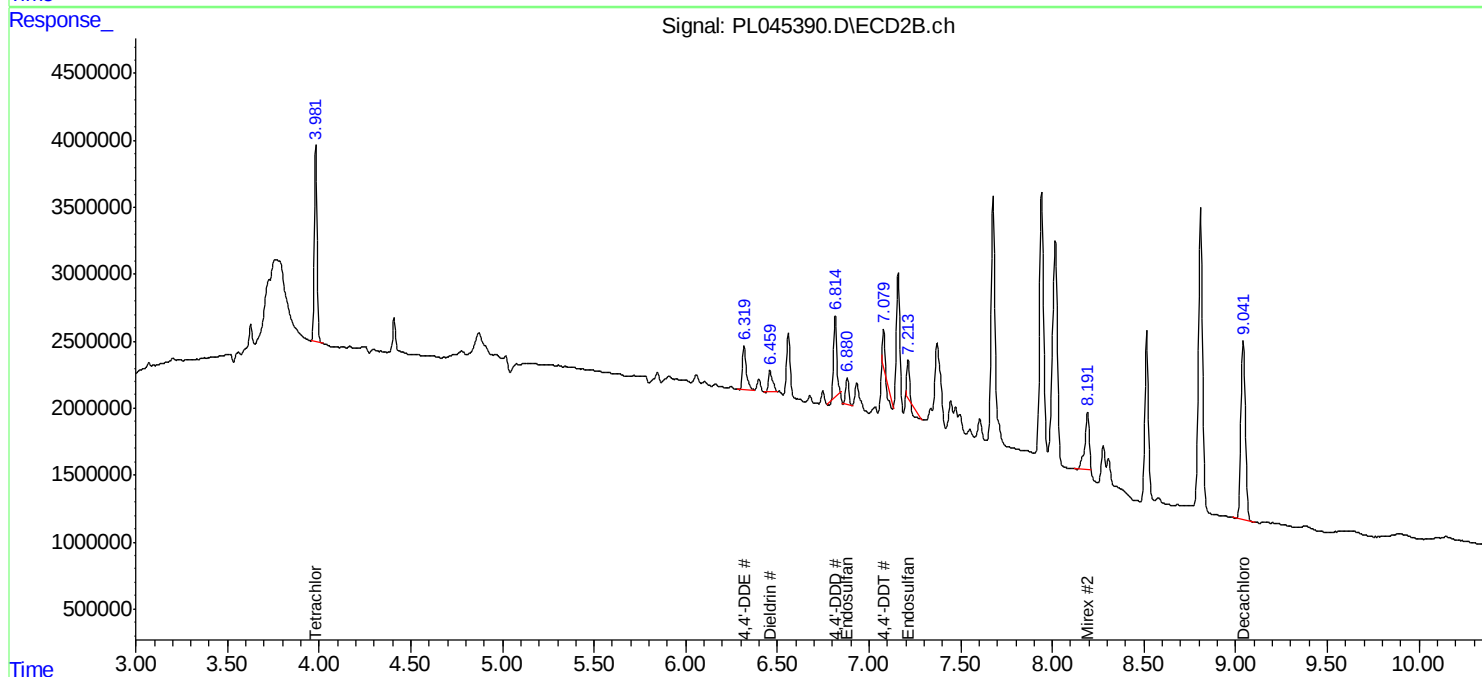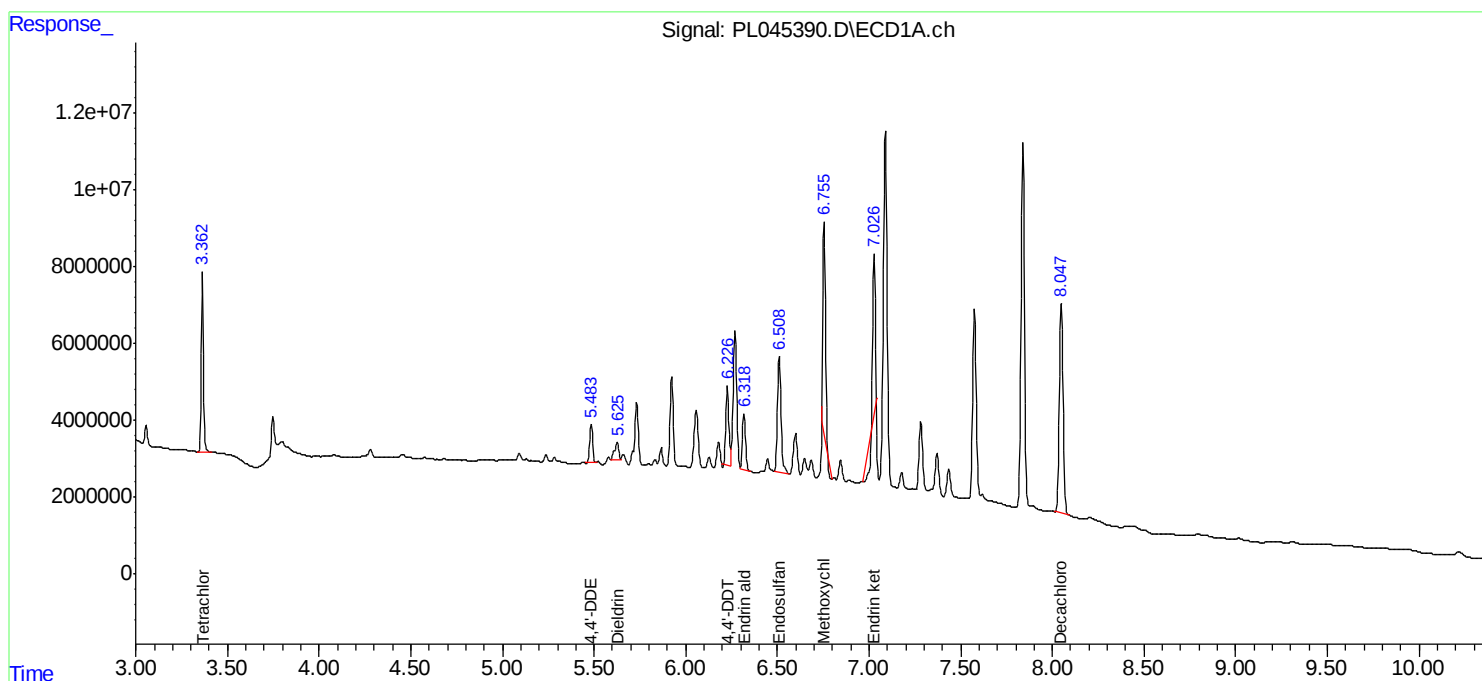


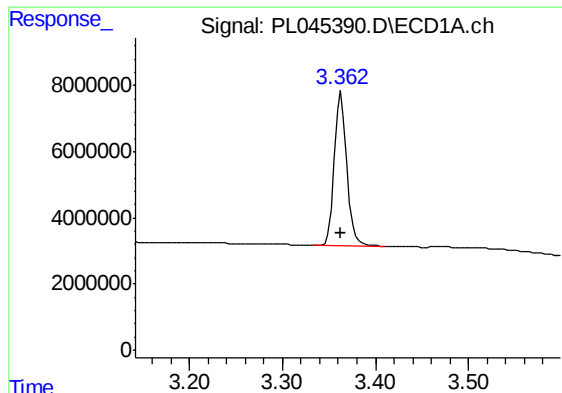

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 43829236
Conc: 6.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
S11

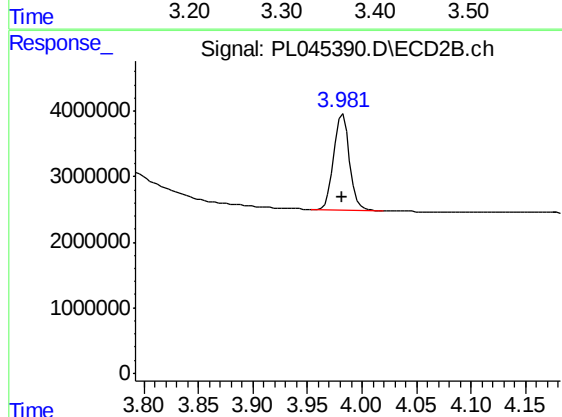


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 14606993
Conc: 6.82 ng/ml

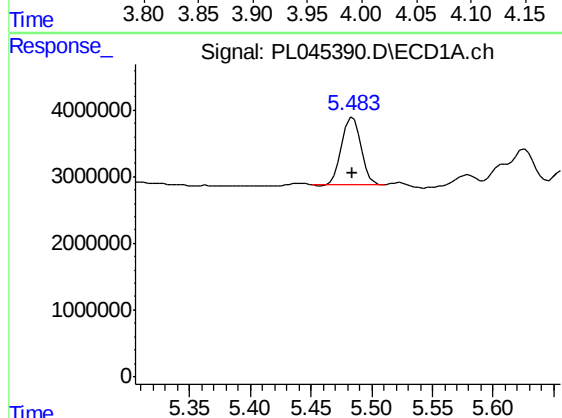


#12 4,4'-DDE

R.T.: 5.485 min
Delta R.T.: 0.000 min
Response: 11279257
Conc: 1.28 ng/ml

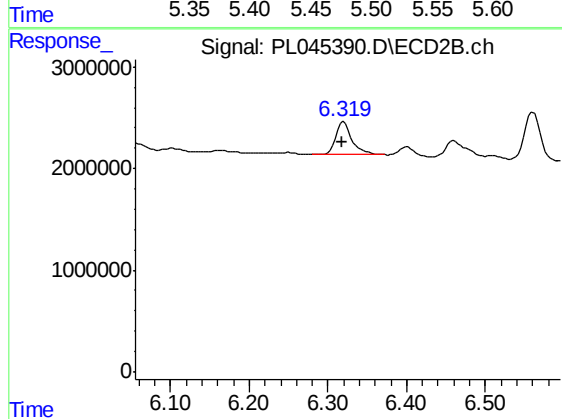

#12 4,4'-DDE


R.T.: 6.320 min
Delta R.T.: 0.002 min
Response: 4656547
Conc: 1.99 ng/ml

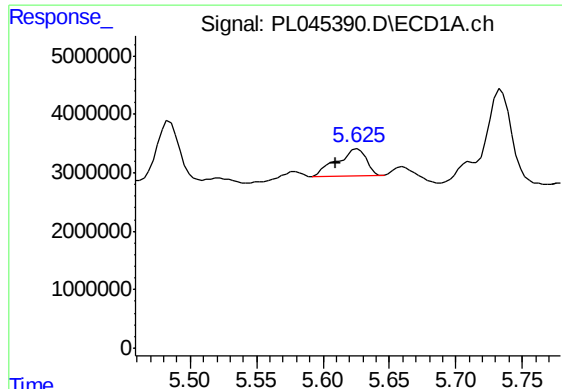

#13 Dieldrin


R.T.: 5.626 min
Delta R.T.: 0.017 min
Response: 7192310
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
S11

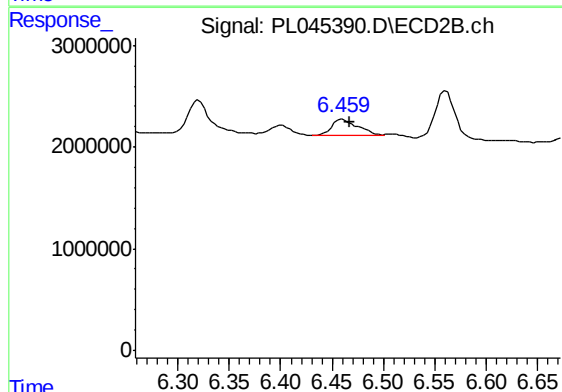


#13 Dieldrin

R.T.: 6.460 min
Delta R.T.: -0.006 min
Response: 2629582
Conc: 1.02 ng/ml

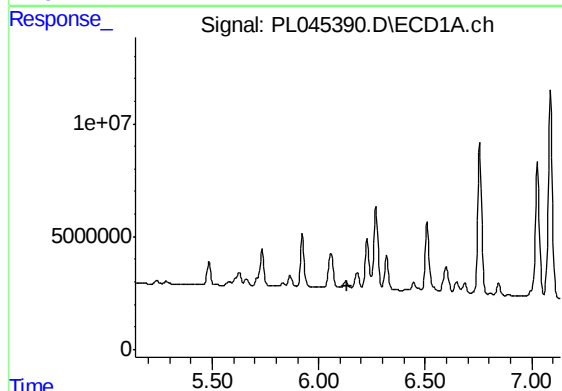


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

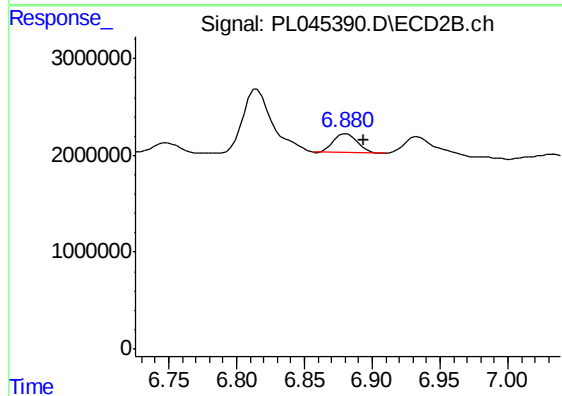

#15 Endosulfan II


R.T.: 6.881 min
Delta R.T.: -0.013 min
Response: 2427178
Conc: 1.03 ng/ml

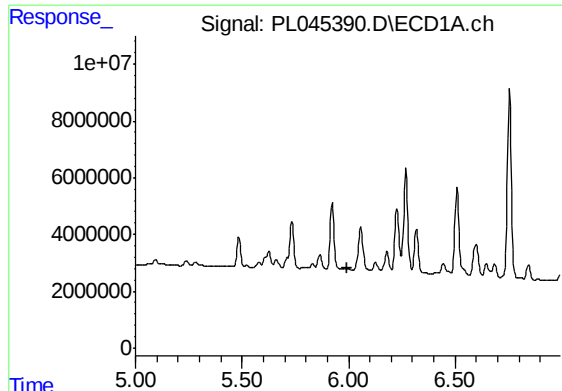

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S11

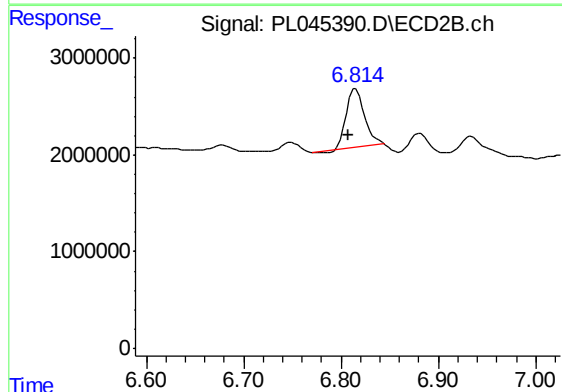


#16 4,4'-DDD

R.T.: 6.815 min
Delta R.T.: 0.008 min
Response: 7752913
Conc: 4.03 ng/ml

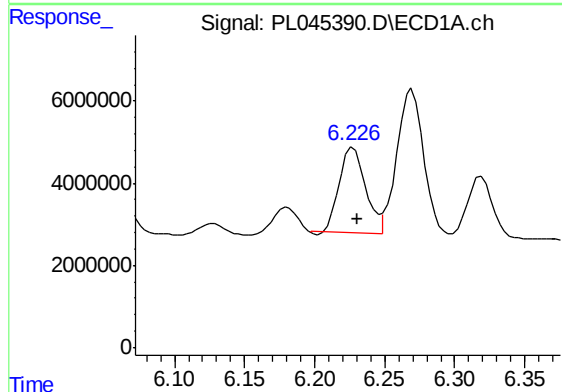


#17 4,4'-DDT

R.T.: 6.227 min
Delta R.T.: -0.003 min
Response: 26578672
Conc: 3.54 ng/ml

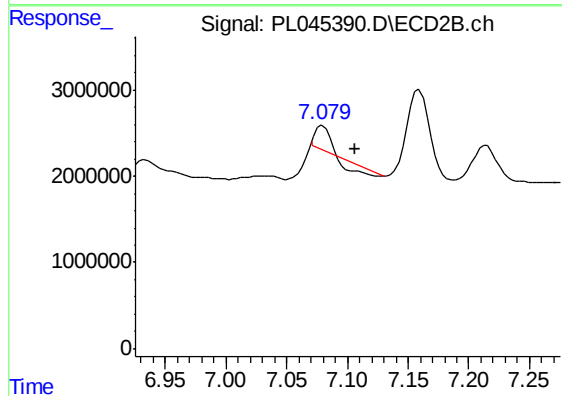

#17 4,4'-DDT


R.T.: 7.080 min
Delta R.T.: -0.026 min
Response: 1173051
Conc: 0.59 ng/ml

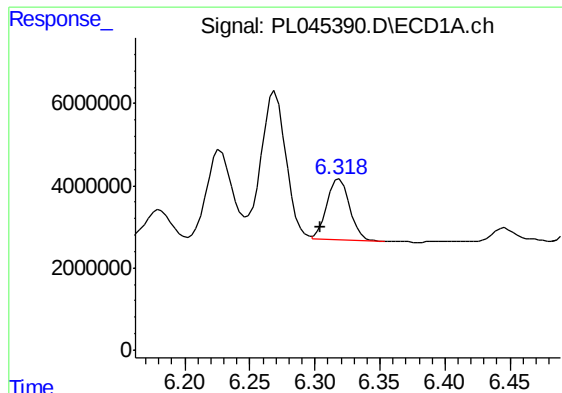

#18 Endrin aldehyde


R.T.: 6.319 min
Delta R.T.: 0.015 min
Response: 17700320
Conc: 2.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
S11

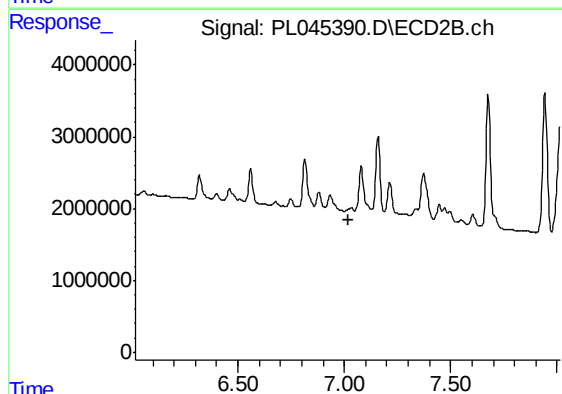


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.017 min
Response: 0
Conc: N.D.

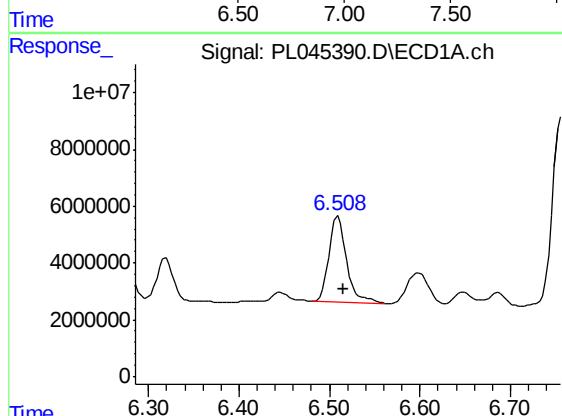


#19 Endosulfan Sulfate

R.T.: 6.510 min
Delta R.T.: -0.006 min
Response: 40617476
Conc: 5.00 ng/ml

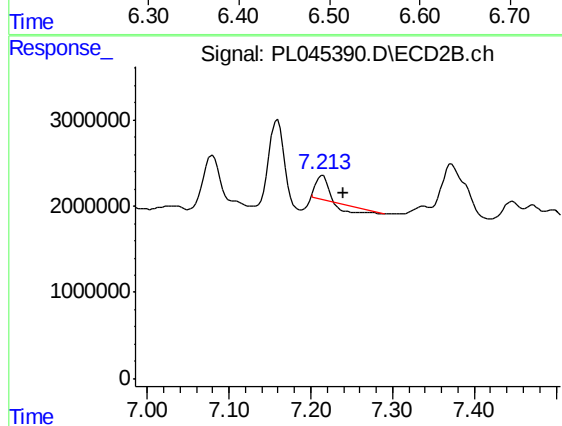

#19 Endosulfan Sulfate


R.T.: 7.214 min
Delta R.T.: -0.026 min
Response: 1001534
Conc: 0.45 ng/ml

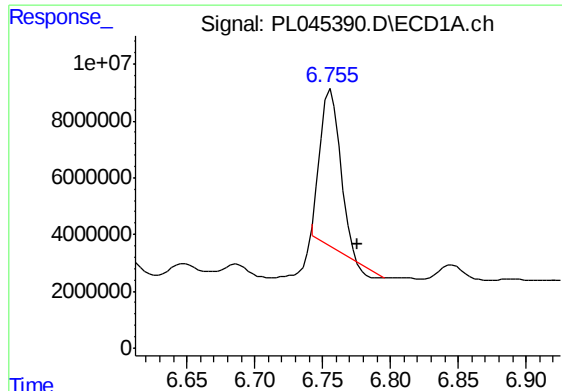

#20 Methoxychlor


R.T.: 6.756 min
Delta R.T.: -0.020 min
Response: 56650067
Conc: 12.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
S11

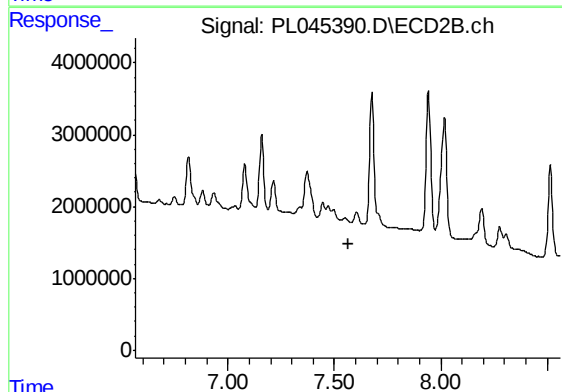


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

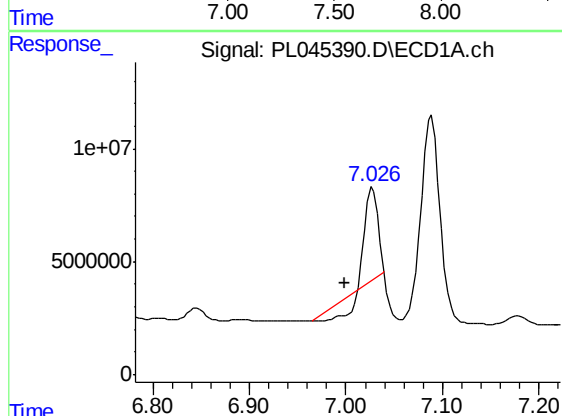


#21 Endrin ketone

R.T.: 7.028 min
Delta R.T.: 0.028 min
Response: 27214784
Conc: 2.95 ng/ml

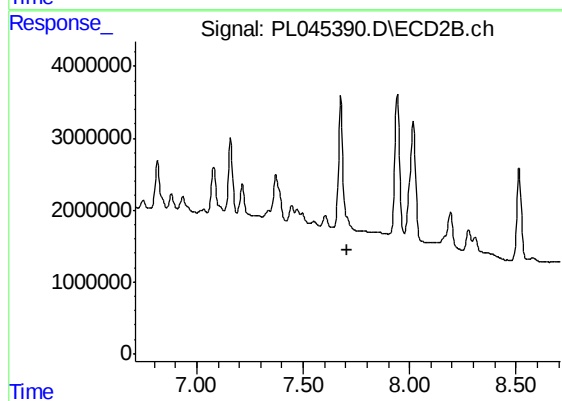

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.710 min
Response: 0
Conc: N.D.

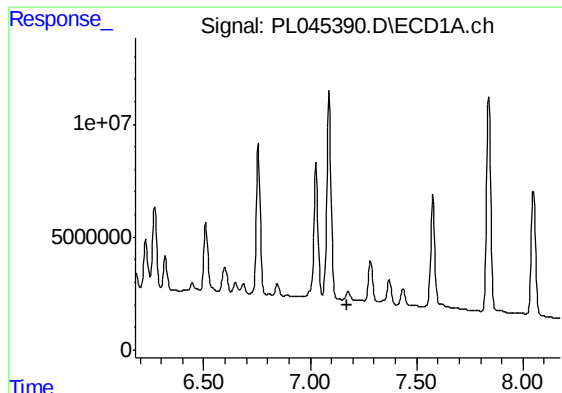

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.176 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S11

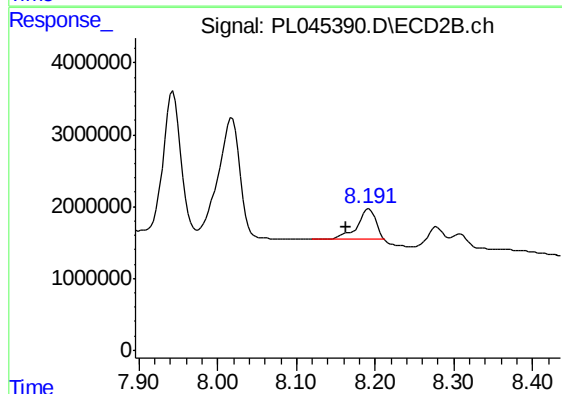


#22 Mirex

R.T.: 8.193 min
Delta R.T.: 0.030 min
Response: 6762518
Conc: 3.40 ng/ml

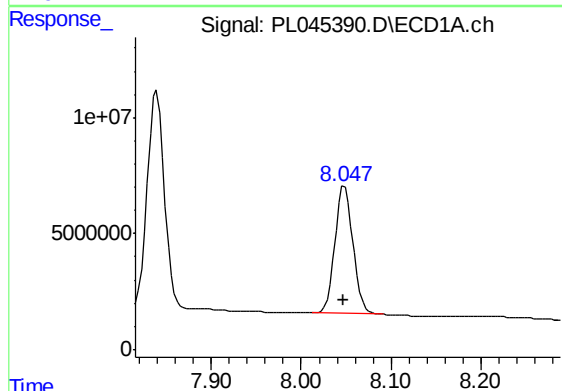

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.001 min
Response: 76345887
Conc: 9.12 ng/ml

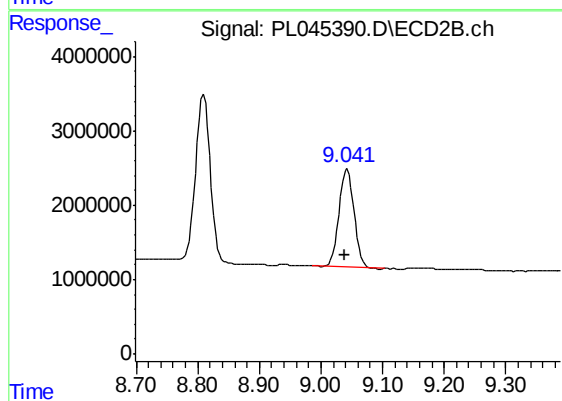

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.004 min
Response: 22610135
Conc: 9.90 ng/ml