

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
 Data File : PL045395.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 14:59
 Operator : AJ\SJ
 Sample : K1712-15
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 Z-2-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 23:53:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.364	3.982	58892583	19360539	8.561	9.040
28)	SA Decachlor...	8.049	9.043	88548239	26114950	10.582	11.429
Target Compounds							
10)	B gamma-Chl...	5.247	0.000	4206971	0	0.430	N.D. #
12)	B 4,4'-DDE	5.485	6.320	6681060	2175229	0.761	0.931
17)	MA 4,4'-DDT	6.229	0.000	6626093	0	0.883	N.D. #
20)	A Methoxychlor	6.756f	0.000	5344357	0	1.217	N.D. #
25)	Chlordane-3	5.247	0.000	4206971	0	3.668	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
Data File : PL045395.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 14:59
Operator : AJ\SJ
Sample : K1712-15
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
Z-2-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 23:53:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

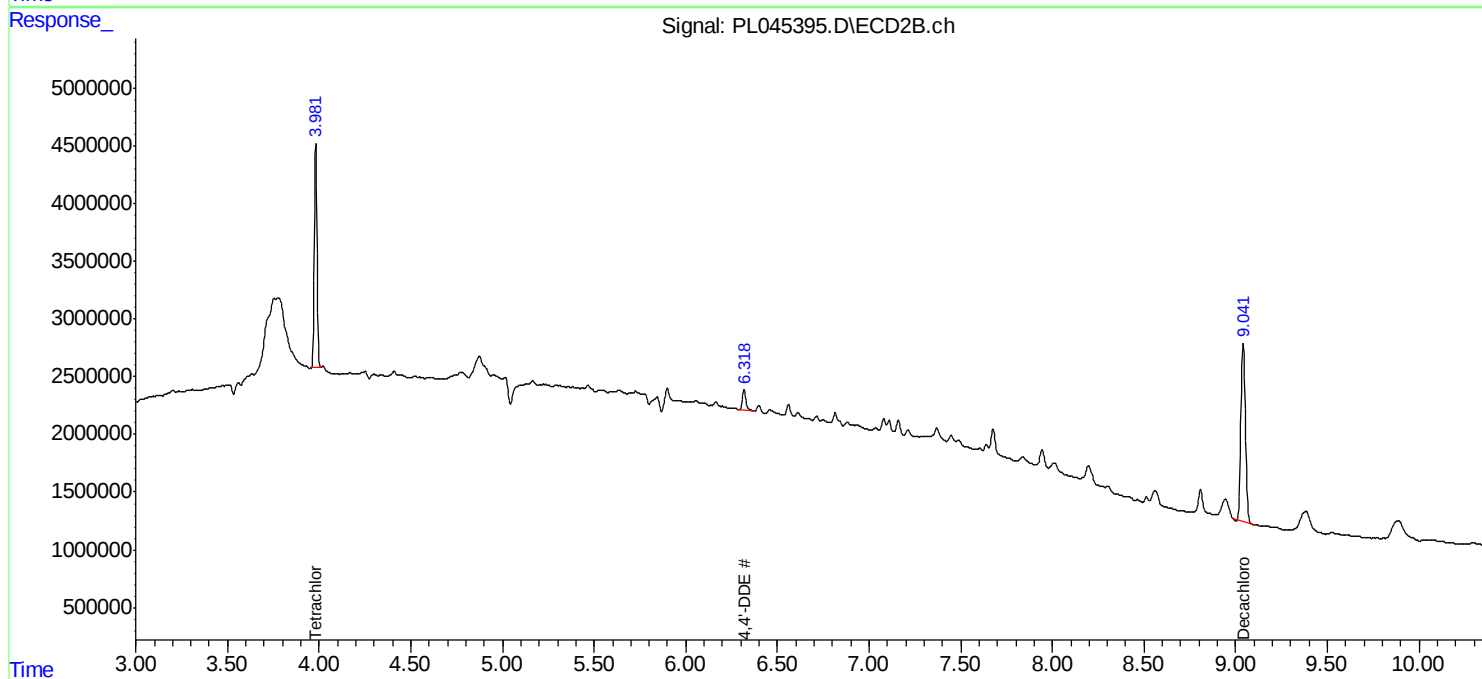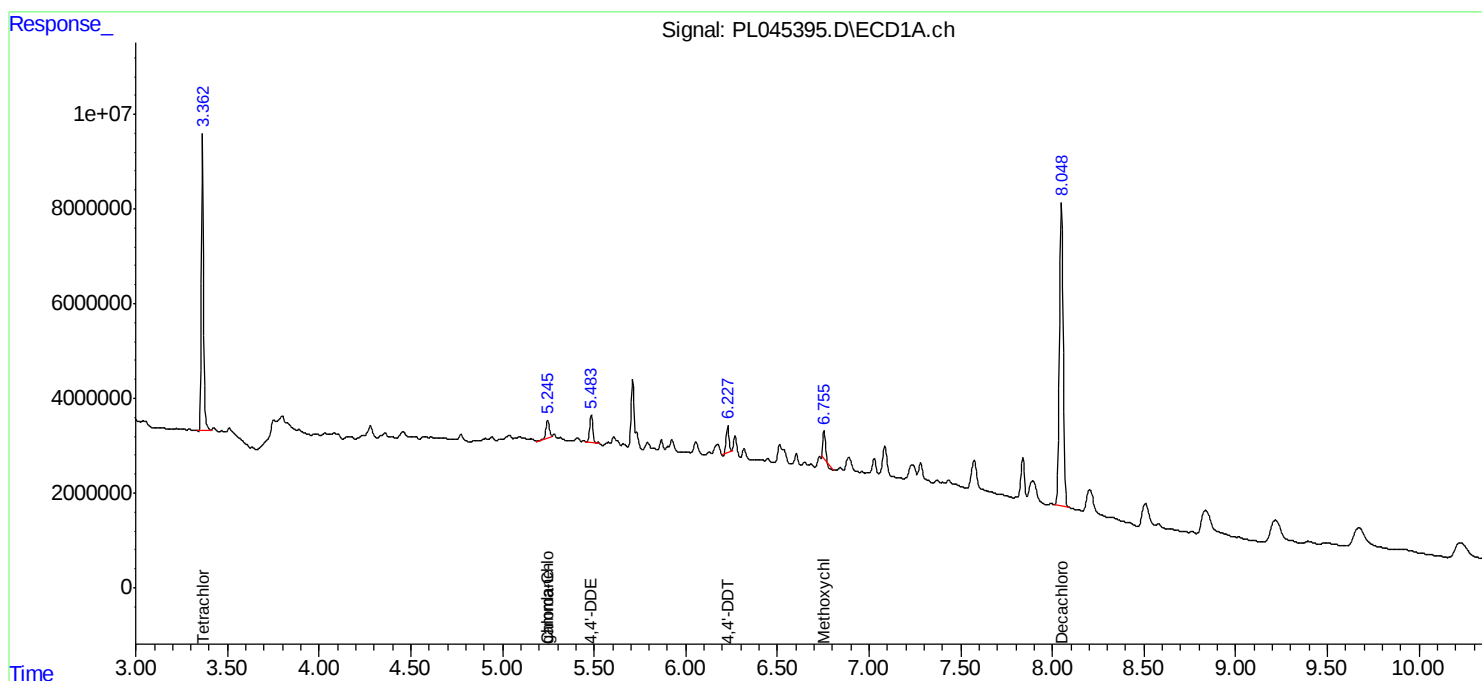


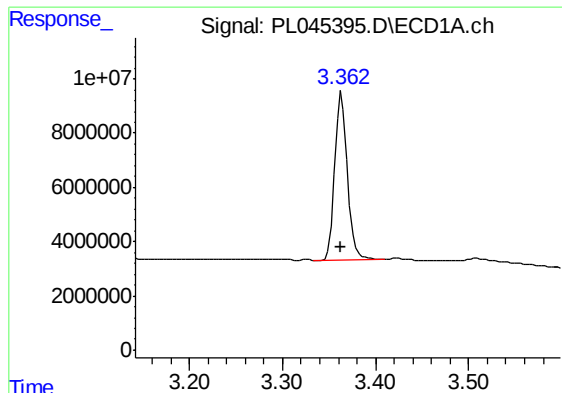

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 58892583
Conc: 8.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z-2-3

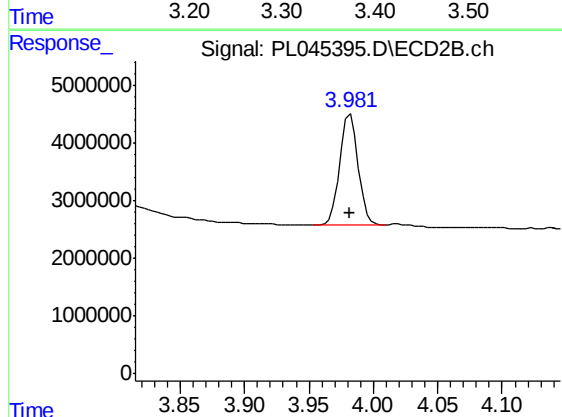


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 19360539
Conc: 9.04 ng/ml

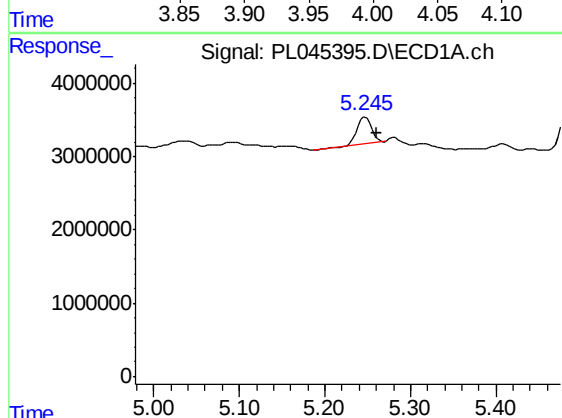


#10 gamma-Chlordane

R.T.: 5.247 min
Delta R.T.: -0.013 min
Response: 4206971
Conc: 0.43 ng/ml

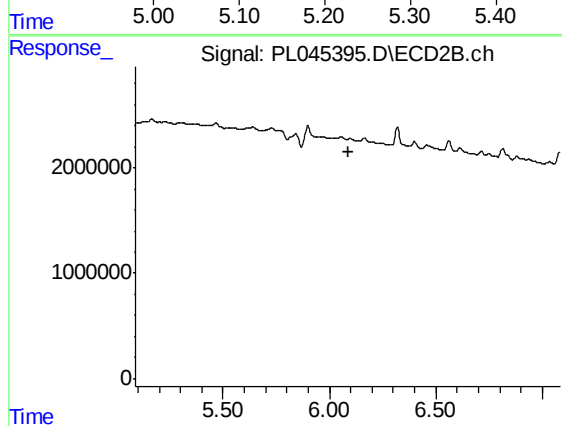

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

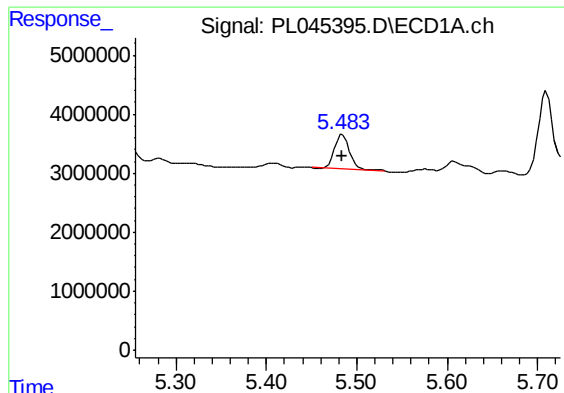

#12 4,4'-DDE


R.T.: 5.485 min
Delta R.T.: 0.000 min
Response: 6681060
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z-2-3

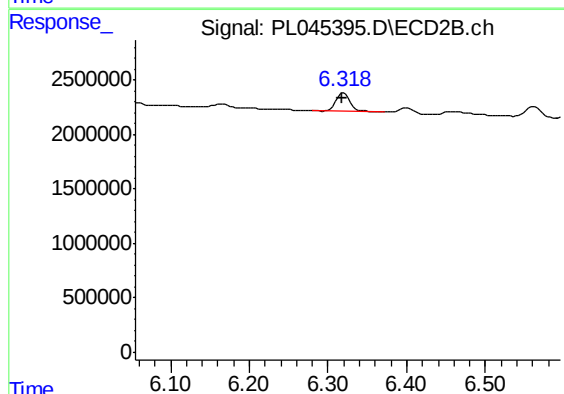


#12 4,4'-DDE

R.T.: 6.320 min
Delta R.T.: 0.002 min
Response: 2175229
Conc: 0.93 ng/ml

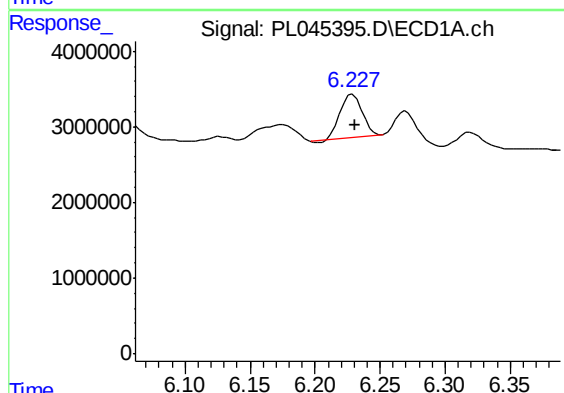


#17 4,4'-DDT

R.T.: 6.229 min
Delta R.T.: -0.002 min
Response: 6626093
Conc: 0.88 ng/ml

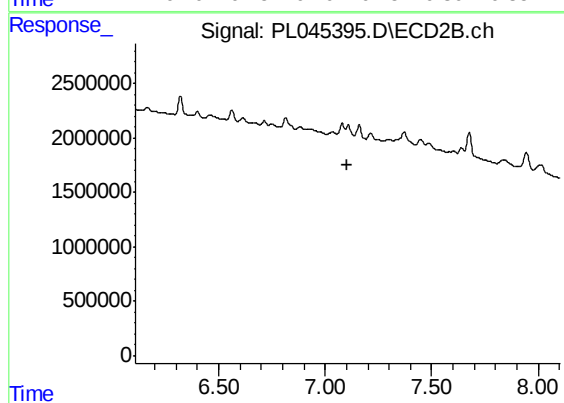

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

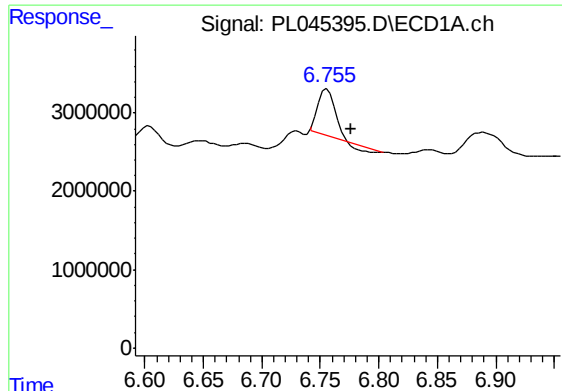

#20 Methoxychlor


R.T.: 6.756 min
Delta R.T.: -0.020 min
Response: 5344357
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z-2-3

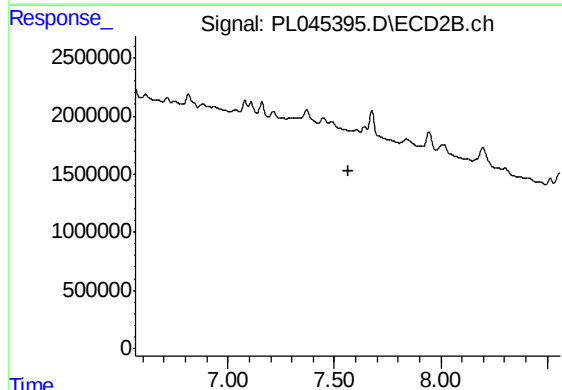


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.564 min
Response: 0
Conc: N.D.

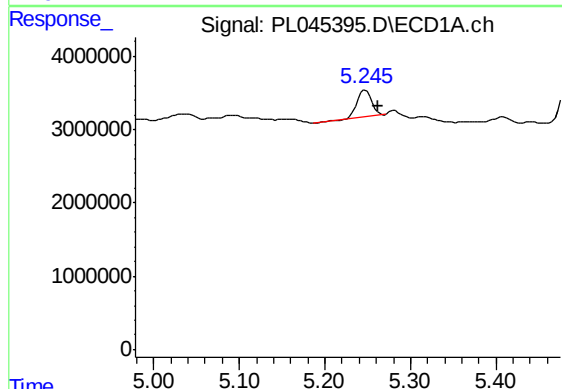


#25 Chlordane-3

R.T.: 5.247 min
Delta R.T.: -0.015 min
Response: 4206971
Conc: 3.67 ng/ml

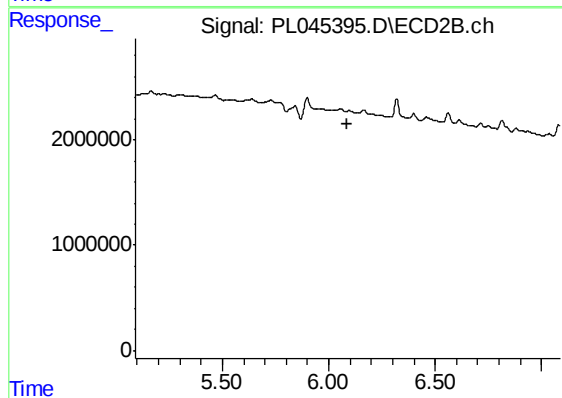

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

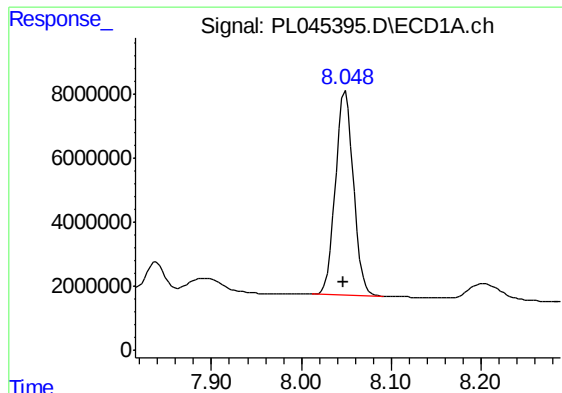

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 88548239
Conc: 10.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
Z-2-3

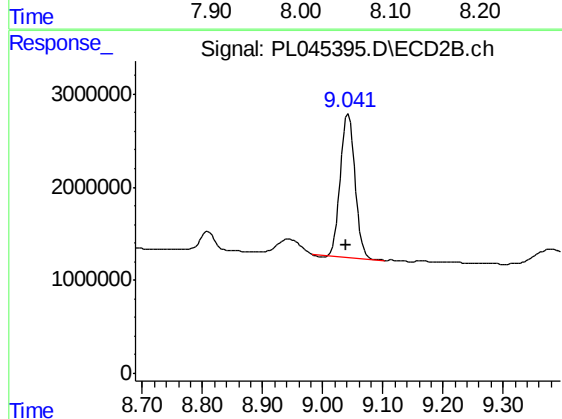

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.004 min
Response: 26114950
Conc: 11.43 ng/ml