

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030419\  
 Data File : PL045406.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 04 Mar 2019 17:34  
 Operator : AJ\SJ  
 Sample : K1714-01  
 Misc :  
 ALS Vial : 34 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 SB-A-0-2

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 04 23:56:09 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL022719.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Feb 27 17:00:03 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|---------|
| -----                       |                 |        |        |          |          |        |         |
| System Monitoring Compounds |                 |        |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.364  | 3.982  | 78678864 | 25909743 | 11.437 | 12.099  |
| 28)                         | SA Decachlor... | 8.050  | 9.043  | 108.7E6  | 32308798 | 12.995 | 14.140  |
| Target Compounds            |                 |        |        |          |          |        |         |
| 10)                         | B gamma-Chl...  | 5.247  | 0.000  | 5021481  | 0        | 0.513  | N.D. #  |
| 19)                         | B Endosulfa...  | 6.536f | 0.000  | 8476728  | 0        | 1.043  | N.D. #  |
| 20)                         | A Methoxychlor  | 0.000  | 7.585f | 0        | 3007842  | N.D.   | 2.451 # |
| 25)                         | Chlordane-3     | 5.247  | 0.000  | 5021481  | 0        | 4.378  | N.D. #  |
| -----                       |                 |        |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL030419\  
Data File : PL045406.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Mar 2019 17:34  
Operator : AJ\SJ  
Sample : K1714-01  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
SB-A-0-2

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 04 23:56:09 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL022719.M  
Quant Title : GC Extractables  
QLast Update : Wed Feb 27 17:00:03 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

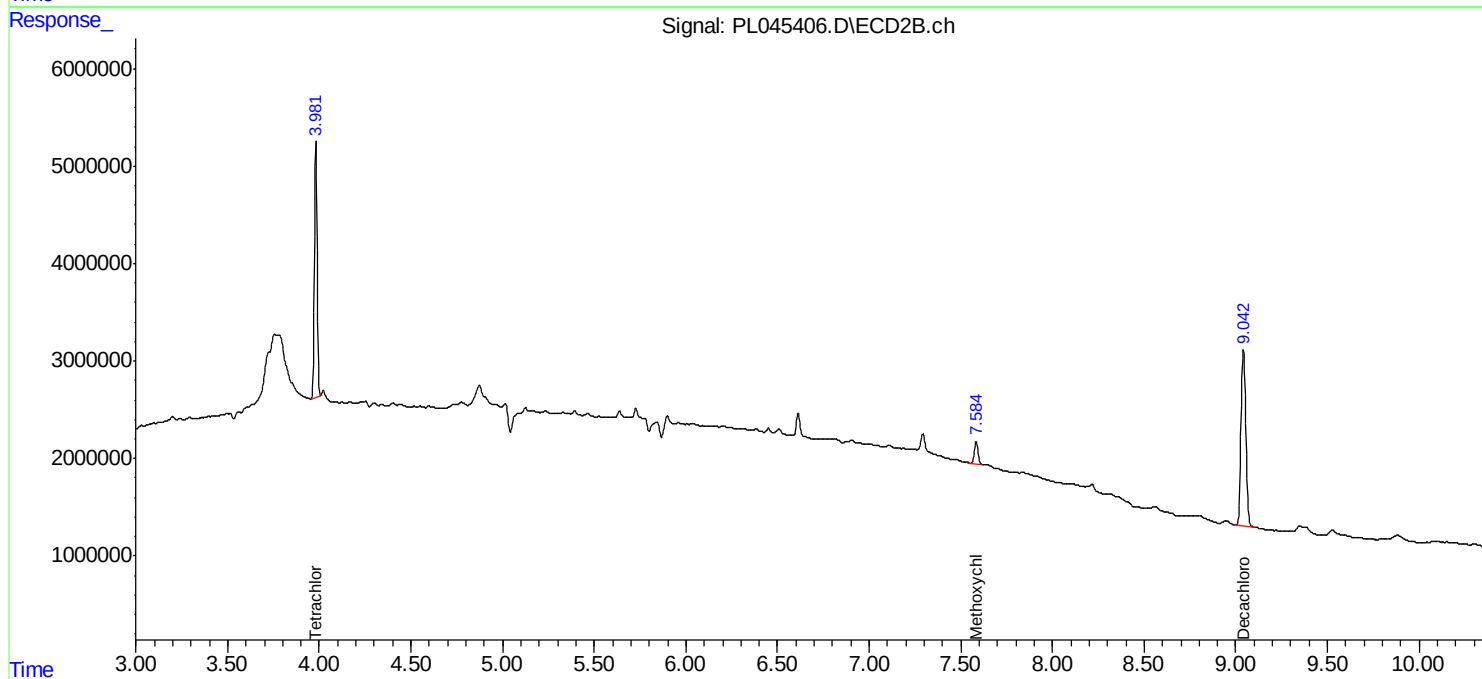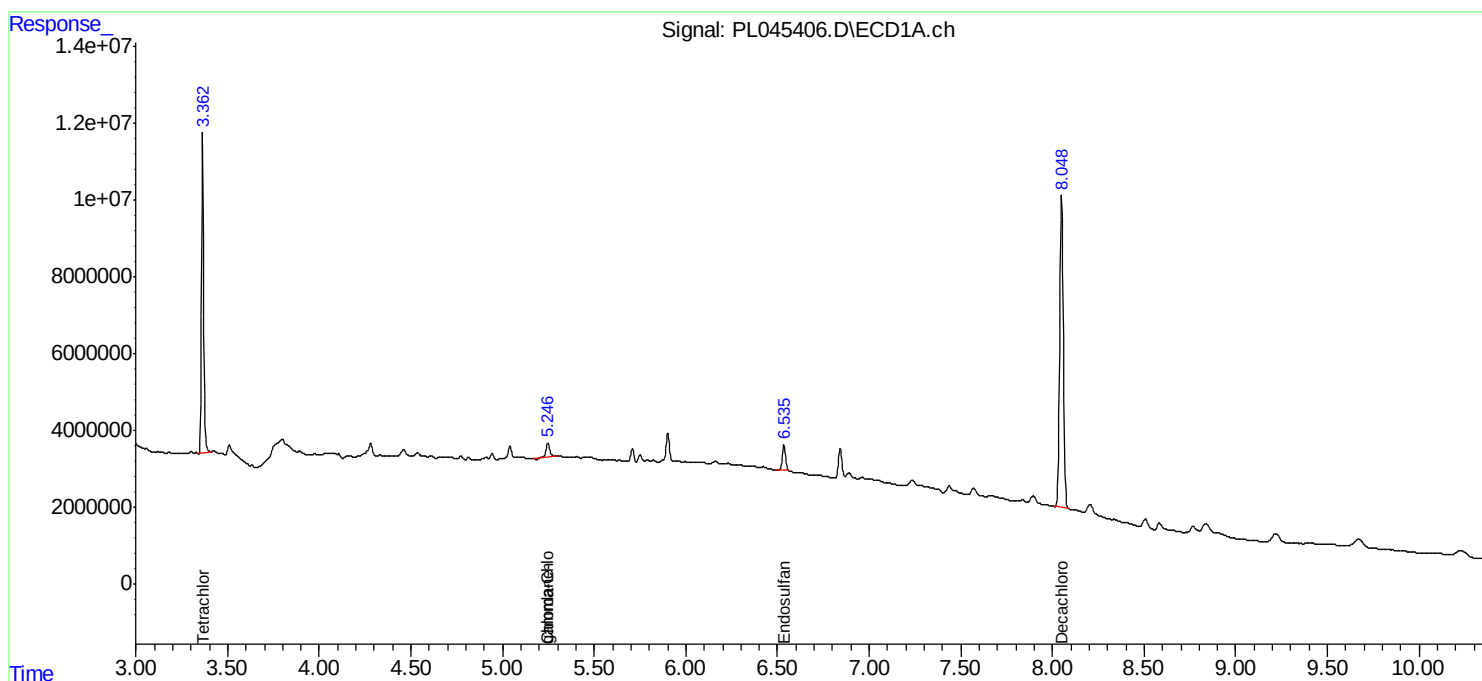


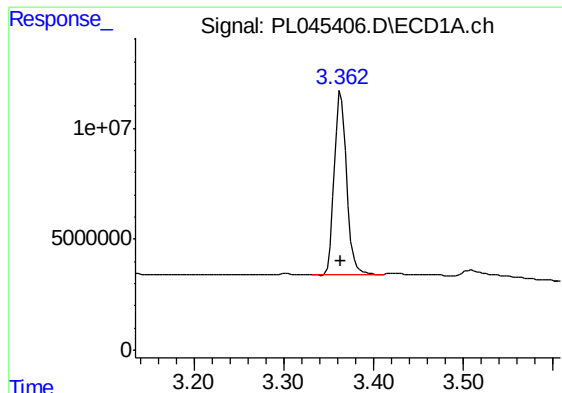

#1 Tetrachloro-m-xylene


R.T.: 3.364 min  
Delta R.T.: 0.000 min  
Response: 78678864  
Conc: 11.44 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
SB-A-0-2

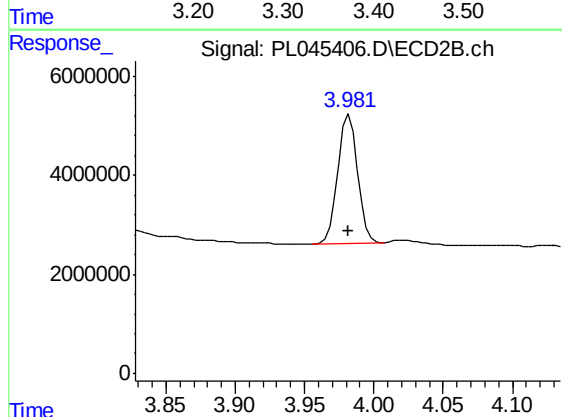


#1 Tetrachloro-m-xylene

R.T.: 3.982 min  
Delta R.T.: 0.000 min  
Response: 25909743  
Conc: 12.10 ng/ml

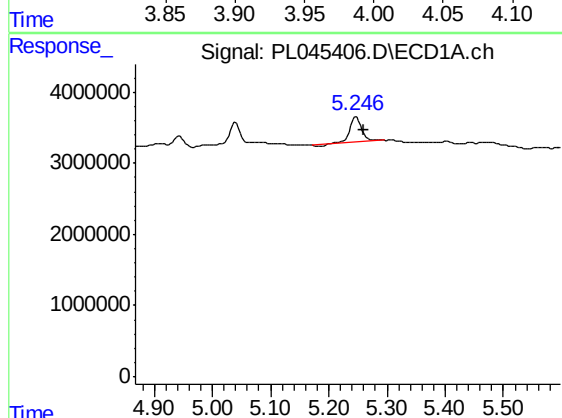


#10 gamma-Chlordane

R.T.: 5.247 min  
Delta R.T.: -0.013 min  
Response: 5021481  
Conc: 0.51 ng/ml

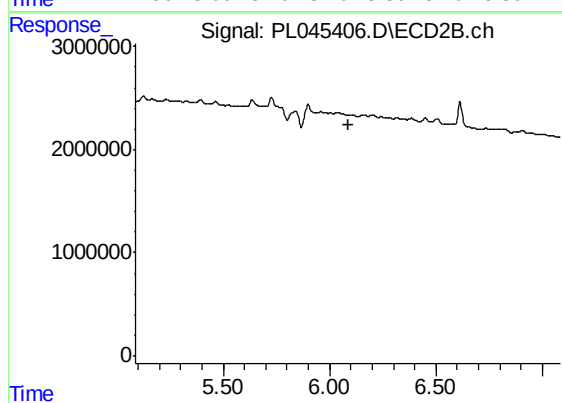

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T. : 6.088 min  
Response: 0  
Conc: N.D.

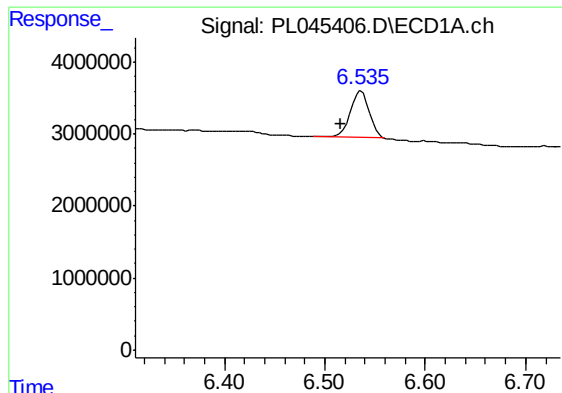

#19 Endosulfan Sulfate


R.T.: 6.536 min  
Delta R.T.: 0.021 min  
Response: 8476728  
Conc: 1.04 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
SB-A-0-2

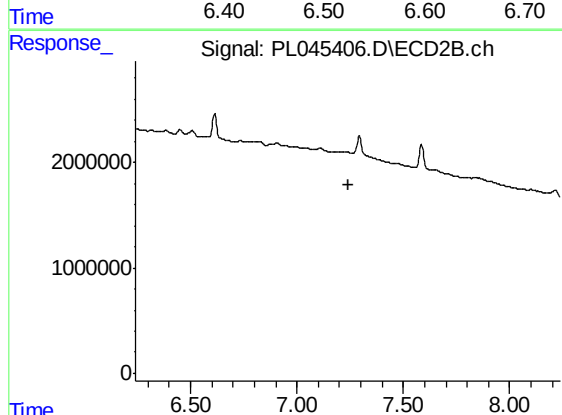


#19 Endosulfan Sulfate

R.T.: 0.000 min  
Exp R.T. : 7.241 min  
Response: 0  
Conc: N.D.

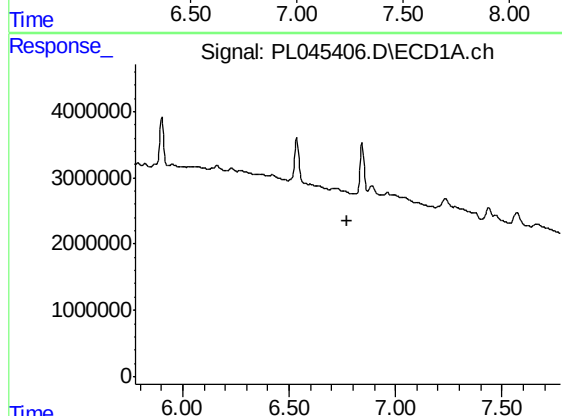


#20 Methoxychlor

R.T.: 0.000 min  
Exp R.T. : 6.776 min  
Response: 0  
Conc: N.D.

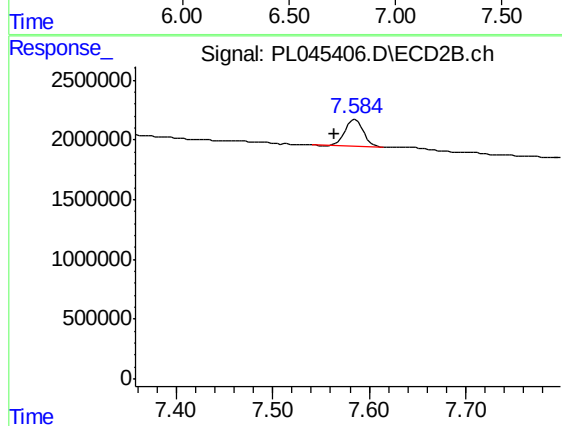

#20 Methoxychlor


R.T.: 7.585 min  
Delta R.T.: 0.021 min  
Response: 3007842  
Conc: 2.45 ng/ml

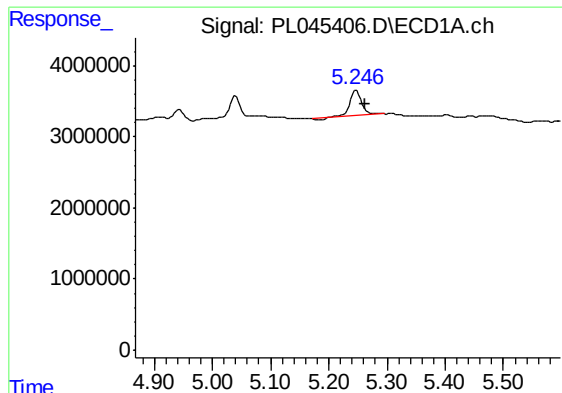

#25 Chlordane-3


R.T.: 5.247 min  
Delta R.T.: -0.014 min  
Response: 5021481  
Conc: 4.38 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
SB-A-0-2

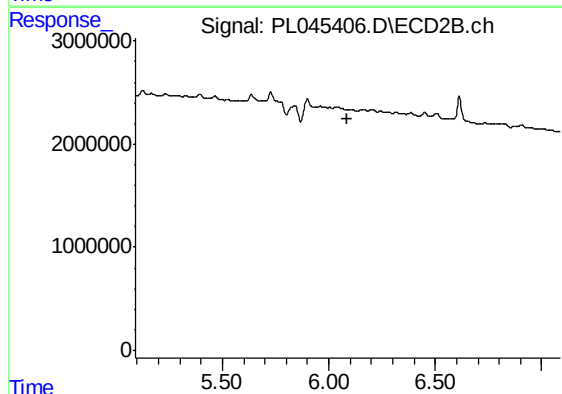


#25 Chlordane-3

R.T.: 0.000 min  
Exp R.T. : 6.089 min  
Response: 0  
Conc: N.D.

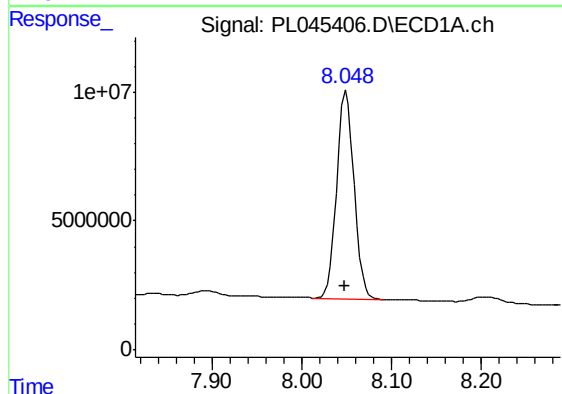

#28 Decachlorobiphenyl

R.T.: 8.050 min  
Delta R.T.: 0.002 min  
Response: 108737846  
Conc: 13.00 ng/ml

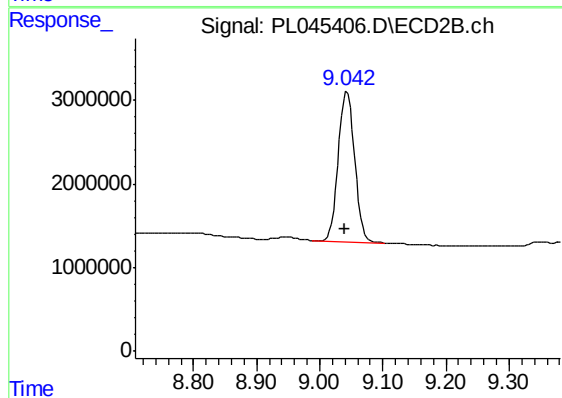

#28 Decachlorobiphenyl

R.T.: 9.043 min  
Delta R.T.: 0.004 min  
Response: 32308798  
Conc: 14.14 ng/ml