

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
 Data File : PL045411.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2019 18:45
 Operator : AJ\SJ
 Sample : K1714-06
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SB-A-14-18

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 03:10:08 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.364	3.983	131.3E6	42091415	19.080	19.655
28) SA Decachlor...	8.049	9.043	141.4E6	41937462	16.897	18.354
Target Compounds						
15) B Endosulfa...	0.000	6.909f	0	2561296	N.D.	1.089 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030419\
Data File : PL045411.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2019 18:45
Operator : AJ\SJ
Sample : K1714-06
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SB-A-14-18

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 03:10:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

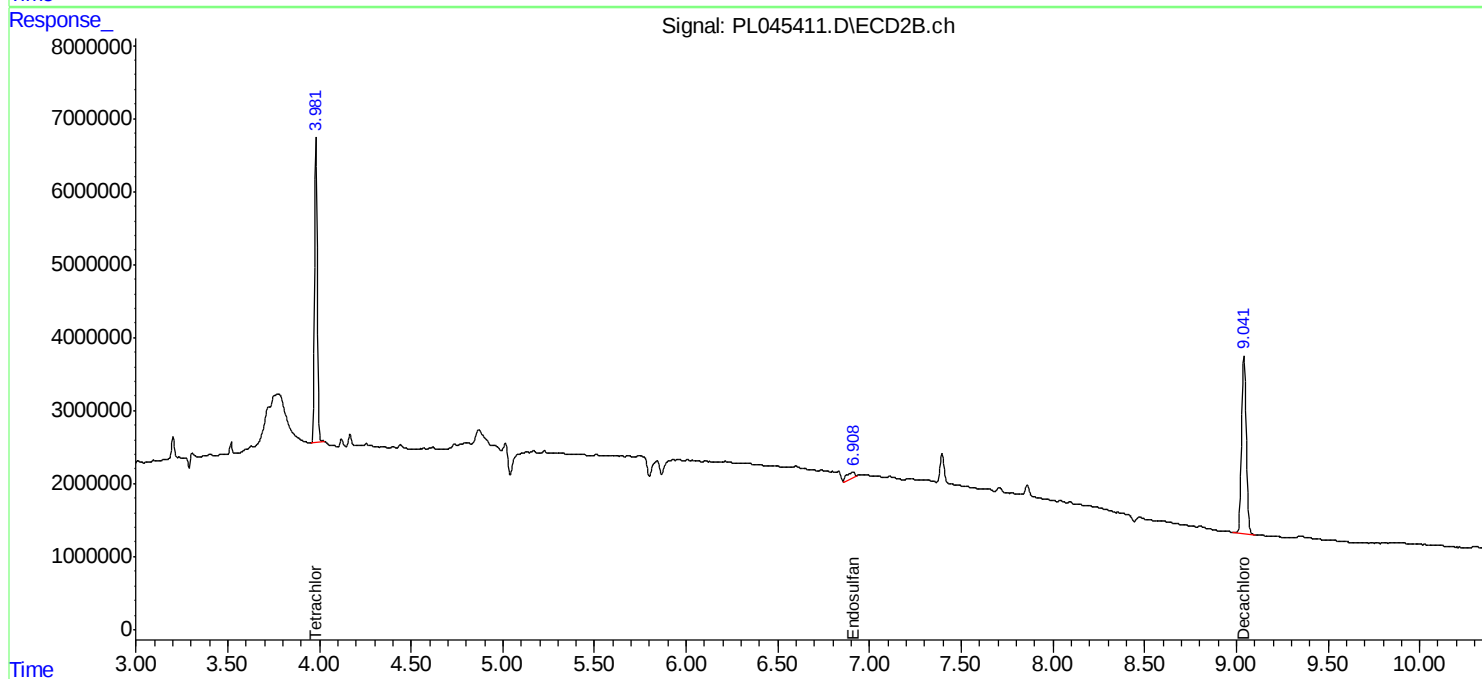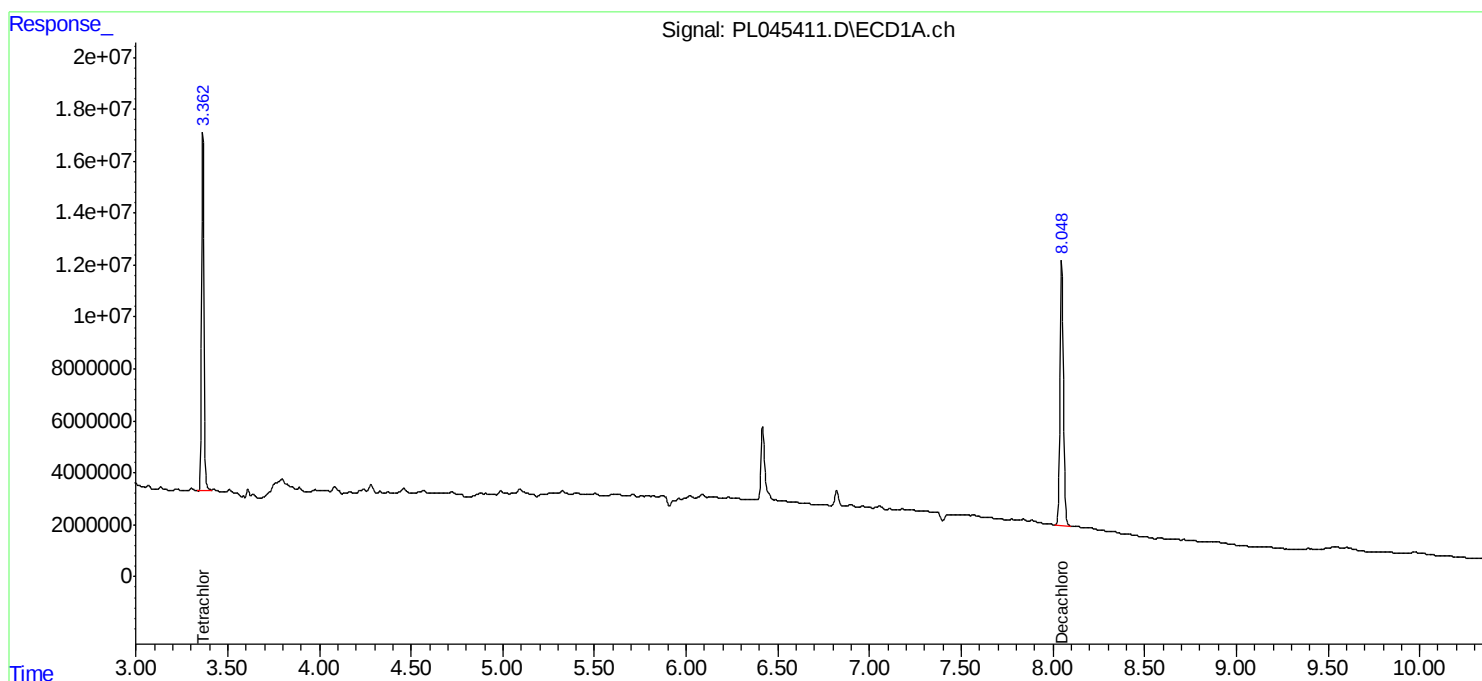


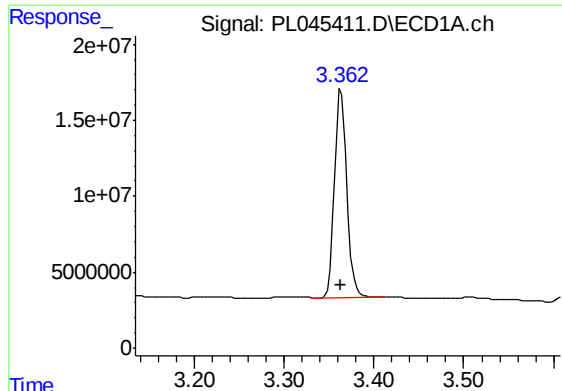

#1 Tetrachloro-m-xylene


R.T.: 3.364 min
Delta R.T.: 0.000 min
Response: 131254547
Conc: 19.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-A-14-18

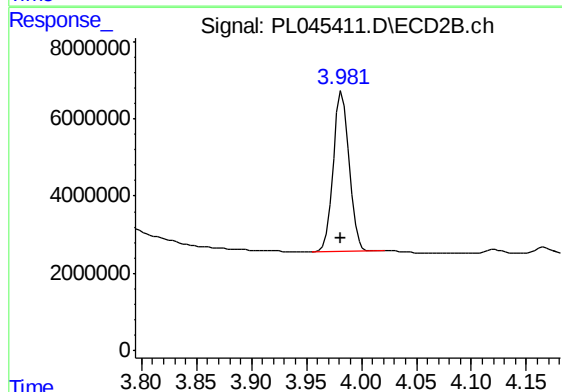


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.001 min
Response: 42091415
Conc: 19.65 ng/ml

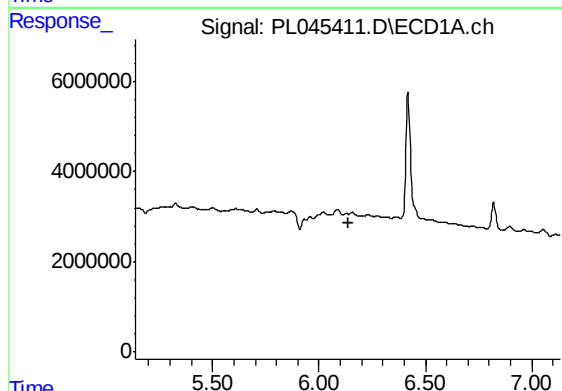


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

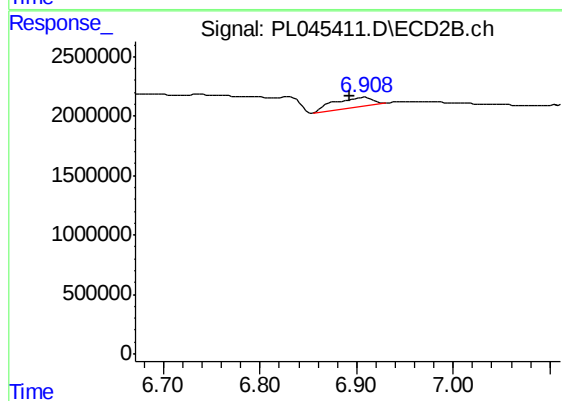

#15 Endosulfan II


R.T.: 6.909 min
Delta R.T.: 0.015 min
Response: 2561296
Conc: 1.09 ng/ml

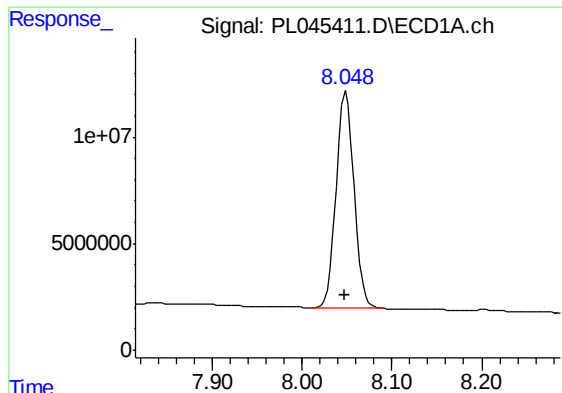

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 141381720
Conc: 16.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
SB-A-14-18

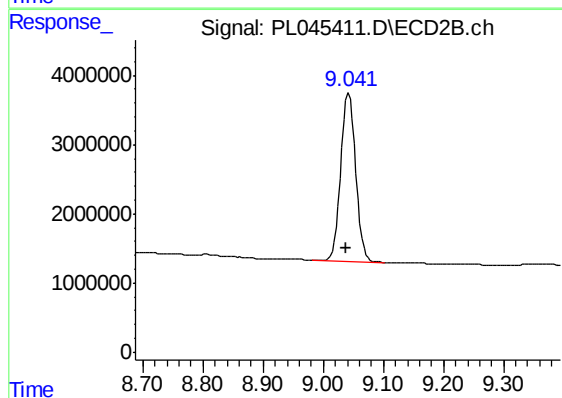

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.004 min
Response: 41937462
Conc: 18.35 ng/ml