

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
 Data File : PL057057.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 20:45
 Operator : AJ\MA
 Sample : L1775-13
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 02:51:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	182.2E6	48551100	21.380	22.756
28)	SA Decachlor...	8.211	8.983	165.4E6	39564185	17.114	18.621
Target Compounds							
6)	B beta-BHC	0.000	4.782f	0	1545290	N.D.	1.096 #
8)	B Heptachlo...	0.000	5.799f	0	13027635	N.D.	4.701 #
9)	A Endosulfan I	5.537f	0.000	4873915	0	0.430	N.D. #
15)	B Endosulfa...	6.292	6.869	7506528	6877425	0.695	2.451 #
18)	B Endrin al...	0.000	6.996f	0	1139172	N.D.	0.492 #
21)	B Endrin ke...	0.000	7.670	0	3437059	N.D.	1.254 #
23)	Chlordane-1	4.353f	0.000	4436389	0	14.596	N.D. #
27)	Chlordane-5	6.292	6.951f	7506528	3338385	20.666	40.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
Data File : PL057057.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 20:45
Operator : AJ\MA
Sample : L1775-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 02:51:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

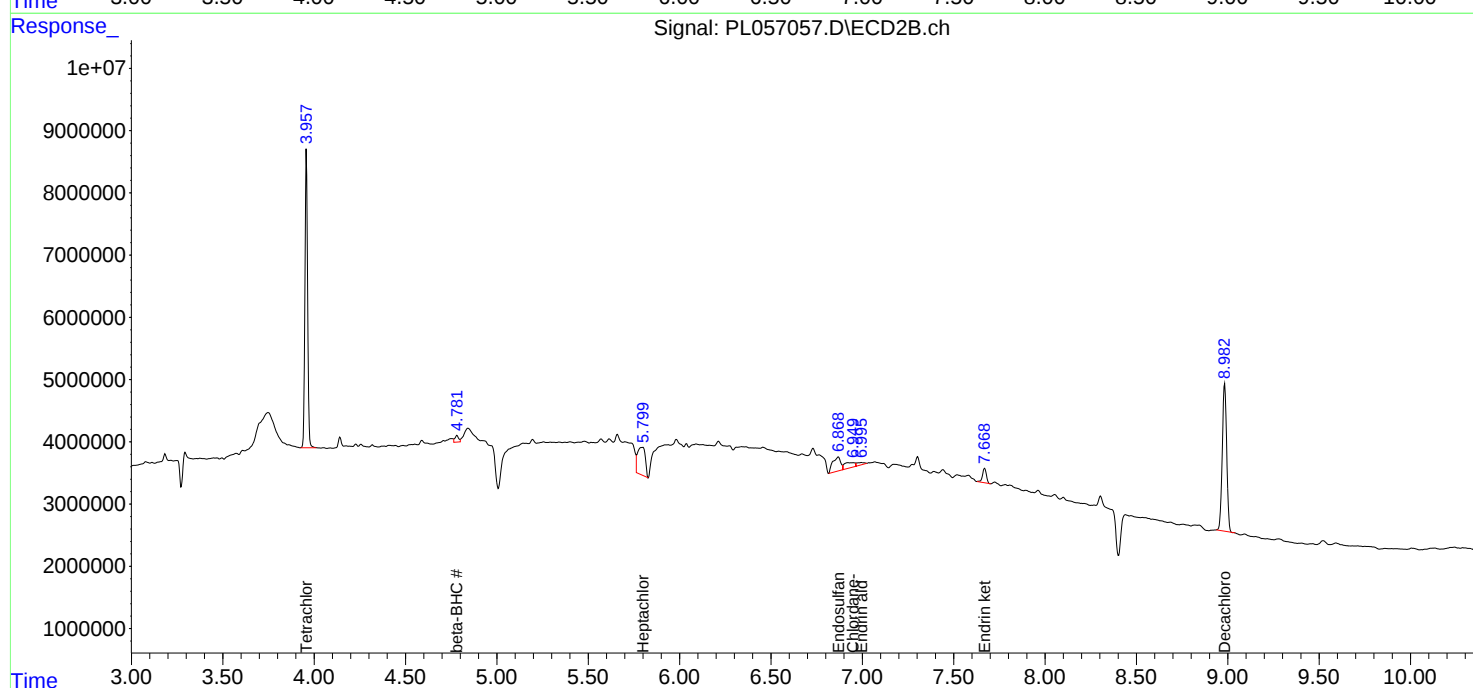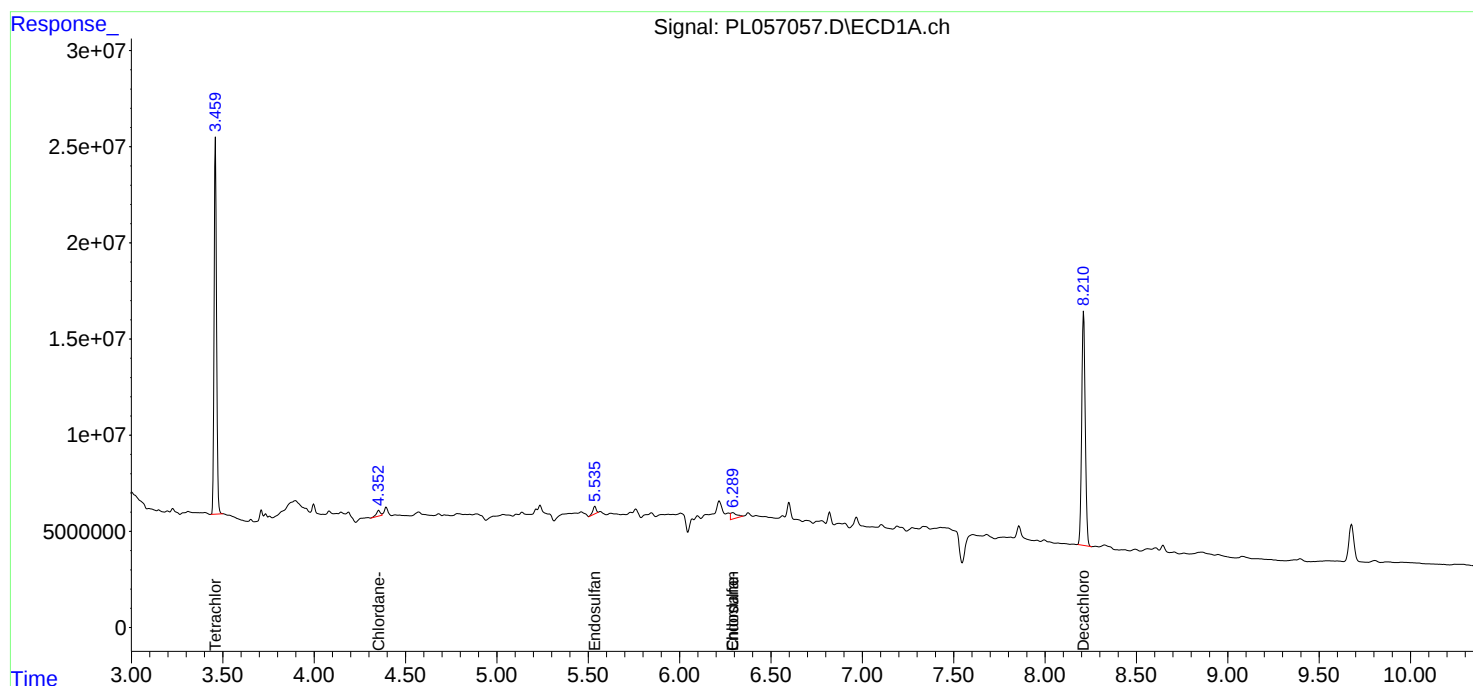


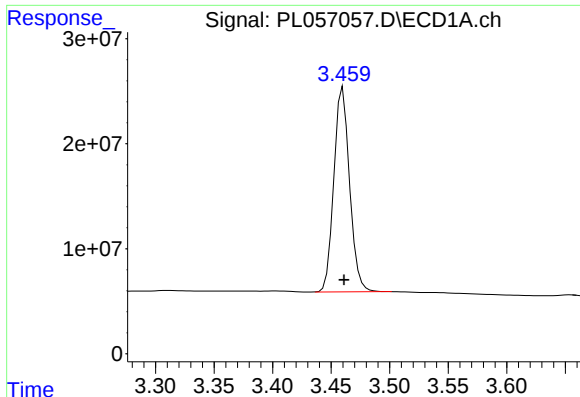

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 182206408
Conc: 21.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

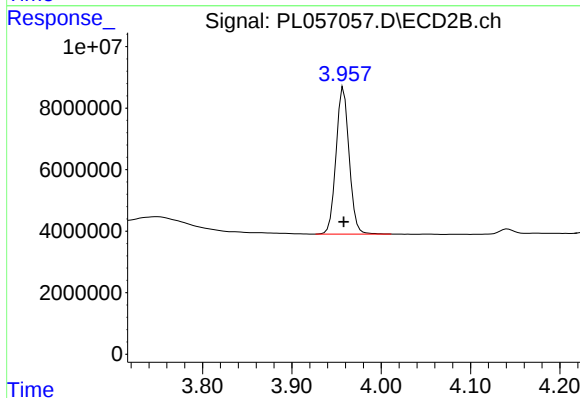


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 48551100
Conc: 22.76 ng/ml

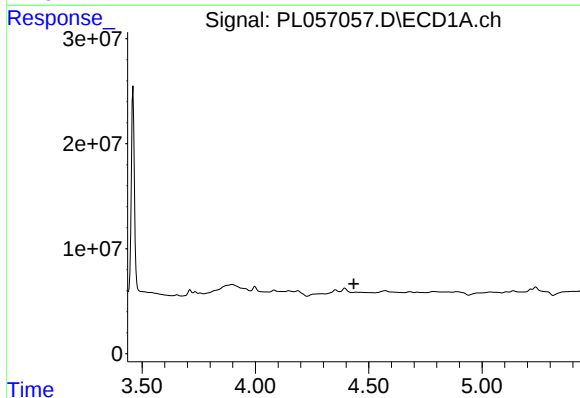


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.434 min
Response: 0
Conc: N.D.

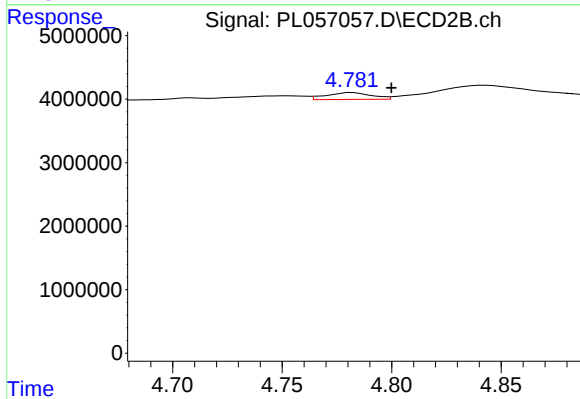

#6 beta-BHC


R.T.: 4.782 min
Delta R.T.: -0.018 min
Response: 1545290
Conc: 1.10 ng/ml

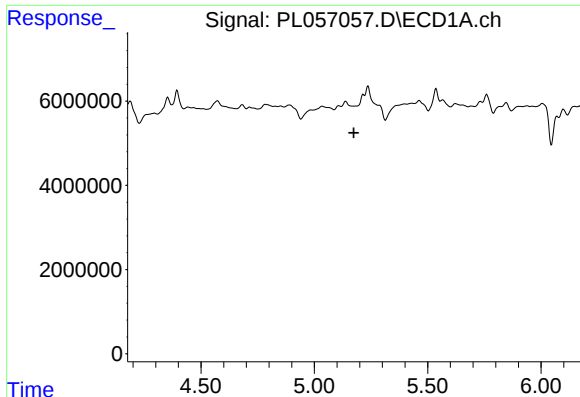

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

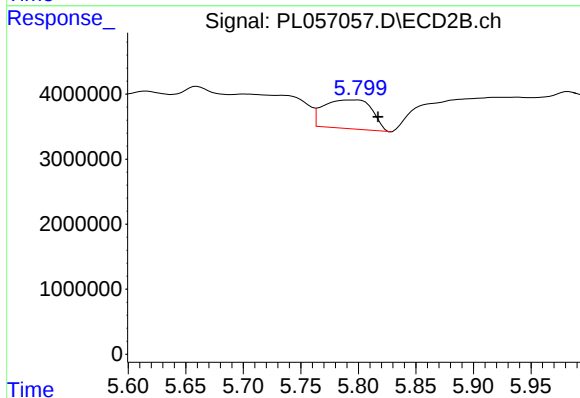


#8 Heptachlor epoxide

R.T.: 5.799 min
Delta R.T.: -0.018 min
Response: 13027635
Conc: 4.70 ng/ml

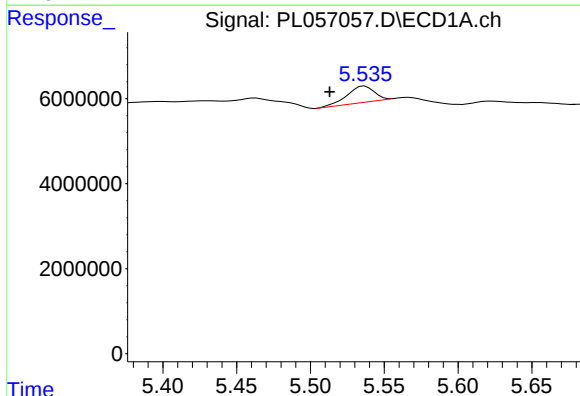


#9 Endosulfan I

R.T.: 5.537 min
Delta R.T.: 0.024 min
Response: 4873915
Conc: 0.43 ng/ml

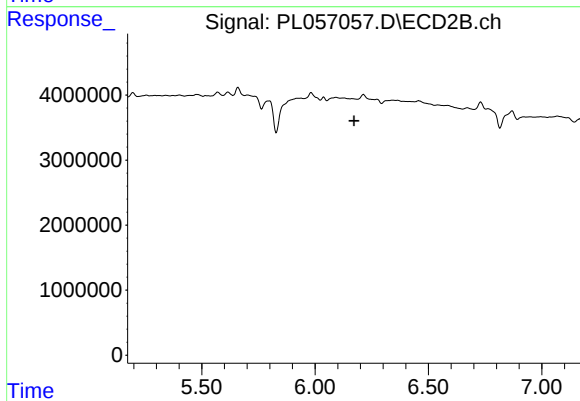

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.172 min
Response: 0
Conc: N.D.

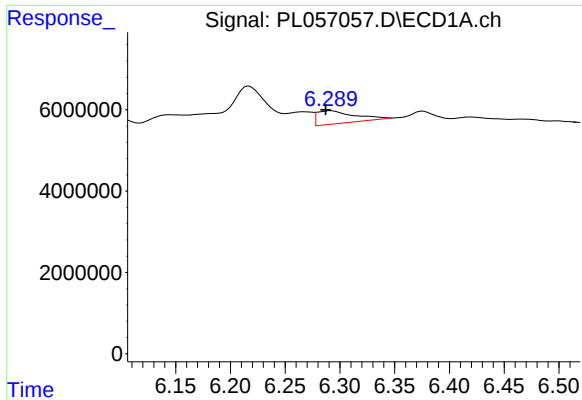

#15 Endosulfan II


R.T.: 6.292 min
Delta R.T.: 0.005 min
Response: 7506528
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

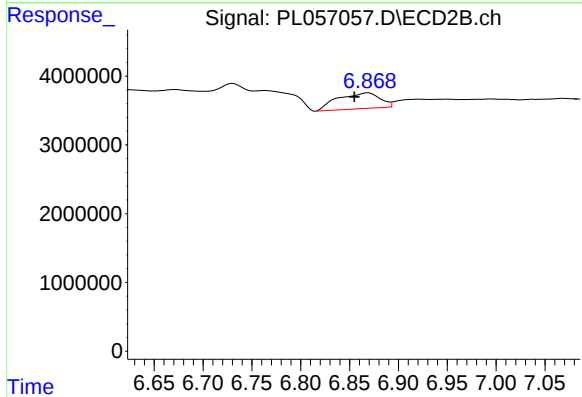


#15 Endosulfan II

R.T.: 6.869 min
Delta R.T.: 0.014 min
Response: 6877425
Conc: 2.45 ng/ml

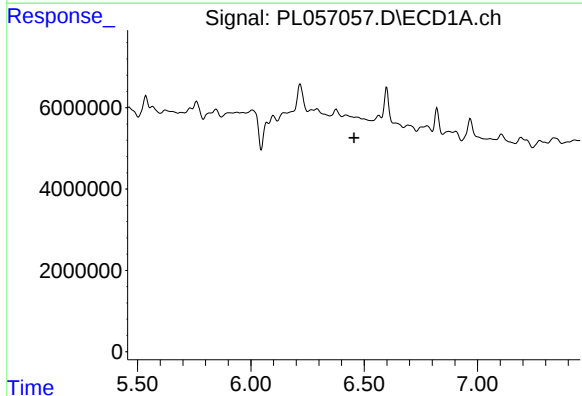


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

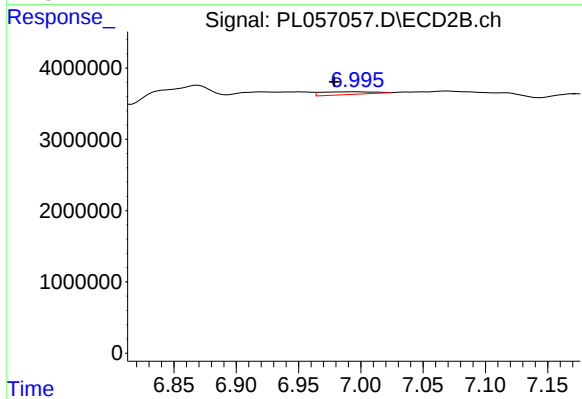

#18 Endrin aldehyde


R.T.: 6.996 min
Delta R.T.: 0.017 min
Response: 1139172
Conc: 0.49 ng/ml

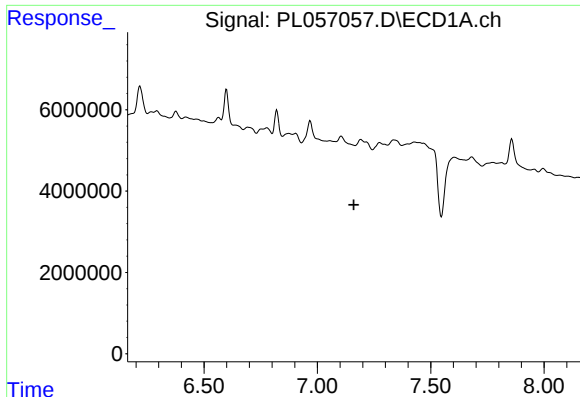

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T.: 7.160 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

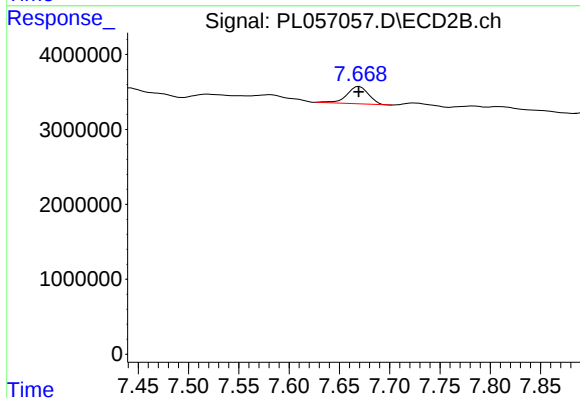


#21 Endrin ketone

R.T.: 7.670 min
Delta R.T.: 0.000 min
Response: 3437059
Conc: 1.25 ng/ml

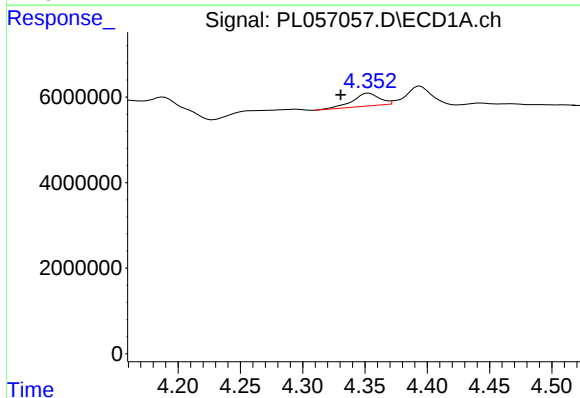


#23 Chlordane-1

R.T.: 4.353 min
Delta R.T.: 0.023 min
Response: 4436389
Conc: 14.60 ng/ml

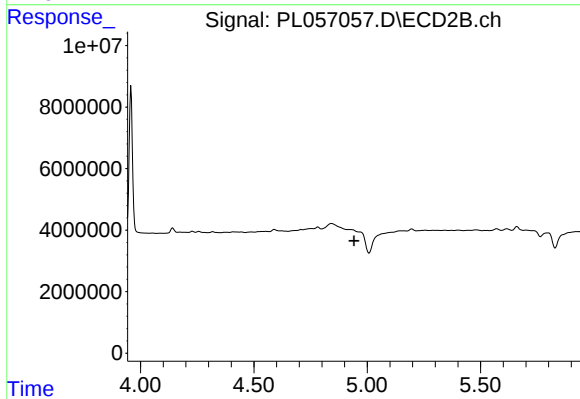

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

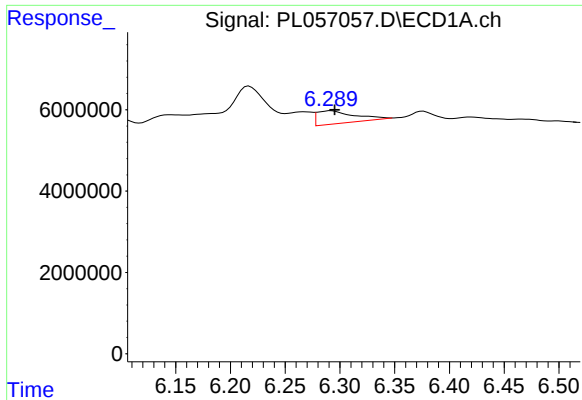

#27 Chlordane-5


R.T.: 6.292 min
Delta R.T.: -0.003 min
Response: 7506528
Conc: 20.67 ng/ml

Instrument :
ECD_L
ClientSampleId :

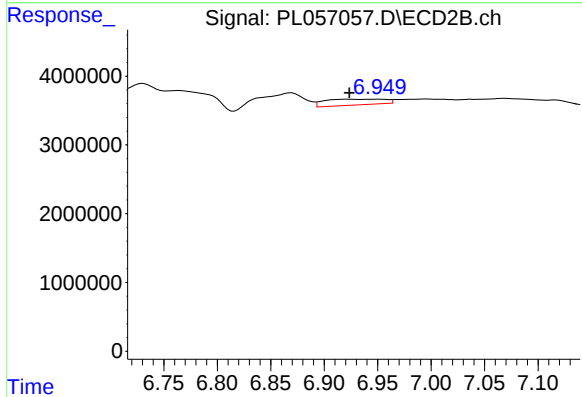


#27 Chlordane-5

R.T.: 6.951 min
Delta R.T.: 0.028 min
Response: 3338385
Conc: 40.01 ng/ml

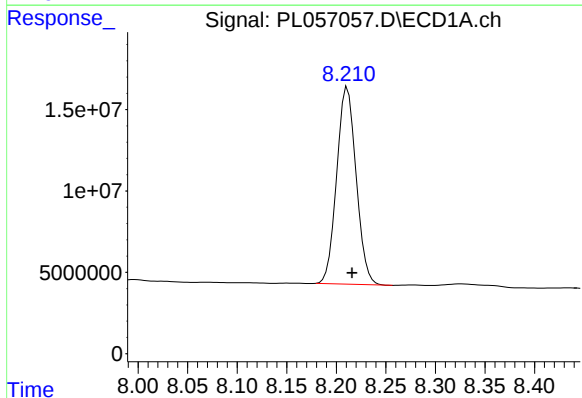

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.005 min
Response: 165411757
Conc: 17.11 ng/ml

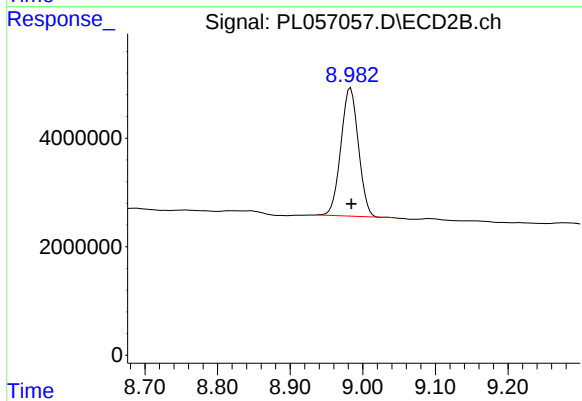

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: -0.001 min
Response: 39564185
Conc: 18.62 ng/ml