

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
 Data File : PL057058.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 20:59
 Operator : AJ\MA
 Sample : L1677-01
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 02:51:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	36661983	10024062	4.302	4.698
28)	SA Decachlor...	8.211	8.984	49304808	10650004	5.101	5.012
Target Compounds							
8)	B Heptachlo...	0.000	5.792f	0	8703885	N.D.	3.141 #
9)	A Endosulfan I	5.520	0.000	23909415	0	2.109	N.D. #
10)	B gamma-Chl...	0.000	6.042	0	3210913	N.D.	1.073 #
13)	MA Dieldrin	5.732f	0.000	21054262	0	1.722	N.D. #
15)	B Endosulfa...	0.000	6.871f	0	4840052	N.D.	1.725 #
16)	A 4,4'-DDD	6.146	0.000	20888980	0	2.158	N.D. #
18)	B Endrin al...	0.000	6.976	0	20284951	N.D.	8.754 #
23)	Chlordane-1	4.342	0.000	5162508	0	16.985	N.D. #
25)	Chlordane-3	0.000	6.042	0	3210913	N.D.	8.472 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
Data File : PL057058.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 20:59
Operator : AJ\MA
Sample : L1677-01
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 02:51:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

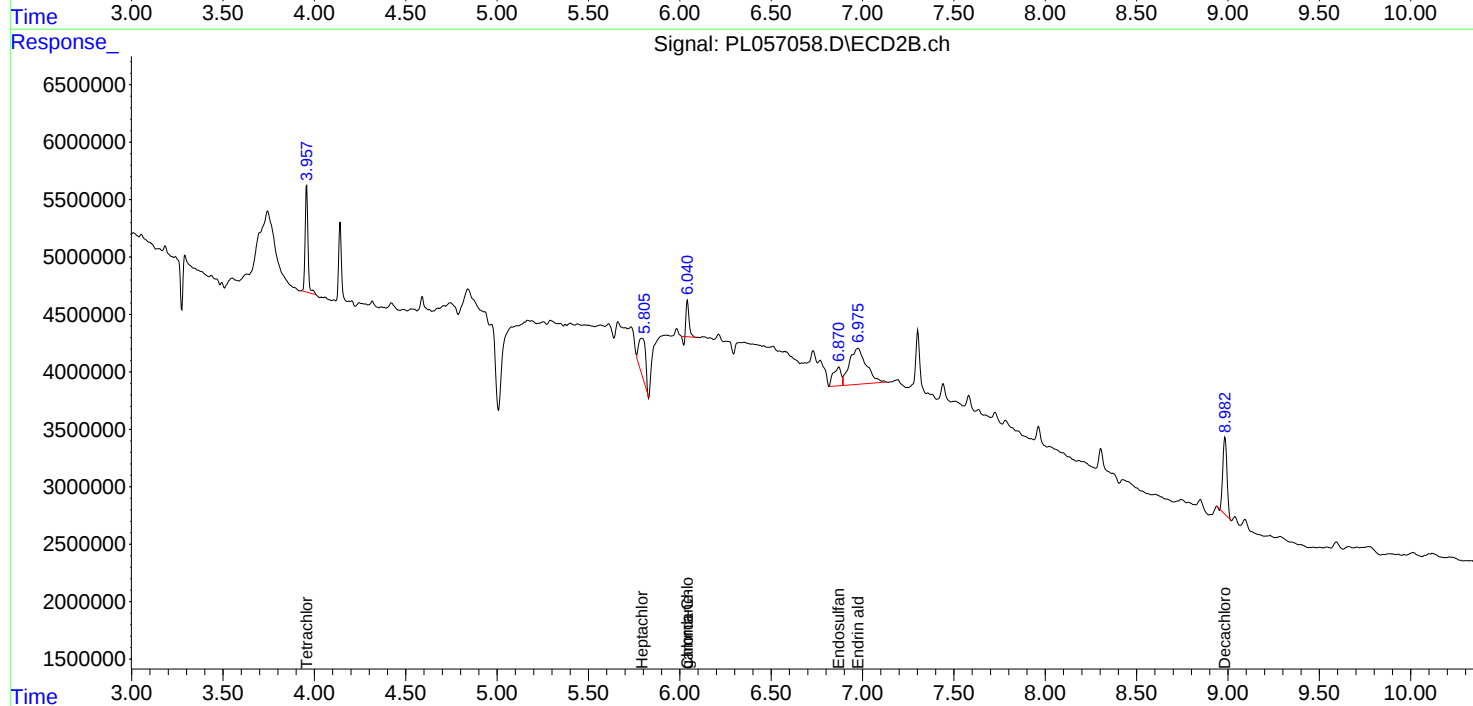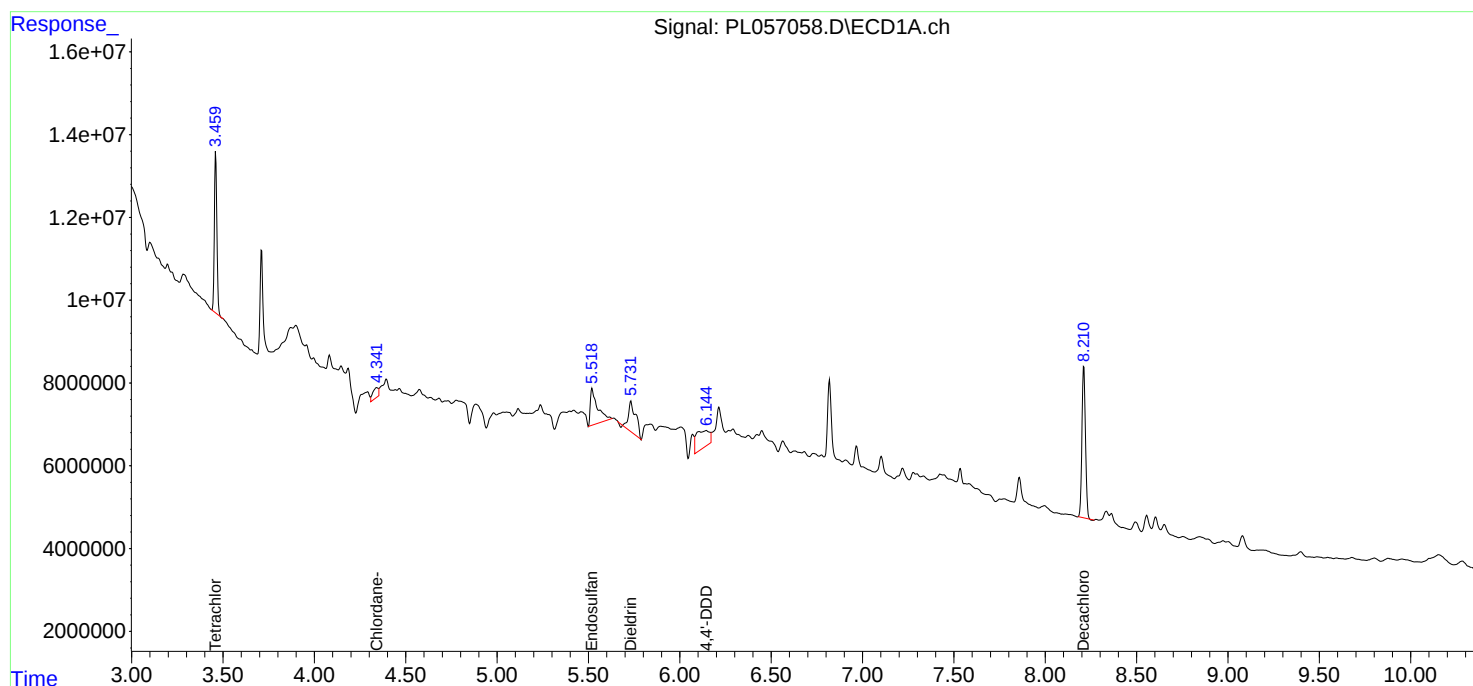


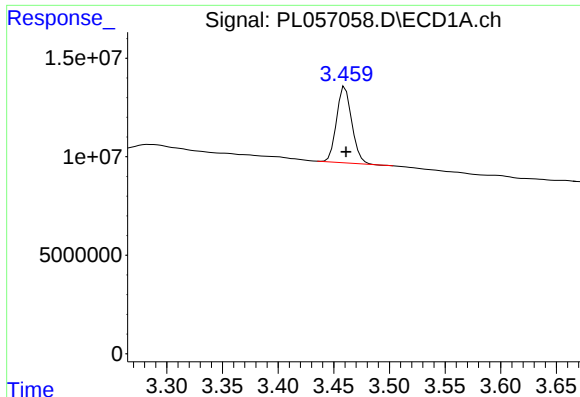

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 36661983
Conc: 4.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

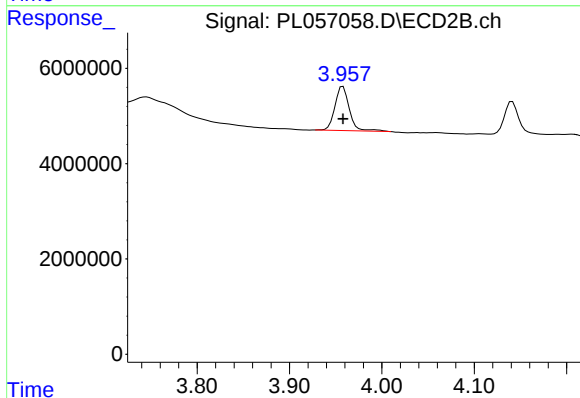


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 10024062
Conc: 4.70 ng/ml

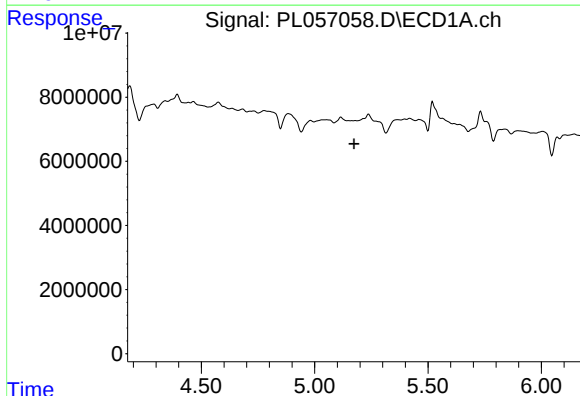


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

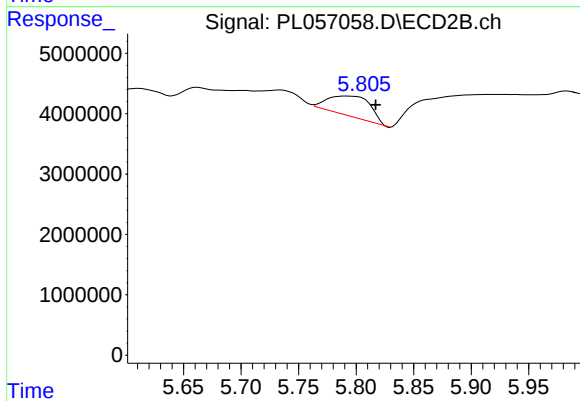

#8 Heptachlor epoxide


R.T.: 5.792 min
Delta R.T.: -0.026 min
Response: 8703885
Conc: 3.14 ng/ml

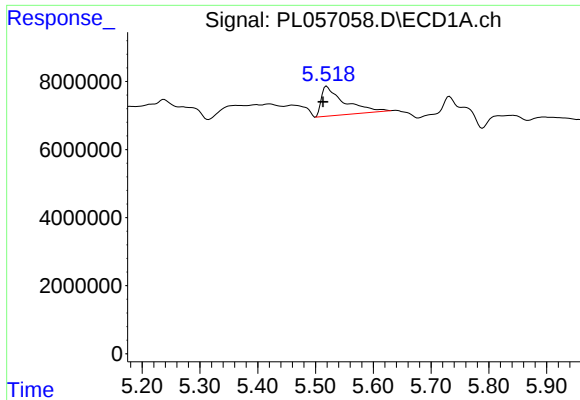

#9 Endosulfan I


R.T.: 5.520 min
Delta R.T.: 0.007 min
Response: 23909415
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

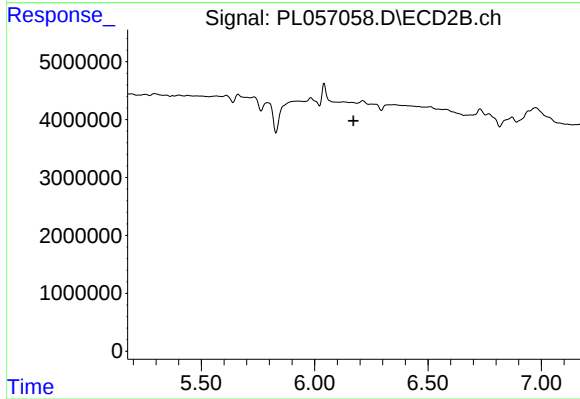


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.172 min
Response: 0
Conc: N.D.

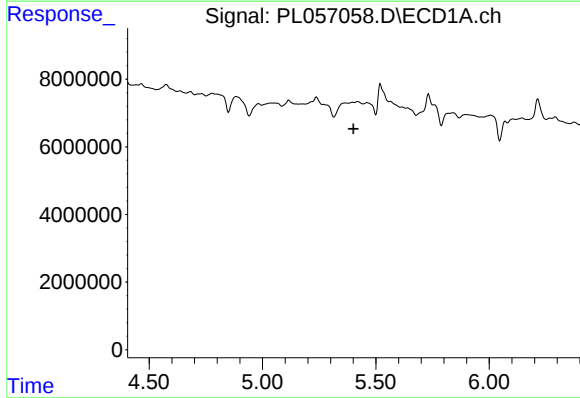


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

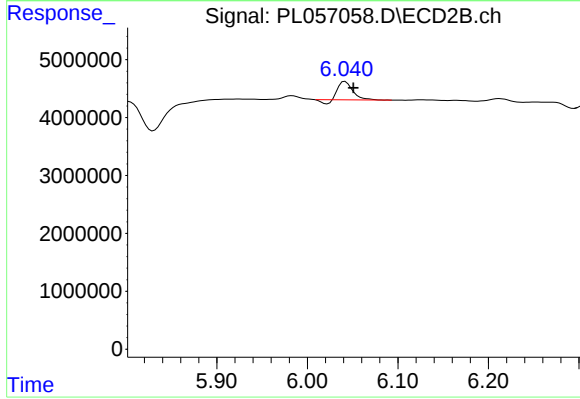

#10 gamma-Chlordane


R.T.: 6.042 min
Delta R.T.: -0.009 min
Response: 3210913
Conc: 1.07 ng/ml

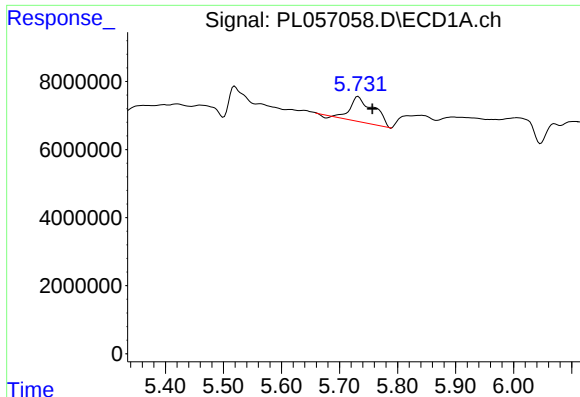

#13 Dieldrin


R.T.: 5.732 min
Delta R.T.: -0.025 min
Response: 21054262
Conc: 1.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

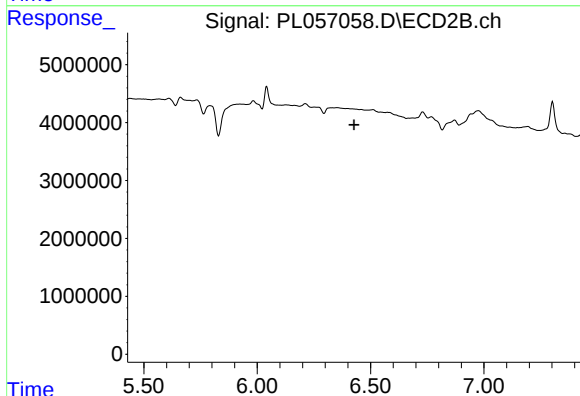


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

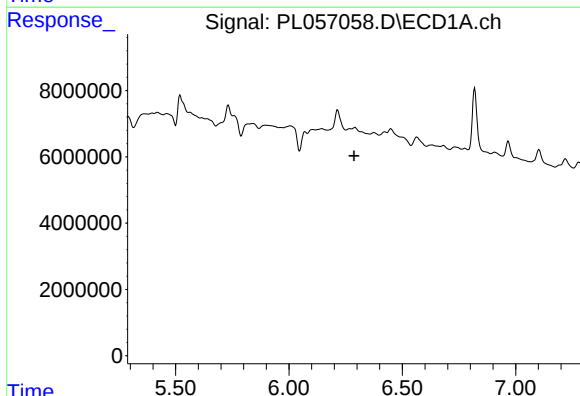


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

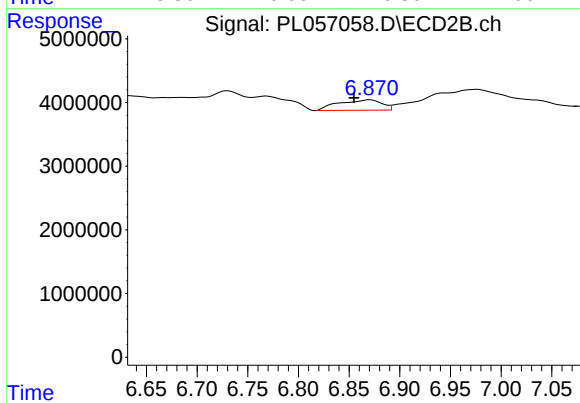

#15 Endosulfan II


R.T.: 6.871 min
Delta R.T.: 0.016 min
Response: 4840052
Conc: 1.72 ng/ml

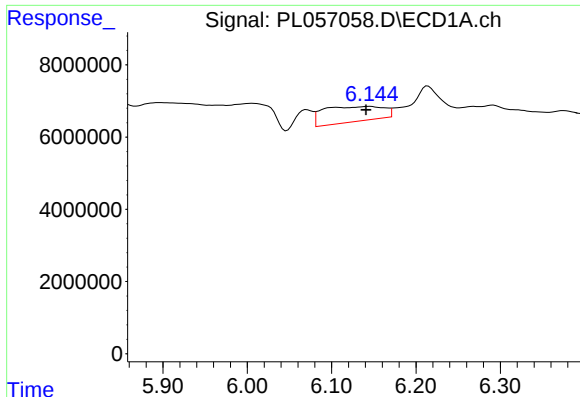

#16 4,4'-DDD


R.T.: 6.146 min
Delta R.T.: 0.005 min
Response: 20888980
Conc: 2.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

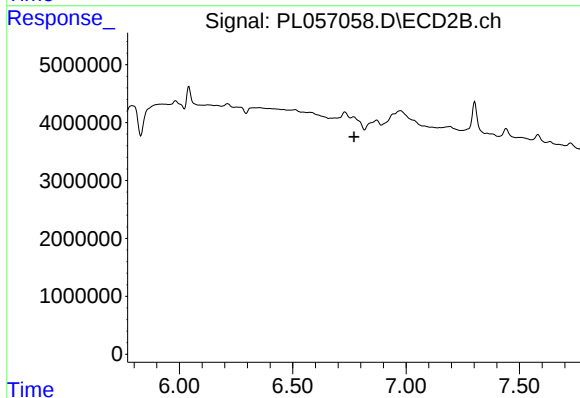


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

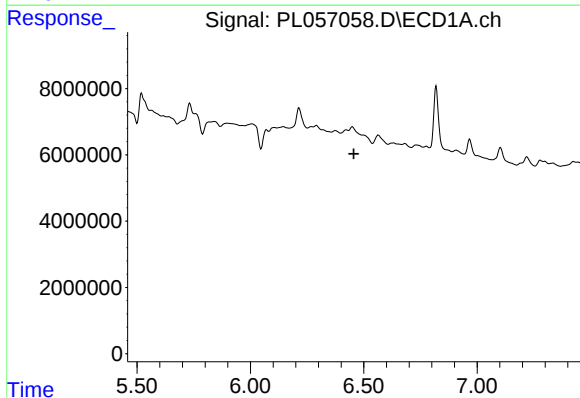


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 6.456 min
Response: 0
Conc: N.D.

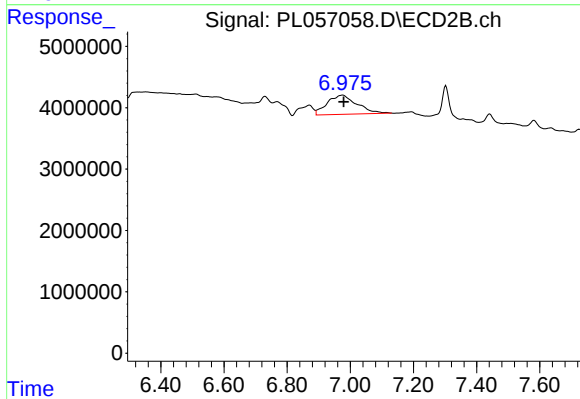

#18 Endrin aldehyde


R.T.: 6.976 min
Delta R.T.: -0.003 min
Response: 20284951
Conc: 8.75 ng/ml

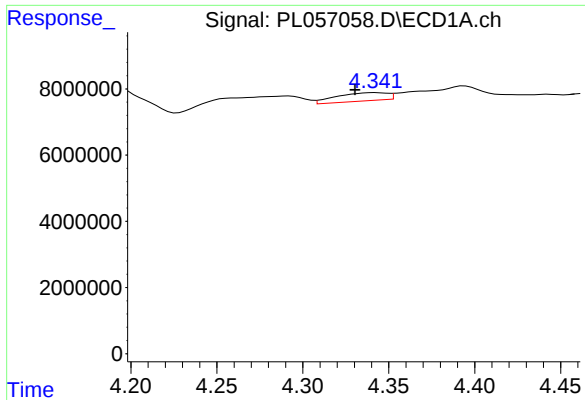

#23 Chlordane-1


R.T.: 4.342 min
Delta R.T.: 0.012 min
Response: 5162508
Conc: 16.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

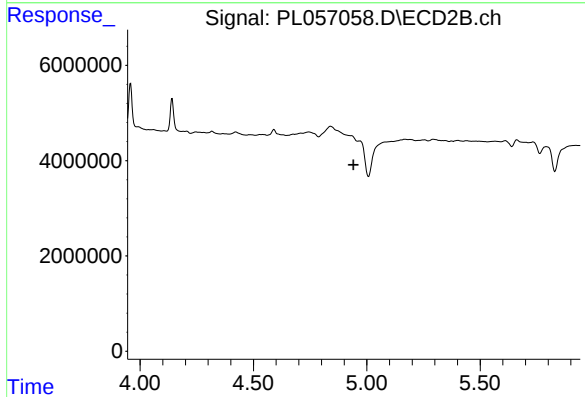


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

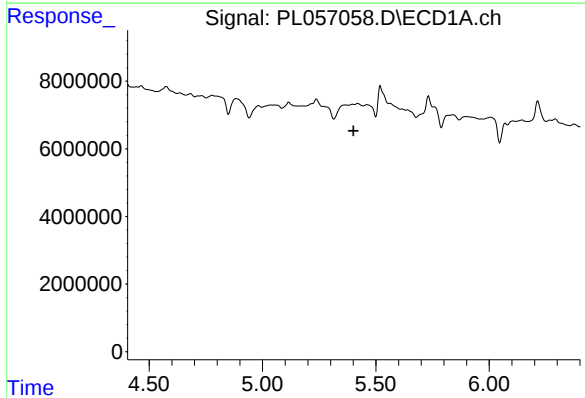


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.402 min
Response: 0
Conc: N.D.

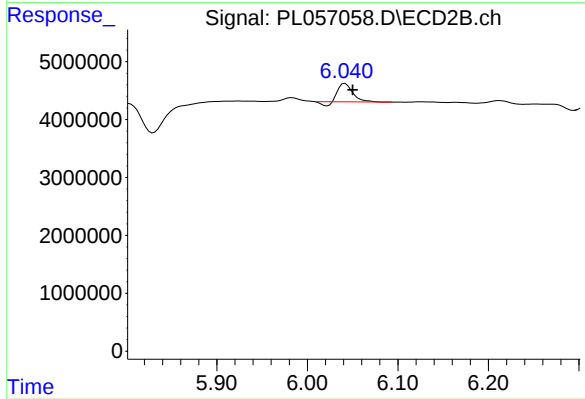

#25 Chlordane-3


R.T.: 6.042 min
Delta R.T.: -0.008 min
Response: 3210913
Conc: 8.47 ng/ml

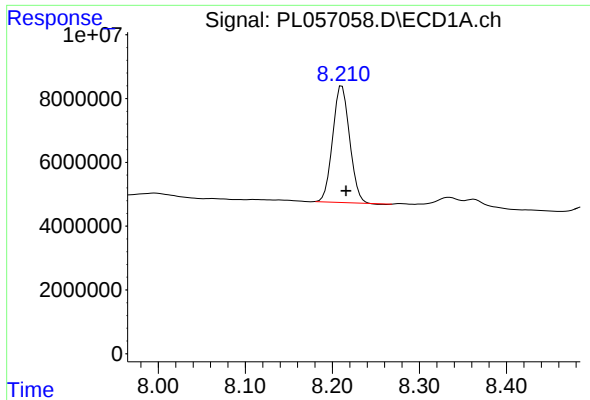

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.005 min
Response: 49304808
Conc: 5.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

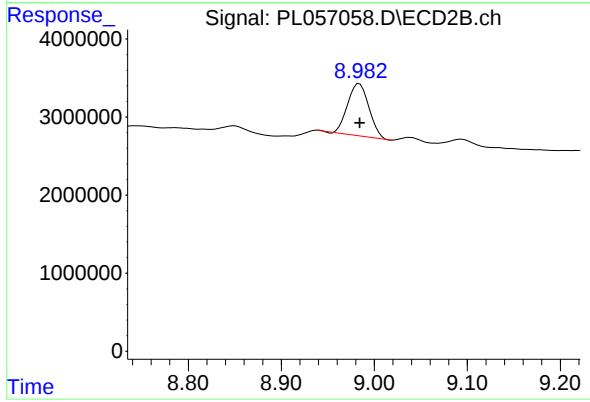

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 10650004
Conc: 5.01 ng/ml