

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
 Data File : PL057062.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 21:56
 Operator : AJ\MA
 Sample : PB127262TB
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 02:52:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	194.8E6	49872127	22.861	23.376
28)	SA Decachlor...	8.212	8.984	197.4E6	47191905	20.422	22.211
Target Compounds							
4)	MA Heptachlor	0.000	5.156f	0	43627598	N.D.	14.017 #
5)	MB Aldrin	0.000	5.447	0	2016938	N.D.	0.675 #
6)	B beta-BHC	4.443	0.000	4839450	0	0.914	N.D. #
8)	B Heptachlo...	0.000	5.800f	0	20437015	N.D.	7.375 #
15)	B Endosulfa...	6.296	6.872f	10325983	4963674	0.956	1.769 #
23)	Chlordane-1	4.346f	0.000	88074394	0	289.766	N.D. #
24)	Chlordane-2	0.000	5.396	0	8363823	N.D.	87.621 #
27)	Chlordane-5	6.296	0.000	10325983	0	28.429	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
Data File : PL057062.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 21:56
Operator : AJ\MA
Sample : PB127262TB
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 02:52:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

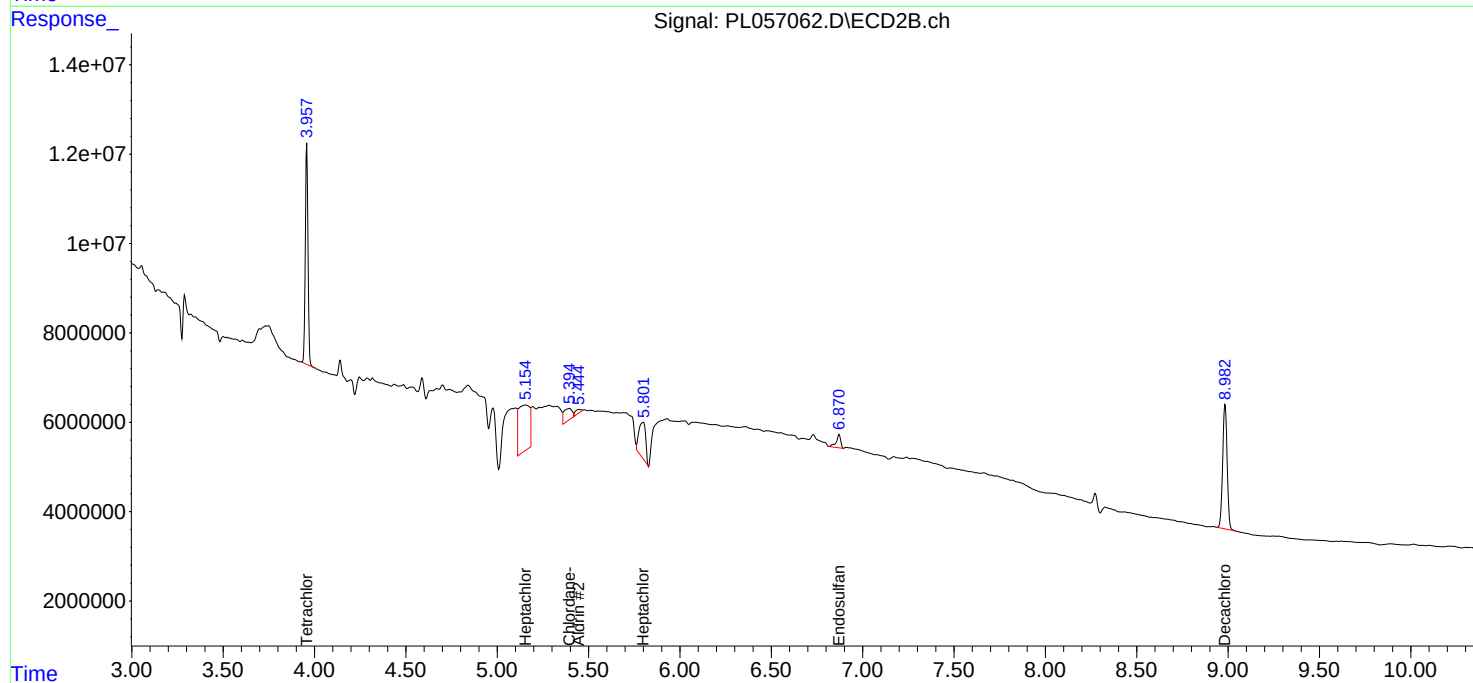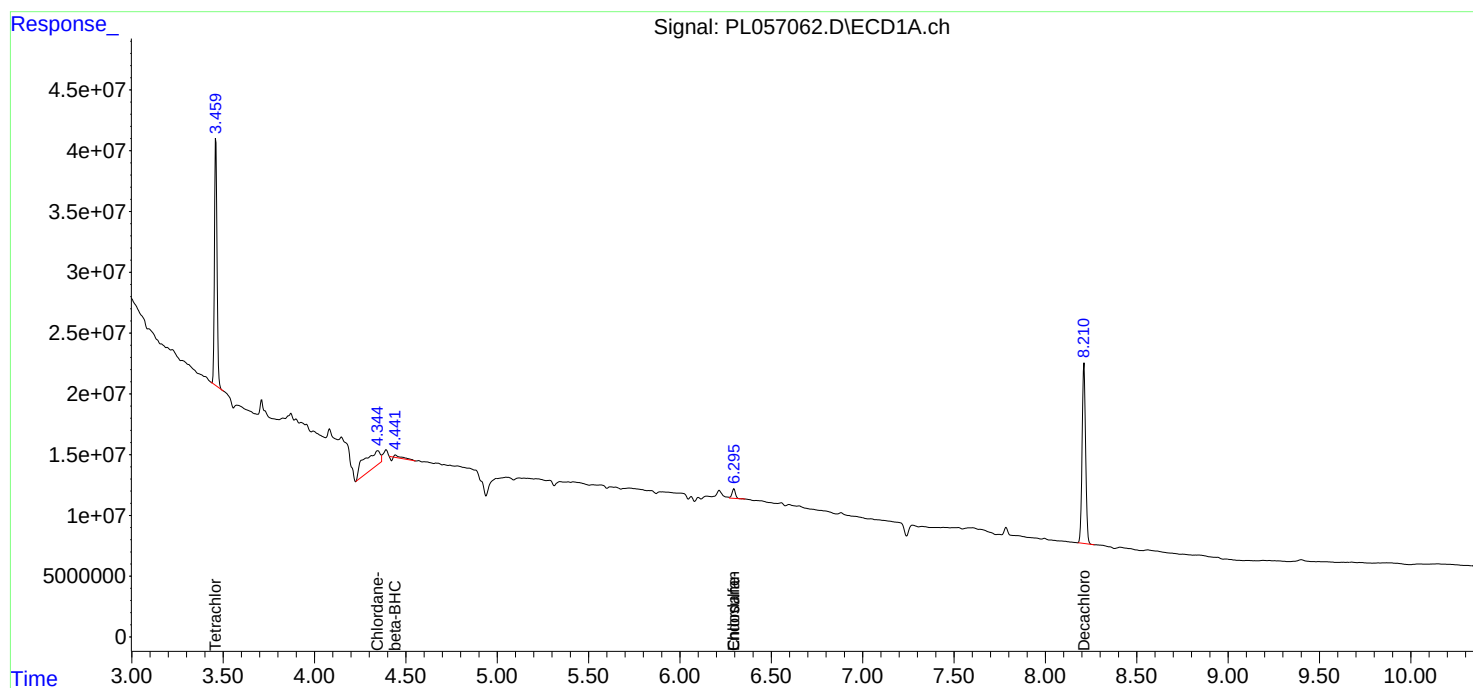


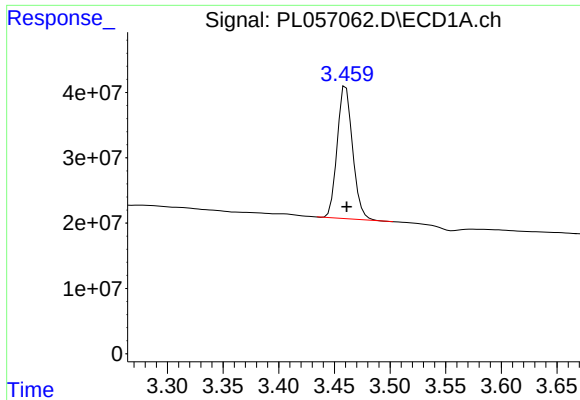

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 194830823
Conc: 22.86 ng/ml

Instrument :
ECD_L
ClientSampleId :

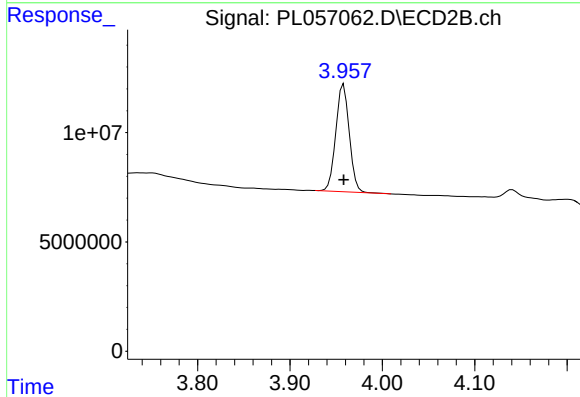


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 49872127
Conc: 23.38 ng/ml

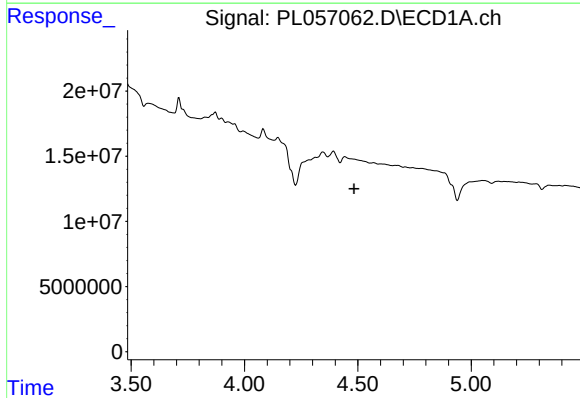


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

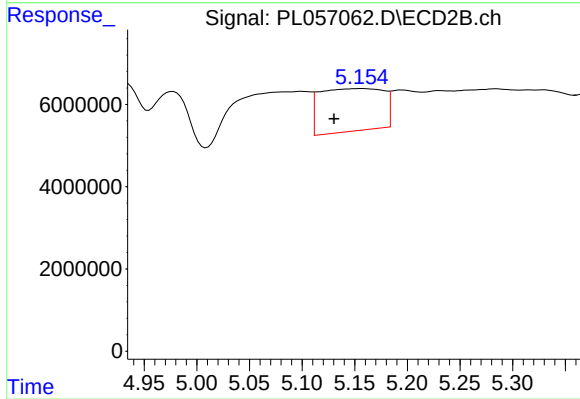

#4 Heptachlor


R.T.: 5.156 min
Delta R.T.: 0.026 min
Response: 43627598
Conc: 14.02 ng/ml

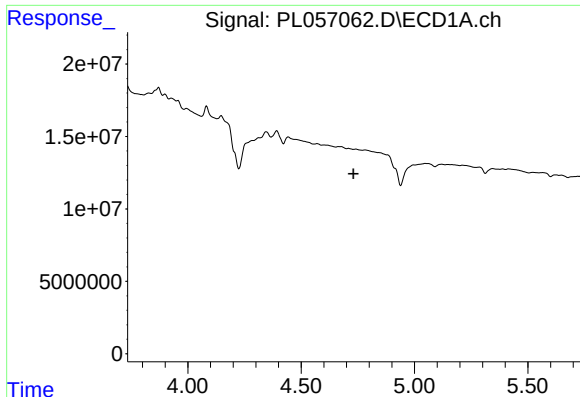

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 4.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

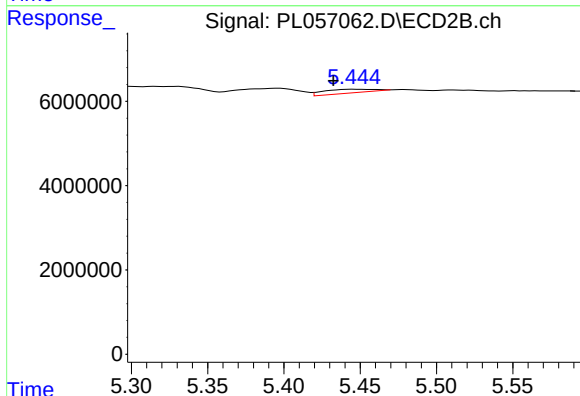


#5 Aldrin

R.T.: 5.447 min
Delta R.T.: 0.014 min
Response: 2016938
Conc: 0.67 ng/ml

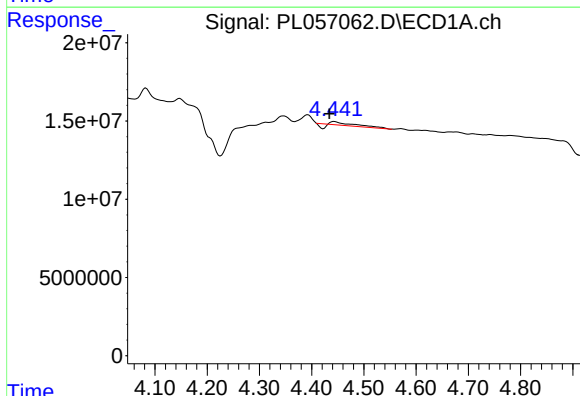


#6 beta-BHC

R.T.: 4.443 min
Delta R.T.: 0.009 min
Response: 4839450
Conc: 0.91 ng/ml

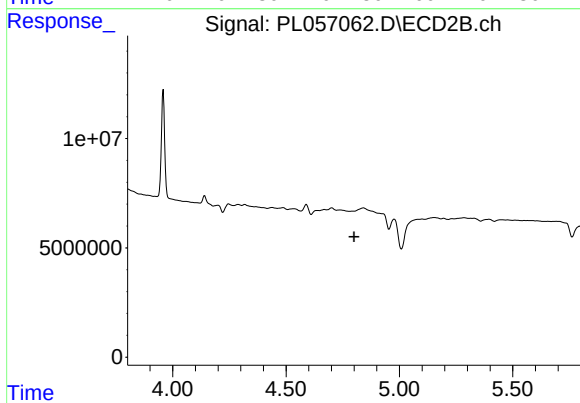

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.800 min
Response: 0
Conc: N.D.

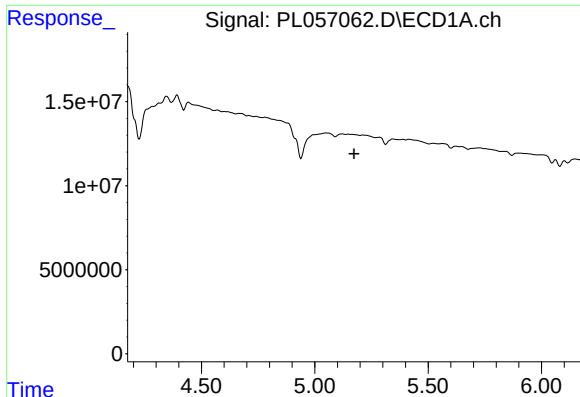

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

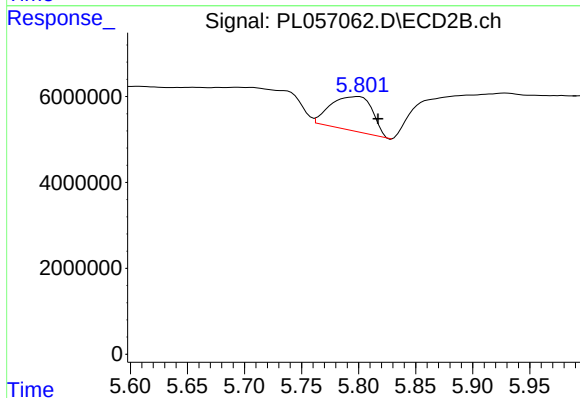


#8 Heptachlor epoxide

R.T.: 5.800 min
Delta R.T.: -0.017 min
Response: 20437015
Conc: 7.38 ng/ml

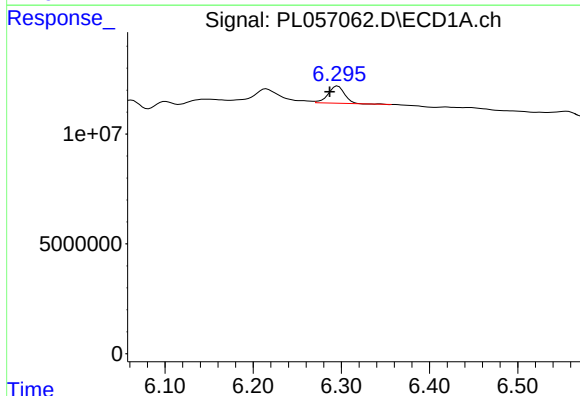


#15 Endosulfan II

R.T.: 6.296 min
Delta R.T.: 0.009 min
Response: 10325983
Conc: 0.96 ng/ml

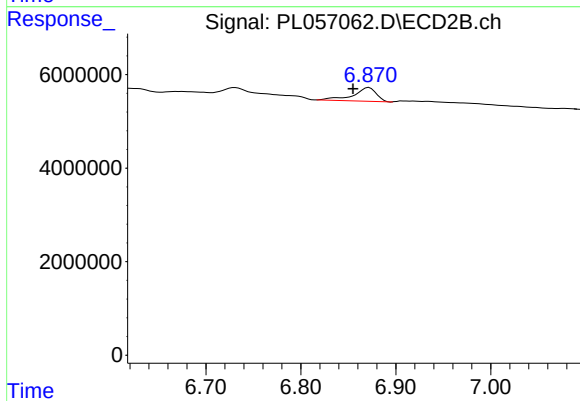

#15 Endosulfan II


R.T.: 6.872 min
Delta R.T.: 0.017 min
Response: 4963674
Conc: 1.77 ng/ml

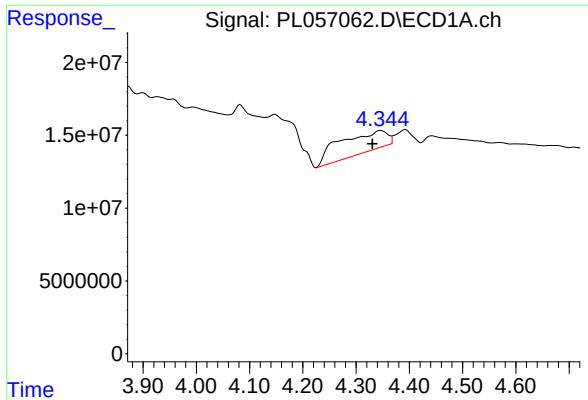

#23 Chlordane-1


R.T.: 4.346 min
Delta R.T.: 0.016 min
Response: 88074394
Conc: 289.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

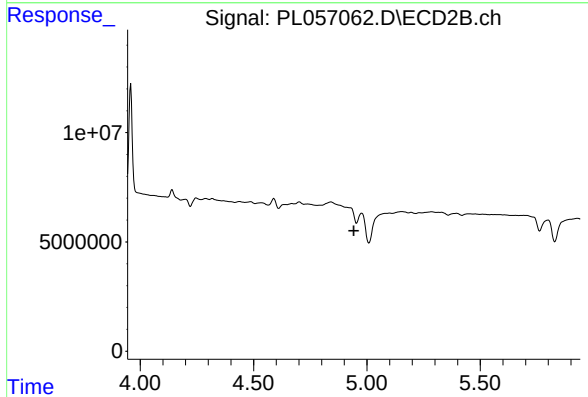


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

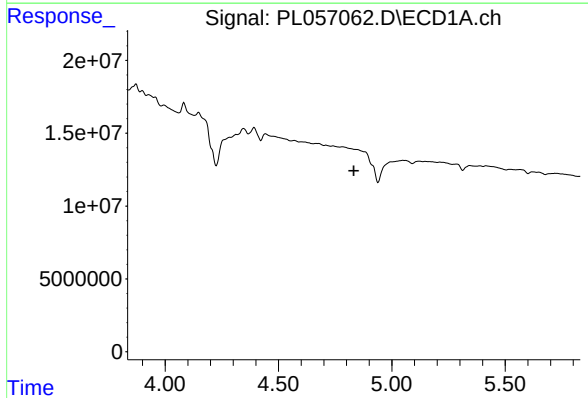


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 4.832 min
Response: 0
Conc: N.D.

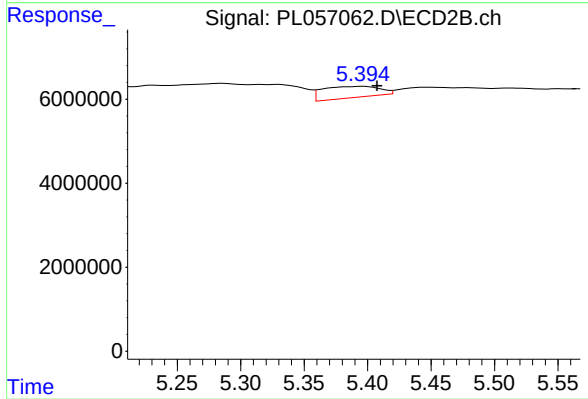

#24 Chlordane-2


R.T.: 5.396 min
Delta R.T.: -0.011 min
Response: 8363823
Conc: 87.62 ng/ml

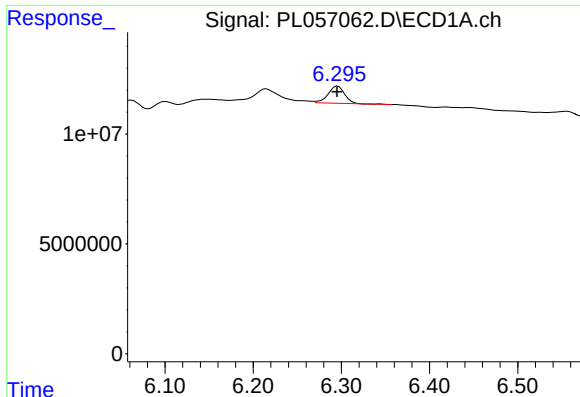

#27 Chlordane-5


R.T.: 6.296 min
Delta R.T.: 0.000 min
Response: 10325983
Conc: 28.43 ng/ml

Instrument :
ECD_L
ClientSampleId :

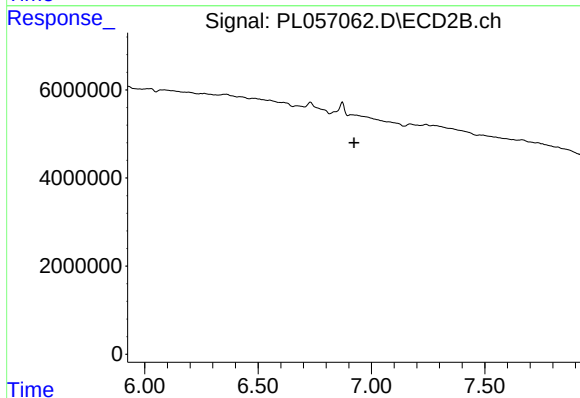


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.923 min
Response: 0
Conc: N.D.

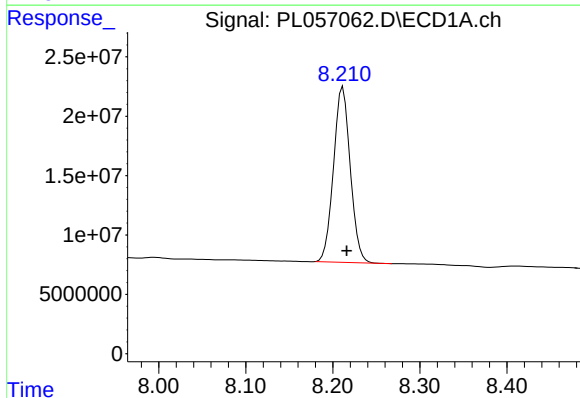

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.004 min
Response: 197383685
Conc: 20.42 ng/ml

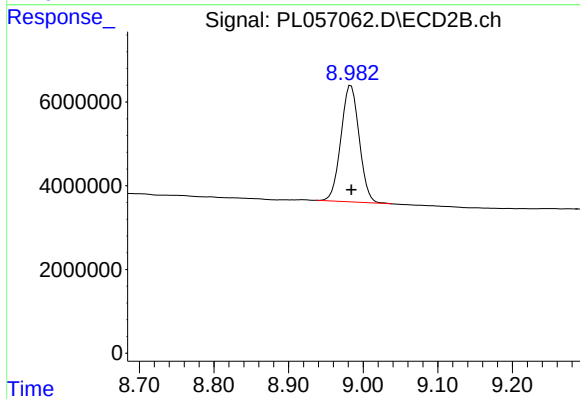

#28 Decachlorobiphenyl

R.T.: 8.984 min
Delta R.T.: 0.000 min
Response: 47191905
Conc: 22.21 ng/ml