

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
 Data File : PL057063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 22:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 02:52:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.958	184.9E6	49720572	21.692	23.305
28)	SA Decachlor...	8.212	8.983	184.4E6	44879217	19.074	21.122
Target Compounds							
8)	B Heptachlo...	0.000	5.809	0	10323706	N.D.	3.726 #
12)	B 4,4'-DDE	5.648f	0.000	32150362	0	2.744	N.D. #
13)	MA Dieldrin	5.735f	0.000	39769456	0	3.253	N.D. #
14)	MA Endrin	0.000	6.645	0	7169976	N.D.	2.780 #
15)	B Endosulfa...	0.000	6.870f	0	4846809	N.D.	1.727 #
16)	A 4,4'-DDD	0.000	6.786f	0	4226402	N.D.	1.735 #
23)	Chlordane-1	4.359f	0.000	15764555	0	51.866	N.D. #
27)	Chlordane-5	0.000	6.917	0	2543982	N.D.	30.493 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
Data File : PL057063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 22:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 02:52:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

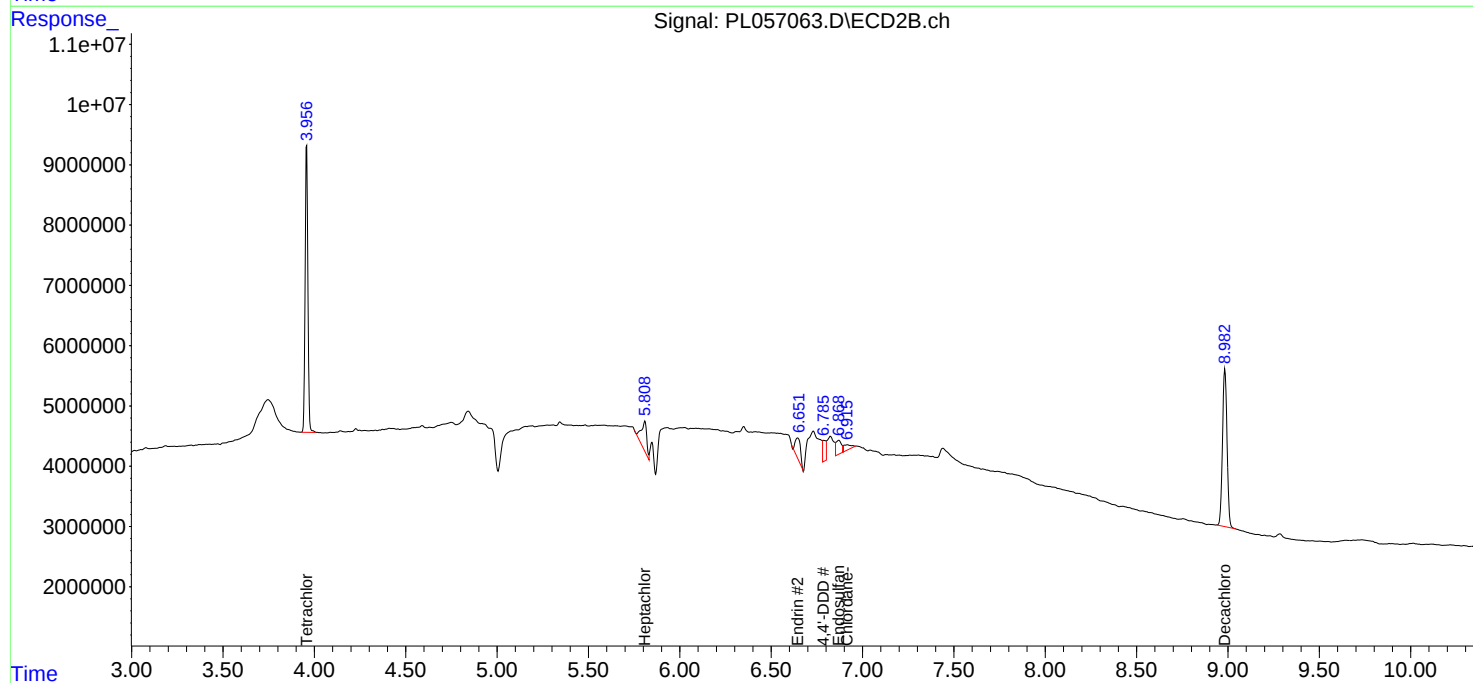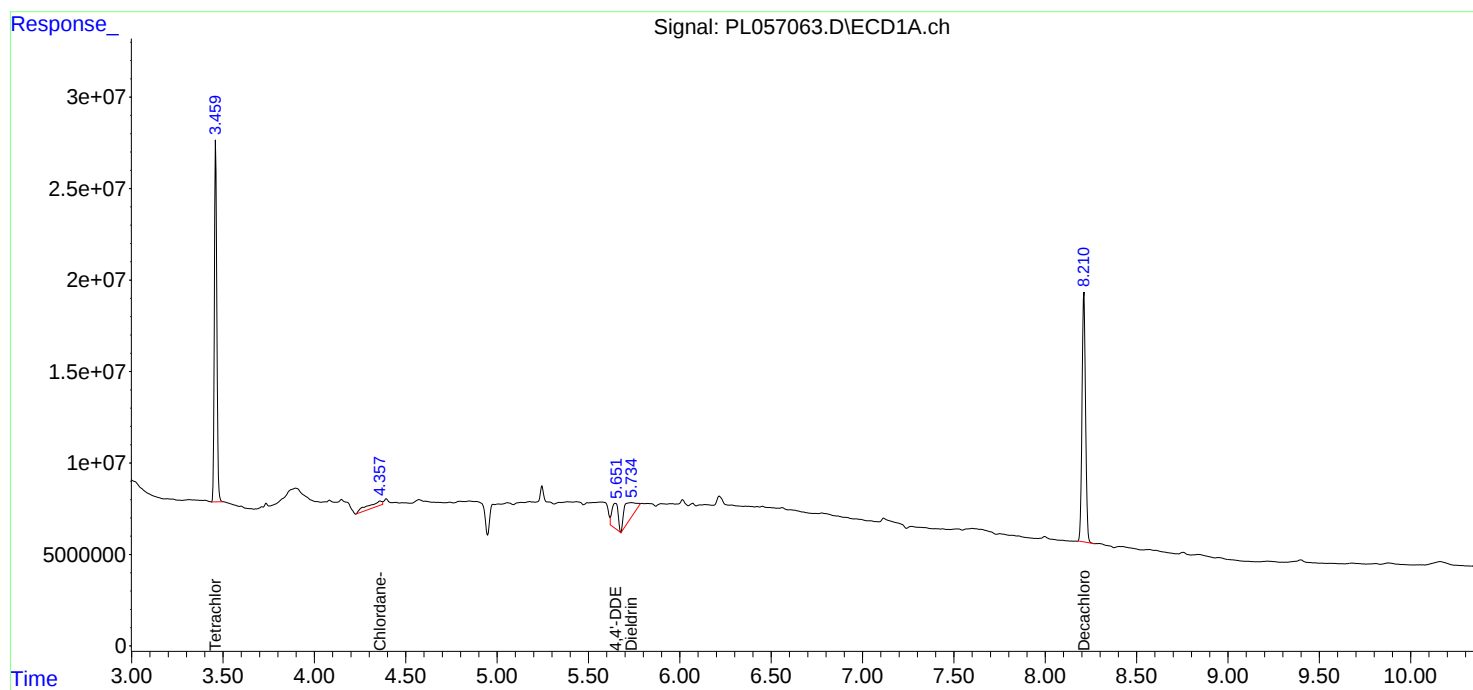


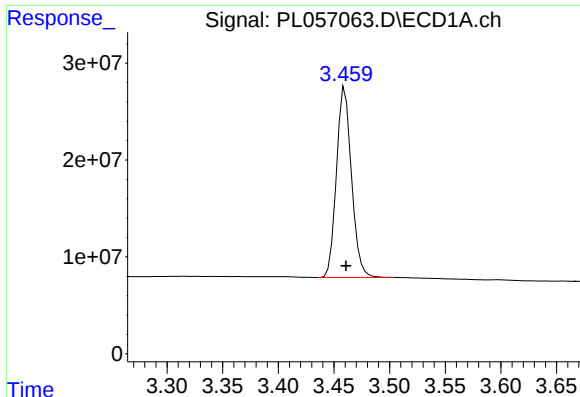

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 184868272
Conc: 21.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

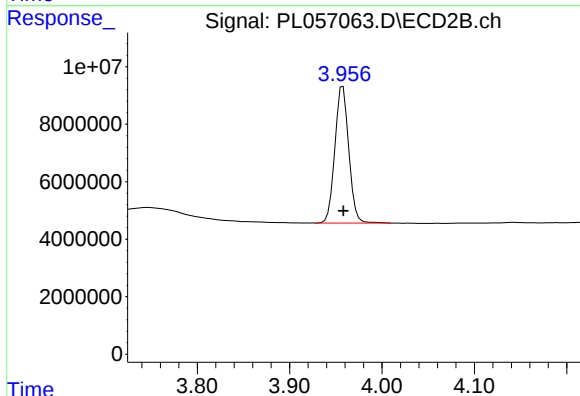


#1 Tetrachloro-m-xylene

R.T.: 3.958 min
Delta R.T.: 0.000 min
Response: 49720572
Conc: 23.30 ng/ml

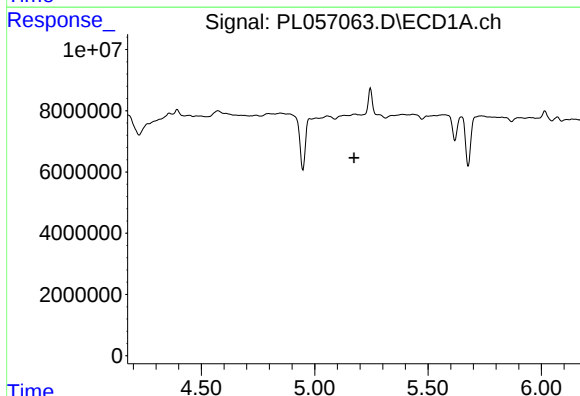


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

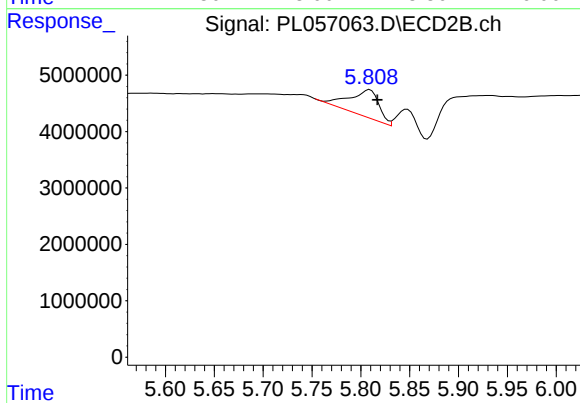

#8 Heptachlor epoxide


R.T.: 5.809 min
Delta R.T.: -0.008 min
Response: 10323706
Conc: 3.73 ng/ml

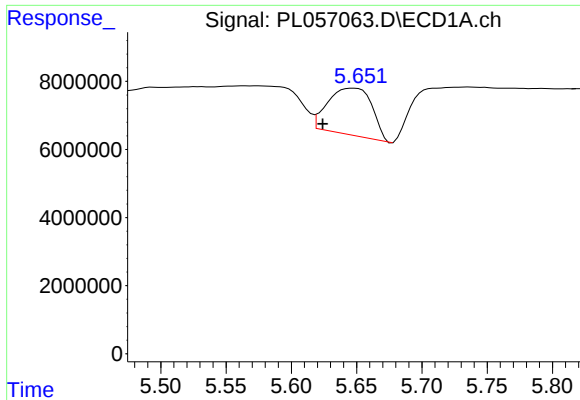

#12 4,4'-DDE


R.T.: 5.648 min
Delta R.T.: 0.024 min
Response: 32150362
Conc: 2.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

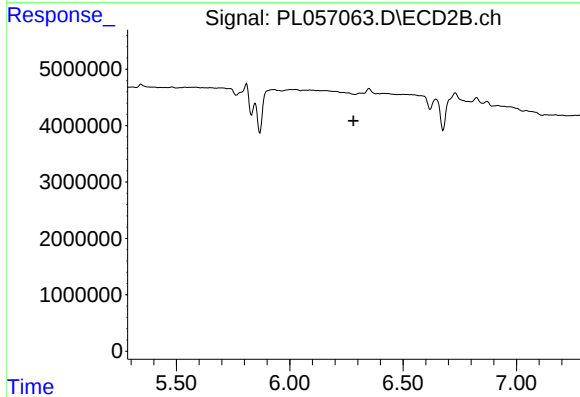


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.282 min
Response: 0
Conc: N.D.

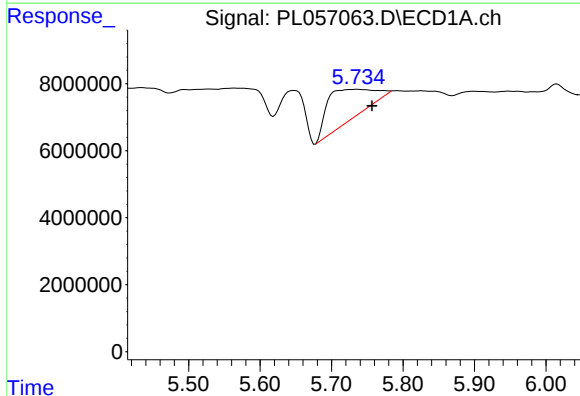


#13 Dieldrin

R.T.: 5.735 min
Delta R.T.: -0.021 min
Response: 39769456
Conc: 3.25 ng/ml

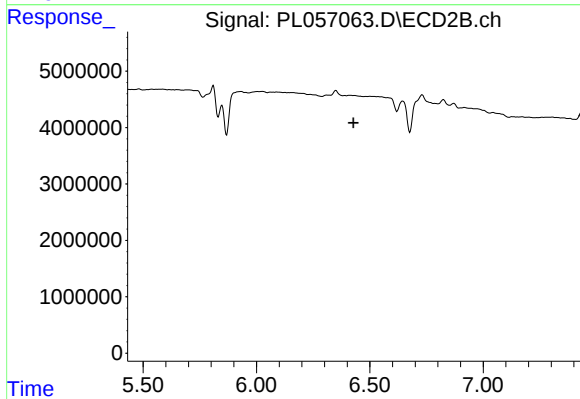

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

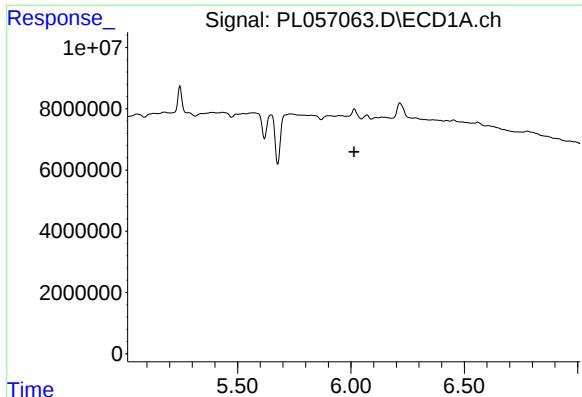

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

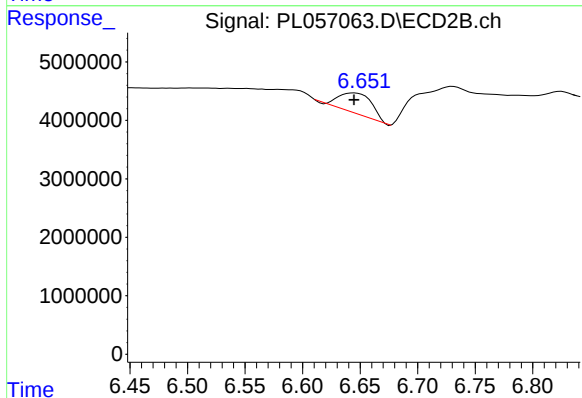


#14 Endrin

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 7169976
Conc: 2.78 ng/ml

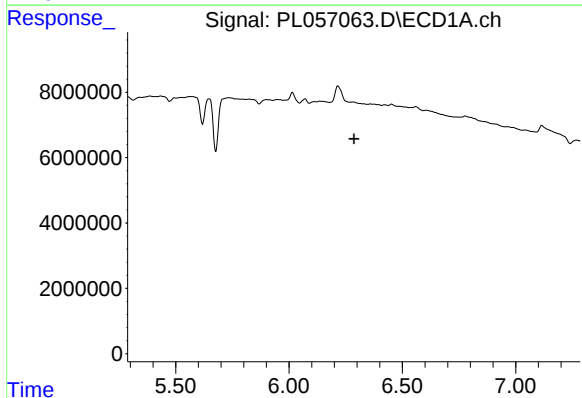


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

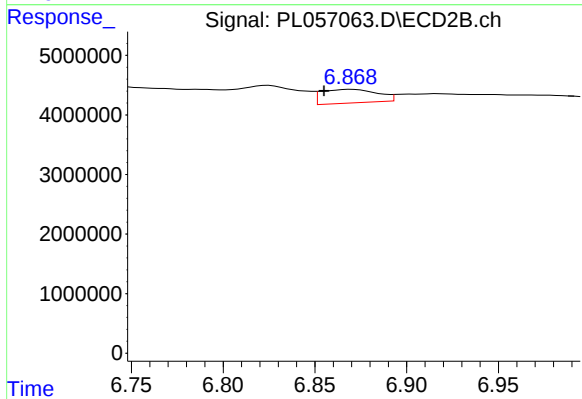

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 4846809
Conc: 1.73 ng/ml

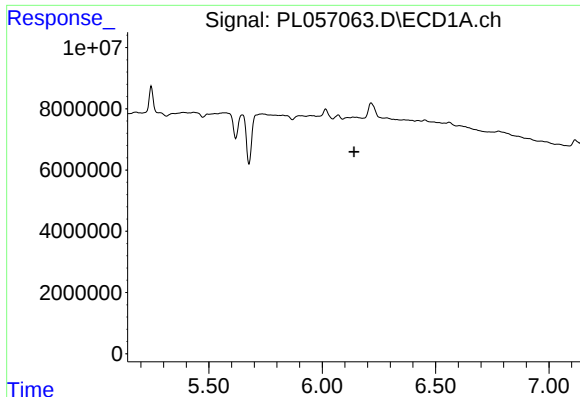

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

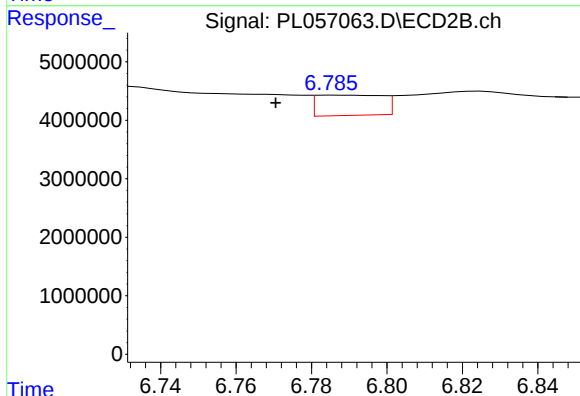


#16 4,4'-DDD

R.T.: 6.786 min
Delta R.T.: 0.015 min
Response: 4226402
Conc: 1.73 ng/ml

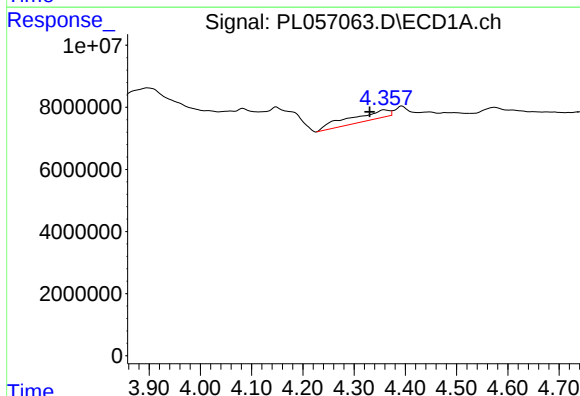


#23 Chlordane-1

R.T.: 4.359 min
Delta R.T.: 0.028 min
Response: 15764555
Conc: 51.87 ng/ml

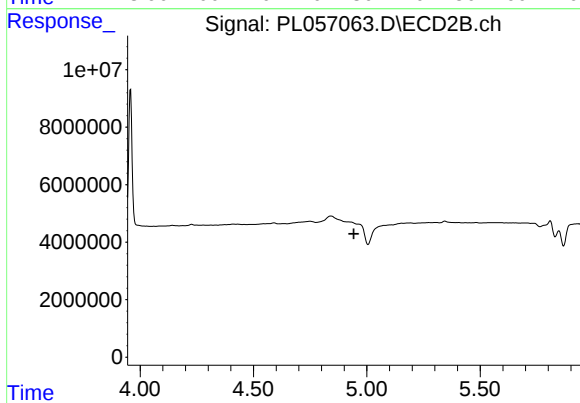

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.942 min
Response: 0
Conc: N.D.

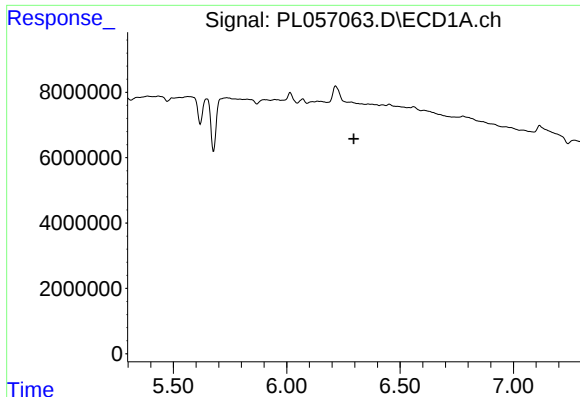

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

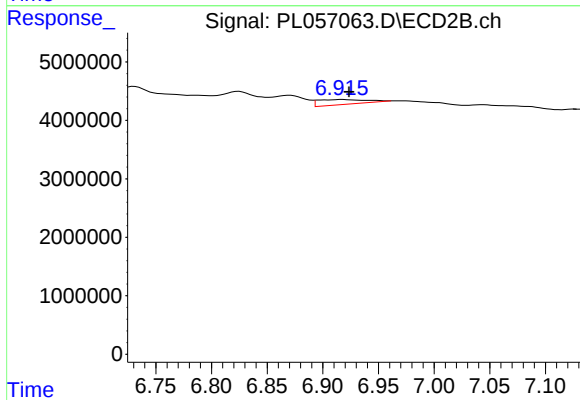


#27 Chlordane-5

R.T.: 6.917 min
Delta R.T.: -0.006 min
Response: 2543982
Conc: 30.49 ng/ml

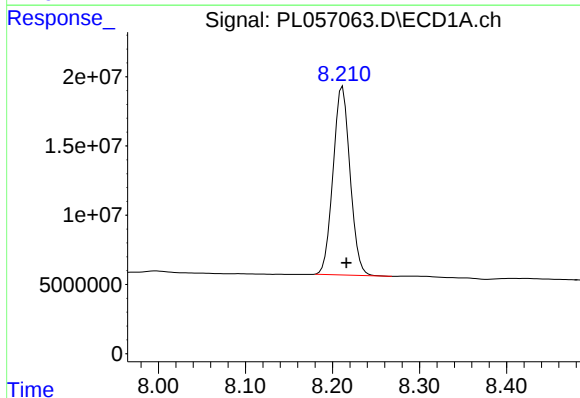

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.004 min
Response: 184351903
Conc: 19.07 ng/ml

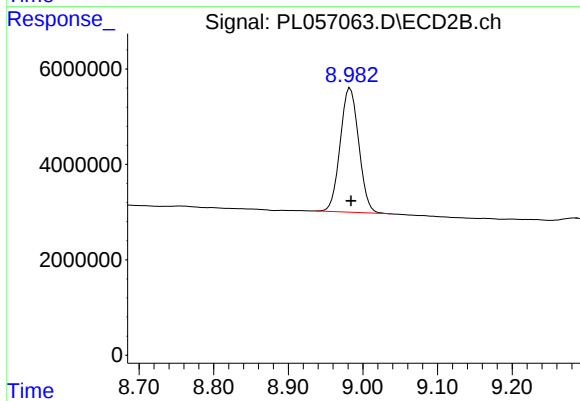

#28 Decachlorobiphenyl

R.T.: 8.983 min
Delta R.T.: -0.001 min
Response: 44879217
Conc: 21.12 ng/ml