

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
 Data File : PL057040.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2020 16:06
 Operator : AJ\MA
 Sample : L1743-04DL 200X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 C-8DL

Manual Integrations
 APPROVED

mohammad
 3/6/2020 11:22:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:25:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
4) MA	Heptachlor	4.482	5.129	185.9E6	47099292	13.682 15.133m
10) B	gamma-Chl...	5.400	6.050	556.7E6	191.6E6	44.824 64.016m#
11) B	alpha-Chl...	5.458	6.124	508.5E6	226.9E6	41.386 75.281 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030420\
Data File : PL057040.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2020 16:06
Operator : AJ\MA
Sample : L1743-04DL 200X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
C-8DL


Manual Integrations
APPROVED

mohammad
3/6/2020 11:22:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:25:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

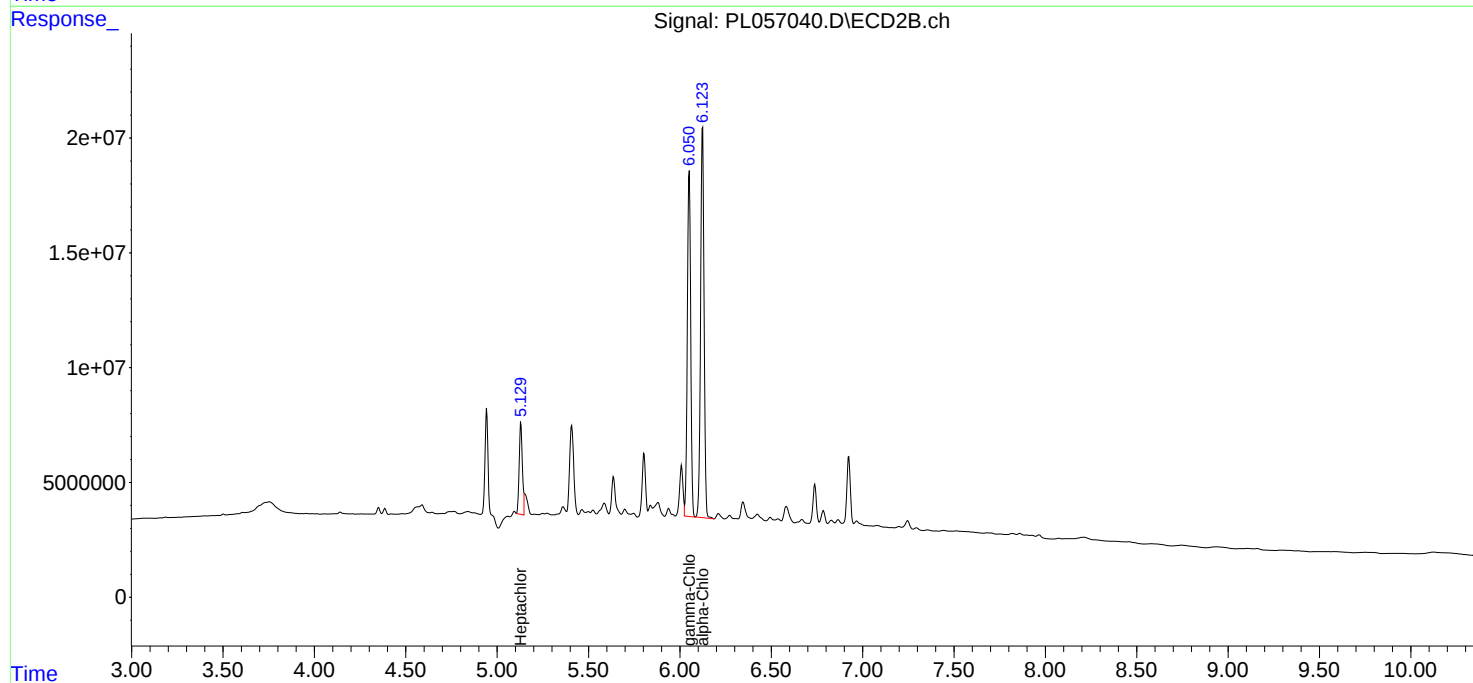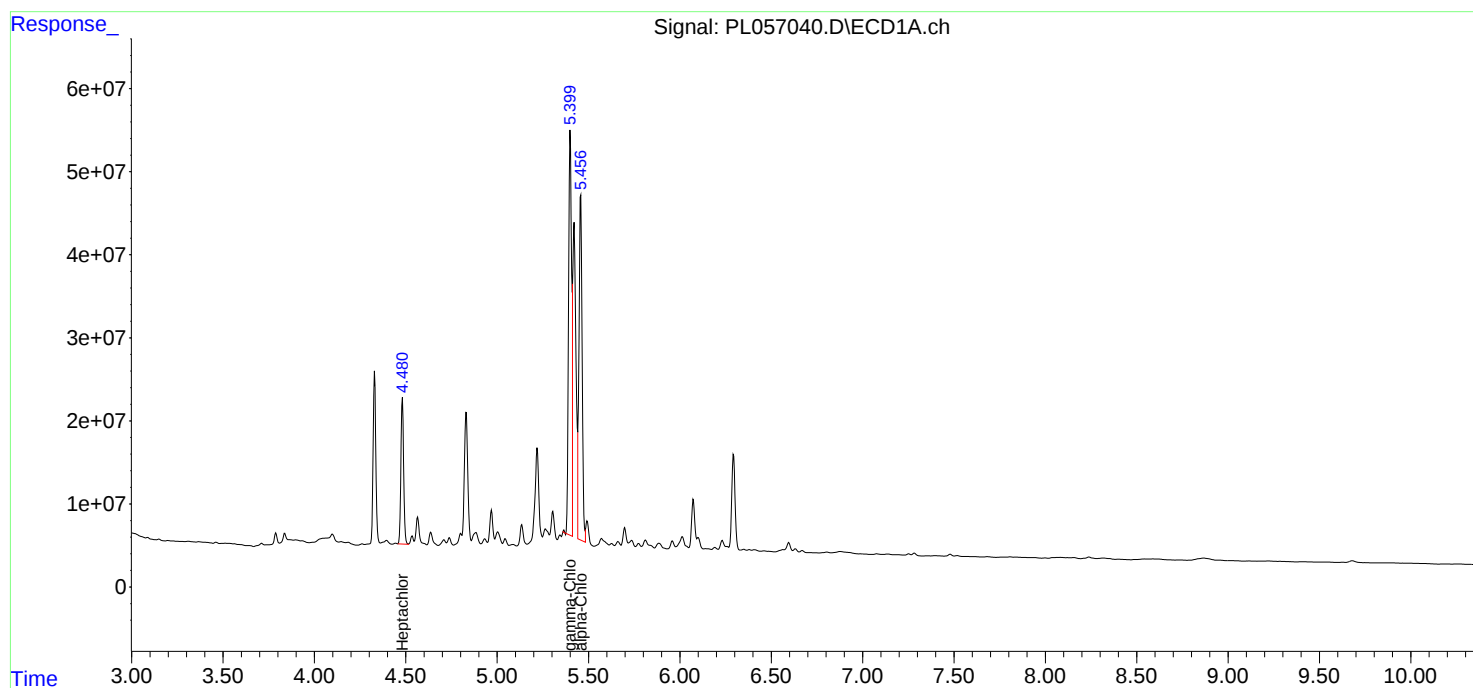

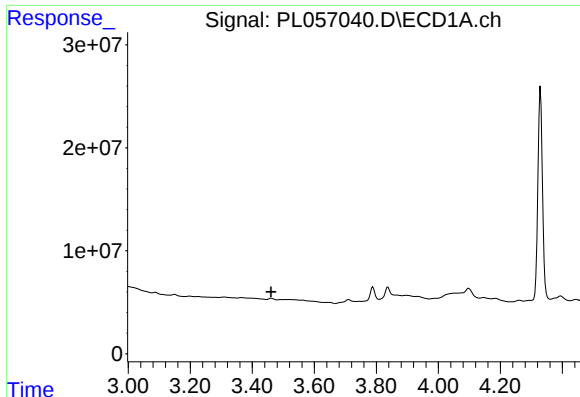


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.461 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
C-8DL


Manual Integrations
APPROVED

mohammad
3/6/2020 11:22:46 AM

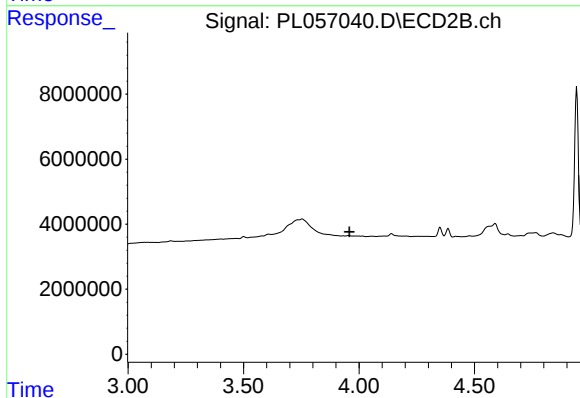


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.958 min
Response: 0
Conc: N.D.

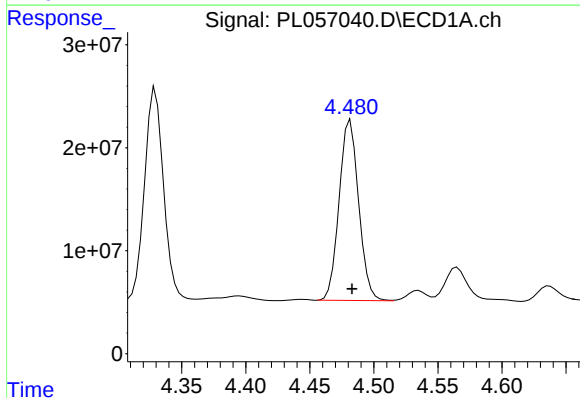


#4 Heptachlor

R.T.: 4.482 min
Delta R.T.: -0.001 min
Response: 185859102
Conc: 13.68 ng/ml

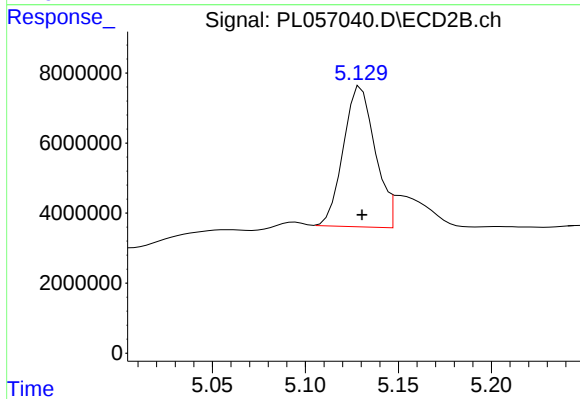

#4 Heptachlor

R.T.: 5.129 min
Delta R.T.: -0.002 min
Response: 47099292
Conc: 15.13 ng/ml m

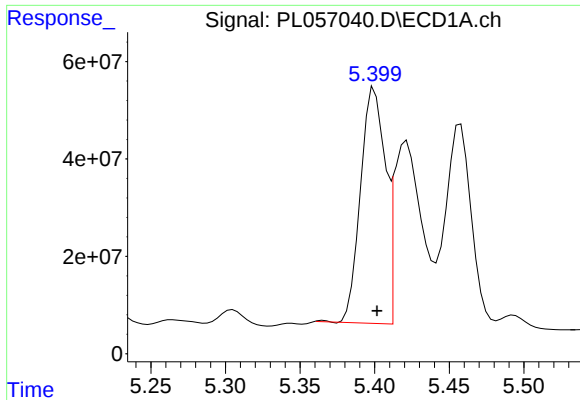


#10 gamma-Chlordane

R.T.: 5.400 min
Delta R.T.: -0.002 min
Response: 556747358
Conc: 44.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
C-8DL


Manual Integrations
APPROVED

mohammad
3/6/2020 11:22:46 AM

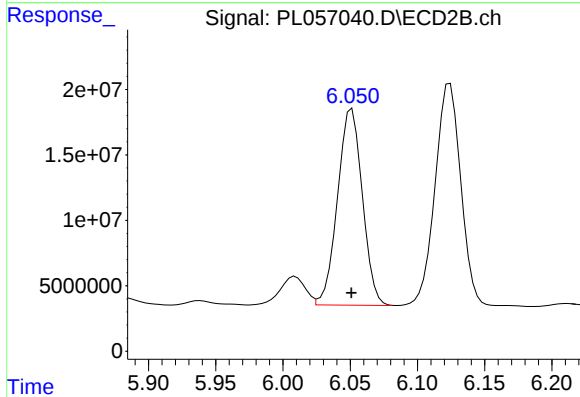


#10 gamma-Chlordane

R.T.: 6.050 min
Delta R.T.: -0.001 min
Response: 191640228
Conc: 64.02 ng/ml m

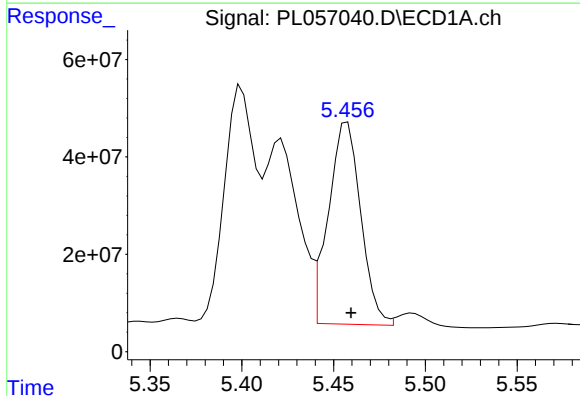


#11 alpha-Chlordane

R.T.: 5.458 min
Delta R.T.: -0.002 min
Response: 508472249
Conc: 41.39 ng/ml

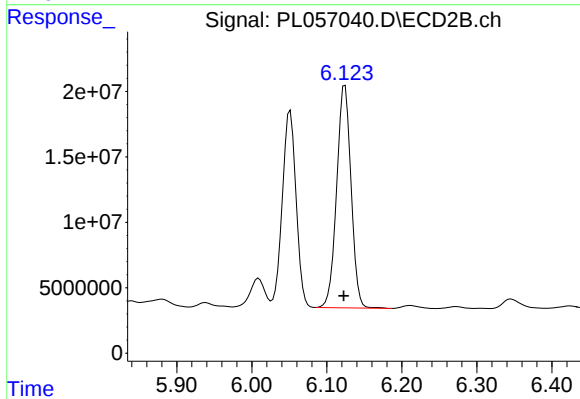

#11 alpha-Chlordane

R.T.: 6.124 min
Delta R.T.: 0.002 min
Response: 226932177
Conc: 75.28 ng/ml

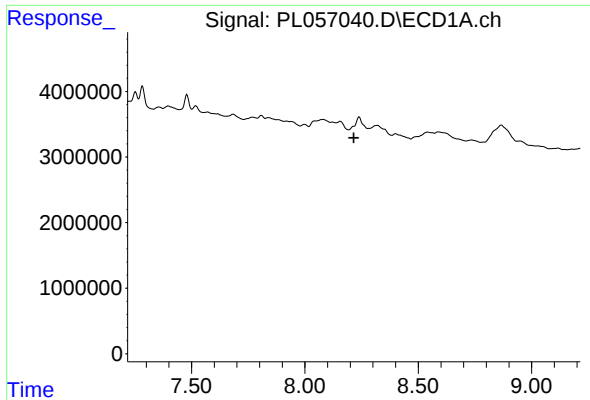


#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.216 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
C-8DL

Manual Integrations
APPROVED

mohammad
3/6/2020 11:22:46 AM

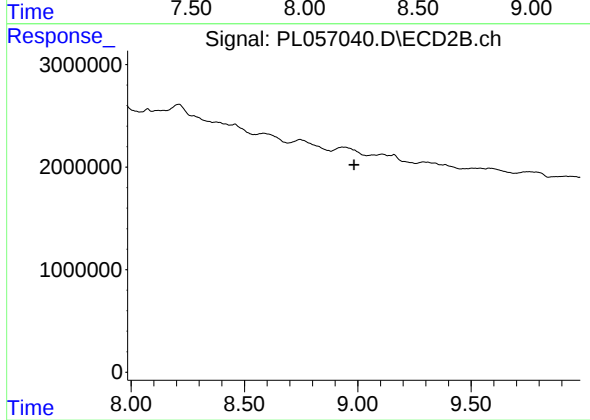

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.984 min
Response: 0
Conc: N.D.