

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
 Data File : PL065045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 08:52
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:03:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.423	0.000	2026336	0	0.720	N.D. #
Target Compounds						
6) B beta-BHC	0.000	4.975	0	8361091	N.D.	2.861 #
8) B Heptachlo...	0.000	6.002	0	19396062	N.D.	8.791 #
14) MA Endrin	5.957	0.000	12091389	0	4.026	N.D. #
15) B Endosulfa...	6.248f	0.000	1554804	0	0.540	N.D. #
23) Chlordane-1	4.298	0.000	358442	0	3.153	N.D. #
27) Chlordane-5	6.248	0.000	1554804	0	15.367	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
Data File : PL065045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 08:52
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:03:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

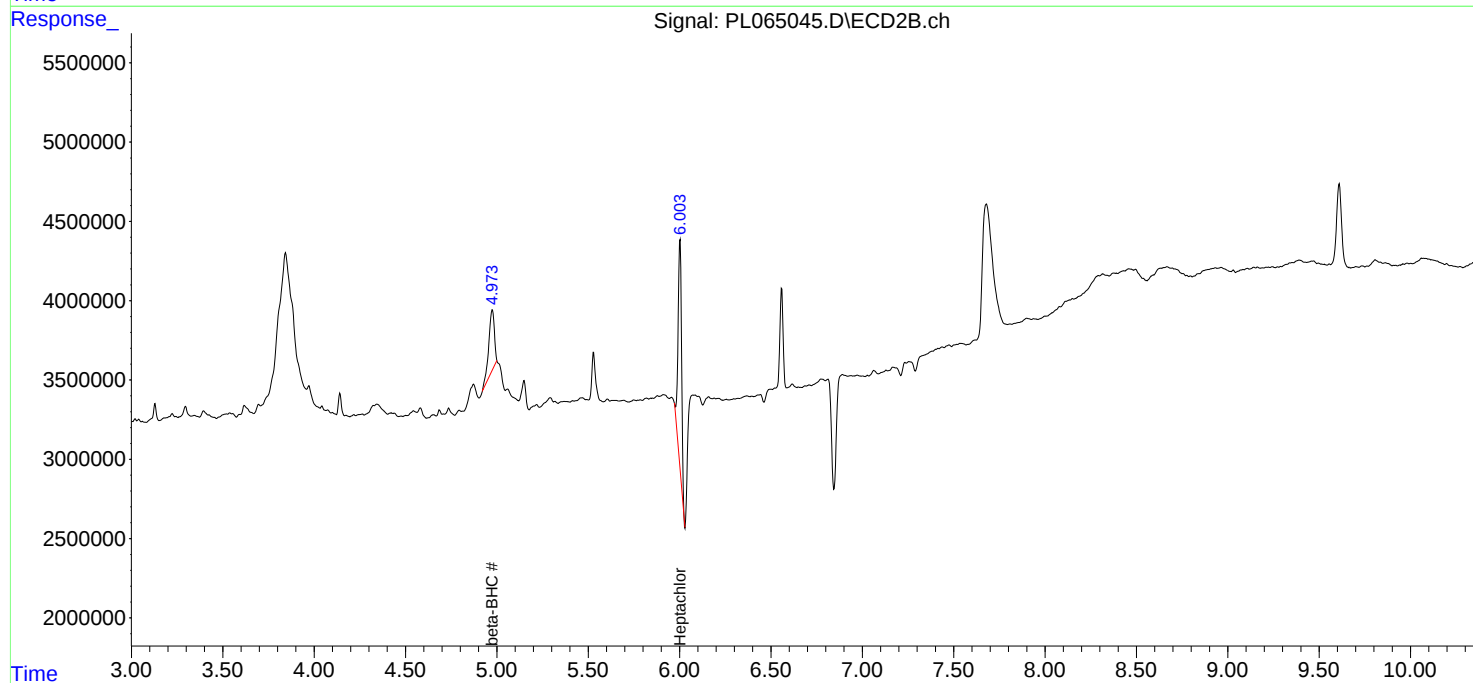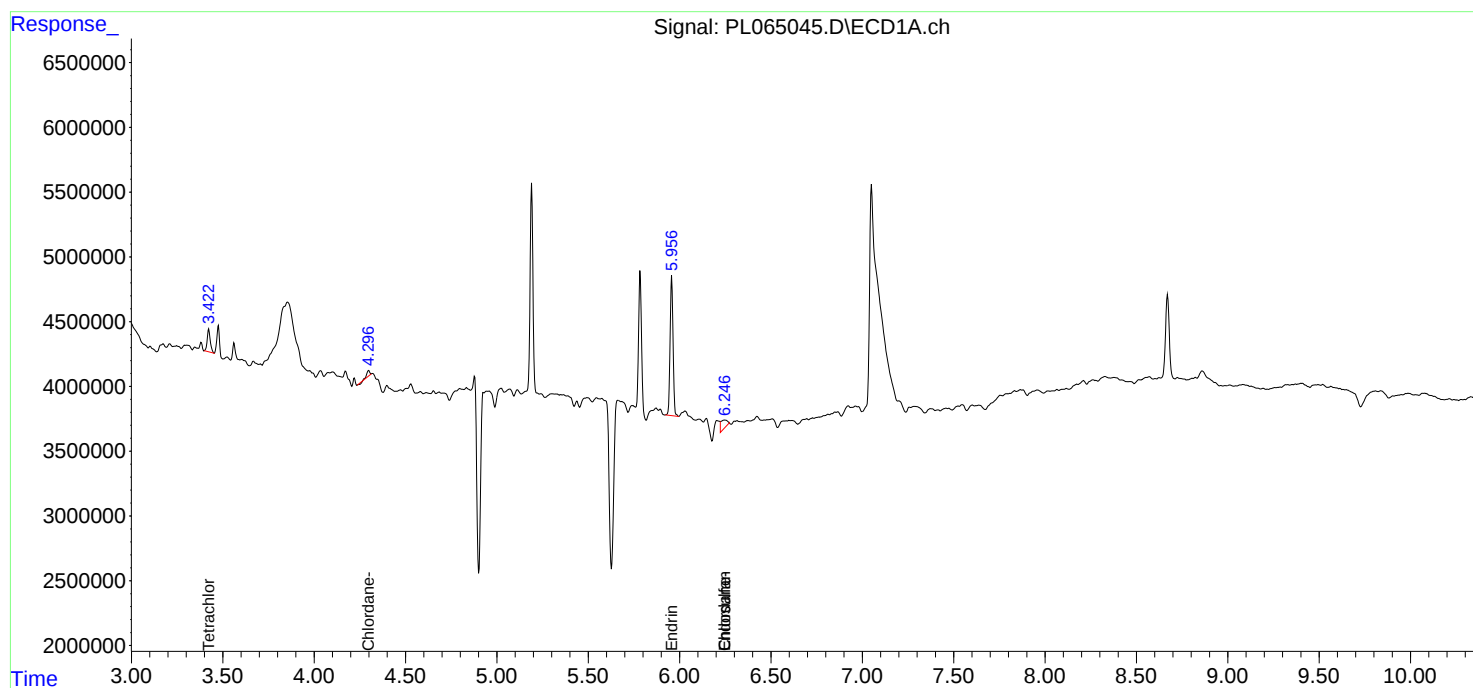


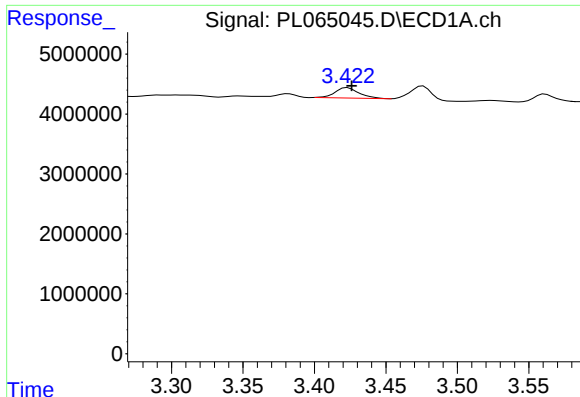

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 2026336
Conc: 0.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

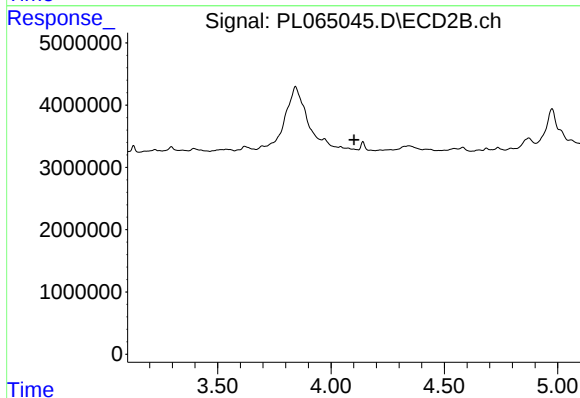


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.102 min
Response: 0
Conc: N.D.

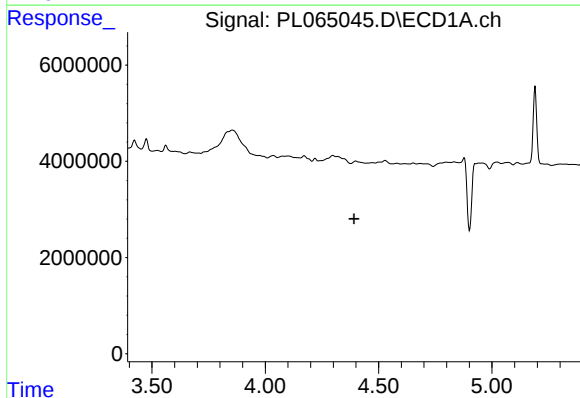


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

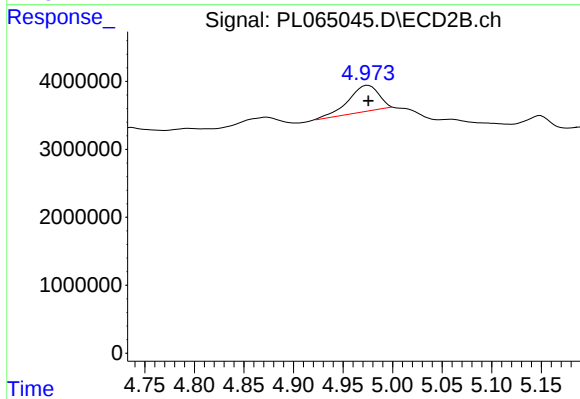

#6 beta-BHC

R.T.: 4.975 min
Delta R.T.: 0.000 min
Response: 8361091
Conc: 2.86 ng/ml

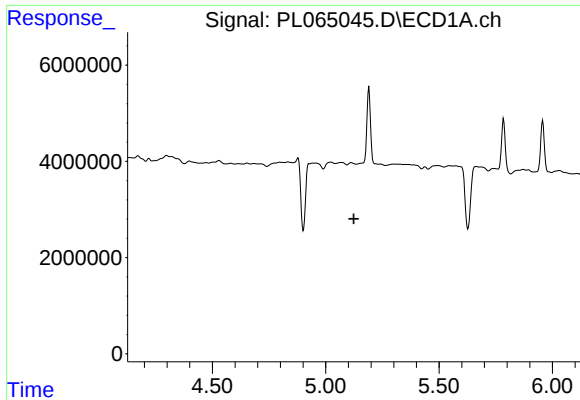


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :


Time

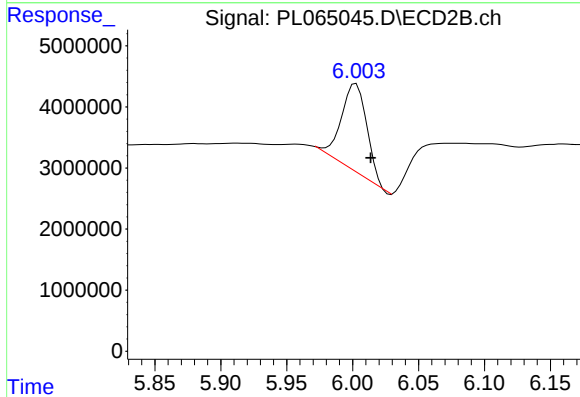

#8 Heptachlor epoxide

R.T.: 6.002 min
Delta R.T.: -0.011 min
Response: 19396062
Conc: 8.79 ng/ml


Time

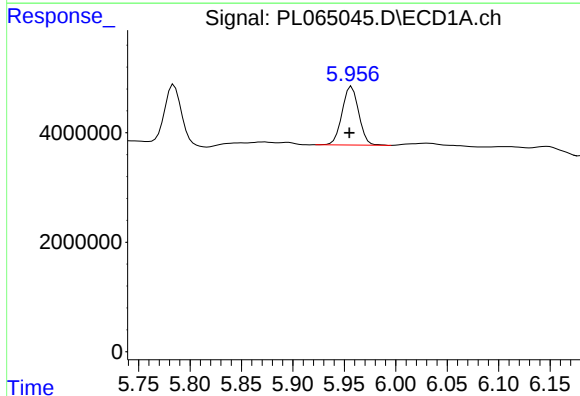

#14 Endrin


R.T.: 5.957 min
Delta R.T.: 0.002 min
Response: 12091389
Conc: 4.03 ng/ml

Time

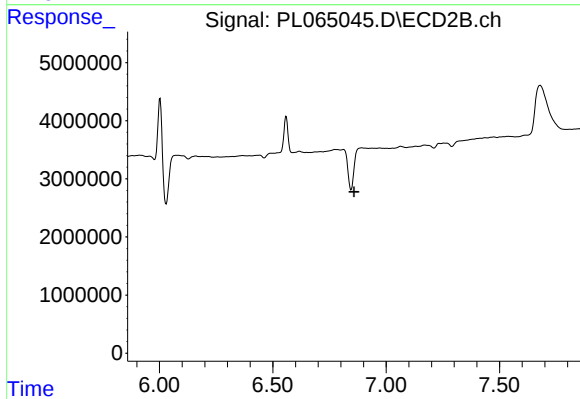

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.858 min
Response: 0
Conc: N.D.

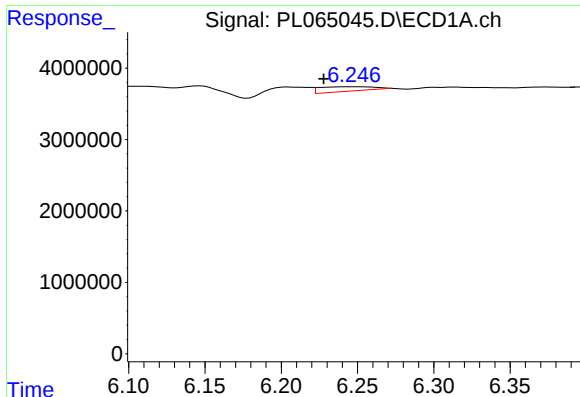

#15 Endosulfan II


R.T.: 6.248 min
Delta R.T.: 0.020 min
Response: 1554804
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

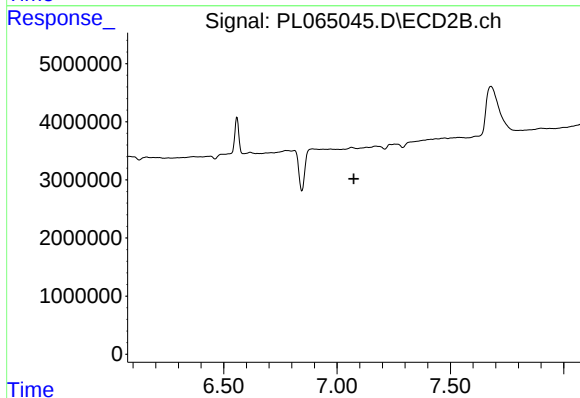


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.073 min
Response: 0
Conc: N.D.

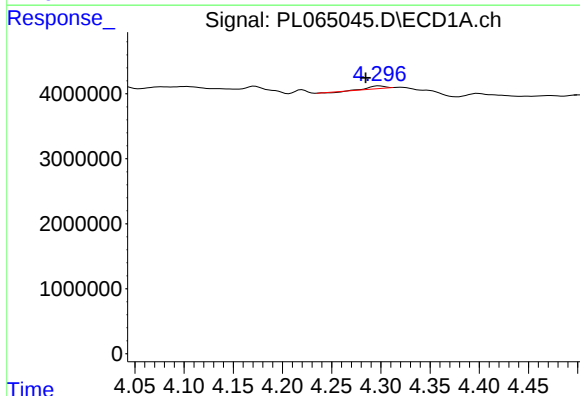


#23 Chlordane-1

R.T.: 4.298 min
Delta R.T.: 0.014 min
Response: 358442
Conc: 3.15 ng/ml

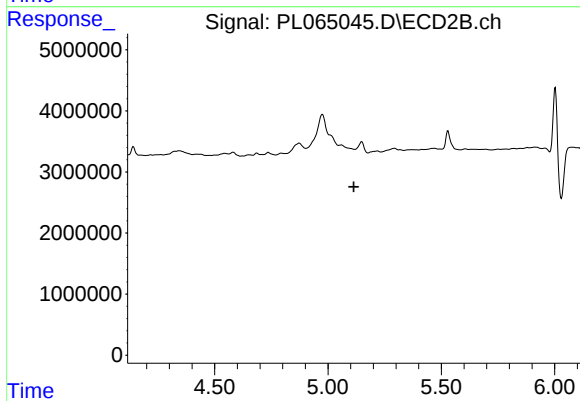

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

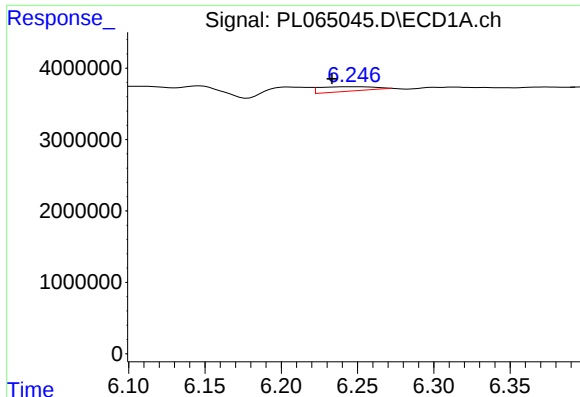

#27 Chlordane-5


R.T.: 6.248 min
Delta R.T.: 0.014 min
Response: 1554804
Conc: 15.37 ng/ml

Instrument :
ECD_L
ClientSampleId :

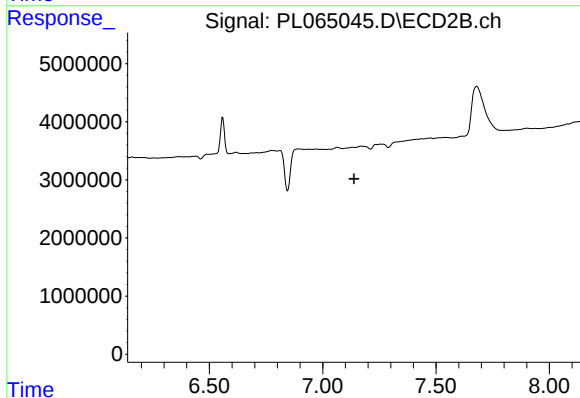


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.139 min
Response: 0
Conc: N.D.

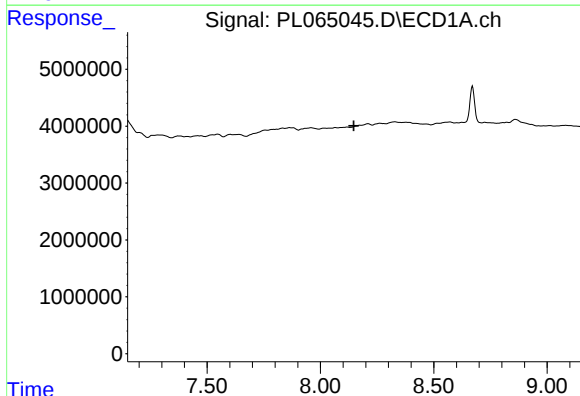

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.148 min
Response: 0
Conc: N.D.

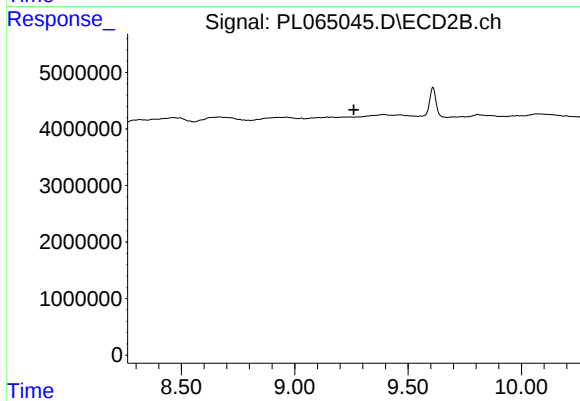

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.