

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
 Data File : PL065054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 11:45
 Operator : AR\AJ
 Sample : M1539-01DL2 100X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:05:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml	

System Monitoring Compounds								
28)	SA Decachlor...	8.144	0.000	1369743	0	0.609	N.D.	#
Target Compounds								
9)	A Endosulfan I	5.484f	0.000	4334254	0	1.352	N.D.	#
10)	B gamma-Chl...	5.337	0.000	7017669	0	2.001	N.D.	#
12)	B 4,4'-DDE	5.563	6.473	8569462	3993710	2.738	1.969	#
13)	MA Dieldrin	0.000	6.644	0	1324202	N.D.	0.619	#
16)	A 4,4'-DDD	6.079	6.973	12927065	15066990	5.104	8.691	#
17)	MA 4,4'-DDT	6.318	7.272	91948052	67399123	40.776	44.206	
20)	A Methoxychlor	0.000	7.769f	0	7012843	N.D.	7.758	#
23)	Chlordane-1	4.296	0.000	578603	0	5.090	N.D.	#
25)	Chlordane-3	5.337	0.000	7017669	0	21.355	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
Data File : PL065054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 11:45
Operator : AR\AJ
Sample : M1539-01DL2 100X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:05:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

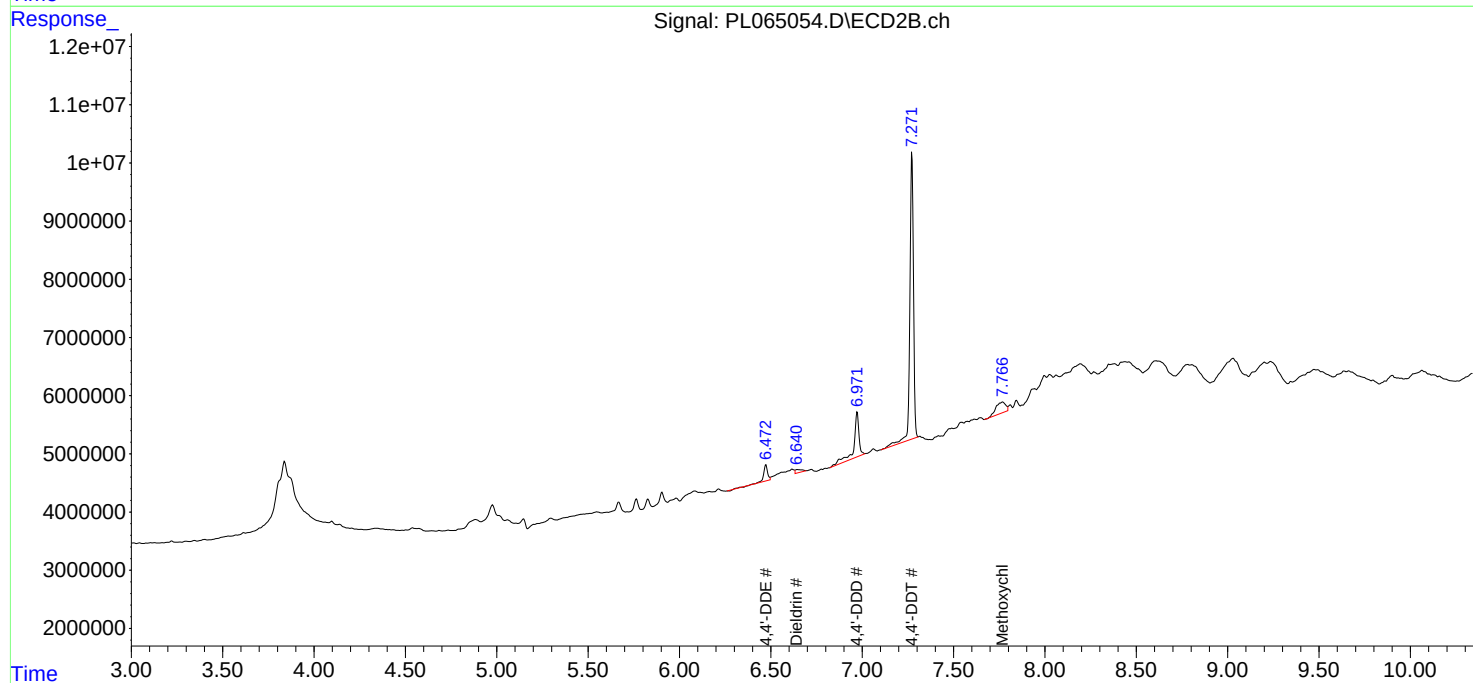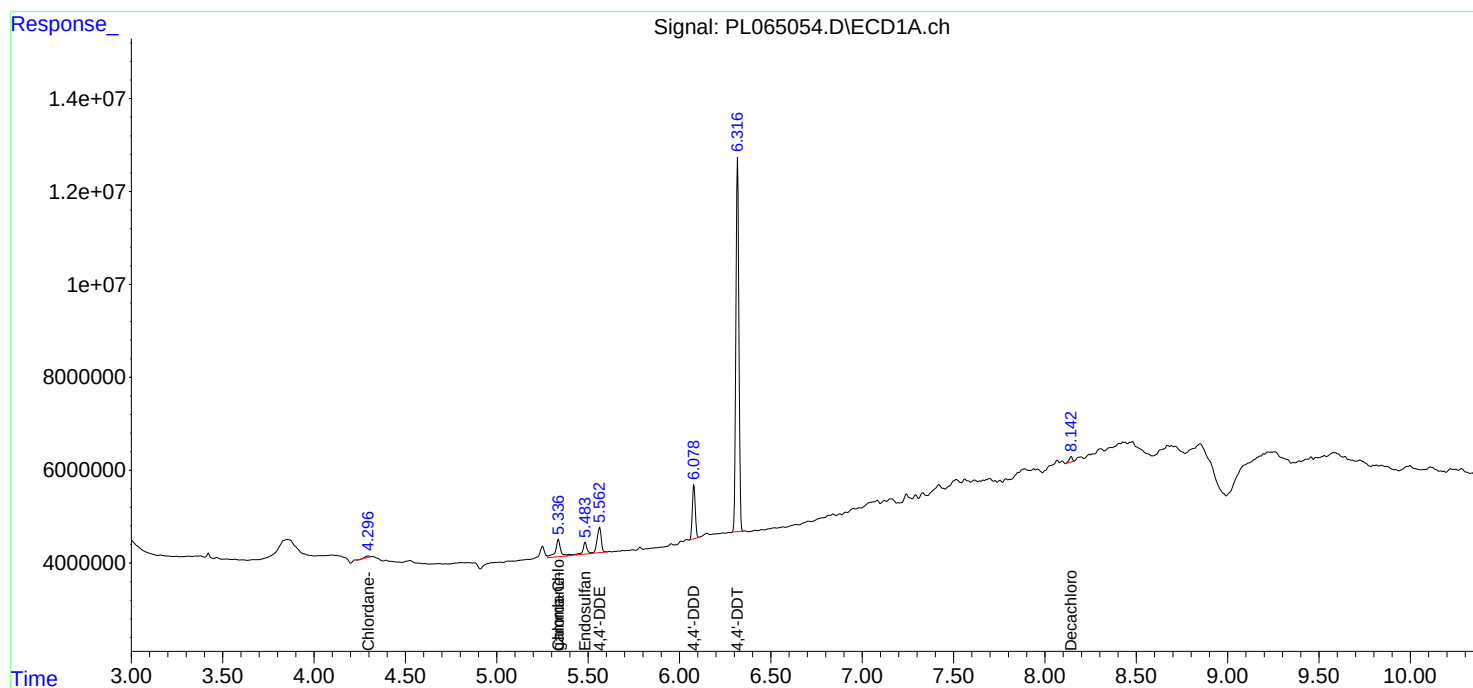


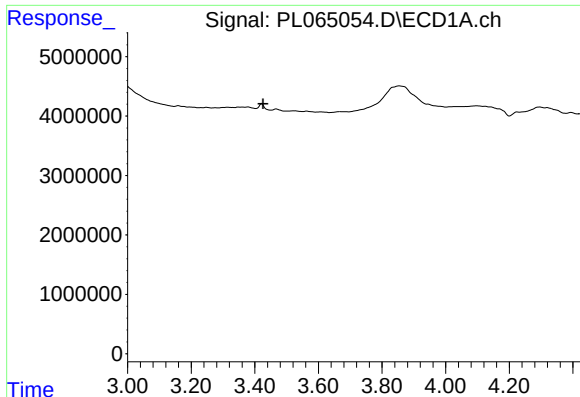

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.426 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

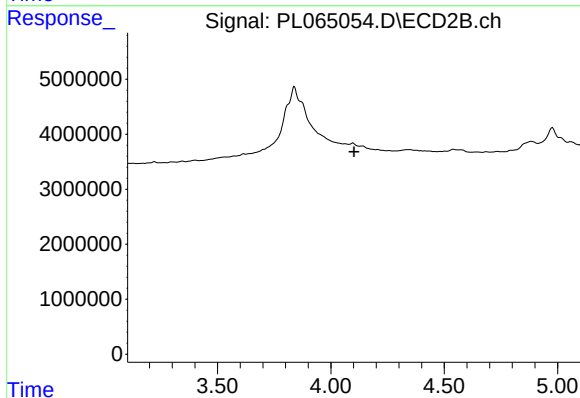


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.102 min
Response: 0
Conc: N.D.

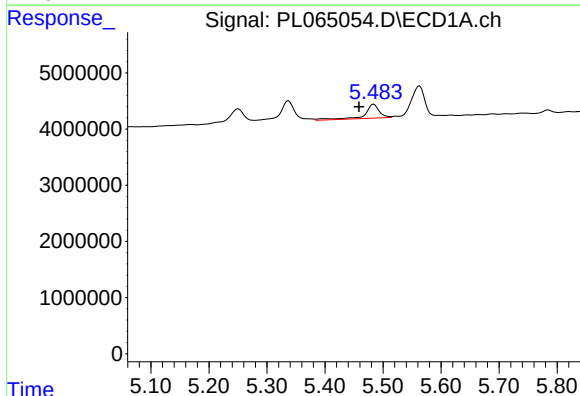


#9 Endosulfan I

R.T.: 5.484 min
Delta R.T.: 0.026 min
Response: 4334254
Conc: 1.35 ng/ml

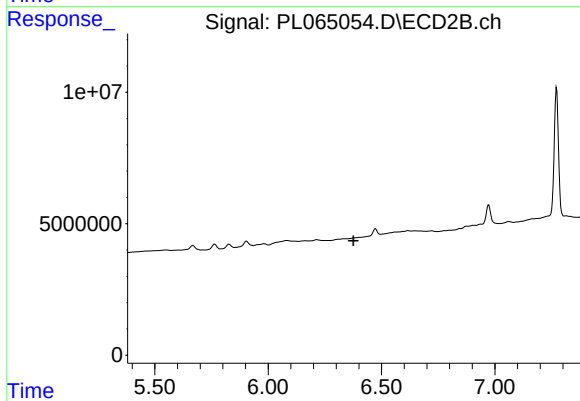

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

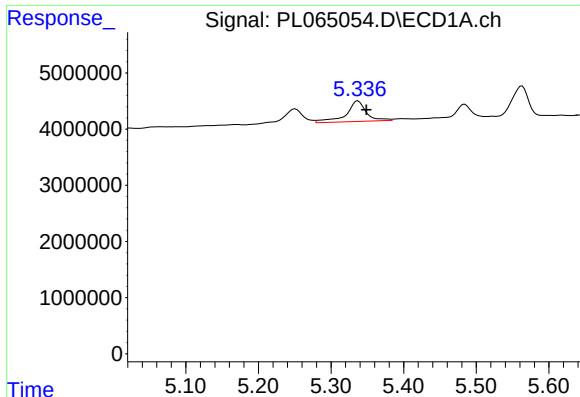

#10 gamma-Chlordane


R.T.: 5.337 min
Delta R.T.: -0.011 min
Response: 7017669
Conc: 2.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

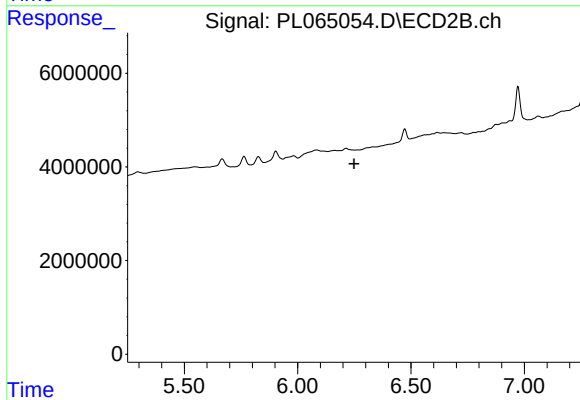


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

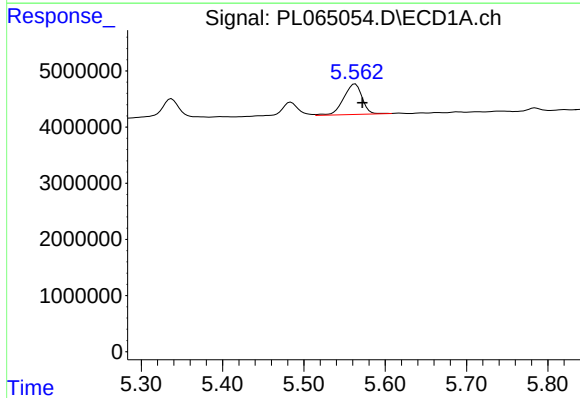


#12 4,4'-DDE

R.T.: 5.563 min
Delta R.T.: -0.009 min
Response: 8569462
Conc: 2.74 ng/ml

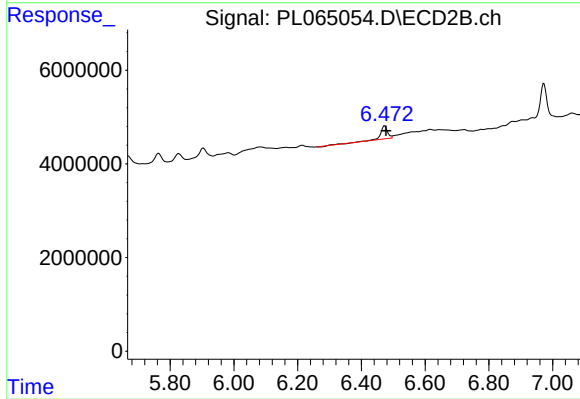

#12 4,4'-DDE


R.T.: 6.473 min
Delta R.T.: -0.005 min
Response: 3993710
Conc: 1.97 ng/ml

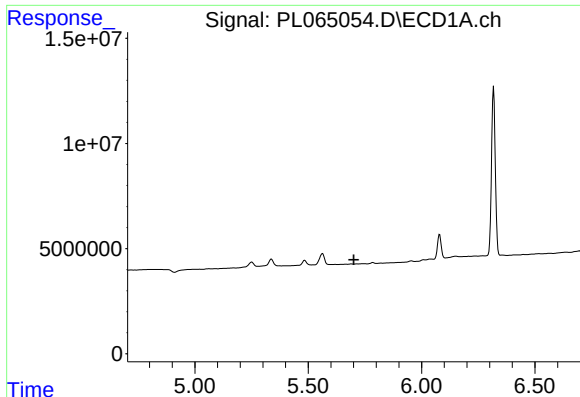

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

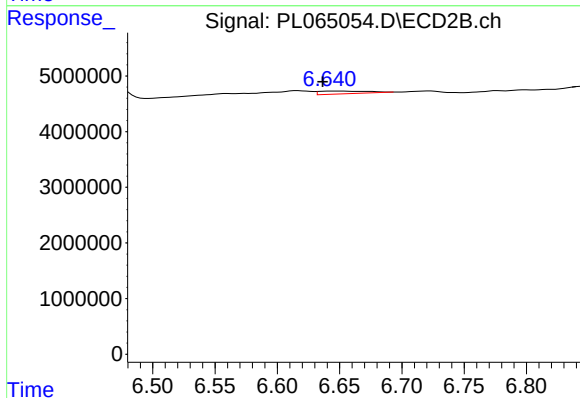


#13 Dieldrin

R.T.: 6.644 min
Delta R.T.: 0.008 min
Response: 1324202
Conc: 0.62 ng/ml

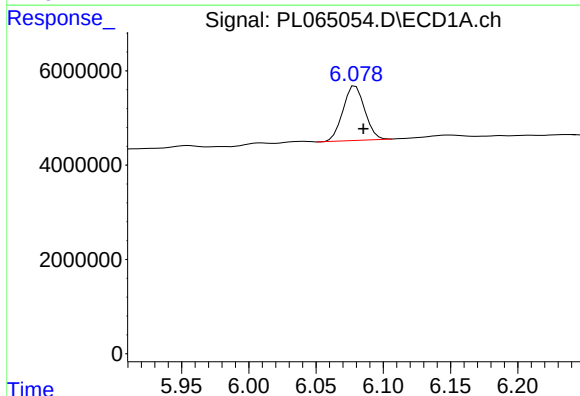


#16 4,4'-DDD

R.T.: 6.079 min
Delta R.T.: -0.006 min
Response: 12927065
Conc: 5.10 ng/ml

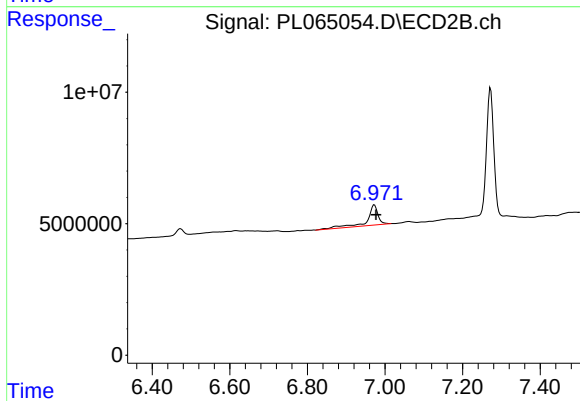

#16 4,4'-DDD


R.T.: 6.973 min
Delta R.T.: -0.005 min
Response: 15066990
Conc: 8.69 ng/ml

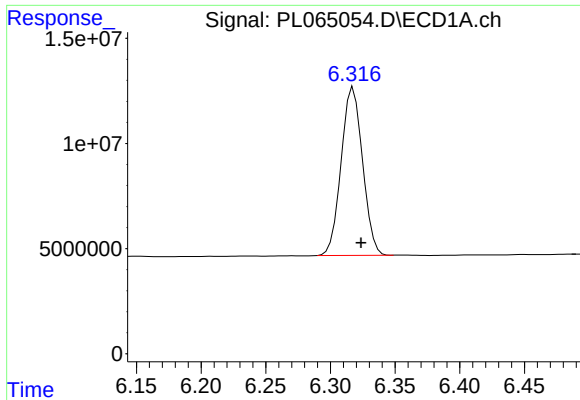

#17 4,4'-DDT


R.T.: 6.318 min
Delta R.T.: -0.006 min
Response: 91948052
Conc: 40.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

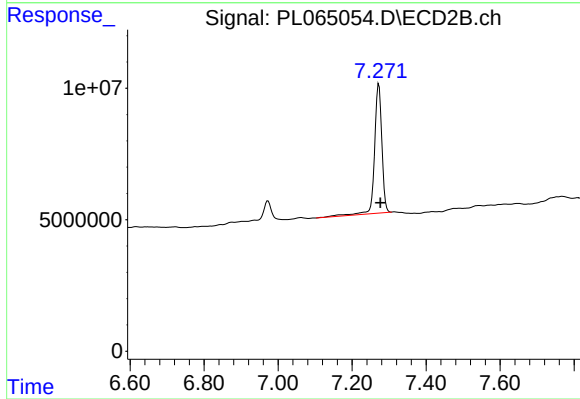


#17 4,4'-DDT

R.T.: 7.272 min
Delta R.T.: -0.004 min
Response: 67399123
Conc: 44.21 ng/ml

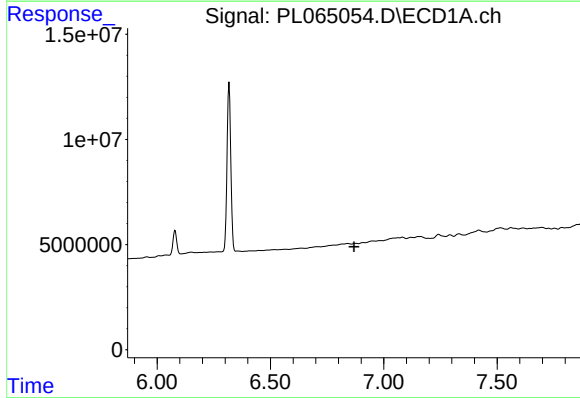


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.869 min
Response: 0
Conc: N.D.

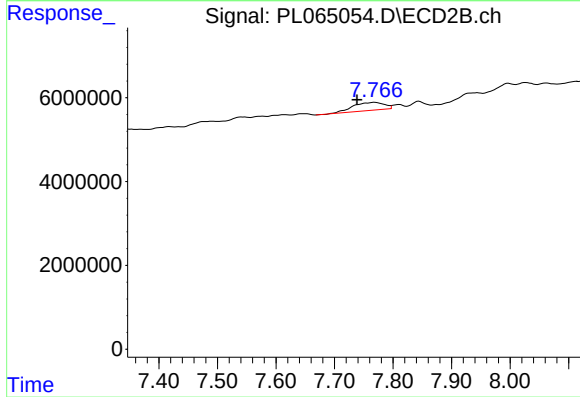

#20 Methoxychlor


R.T.: 7.769 min
Delta R.T.: 0.030 min
Response: 7012843
Conc: 7.76 ng/ml

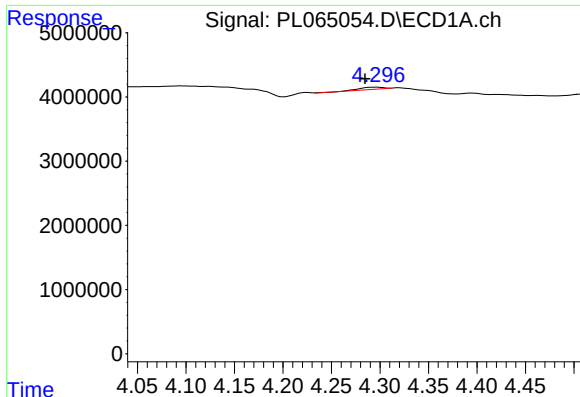

#23 Chlordane-1


R.T.: 4.296 min
Delta R.T.: 0.012 min
Response: 578603
Conc: 5.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

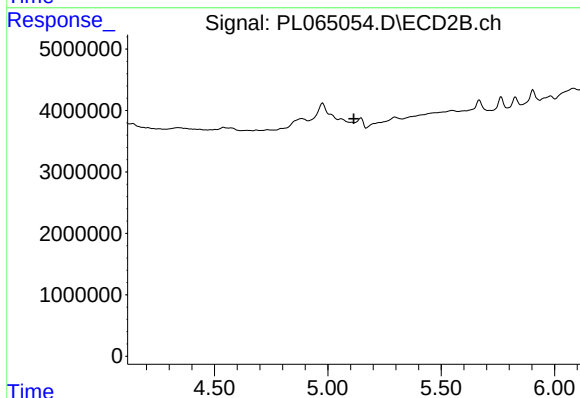


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

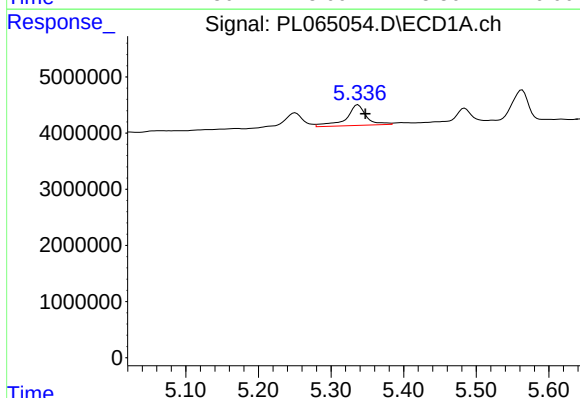


#25 Chlordane-3

R.T.: 5.337 min
Delta R.T.: -0.010 min
Response: 7017669
Conc: 21.36 ng/ml

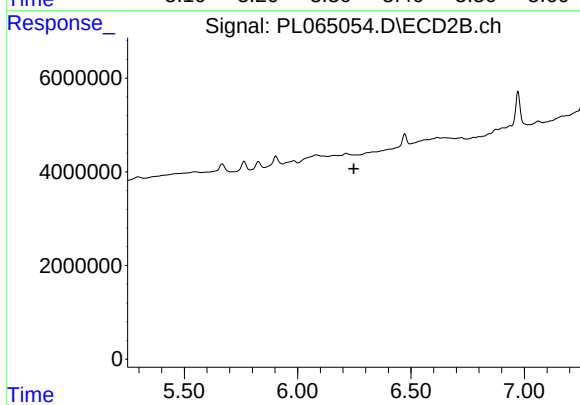

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

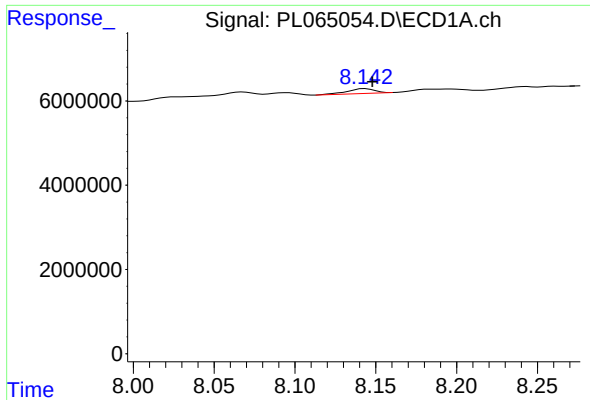

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.004 min
Response: 1369743
Conc: 0.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

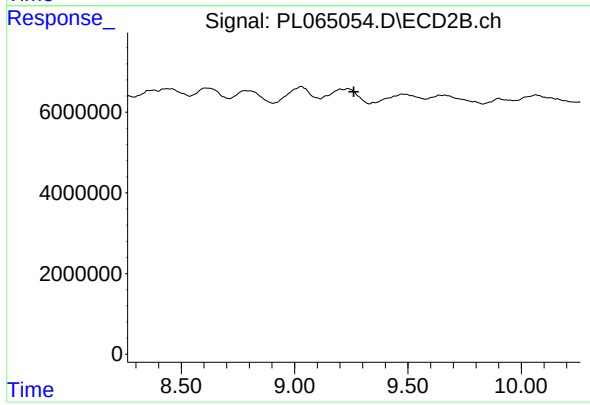

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.