

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
 Data File : PL065049.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 10:29
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:04:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.429	4.100	140.9E6	115.2E6	50.072	53.332
28)	SA Decachlor...	8.152	9.262	102.8E6	84783905	45.718	44.638
Target Compounds							
23)	Chlordane-1	4.289	5.114	47739145	44127217	419.955	502.427
24)	Chlordane-2	4.788	5.590	52006403	41660203	420.320	477.786
25)	Chlordane-3	5.352	6.247	143.3E6	150.5E6	435.950	492.156
26)	Chlordane-4	5.410	6.320	120.7E6	181.8E6	438.525	490.827
27)	Chlordane-5	6.238	7.140	42916801	23882537	424.168	423.195



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
Data File : PL065049.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 10:29
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:04:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

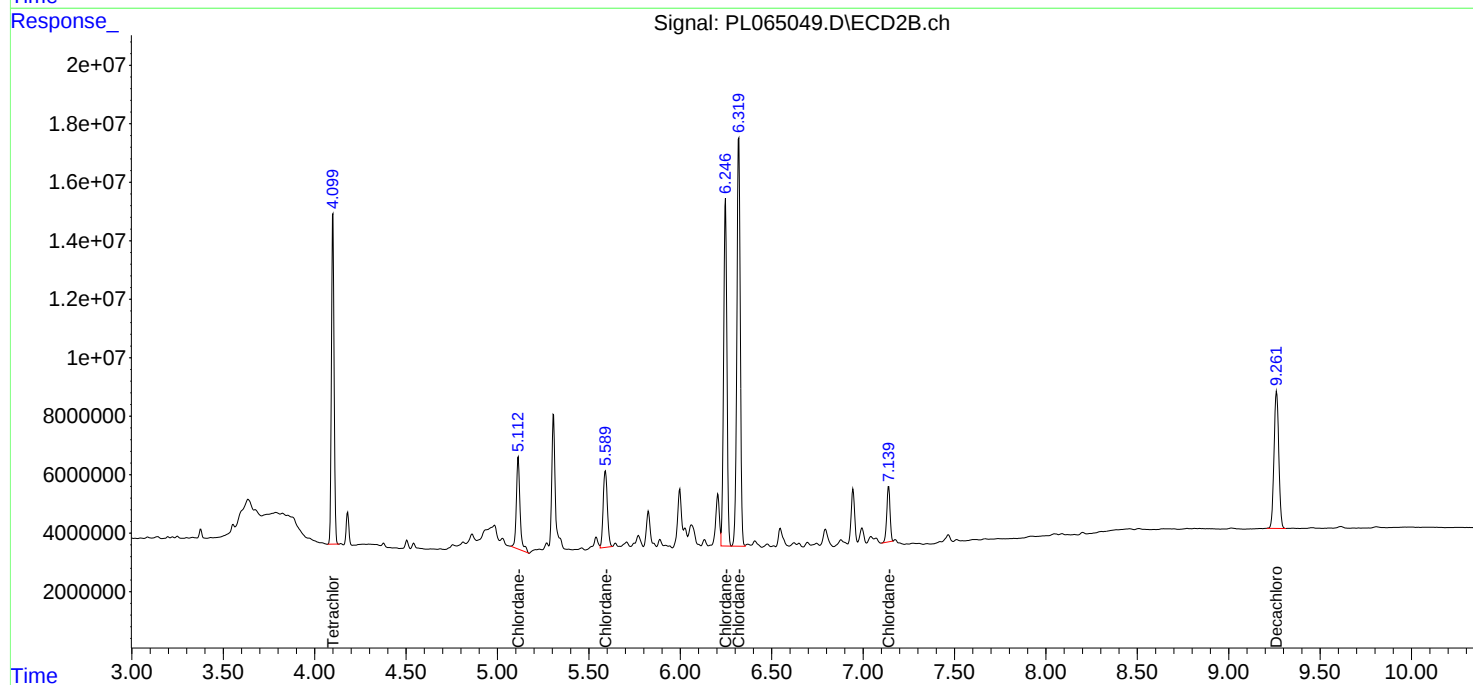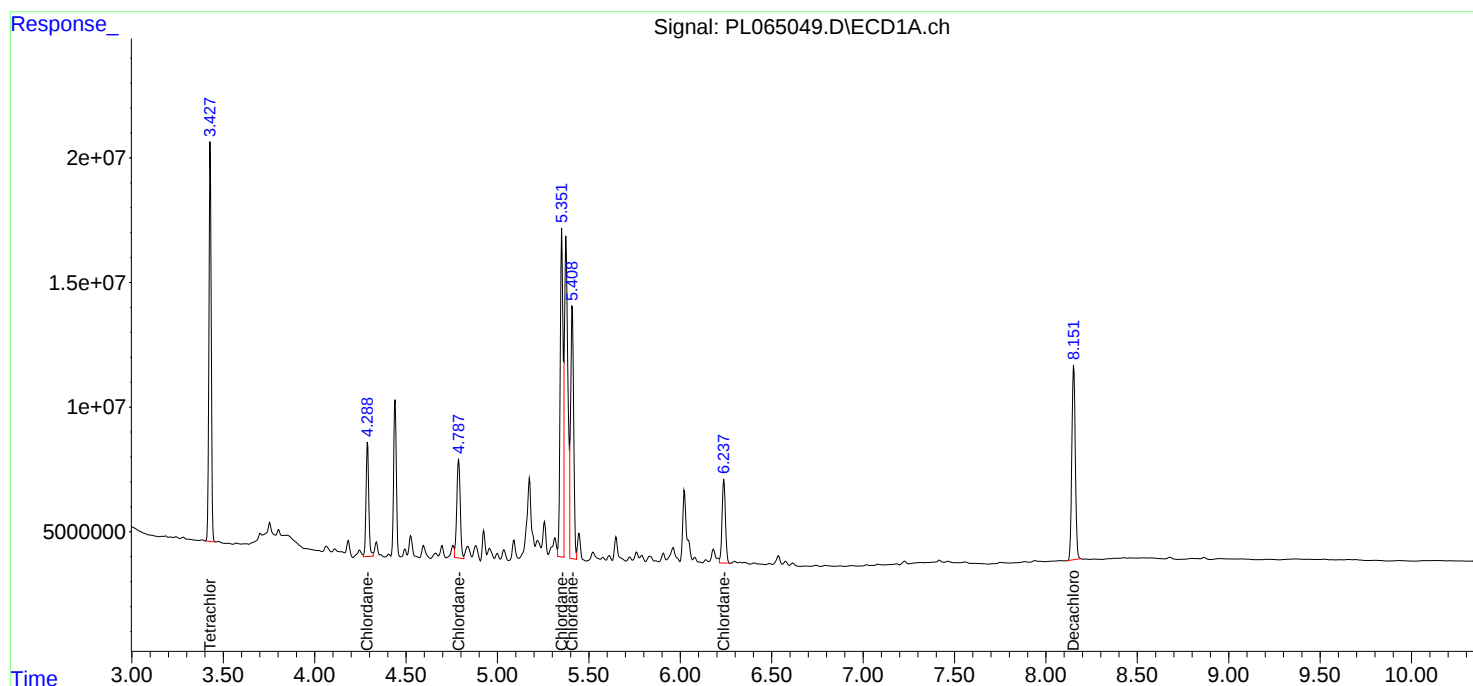


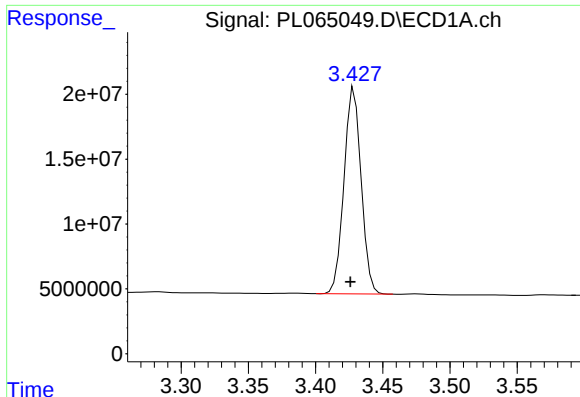

#1 Tetrachloro-m-xylene


R.T.: 3.429 min
Delta R.T.: 0.003 min
Response: 140878314
Conc: 50.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

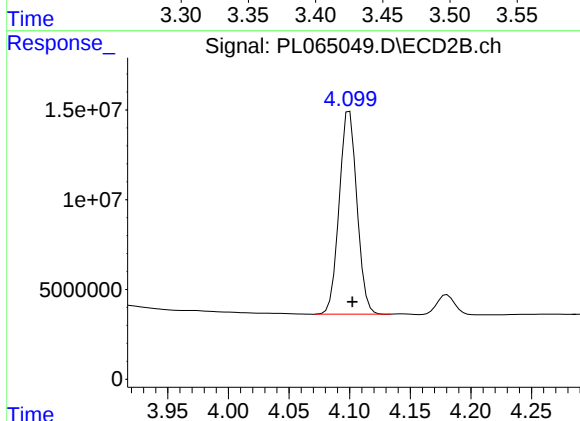


#1 Tetrachloro-m-xylene

R.T.: 4.100 min
Delta R.T.: -0.002 min
Response: 115208283
Conc: 53.33 ng/ml

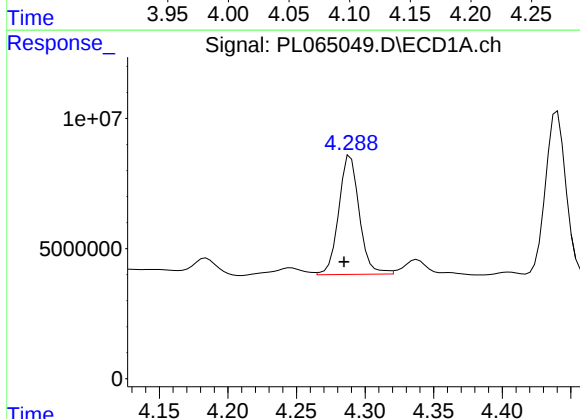


#23 Chlordane-1

R.T.: 4.289 min
Delta R.T.: 0.005 min
Response: 47739145
Conc: 419.96 ng/ml

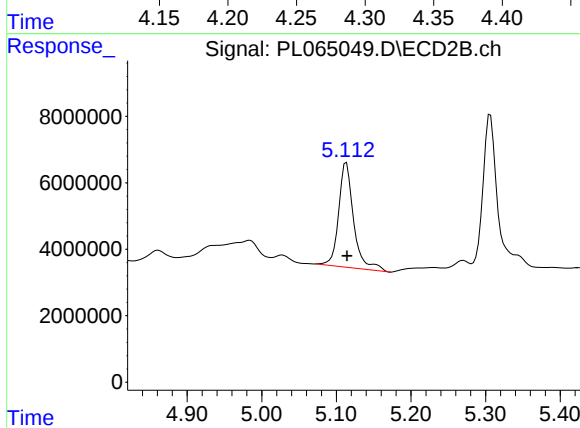

#23 Chlordane-1


R.T.: 5.114 min
Delta R.T.: 0.000 min
Response: 44127217
Conc: 502.43 ng/ml

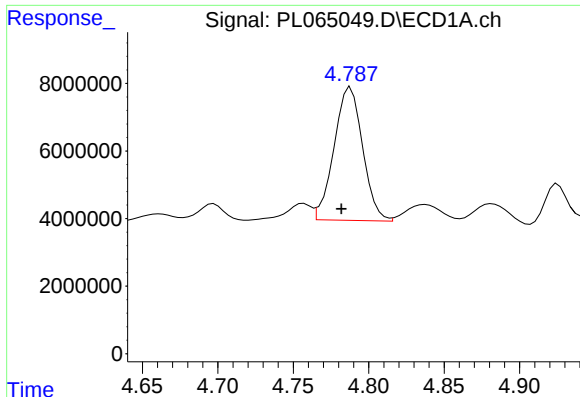

#24 Chlordane-2


R.T.: 4.788 min
Delta R.T.: 0.006 min
Response: 52006403
Conc: 420.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

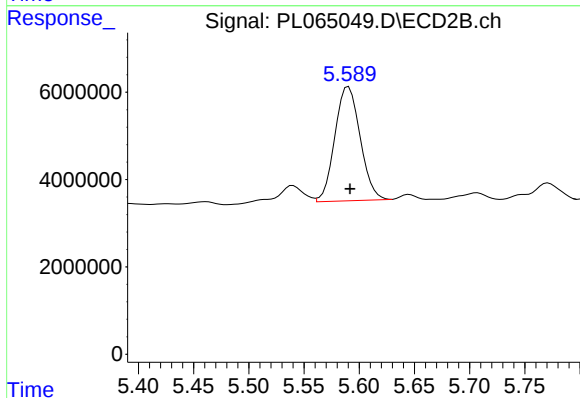


#24 Chlordane-2

R.T.: 5.590 min
Delta R.T.: -0.001 min
Response: 41660203
Conc: 477.79 ng/ml

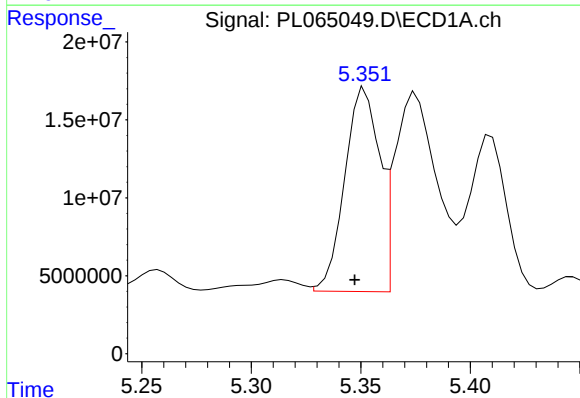


#25 Chlordane-3

R.T.: 5.352 min
Delta R.T.: 0.005 min
Response: 143259640
Conc: 435.95 ng/ml

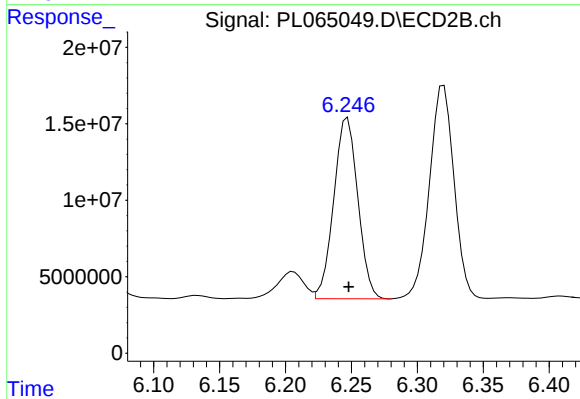

#25 Chlordane-3


R.T.: 6.247 min
Delta R.T.: 0.000 min
Response: 150480727
Conc: 492.16 ng/ml

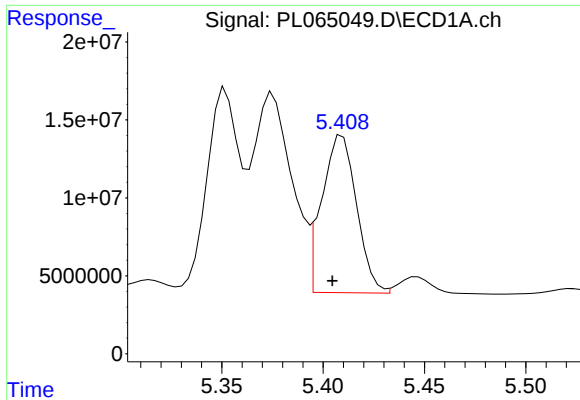

#26 Chlordane-4


R.T.: 5.410 min
Delta R.T.: 0.005 min
Response: 120658337
Conc: 438.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

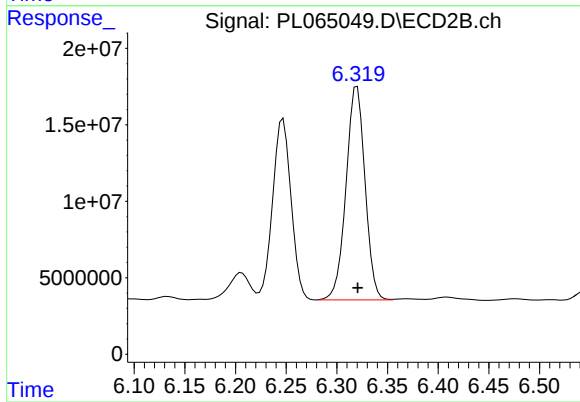


#26 Chlordane-4

R.T.: 6.320 min
Delta R.T.: 0.000 min
Response: 181840406
Conc: 490.83 ng/ml

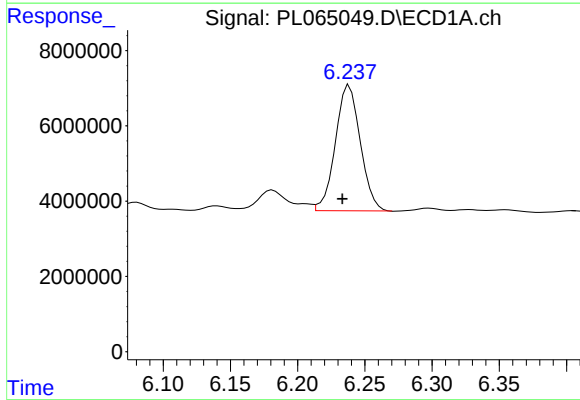


#27 Chlordane-5

R.T.: 6.238 min
Delta R.T.: 0.005 min
Response: 42916801
Conc: 424.17 ng/ml

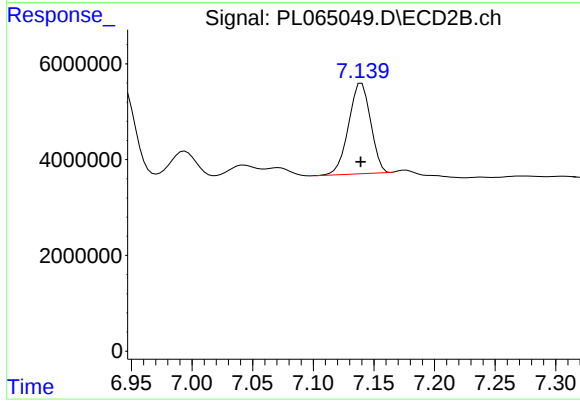

#27 Chlordane-5


R.T.: 7.140 min
Delta R.T.: 0.000 min
Response: 23882537
Conc: 423.20 ng/ml

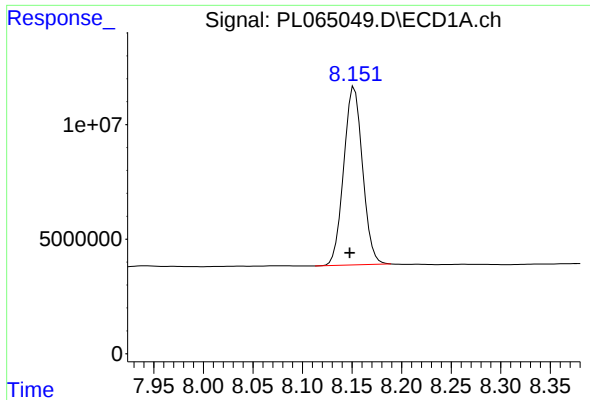

#28 Decachlorobiphenyl

R.T.: 8.152 min
Delta R.T.: 0.005 min
Response: 102810741
Conc: 45.72 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

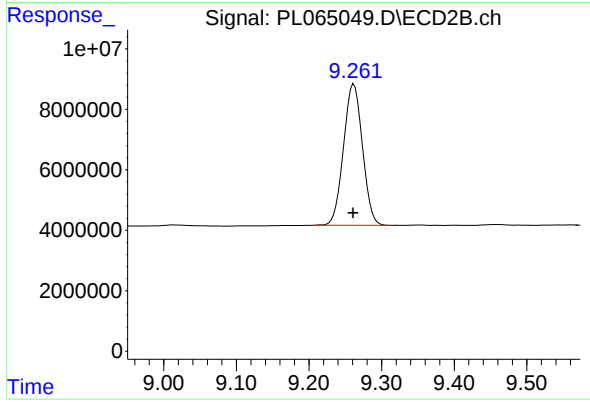

#28 Decachlorobiphenyl

R.T.: 9.262 min
Delta R.T.: 0.001 min
Response: 84783905
Conc: 44.64 ng/ml