

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
 Data File : PL065051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 11:02
 Operator : AR\AJ
 Sample : M1520-02RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NCQ-632RE

Manual Integrations
 APPROVED

Ankita
 3/5/2021 8:59:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:04:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.424	4.089	187.2E6	96491087	66.546m	44.668m#
28)	SA Decachlor...	8.148	9.255	23184476	21946848	10.310m	11.555

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
Data File : PL065051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 11:02
Operator : AR\AJ
Sample : M1520-02RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NCQ-632RE


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:04:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

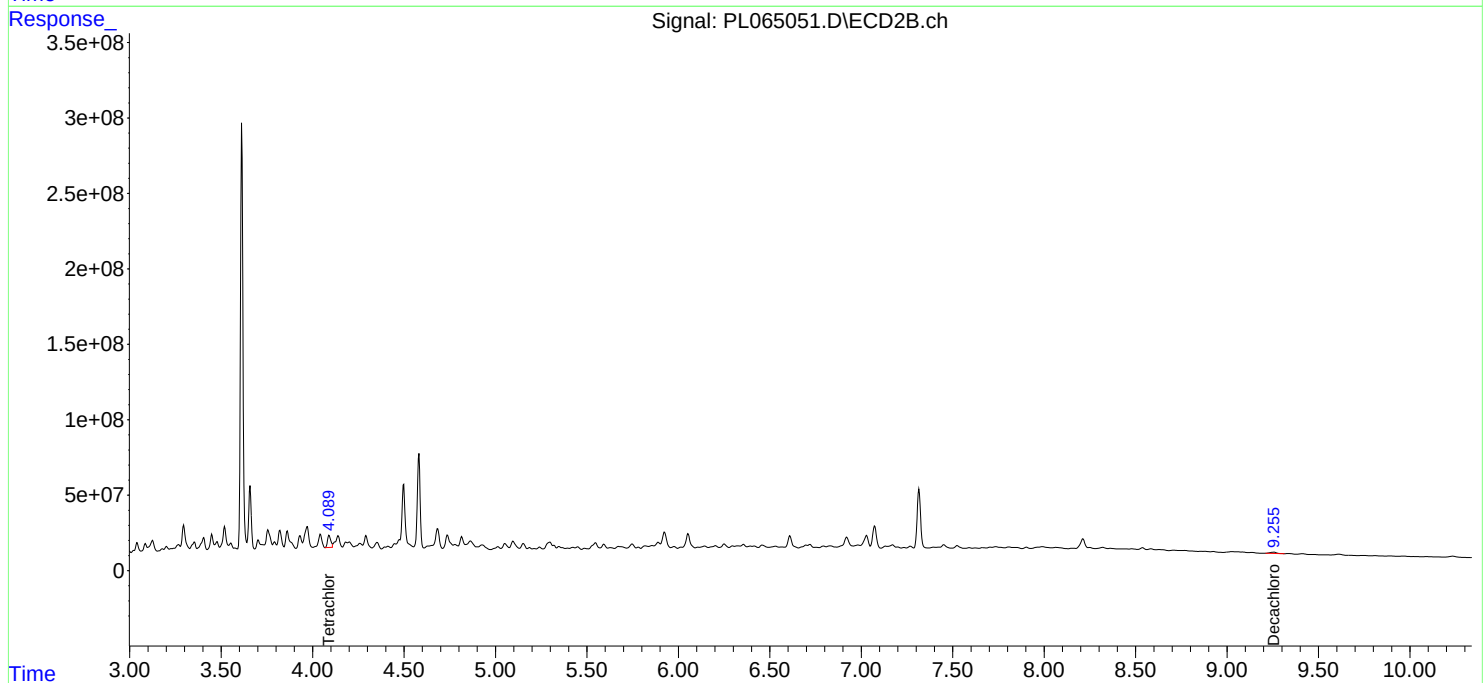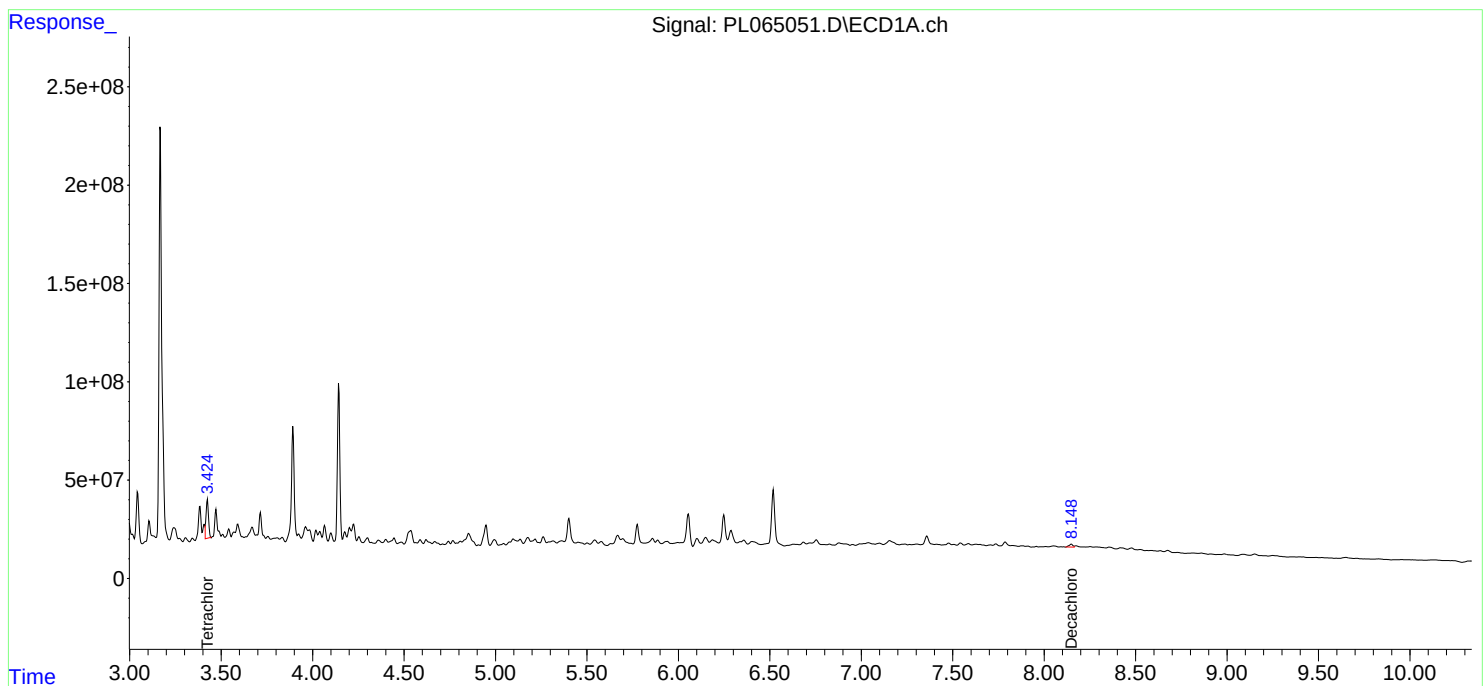

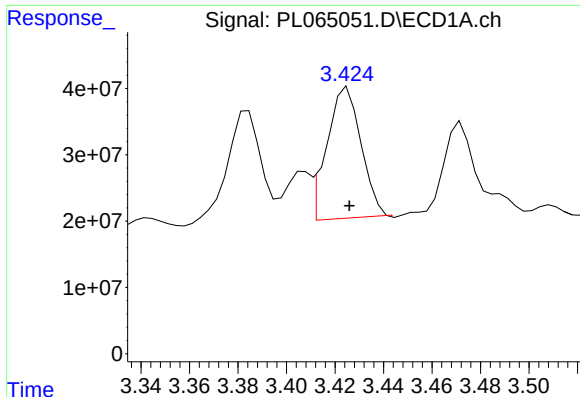


#1 Tetrachloro-m-xylene

R.T.: 3.424 min
Delta R.T.: -0.002 min
Response: 187227215
Conc: 66.55 ng/ml m

Instrument :
ECD_L
ClientSampleId :
NCQ-632RE


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:53 AM

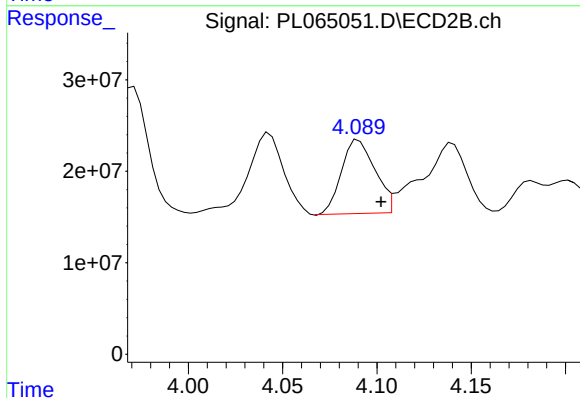


#1 Tetrachloro-m-xylene

R.T.: 4.089 min
Delta R.T.: -0.013 min
Response: 96491087
Conc: 44.67 ng/ml m

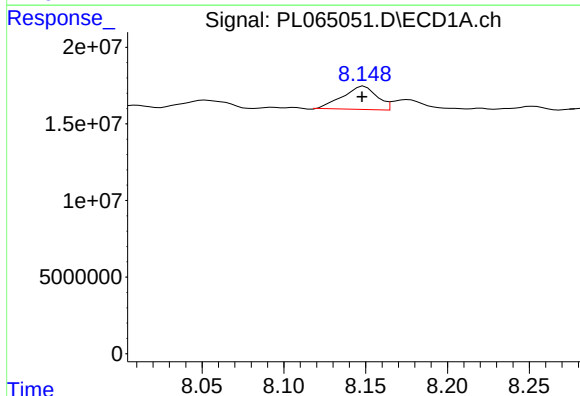

#28 Decachlorobiphenyl

R.T.: 8.148 min
Delta R.T.: 0.000 min
Response: 23184476
Conc: 10.31 ng/ml m

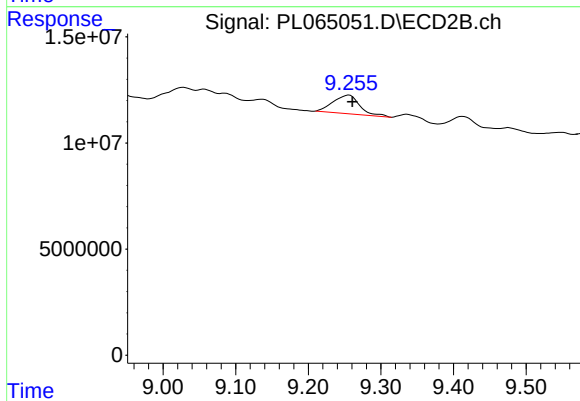

#28 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.006 min
Response: 21946848
Conc: 11.55 ng/ml