

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
 Data File : PL065052.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 11:17
 Operator : AR\AJ
 Sample : M1521-05RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OB-722RE

Manual Integrations
 APPROVED

Ankita
 3/5/2021 8:59:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:05:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.089	106.2E6	77302434	37.750m	35.785m
28)	SA Decachlor...	8.143	9.255	22197492	17947643	9.871m	9.449m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
Data File : PL065052.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 11:17
Operator : AR\AJ
Sample : M1521-05RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OB-722RE


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:05:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

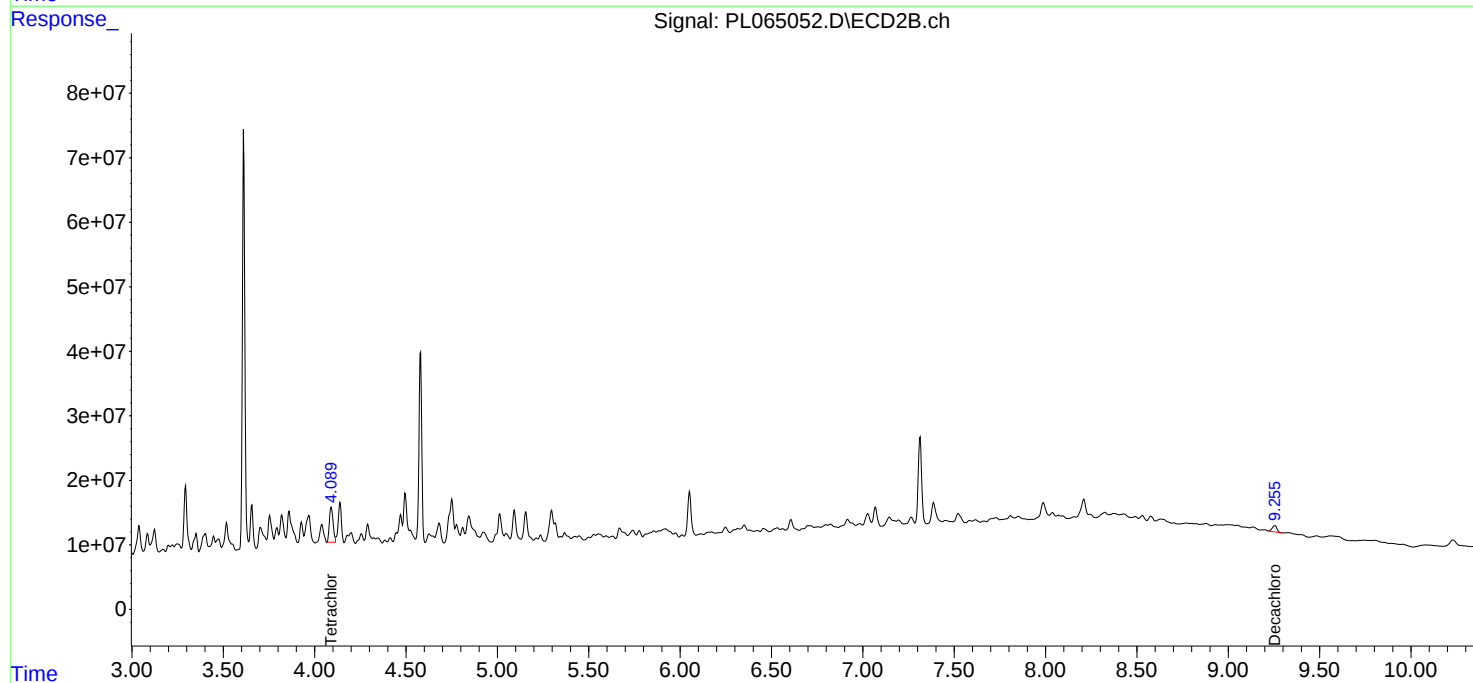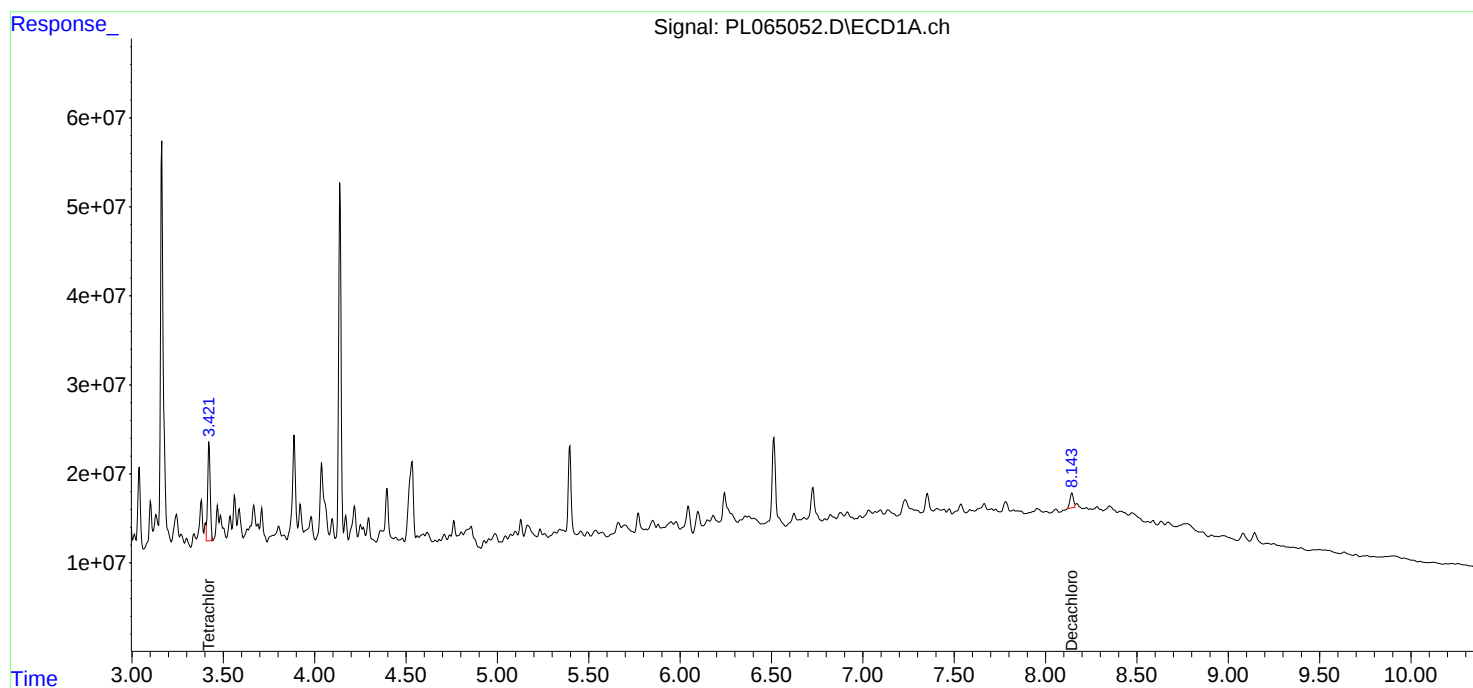

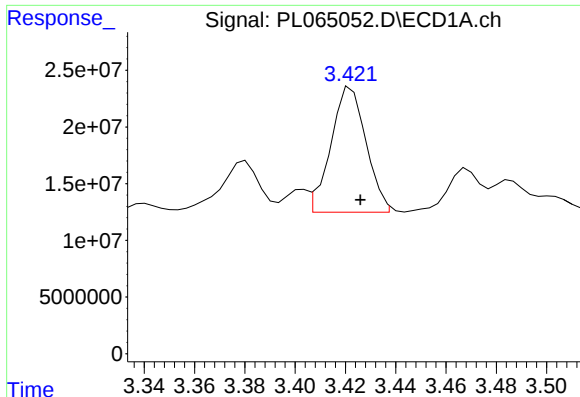


#1 Tetrachloro-m-xylene

R.T.: 3.421 min
Delta R.T.: -0.005 min
Response: 106209786
Conc: 37.75 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OB-722RE


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:54 AM

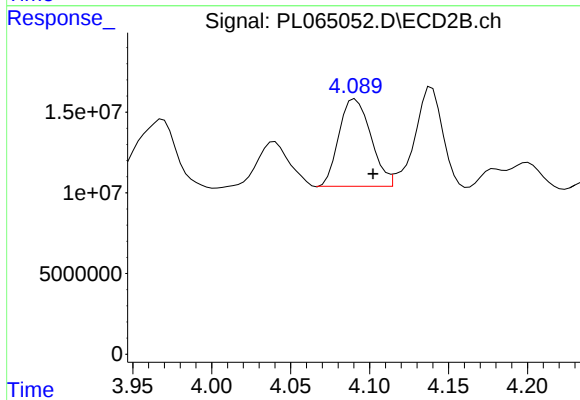


#1 Tetrachloro-m-xylene

R.T.: 4.089 min
Delta R.T.: -0.013 min
Response: 77302434
Conc: 35.78 ng/ml m

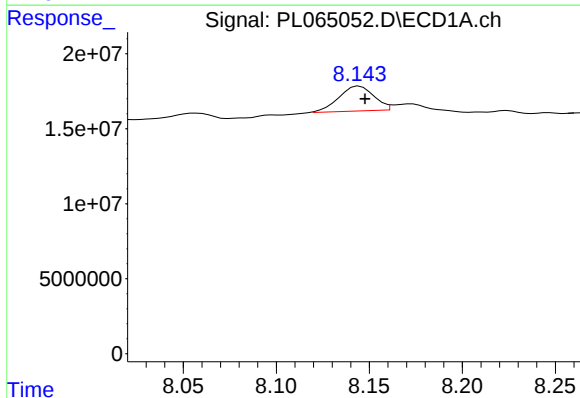

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: -0.004 min
Response: 22197492
Conc: 9.87 ng/ml m

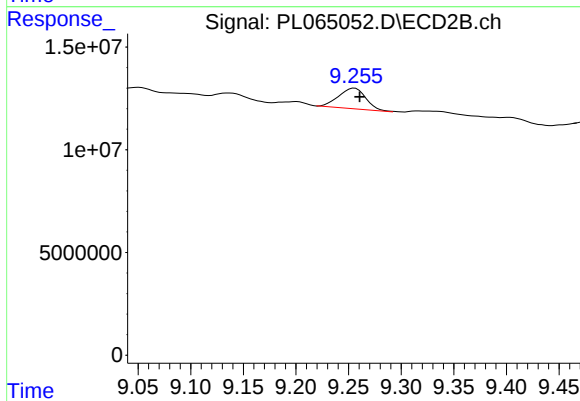

#28 Decachlorobiphenyl

R.T.: 9.255 min
Delta R.T.: -0.006 min
Response: 17947643
Conc: 9.45 ng/ml m