

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
 Data File : PL065054.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 11:45
 Operator : AR\AJ
 Sample : M1539-01DL2 100X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JC-02-030221DL2

Manual Integrations
 APPROVED

Ankita
 3/5/2021 8:59:58 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 16:05:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
12) B	4,4'-DDE	5.562	6.472	7763753	2825398	2.481m 1.393m#
16) A	4,4'-DDD	6.079	6.971	12927065	10509423	5.104 6.062m
17) MA	4,4'-DDT	6.318	7.271	91948052	63300229	40.776 41.518m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030421\
Data File : PL065054.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 11:45
Operator : AR\AJ
Sample : M1539-01DL2 100X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
JC-02-030221DL2


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:58 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 16:05:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

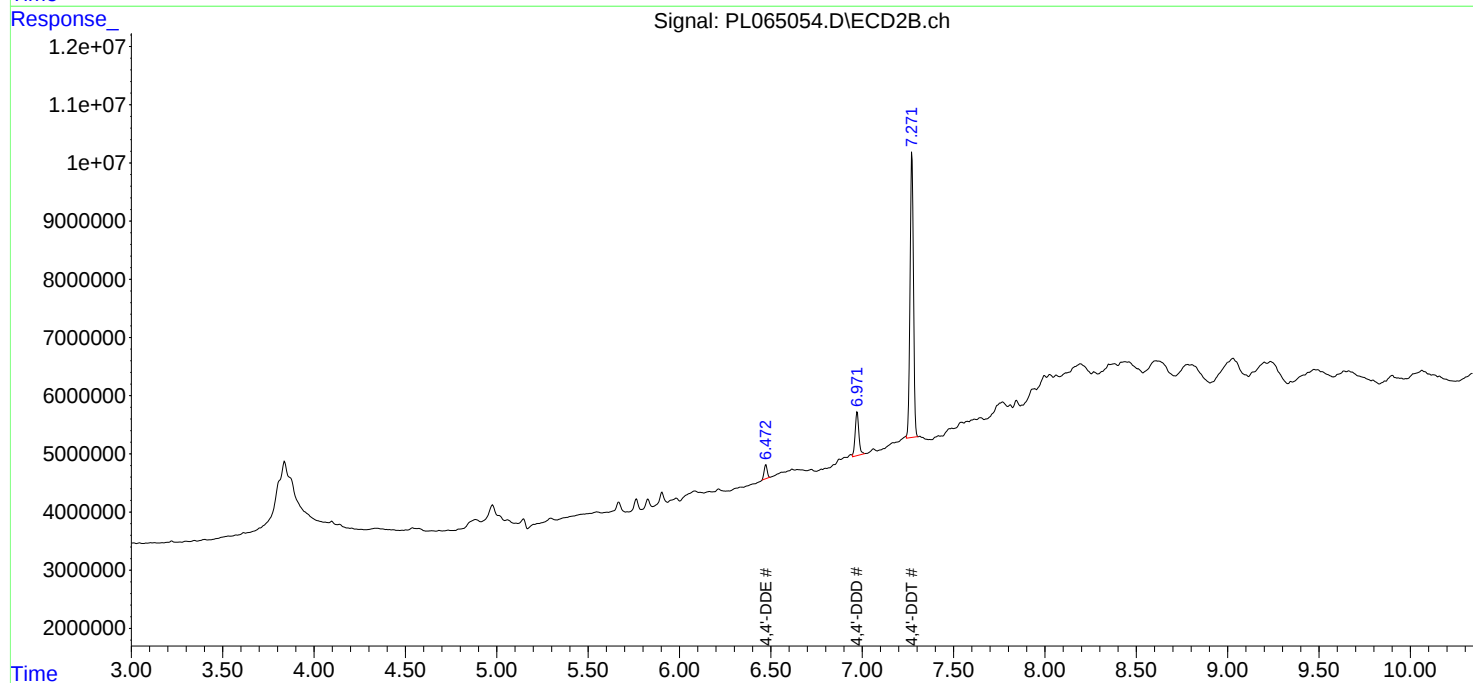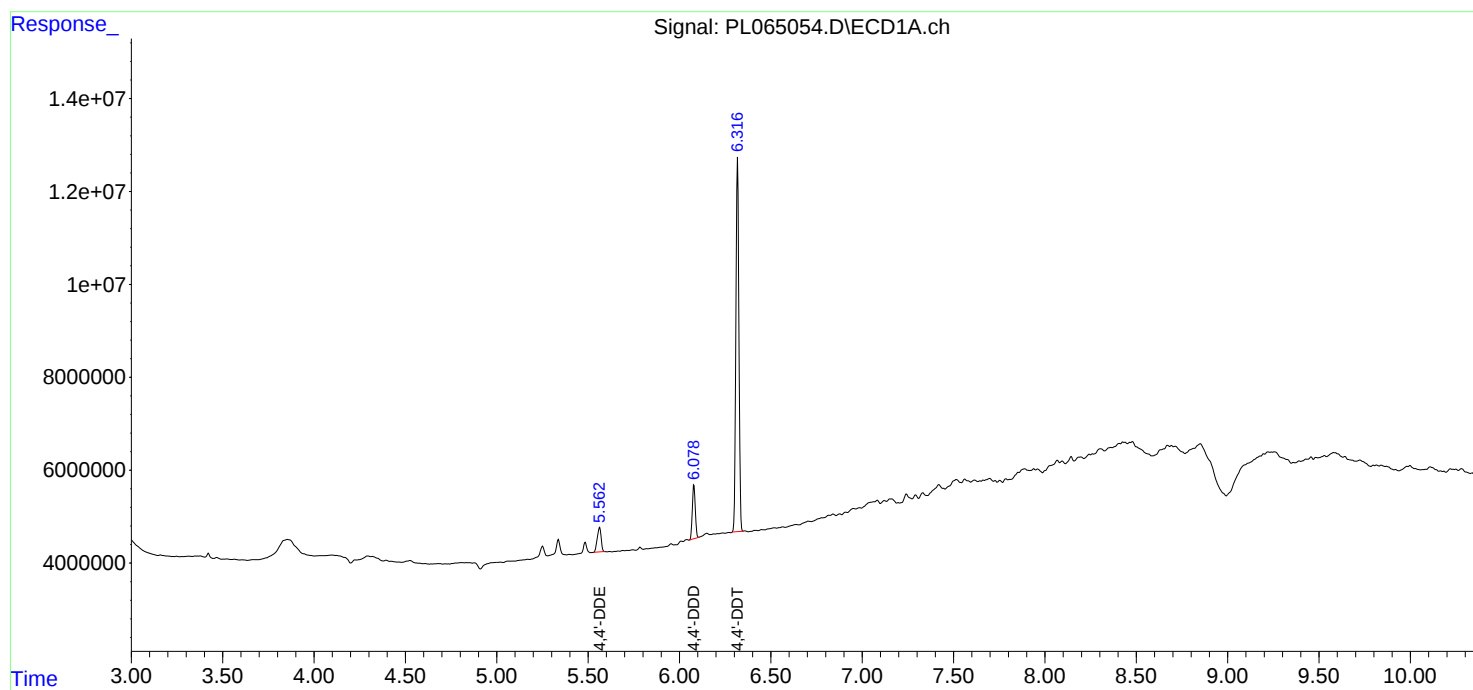

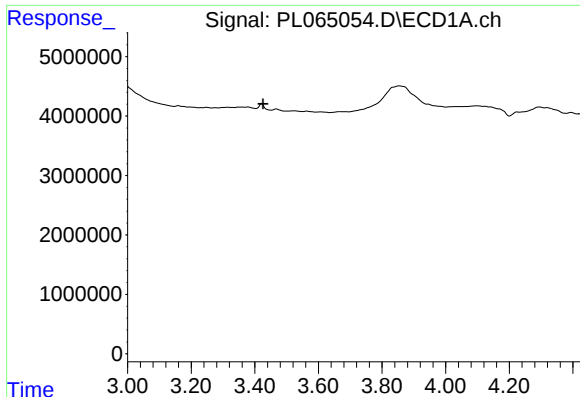


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.426 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-030221DL2


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:58 AM

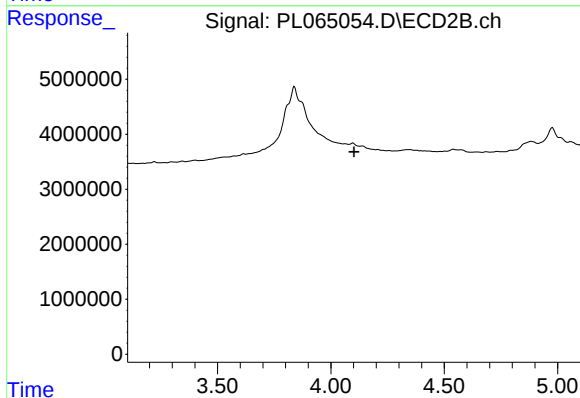


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.102 min
Response: 0
Conc: N.D.

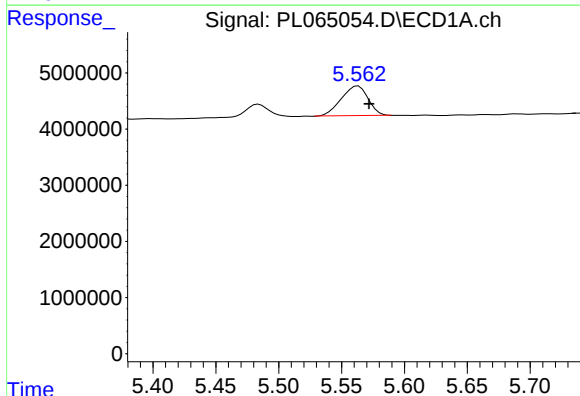


#12 4,4'-DDE

R.T.: 5.562 min
Delta R.T.: -0.010 min
Response: 7763753
Conc: 2.48 ng/ml m

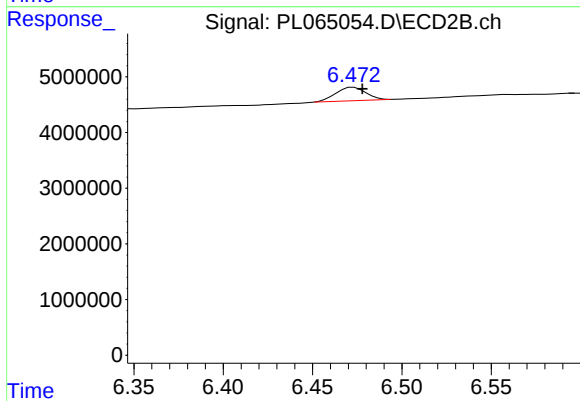

#12 4,4'-DDE

R.T.: 6.472 min
Delta R.T.: -0.006 min
Response: 2825398
Conc: 1.39 ng/ml m

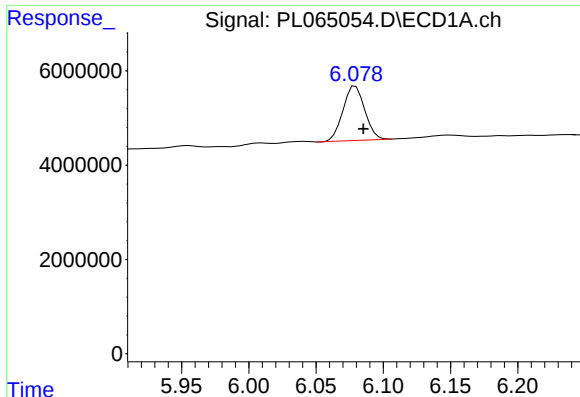


#16 4,4'-DDD

R.T.: 6.079 min
Delta R.T.: -0.006 min
Response: 12927065
Conc: 5.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
JC-02-030221DL2


Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:58 AM

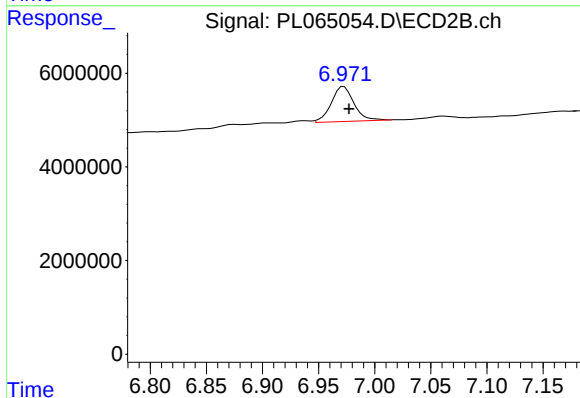


#16 4,4'-DDD

R.T.: 6.971 min
Delta R.T.: -0.006 min
Response: 10509423
Conc: 6.06 ng/ml m

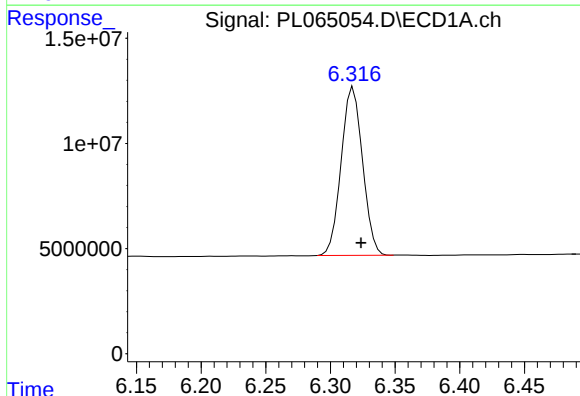


#17 4,4'-DDT

R.T.: 6.318 min
Delta R.T.: -0.006 min
Response: 91948052
Conc: 40.78 ng/ml

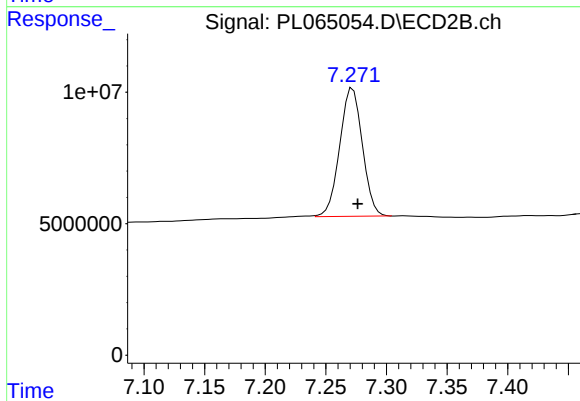

#17 4,4'-DDT

R.T.: 7.271 min
Delta R.T.: -0.006 min
Response: 63300229
Conc: 41.52 ng/ml m

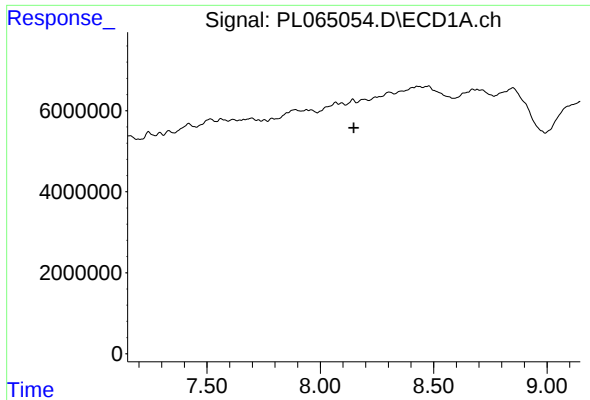


#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 8.148 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JC-02-030221DL2

Manual Integrations
APPROVED

Ankita
3/5/2021 8:59:58 AM

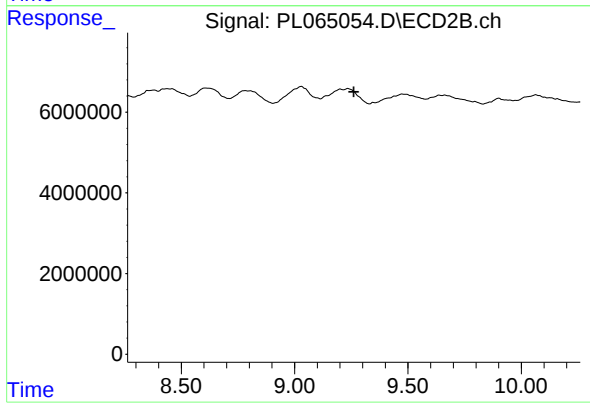

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T.: 9.261 min
Response: 0
Conc: N.D.