

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030424\
 Data File : PL088396.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2024 14:24
 Operator : AR\AJ
 Sample : P1669-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-14

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 03/05/2024
 Supervised By :Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:32:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.635	2.854	45145476	22603519	16.436	16.116
28) SA Decachlor...	9.298	8.080	35249518	21023238	18.303	16.511
Target Compounds						
20) A Methoxychlor	7.649	6.759	1614227	802443	1.219	1.024m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030424\
Data File : PL088396.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2024 14:24
Operator : AR\AJ
Sample : P1669-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-14


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/05/2024
Supervised By : Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:32:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

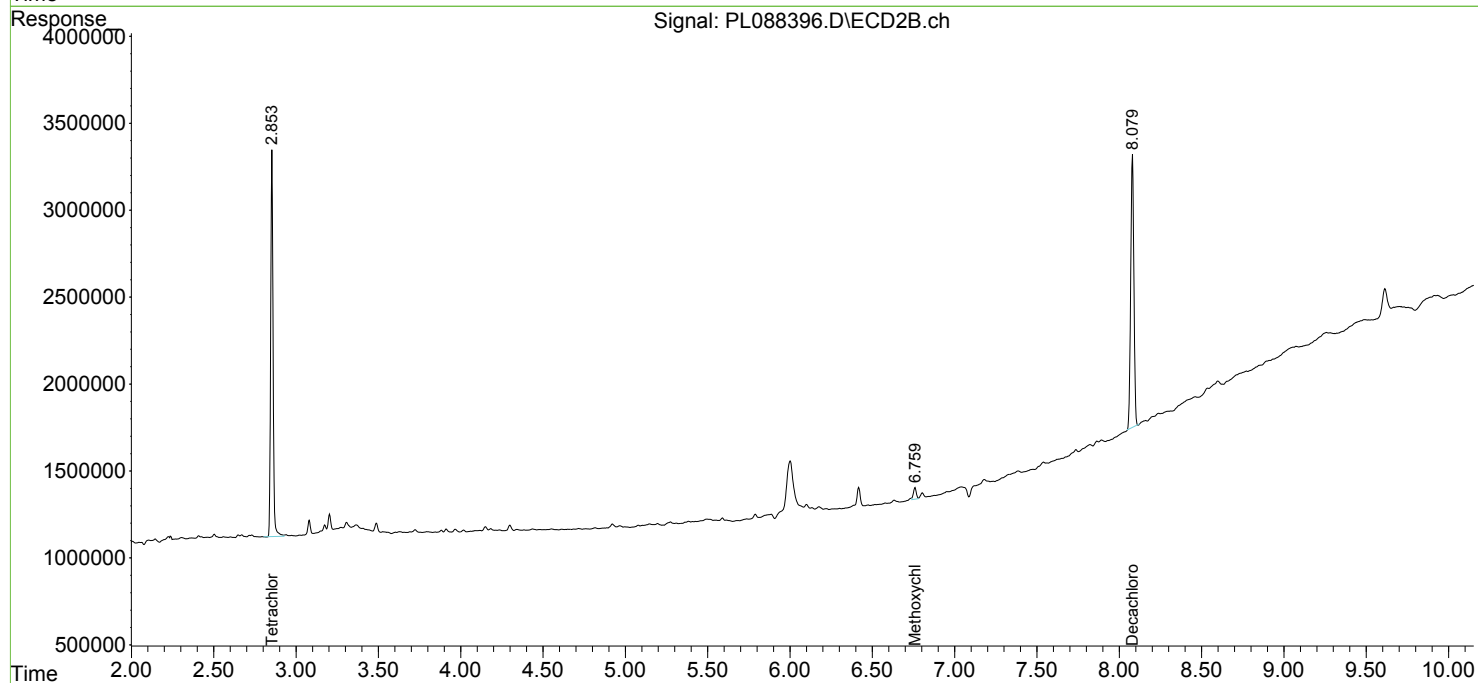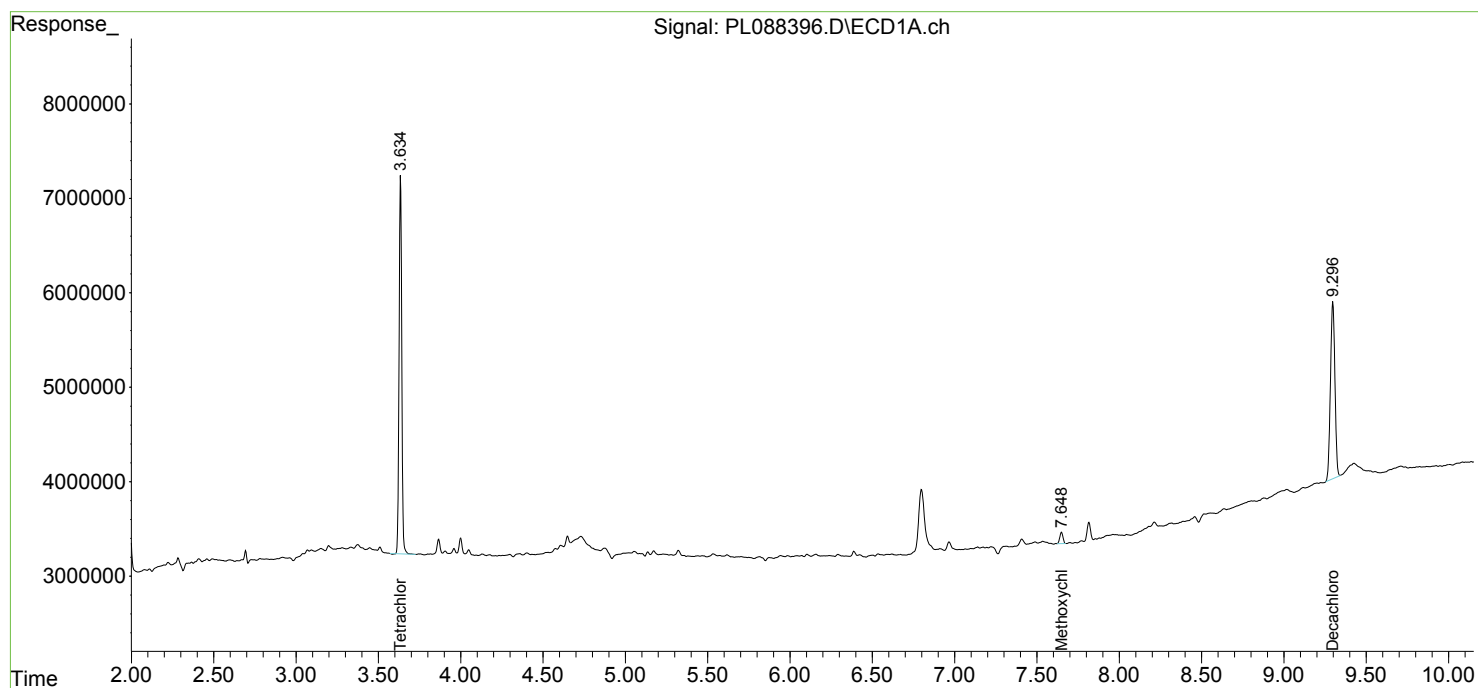

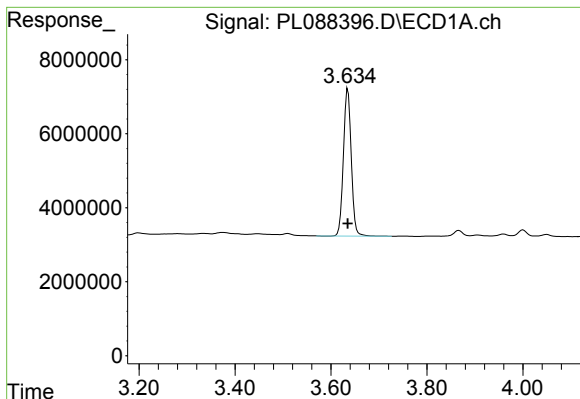


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 45145476
Conc: 16.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/05/2024
Supervised By :Ankita Jodhani 03/05/2024

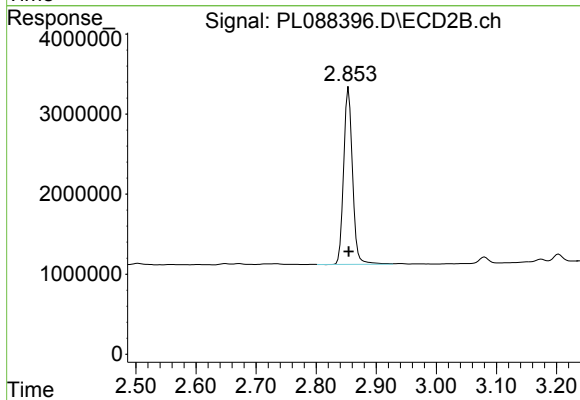


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 22603519
Conc: 16.12 ng/ml

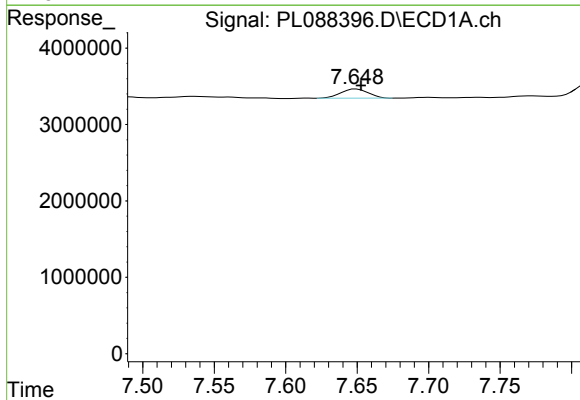


#20 Methoxychlor

R.T.: 7.649 min
Delta R.T.: -0.003 min
Response: 1614227
Conc: 1.22 ng/ml

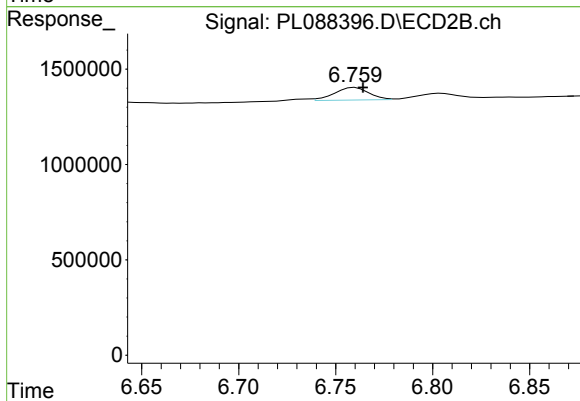

#20 Methoxychlor

R.T.: 6.759 min
Delta R.T.: -0.005 min
Response: 802443
Conc: 1.02 ng/ml m

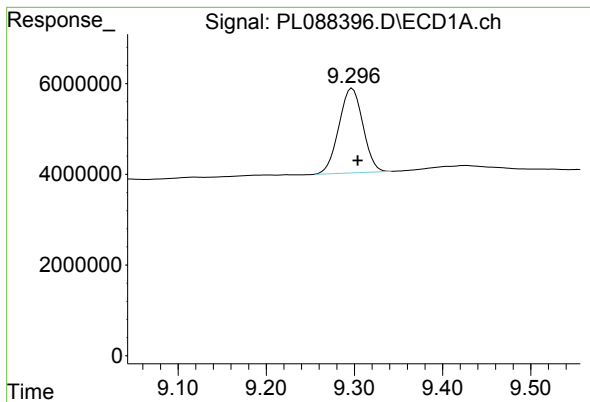


#28 Decachlorobiphenyl

R.T.: 9.298 min
Delta R.T.: -0.006 min
Response: 35249518
Conc: 18.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-14

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/05/2024
Supervised By :Ankita Jodhani 03/05/2024

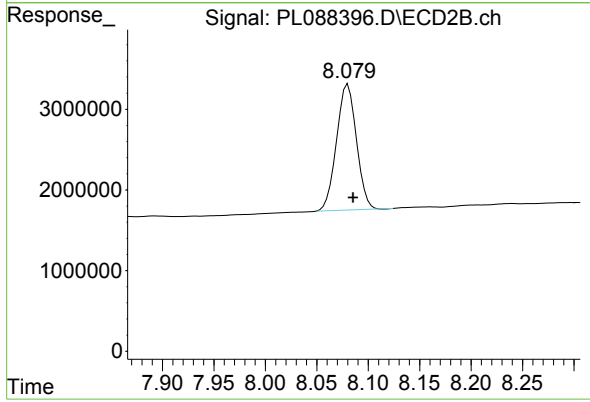

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: -0.005 min
Response: 21023238
Conc: 16.51 ng/ml