

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030424\
 Data File : PL088400.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2024 15:19
 Operator : AR\AJ
 Sample : P1669-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-6

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/05/2024
 Supervised By : Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:33:09 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.635	2.853	32510705	16037281	11.836	11.435m
28) SA Decachlor...	9.296	8.080	24658723	15028417	12.804	11.803

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030424\
Data File : PL088400.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2024 15:19
Operator : AR\AJ
Sample : P1669-09
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/05/2024
Supervised By : Ankita Jodhani 03/05/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:33:09 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

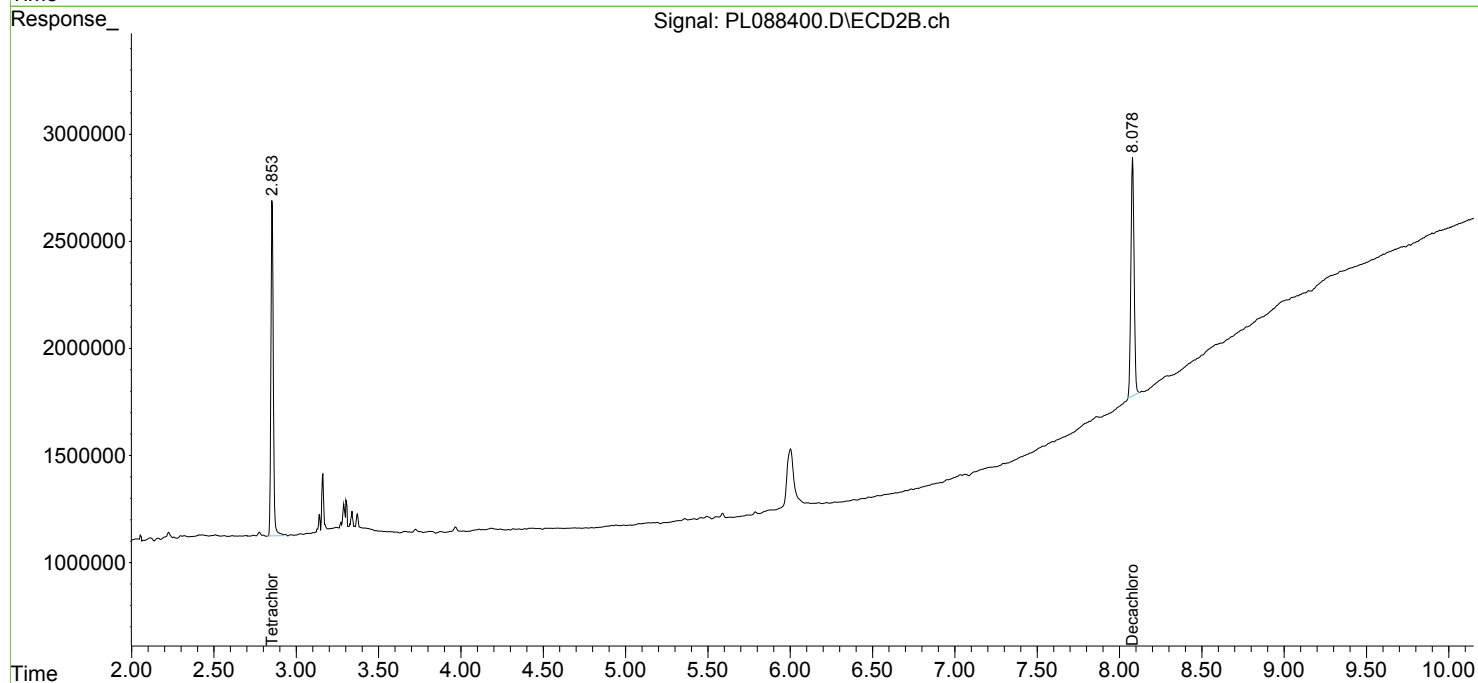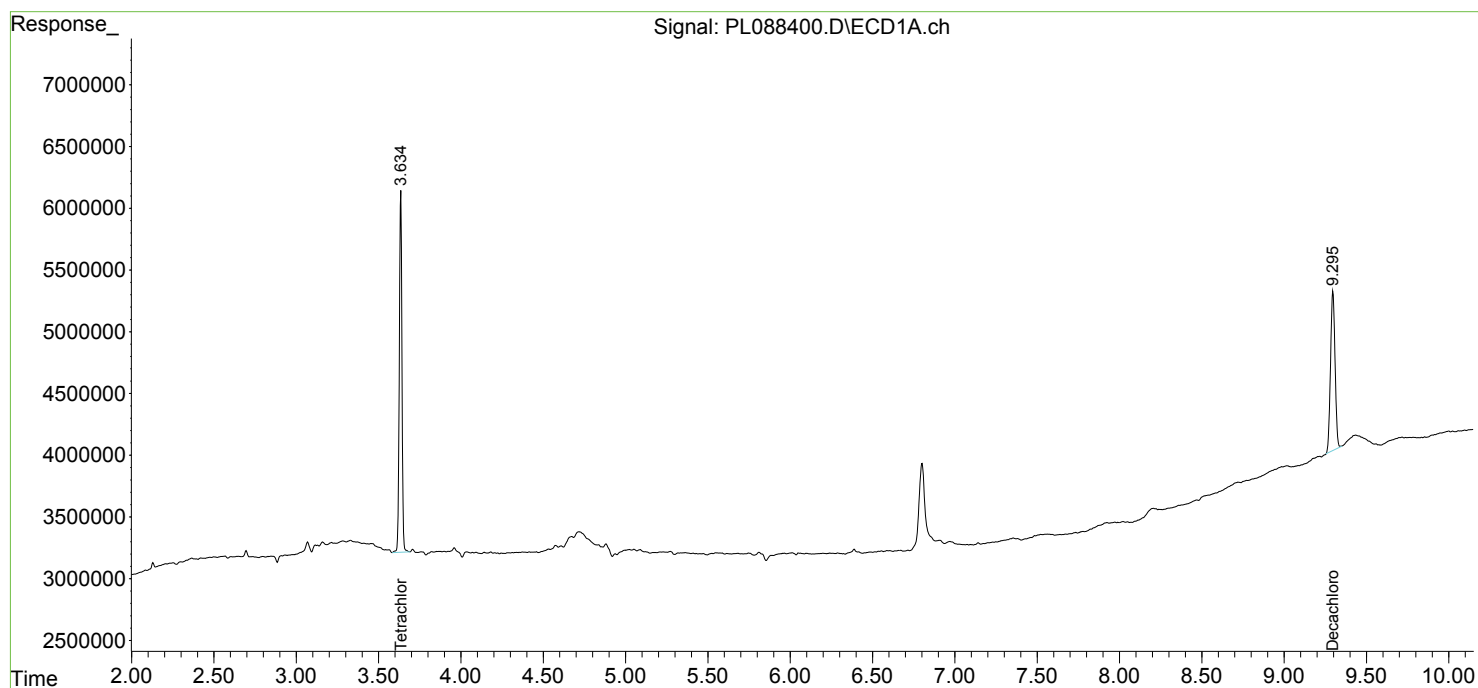

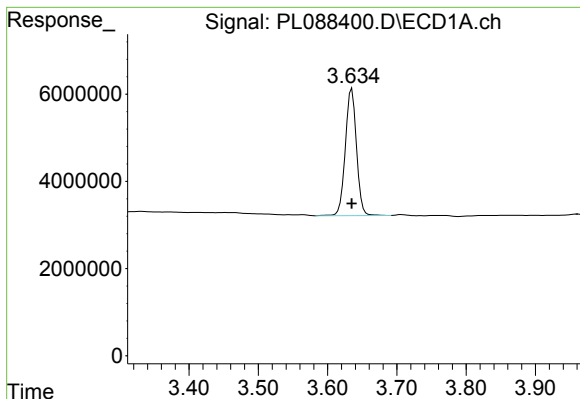


#1 Tetrachloro-m-xylene

R.T.: 3.635 min
Delta R.T.: 0.000 min
Response: 32510705
Conc: 11.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-6


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/05/2024
Supervised By :Ankita Jodhani 03/05/2024

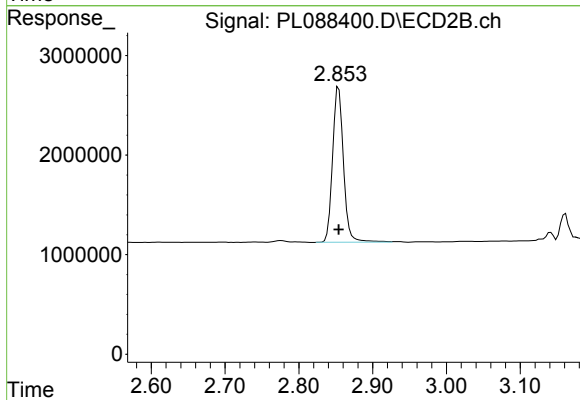


#1 Tetrachloro-m-xylene

R.T.: 2.853 min
Delta R.T.: -0.001 min
Response: 16037281
Conc: 11.43 ng/ml m

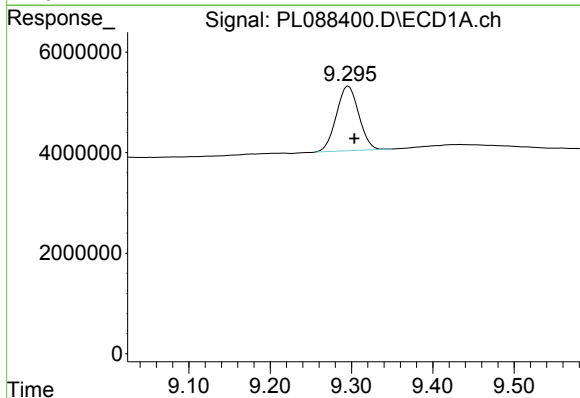

#28 Decachlorobiphenyl

R.T.: 9.296 min
Delta R.T.: -0.007 min
Response: 24658723
Conc: 12.80 ng/ml

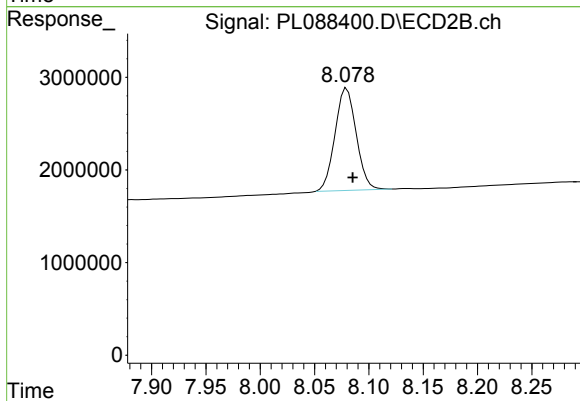

#28 Decachlorobiphenyl

R.T.: 8.080 min
Delta R.T.: -0.005 min
Response: 15028417
Conc: 11.80 ng/ml