

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030425\
 Data File : PL094479.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2025 13:57
 Operator : AR\AJ
 Sample : Q1475-01 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TR-04-02282025

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/05/2025
 Supervised By : Ankita Jodhani 03/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 01:30:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.770	6277172	8332462	2.472m	2.611m
28) SA Decachlor...	9.049	7.905	5022707	7057858	2.361m	1.835m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030425\
Data File : PL094479.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2025 13:57
Operator : AR\AJ
Sample : Q1475-01 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
TR-04-02282025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/05/2025
Supervised By : Ankita Jodhani 03/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 01:30:03 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

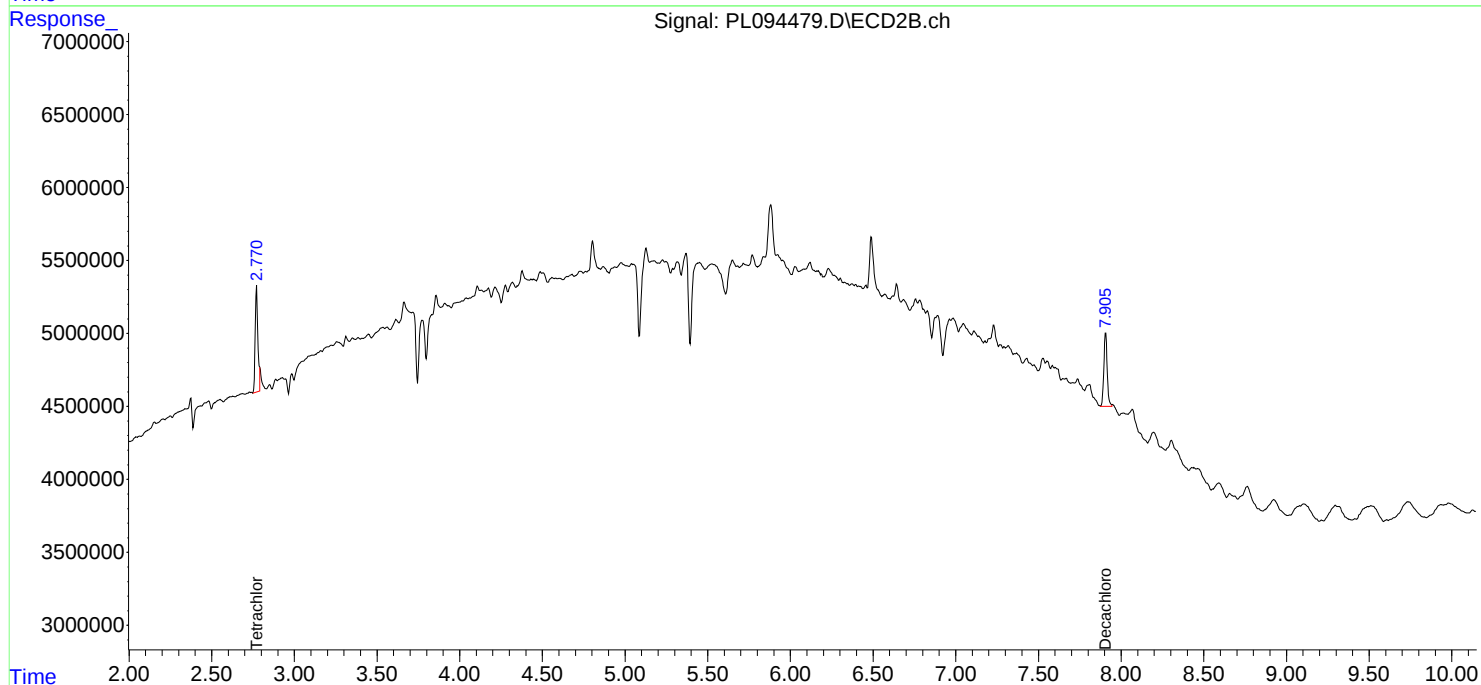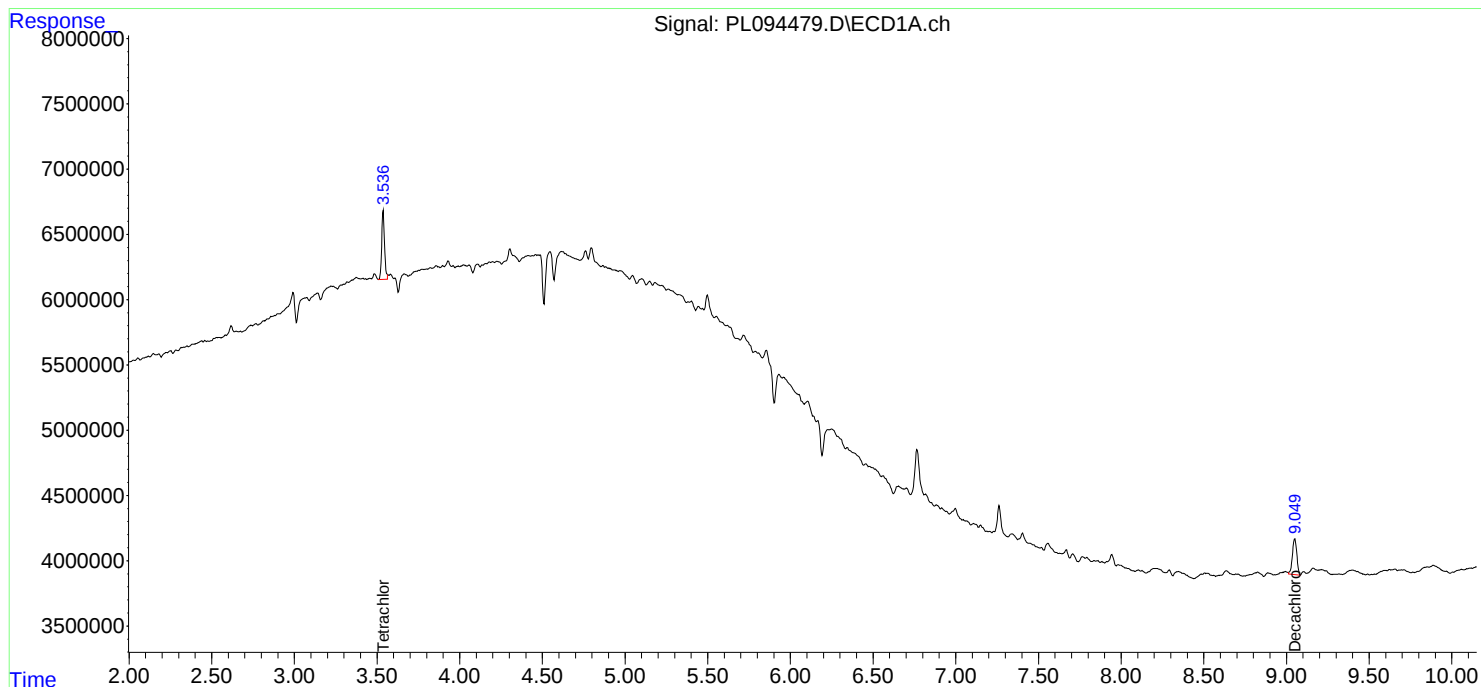

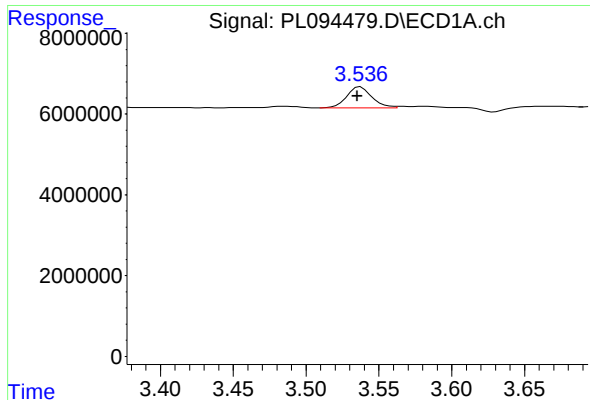


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: 0.001 min
Response: 6277172
Conc: 2.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
TR-04-02282025


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/05/2025
Supervised By :Ankita Jodhani 03/05/2025

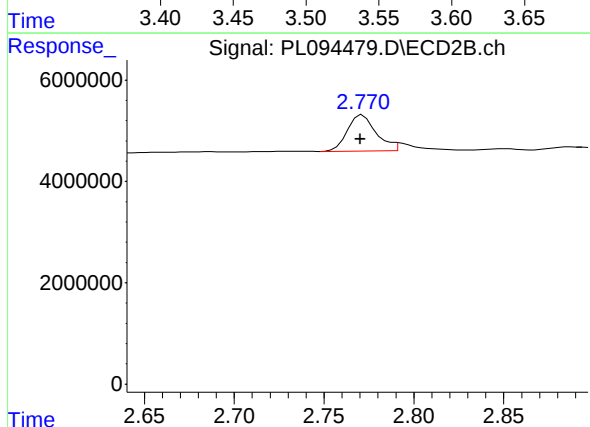


#1 Tetrachloro-m-xylene

R.T.: 2.770 min
Delta R.T.: 0.000 min
Response: 8332462
Conc: 2.61 ng/ml m

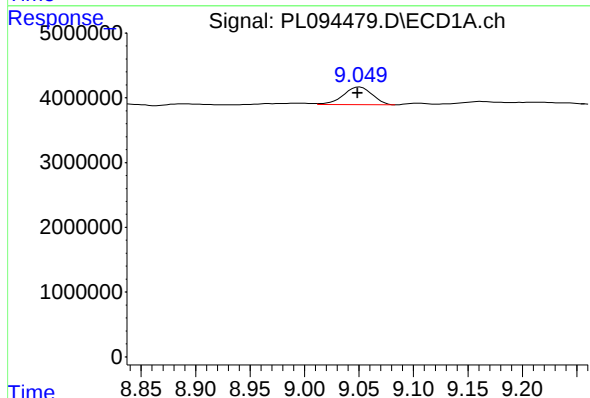

#28 Decachlorobiphenyl

R.T.: 9.049 min
Delta R.T.: 0.000 min
Response: 5022707
Conc: 2.36 ng/ml m

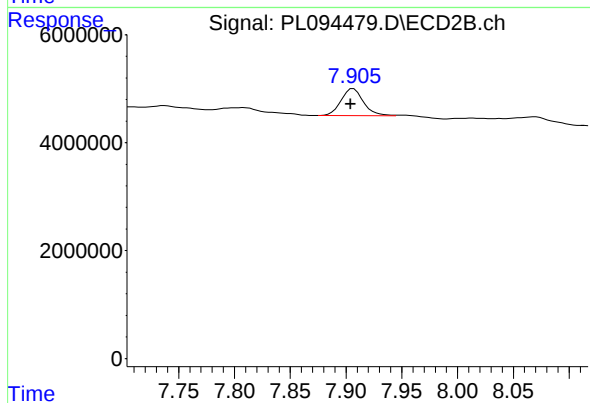

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 7057858
Conc: 1.84 ng/ml m