

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
 Data File : PL045469.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2019 14:06
 Operator : AJ\SJ
 Sample : K1705-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 EXT-028-SW003-022719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:08:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	164.0E6	43199960	23.844	20.172
28)	SA Decachlor...	8.047	9.041	99123764	28340327	11.846	12.403
Target Compounds							
9)	A Endosulfan I	5.399f	0.000	4974777	0	0.557	N.D. #
10)	B gamma-Chl...	0.000	6.076	0	2668555	N.D.	0.995 #
12)	B 4,4'-DDE	5.483	6.319	29180296	8363750	3.324	3.581
13)	MA Dieldrin	5.601	0.000	14252932	0	1.491	N.D. #
15)	B Endosulfa...	0.000	6.909f	0	2703331	N.D.	1.150 #
17)	MA 4,4'-DDT	6.231	7.107	25507191	7458041	3.401	3.779
25)	Chlordane-3	0.000	6.076	0	2668555	N.D.	6.849 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
Data File : PL045469.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2019 14:06
Operator : AJ\SJ
Sample : K1705-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
EXT-028-SW003-022719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:08:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

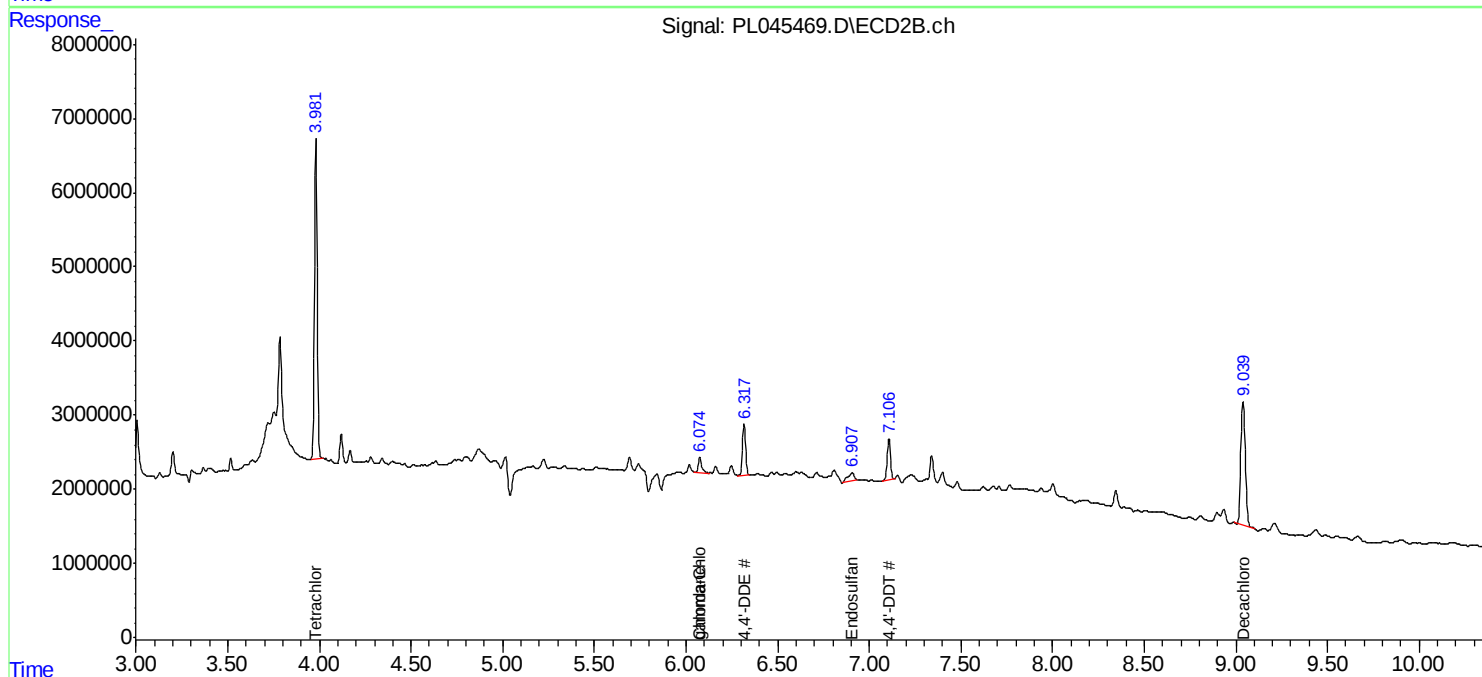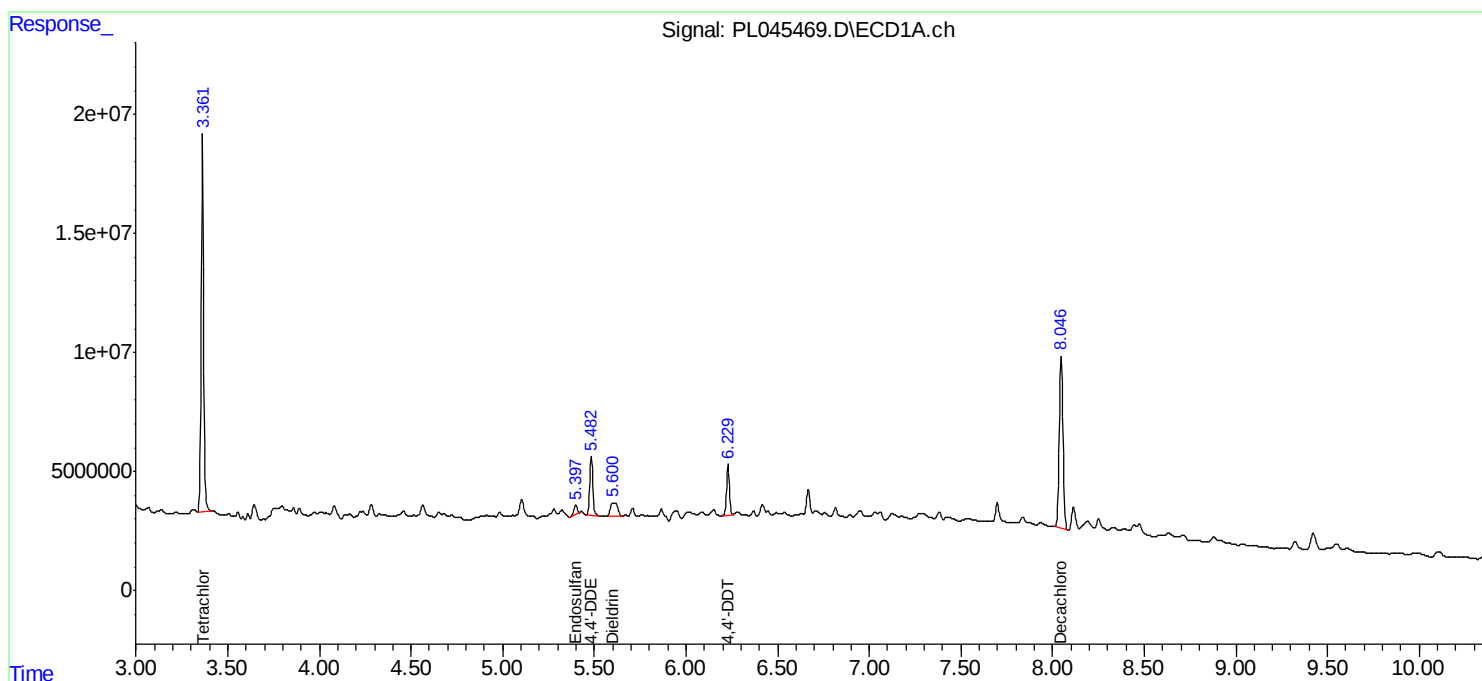


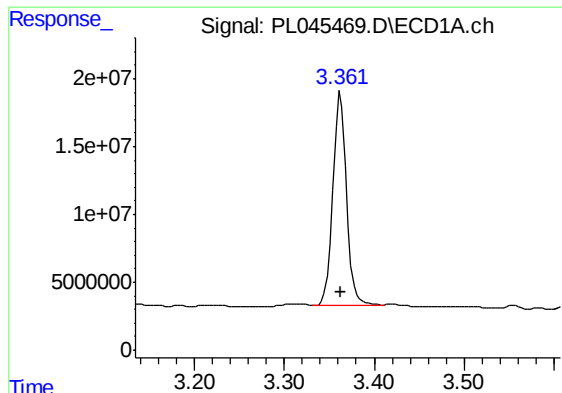

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 164026704
Conc: 23.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-028-SW003-022719

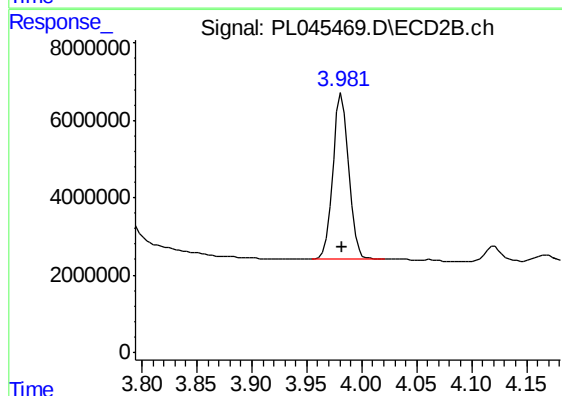


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 43199960
Conc: 20.17 ng/ml

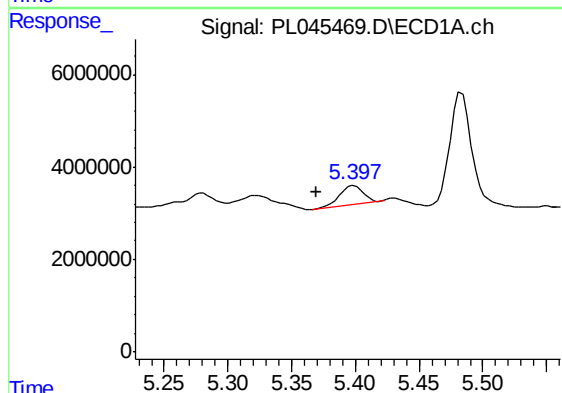


#9 Endosulfan I

R.T.: 5.399 min
Delta R.T.: 0.030 min
Response: 4974777
Conc: 0.56 ng/ml

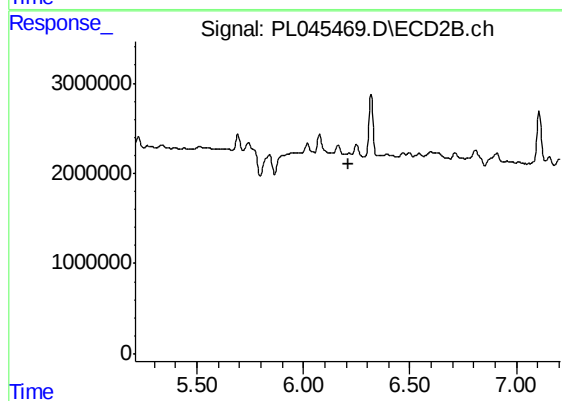

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

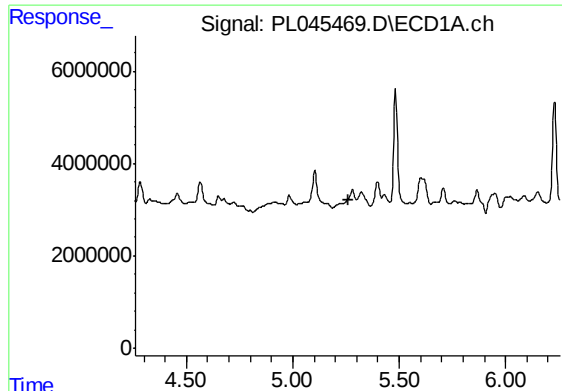

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
EXT-028-SW003-022719

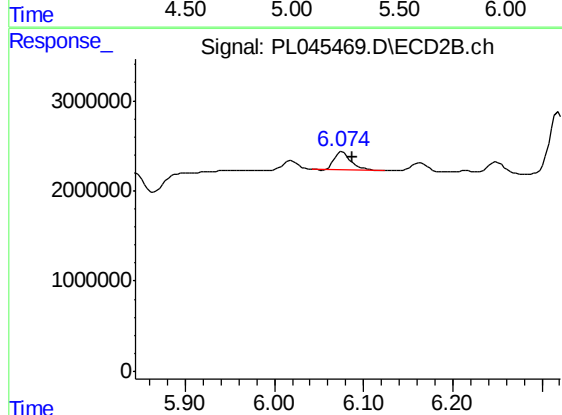


#10 gamma-Chlordane

R.T.: 6.076 min
Delta R.T.: -0.012 min
Response: 2668555
Conc: 0.99 ng/ml

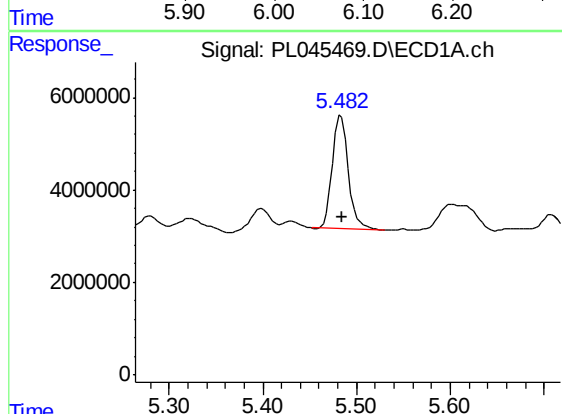


#12 4,4'-DDE

R.T.: 5.483 min
Delta R.T.: 0.000 min
Response: 29180296
Conc: 3.32 ng/ml

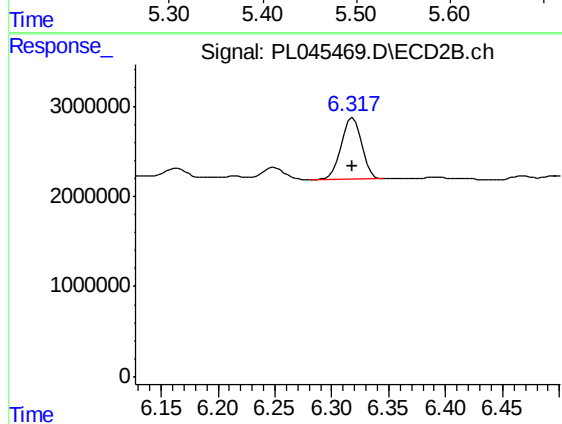

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 8363750
Conc: 3.58 ng/ml

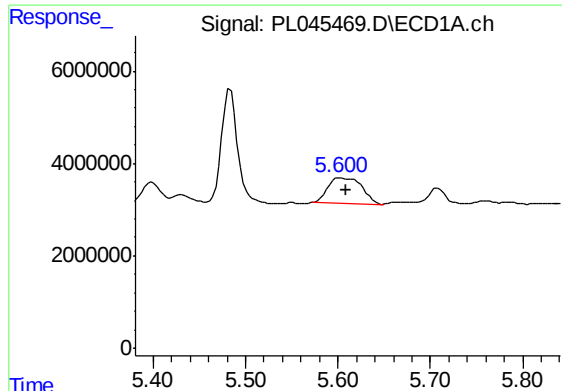

#13 Dielddrin


R.T.: 5.601 min
Delta R.T.: -0.008 min
Response: 14252932
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-028-SW003-022719

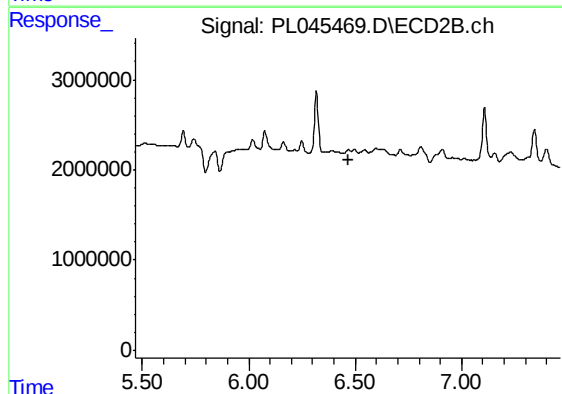


#13 Dielddrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

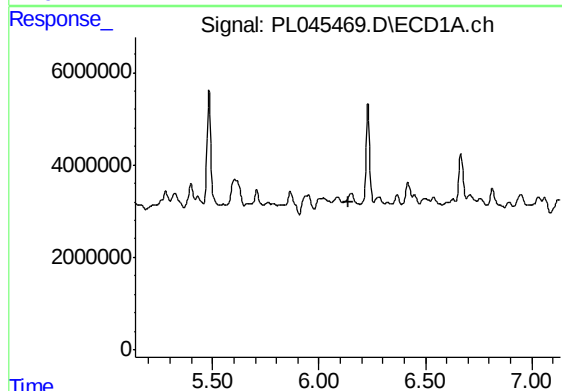


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

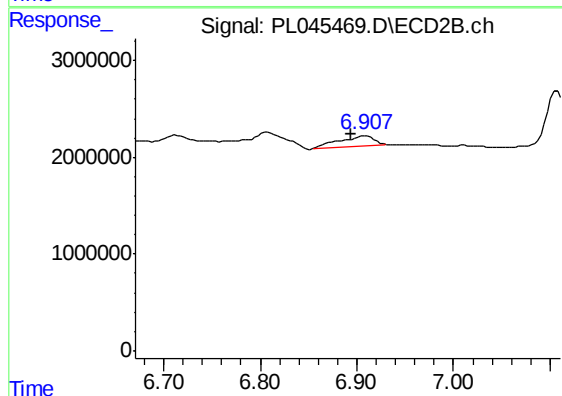

#15 Endosulfan II


R.T.: 6.909 min
Delta R.T.: 0.015 min
Response: 2703331
Conc: 1.15 ng/ml

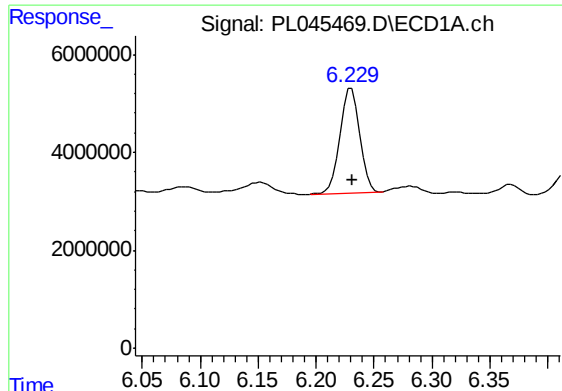

#17 4,4'-DDT


R.T.: 6.231 min
Delta R.T.: 0.000 min
Response: 25507191
Conc: 3.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-028-SW003-022719

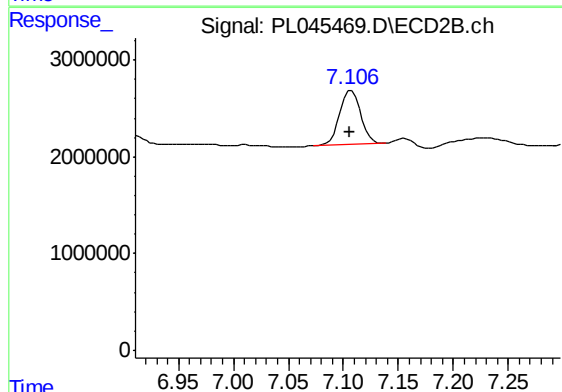


#17 4,4'-DDT

R.T.: 7.107 min
Delta R.T.: 0.002 min
Response: 7458041
Conc: 3.78 ng/ml

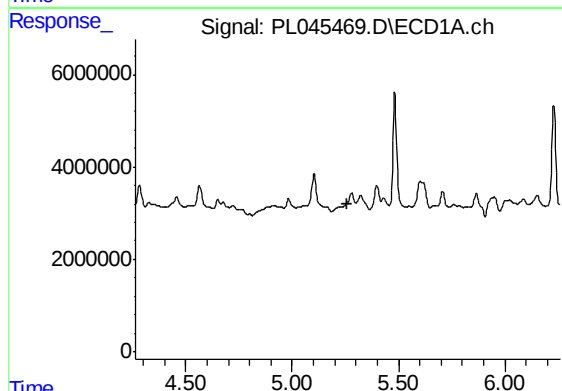


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.262 min
Response: 0
Conc: N.D.

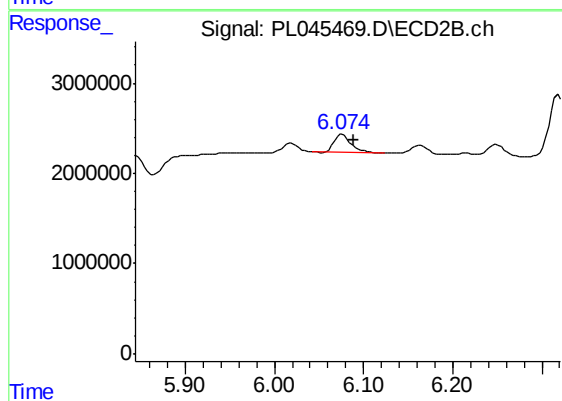

#25 Chlordane-3


R.T.: 6.076 min
Delta R.T.: -0.013 min
Response: 2668555
Conc: 6.85 ng/ml

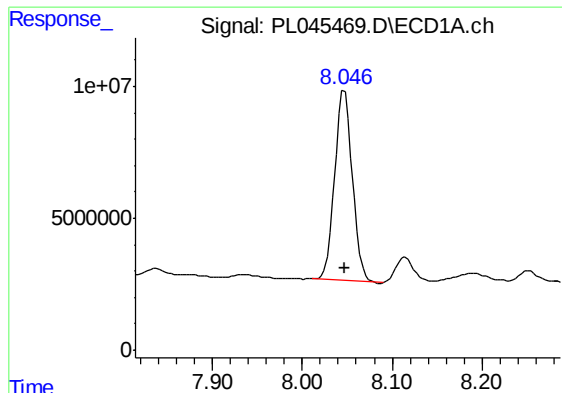

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 99123764
Conc: 11.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
EXT-028-SW003-022719

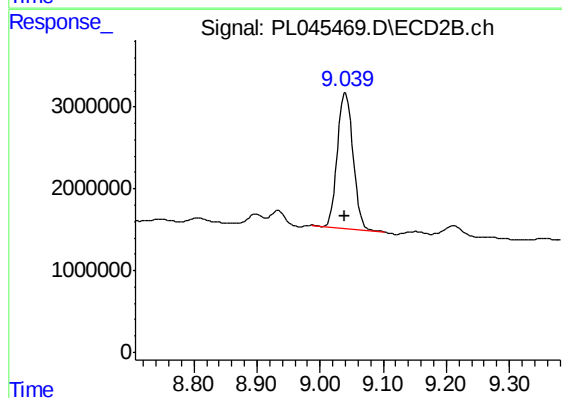

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 28340327
Conc: 12.40 ng/ml