

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
 Data File : PL045484.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2019 17:38
 Operator : AJ\SJ
 Sample : K1705-15
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-028-B097-022719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:11:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.983	86007346	28389431	12.502	13.257
28)	SA Decachlor...	8.048	9.042	104.0E6	29386340	12.429	12.861
Target Compounds							
10)	B gamma-Chl...	5.281f	0.000	9269347	0	0.947	N.D. #
11)	B alpha-Chl...	0.000	6.164	0	4823266	N.D.	1.788 #
12)	B 4,4'-DDE	5.483	6.319	44375031	14932481	5.055	6.393 #
14)	MA Endrin	5.866	6.714f	2575647	905851	0.286	0.398 #
16)	A 4,4'-DDD	0.000	6.815	0	2768123	N.D.	1.439 #
17)	MA 4,4'-DDT	6.229	7.108	36082494	7044532	4.811	3.570 #
25)	Chlordane-3	5.281f	0.000	9269347	0	8.081	N.D. #
26)	Chlordane-4	0.000	6.164	0	4823266	N.D.	10.310 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
Data File : PL045484.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2019 17:38
Operator : AJ\SJ
Sample : K1705-15
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-028-B097-022719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:11:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

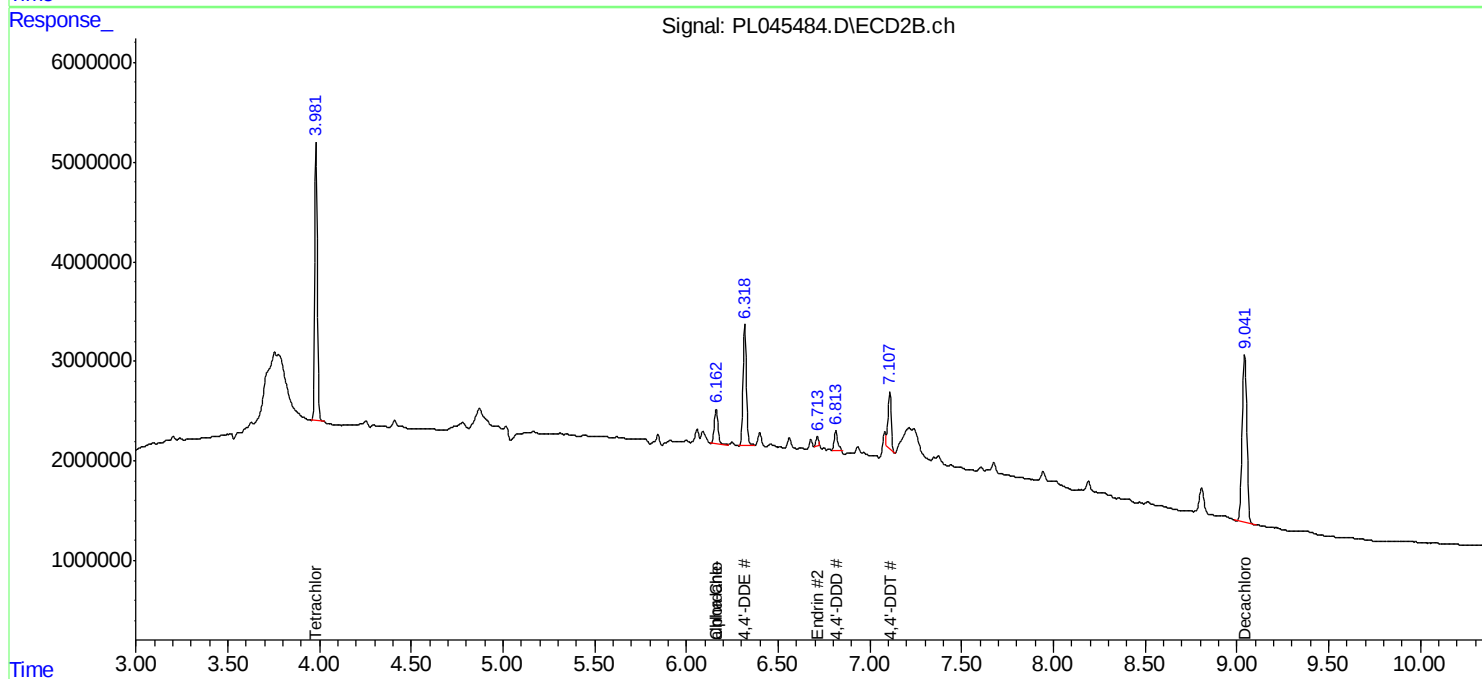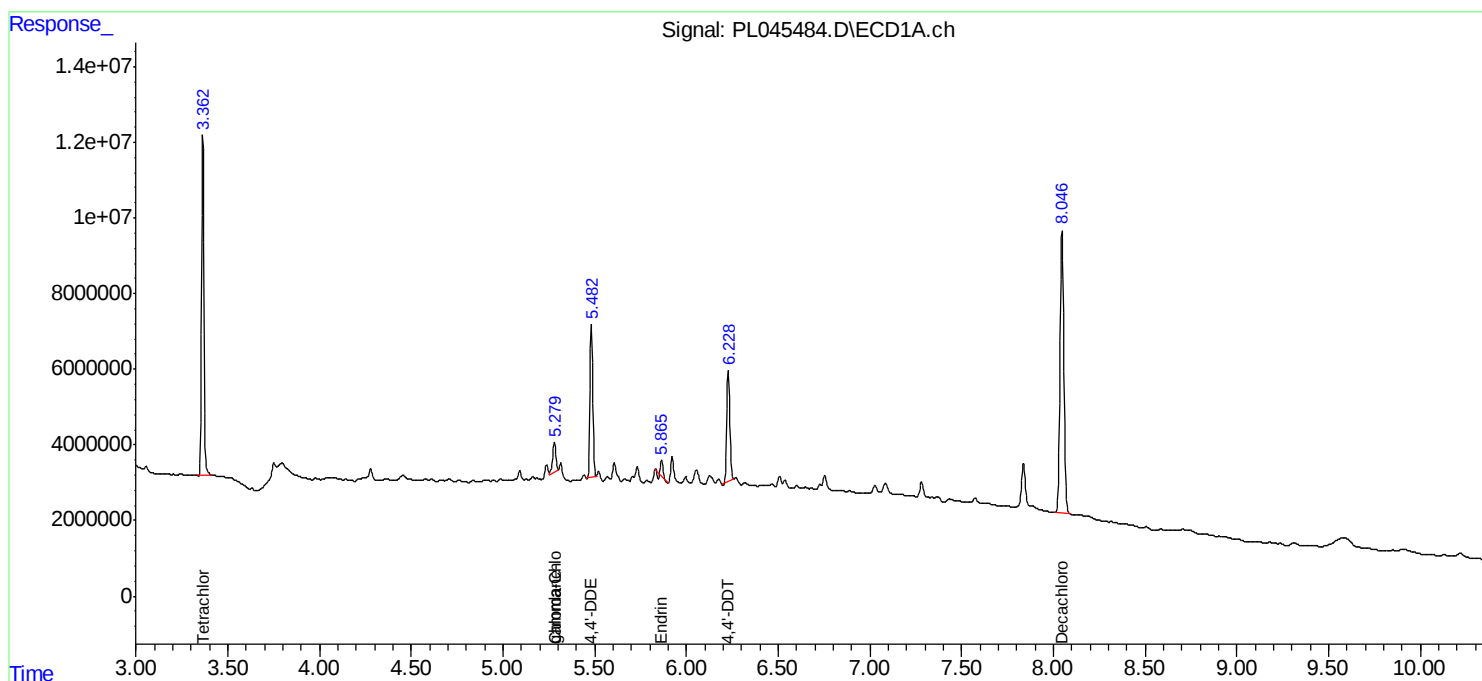


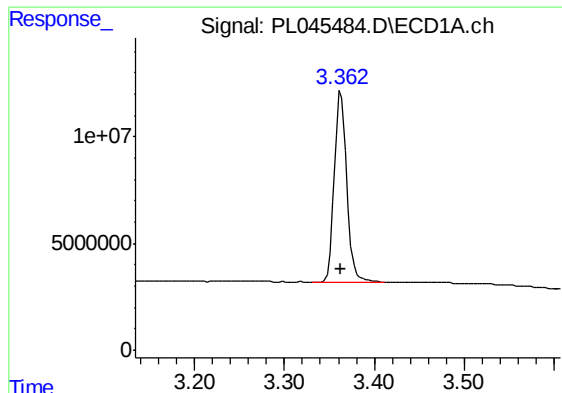

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 86007346
Conc: 12.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-B097-022719

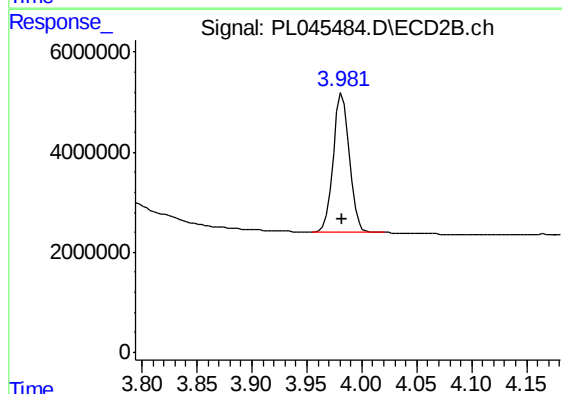


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: 0.000 min
Response: 28389431
Conc: 13.26 ng/ml

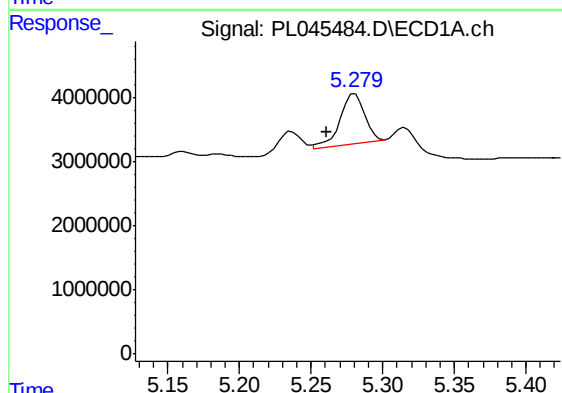


#10 gamma-Chlordane

R.T.: 5.281 min
Delta R.T.: 0.020 min
Response: 9269347
Conc: 0.95 ng/ml

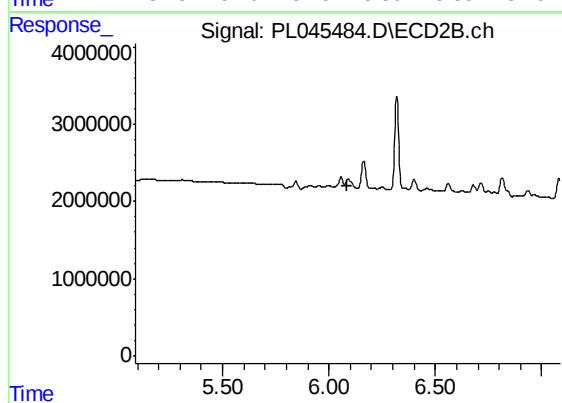

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.088 min
Response: 0
Conc: N.D.

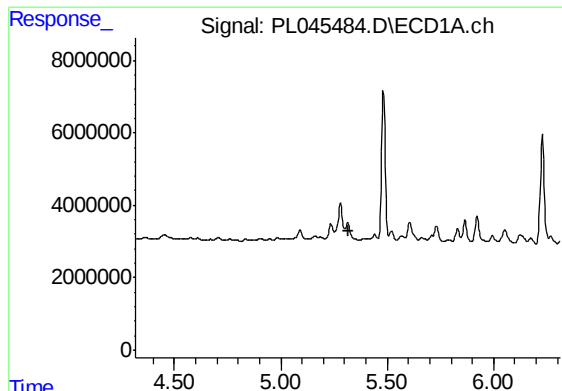

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-028-B097-022719

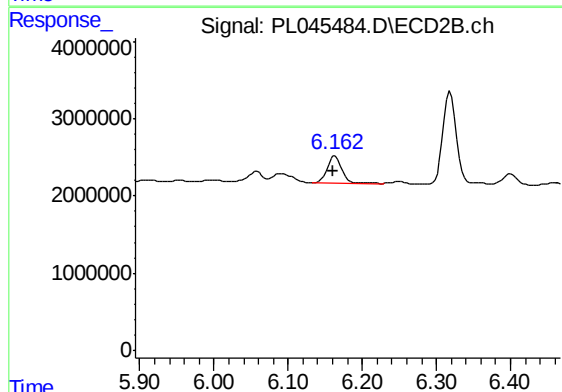


#11 alpha-Chlordane

R.T.: 6.164 min
Delta R.T.: 0.003 min
Response: 4823266
Conc: 1.79 ng/ml

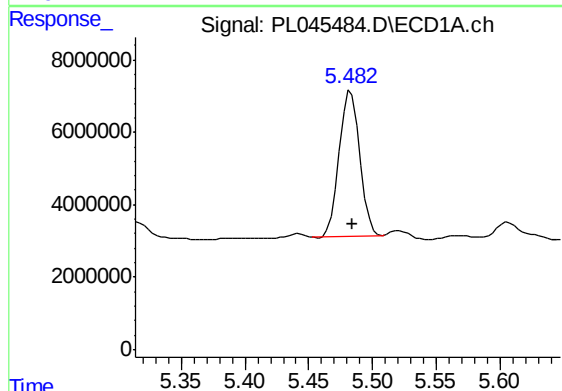


#12 4,4'-DDE

R.T.: 5.483 min
Delta R.T.: 0.000 min
Response: 44375031
Conc: 5.06 ng/ml

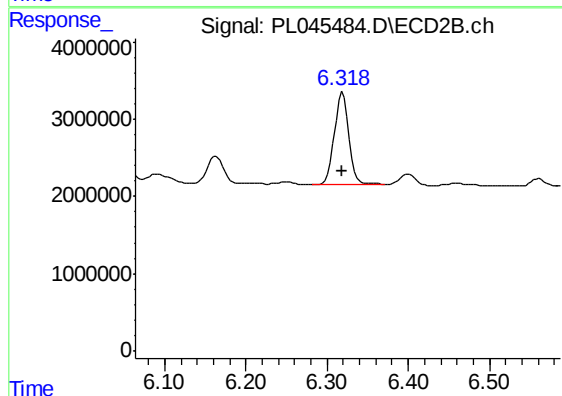

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 14932481
Conc: 6.39 ng/ml

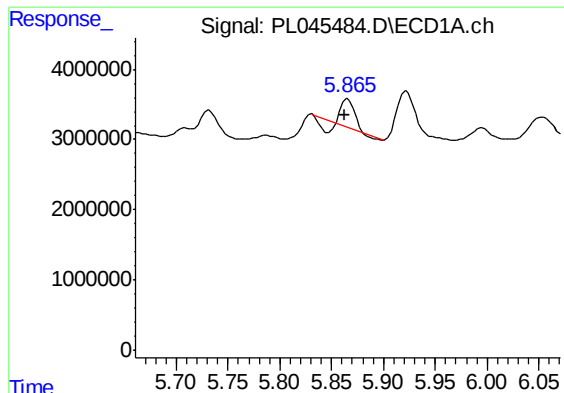

#14 Endrin


R.T.: 5.866 min
Delta R.T.: 0.004 min
Response: 2575647
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-B097-022719

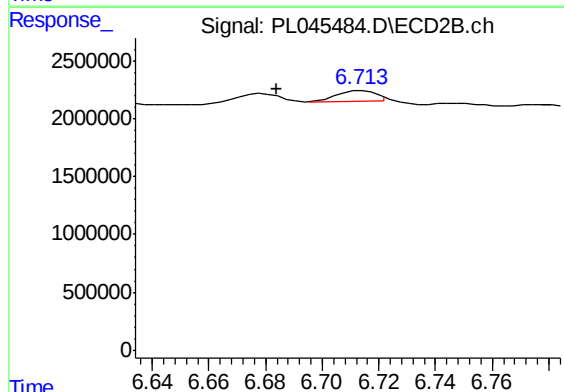


#14 Endrin

R.T.: 6.714 min
Delta R.T.: 0.030 min
Response: 905851
Conc: 0.40 ng/ml

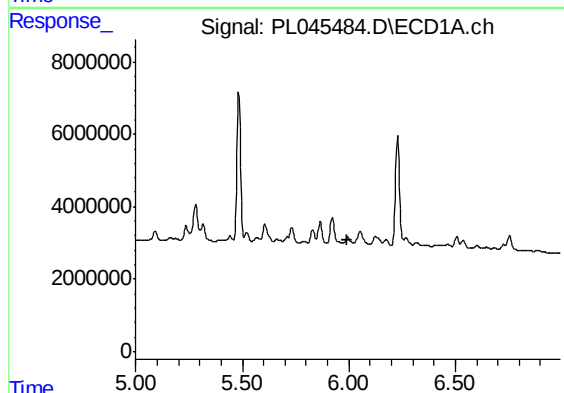


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

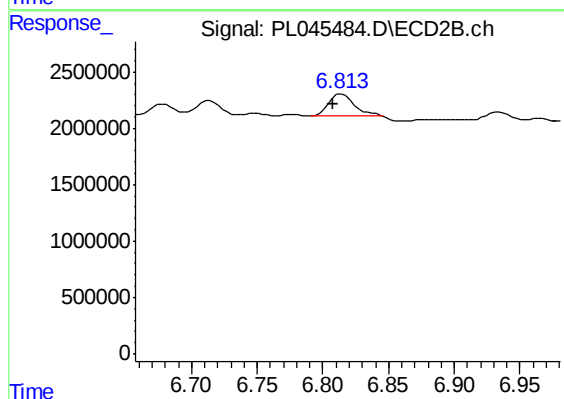

#16 4,4'-DDD


R.T.: 6.815 min
Delta R.T.: 0.007 min
Response: 2768123
Conc: 1.44 ng/ml

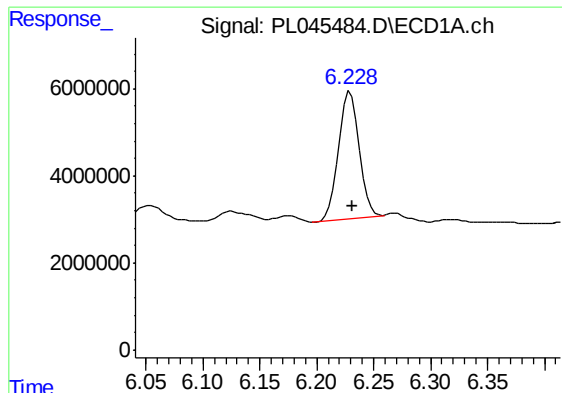

#17 4,4'-DDT


R.T.: 6.229 min
Delta R.T.: -0.001 min
Response: 36082494
Conc: 4.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-B097-022719

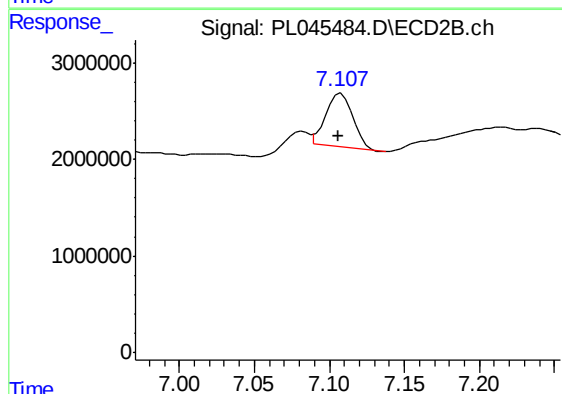


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.002 min
Response: 7044532
Conc: 3.57 ng/ml

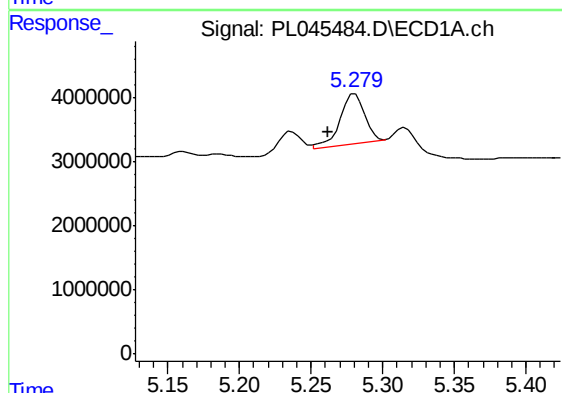


#25 Chlordane-3

R.T.: 5.281 min
Delta R.T.: 0.019 min
Response: 9269347
Conc: 8.08 ng/ml

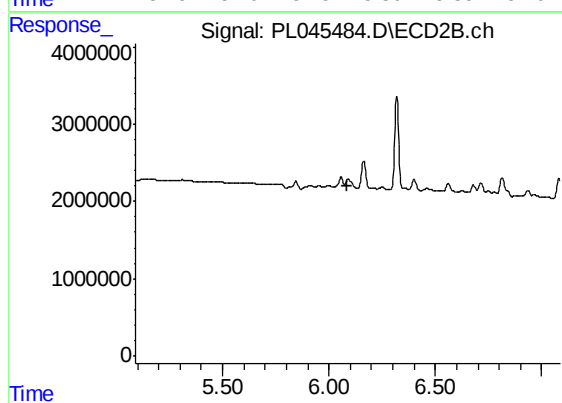

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.089 min
Response: 0
Conc: N.D.

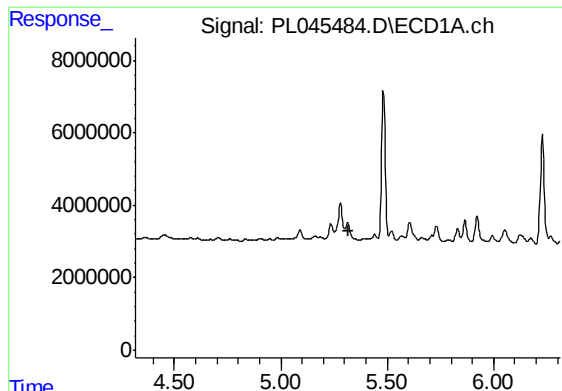

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-028-B097-022719

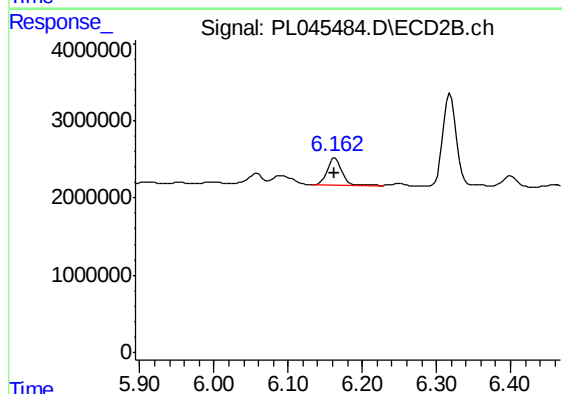


#26 Chlordane-4

R.T.: 6.164 min
Delta R.T.: 0.001 min
Response: 4823266
Conc: 10.31 ng/ml

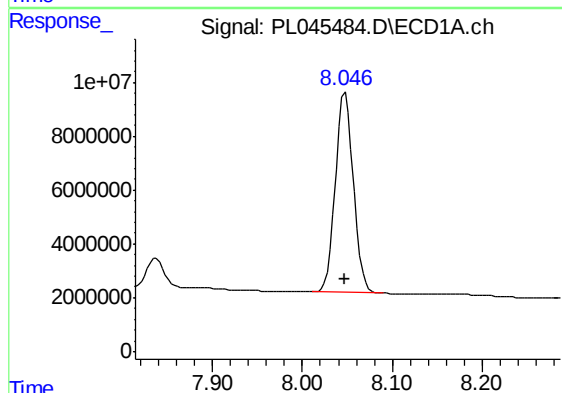

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 103996634
Conc: 12.43 ng/ml

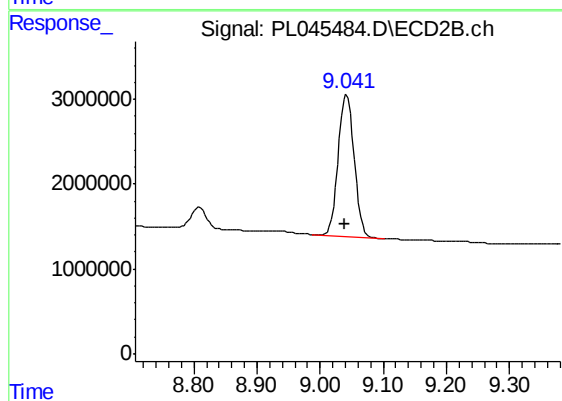

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.003 min
Response: 29386340
Conc: 12.86 ng/ml