

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
 Data File : PL045498.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2019 20:56
 Operator : AJ\SJ
 Sample : K1704-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-027-B114-022719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:15:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	157.1E6	46271778	22.840	21.607
28)	SA Decachlor...	8.048	9.041	150.0E6	42816891	17.930	18.739
Target Compounds							
3)	MA gamma-BHC...	4.080	0.000	6885630	0	0.681	N.D. #
9)	A Endosulfan I	5.399f	0.000	5181906	0	0.580	N.D. #
10)	B gamma-Chl...	0.000	6.076	0	4877241	N.D.	1.818 #
12)	B 4,4'-DDE	5.483	6.319	26518361	7687675	3.021	3.291
13)	MA Dieldrin	5.619	0.000	12100789	0	1.266	N.D. #
16)	A 4,4'-DDD	0.000	6.807	0	2670217	N.D.	1.389 #
17)	MA 4,4'-DDT	6.230	7.108	11057703	2866135	1.474	1.452
19)	B Endosulfa...	6.541f	0.000	6937729	0	0.854	N.D. #
25)	Chlordane-3	0.000	6.076	0	4877241	N.D.	12.518 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
Data File : PL045498.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2019 20:56
Operator : AJ\SJ
Sample : K1704-04
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:15:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

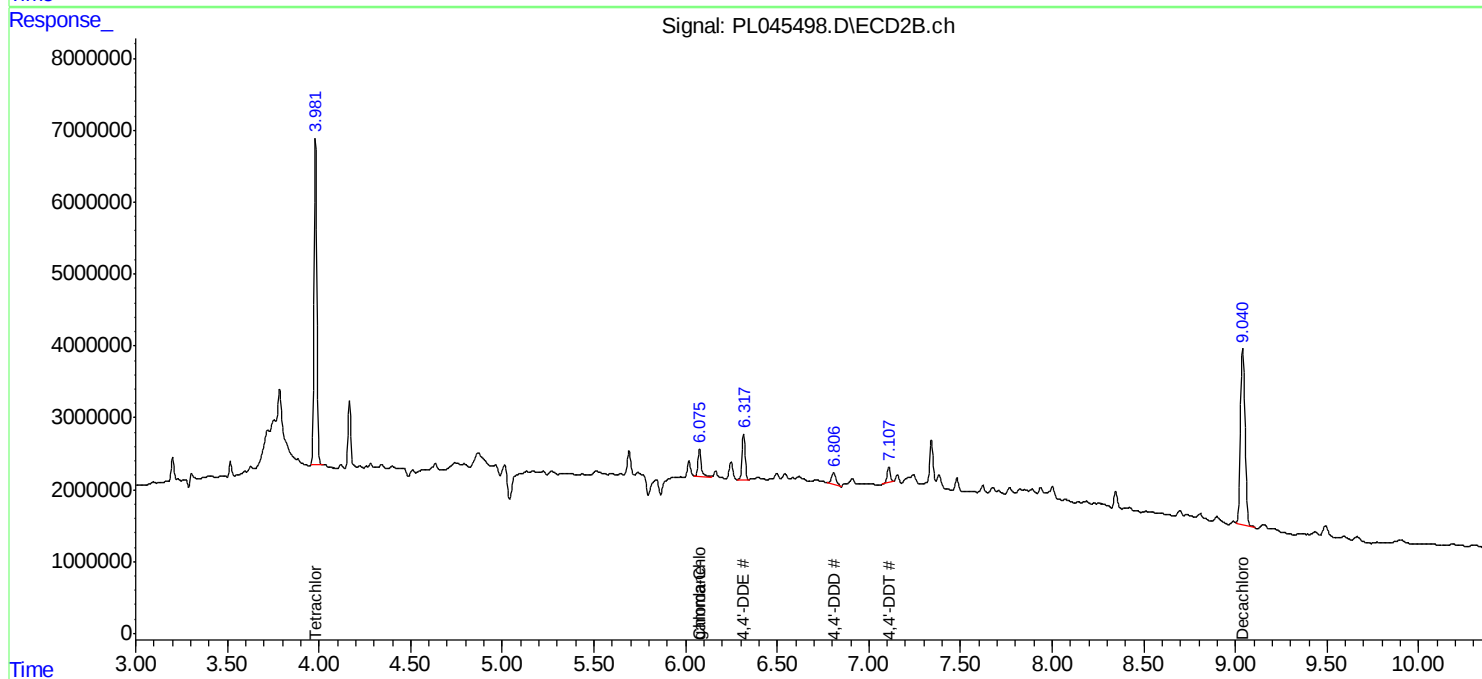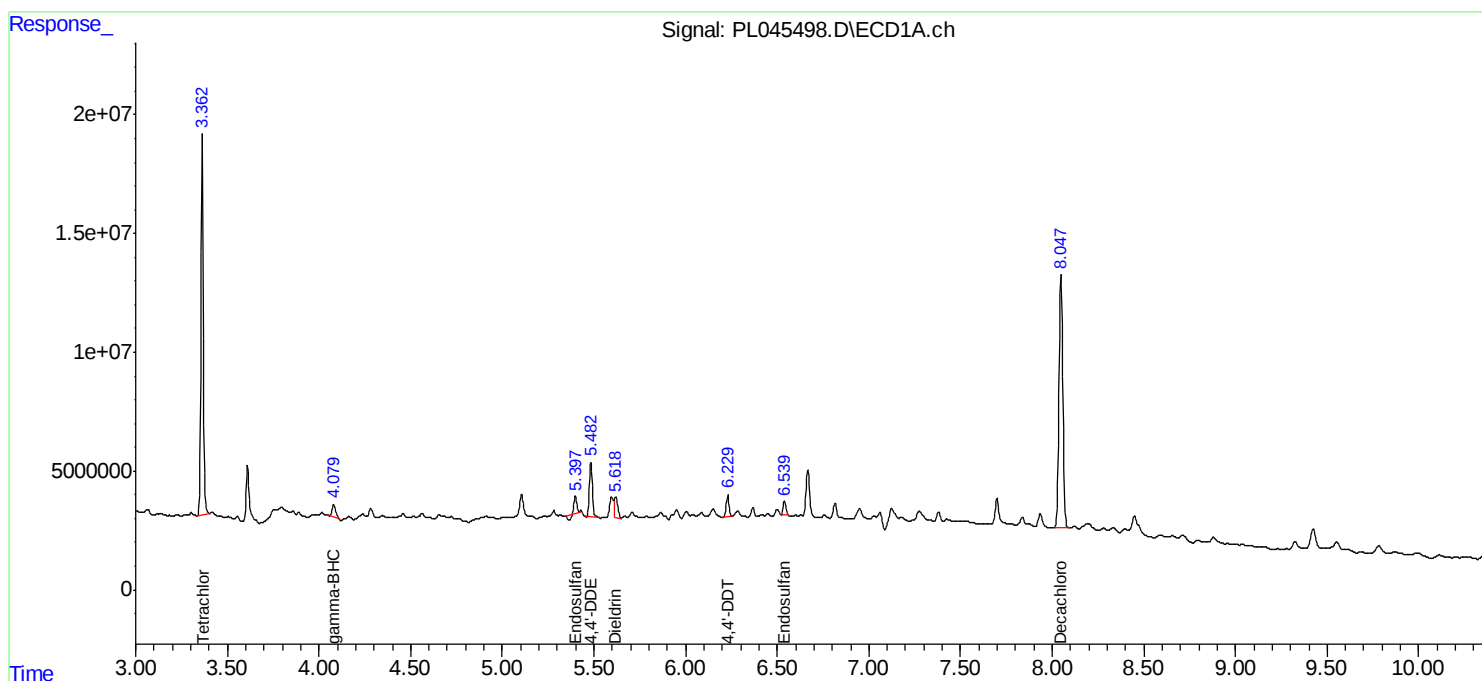


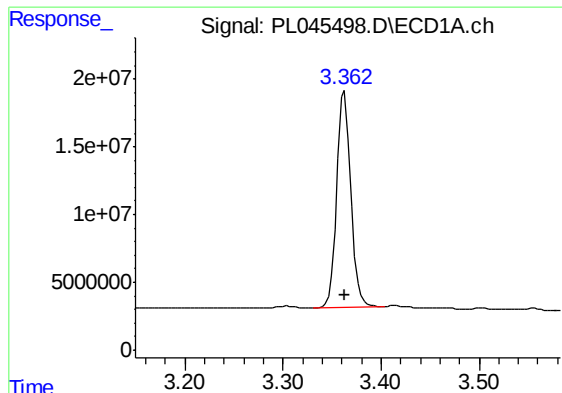

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 157123943
Conc: 22.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

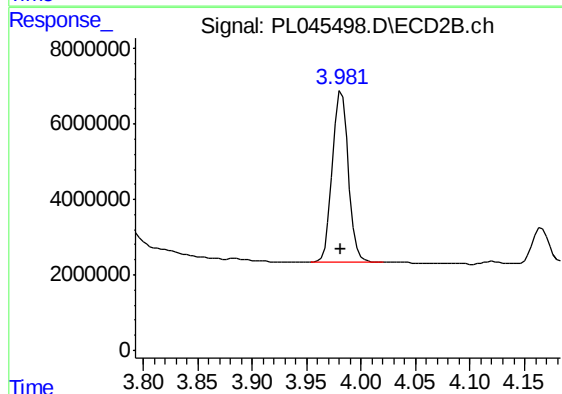


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 46271778
Conc: 21.61 ng/ml

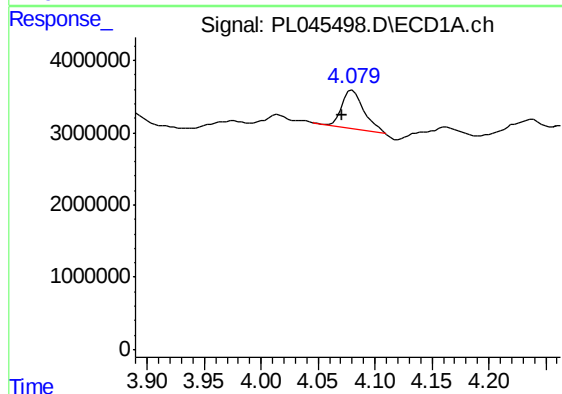


#3 gamma-BHC (Lindane)

R.T.: 4.080 min
Delta R.T.: 0.010 min
Response: 6885630
Conc: 0.68 ng/ml

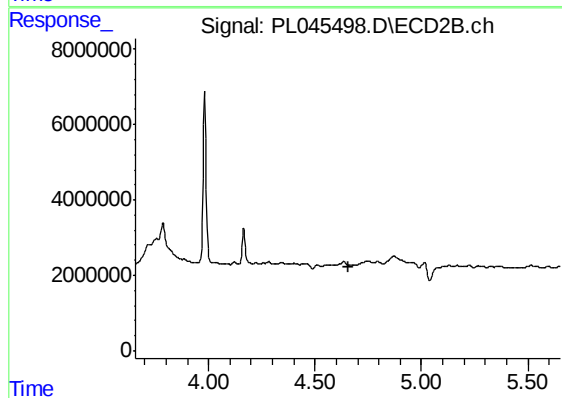

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.656 min
Response: 0
Conc: N.D.

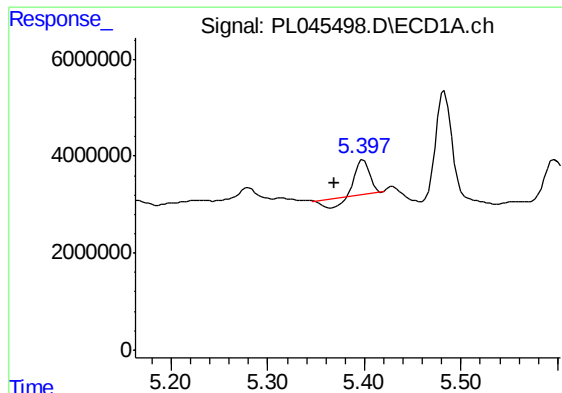

#9 Endosulfan I


R.T.: 5.399 min
Delta R.T.: 0.030 min
Response: 5181906
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

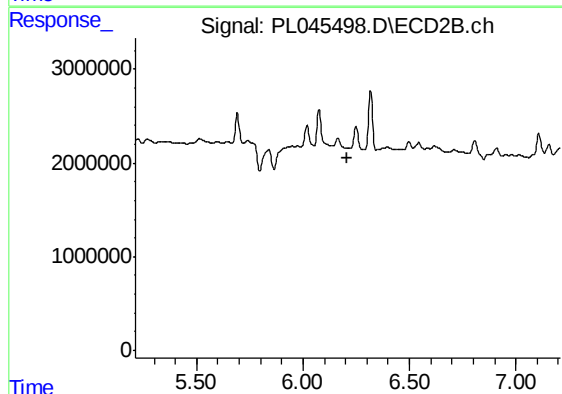


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.210 min
Response: 0
Conc: N.D.

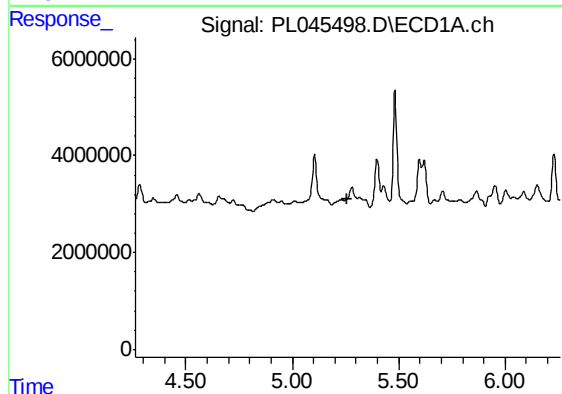


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.261 min
Response: 0
Conc: N.D.

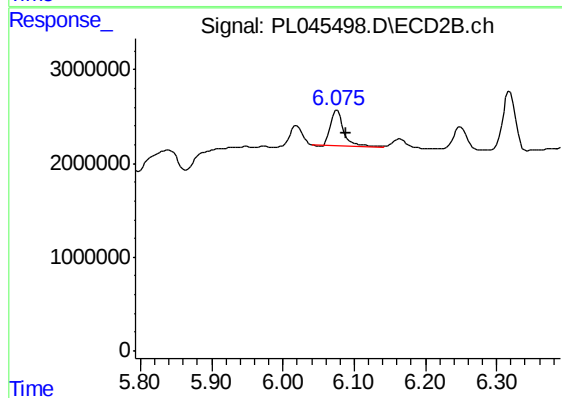

#10 gamma-Chlordane


R.T.: 6.076 min
Delta R.T.: -0.012 min
Response: 4877241
Conc: 1.82 ng/ml

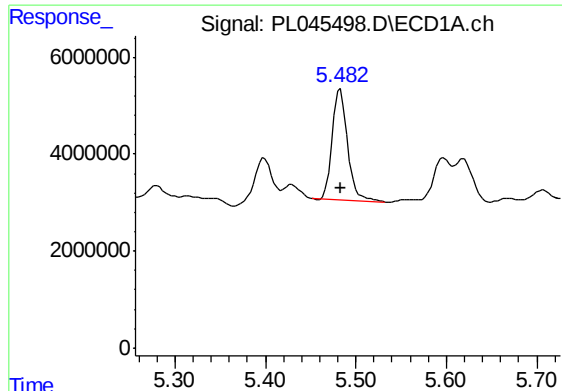

#12 4,4'-DDE


R.T.: 5.483 min
Delta R.T.: 0.000 min
Response: 26518361
Conc: 3.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

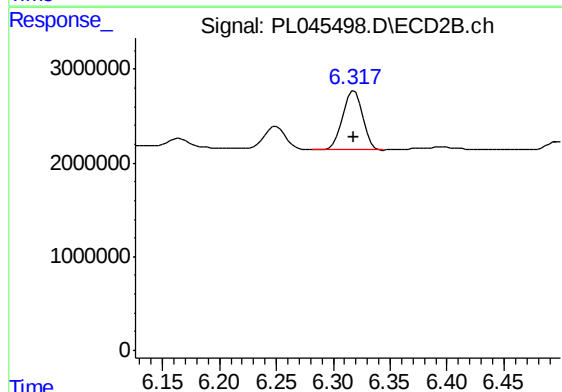


#12 4,4'-DDE

R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 7687675
Conc: 3.29 ng/ml

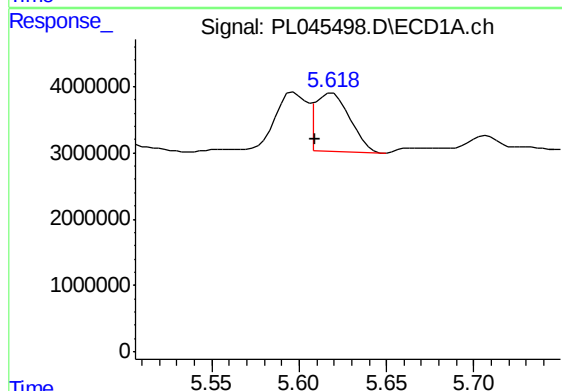


#13 Dieldrin

R.T.: 5.619 min
Delta R.T.: 0.010 min
Response: 12100789
Conc: 1.27 ng/ml

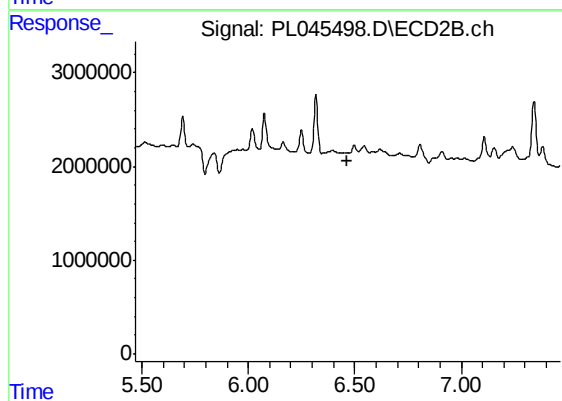

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

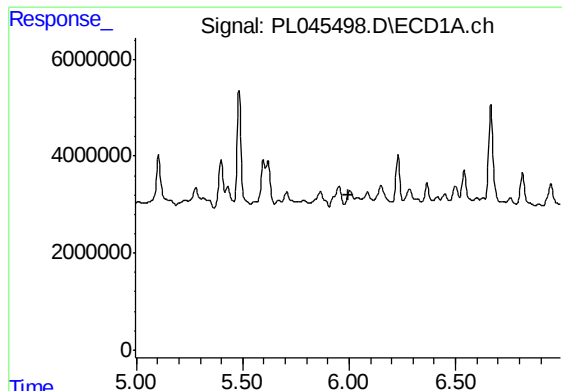

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.996 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

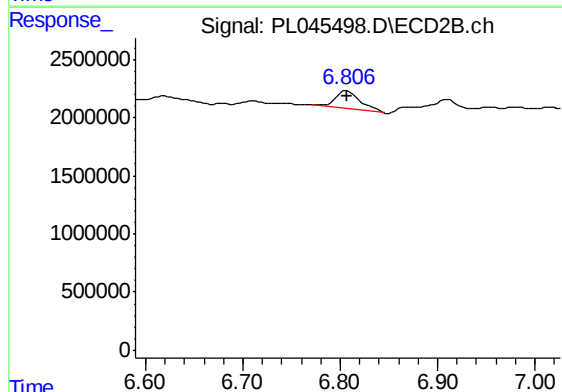


#16 4,4'-DDD

R.T.: 6.807 min
Delta R.T.: -0.001 min
Response: 2670217
Conc: 1.39 ng/ml

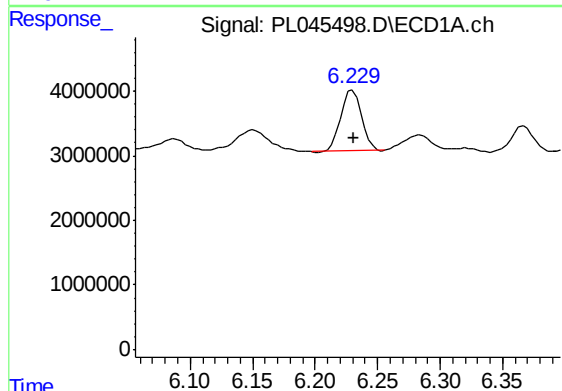


#17 4,4'-DDT

R.T.: 6.230 min
Delta R.T.: 0.000 min
Response: 11057703
Conc: 1.47 ng/ml

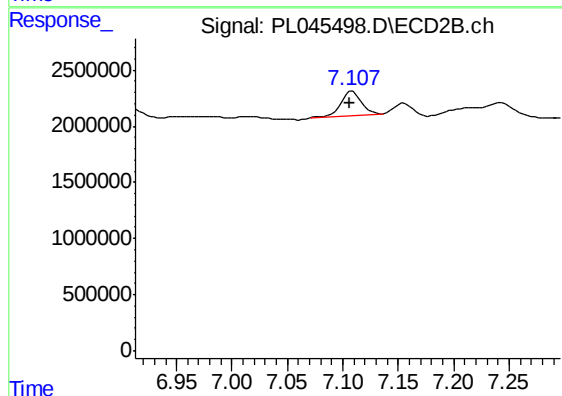

#17 4,4'-DDT


R.T.: 7.108 min
Delta R.T.: 0.003 min
Response: 2866135
Conc: 1.45 ng/ml

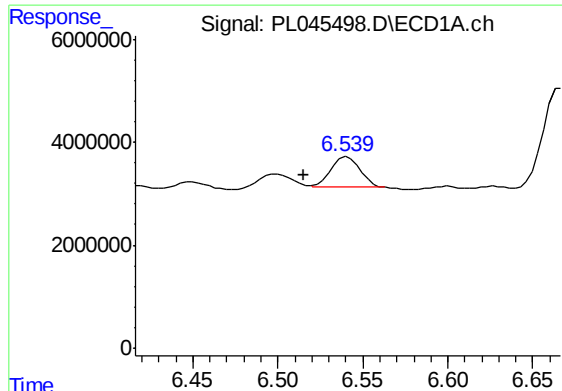

#19 Endosulfan Sulfate


R.T.: 6.541 min
Delta R.T.: 0.025 min
Response: 6937729
Conc: 0.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

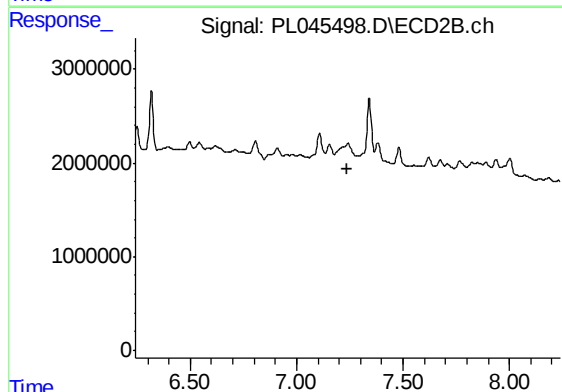


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.241 min
Response: 0
Conc: N.D.

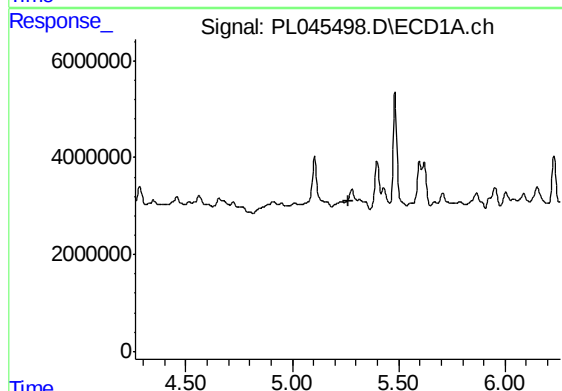


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.262 min
Response: 0
Conc: N.D.

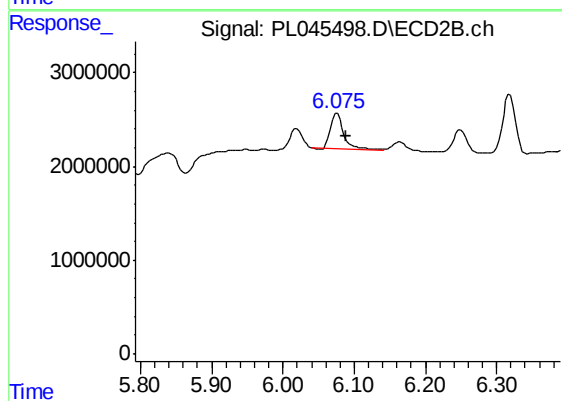

#25 Chlordane-3


R.T.: 6.076 min
Delta R.T.: -0.013 min
Response: 4877241
Conc: 12.52 ng/ml

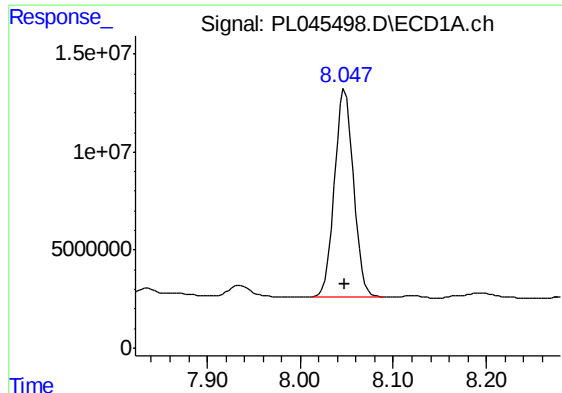

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 150024382
Conc: 17.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-027-B114-022719

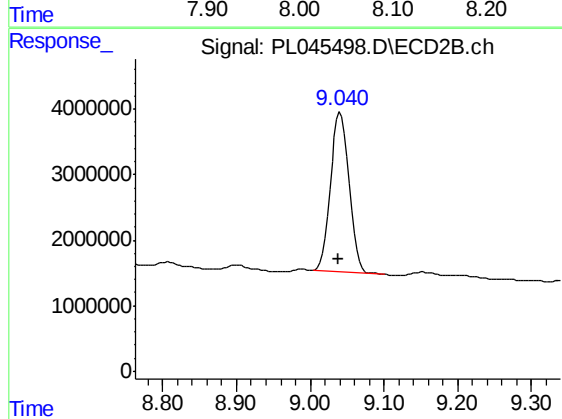

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 42816891
Conc: 18.74 ng/ml