

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
 Data File : PL045508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2019 23:17
 Operator : AJ\SJ
 Sample : K1704-10
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PST-028-SW062-022719

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:18:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	131.3E6	35486320	19.093	16.570
28)	SA Decachlor...	8.048	9.041	85473331	24326545	10.215	10.647
Target Compounds							
10)	B gamma-Chl...	5.281f	6.076	4859326	2980726	0.497	1.111 #
11)	B alpha-Chl...	0.000	6.164	0	1632632	N.D.	0.605 #
12)	B 4,4'-DDE	5.484	6.319	15027116	4811154	1.712	2.060
13)	MA Dieldrin	5.600	0.000	13366612	0	1.398	N.D. #
15)	B Endosulfa...	0.000	6.910f	0	1854110	N.D.	0.788 #
17)	MA 4,4'-DDT	6.230	7.108	7285517	1646462	0.971	0.834
25)	Chlordane-3	5.281f	6.076	4859326	2980726	4.236	7.650 #
26)	Chlordane-4	0.000	6.164	0	1632632	N.D.	3.490 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
Data File : PL045508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2019 23:17
Operator : AJ\SJ
Sample : K1704-10
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PST-028-SW062-022719

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:18:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

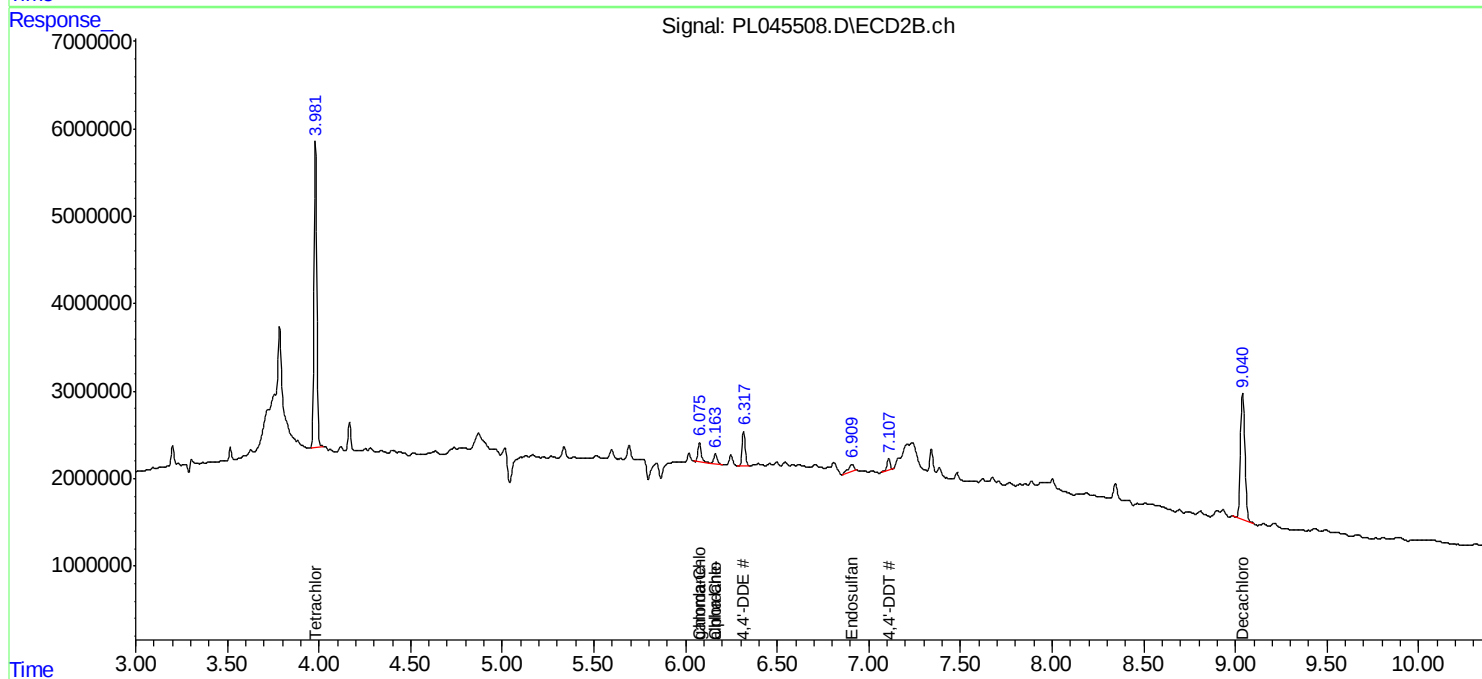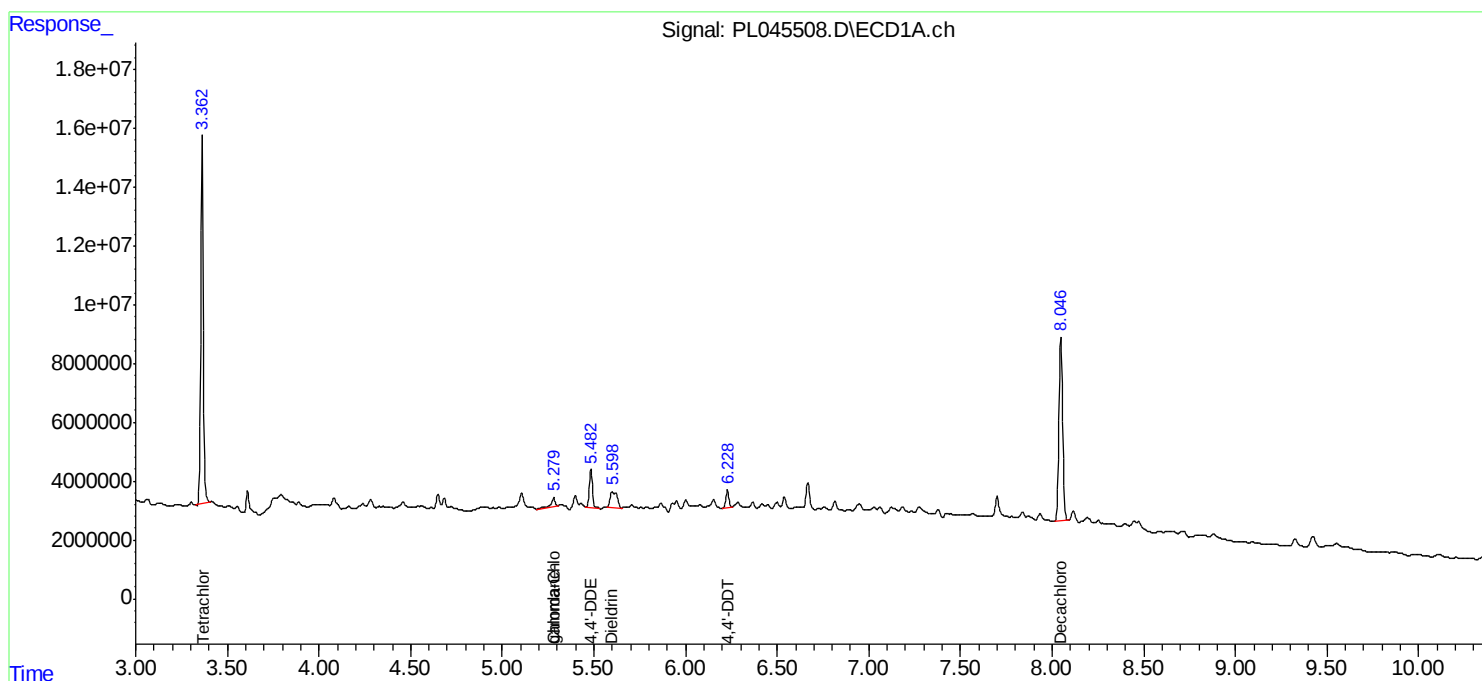


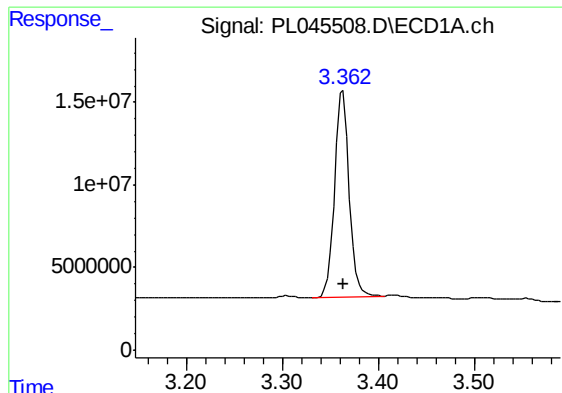

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 131343662
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-SW062-022719

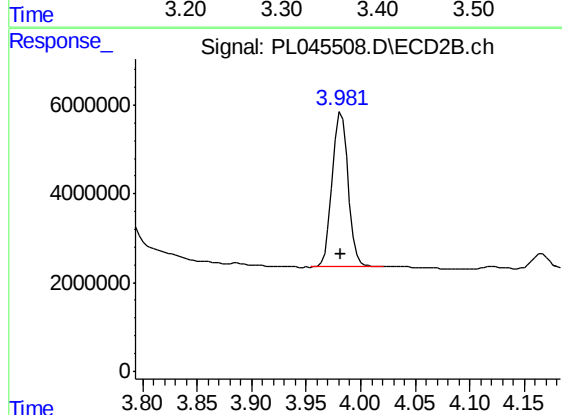


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 35486320
Conc: 16.57 ng/ml

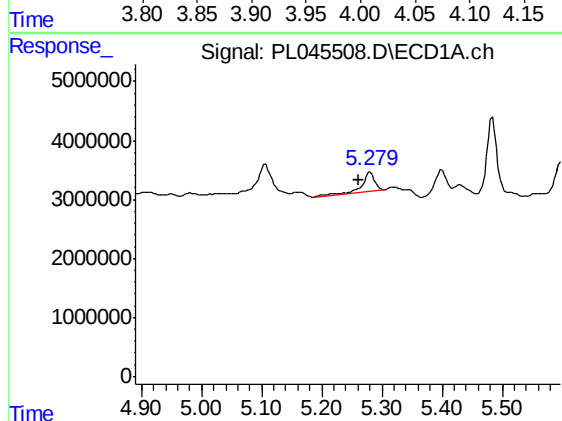


#10 gamma-Chlordane

R.T.: 5.281 min
Delta R.T.: 0.020 min
Response: 4859326
Conc: 0.50 ng/ml

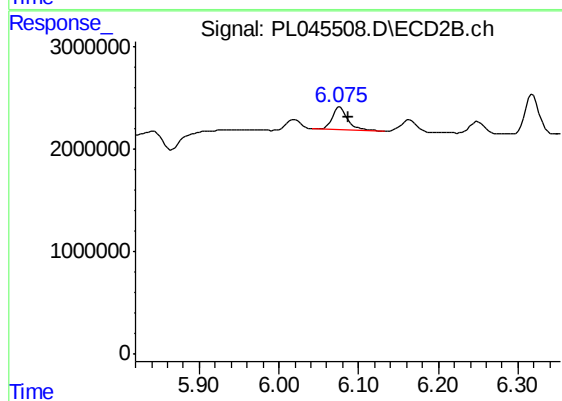

#10 gamma-Chlordane


R.T.: 6.076 min
Delta R.T.: -0.012 min
Response: 2980726
Conc: 1.11 ng/ml

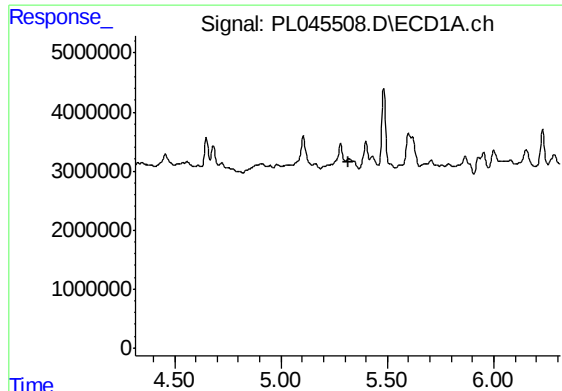

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-028-SW062-022719

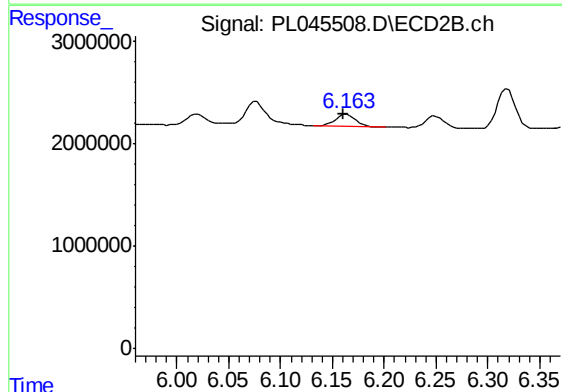


#11 alpha-Chlordane

R.T.: 6.164 min
Delta R.T.: 0.004 min
Response: 1632632
Conc: 0.61 ng/ml

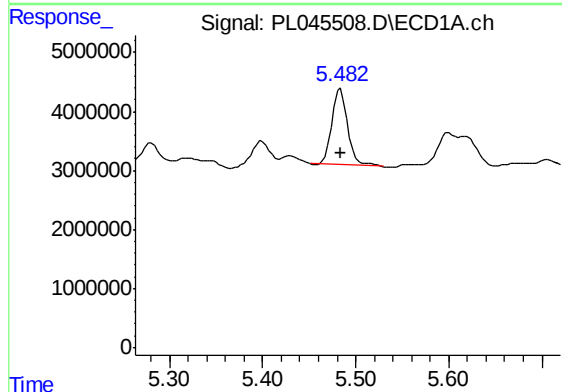


#12 4,4'-DDE

R.T.: 5.484 min
Delta R.T.: 0.000 min
Response: 15027116
Conc: 1.71 ng/ml

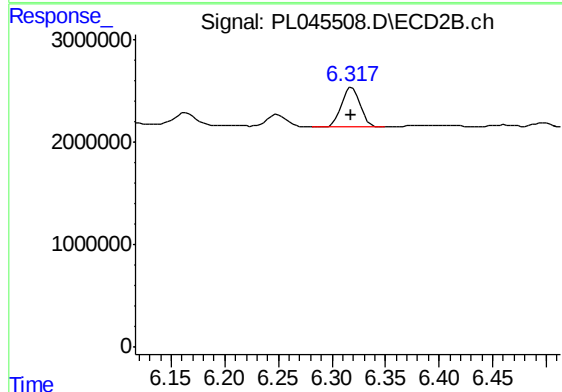

#12 4,4'-DDE


R.T.: 6.319 min
Delta R.T.: 0.000 min
Response: 4811154
Conc: 2.06 ng/ml

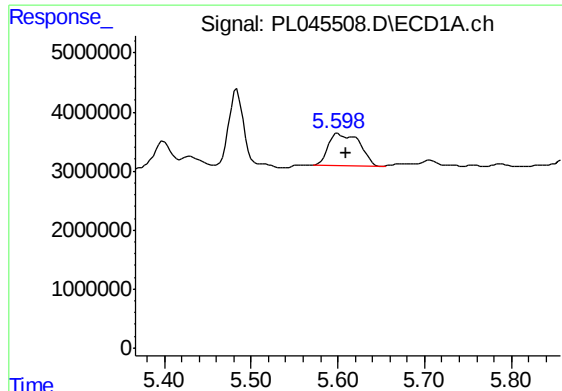

#13 Dieldrin


R.T.: 5.600 min
Delta R.T.: -0.009 min
Response: 13366612
Conc: 1.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-SW062-022719

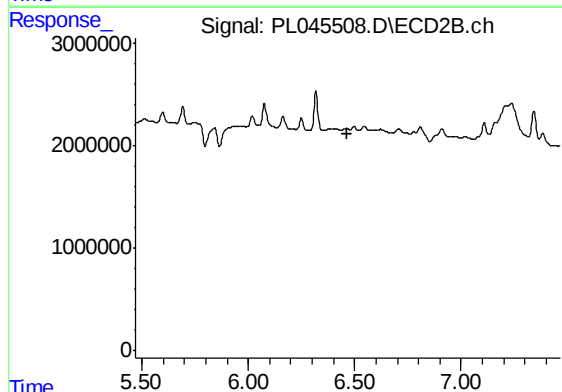


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.467 min
Response: 0
Conc: N.D.

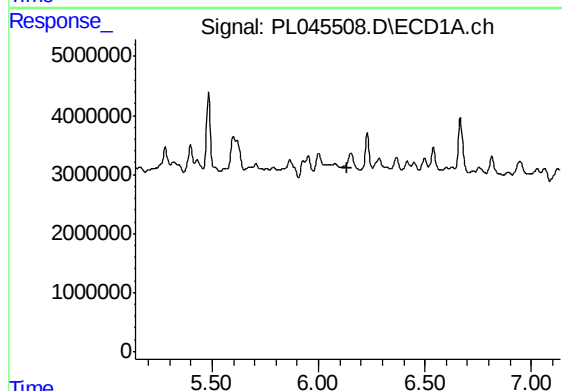


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.137 min
Response: 0
Conc: N.D.

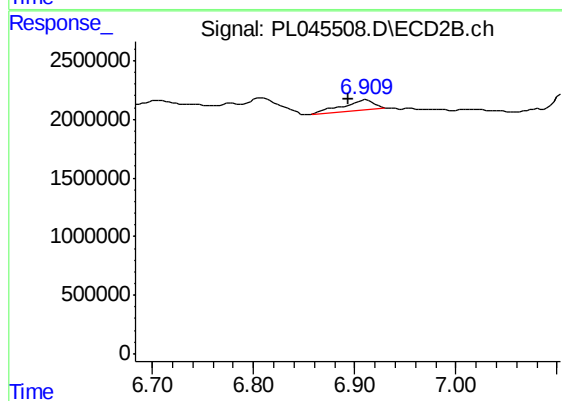

#15 Endosulfan II


R.T.: 6.910 min
Delta R.T.: 0.017 min
Response: 1854110
Conc: 0.79 ng/ml

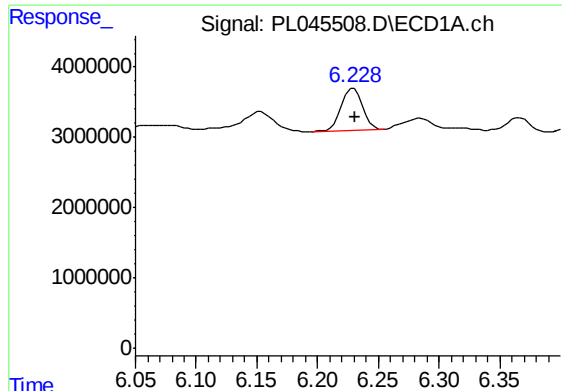

#17 4,4'-DDT


R.T.: 6.230 min
Delta R.T.: -0.001 min
Response: 7285517
Conc: 0.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PST-028-SW062-022719

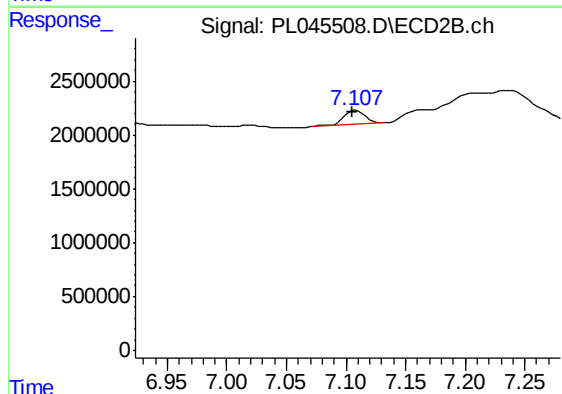


#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.002 min
Response: 1646462
Conc: 0.83 ng/ml

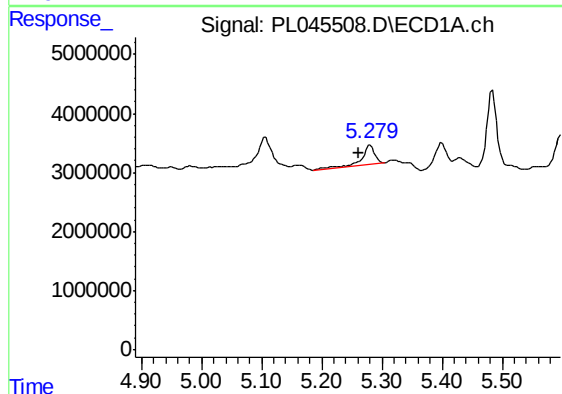


#25 Chlordane-3

R.T.: 5.281 min
Delta R.T.: 0.019 min
Response: 4859326
Conc: 4.24 ng/ml

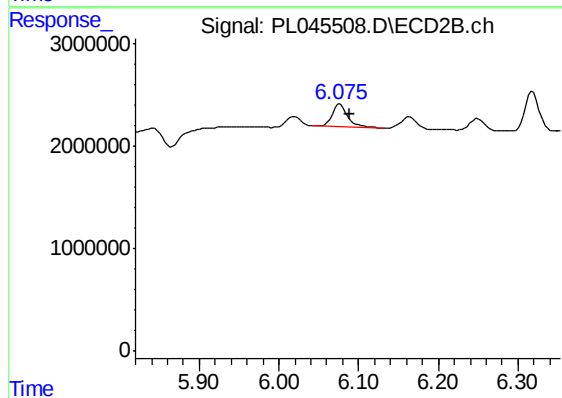

#25 Chlordane-3


R.T.: 6.076 min
Delta R.T.: -0.013 min
Response: 2980726
Conc: 7.65 ng/ml

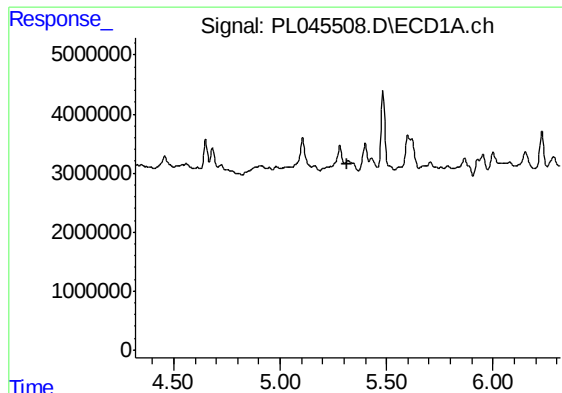

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.317 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PST-028-SW062-022719

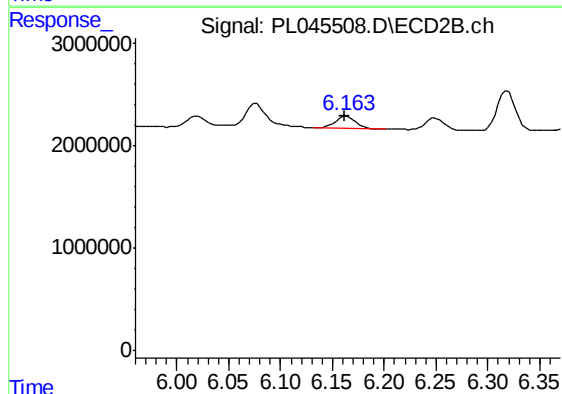


#26 Chlordane-4

R.T.: 6.164 min
Delta R.T.: 0.002 min
Response: 1632632
Conc: 3.49 ng/ml

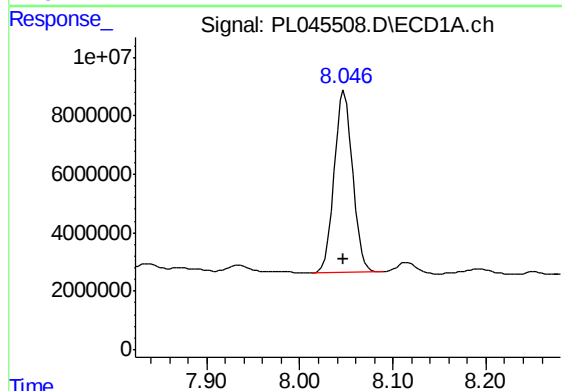

#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 85473331
Conc: 10.21 ng/ml

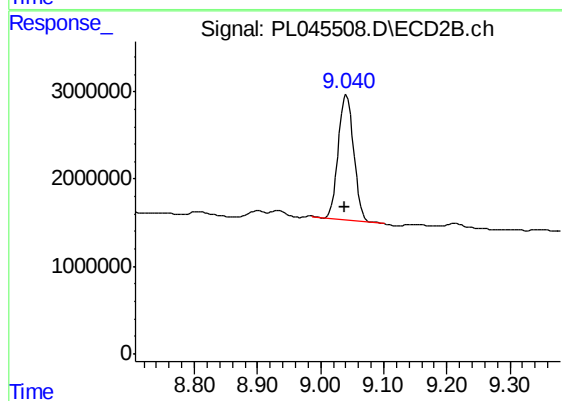

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 24326545
Conc: 10.65 ng/ml