

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
 Data File : PL045521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2019 02:21
 Operator : AJ\SJ
 Sample : K1715-13
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-4-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 04:30:27 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
 Quant Title : GC Extractables
 QLast Update : Wed Feb 27 17:00:03 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.363	3.982	131.2E6	41613158	19.067	19.431
28)	SA Decachlor...	8.047	9.041	139.3E6	41069583	16.651	17.974
Target Compounds							
9)	A Endosulfan I	5.359	6.192f	5685536	2307684	0.636	0.927 #
14)	MA Endrin	0.000	6.704f	0	1362866	N.D.	0.599 #
15)	B Endosulfa...	6.155f	6.910f	5733510	1732986	0.661	0.737
17)	MA 4,4'-DDT	6.239	0.000	13579941	0	1.811	N.D. #
26)	Chlordane-4	0.000	6.192f	0	2307684	N.D.	4.933 #
27)	Chlordane-5	6.155	0.000	5733510	0	16.602	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030519\
Data File : PL045521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2019 02:21
Operator : AJ\SJ
Sample : K1715-13
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-4-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 04:30:27 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022719.M
Quant Title : GC Extractables
QLast Update : Wed Feb 27 17:00:03 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

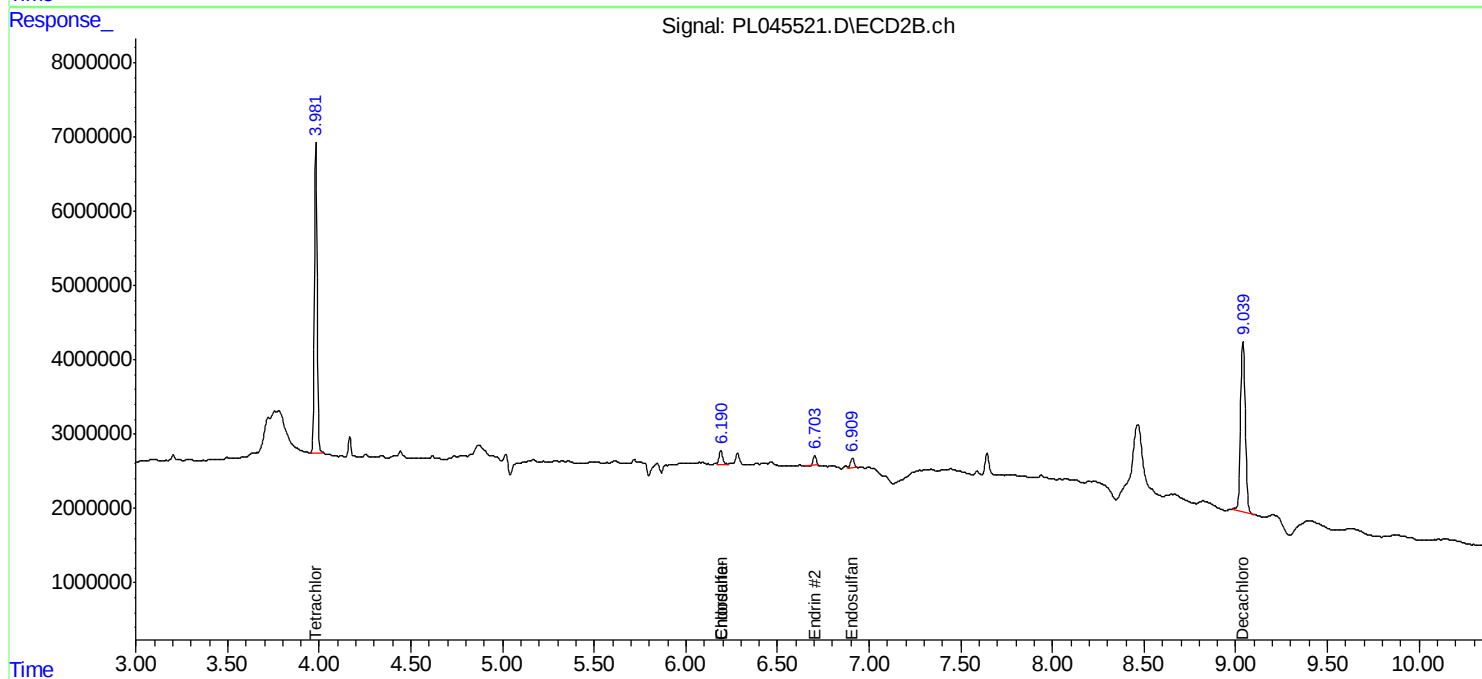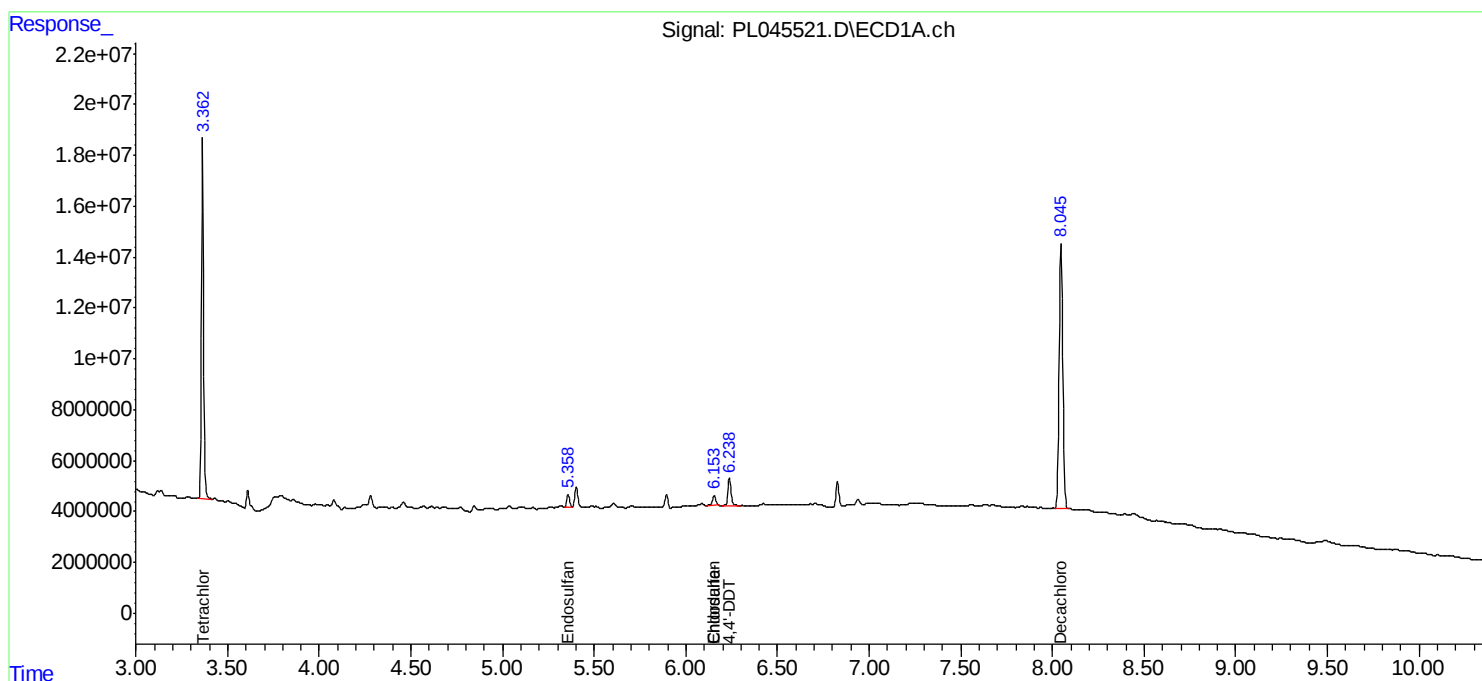


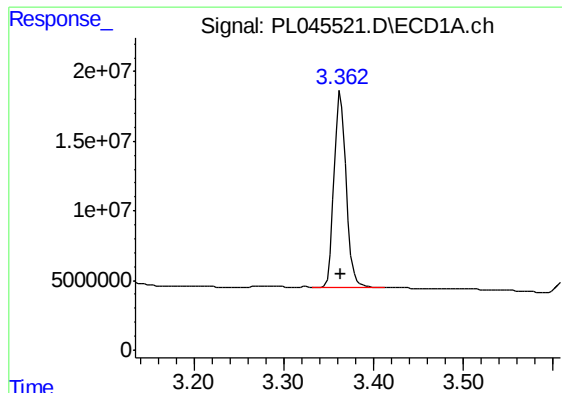

#1 Tetrachloro-m-xylene


R.T.: 3.363 min
Delta R.T.: 0.000 min
Response: 131163999
Conc: 19.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

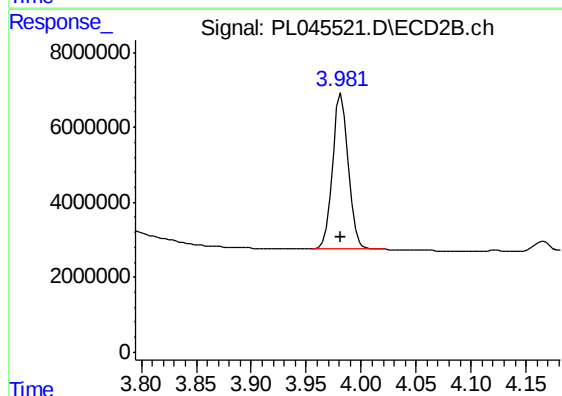


#1 Tetrachloro-m-xylene

R.T.: 3.982 min
Delta R.T.: 0.000 min
Response: 41613158
Conc: 19.43 ng/ml

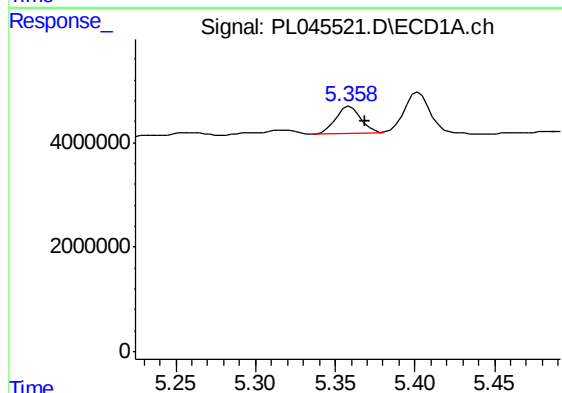


#9 Endosulfan I

R.T.: 5.359 min
Delta R.T.: -0.010 min
Response: 5685536
Conc: 0.64 ng/ml

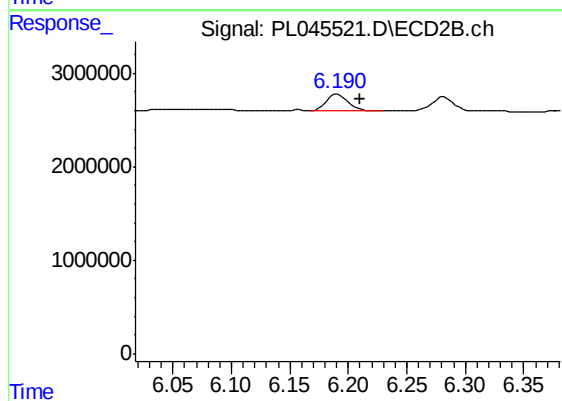

#9 Endosulfan I


R.T.: 6.192 min
Delta R.T.: -0.018 min
Response: 2307684
Conc: 0.93 ng/ml

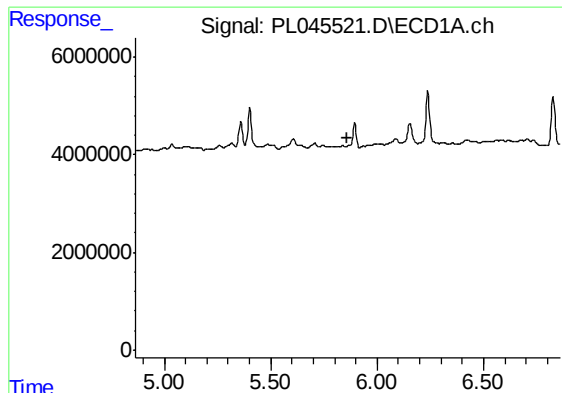

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 5.862 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-4-B

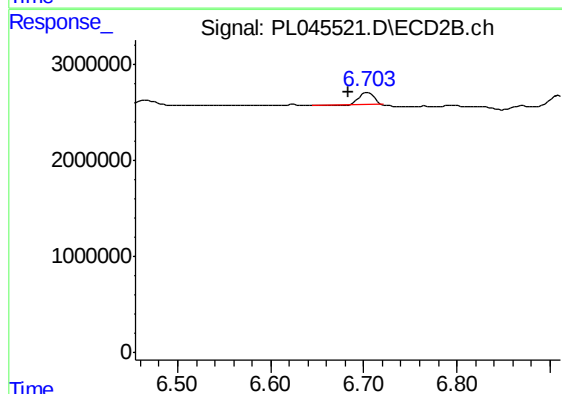


#14 Endrin

R.T.: 6.704 min
Delta R.T.: 0.020 min
Response: 1362866
Conc: 0.60 ng/ml

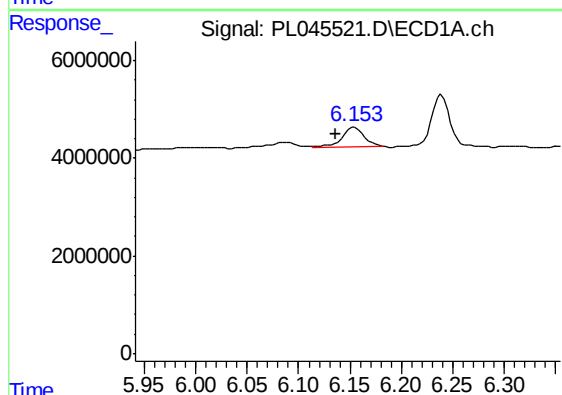


#15 Endosulfan II

R.T.: 6.155 min
Delta R.T.: 0.018 min
Response: 5733510
Conc: 0.66 ng/ml

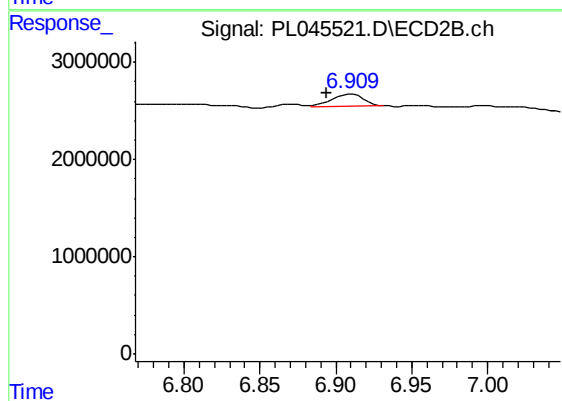

#15 Endosulfan II


R.T.: 6.910 min
Delta R.T.: 0.017 min
Response: 1732986
Conc: 0.74 ng/ml

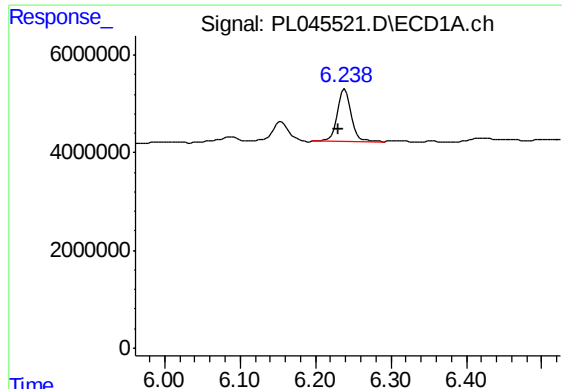

#17 4,4'-DDT


R.T.: 6.239 min
Delta R.T.: 0.008 min
Response: 13579941
Conc: 1.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

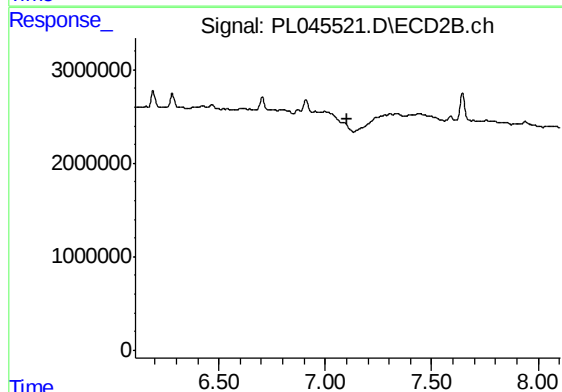


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

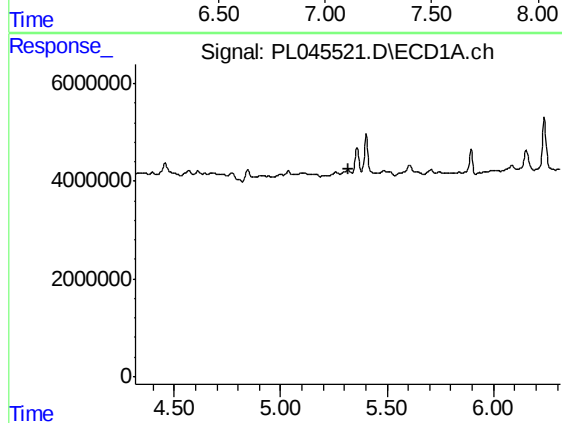


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.317 min
Response: 0
Conc: N.D.

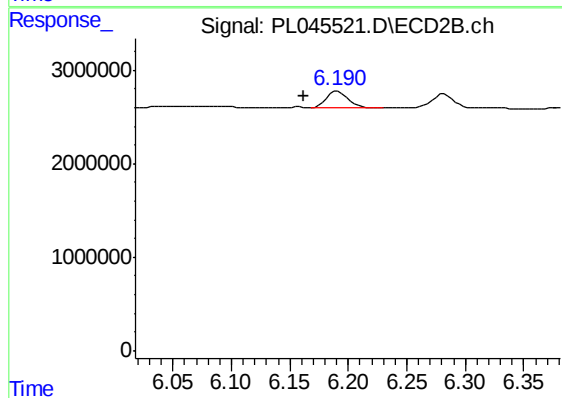

#26 Chlordane-4


R.T.: 6.192 min
Delta R.T.: 0.029 min
Response: 2307684
Conc: 4.93 ng/ml

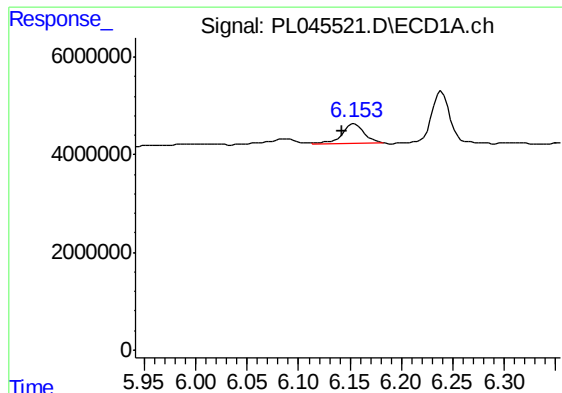

#27 Chlordane-5


R.T.: 6.155 min
Delta R.T.: 0.012 min
Response: 5733510
Conc: 16.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-4-B

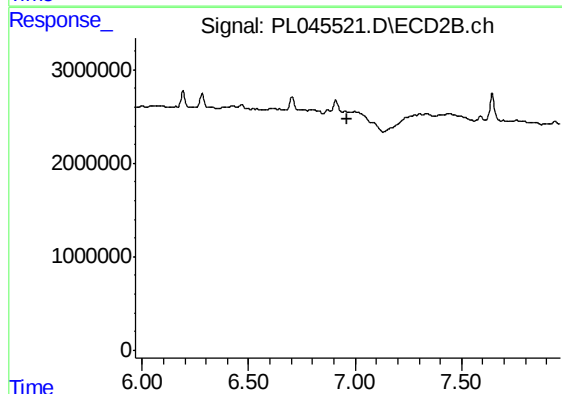


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.966 min
Response: 0
Conc: N.D.

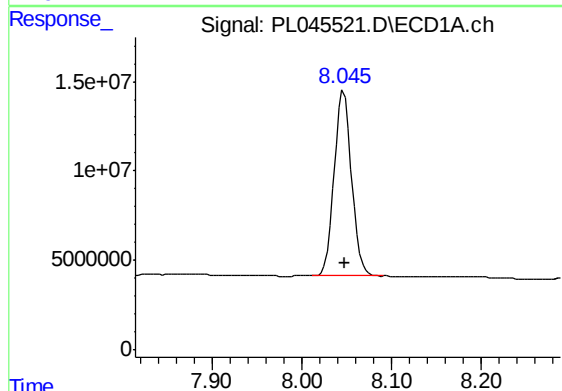

#28 Decachlorobiphenyl

R.T.: 8.047 min
Delta R.T.: 0.000 min
Response: 139328037
Conc: 16.65 ng/ml

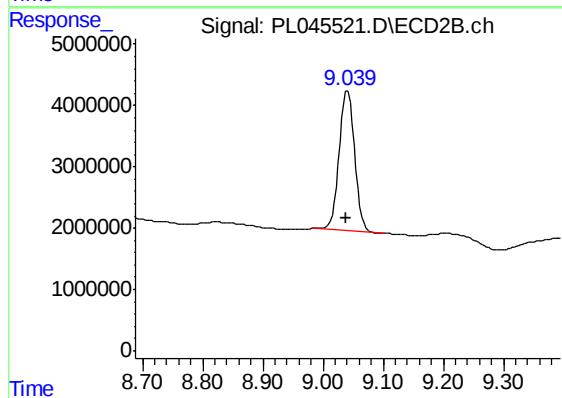

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: 0.002 min
Response: 41069583
Conc: 17.97 ng/ml