

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
 Data File : PL057075.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2020 11:33
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 03:13:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.956	199.1E6	50698726	23.364	23.763
28)	SA Decachlor...	8.211	8.980	206.4E6	43919065	21.350	20.670
Target Compounds							
5)	MB Aldrin	0.000	5.409f	0	720831	N.D.	0.241 #
8)	B Heptachlo...	0.000	5.810	0	17244065	N.D.	6.223 #
12)	B 4,4'-DDE	5.648f	0.000	15793589	0	1.348	N.D. #
14)	MA Endrin	0.000	6.645	0	7563174	N.D.	2.933 #
15)	B Endosulfa...	0.000	6.870	0	10887197	N.D.	3.880 #
17)	MA 4,4'-DDT	0.000	7.044f	0	5421596	N.D.	2.204 #
24)	Chlordane-2	0.000	5.409	0	720831	N.D.	7.552 #
27)	Chlordane-5	0.000	6.948f	0	28741469	N.D.	344.499 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
Data File : PL057075.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2020 11:33
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 03:13:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

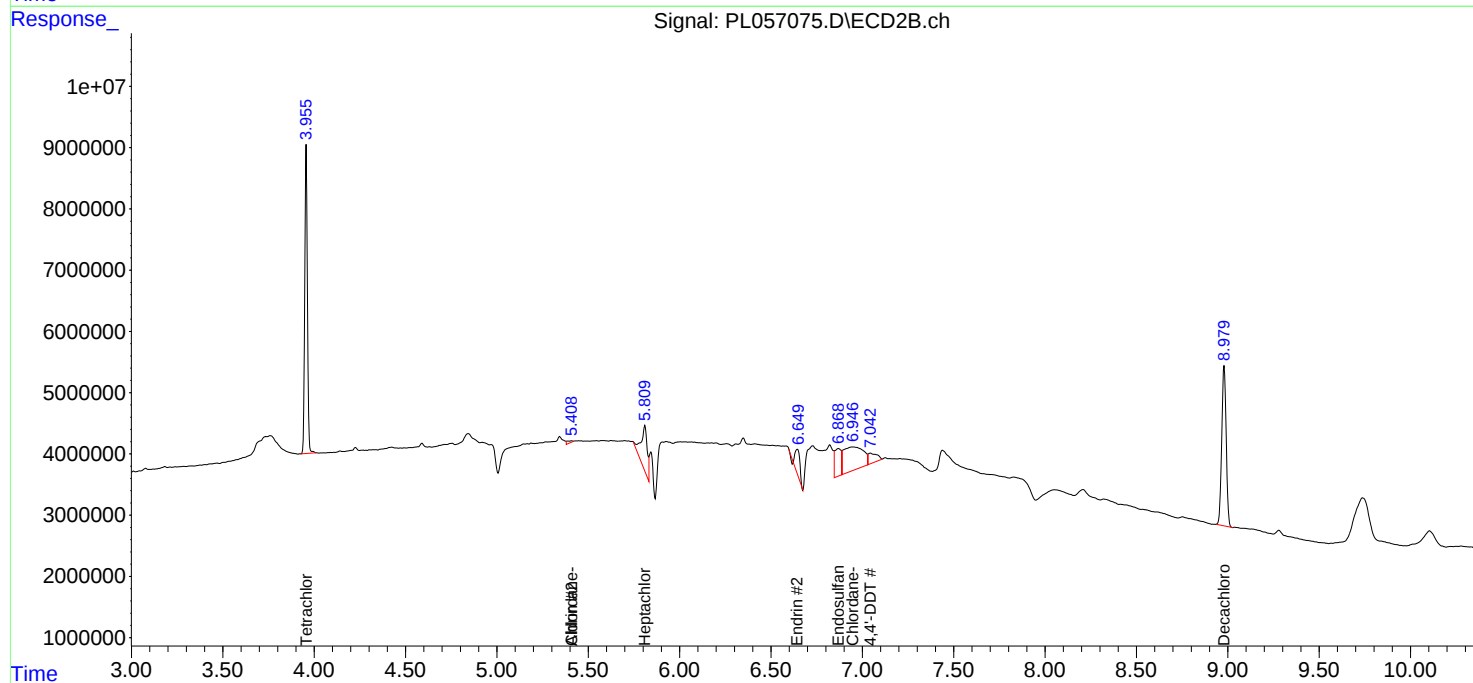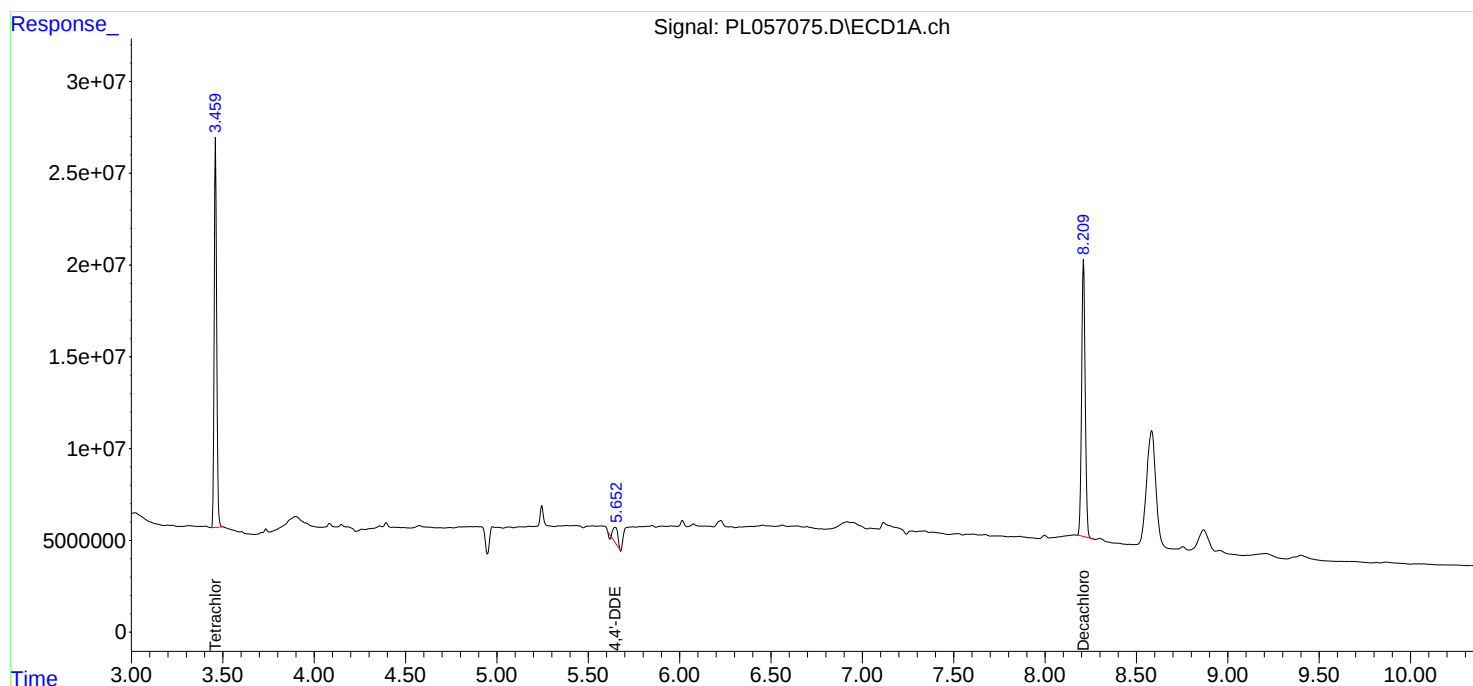


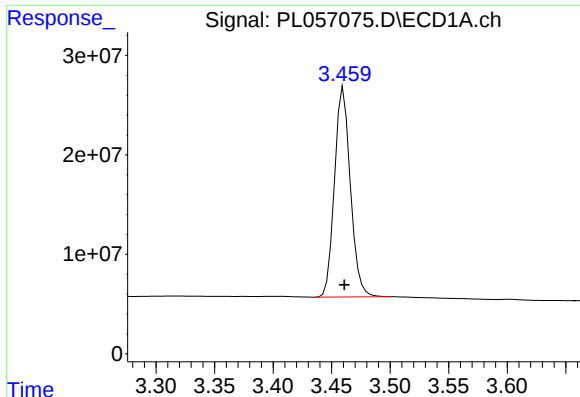

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 199117356
Conc: 23.36 ng/ml

Instrument :
ECD_L
ClientSampleId :

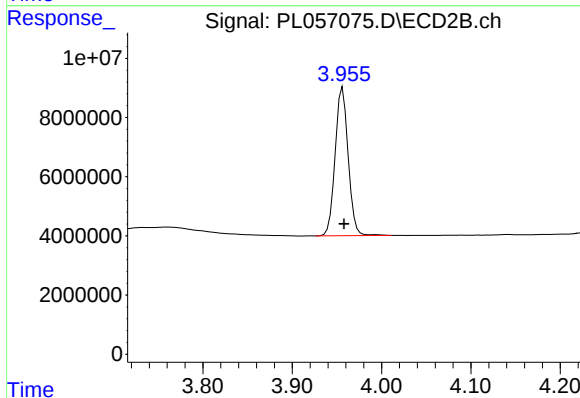


#1 Tetrachloro-m-xylene

R.T.: 3.956 min
Delta R.T.: -0.002 min
Response: 50698726
Conc: 23.76 ng/ml

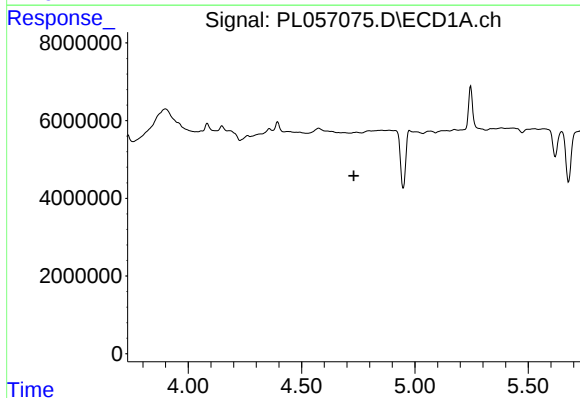


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 4.731 min
Response: 0
Conc: N.D.

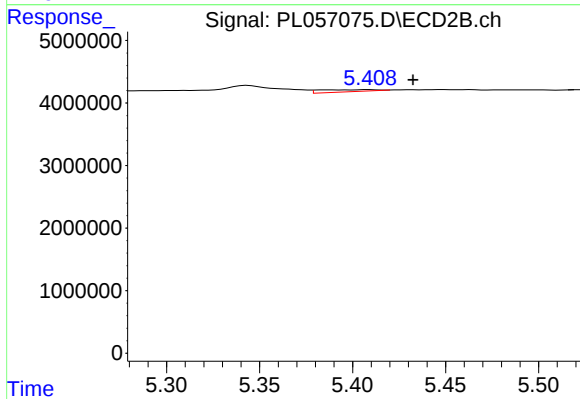

#5 Aldrin


R.T.: 5.409 min
Delta R.T.: -0.023 min
Response: 720831
Conc: 0.24 ng/ml

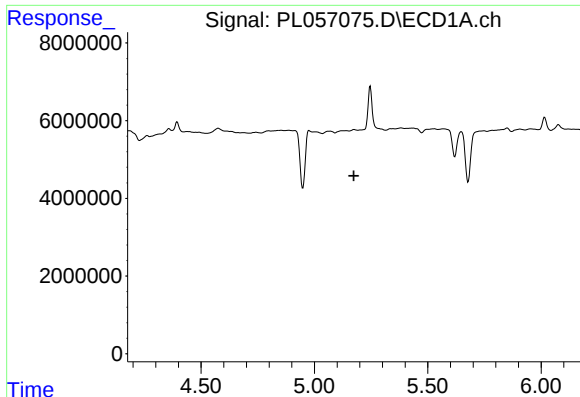

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.174 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

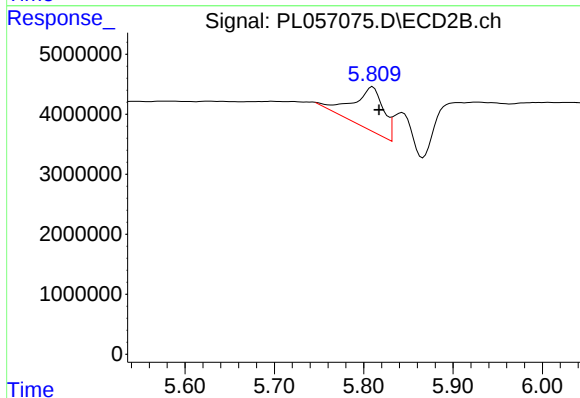


#8 Heptachlor epoxide

R.T.: 5.810 min
Delta R.T.: -0.007 min
Response: 17244065
Conc: 6.22 ng/ml

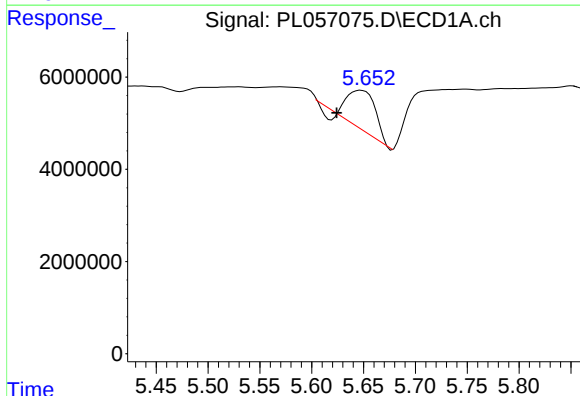


#12 4,4'-DDE

R.T.: 5.648 min
Delta R.T.: 0.024 min
Response: 15793589
Conc: 1.35 ng/ml

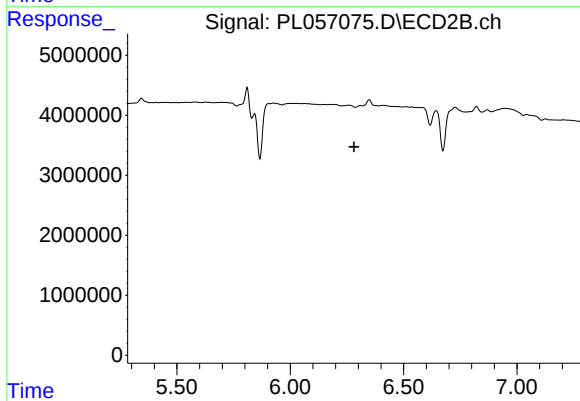

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

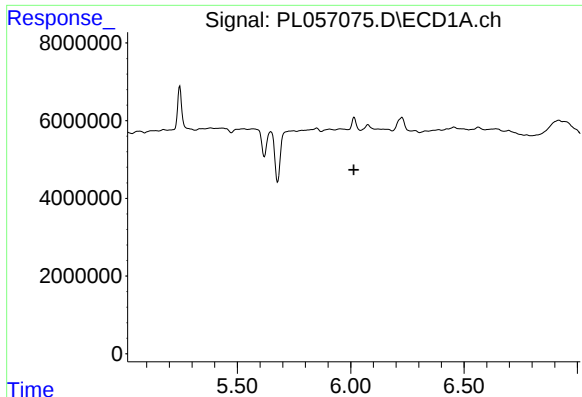

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.014 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

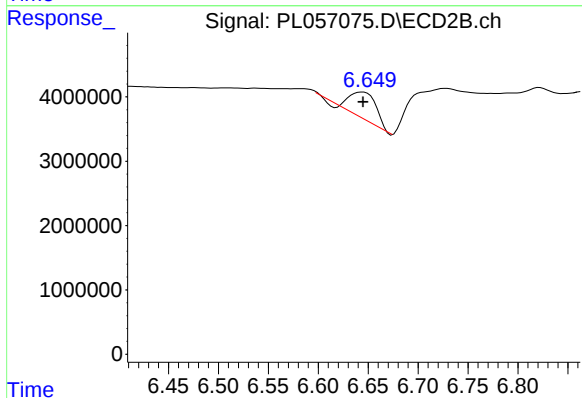


#14 Endrin

R.T.: 6.645 min
Delta R.T.: 0.000 min
Response: 7563174
Conc: 2.93 ng/ml

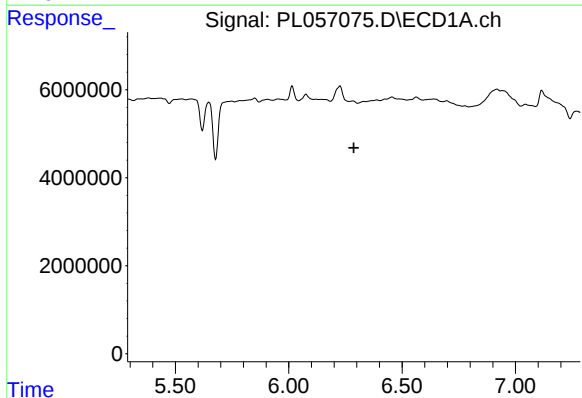


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

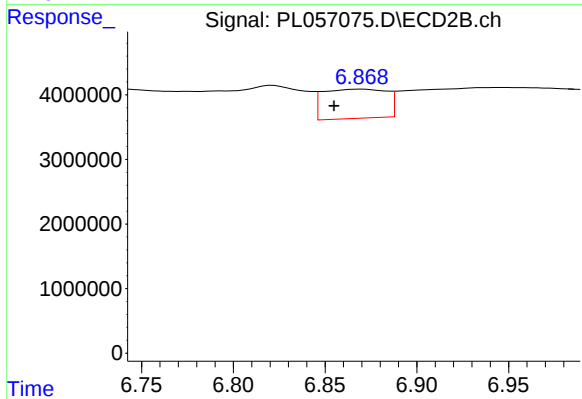

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 10887197
Conc: 3.88 ng/ml

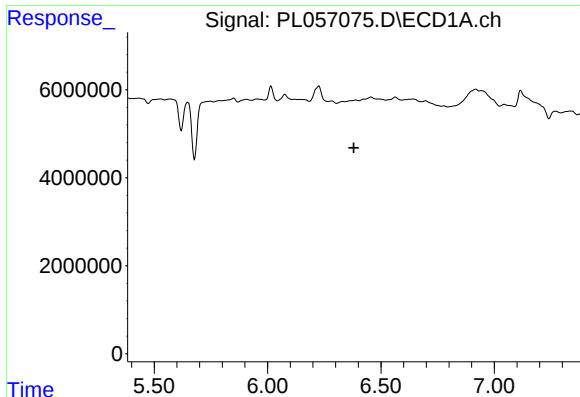

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.381 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

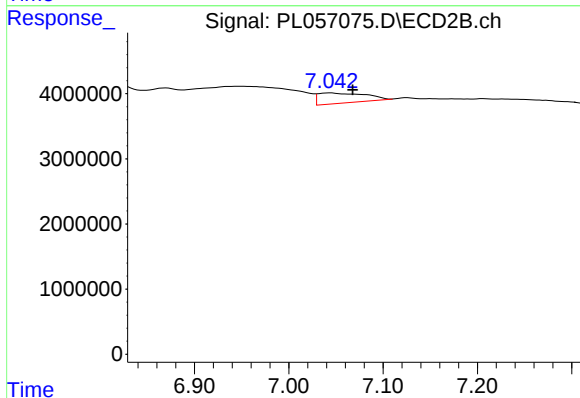


#17 4,4'-DDT

R.T.: 7.044 min
Delta R.T.: -0.023 min
Response: 5421596
Conc: 2.20 ng/ml

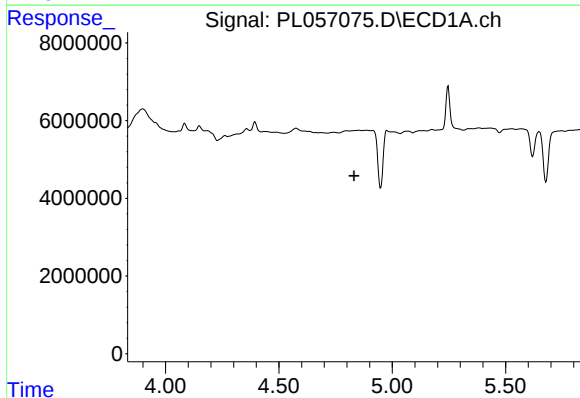


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 4.832 min
Response: 0
Conc: N.D.

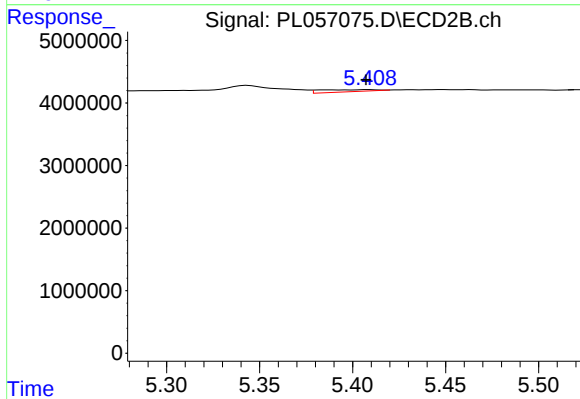

#24 Chlordane-2


R.T.: 5.409 min
Delta R.T.: 0.002 min
Response: 720831
Conc: 7.55 ng/ml

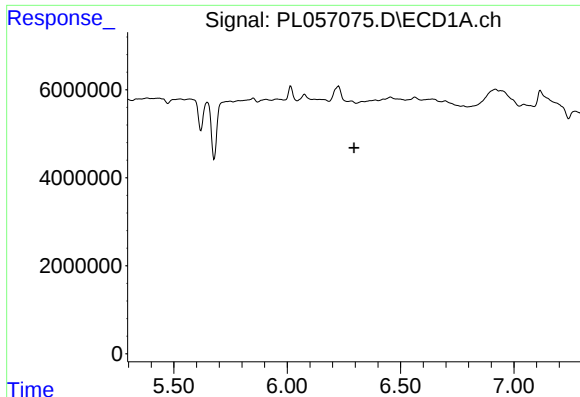

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.295 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

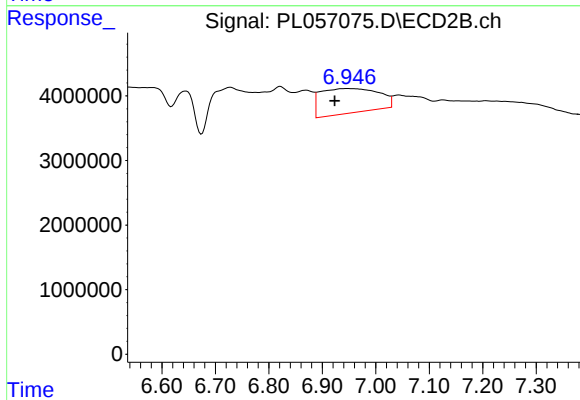


#27 Chlordane-5

R.T.: 6.948 min
Delta R.T.: 0.025 min
Response: 28741469
Conc: 344.50 ng/ml

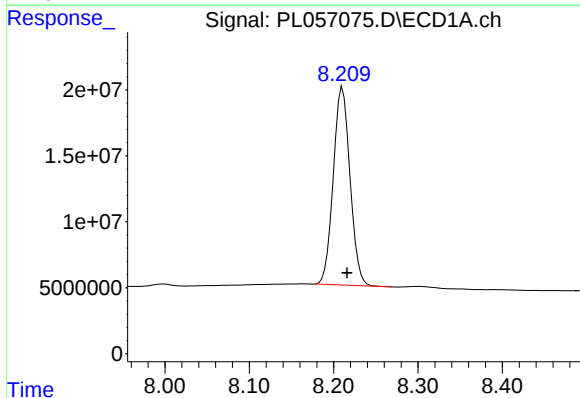

#28 Decachlorobiphenyl

R.T.: 8.211 min
Delta R.T.: -0.005 min
Response: 206351468
Conc: 21.35 ng/ml

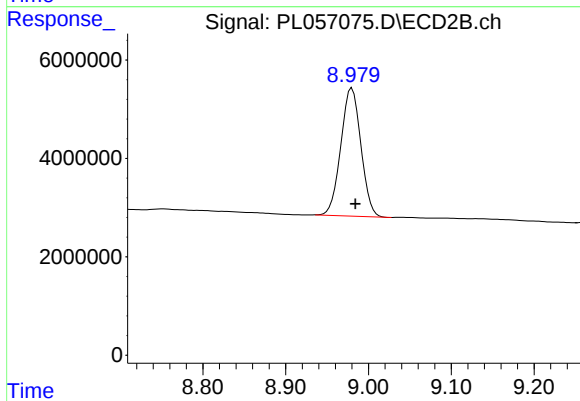

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.004 min
Response: 43919065
Conc: 20.67 ng/ml