

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
 Data File : PL057091.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2020 16:56
 Operator : AJ\MA
 Sample : L1778-21
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 03:16:51 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	114.0E6	31284768	13.382	14.663
28)	SA Decachlor...	8.208	8.981	133.6E6	30871974	13.826	14.530
Target Compounds							
10)	B gamma-Chl...	5.419f	0.000	10880713	0	0.876	N.D. #
11)	B alpha-Chl...	0.000	6.124	0	4454985	N.D.	1.478 #
17)	MA 4,4'-DDT	6.373	0.000	9048626	0	0.925	N.D. #
20)	A Methoxychlor	6.905f	0.000	13144304	0	2.636	N.D. #
25)	Chlordane-3	5.419f	0.000	10880713	0	10.088	N.D. #
26)	Chlordane-4	0.000	6.124	0	4454985	N.D.	9.716 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
Data File : PL057091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2020 16:56
Operator : AJ\MA
Sample : L1778-21
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 03:16:51 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

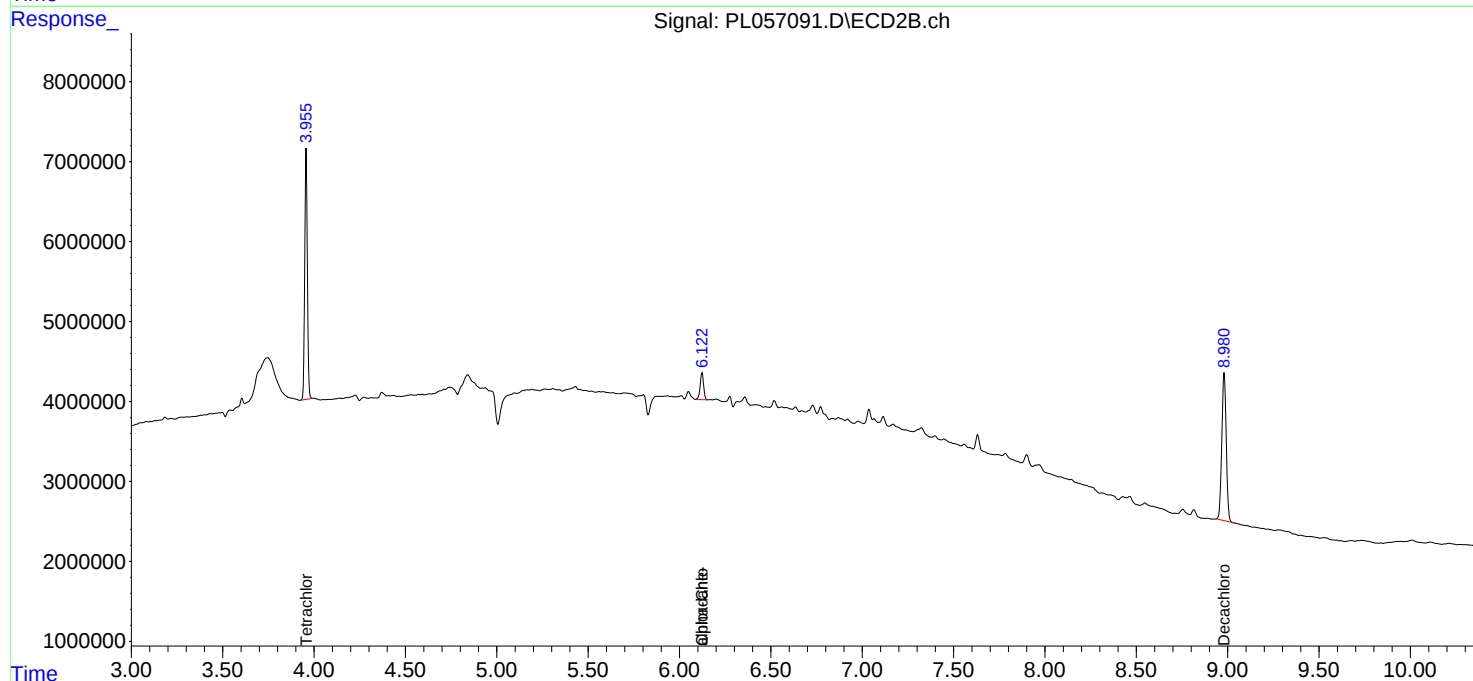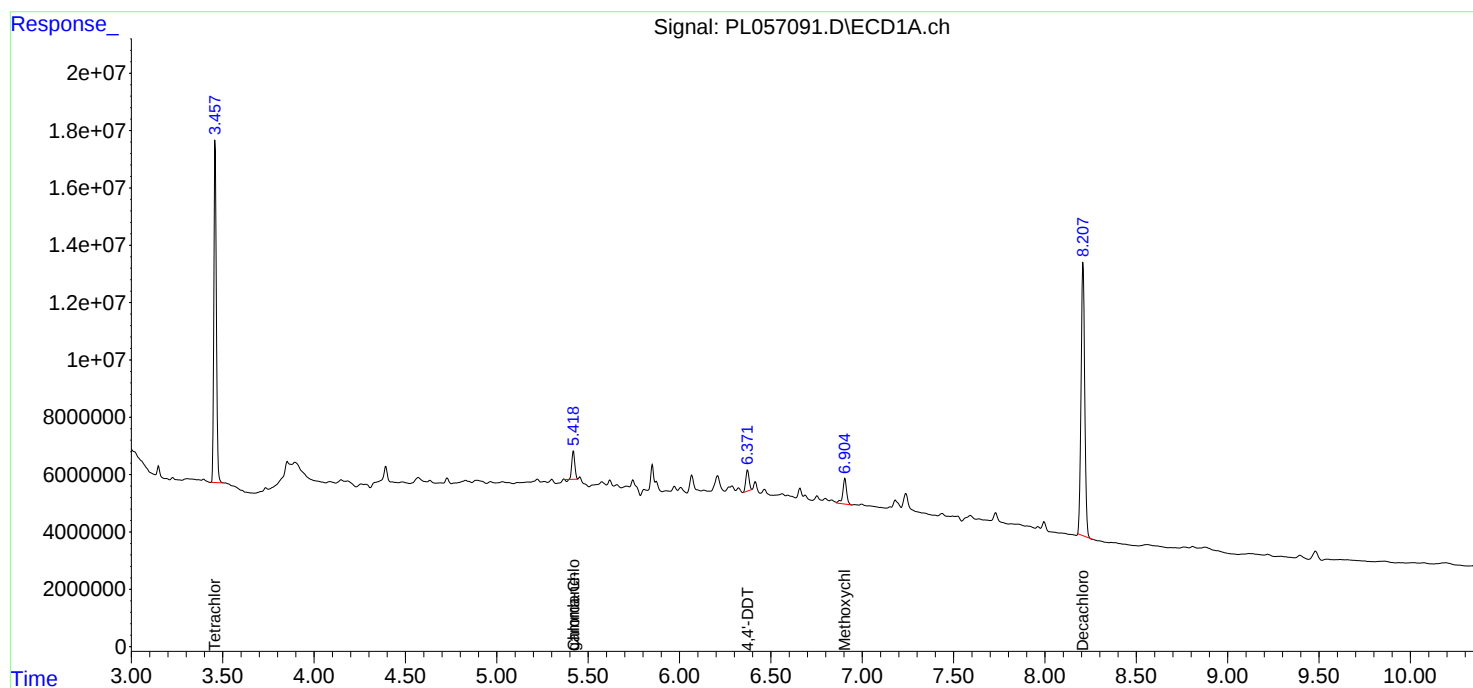


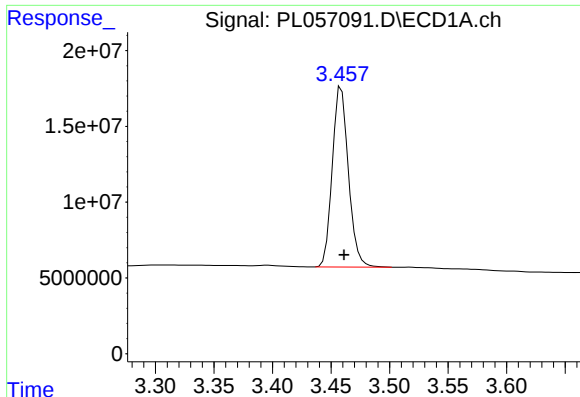

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 114044019
Conc: 13.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

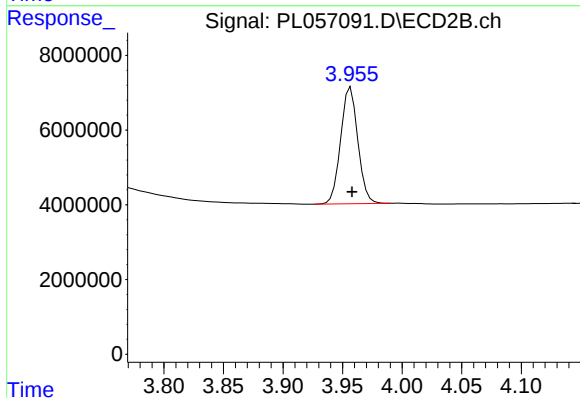


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 31284768
Conc: 14.66 ng/ml

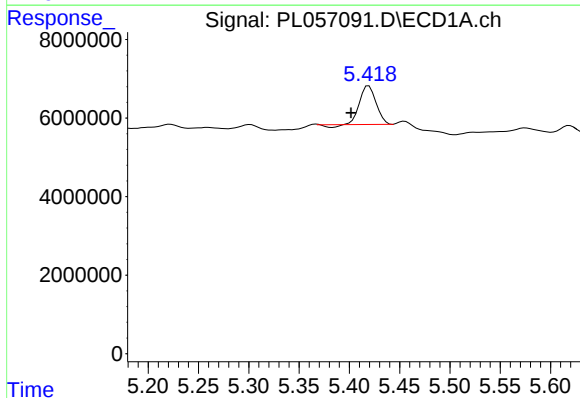


#10 gamma-Chlordane

R.T.: 5.419 min
Delta R.T.: 0.018 min
Response: 10880713
Conc: 0.88 ng/ml

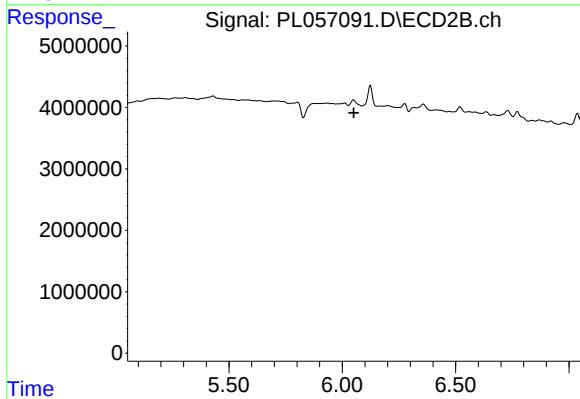

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.051 min
Response: 0
Conc: N.D.

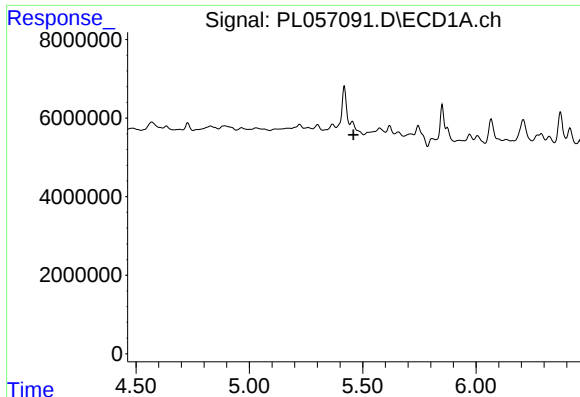

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

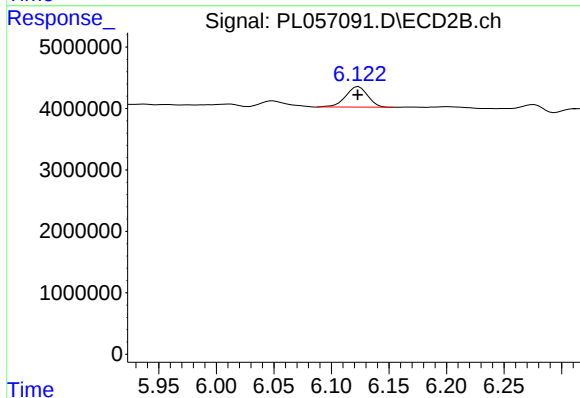


#11 alpha-Chlordane

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 4454985
Conc: 1.48 ng/ml

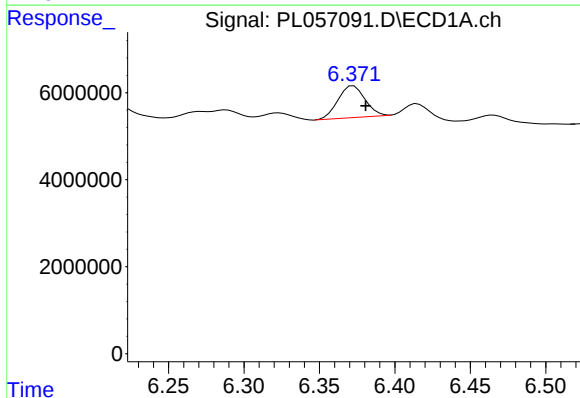


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.008 min
Response: 9048626
Conc: 0.92 ng/ml

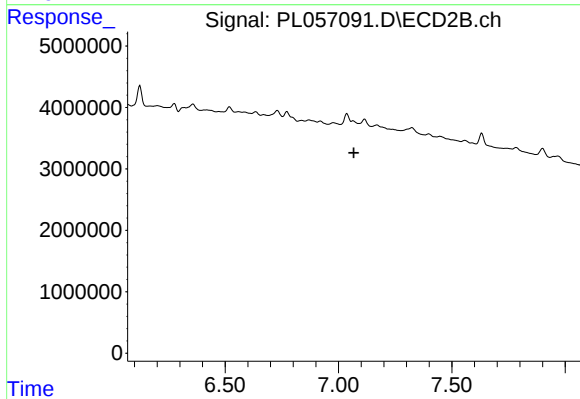

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.068 min
Response: 0
Conc: N.D.

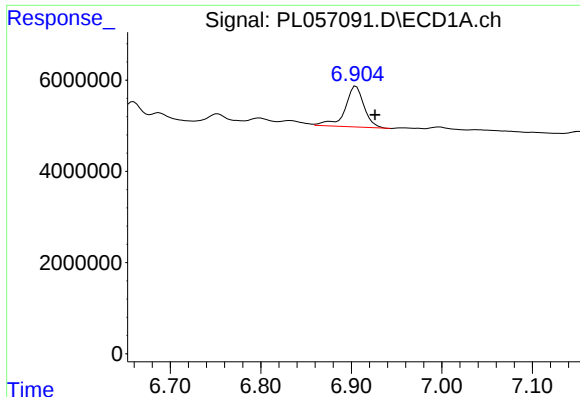

#20 Methoxychlor


R.T.: 6.905 min
Delta R.T.: -0.021 min
Response: 13144304
Conc: 2.64 ng/ml

Instrument :
ECD_L
ClientSampleId :

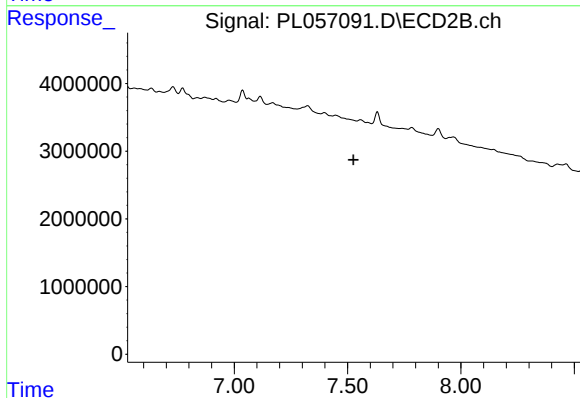


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.527 min
Response: 0
Conc: N.D.

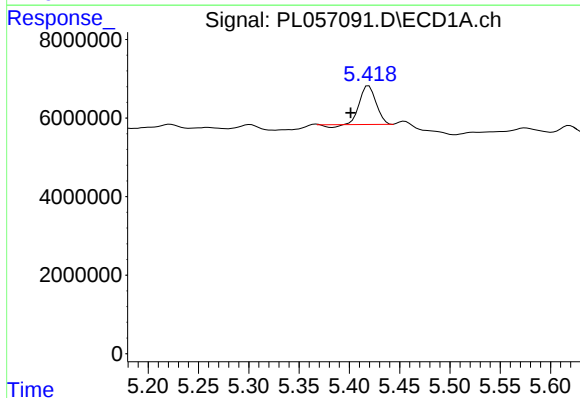


#25 Chlordane-3

R.T.: 5.419 min
Delta R.T.: 0.018 min
Response: 10880713
Conc: 10.09 ng/ml

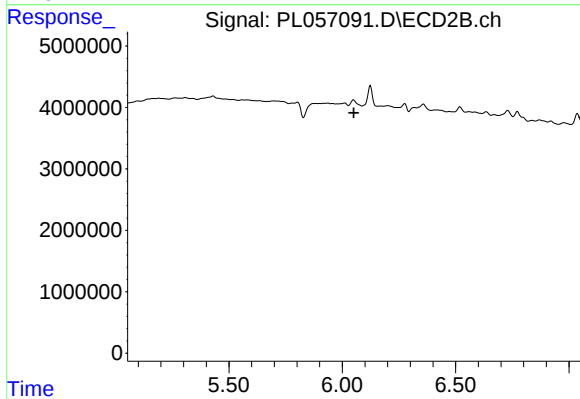

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

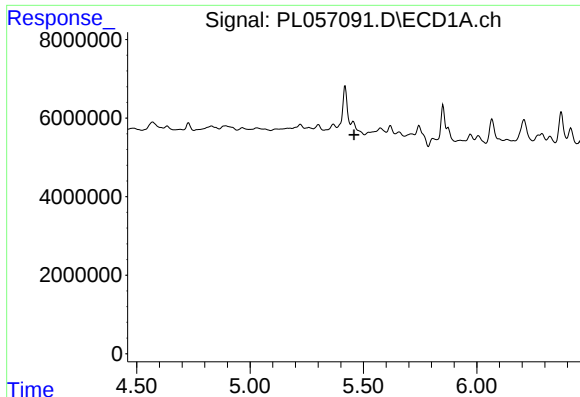

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

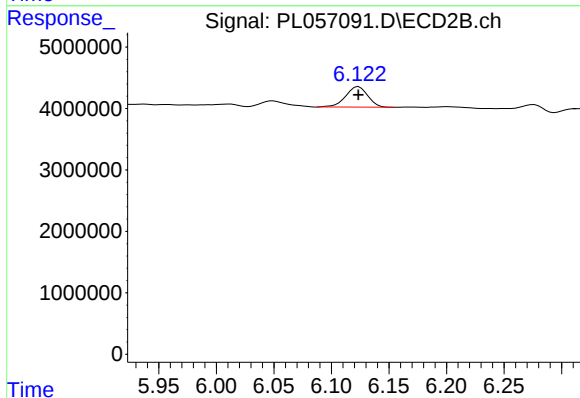


#26 Chlordane-4

R.T.: 6.124 min
Delta R.T.: 0.000 min
Response: 4454985
Conc: 9.72 ng/ml

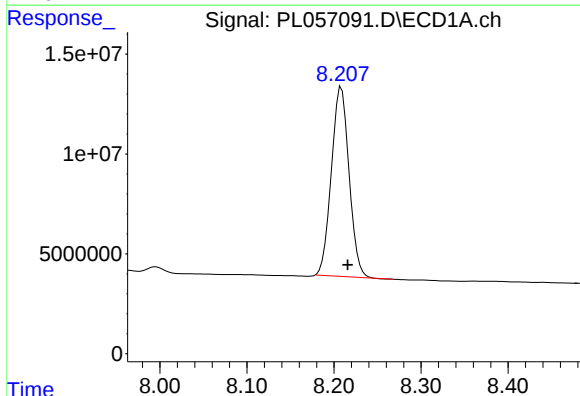

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.007 min
Response: 133628360
Conc: 13.83 ng/ml

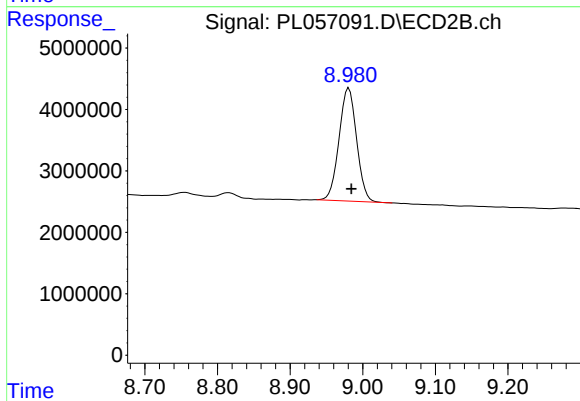

#28 Decachlorobiphenyl

R.T.: 8.981 min
Delta R.T.: -0.003 min
Response: 30871974
Conc: 14.53 ng/ml