

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
 Data File : PL057092.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2020 17:10
 Operator : AJ\MA
 Sample : L1778-23
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 S9

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 03:17:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	111.9E6	31144754	13.129	14.598
28)	SA Decachlor...	8.206	8.980	146.4E6	25941443	15.146	12.209
Target Compounds							
10)	B gamma-Chl...	5.419f	6.049	11731786	553223	0.945	0.185 #
11)	B alpha-Chl...	0.000	6.123	0	3115904	N.D.	1.034 #
13)	MA Dieldrin	5.745	0.000	25022591	0	2.047	N.D. #
16)	A 4,4'-DDD	0.000	6.773	0	6475741	N.D.	2.658 #
17)	MA 4,4'-DDT	6.373	0.000	27110446	0	2.771	N.D. #
19)	B Endosulfa...	6.659	0.000	3676597	0	0.368	N.D. #
20)	A Methoxychlor	6.905f	0.000	27067344	0	5.428	N.D. #
25)	Chlordane-3	5.419f	6.049	11731786	553223	10.877	1.460 #
26)	Chlordane-4	0.000	6.123	0	3115904	N.D.	6.795 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
Data File : PL057092.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2020 17:10
Operator : AJ\MA
Sample : L1778-23
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
S9

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 03:17:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

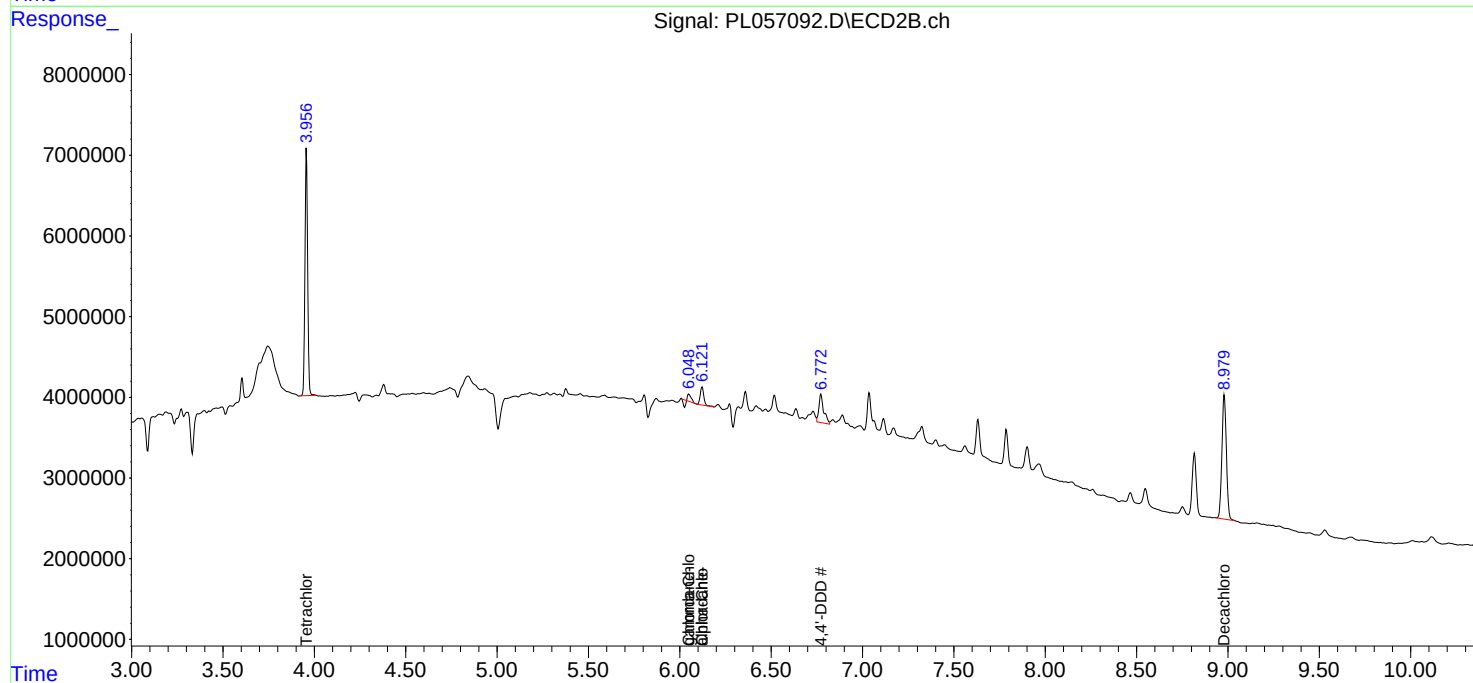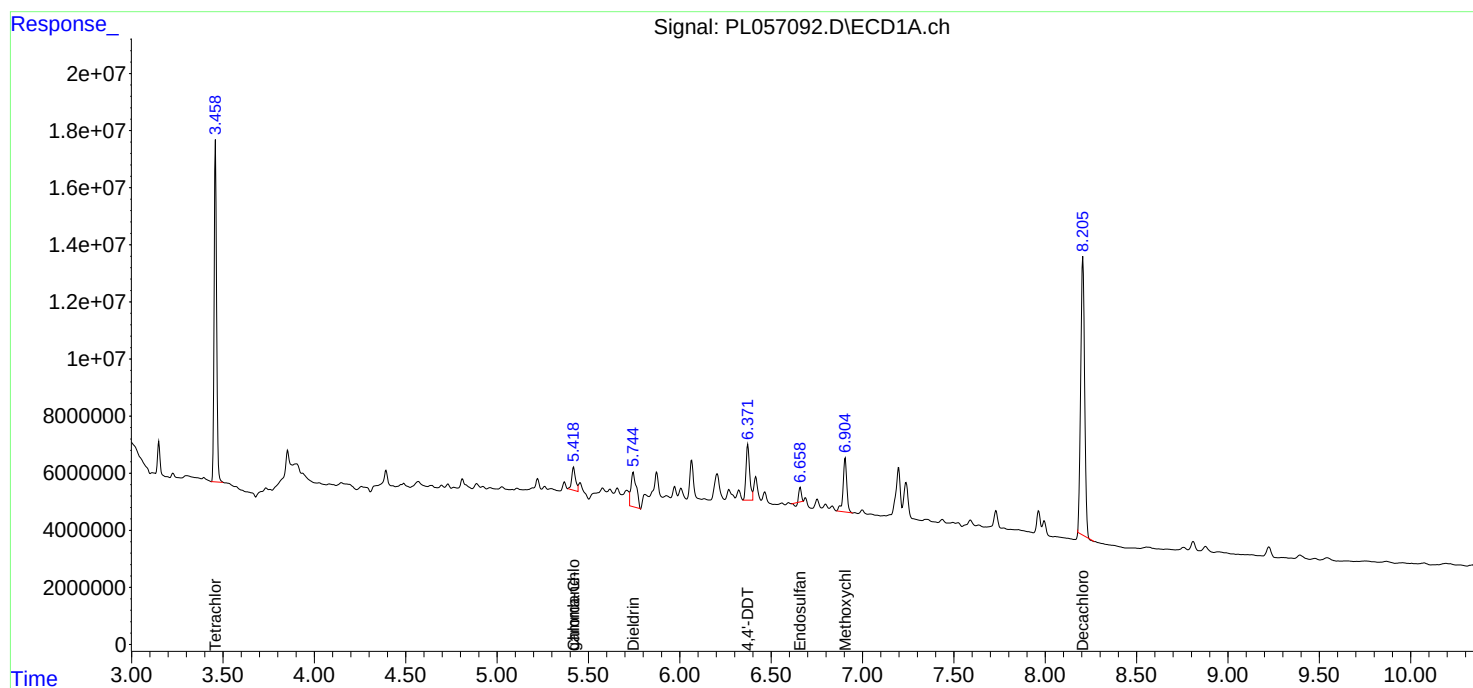


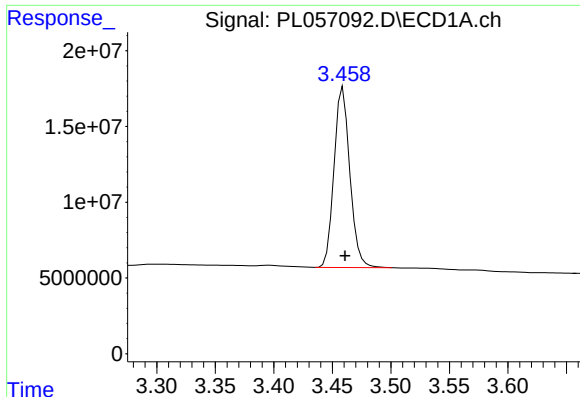

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 111888338
Conc: 13.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
S9

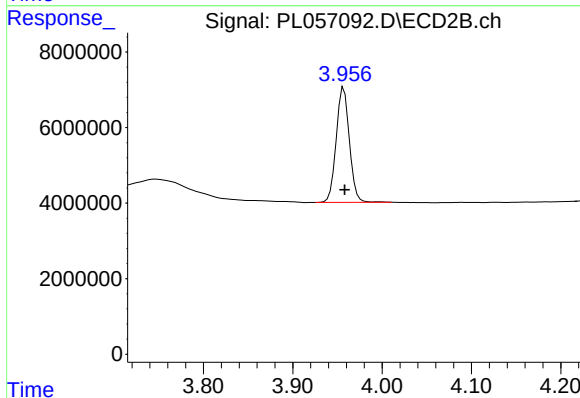


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: 0.000 min
Response: 31144754
Conc: 14.60 ng/ml

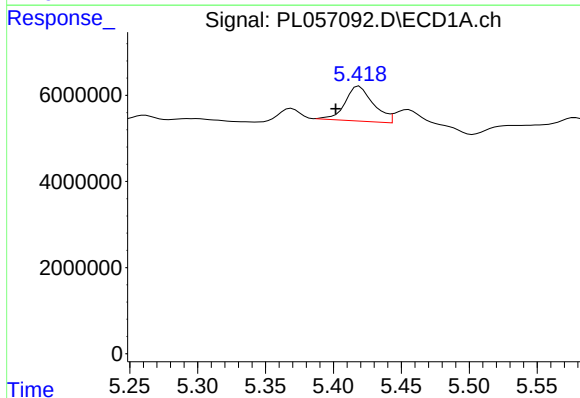


#10 gamma-Chlordane

R.T.: 5.419 min
Delta R.T.: 0.017 min
Response: 11731786
Conc: 0.94 ng/ml

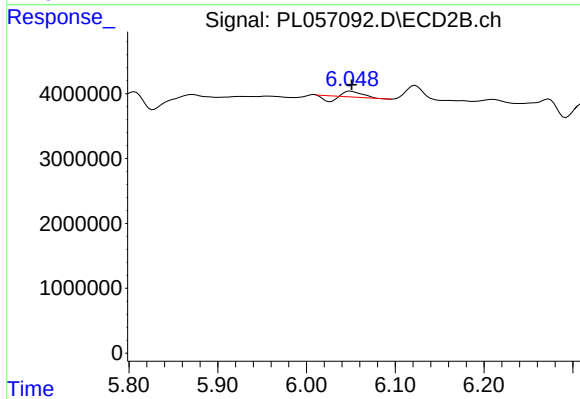

#10 gamma-Chlordane


R.T.: 6.049 min
Delta R.T.: -0.001 min
Response: 553223
Conc: 0.18 ng/ml

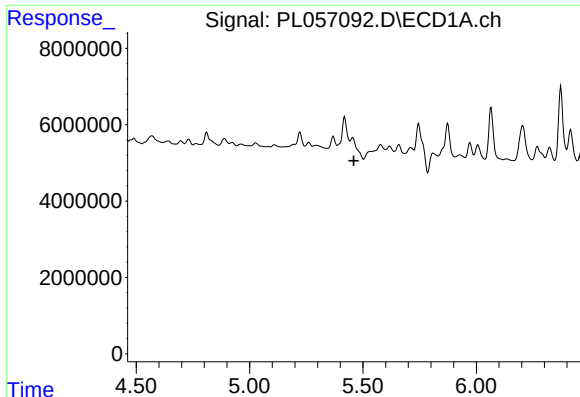

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.460 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S9

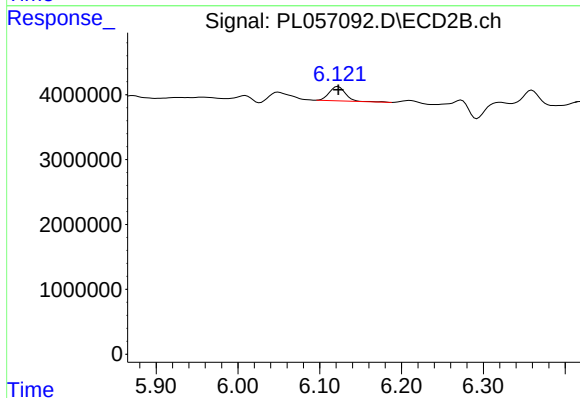


#11 alpha-Chlordane

R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 3115904
Conc: 1.03 ng/ml

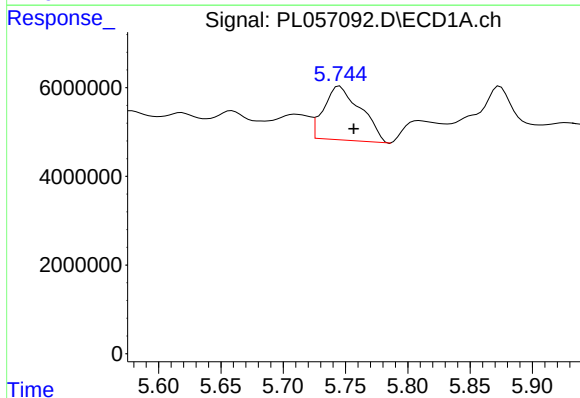


#13 Dieldrin

R.T.: 5.745 min
Delta R.T.: -0.011 min
Response: 25022591
Conc: 2.05 ng/ml

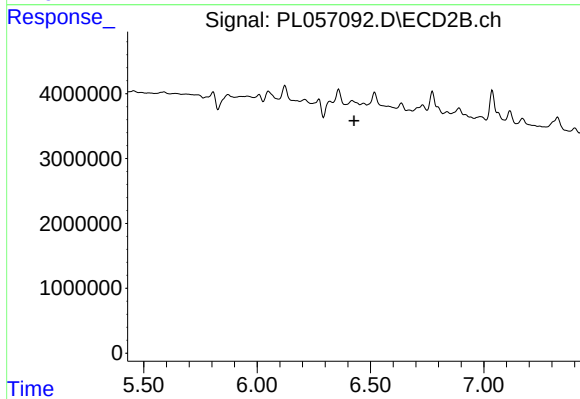

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.428 min
Response: 0
Conc: N.D.

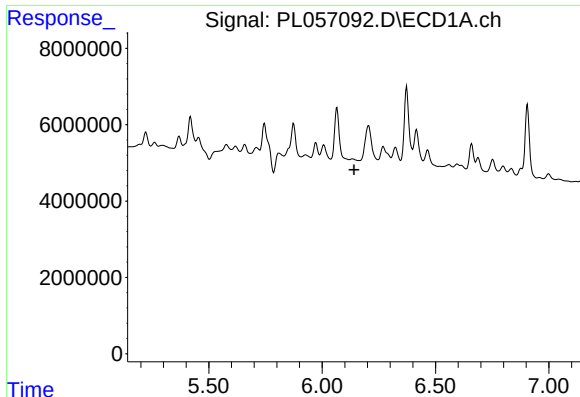

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
S9

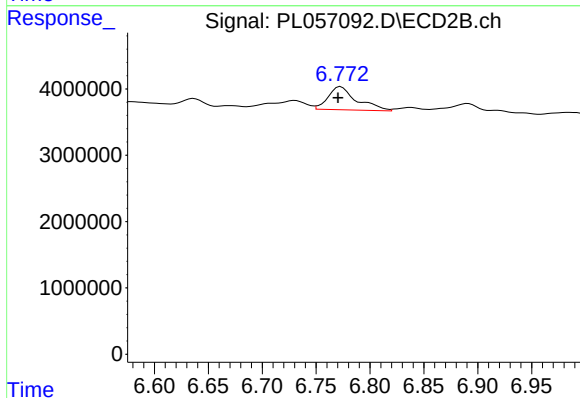


#16 4,4'-DDD

R.T.: 6.773 min
Delta R.T.: 0.002 min
Response: 6475741
Conc: 2.66 ng/ml

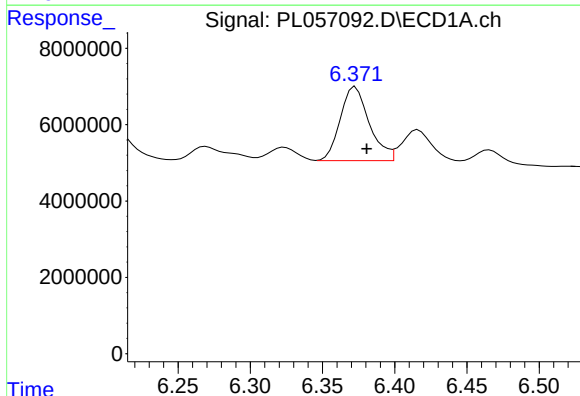


#17 4,4'-DDT

R.T.: 6.373 min
Delta R.T.: -0.008 min
Response: 27110446
Conc: 2.77 ng/ml

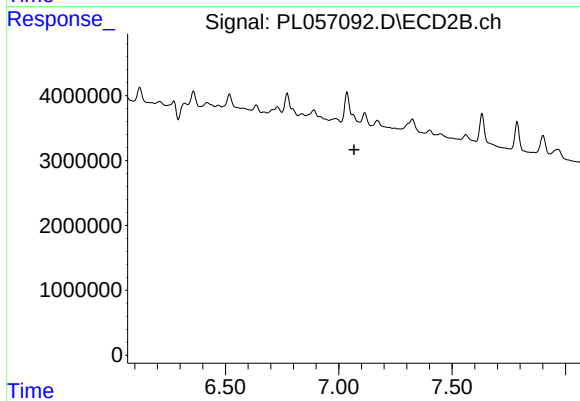

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.068 min
Response: 0
Conc: N.D.

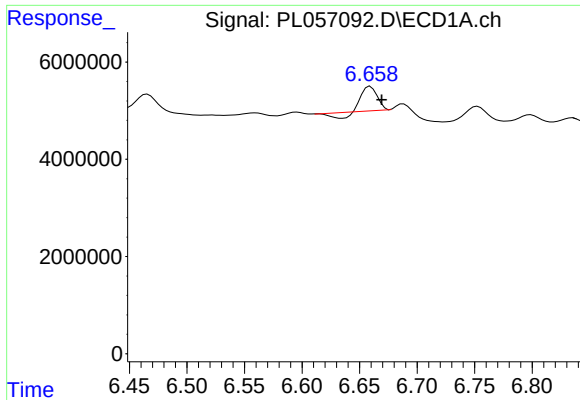

#19 Endosulfan Sulfate


R.T.: 6.659 min
Delta R.T.: -0.010 min
Response: 3676597
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
S9

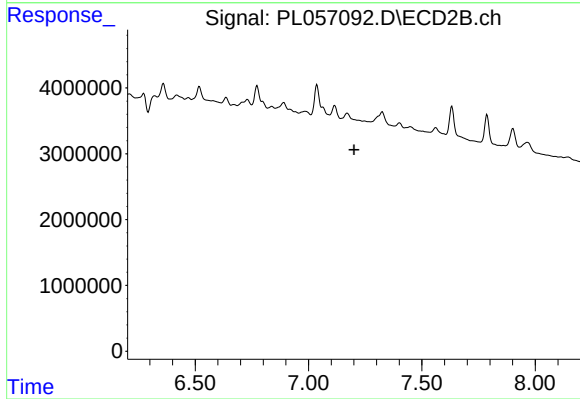


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.201 min
Response: 0
Conc: N.D.

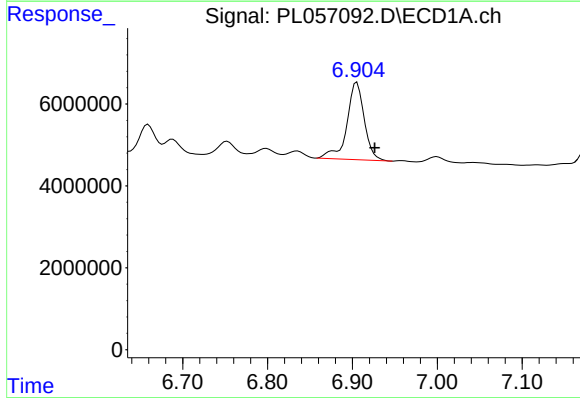


#20 Methoxychlor

R.T.: 6.905 min
Delta R.T.: -0.021 min
Response: 27067344
Conc: 5.43 ng/ml

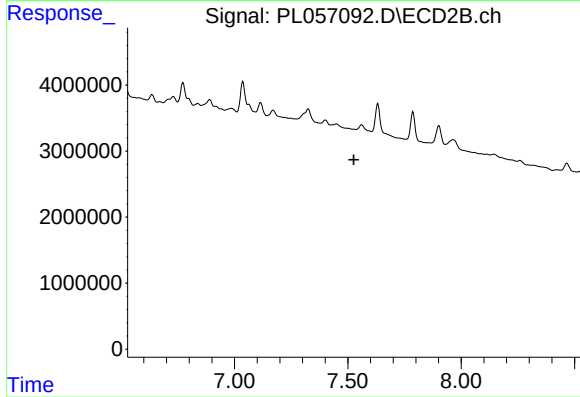

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.527 min
Response: 0
Conc: N.D.

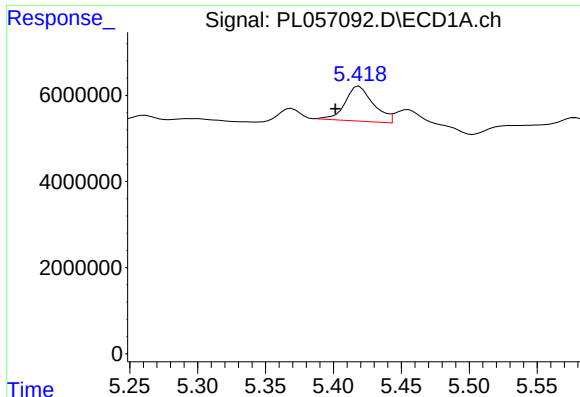

#25 Chlordane-3


R.T.: 5.419 min
Delta R.T.: 0.017 min
Response: 11731786
Conc: 10.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
S9

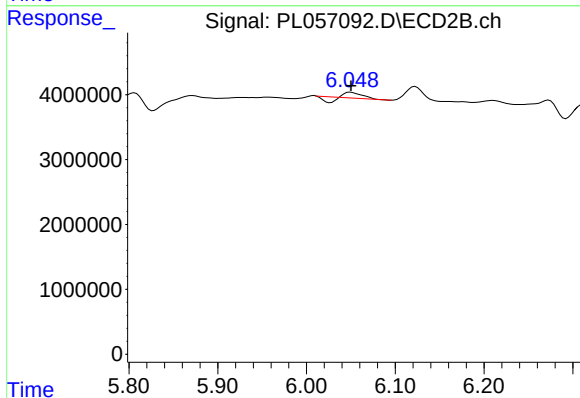


#25 Chlordane-3

R.T.: 6.049 min
Delta R.T.: 0.000 min
Response: 553223
Conc: 1.46 ng/ml

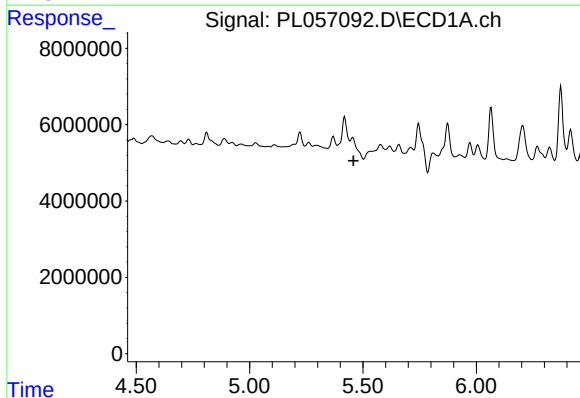


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

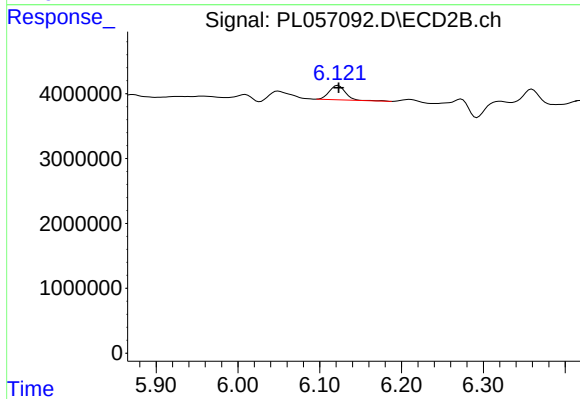

#26 Chlordane-4


R.T.: 6.123 min
Delta R.T.: 0.000 min
Response: 3115904
Conc: 6.80 ng/ml

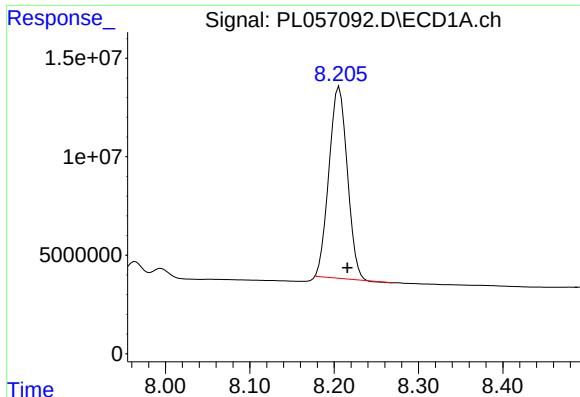

#28 Decachlorobiphenyl

R.T.: 8.206 min
Delta R.T.: -0.010 min
Response: 146386093
Conc: 15.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
S9

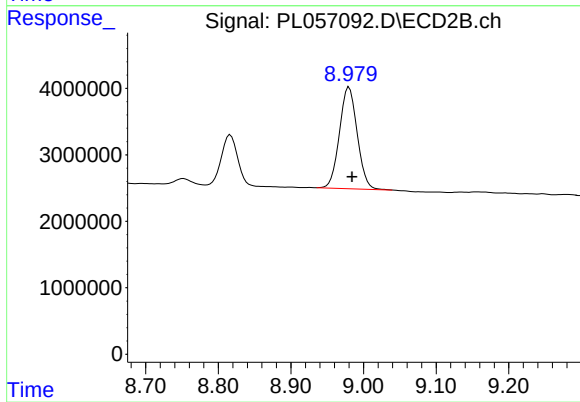

#28 Decachlorobiphenyl

R.T.: 8.980 min
Delta R.T.: -0.004 min
Response: 25941443
Conc: 12.21 ng/ml