

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
 Data File : PL057093.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2020 17:24
 Operator : AJ\MA
 Sample : L1792-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 03:17:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.459	3.957	201.0E6	52326775	23.585	24.526
28)	SA Decachlor...	8.208	8.982	192.6E6	44367256	19.927	20.881
Target Compounds							
2)	A alpha-BHC	3.902	0.000	5250149	0	0.354	N.D. #
3)	MA gamma-BHC...	4.192	0.000	157.8E6	0	11.484	N.D. #
5)	MB Aldrin	4.711f	5.421	-89505464	1667.7E6	N.D.	557.910
9)	A Endosulfan I	0.000	6.194f	0	1668133	N.D.	0.597 #
15)	B Endosulfa...	0.000	6.869	0	17339640	N.D.	6.179 #
17)	MA 4,4'-DDT	6.372	0.000	9052561	0	0.925	N.D. #
21)	B Endrin ke...	0.000	7.668	0	4303081	N.D.	1.570 #
24)	Chlordane-2	0.000	5.421	0	1667.7E6	N.D.	17471.196 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030520\
Data File : PL057093.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2020 17:24
Operator : AJ\MA
Sample : L1792-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
TP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 03:17:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

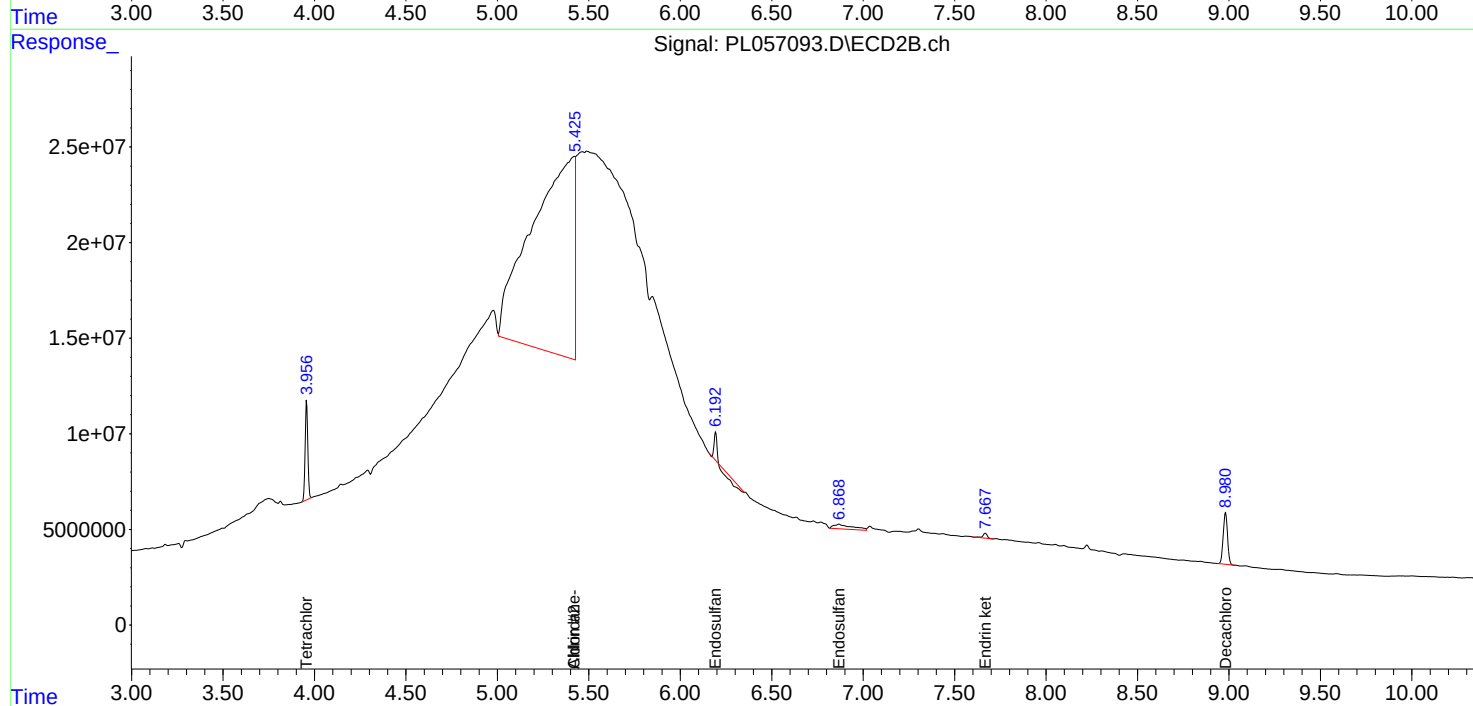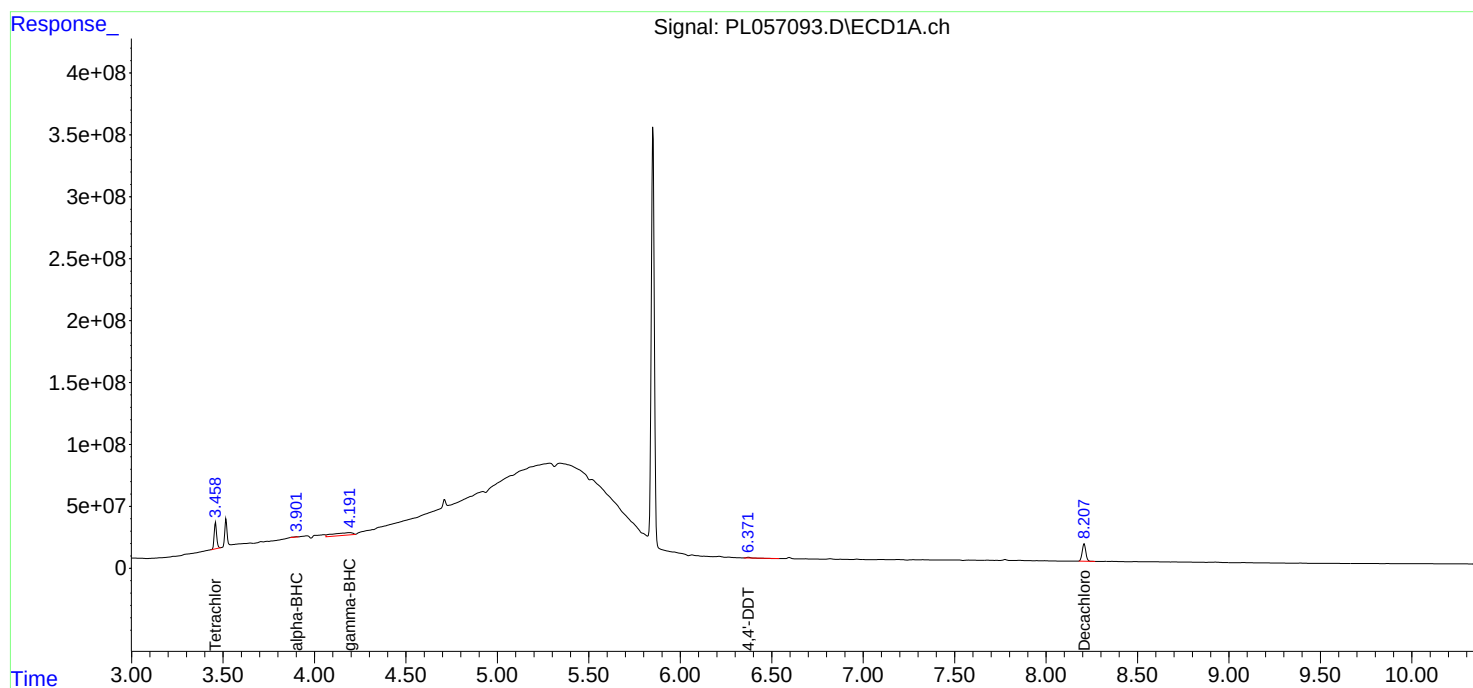


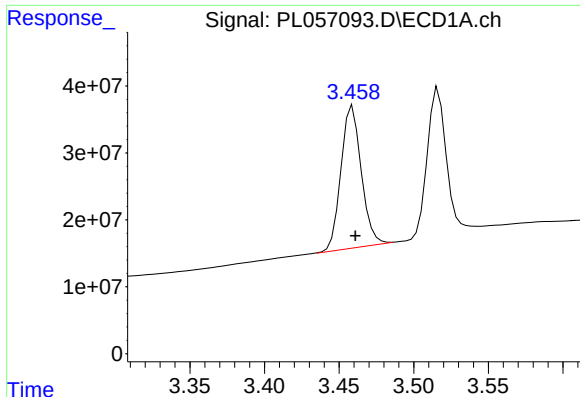

#1 Tetrachloro-m-xylene


R.T.: 3.459 min
Delta R.T.: -0.002 min
Response: 200997922
Conc: 23.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

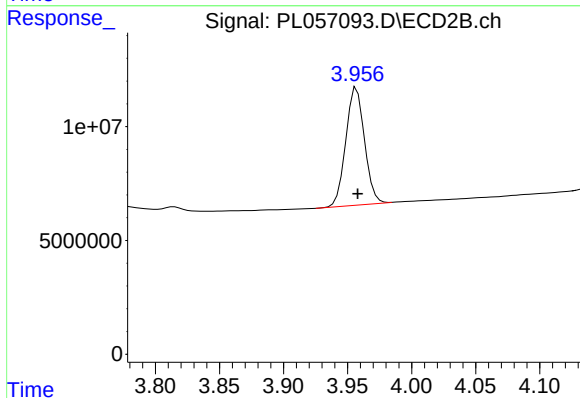


#1 Tetrachloro-m-xylene

R.T.: 3.957 min
Delta R.T.: -0.001 min
Response: 52326775
Conc: 24.53 ng/ml

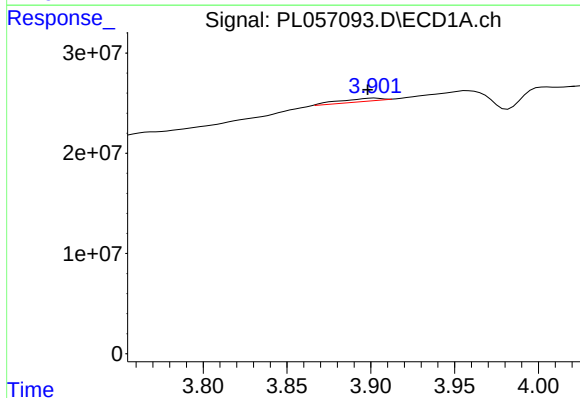


#2 alpha-BHC

R.T.: 3.902 min
Delta R.T.: 0.004 min
Response: 5250149
Conc: 0.35 ng/ml

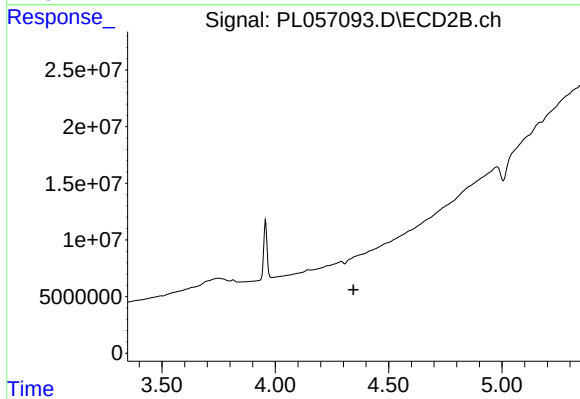

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.345 min
Response: 0
Conc: N.D.

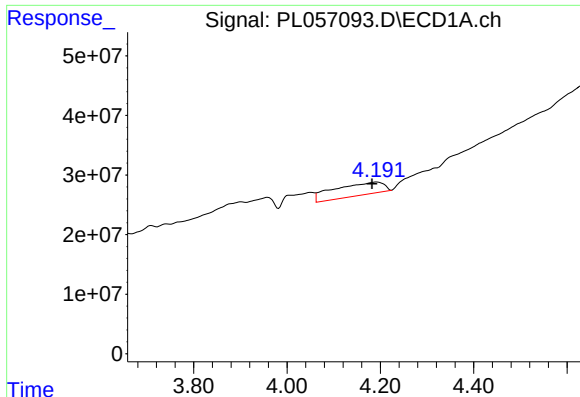

#3 gamma-BHC (Lindane)


R.T.: 4.192 min
Delta R.T.: 0.010 min
Response: 157796731
Conc: 11.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

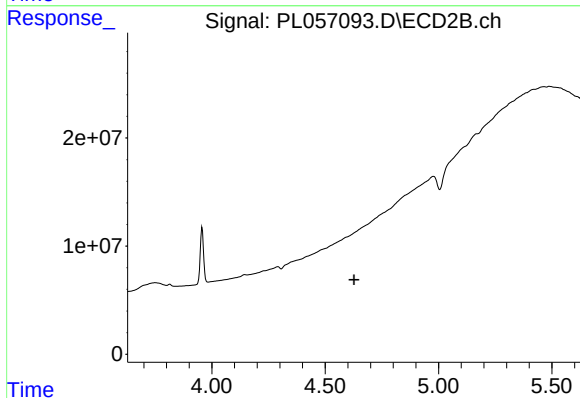


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.627 min
Response: 0
Conc: N.D.

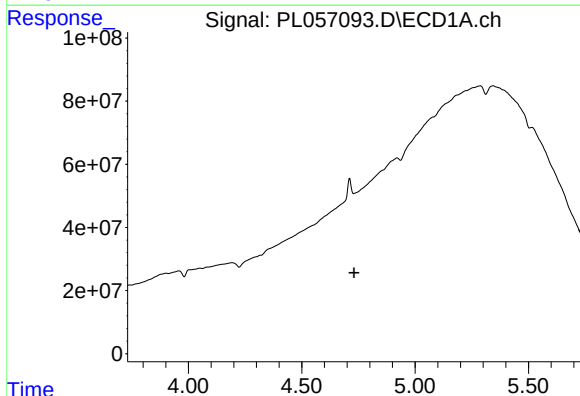


#5 Aldrin

R.T.: 4.711 min
Delta R.T.: -0.020 min
Response: -89505464
Conc: N.D.

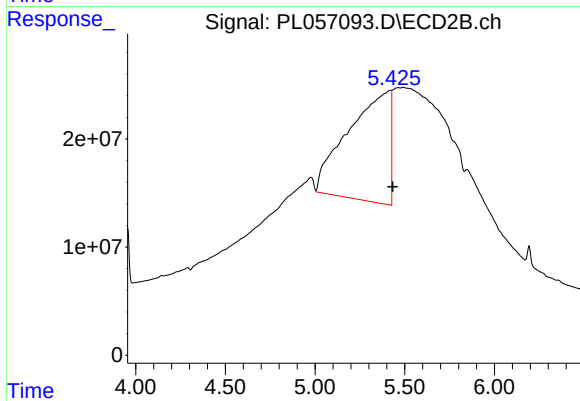

#5 Aldrin


R.T.: 5.421 min
Delta R.T.: -0.011 min
Response: 1667699668
Conc: 557.91 ng/ml

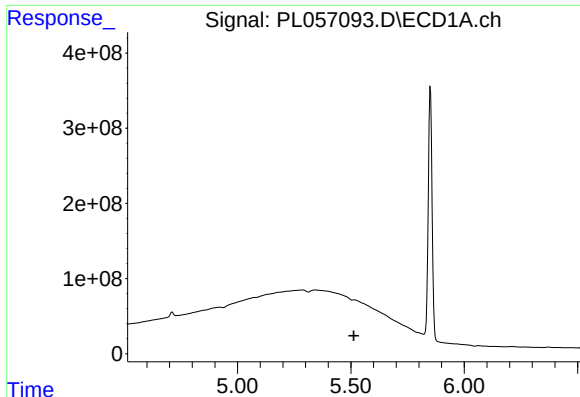

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.513 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

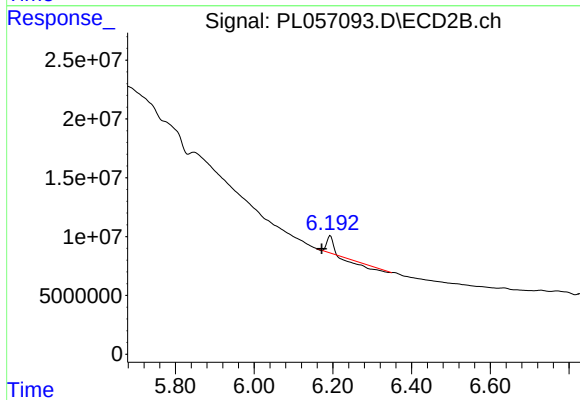


#9 Endosulfan I

R.T.: 6.194 min
Delta R.T.: 0.022 min
Response: 1668133
Conc: 0.60 ng/ml

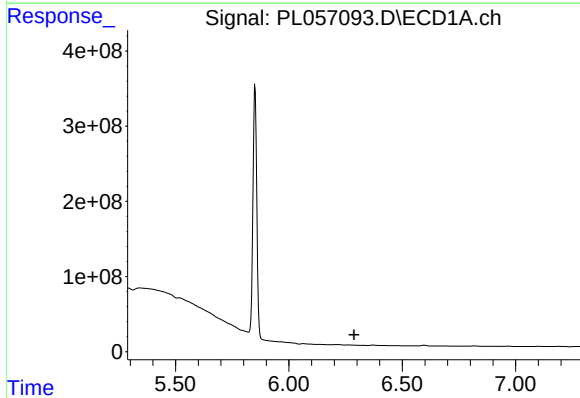


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.287 min
Response: 0
Conc: N.D.

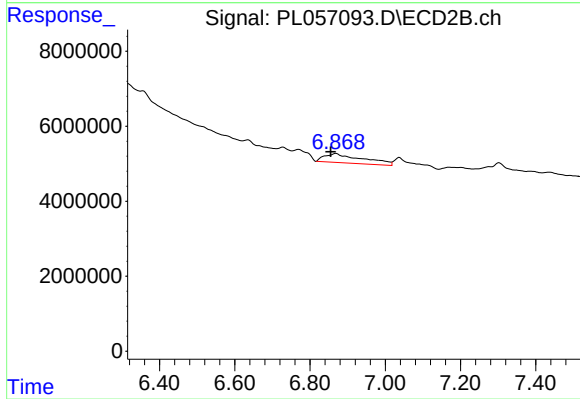

#15 Endosulfan II


R.T.: 6.869 min
Delta R.T.: 0.014 min
Response: 17339640
Conc: 6.18 ng/ml

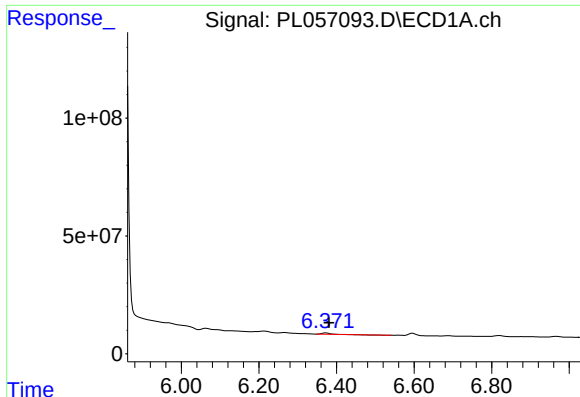

#17 4,4'-DDT


R.T.: 6.372 min
Delta R.T.: -0.009 min
Response: 9052561
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-3

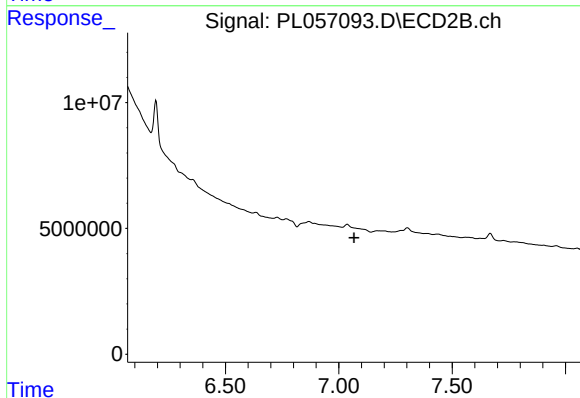


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.068 min
Response: 0
Conc: N.D.

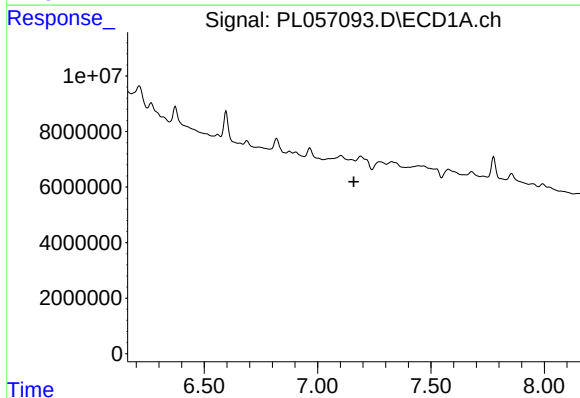


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.160 min
Response: 0
Conc: N.D.

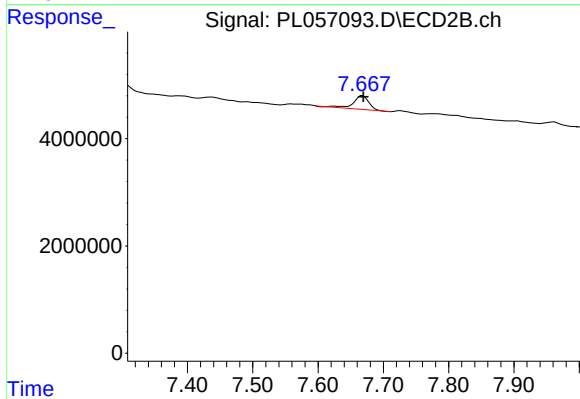

#21 Endrin ketone


R.T.: 7.668 min
Delta R.T.: -0.001 min
Response: 4303081
Conc: 1.57 ng/ml

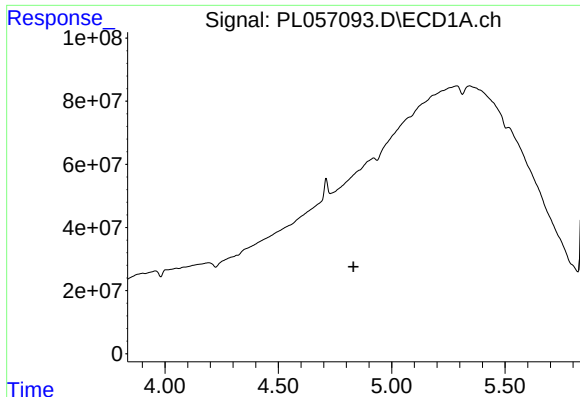

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.832 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TP-3

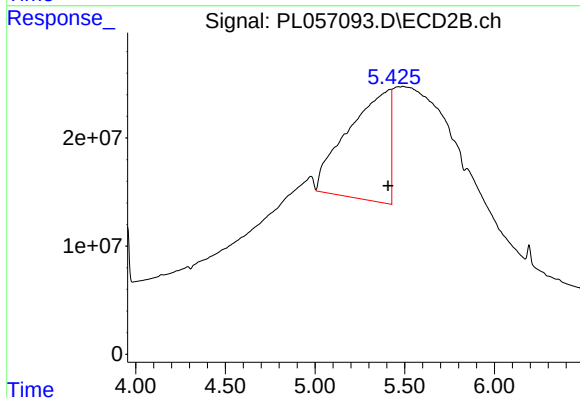


#24 Chlordane-2

R.T.: 5.421 min
Delta R.T.: 0.014 min
Response: 1667699668
Conc: 17471.20 ng/ml

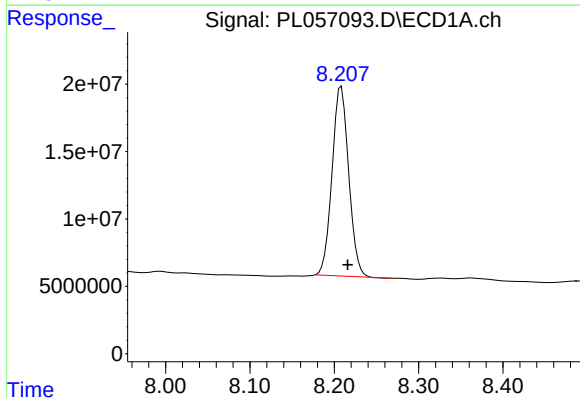

#28 Decachlorobiphenyl

R.T.: 8.208 min
Delta R.T.: -0.008 min
Response: 192600928
Conc: 19.93 ng/ml

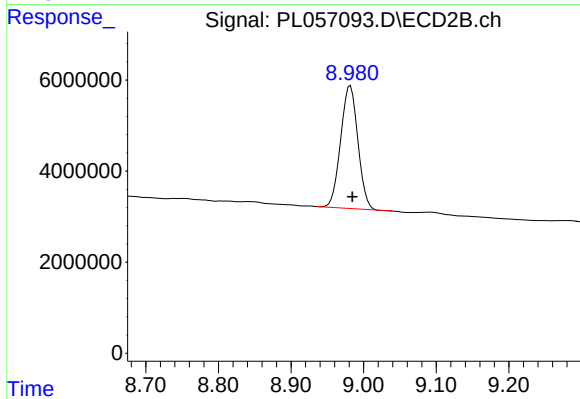

#28 Decachlorobiphenyl

R.T.: 8.982 min
Delta R.T.: -0.003 min
Response: 44367256
Conc: 20.88 ng/ml