

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
 Data File : PL065070.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 21:09
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:41:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 00:38:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.099	332.5E6	245.6E6	100.338	100.023
28)	SA Decachlor...	8.144	9.256	252.8E6	204.9E6	96.919	97.455
Target Compounds							
23)	Chlordane-1	4.281	5.112	118.1E6	101.5E6	957.534	973.784
24)	Chlordane-2	4.779	5.588	125.7E6	105.8E6	963.341	967.446
25)	Chlordane-3	5.342	6.244	394.6E6	407.0E6	997.117	1006.978
26)	Chlordane-4	5.400	6.317	327.6E6	487.1E6	996.805	999.154
27)	Chlordane-5	6.229	7.137	131.1E6	79398091	999.381	1030.594



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
Data File : PL065070.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 21:09
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:41:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 00:38:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

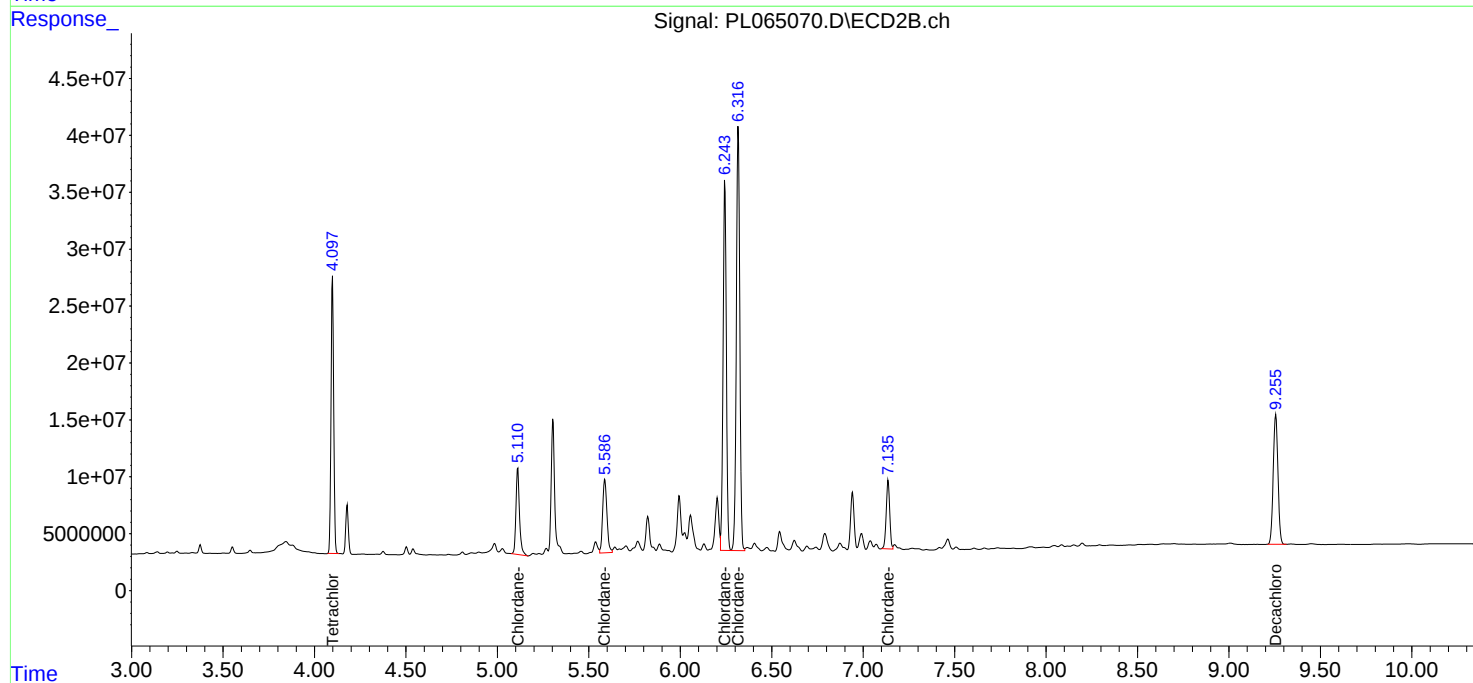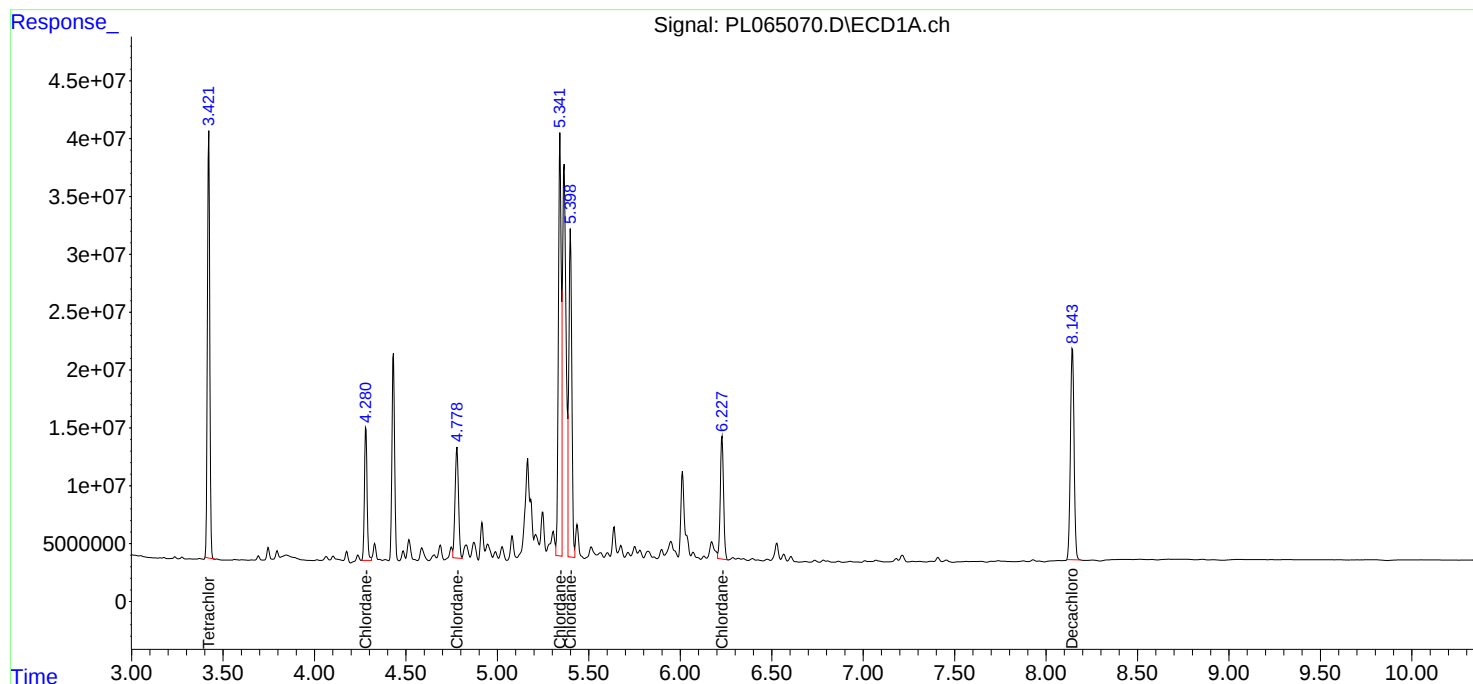


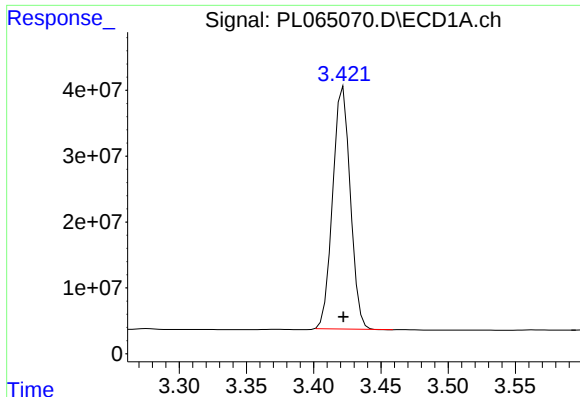

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 332493492
Conc: 100.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

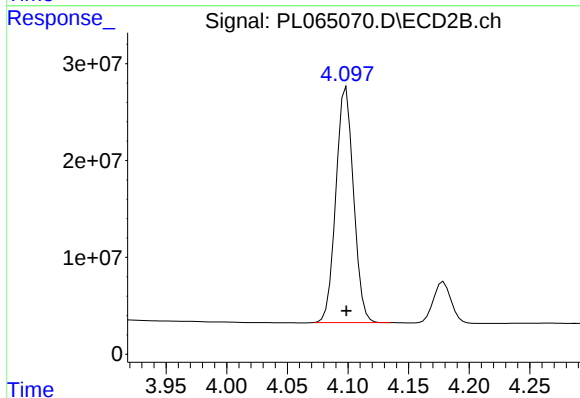


#1 Tetrachloro-m-xylene

R.T.: 4.099 min
Delta R.T.: 0.000 min
Response: 245608438
Conc: 100.02 ng/ml

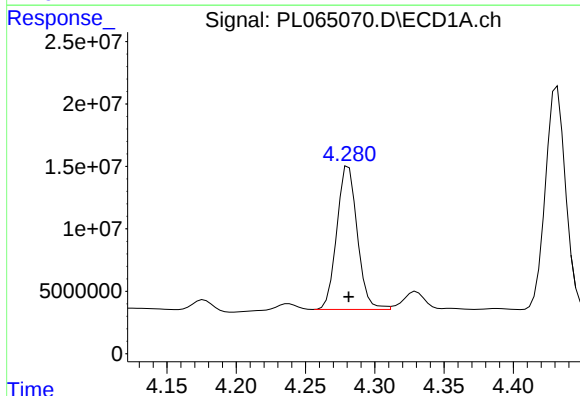


#23 Chlordane-1

R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 118128119
Conc: 957.53 ng/ml

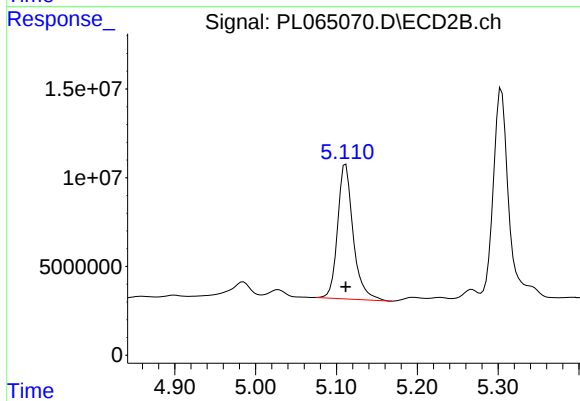

#23 Chlordane-1


R.T.: 5.112 min
Delta R.T.: 0.000 min
Response: 101539899
Conc: 973.78 ng/ml

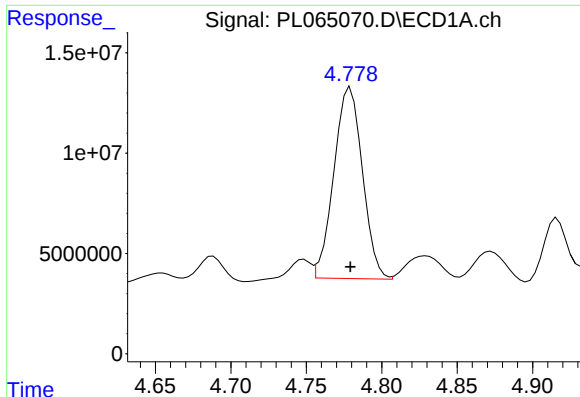

#24 Chlordane-2


R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 125734932
Conc: 963.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

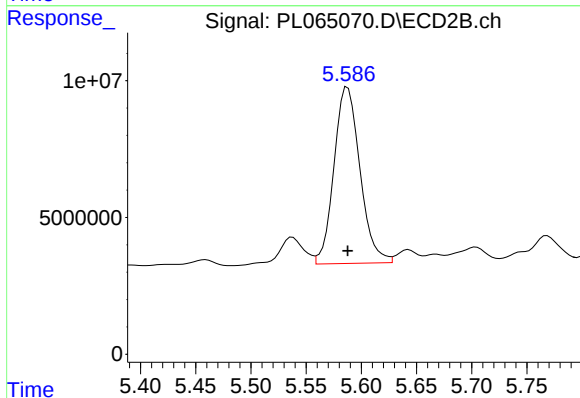


#24 Chlordane-2

R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 105802608
Conc: 967.45 ng/ml

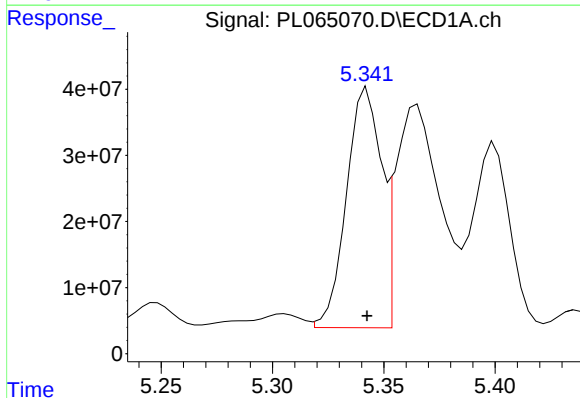


#25 Chlordane-3

R.T.: 5.342 min
Delta R.T.: 0.000 min
Response: 394576841
Conc: 997.12 ng/ml

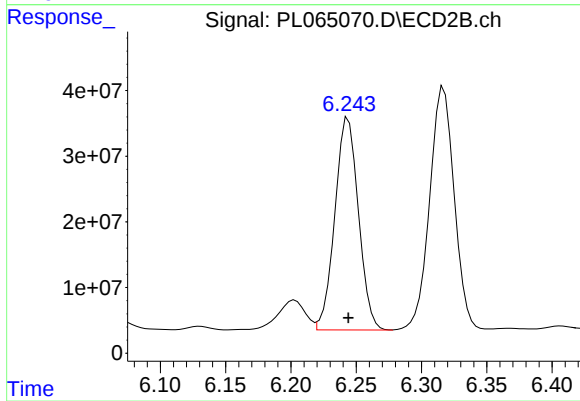

#25 Chlordane-3


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 406953702
Conc: 1006.98 ng/ml

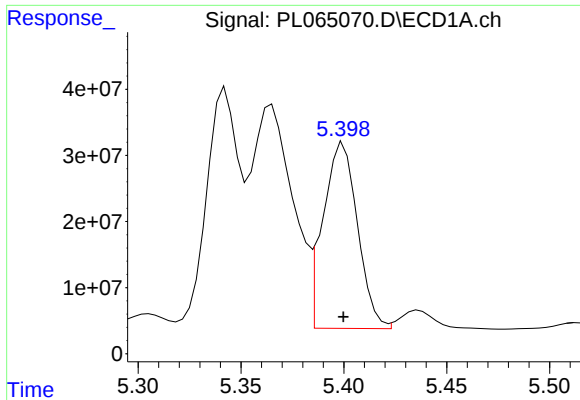

#26 Chlordane-4


R.T.: 5.400 min
Delta R.T.: 0.000 min
Response: 327626783
Conc: 996.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

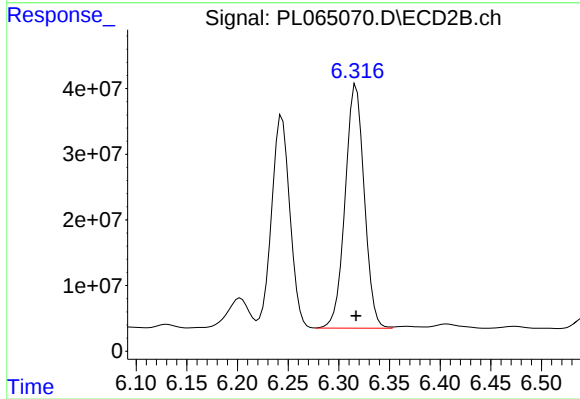


#26 Chlordane-4

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 487121448
Conc: 999.15 ng/ml

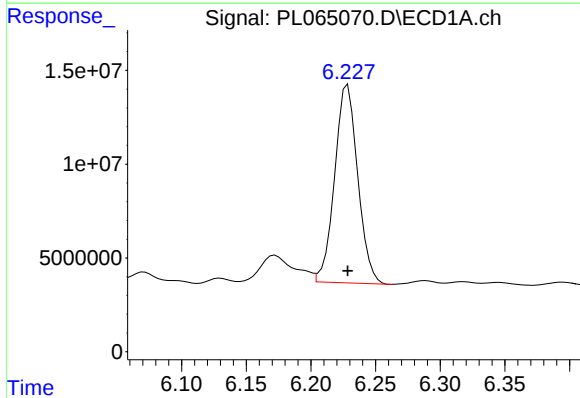


#27 Chlordane-5

R.T.: 6.229 min
Delta R.T.: 0.000 min
Response: 131060027
Conc: 999.38 ng/ml

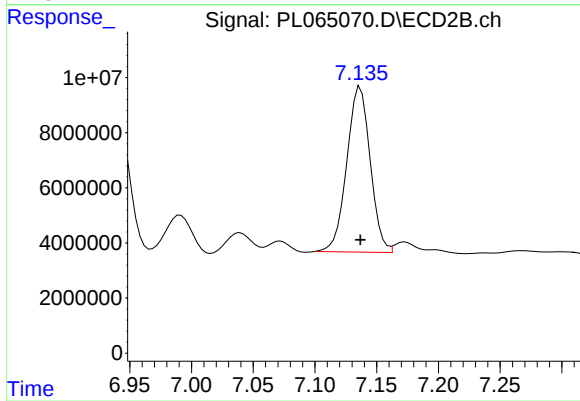

#27 Chlordane-5


R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 79398091
Conc: 1030.59 ng/ml

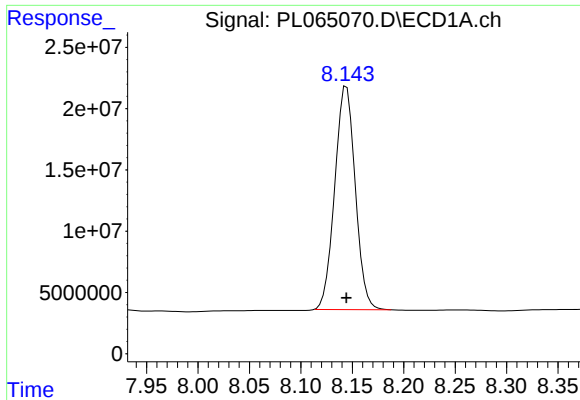

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: 0.000 min
Response: 252781587
Conc: 96.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

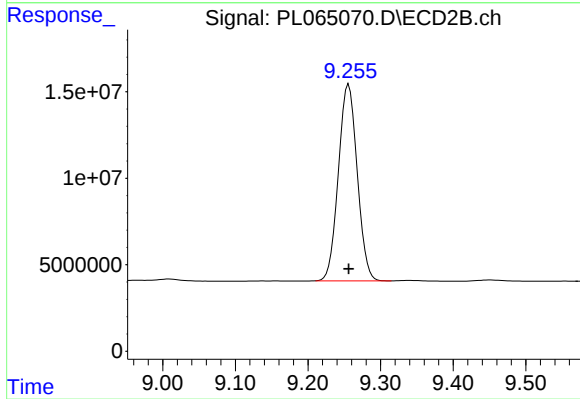

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: 0.000 min
Response: 204857585
Conc: 97.45 ng/ml