

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
 Data File : PL065071.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 21:23
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:42:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 00:38:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.098	252.0E6	185.6E6	75.695	75.382
28)	SA Decachlor...	8.142	9.257	196.9E6	158.9E6	75.325	75.393
Target Compounds							
23)	Chlordane-1	4.281	5.111	89945092	77751790	735.926	747.096
24)	Chlordane-2	4.779	5.587	98174543	82053843	751.453	750.193
25)	Chlordane-3	5.343	6.244	302.4E6	306.6E6	759.315	755.699
26)	Chlordane-4	5.400	6.316	250.6E6	369.2E6	758.285	754.810
27)	Chlordane-5	6.228	7.137	99975866	59726236	758.190	766.647



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
Data File : PL065071.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 21:23
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleID :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:42:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 00:38:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

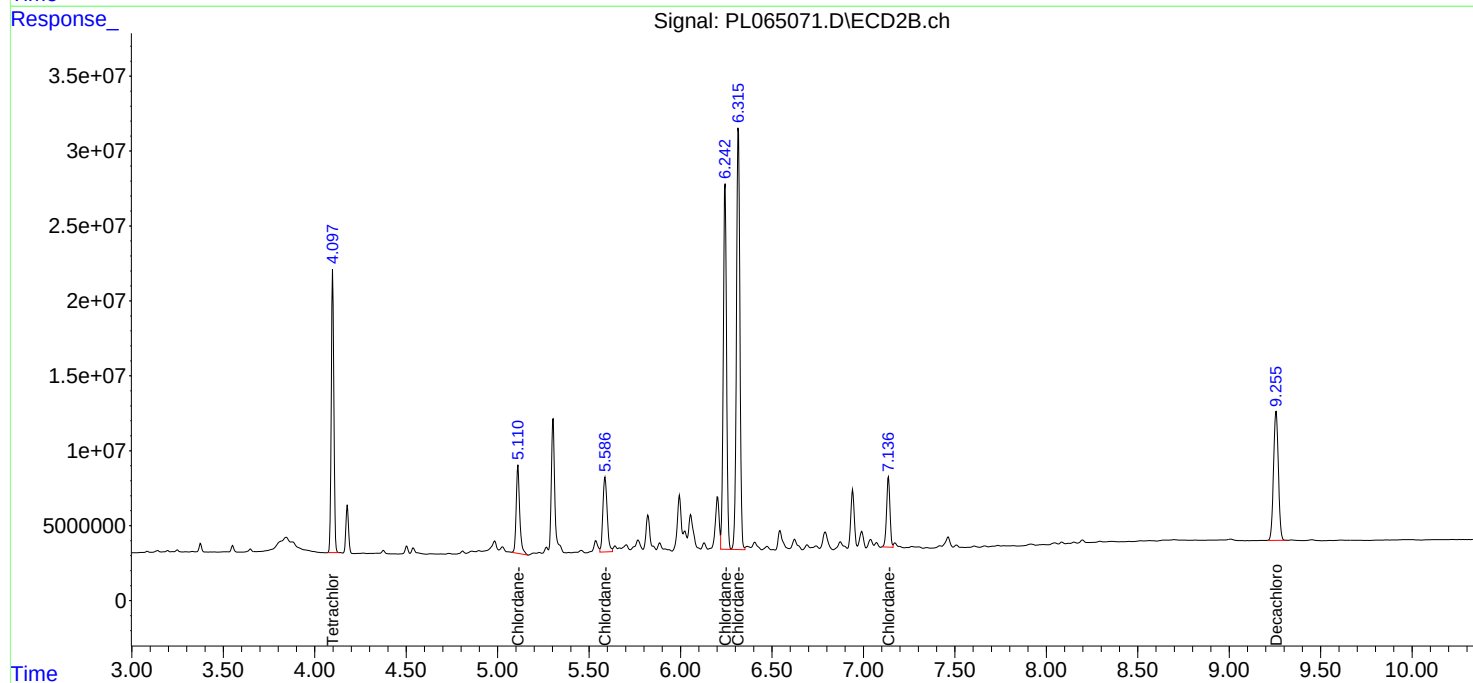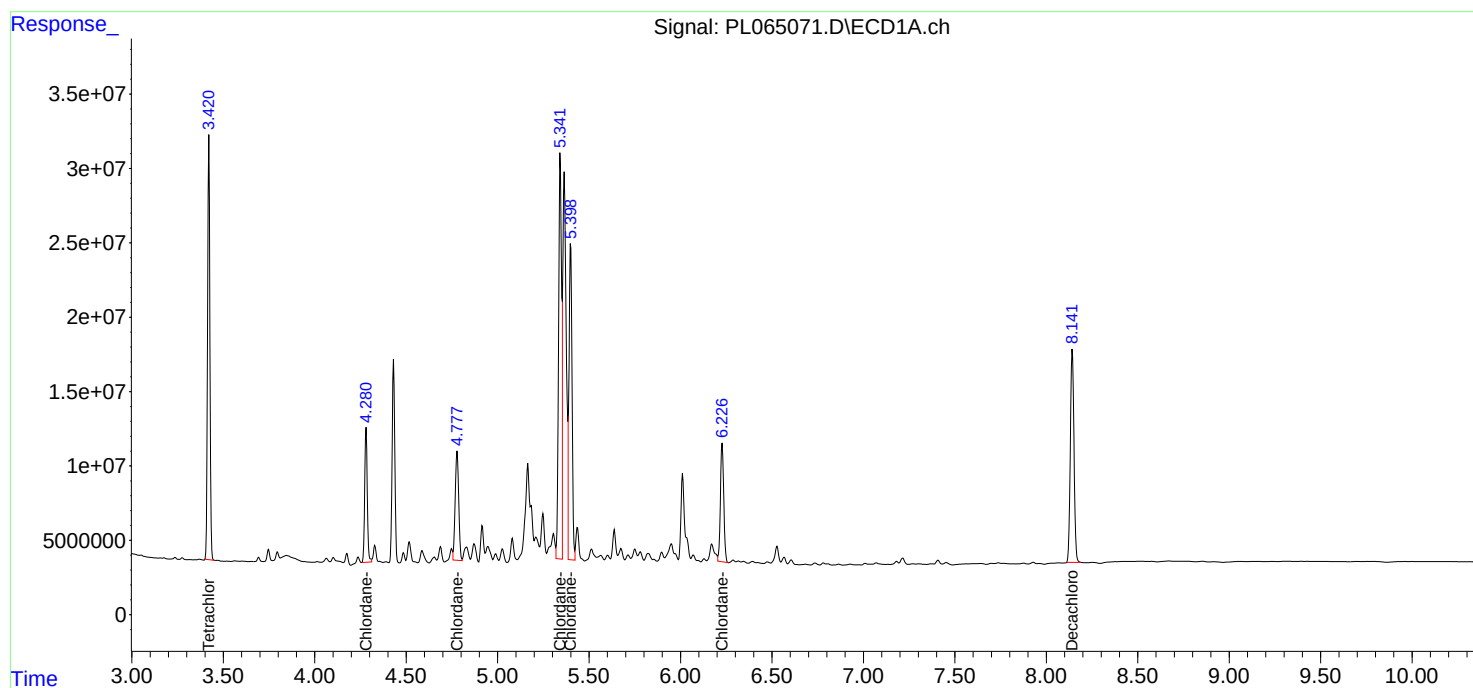


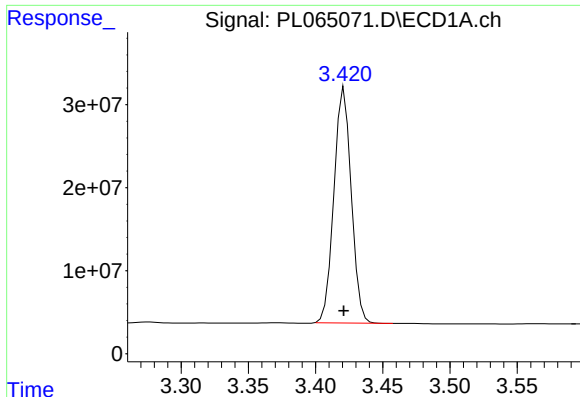

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 251999386
Conc: 75.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

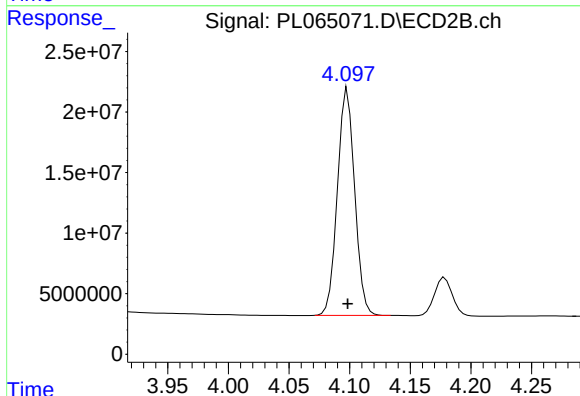


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 185576046
Conc: 75.38 ng/ml

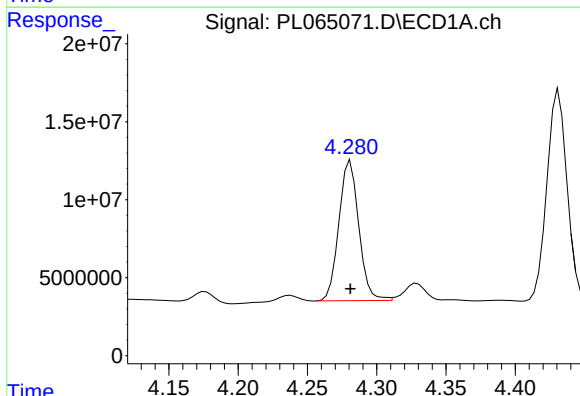


#23 Chlordane-1

R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 89945092
Conc: 735.93 ng/ml

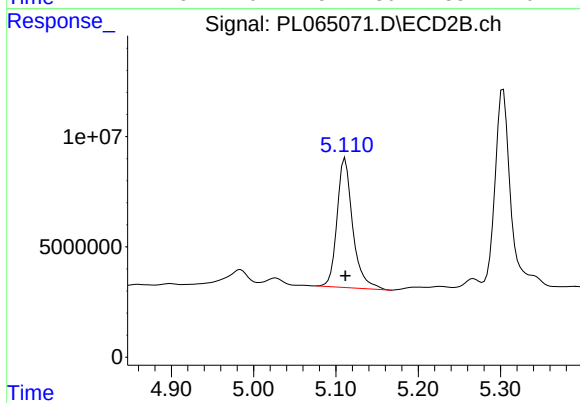

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 77751790
Conc: 747.10 ng/ml

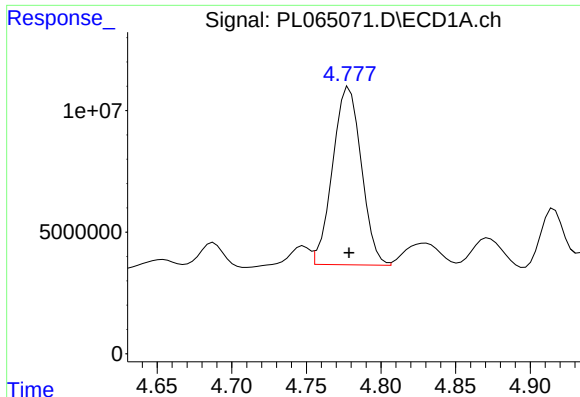

#24 Chlordane-2


R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 98174543
Conc: 751.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

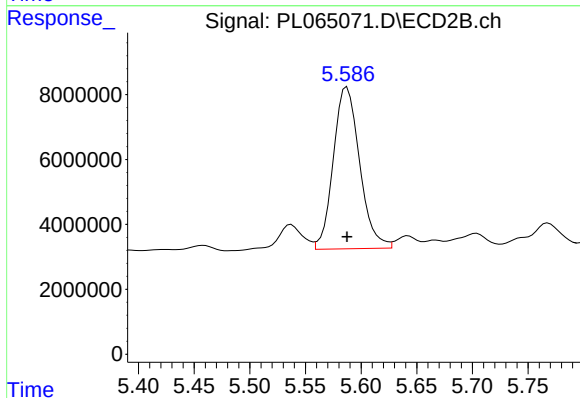


#24 Chlordane-2

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 82053843
Conc: 750.19 ng/ml

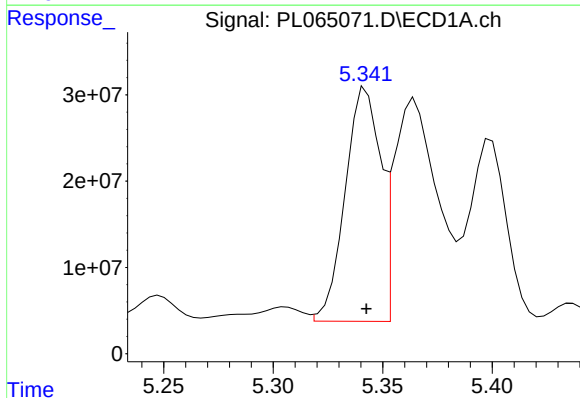


#25 Chlordane-3

R.T.: 5.343 min
Delta R.T.: 0.000 min
Response: 302351912
Conc: 759.31 ng/ml

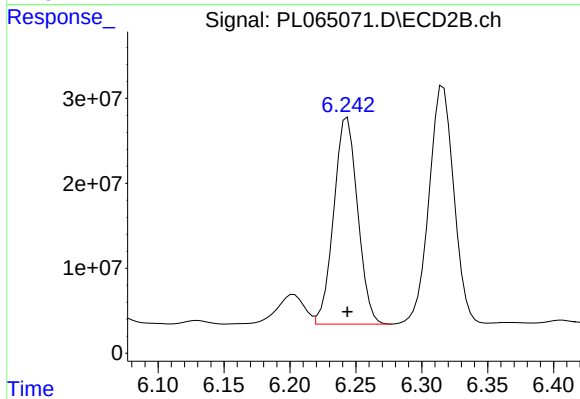

#25 Chlordane-3


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 306567981
Conc: 755.70 ng/ml

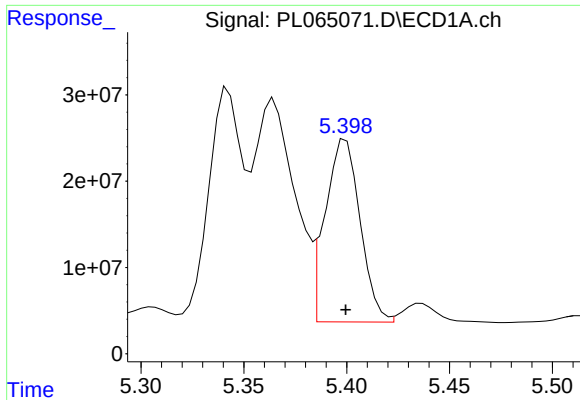

#26 Chlordane-4


R.T.: 5.400 min
Delta R.T.: 0.000 min
Response: 250614710
Conc: 758.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

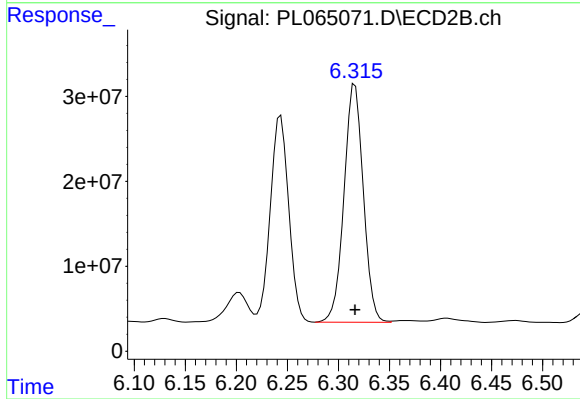


#26 Chlordane-4

R.T.: 6.316 min
Delta R.T.: 0.000 min
Response: 369179358
Conc: 754.81 ng/ml

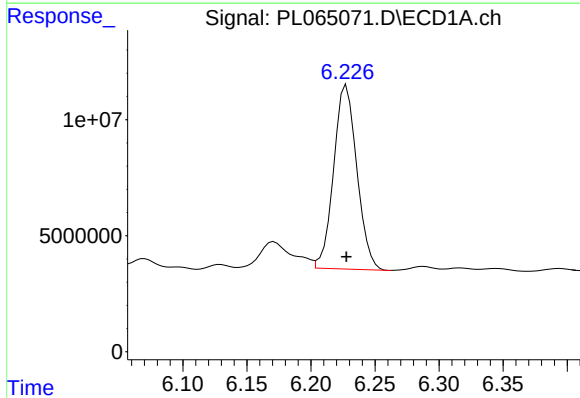


#27 Chlordane-5

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 99975866
Conc: 758.19 ng/ml

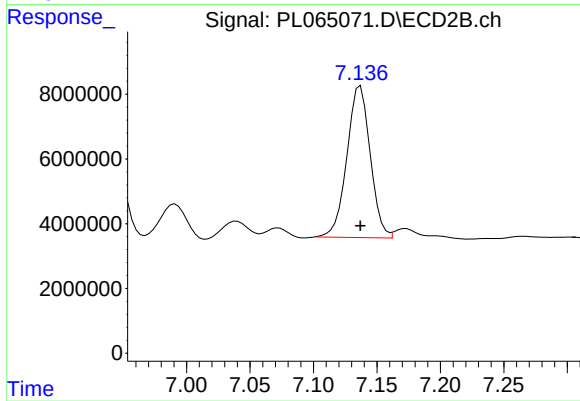

#27 Chlordane-5


R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 59726236
Conc: 766.65 ng/ml

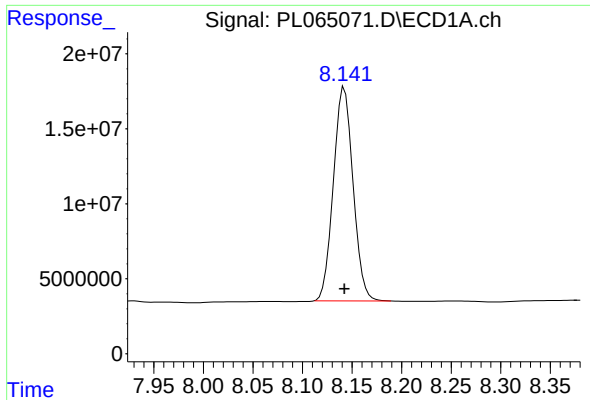

#28 Decachlorobiphenyl

R.T.: 8.142 min
Delta R.T.: 0.000 min
Response: 196888918
Conc: 75.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

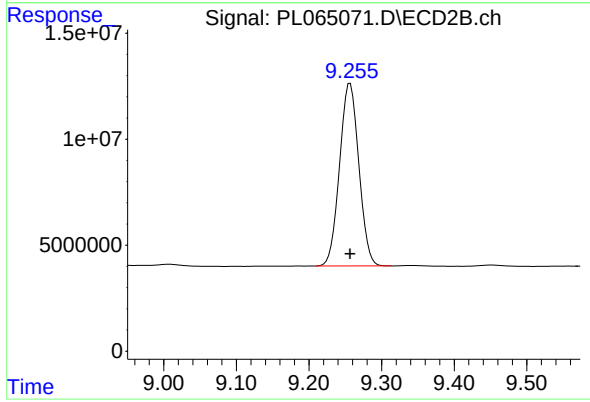

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 158899422
Conc: 75.39 ng/ml