

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
 Data File : PL065072.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 21:37
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:39:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 00:38:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	165.1E6	122.7E6	50.000	50.000
28)	SA Decachlor...	8.143	9.257	134.4E6	107.8E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.281	5.111	64302976	53503627	500.000	500.000
24)	Chlordane-2	4.779	5.587	67652219	56461528	500.000	500.000
25)	Chlordane-3	5.343	6.244	198.4E6	200.7E6	500.000	500.000
26)	Chlordane-4	5.400	6.317	164.9E6	244.0E6	500.000	500.000
27)	Chlordane-5	6.228	7.137	65611165	37342064	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
Data File : PL065072.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 21:37
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:39:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 00:38:45 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

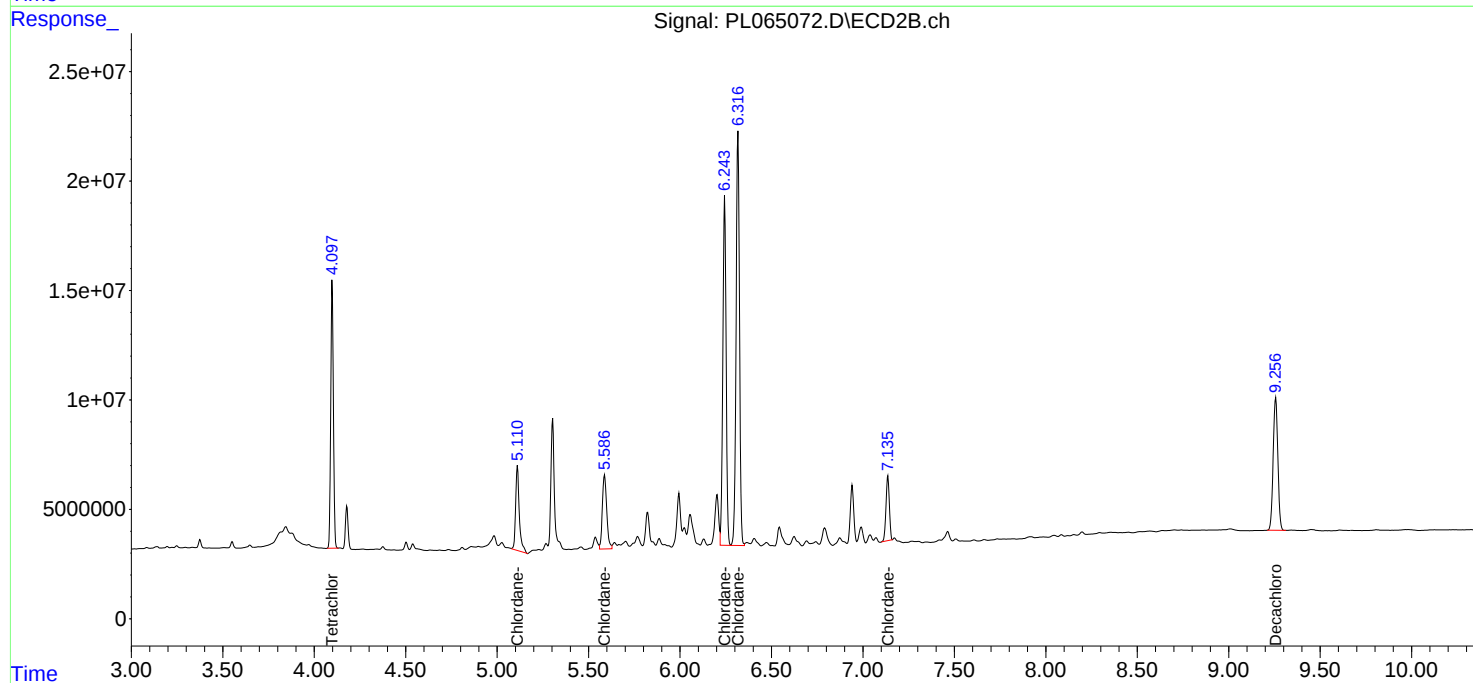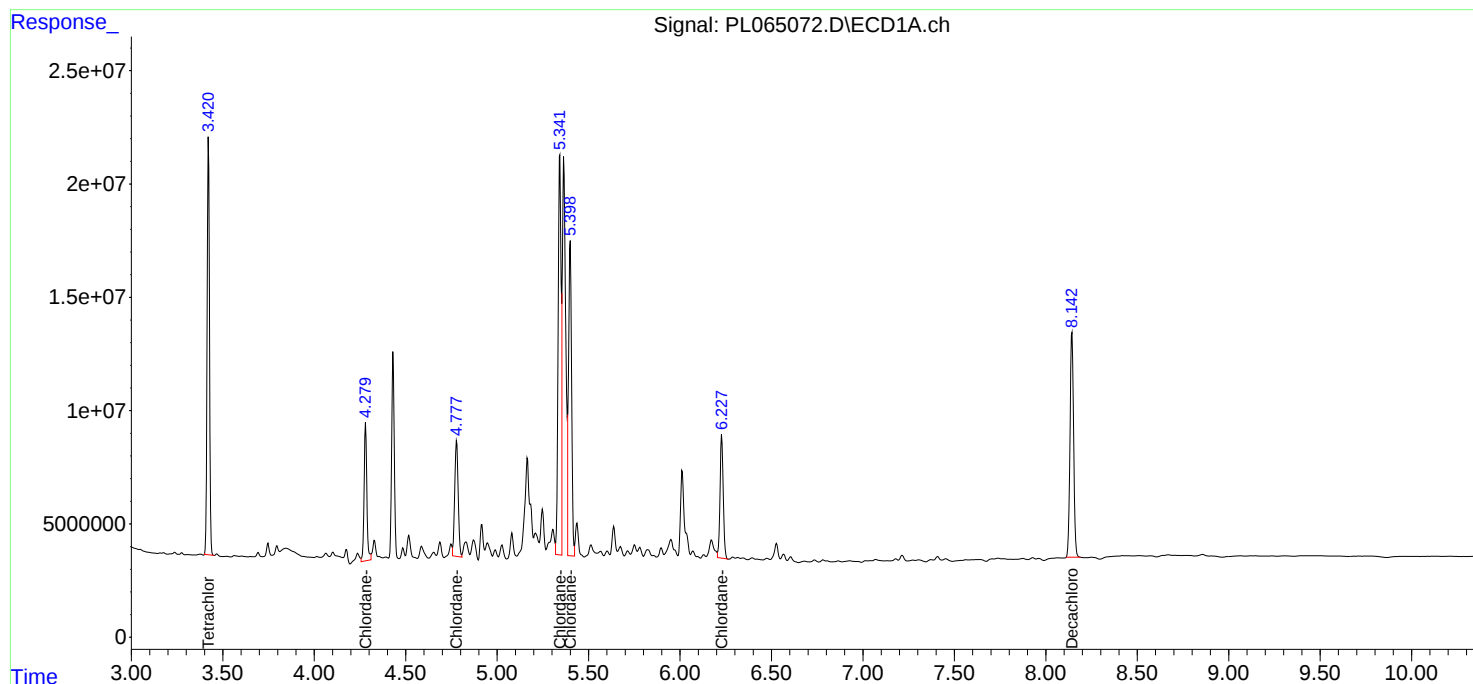


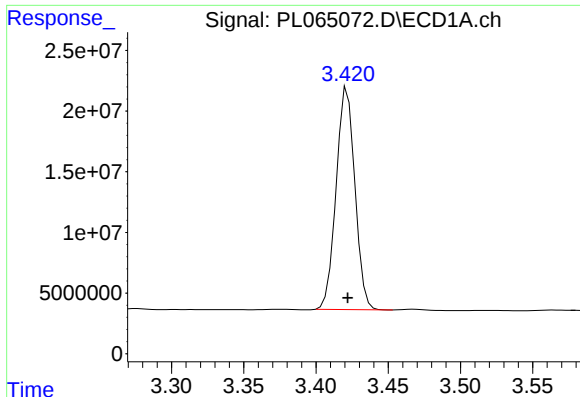

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 165126939
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

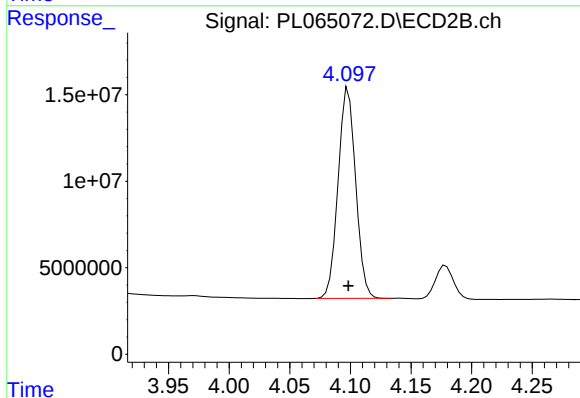


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 122748008
Conc: 50.00 ng/ml

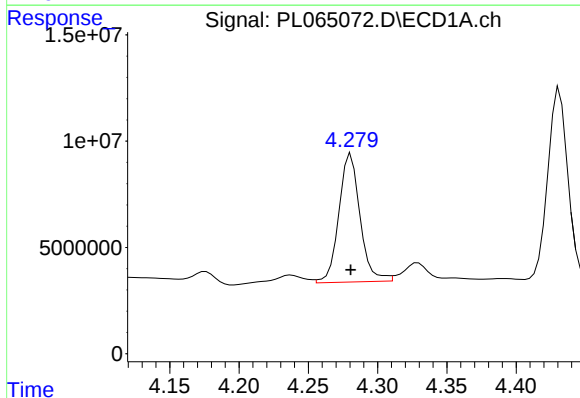


#23 Chlordane-1

R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 64302976
Conc: 500.00 ng/ml

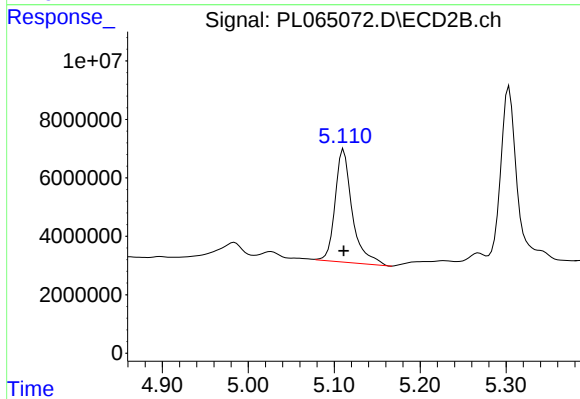

#23 Chlordane-1


R.T.: 5.111 min
Delta R.T.: 0.000 min
Response: 53503627
Conc: 500.00 ng/ml

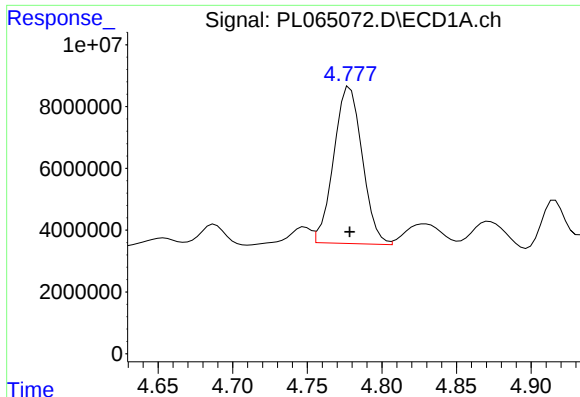

#24 Chlordane-2


R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 67652219
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

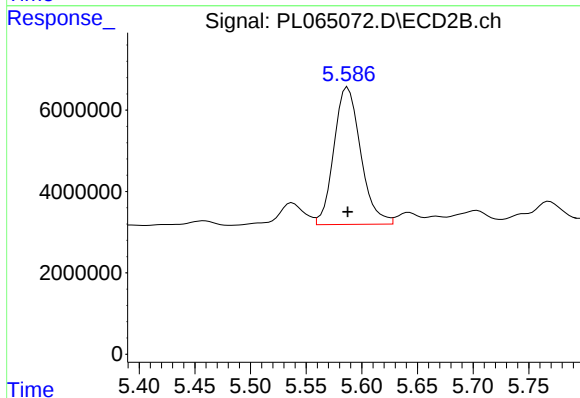


#24 Chlordane-2

R.T.: 5.587 min
Delta R.T.: 0.000 min
Response: 56461528
Conc: 500.00 ng/ml

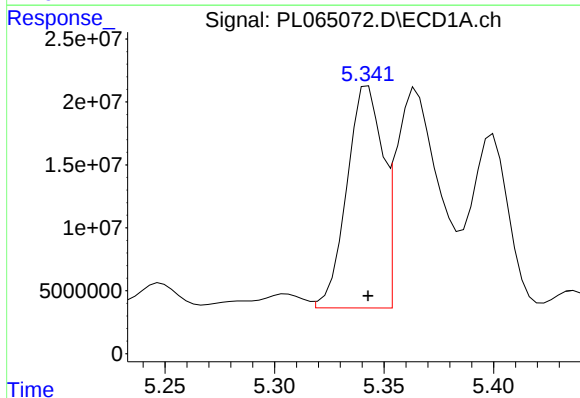


#25 Chlordane-3

R.T.: 5.343 min
Delta R.T.: 0.000 min
Response: 198429333
Conc: 500.00 ng/ml

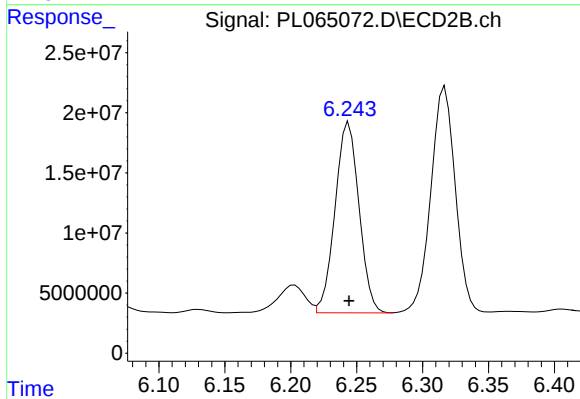

#25 Chlordane-3


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 200656893
Conc: 500.00 ng/ml

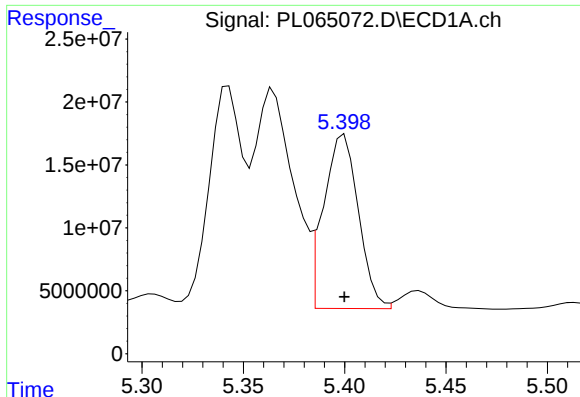

#26 Chlordane-4


R.T.: 5.400 min
Delta R.T.: 0.000 min
Response: 164863384
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

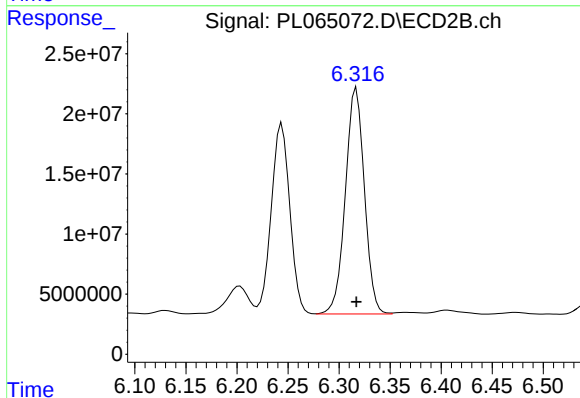


#26 Chlordane-4

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 243972972
Conc: 500.00 ng/ml

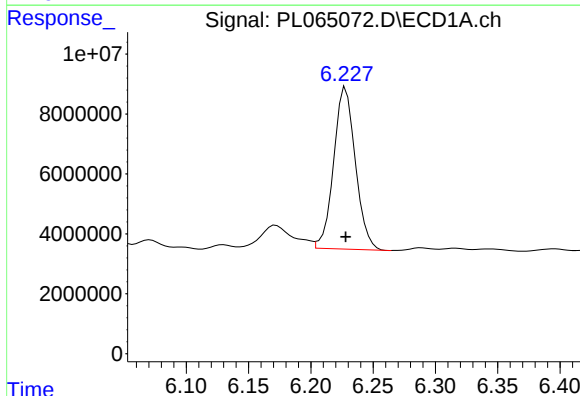


#27 Chlordane-5

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 65611165
Conc: 500.00 ng/ml

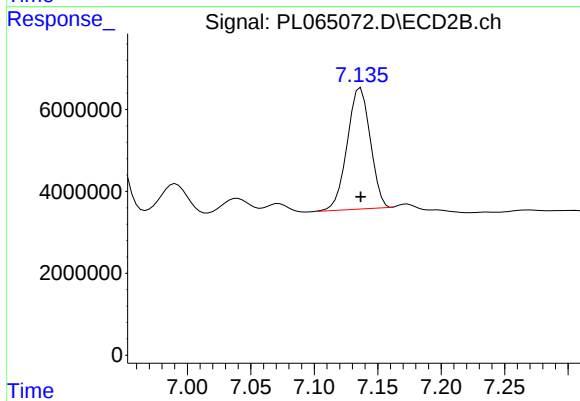

#27 Chlordane-5


R.T.: 7.137 min
Delta R.T.: 0.000 min
Response: 37342064
Conc: 500.00 ng/ml

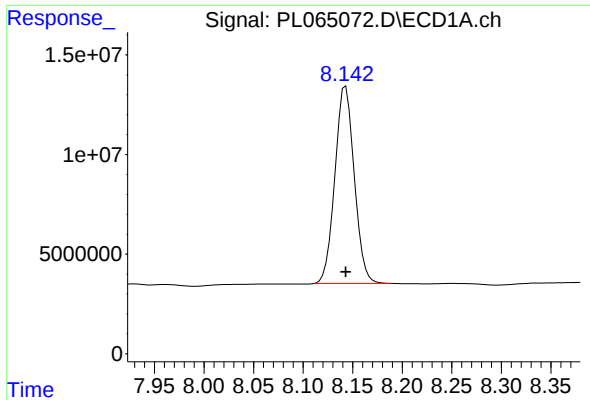

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: 0.000 min
Response: 134427405
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

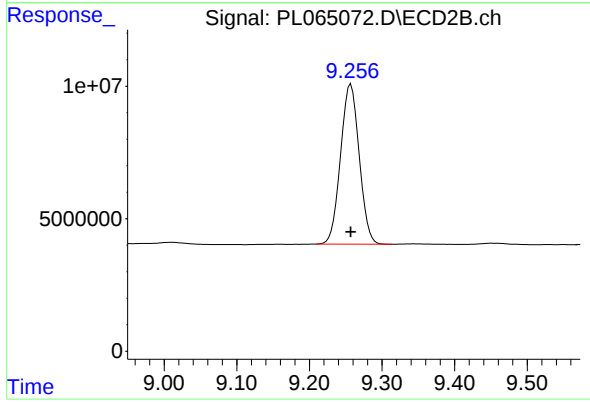

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: 0.000 min
Response: 107778698
Conc: 50.00 ng/ml