

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
 Data File : PL065081.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2021 23:46
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL030521CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:47:58 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 00:47:20 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	162.9E6	123.0E6	49.671	49.741
28)	SA Decachlor...	8.143	9.256	135.0E6	107.9E6	48.613	49.600
Target Compounds							
23)	Chlordane-1	4.281	5.112	58803636	49795080	461.351	477.123
24)	Chlordane-2	4.779	5.588	63338423	52683933	459.342	474.419
25)	Chlordane-3	5.343	6.244	187.0E6	187.2E6	468.727	466.106
26)	Chlordane-4	5.400	6.317	157.2E6	227.8E6	468.550	466.502
27)	Chlordane-5	6.228	7.137	60770601	35264644	468.002	463.571



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030521\
Data File : PL065081.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2021 23:46
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL030521CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:47:58 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 00:47:20 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

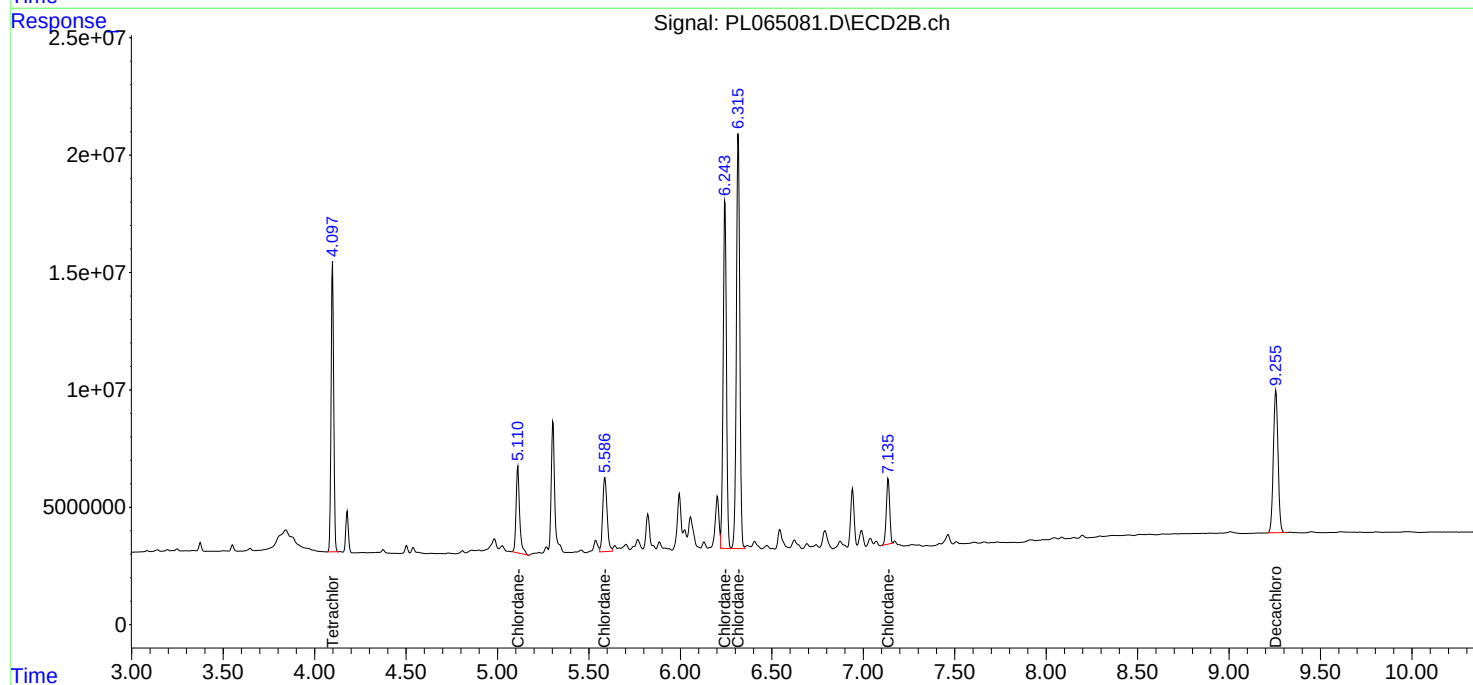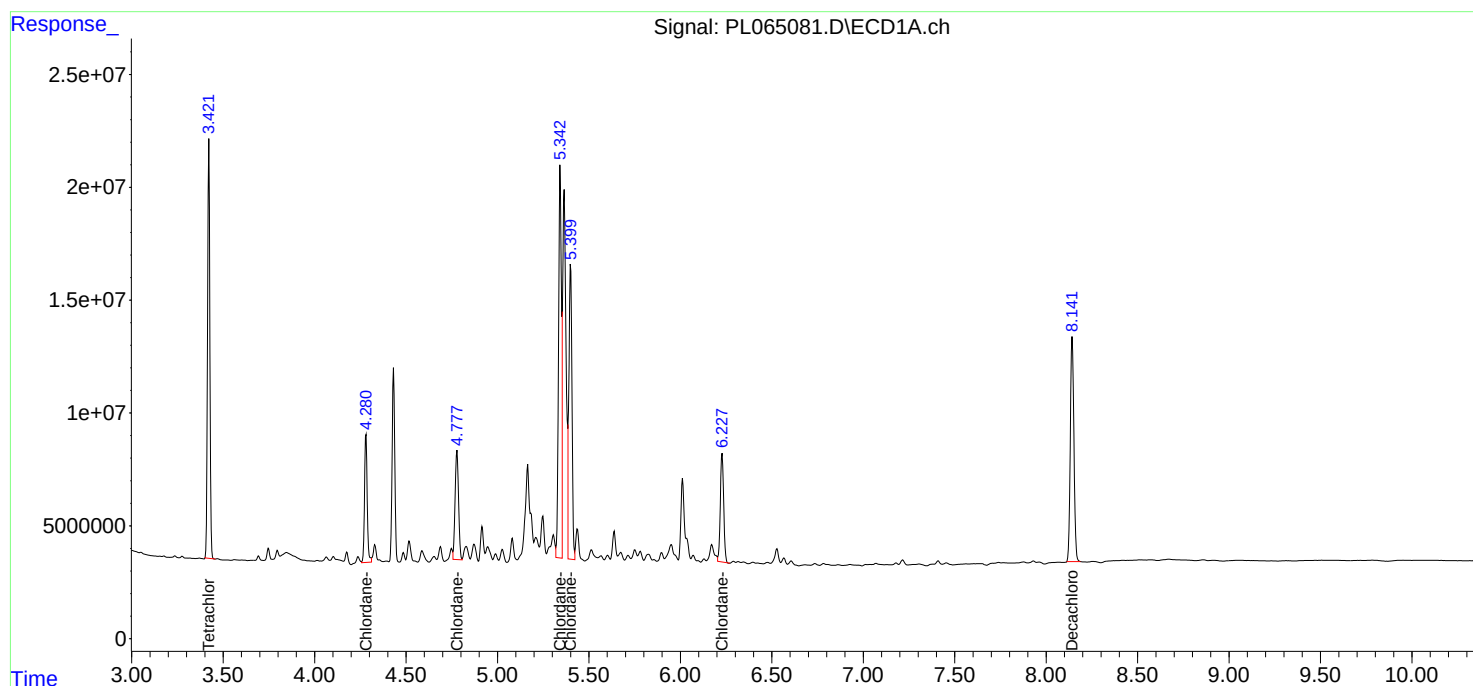


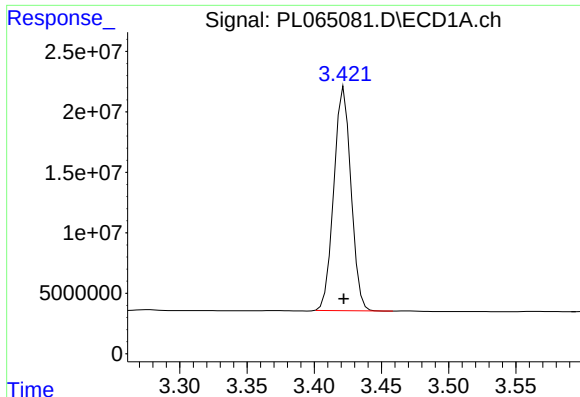

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: 0.000 min
Response: 162886106
Conc: 49.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030521CHLOR

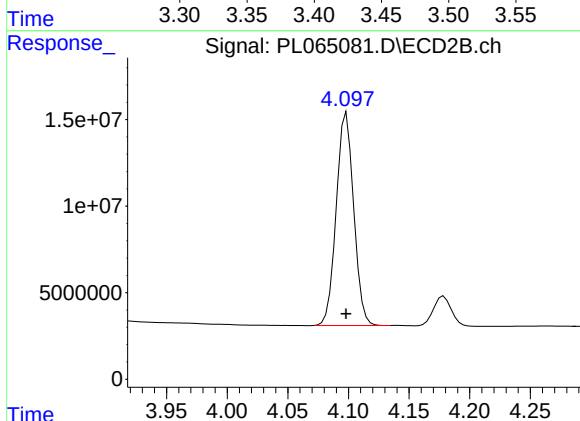


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 122963662
Conc: 49.74 ng/ml

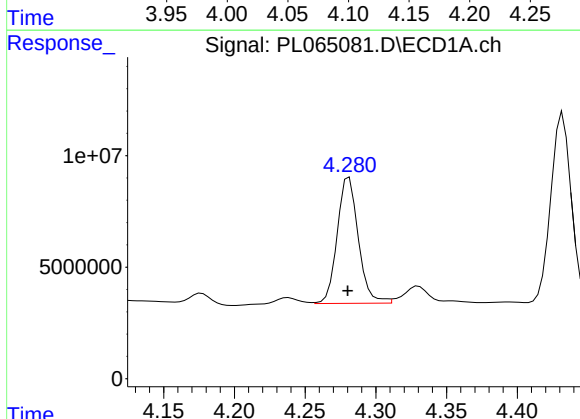


#23 Chlordane-1

R.T.: 4.281 min
Delta R.T.: 0.000 min
Response: 58803636
Conc: 461.35 ng/ml

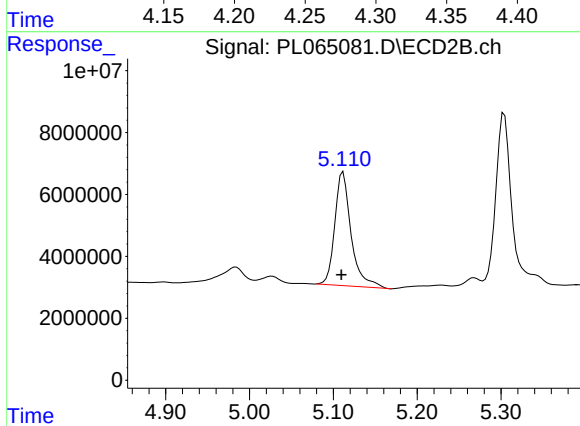

#23 Chlordane-1


R.T.: 5.112 min
Delta R.T.: 0.002 min
Response: 49795080
Conc: 477.12 ng/ml

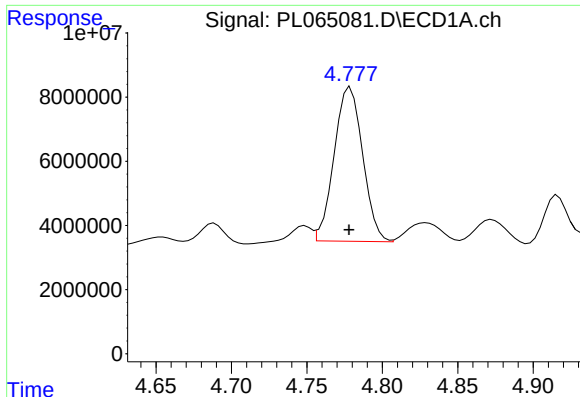

#24 Chlordane-2


R.T.: 4.779 min
Delta R.T.: 0.000 min
Response: 63338423
Conc: 459.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030521CHLOR

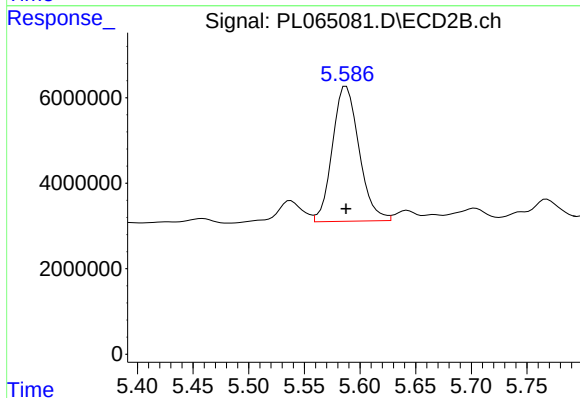


#24 Chlordane-2

R.T.: 5.588 min
Delta R.T.: 0.000 min
Response: 52683933
Conc: 474.42 ng/ml

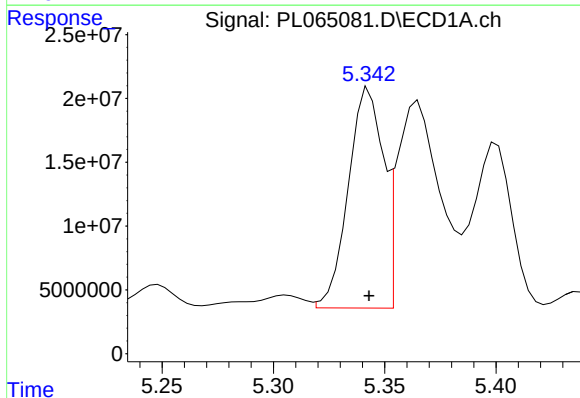


#25 Chlordane-3

R.T.: 5.343 min
Delta R.T.: 0.000 min
Response: 186989382
Conc: 468.73 ng/ml

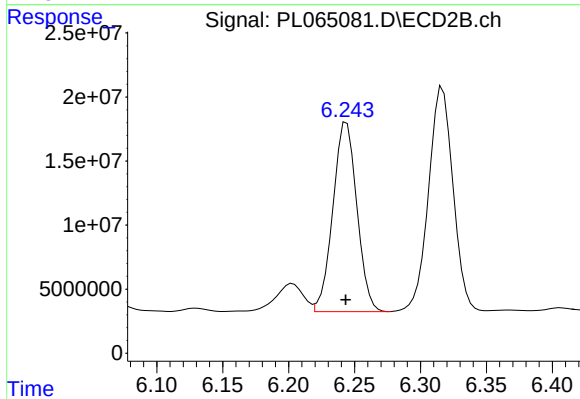

#25 Chlordane-3


R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 187219883
Conc: 466.11 ng/ml

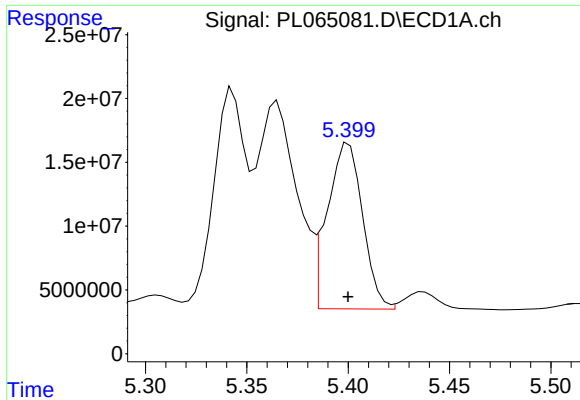

#26 Chlordane-4


R.T.: 5.400 min
Delta R.T.: 0.000 min
Response: 157181528
Conc: 468.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030521CHLOR

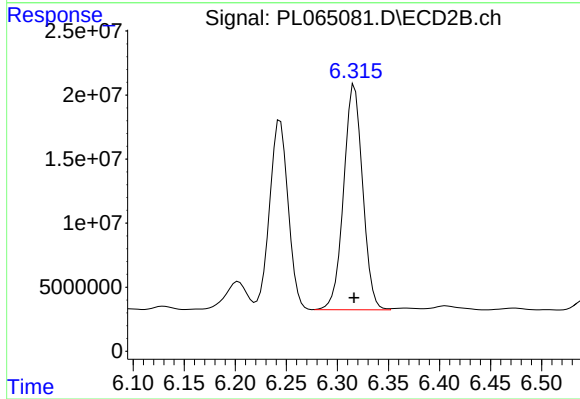


#26 Chlordane-4

R.T.: 6.317 min
Delta R.T.: 0.000 min
Response: 227759192
Conc: 466.50 ng/ml

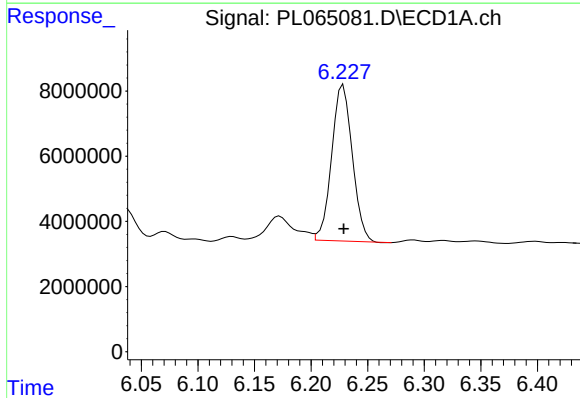


#27 Chlordane-5

R.T.: 6.228 min
Delta R.T.: 0.000 min
Response: 60770601
Conc: 468.00 ng/ml

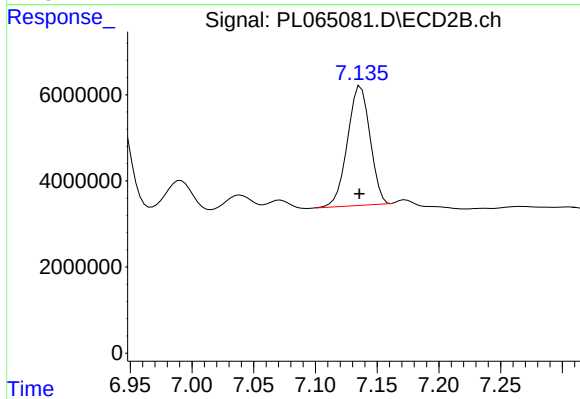

#27 Chlordane-5


R.T.: 7.137 min
Delta R.T.: 0.001 min
Response: 35264644
Conc: 463.57 ng/ml

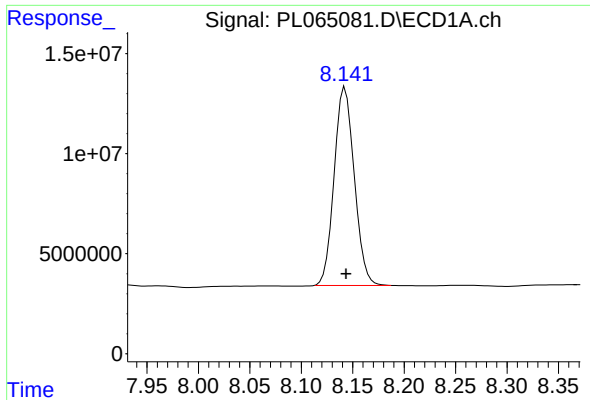

#28 Decachlorobiphenyl

R.T.: 8.143 min
Delta R.T.: -0.001 min
Response: 134999238
Conc: 48.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL030521CHLOR

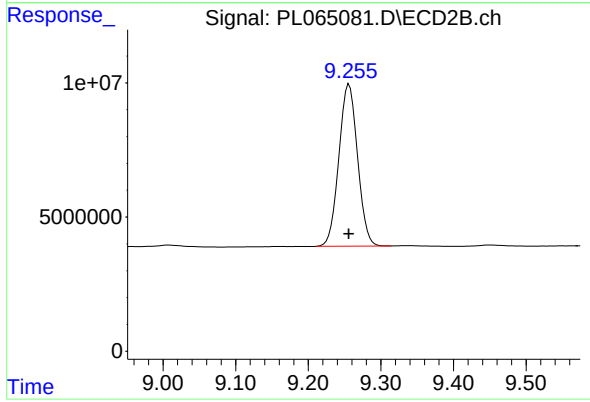

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: 0.000 min
Response: 107943384
Conc: 49.60 ng/ml