

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030524\
 Data File : PL088407.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2024 12:40
 Operator : AR\AJ
 Sample : PB159436BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB159436BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 03/06/2024
 Supervised By : Ankita Jodhani 03/06/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 00:20:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 16 21:46:54 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.645	2.854	54619519	27385548	19.885	19.526m
2)	SA Decachlor...	9.316	8.088	48711759	29501248	25.293m	23.169

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030524\
Data File : PL088407.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2024 12:40
Operator : AR\AJ
Sample : PB159436BL
Misc :
ALS Vial : 5 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB159436BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 03/06/2024
Supervised By : Ankita Jodhani 03/06/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 00:20:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL021524.M
Quant Title : GC Extractables
QLast Update : Fri Feb 16 21:46:54 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

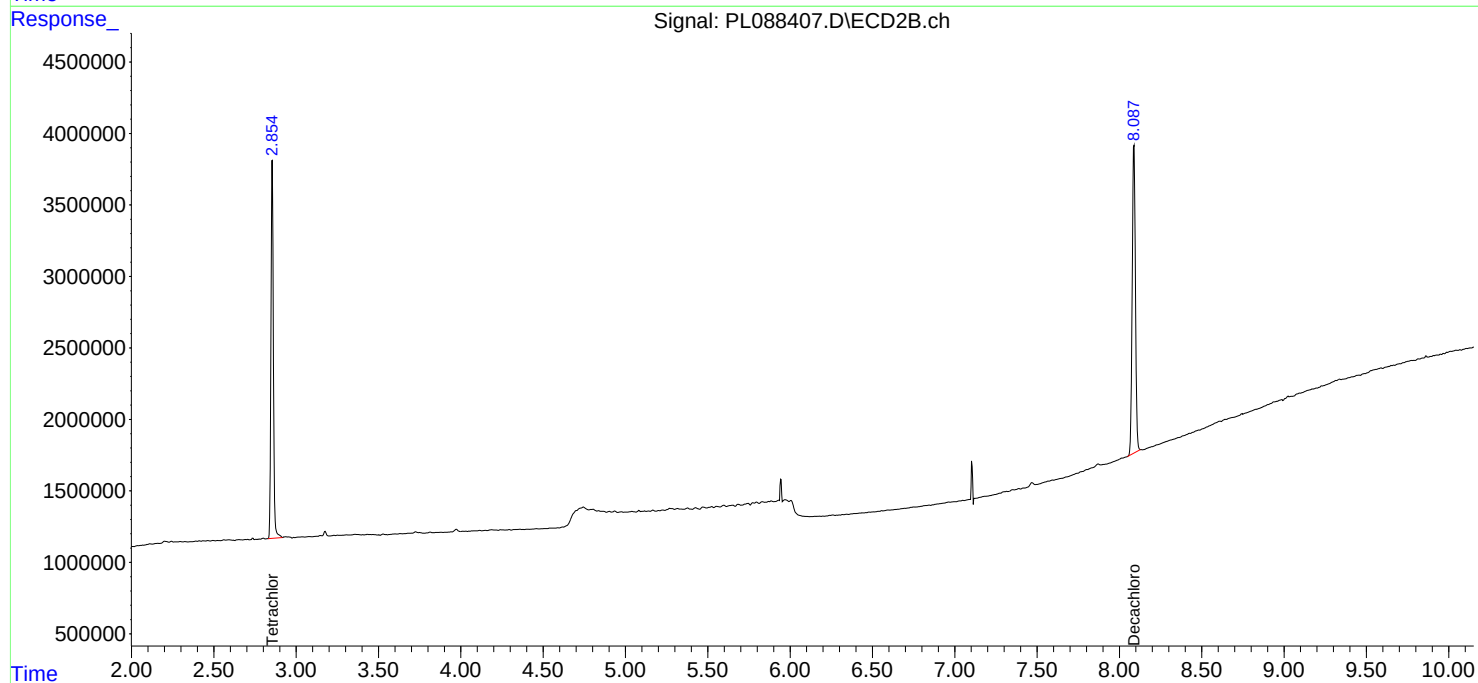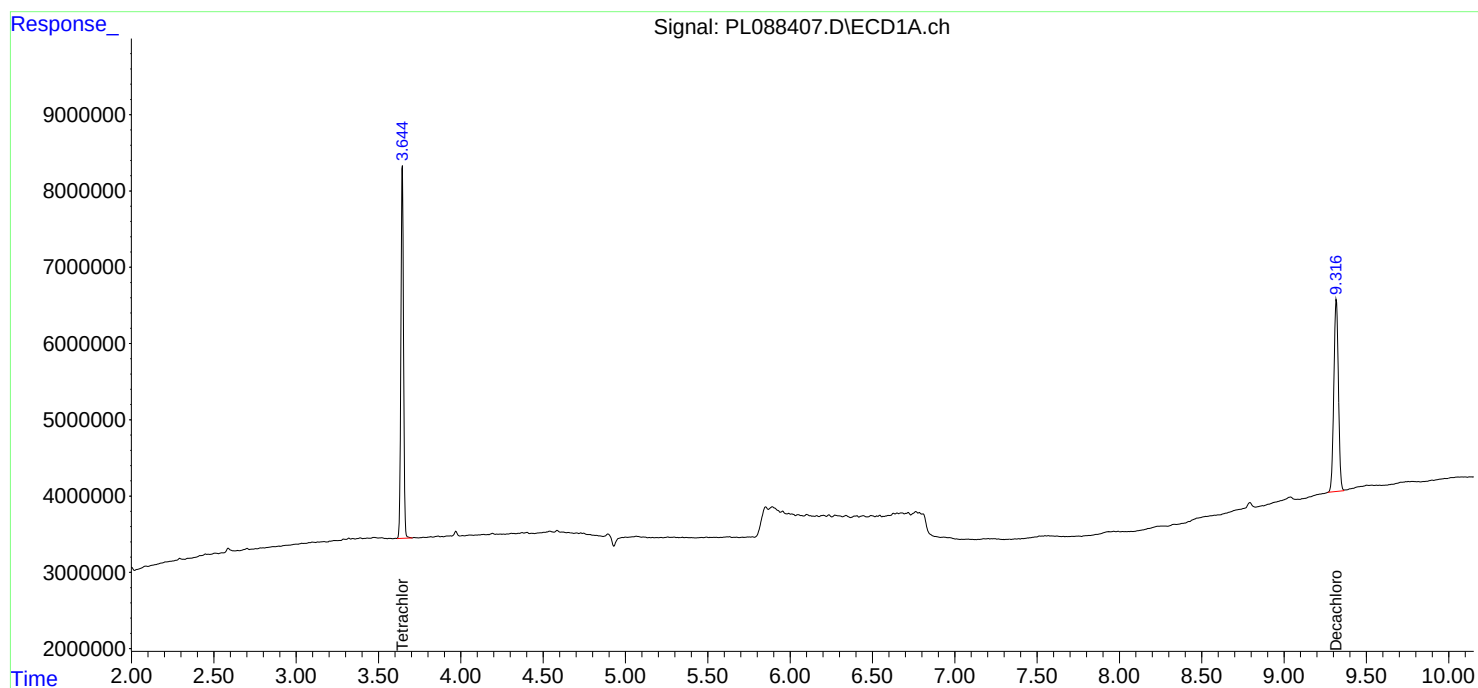

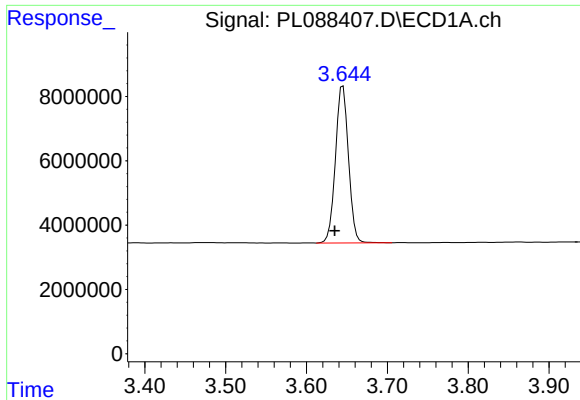


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: 0.010 min
Response: 54619519
Conc: 19.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB159436BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 03/06/2024
Supervised By :Ankita Jodhani 03/06/2024

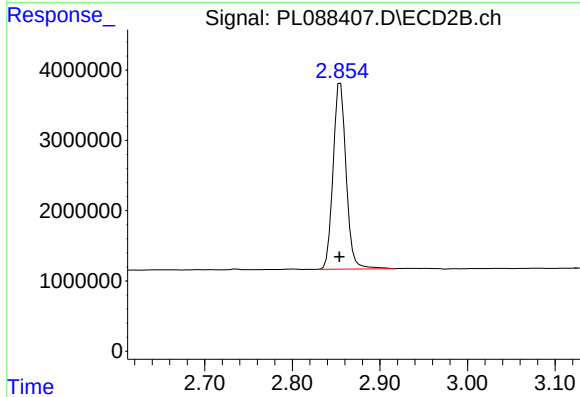


#1 Tetrachloro-m-xylene

R.T.: 2.854 min
Delta R.T.: 0.000 min
Response: 27385548
Conc: 19.53 ng/ml m

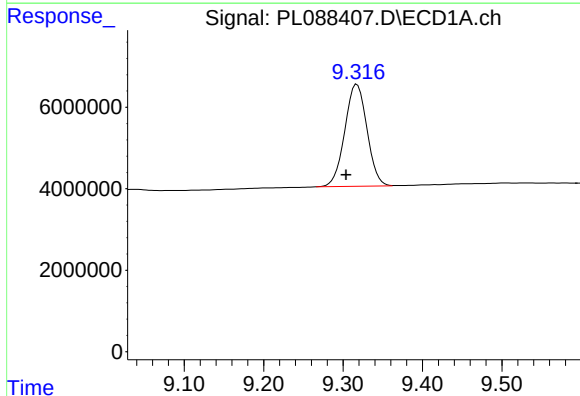

#28 Decachlorobiphenyl

R.T.: 9.316 min
Delta R.T.: 0.012 min
Response: 48711759
Conc: 25.29 ng/ml m

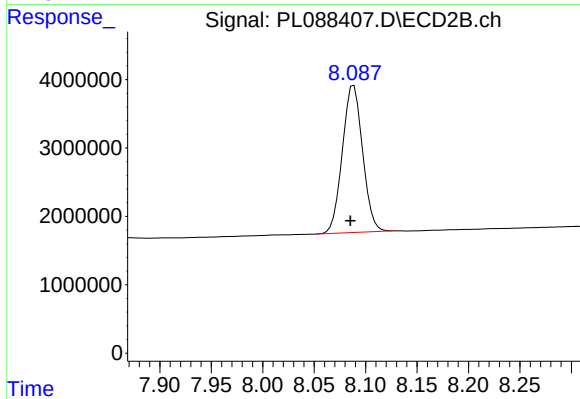

#28 Decachlorobiphenyl

R.T.: 8.088 min
Delta R.T.: 0.003 min
Response: 29501248
Conc: 23.17 ng/ml