

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030525\
 Data File : PL094519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Mar 2025 19:35
 Operator : AR\AJ
 Sample : Q1487-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DN-B-42

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 01:01:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
 Quant Title : GC Extractables
 QLast Update : Fri Feb 21 14:52:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.771	59129872	76545512	23.288m	23.987
28) SA Decachlor...	9.054	7.905	41915445	69528929	19.704	18.080m
Target Compounds						
6) B beta-BHC	4.531	3.907	2191243	2084874	1.372m	1.048



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030525\
Data File : PL094519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Mar 2025 19:35
Operator : AR\AJ
Sample : Q1487-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DN-B-42

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 01:01:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022125.M
Quant Title : GC Extractables
QLast Update : Fri Feb 21 14:52:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

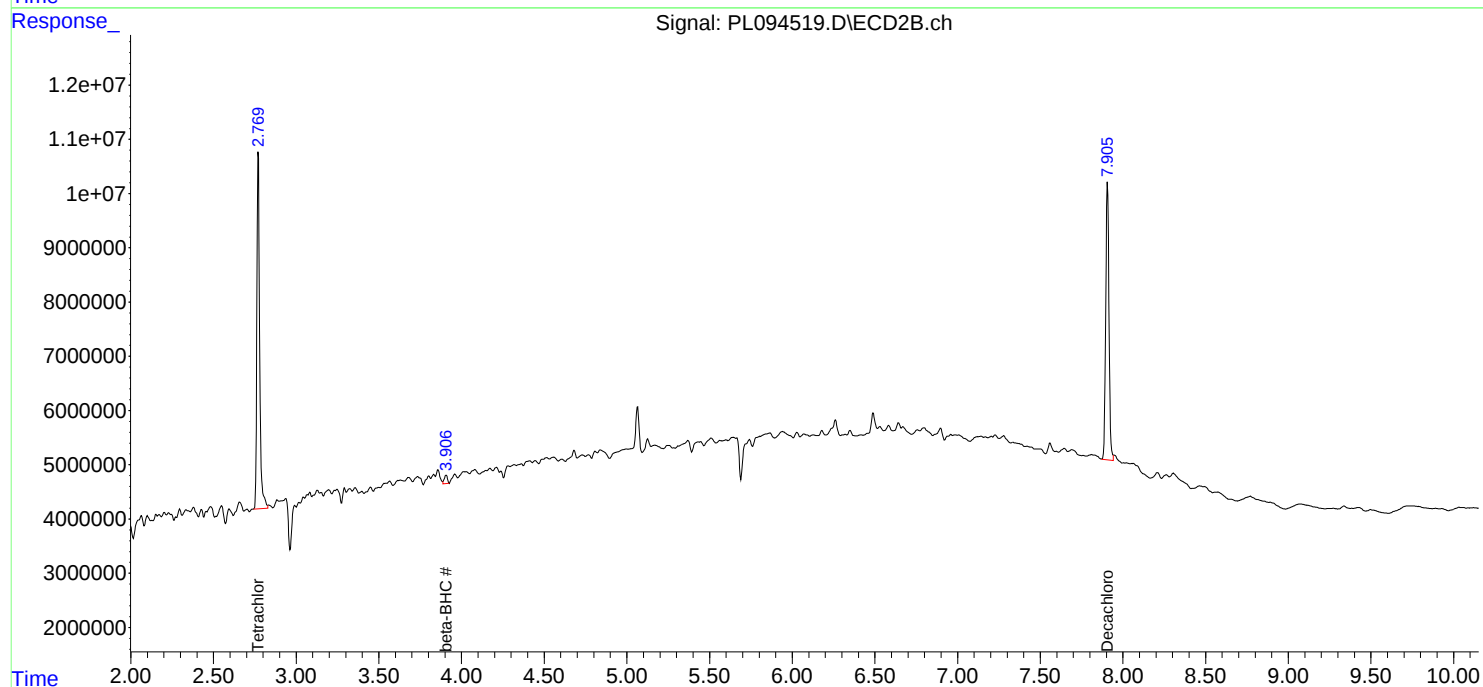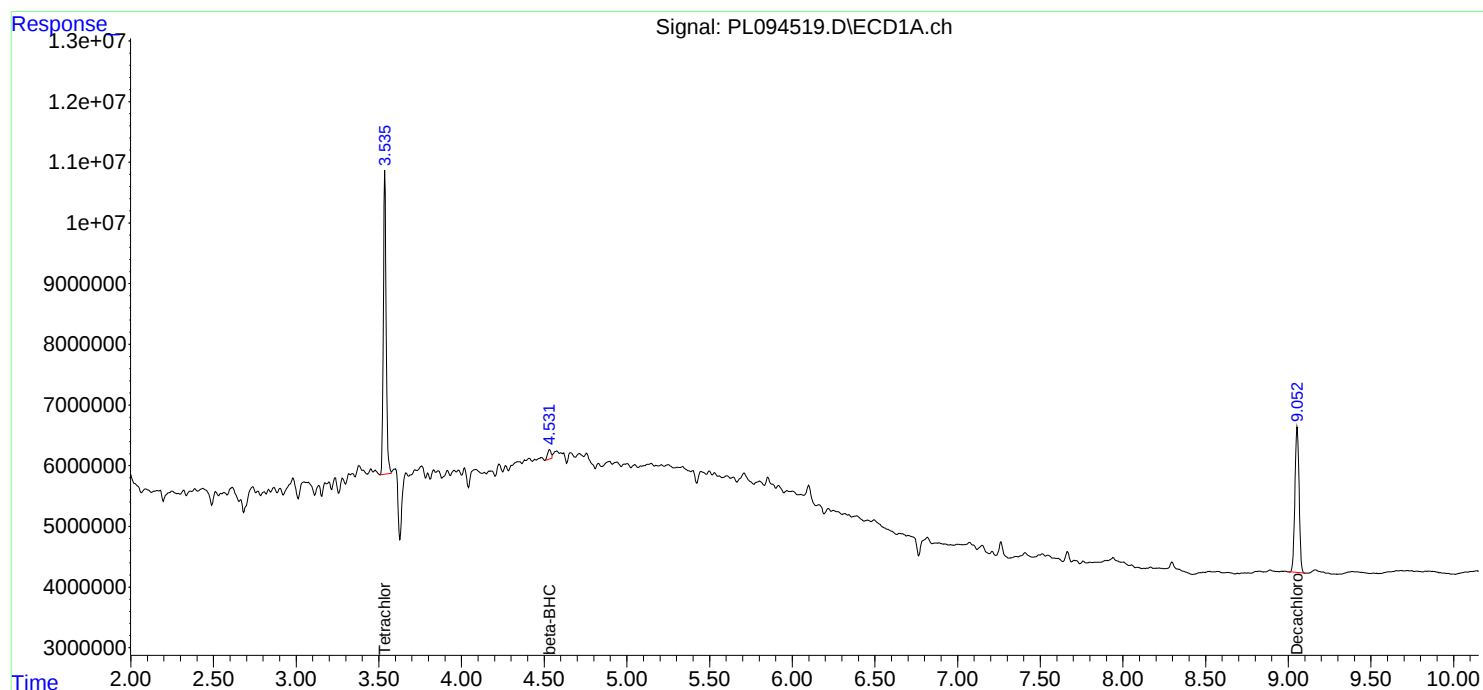


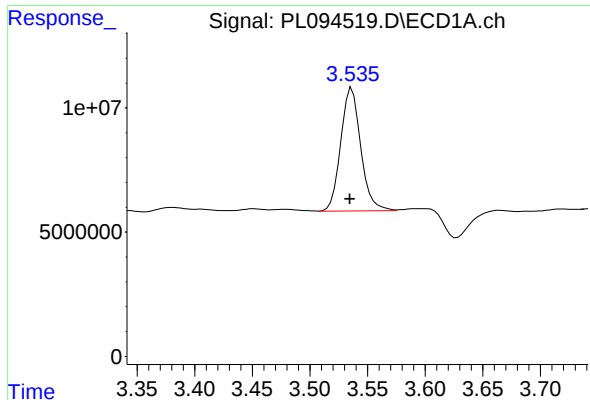

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 59129872
Conc: 23.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
DN-B-42

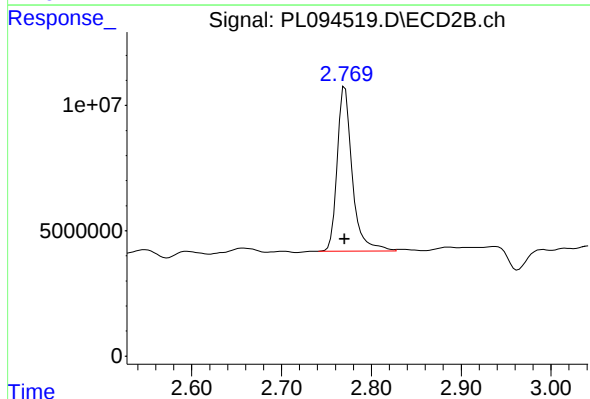


#1 Tetrachloro-m-xylene

R.T.: 2.771 min
Delta R.T.: 0.000 min
Response: 76545512
Conc: 23.99 ng/ml

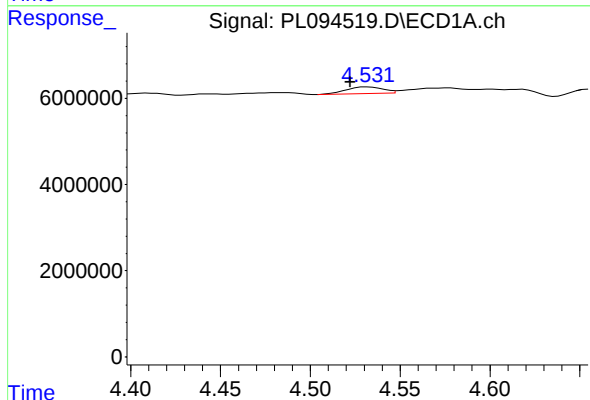


#6 beta-BHC

R.T.: 4.531 min
Delta R.T.: 0.008 min
Response: 2191243
Conc: 1.37 ng/ml m

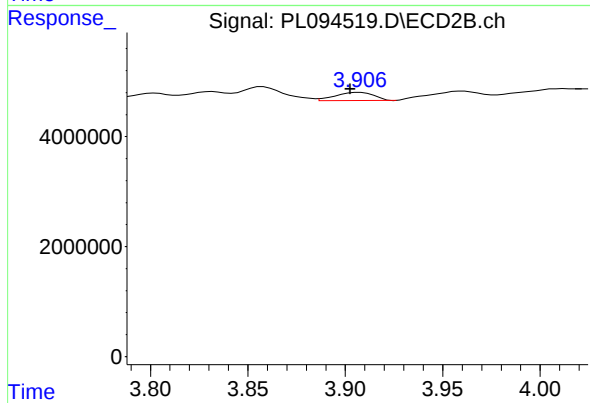

#6 beta-BHC


R.T.: 3.907 min
Delta R.T.: 0.005 min
Response: 2084874
Conc: 1.05 ng/ml

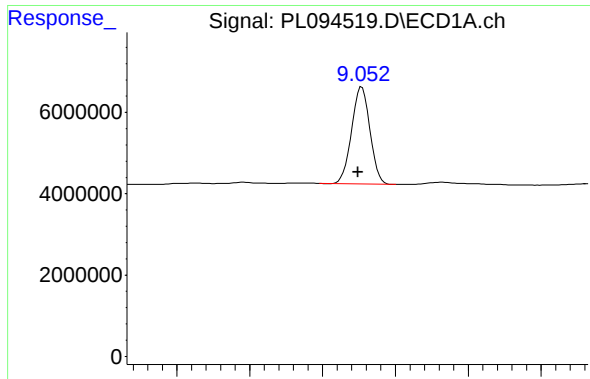

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.005 min
Response: 41915445
Conc: 19.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
DN-B-42

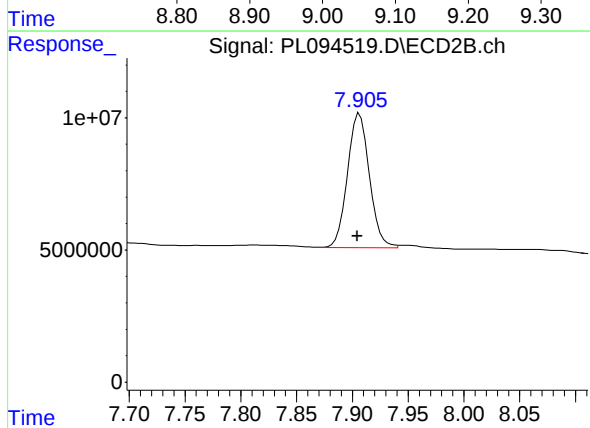

#28 Decachlorobiphenyl

R.T.: 7.905 min
Delta R.T.: 0.000 min
Response: 69528929
Conc: 18.08 ng/ml m