

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
 Data File : PL057122.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 14:56
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:58:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.461	3.959	187.9E6	48302622	22.053	22.640
28)	SA Decachlor...	8.212	8.985	159.2E6	38717290	16.470	18.222
Target Compounds							
8)	B Heptachlo...	0.000	5.815	0	12396192	N.D.	4.473 #
13)	MA Dieldrin	5.730f	0.000	79145282	0	6.473	N.D. #
15)	B Endosulfa...	0.000	6.870	0	4865874	N.D.	1.734 #
16)	A 4,4'-DDD	0.000	6.741f	0	36457127	N.D.	14.966 #
27)	Chlordane-5	0.000	6.918	0	1470845	N.D.	17.630 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
Data File : PL057122.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 14:56
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:58:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

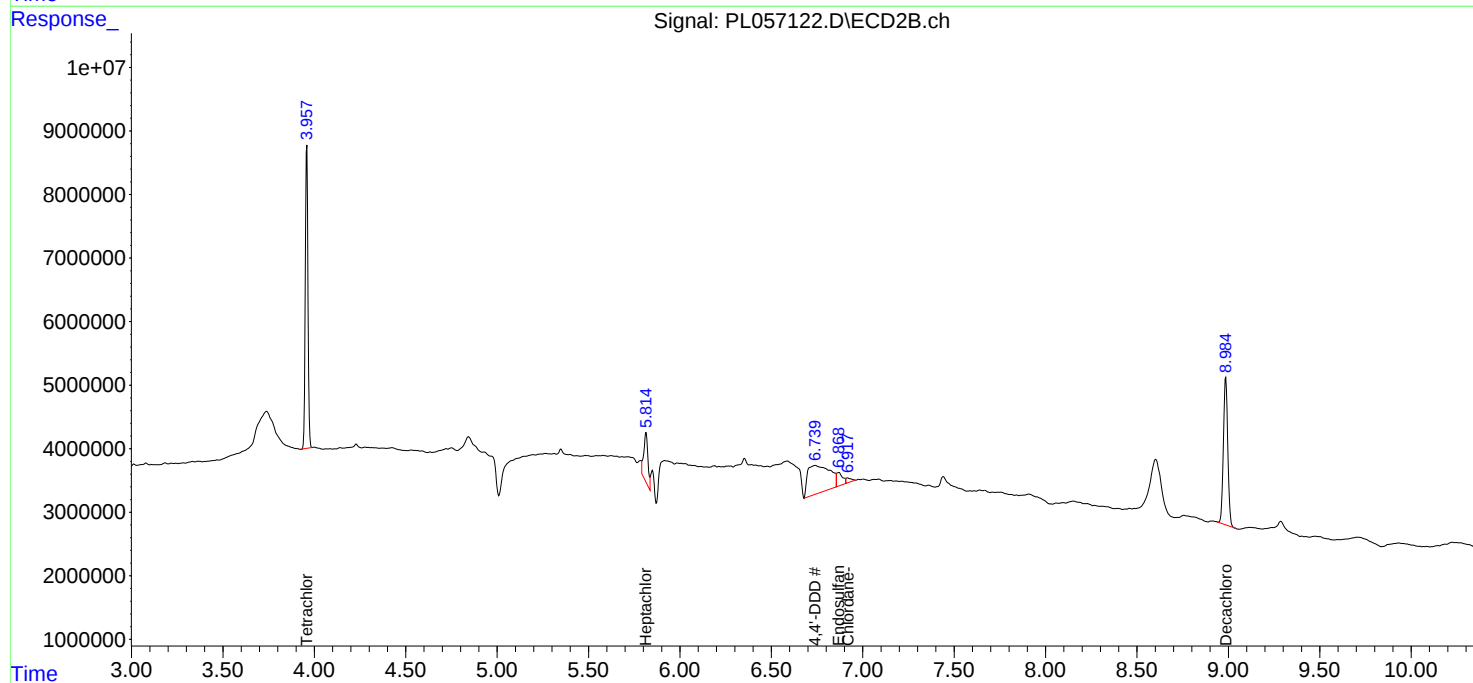


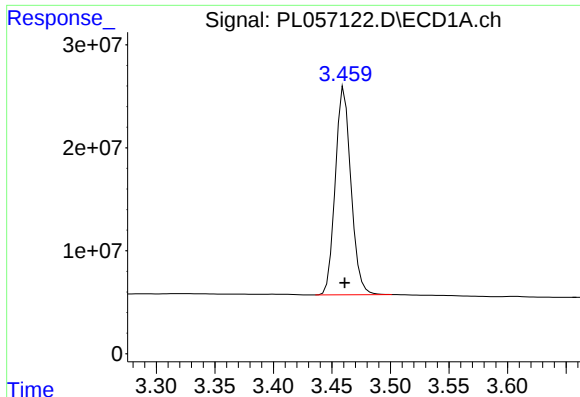

#1 Tetrachloro-m-xylene


R.T.: 3.461 min
Delta R.T.: 0.000 min
Response: 187940304
Conc: 22.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

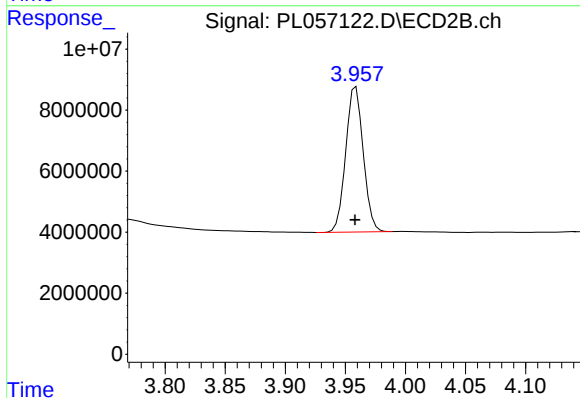


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 48302622
Conc: 22.64 ng/ml

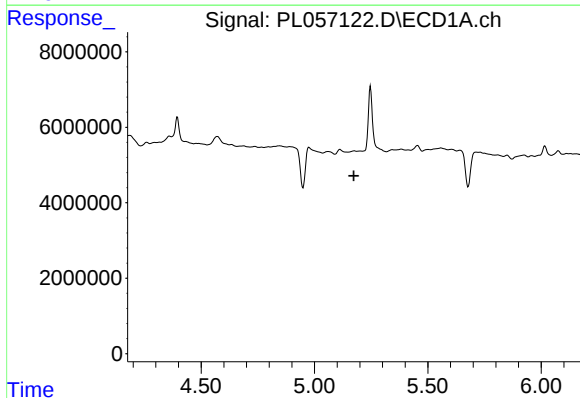


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.174 min
Response: 0
Conc: N.D.

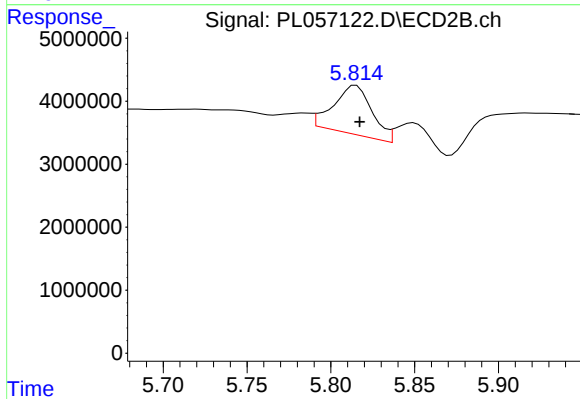

#8 Heptachlor epoxide


R.T.: 5.815 min
Delta R.T.: -0.002 min
Response: 12396192
Conc: 4.47 ng/ml

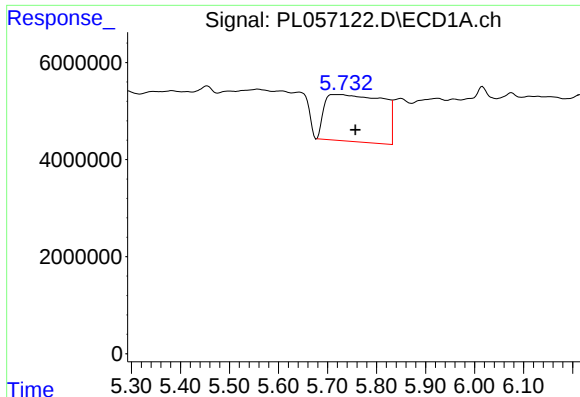

#13 Dieldrin


R.T.: 5.730 min
Delta R.T.: -0.027 min
Response: 79145282
Conc: 6.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

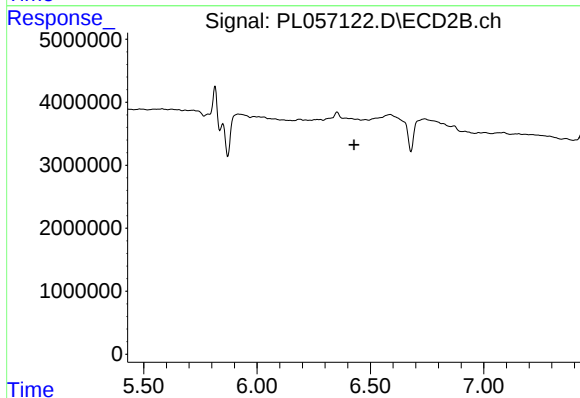


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

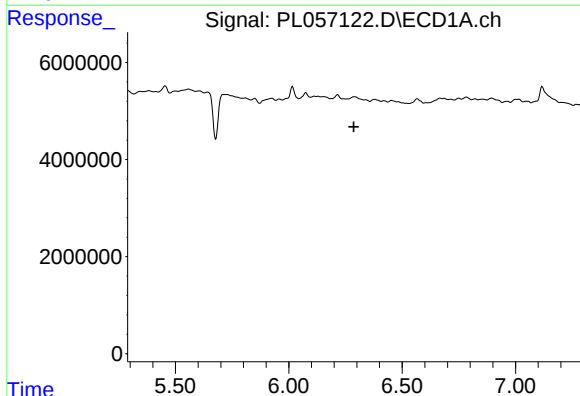


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.287 min
Response: 0
Conc: N.D.

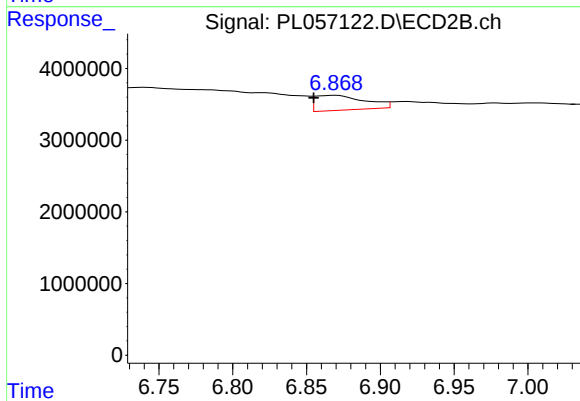

#15 Endosulfan II


R.T.: 6.870 min
Delta R.T.: 0.015 min
Response: 4865874
Conc: 1.73 ng/ml

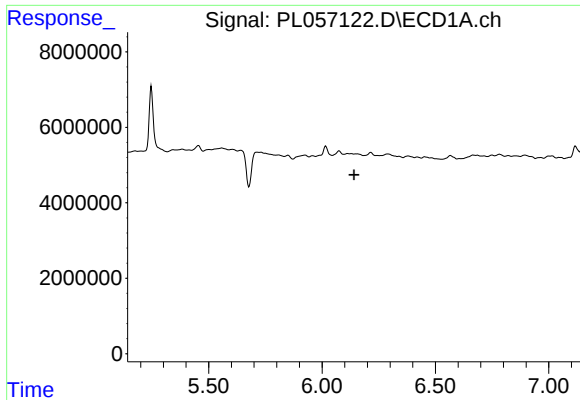

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

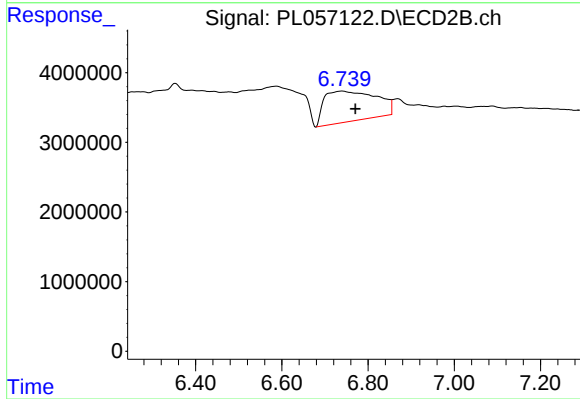


#16 4,4'-DDD

R.T.: 6.741 min
Delta R.T.: -0.030 min
Response: 36457127
Conc: 14.97 ng/ml

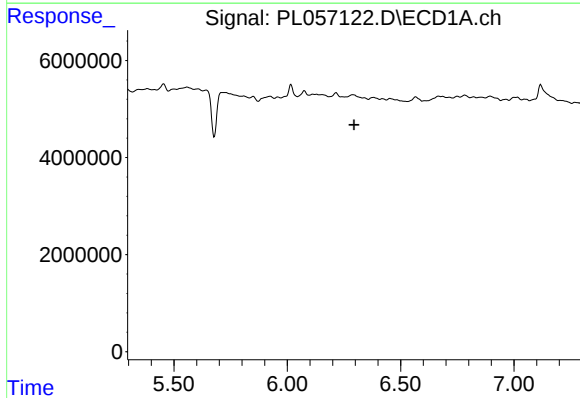


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.295 min
Response: 0
Conc: N.D.

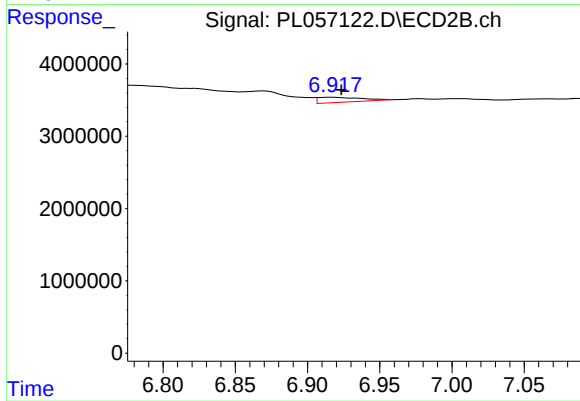

#27 Chlordane-5


R.T.: 6.918 min
Delta R.T.: -0.005 min
Response: 1470845
Conc: 17.63 ng/ml

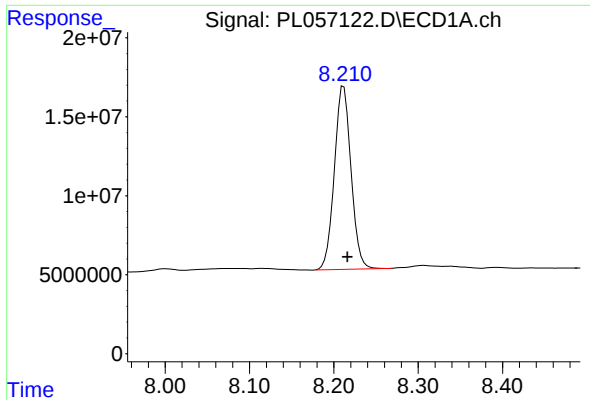

#28 Decachlorobiphenyl

R.T.: 8.212 min
Delta R.T.: -0.004 min
Response: 159182553
Conc: 16.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

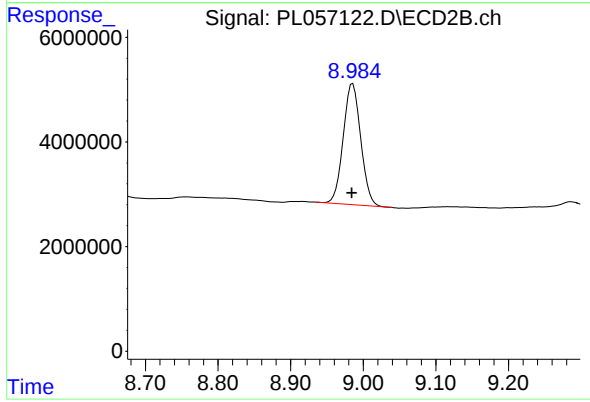

#28 Decachlorobiphenyl

R.T.: 8.985 min
Delta R.T.: 0.001 min
Response: 38717290
Conc: 18.22 ng/ml