

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
 Data File : PL057127.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 17:02
 Operator : AJ\MA
 Sample : PB127332BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 02:59:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.464	3.959	166.7E6	40481218	19.556	18.974
28)	SA Decachlor...	8.214	8.988	159.3E6	38882015	16.478	18.300
Target Compounds							
4)	MA Heptachlor	0.000	5.146f	0	2357551	N.D.	0.757 #
23)	Chlordane-1	4.359f	0.000	12542004	0	41.263	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
Data File : PL057127.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 17:02
Operator : AJ\MA
Sample : PB127332BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 02:59:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

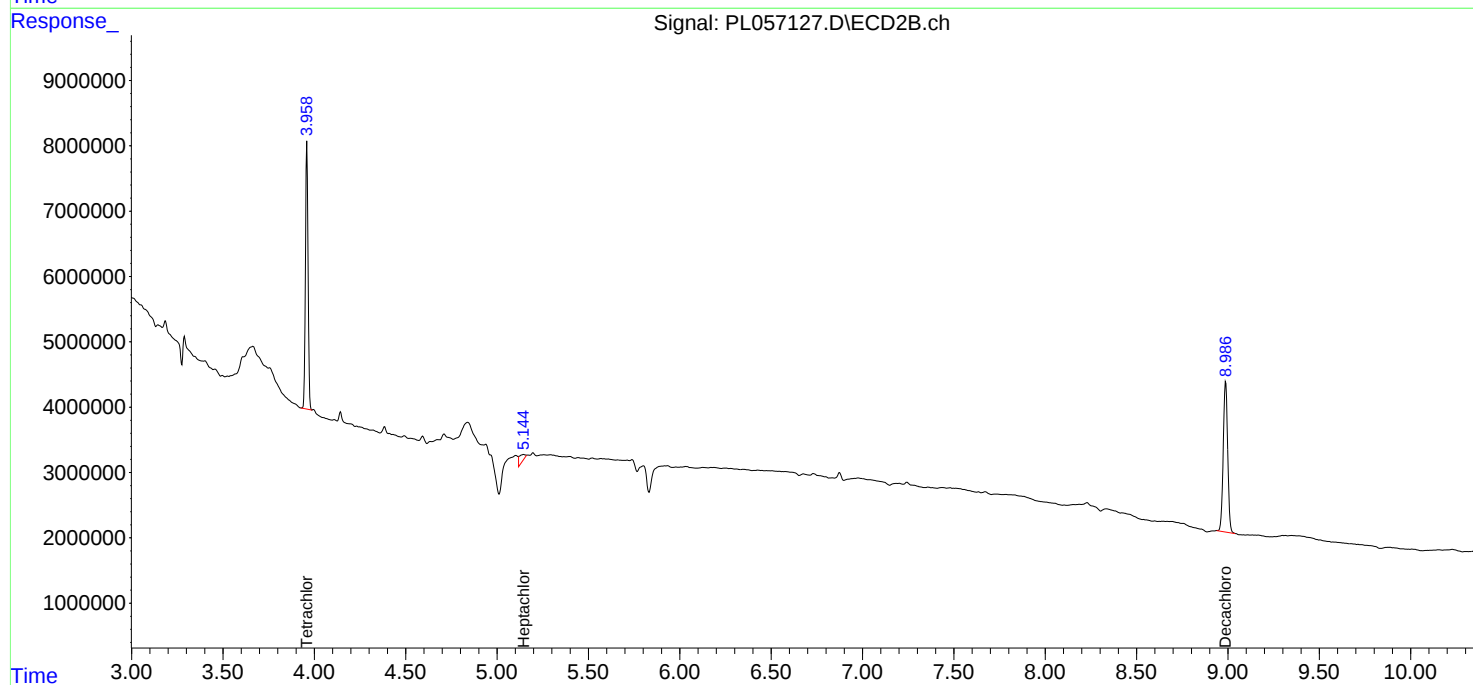


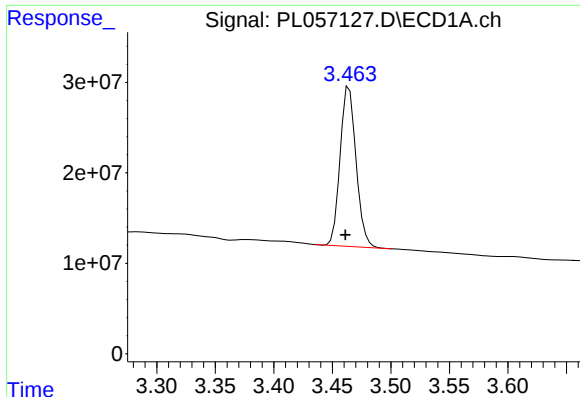

#1 Tetrachloro-m-xylene


R.T.: 3.464 min
Delta R.T.: 0.003 min
Response: 166662399
Conc: 19.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

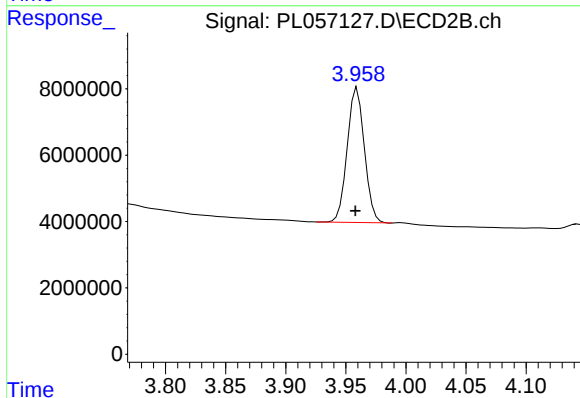


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.001 min
Response: 40481218
Conc: 18.97 ng/ml

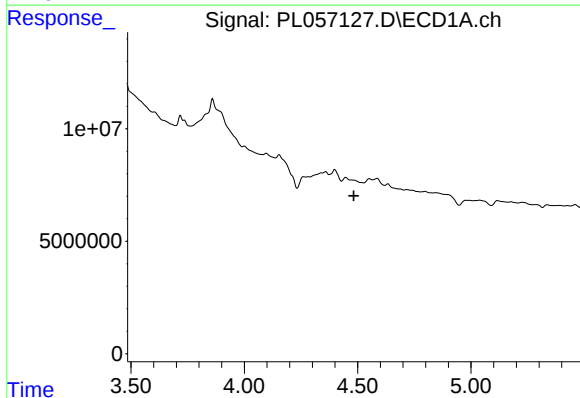


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

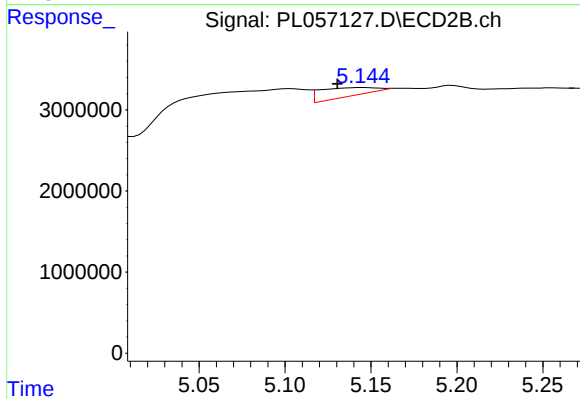

#4 Heptachlor


R.T.: 5.146 min
Delta R.T.: 0.015 min
Response: 2357551
Conc: 0.76 ng/ml

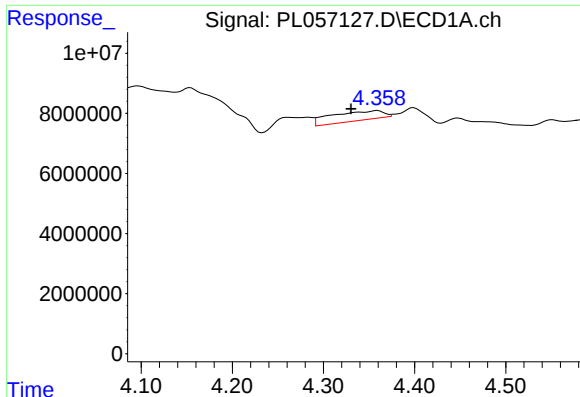

#23 Chlordane-1


R.T.: 4.359 min
Delta R.T.: 0.029 min
Response: 12542004
Conc: 41.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

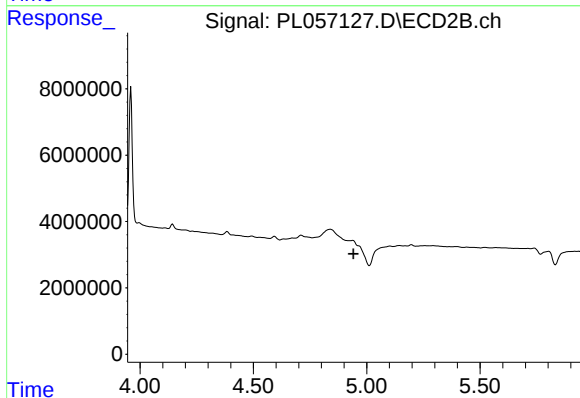


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.942 min
Response: 0
Conc: N.D.

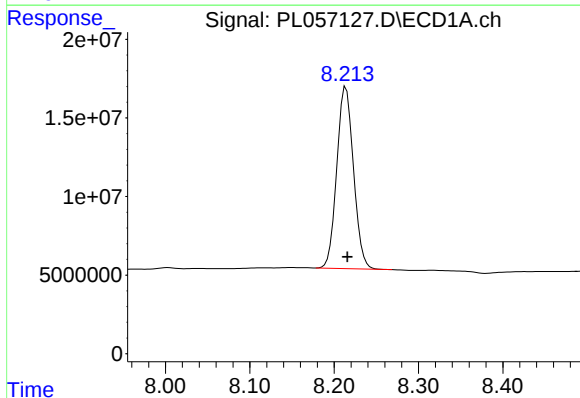

#28 Decachlorobiphenyl

R.T.: 8.214 min
Delta R.T.: -0.002 min
Response: 159265590
Conc: 16.48 ng/ml

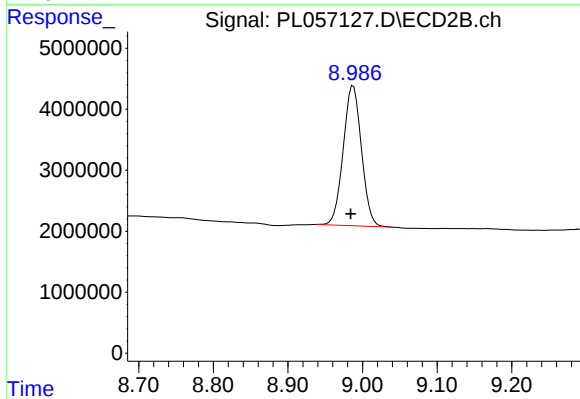

#28 Decachlorobiphenyl

R.T.: 8.988 min
Delta R.T.: 0.003 min
Response: 38882015
Conc: 18.30 ng/ml