

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
 Data File : PL057130.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2020 17:44
 Operator : AJ\MA
 Sample : L1813-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 07 03:00:05 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
 Quant Title : GC Extractables
 QLast Update : Wed Mar 04 03:55:01 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.460	3.959	91173177	24402109	10.698	11.438
28)	SA Decachlor...	8.210	8.986	77515011	19723966	8.020	9.283
Target Compounds							
4)	MA Heptachlor	0.000	5.147f	0	11614127	N.D.	3.732 #
10)	B gamma-Chl...	5.421f	0.000	10083265	0	0.812	N.D. #
11)	B alpha-Chl...	0.000	6.126	0	2849771	N.D.	0.945 #
12)	B 4,4'-DDE	5.622	6.283	244.1E6	55551068	20.832	19.575
14)	MA Endrin	6.011	0.000	6999208	0	0.643	N.D. #
16)	A 4,4'-DDD	0.000	6.775	0	2061010	N.D.	0.846 #
17)	MA 4,4'-DDT	6.378	7.068	52505467	15146243	5.366	6.157
25)	Chlordane-3	5.421f	0.000	10083265	0	9.348	N.D. #
26)	Chlordane-4	0.000	6.126	0	2849771	N.D.	6.215 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030620\
Data File : PL057130.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2020 17:44
Operator : AJ\MA
Sample : L1813-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 07 03:00:05 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030320.M
Quant Title : GC Extractables
QLast Update : Wed Mar 04 03:55:01 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

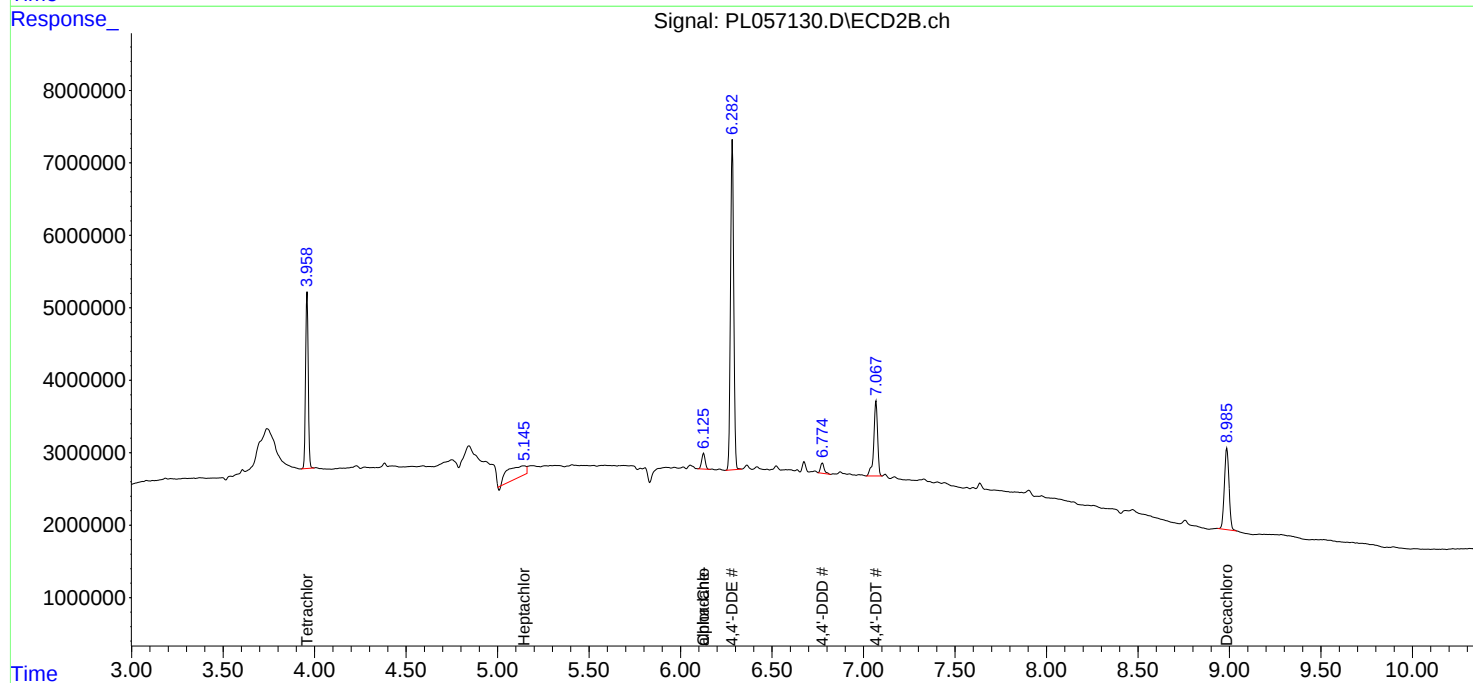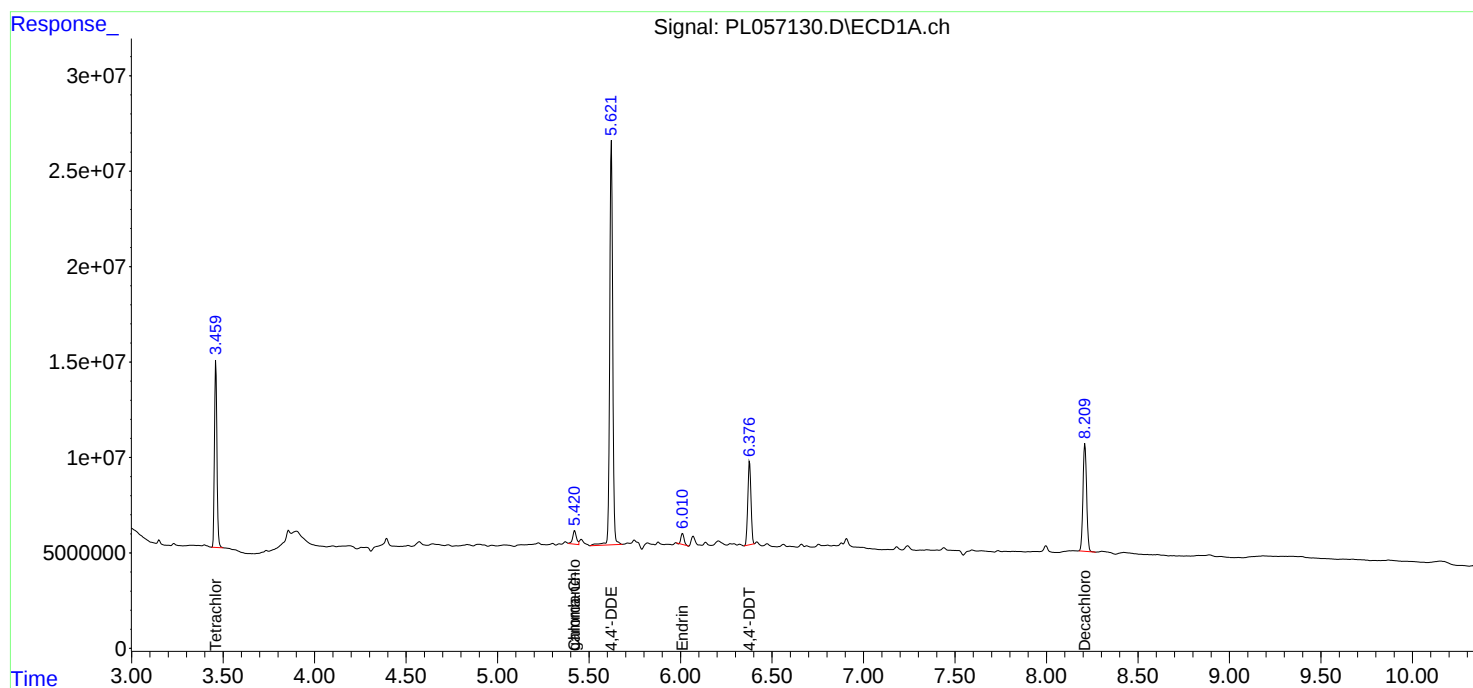


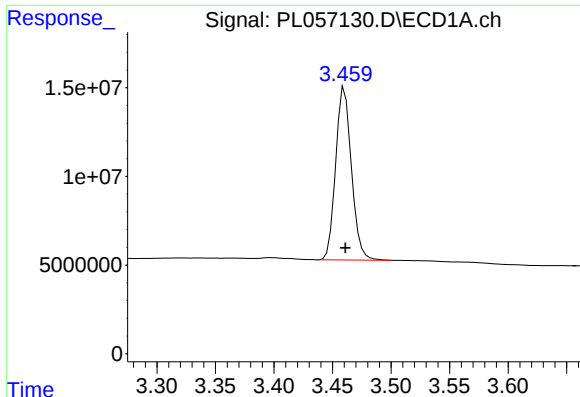

#1 Tetrachloro-m-xylene


R.T.: 3.460 min
Delta R.T.: 0.000 min
Response: 91173177
Conc: 10.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

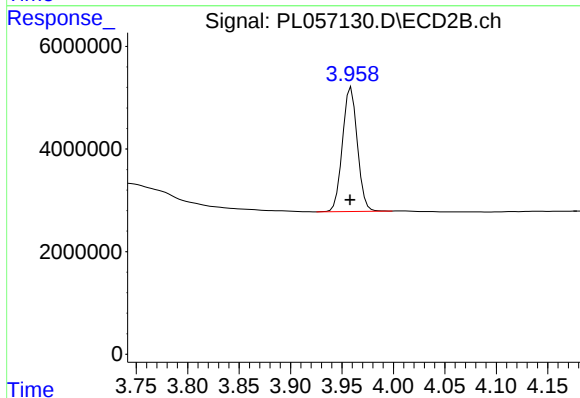


#1 Tetrachloro-m-xylene

R.T.: 3.959 min
Delta R.T.: 0.000 min
Response: 24402109
Conc: 11.44 ng/ml

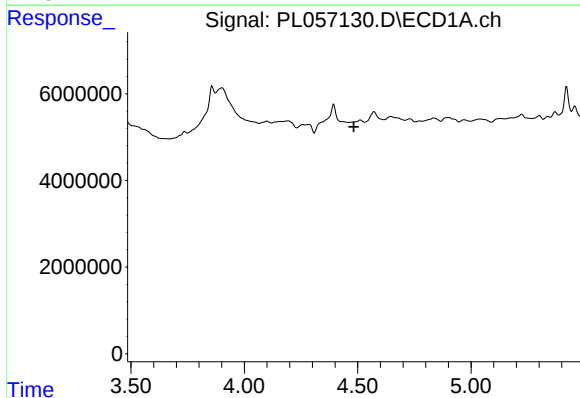


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.483 min
Response: 0
Conc: N.D.

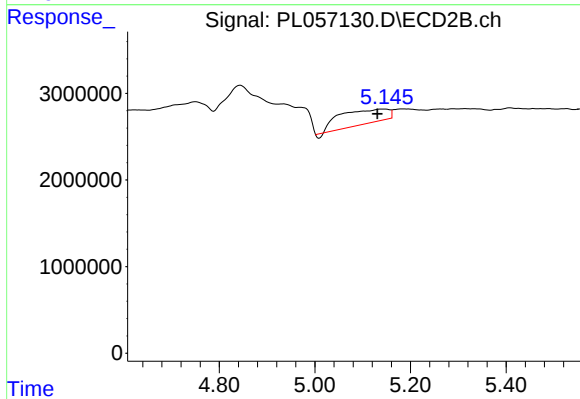

#4 Heptachlor


R.T.: 5.147 min
Delta R.T.: 0.016 min
Response: 11614127
Conc: 3.73 ng/ml

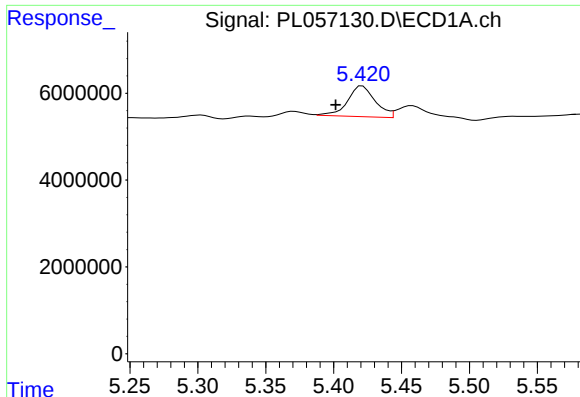

#10 gamma-Chlordane


R.T.: 5.421 min
Delta R.T.: 0.020 min
Response: 10083265
Conc: 0.81 ng/ml

Instrument :
ECD_L
ClientSampleId :

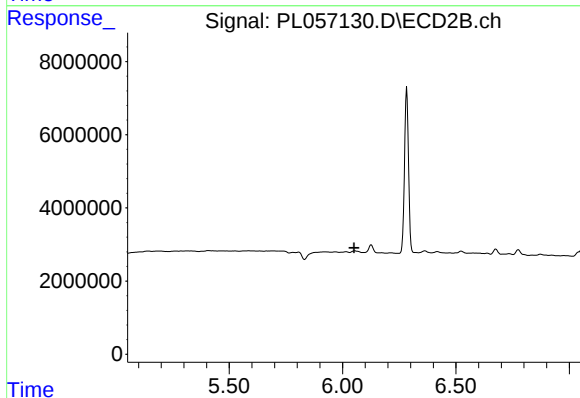


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

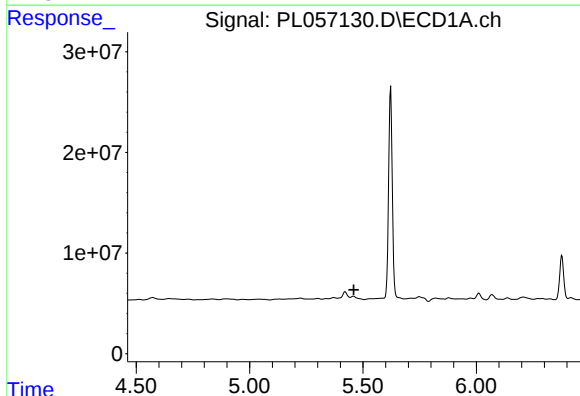


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.460 min
Response: 0
Conc: N.D.

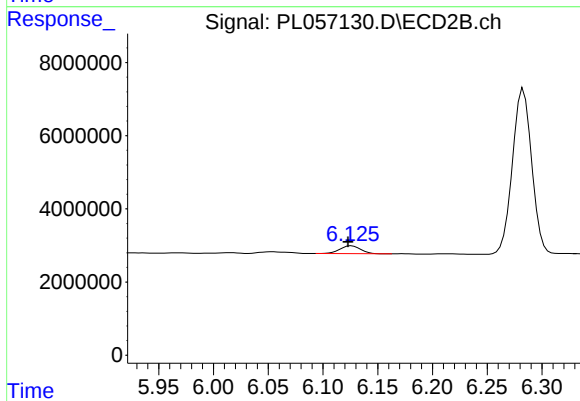

#11 alpha-Chlordane


R.T.: 6.126 min
Delta R.T.: 0.003 min
Response: 2849771
Conc: 0.95 ng/ml

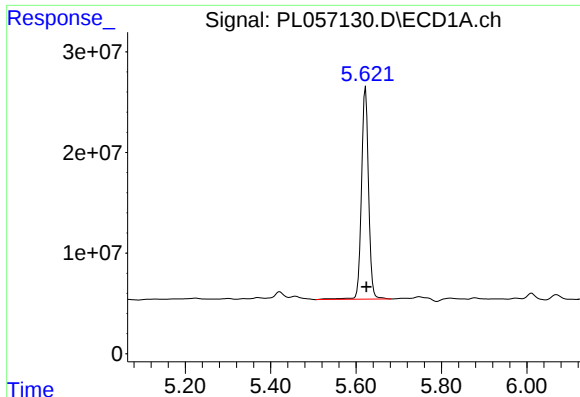

#12 4,4'-DDE


R.T.: 5.622 min
Delta R.T.: -0.002 min
Response: 244111421
Conc: 20.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

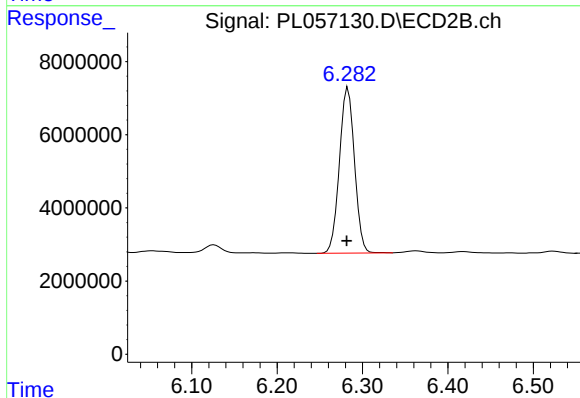


#12 4,4'-DDE

R.T.: 6.283 min
Delta R.T.: 0.001 min
Response: 55551068
Conc: 19.57 ng/ml

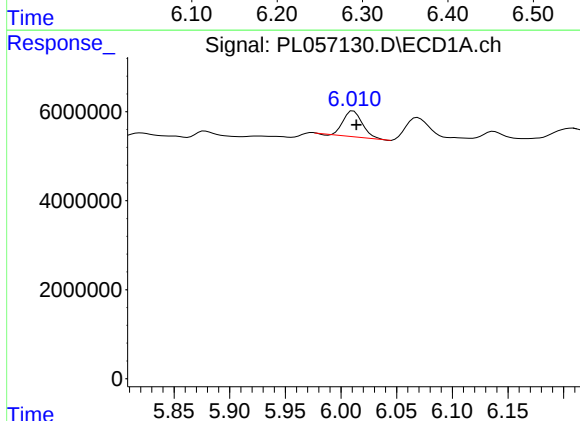


#14 Endrin

R.T.: 6.011 min
Delta R.T.: -0.003 min
Response: 6999208
Conc: 0.64 ng/ml

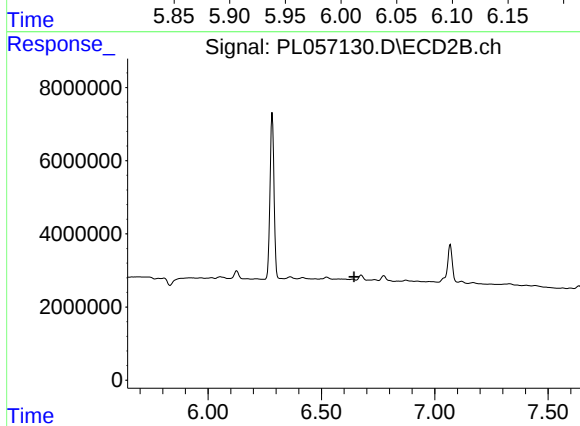

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.645 min
Response: 0
Conc: N.D.

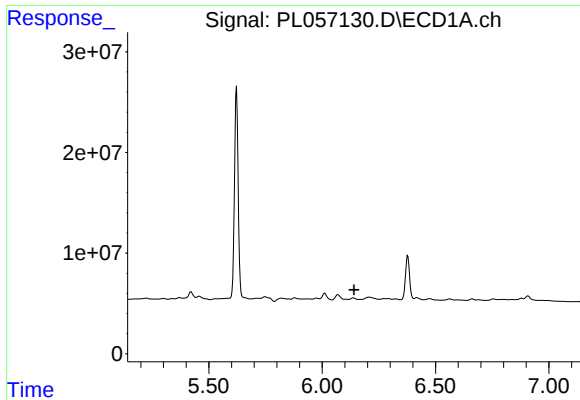

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

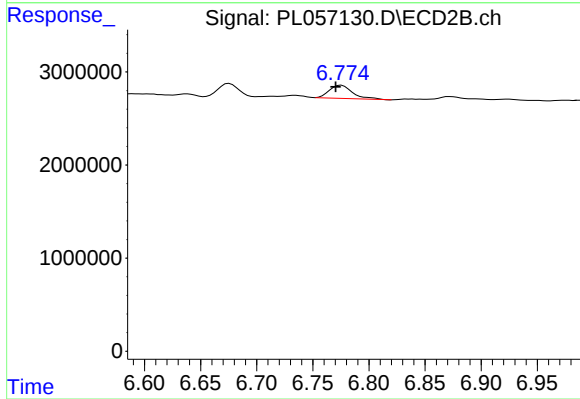


#16 4,4'-DDD

R.T.: 6.775 min
Delta R.T.: 0.005 min
Response: 2061010
Conc: 0.85 ng/ml

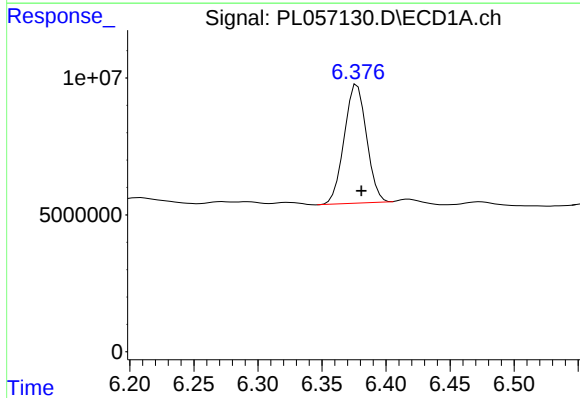


#17 4,4'-DDT

R.T.: 6.378 min
Delta R.T.: -0.003 min
Response: 52505467
Conc: 5.37 ng/ml

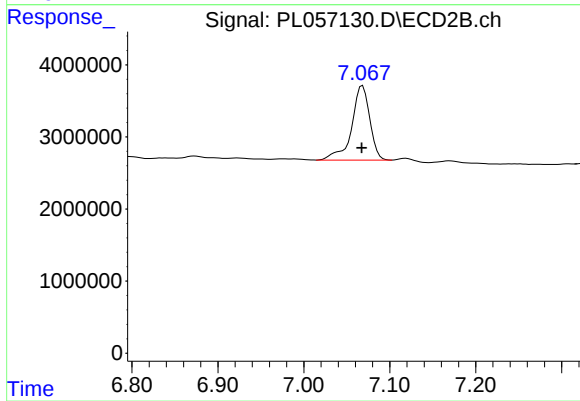

#17 4,4'-DDT


R.T.: 7.068 min
Delta R.T.: 0.000 min
Response: 15146243
Conc: 6.16 ng/ml

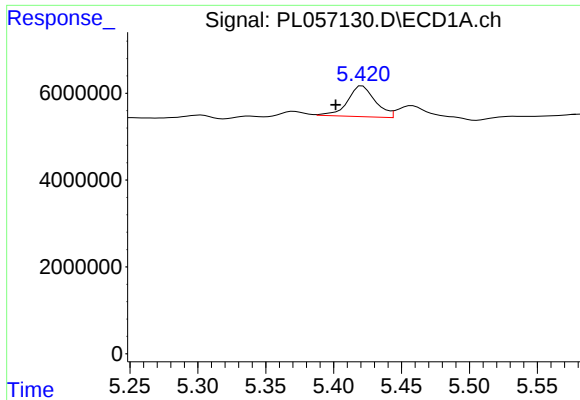

#25 Chlordane-3


R.T.: 5.421 min
Delta R.T.: 0.020 min
Response: 10083265
Conc: 9.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

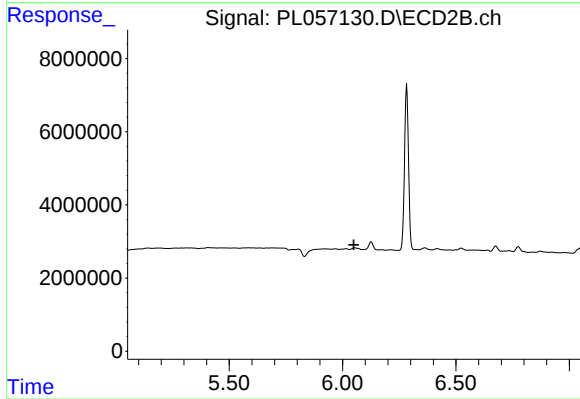


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.050 min
Response: 0
Conc: N.D.

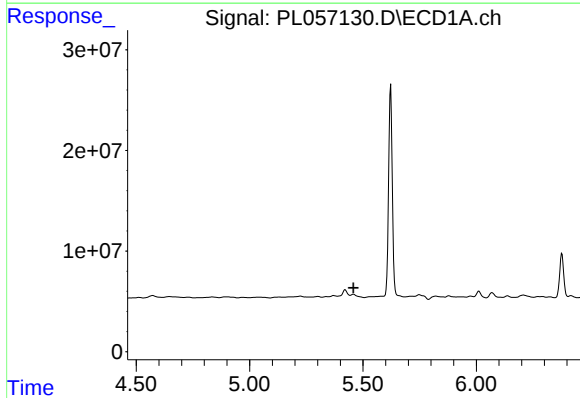


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.459 min
Response: 0
Conc: N.D.

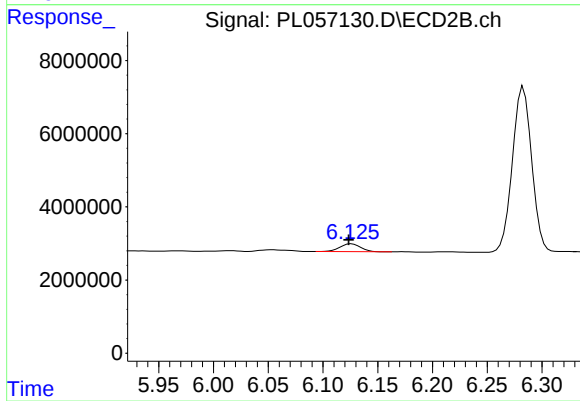

#26 Chlordane-4

R.T.: 6.126 min
Delta R.T.: 0.003 min
Response: 2849771
Conc: 6.21 ng/ml

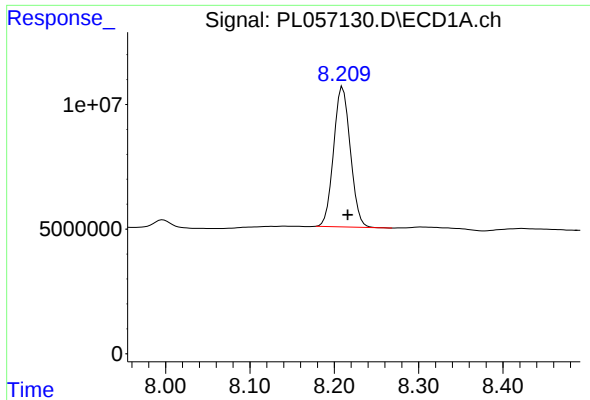

#28 Decachlorobiphenyl


R.T.: 8.210 min

Delta R.T.: -0.006 min

Response: 77515011

Conc: 8.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

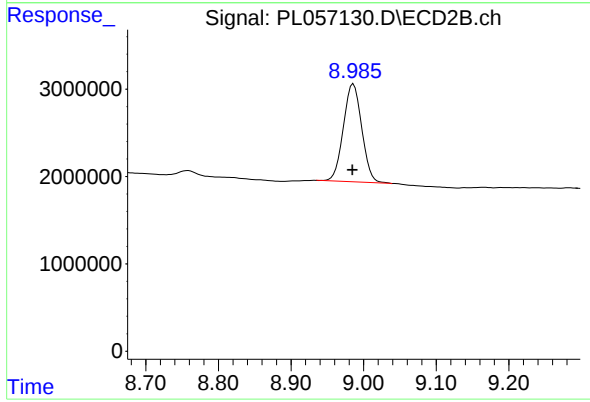

#28 Decachlorobiphenyl

R.T.: 8.986 min

Delta R.T.: 0.002 min

Response: 19723966

Conc: 9.28 ng/ml